

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:00:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

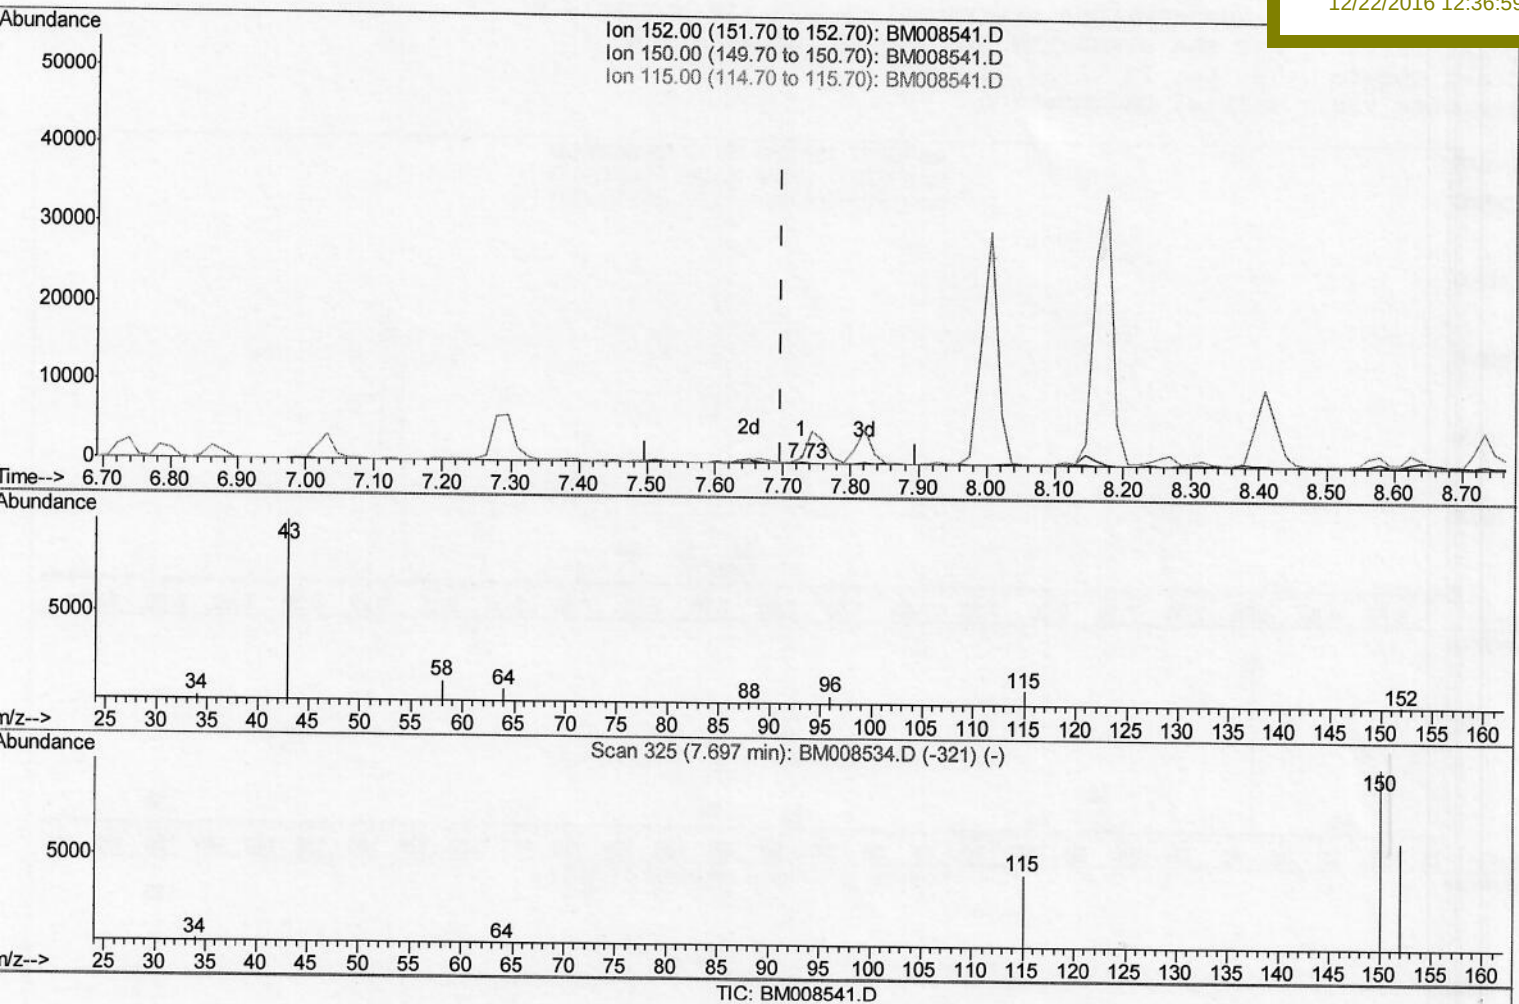

(1) 1,4-Dichlorobenzene-d4 (I)

7.728min (+0.031) 0.40ng/ul

response 80

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	55.66#
115.00	64.90	807.55#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:01:03 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

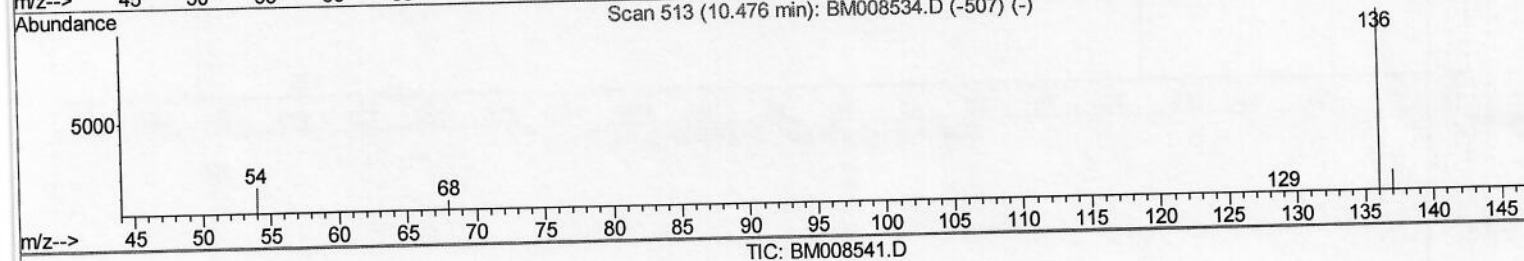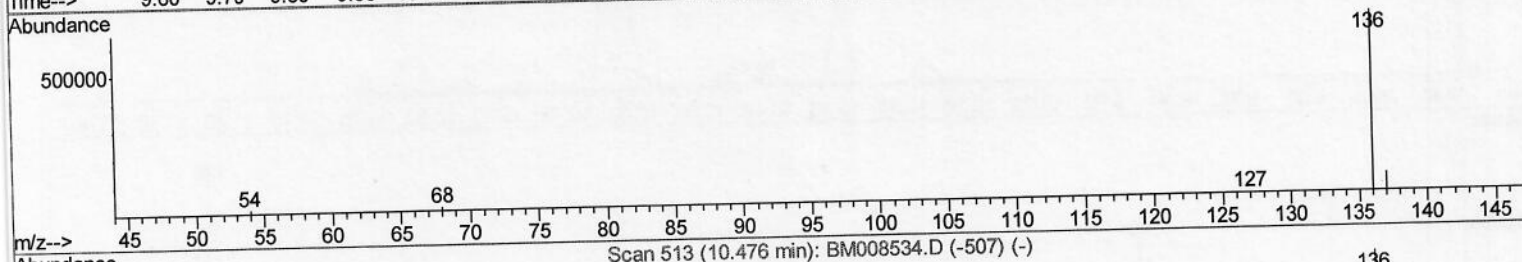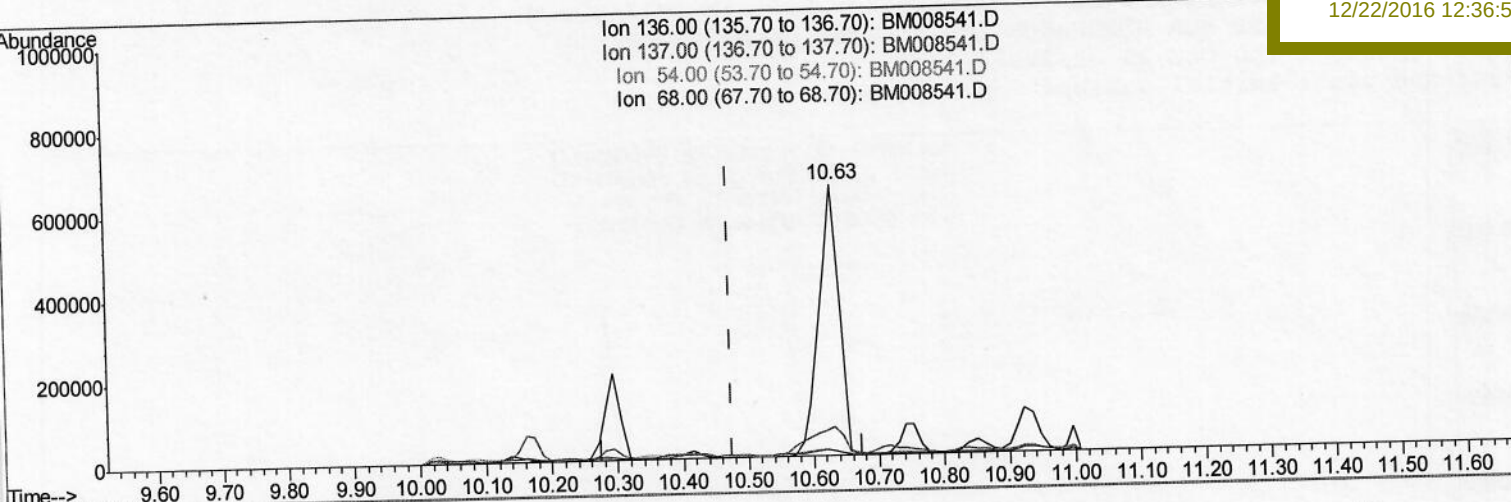

(2) Naphthalene-d8 (I)

10.633min (+0.157) 0.40ng/ul

response 1368844

Ion	Exp%	Act%
136.00	100	100
137.00	13.90	10.38#
54.00	15.50	1.90#
68.00	9.90	2.00#




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
Data File : BM008541.D
Acq On : 22 Dec 2016 05:37
Operator : UM/SJ
Sample : H6039-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8T3

Manual Integrations
APPROVED

Sohil
12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:01:51 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 02:22:34 2016
Response via : Initial Calibration

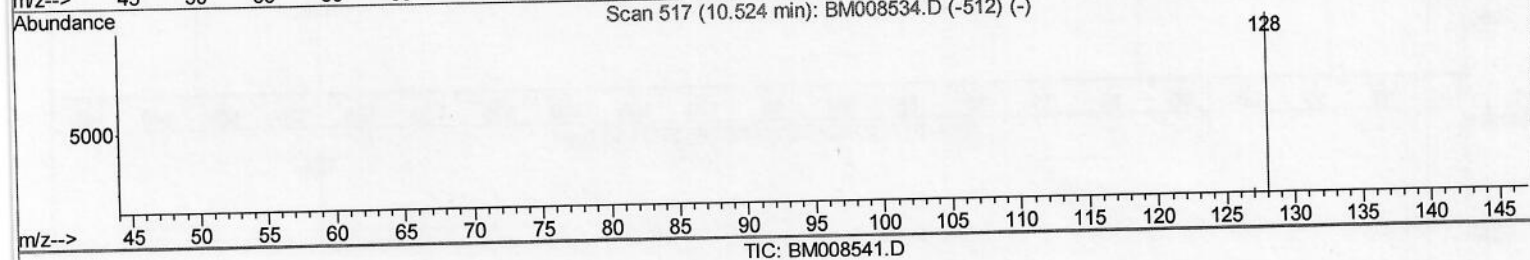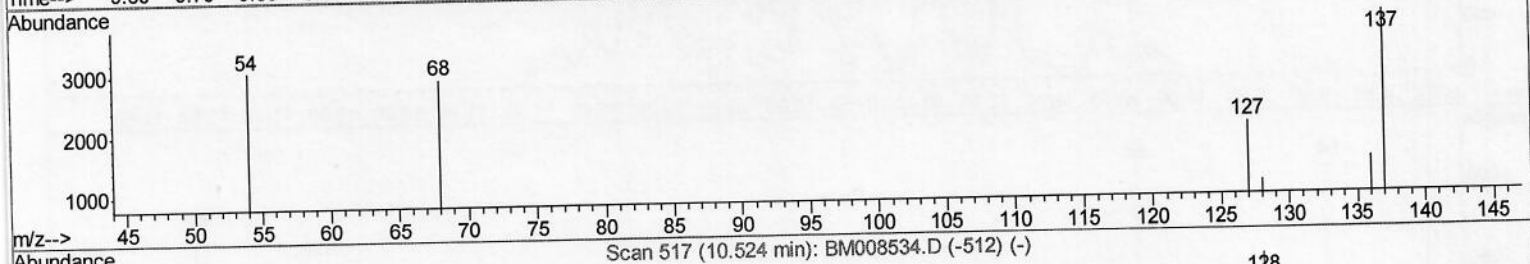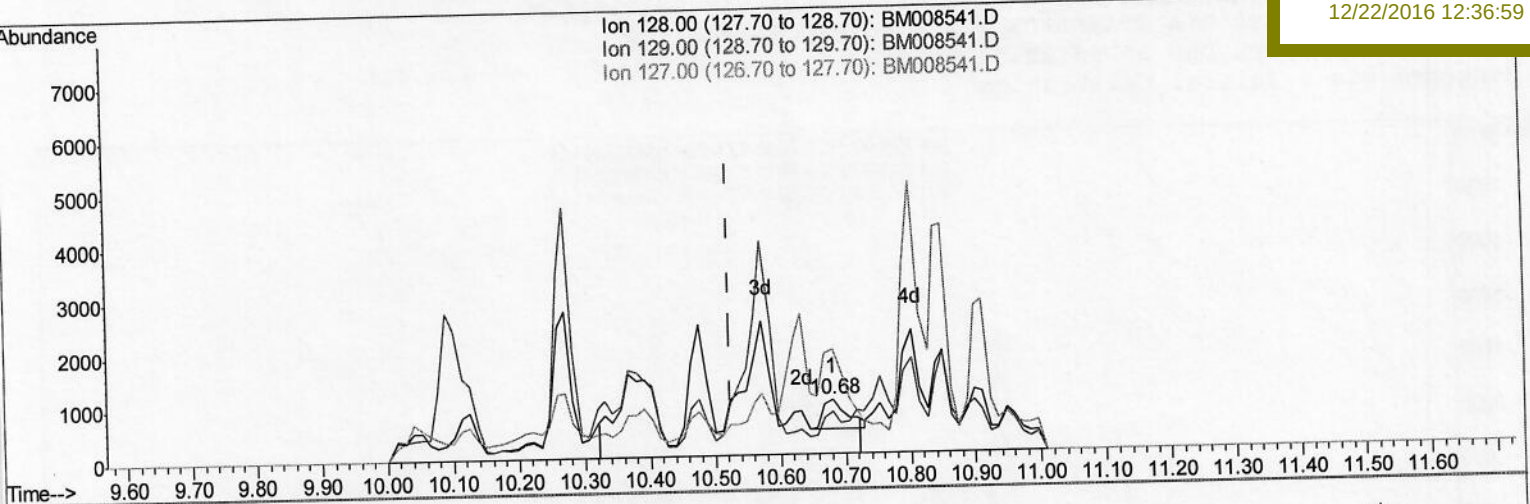

(3) Naphthalene

10.681min (+0.157) 0.01ng/ul

response 1333

Ion	Exp%	Act%
128.00	100	100
129.00	14.10	76.76#
127.00	16.00	194.24#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:01:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

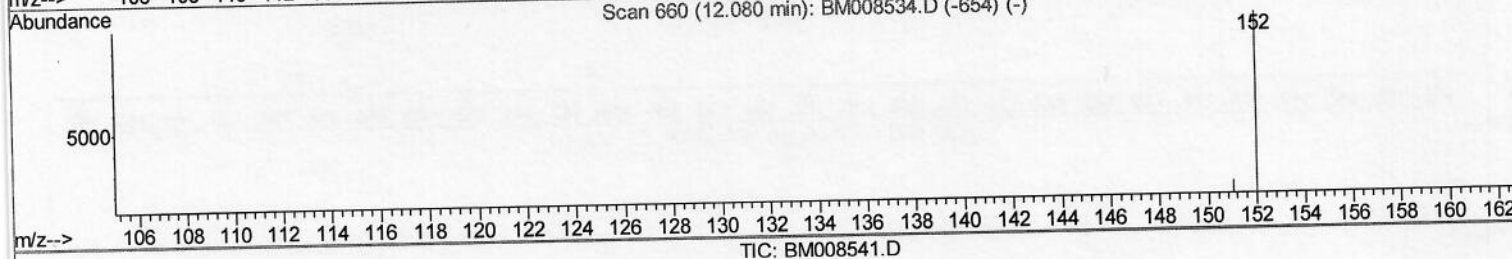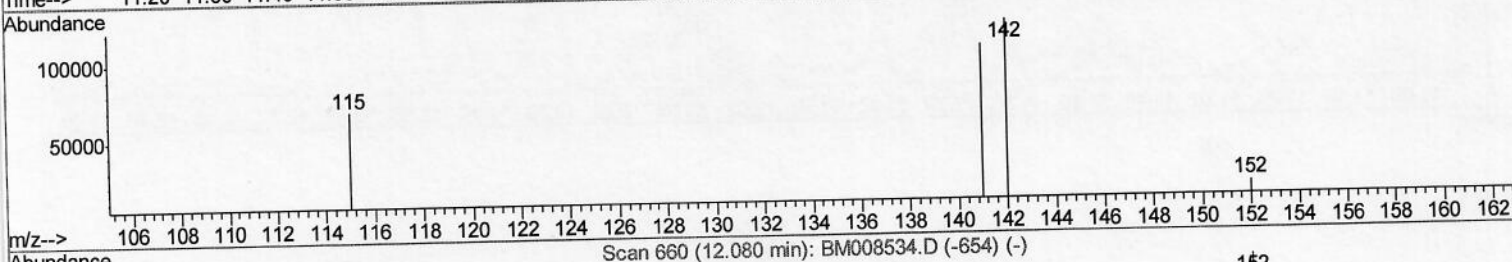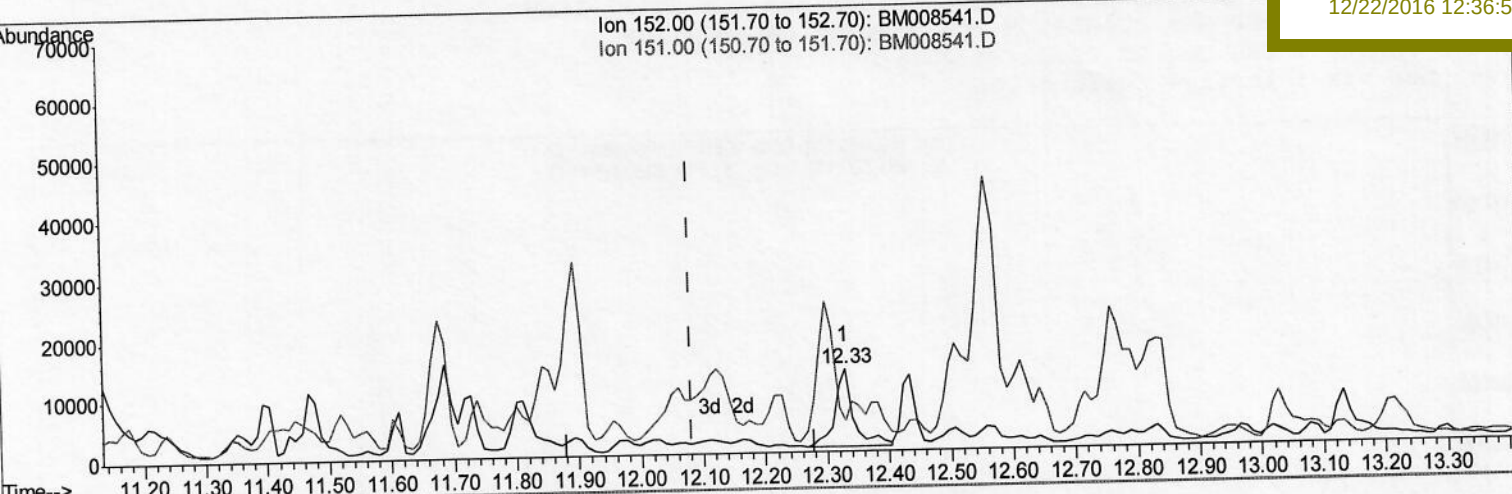

(4) 2-Methylnaphthalene-d10 (SURR)

12.330min (+0.250) 0.52ng/ul

response 25738

Ion	Exp%	Act%
152.00	100	100
151.00	19.30	63.57#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DA8T3

Manual Integrations
APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:01:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

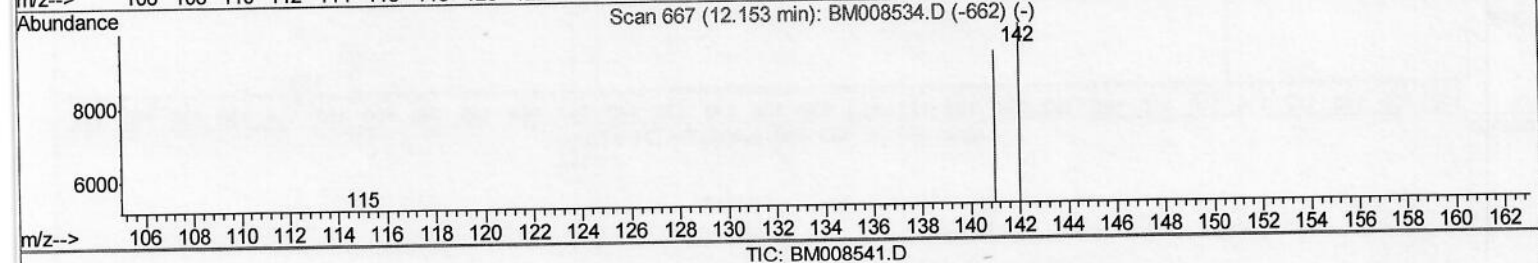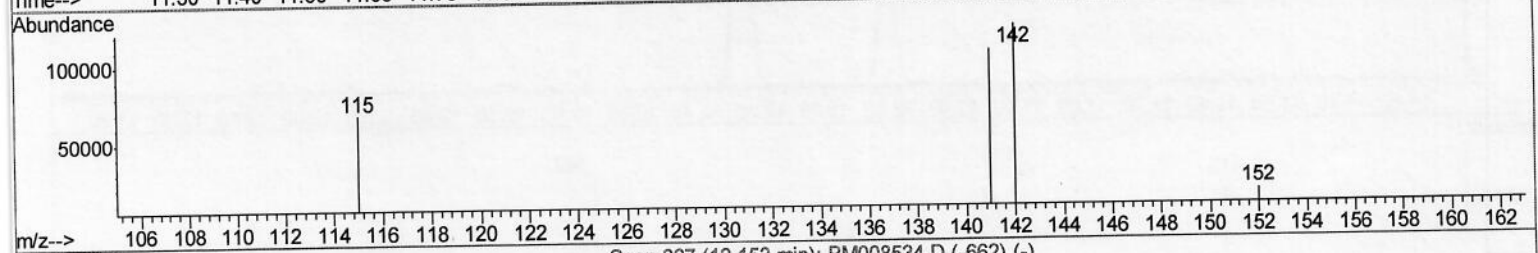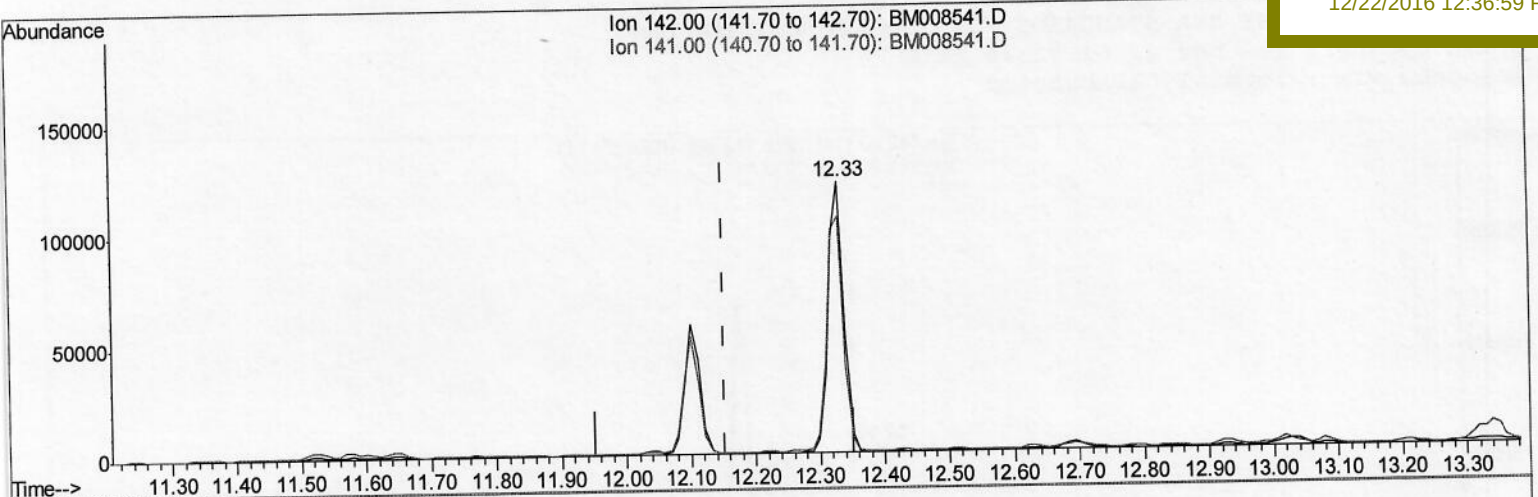

(5) 2-Methylnaphthalene

12.330min (+0.177) 3.27ng/ul

response 200727

Ion	Exp%	Act%
142.00	100	100
141.00	90.70	92.91
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:01:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

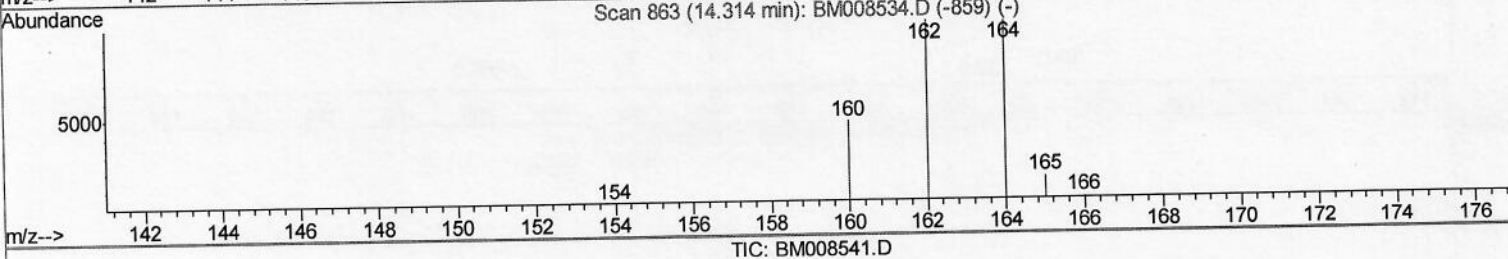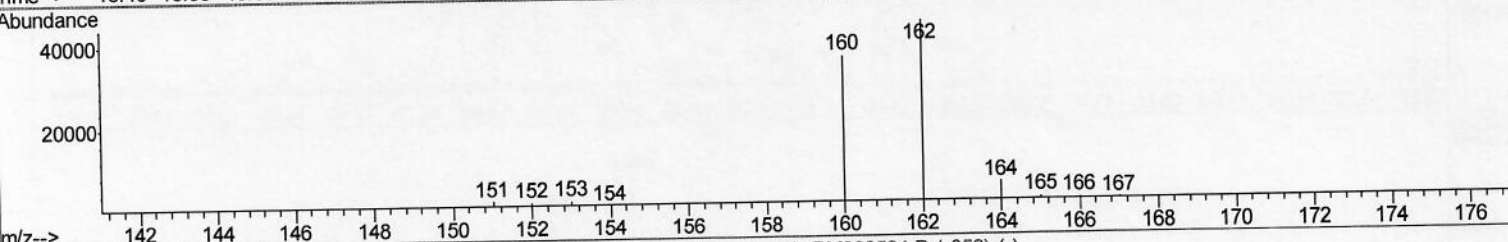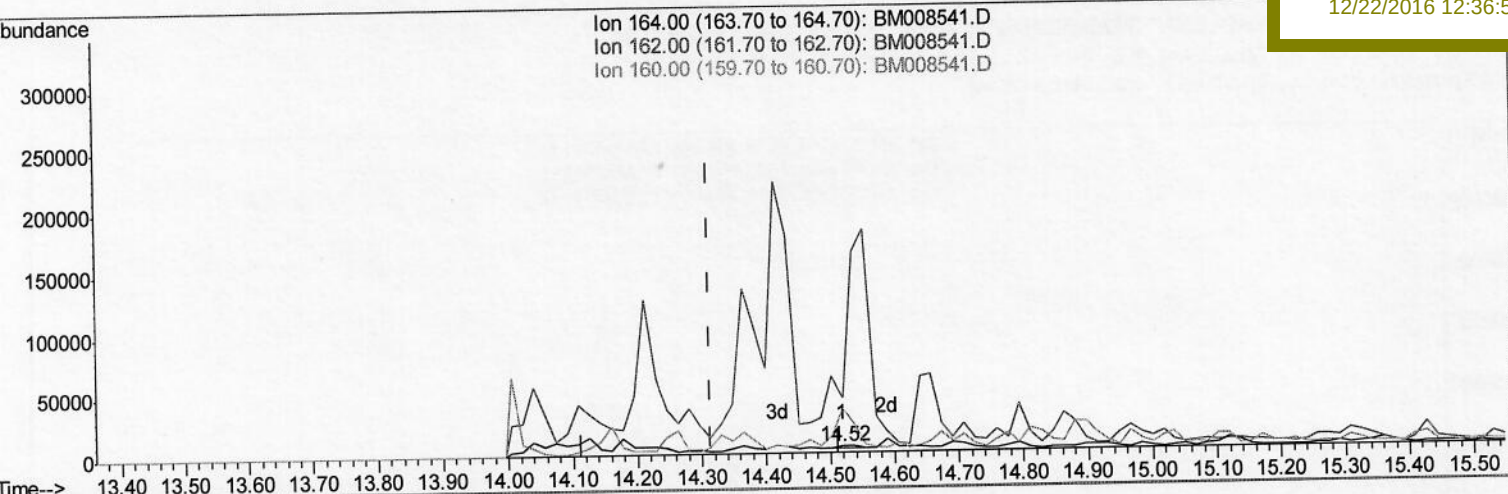

(6) Acenaphthene-d10 (I)

14.520min (+0.206) 0.40ng/ul

response 5245

Ion	Exp%	Act%
164.00	100	100
162.00	98.60	878.65#
160.00	48.80	714.99#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:04:37 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

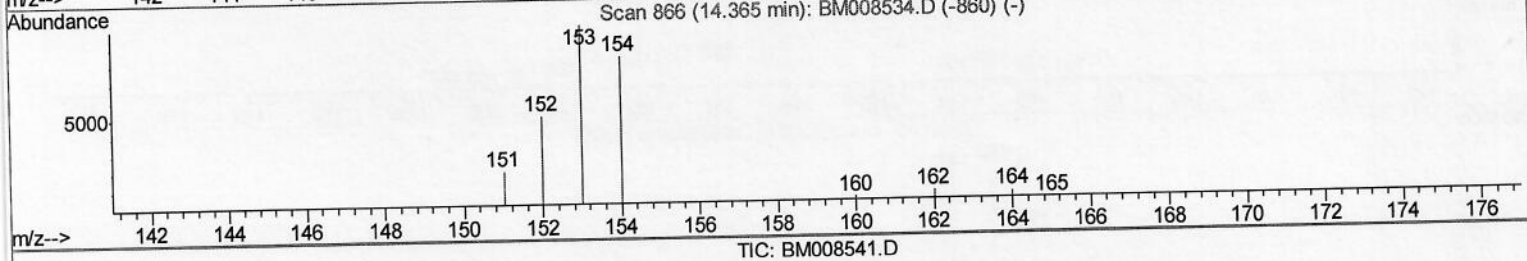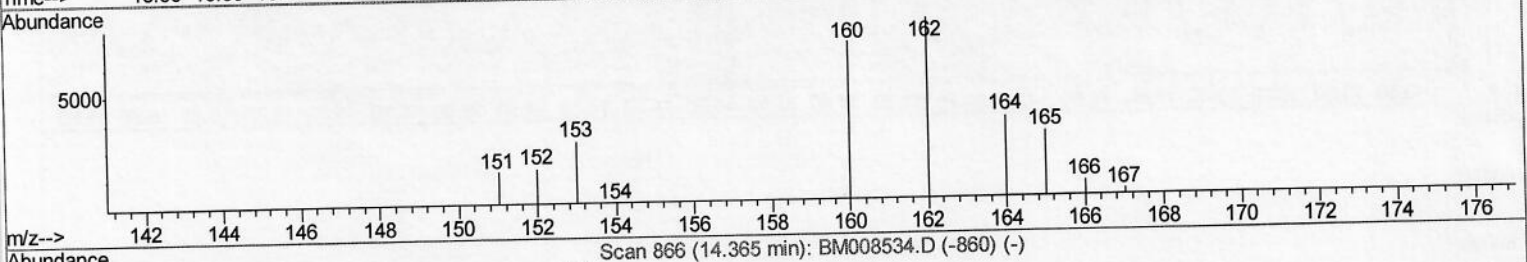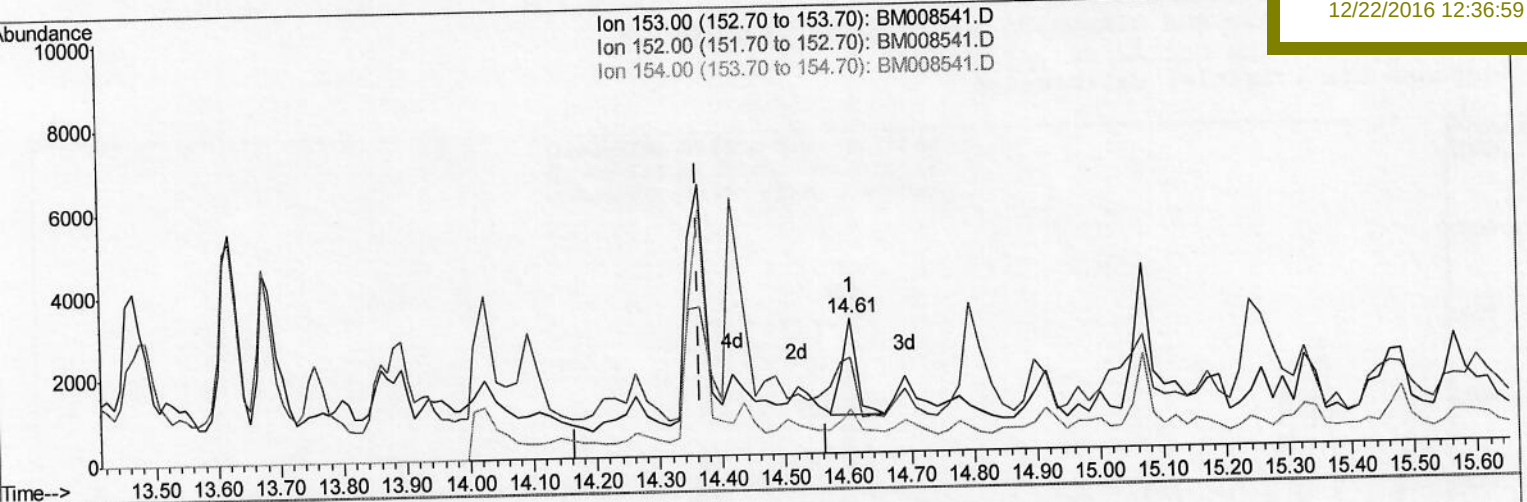

(8) Acenaphthene (C)

14.605min (+0.240) 0.04ng/ul

response 3819

Ion	Exp%	Act%
153.00	100	100
152.00	50.40	69.94#
154.00	89.30	31.34#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DA8T3

Manual Integrations
APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:04:37 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

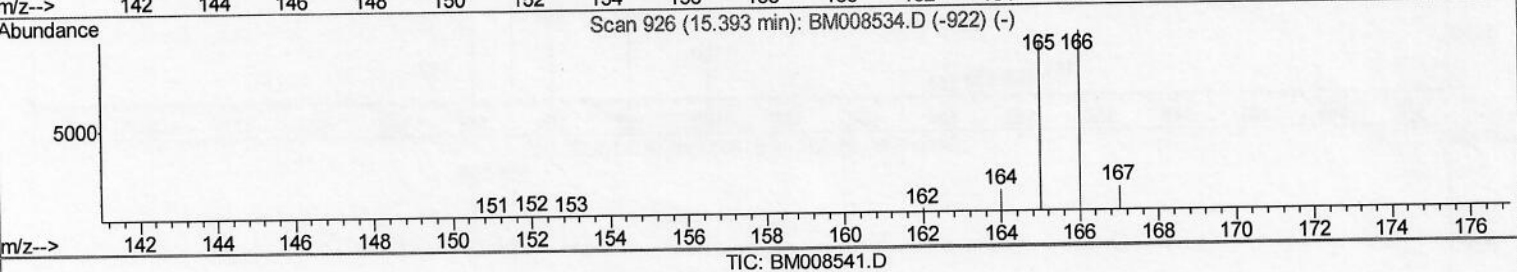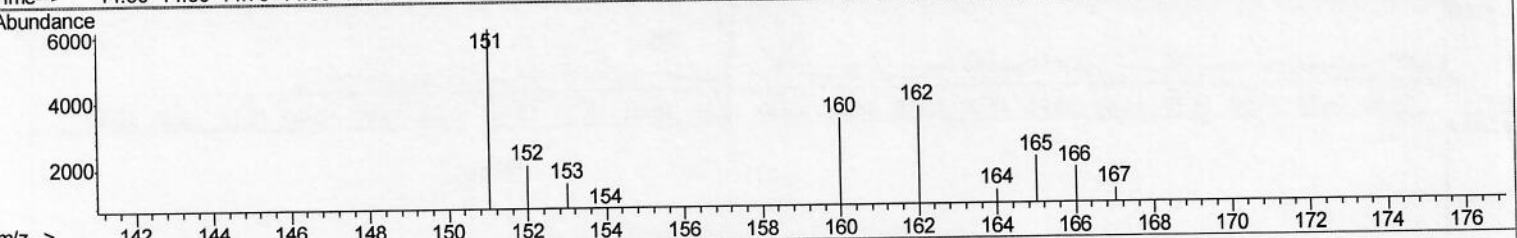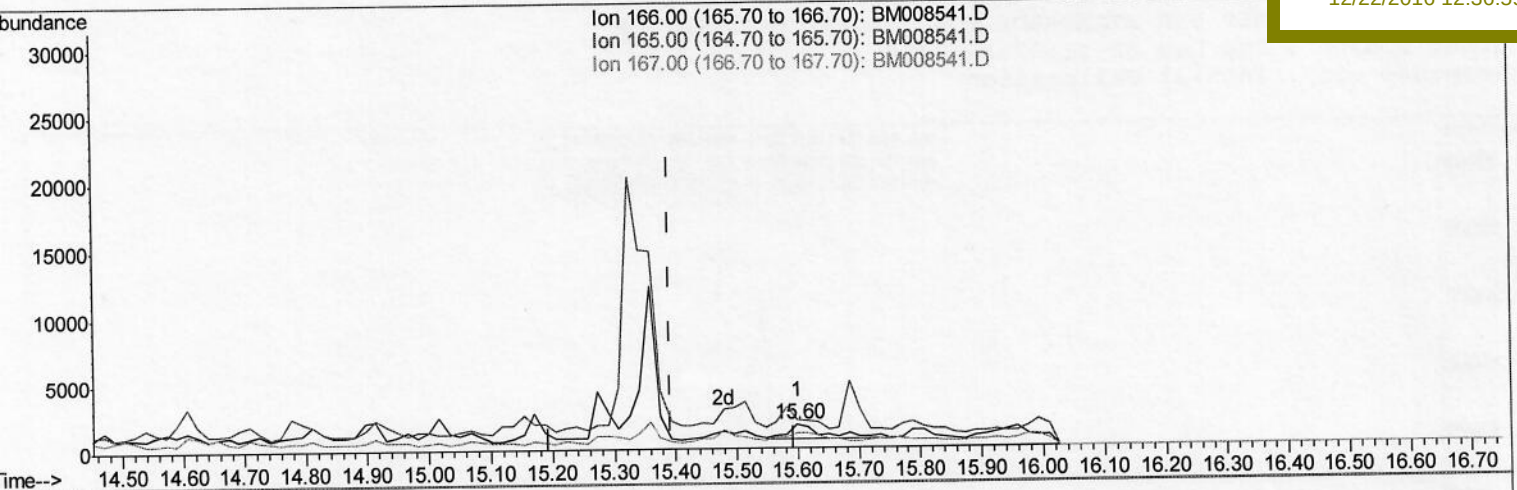

(9) Fluorene

15.599min (+0.206) 0.04ng/ul

response 4522

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	118.15#
167.00	18.30	62.70#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DA8T3

Manual Integrations
APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:04:37 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

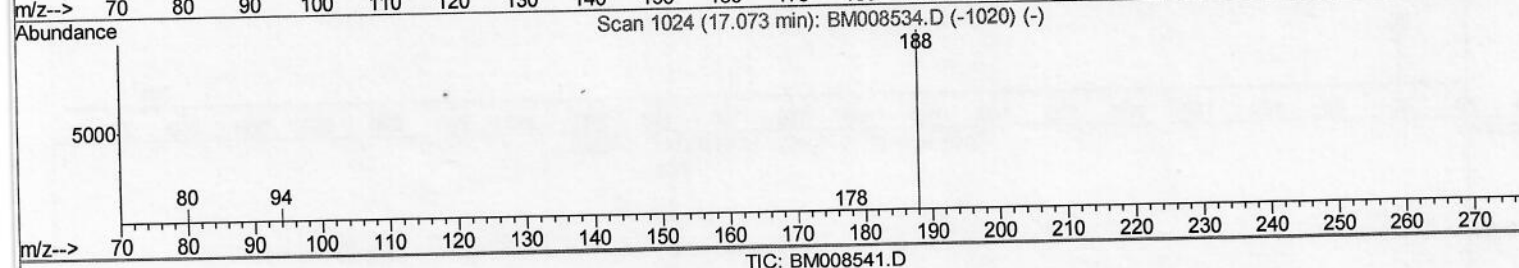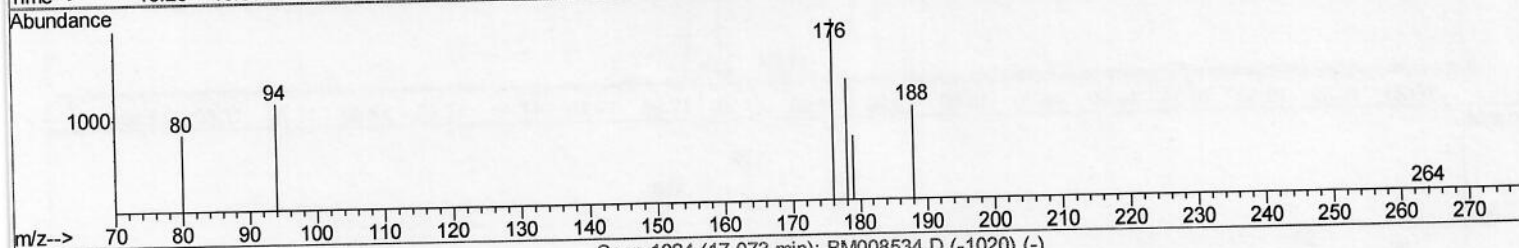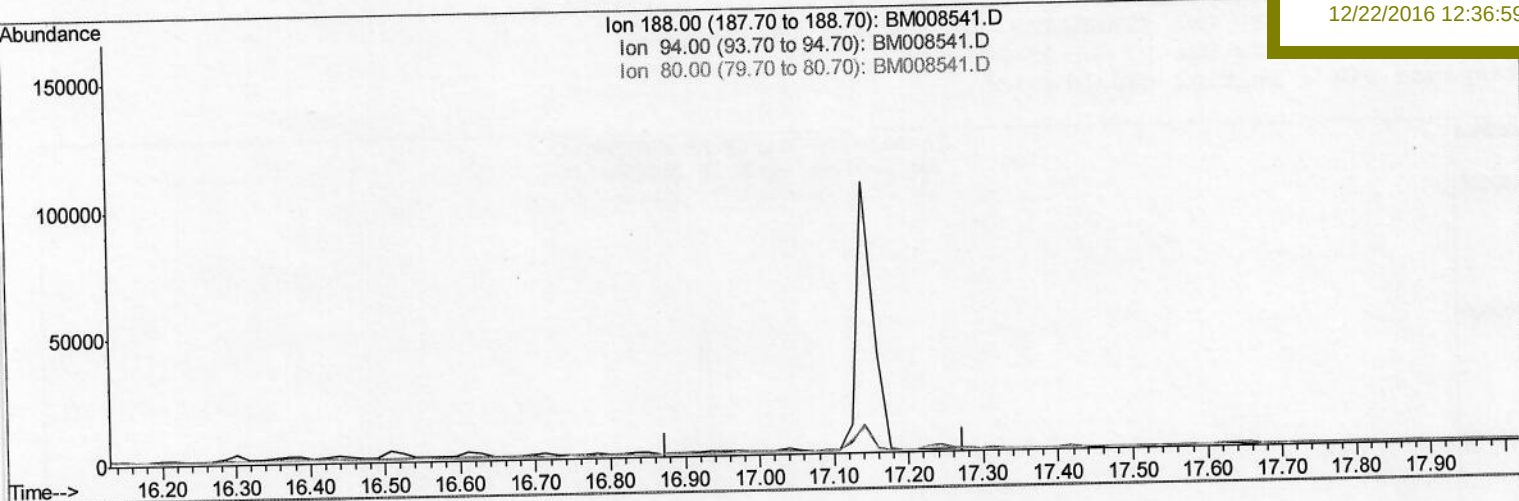

(10) Phenanthrene-d10 (I)

17.073min (-17.073) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DA8T3

Quant Time: Dec 22 11:05:53 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
 12/22/2016 12:36:59 PM

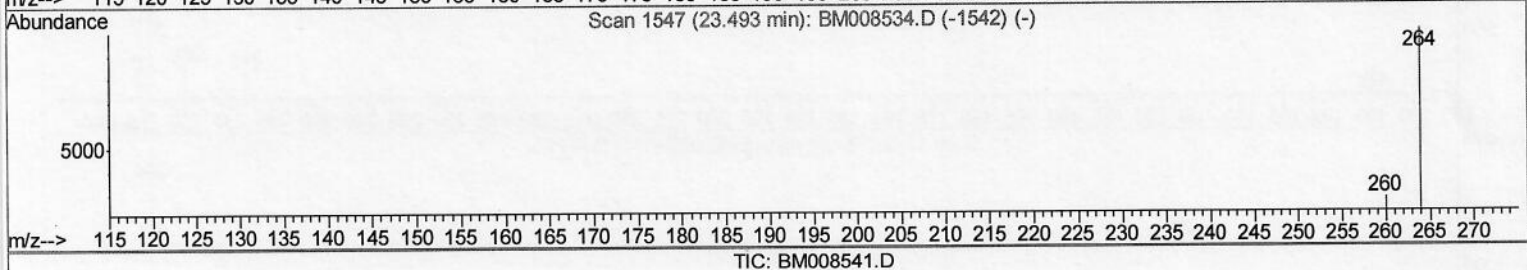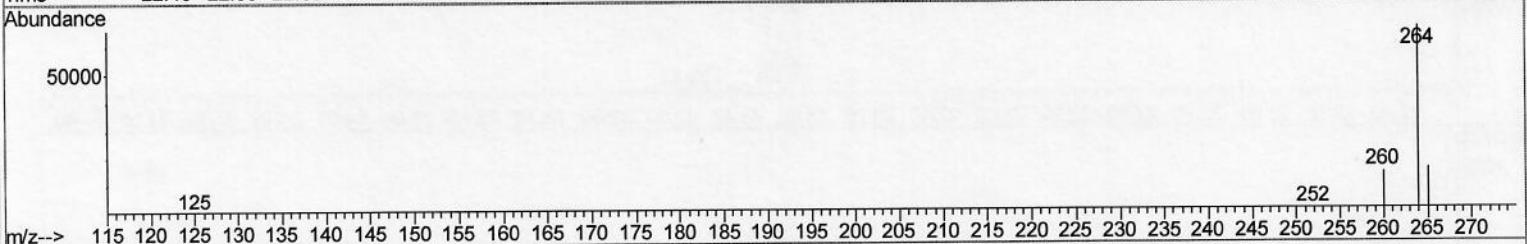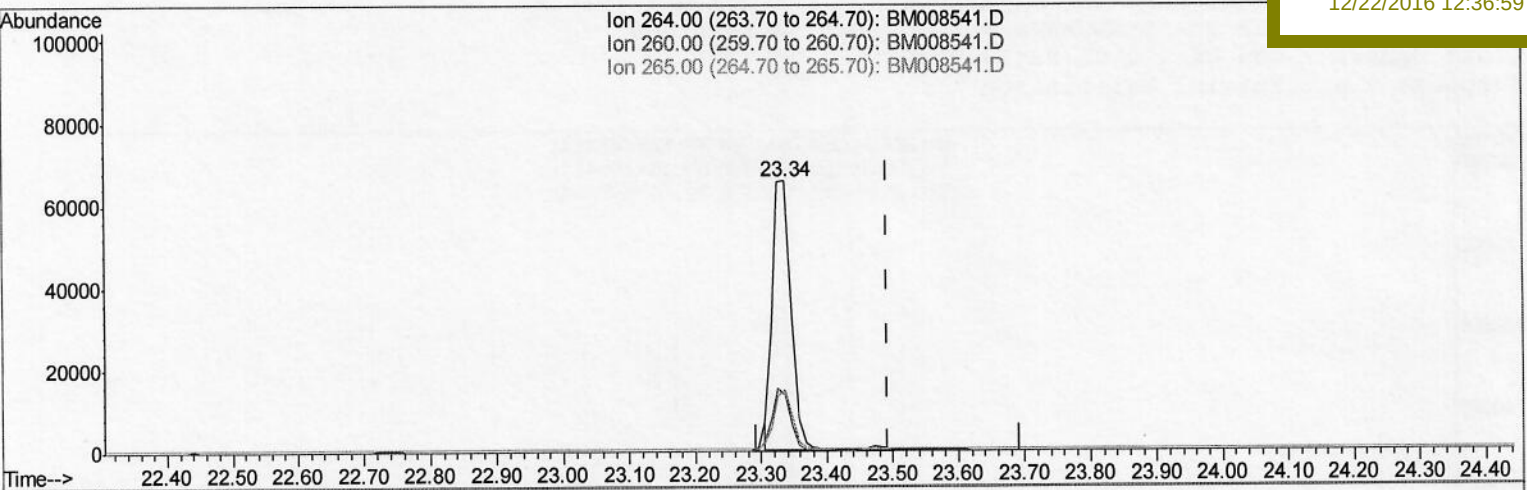

TIC: BM008541.D

(20) Perylene-d12 (I)

23.337min (-0.156) 0.40ng/ul

response 126468

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.93#
265.00	103.50	22.80#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:07:03 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

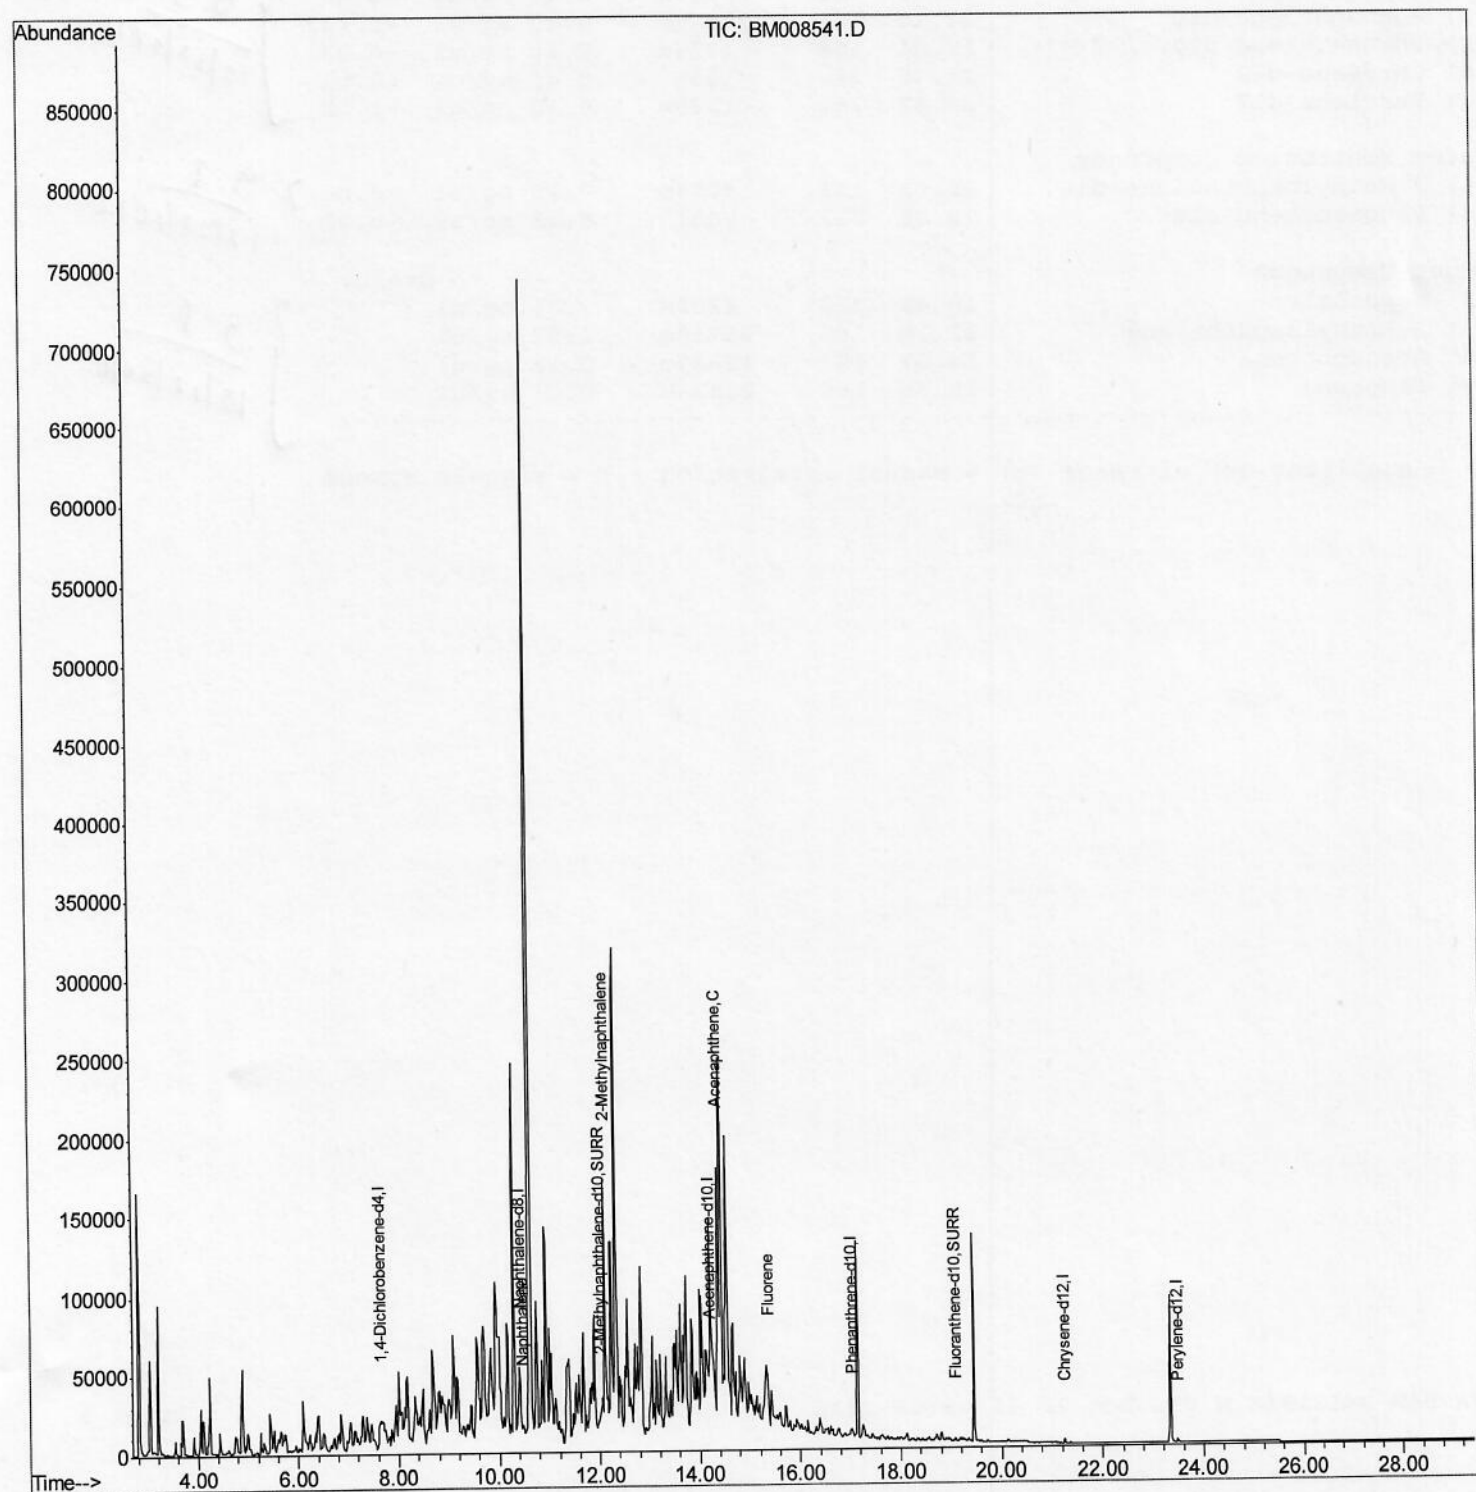

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
Data File : BM008541.D
Acq On : 22 Dec 2016 05:37
Operator : UM/SJ
Sample : H6039-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 22 11:07:03 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 02:22:34 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DA8T3

Manual Integrations
APPROVED

Sohil
12/22/2016 12:36:59 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	509m	0.40	ng/ul	-0.05
2) Naphthalene-d8	10.42	136	32465m	0.40	ng/ul	-0.06
6) Acenaphthene-d10	14.18	164	27800m	0.40	ng/ul	-0.14
10) Phenanthrene-d10	17.04	188	4778m	0.40	ng/ul	-0.03
16) Chrysene-d12	21.25	240	1935	0.40	ng/ul	-0.01
20) Perylene-d12	23.47	264	1575m	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	9077m	0.18	ng/ul	-0.06
14) Fluoranthene-d10	19.08	212	2001	0.15	ng/ul	-0.02
Target Compounds						
3) Naphthalene	10.48	128	4200m	0.05	ng/ul	Qvalue
5) 2-Methylnaphthalene	12.10	142	96730m	1.57	ng/ul	
8) Acenaphthene	14.37	153	12527m	0.13	ng/ul	
9) Fluorene	15.36	166	22924m	0.21	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:05:53 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

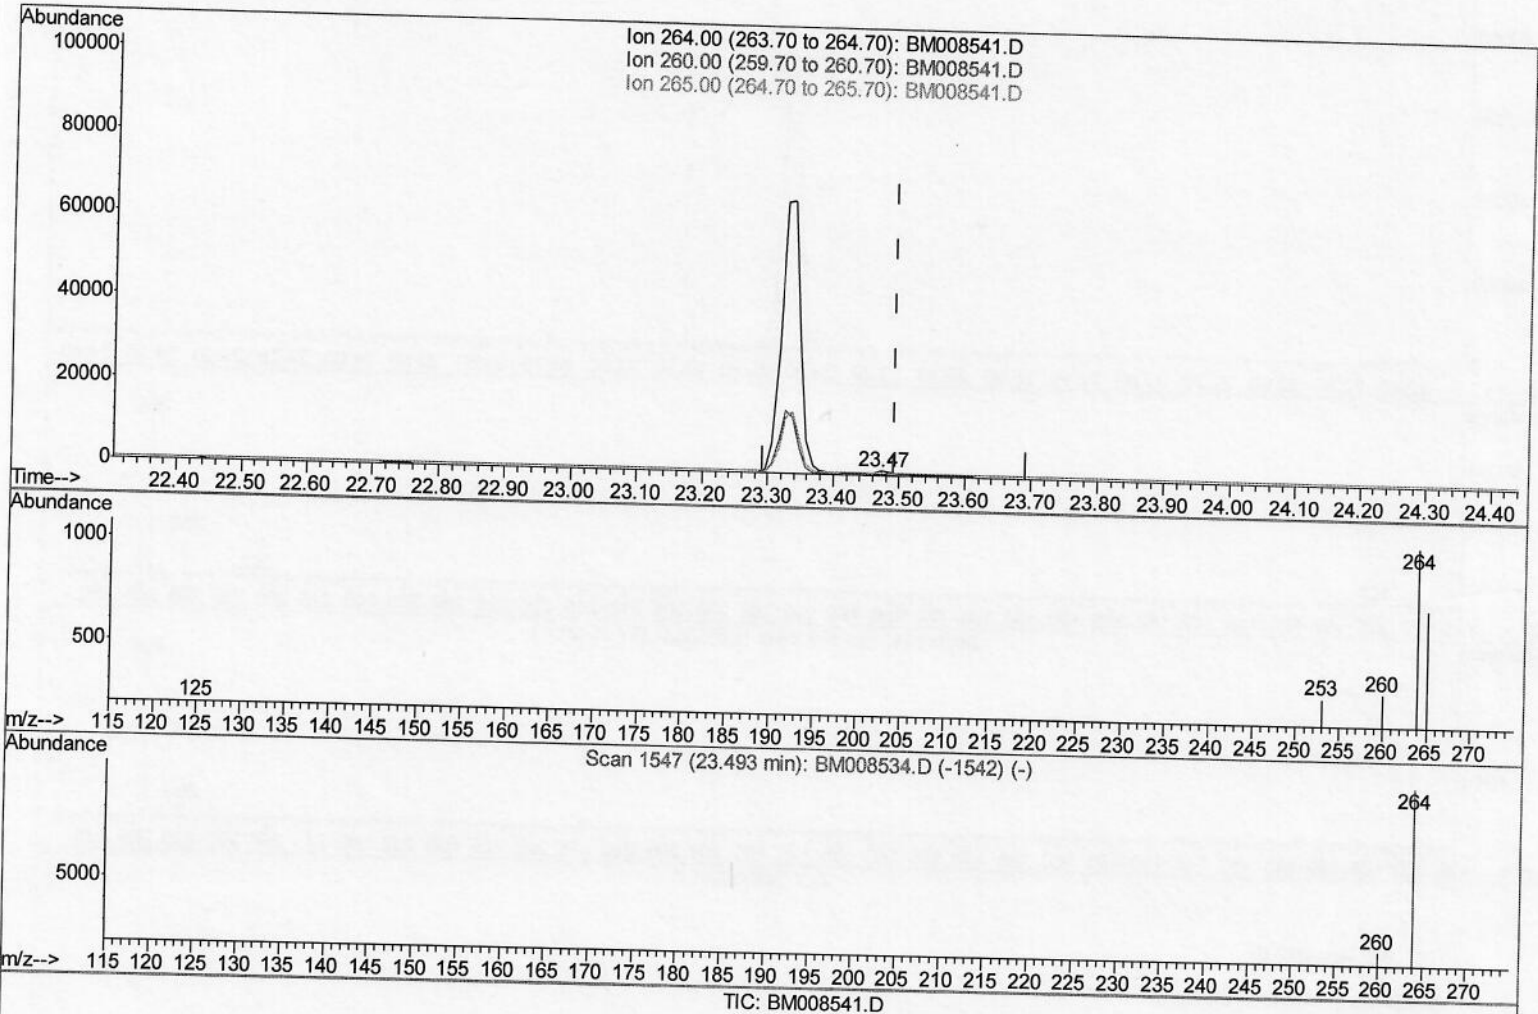

(20) Perylene-d12 (I)

23.472min (-0.021) 0.40ng/ul m

response 1575

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	32.99
265.00	103.50	71.16#
0.00	0.00	0.00

9.7
 12/22/2016

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:04:37 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

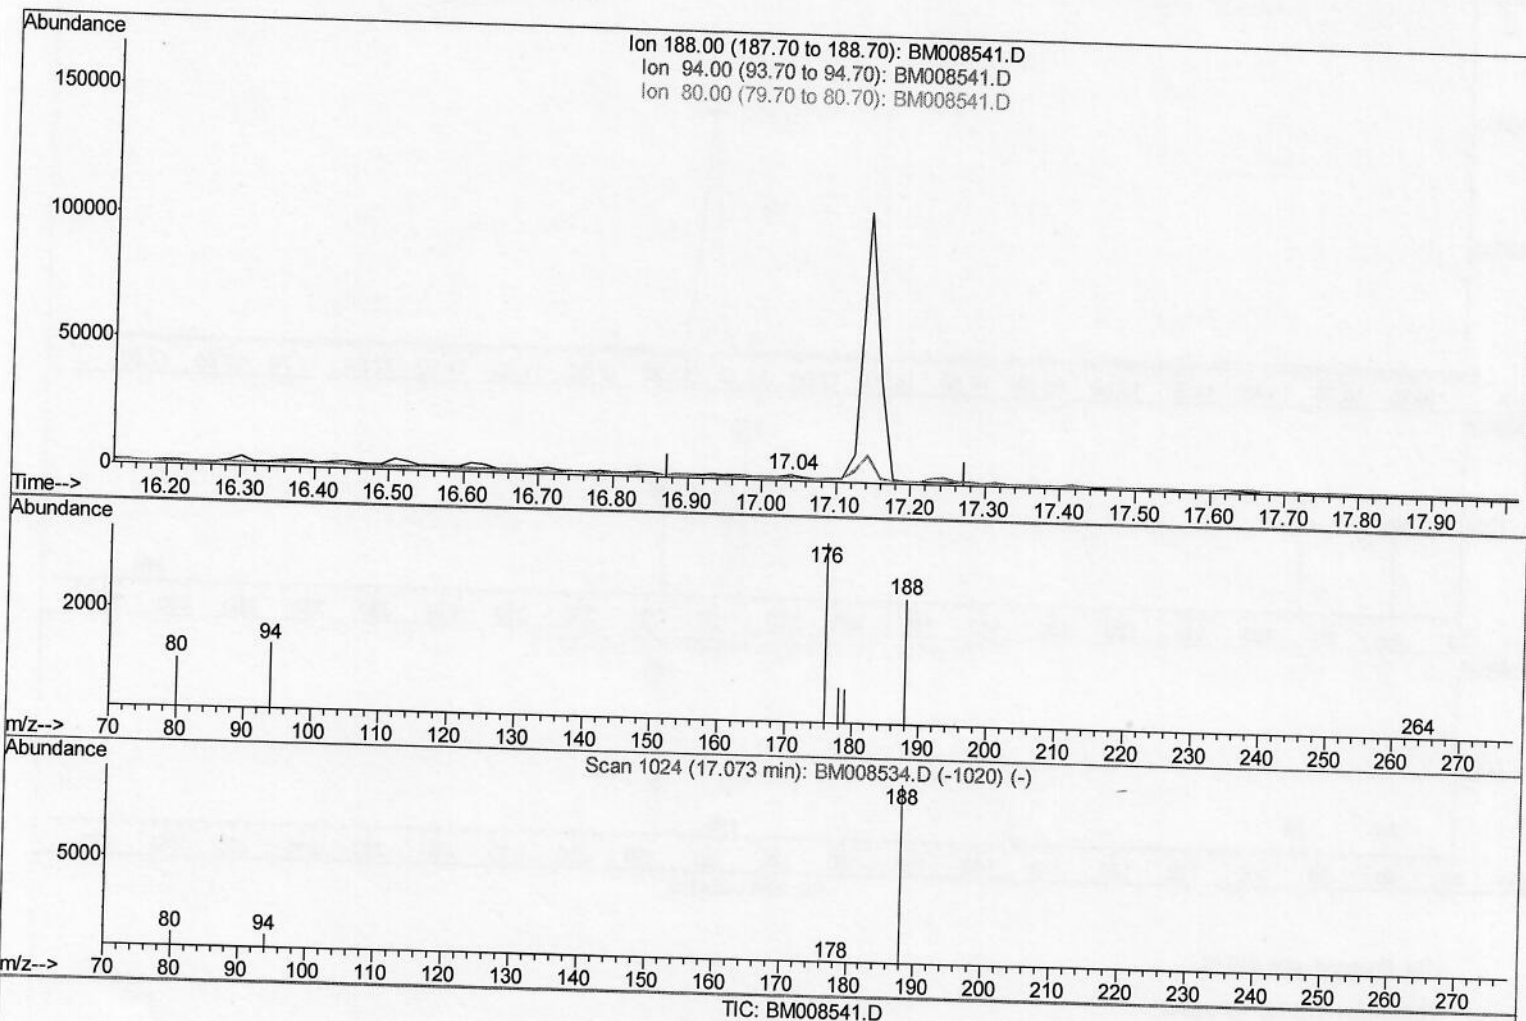

(10) Phenanthrene-d10 (I)

17.039min (-0.034) 0.40ng/ul m

response 4778

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	52.92#
80.00	11.80	40.99#
0.00	0.00	0.00

59.3
 12/22/2016

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:04:37 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

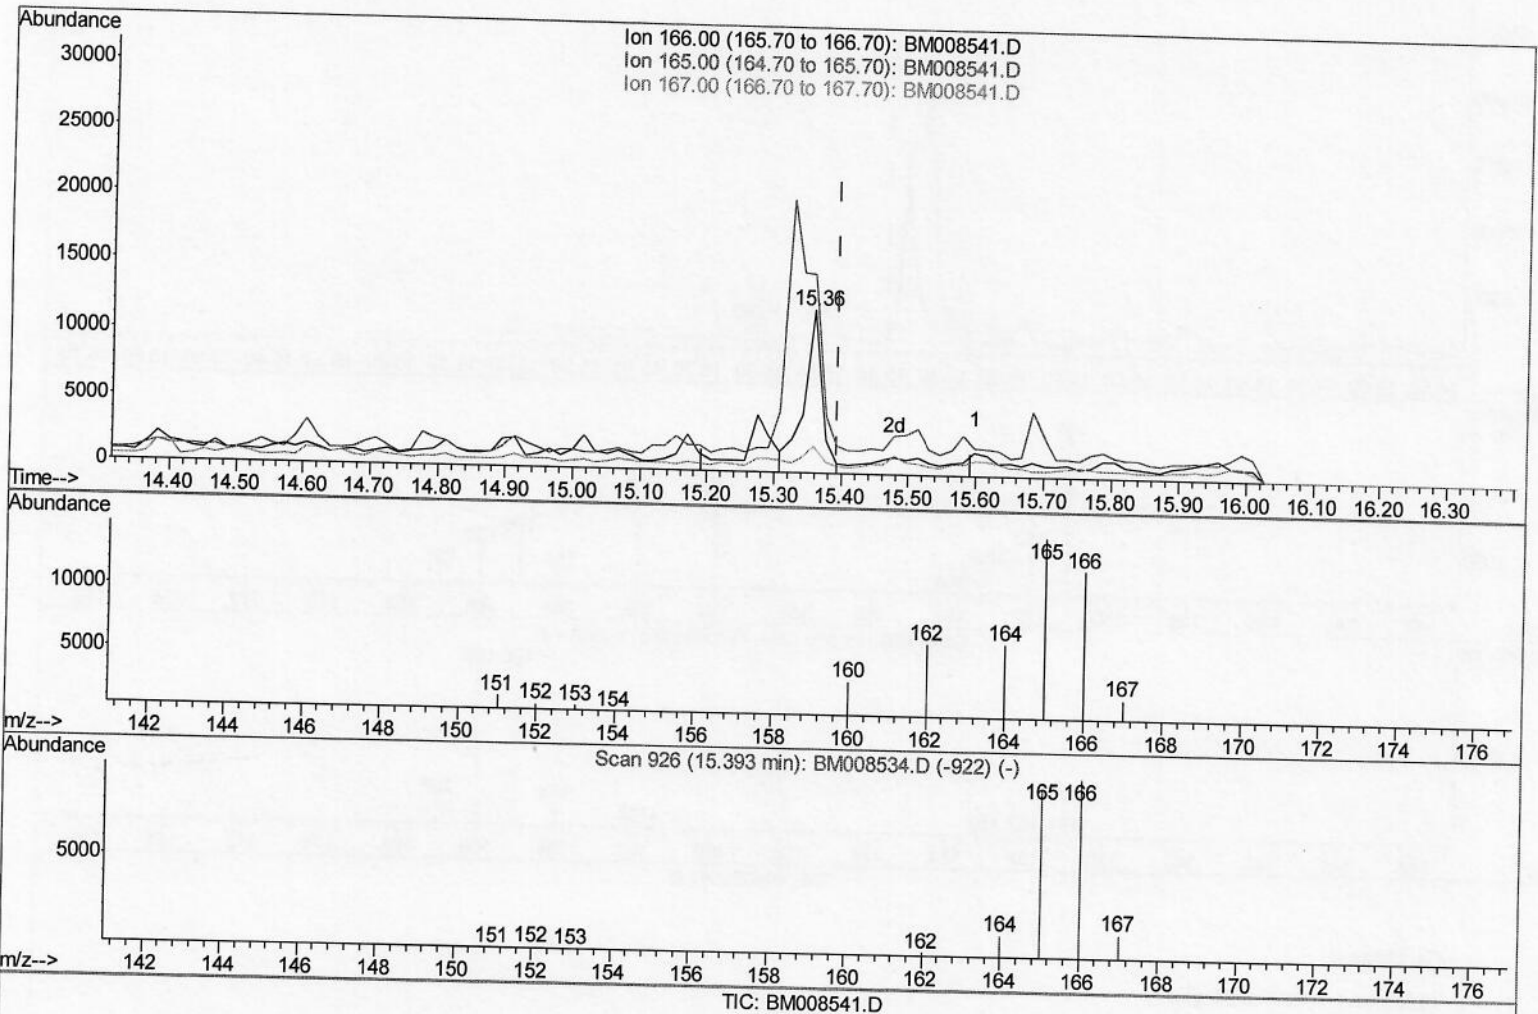

(9) Fluorene

15.359min (-0.034) 0.21ng/ul m > 5.1
 response 22924
 12/22/2016

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	121.10#
167.00	18.30	16.89
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:04:37 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

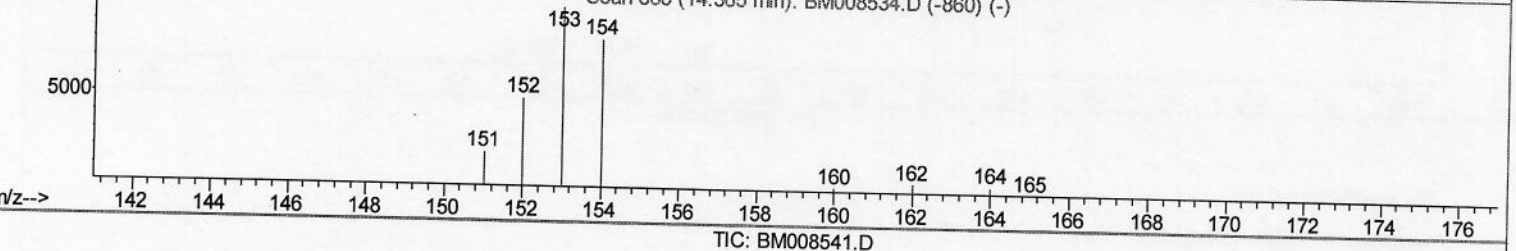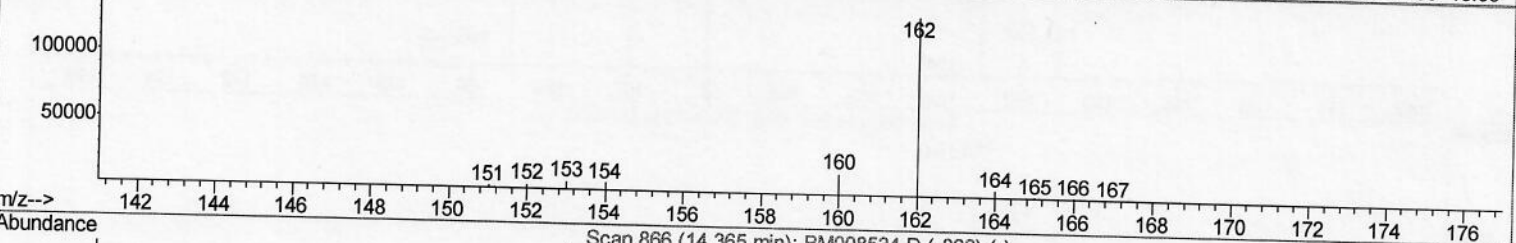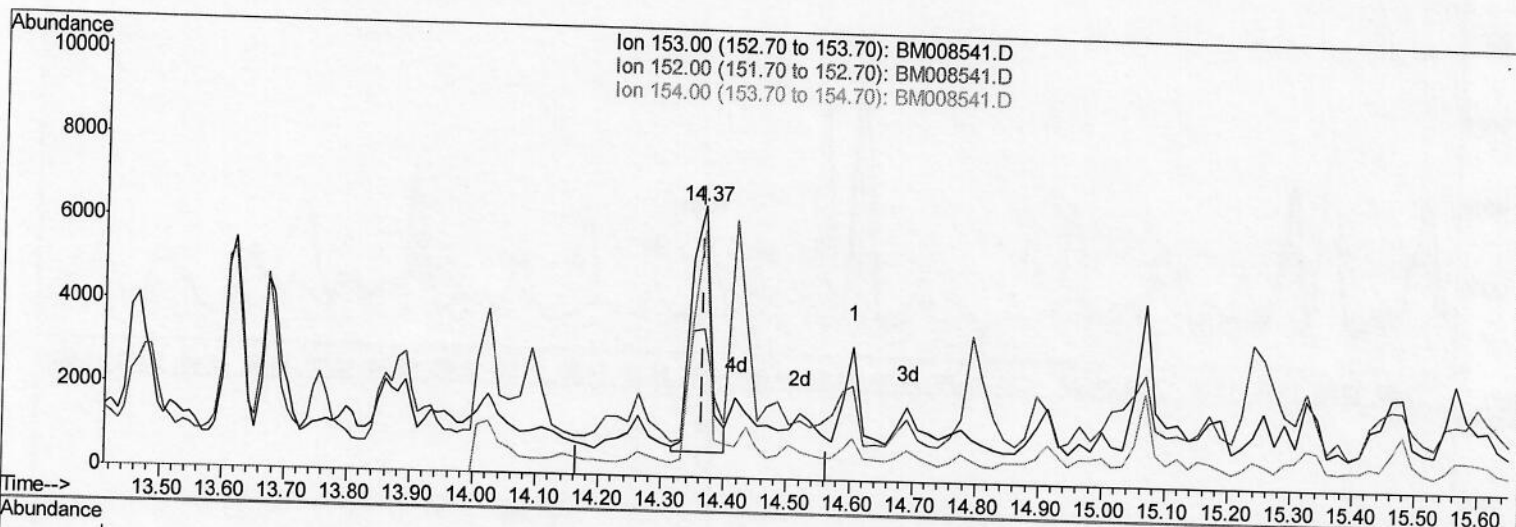

(8) Acenaphthene (C)

14.366min (+0.000) 0.13ng/ul m

response 12527

Ion	Exp%	Act%
153.00	100	100
152.00	50.40	54.72
154.00	89.30	90.98
0.00	0.00	0.00

9.7
 12/22/2016

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:07:03 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

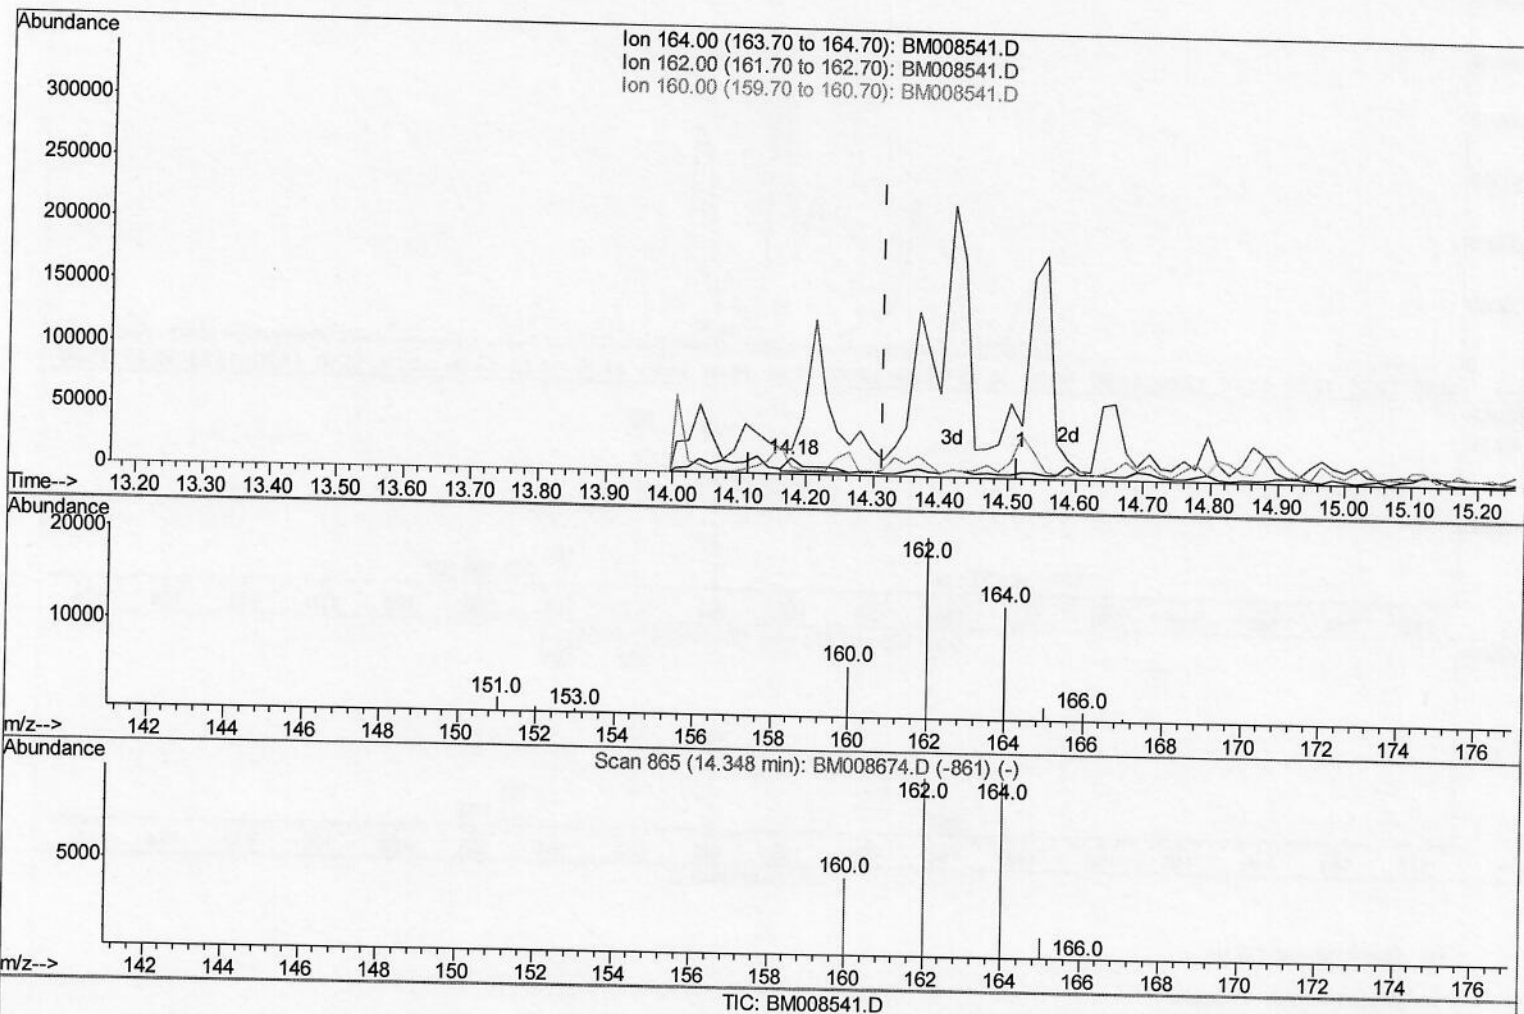

(6) Acenaphthene-d10 (I)

14.177min (-0.137) 0.40ng/ul m

response 27800

Ion	Exp%	Act%
164.00	100	100
162.00	98.60	158.29#
160.00	48.80	46.84
0.00	0.00	0.00

75.1
 12/22/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:01:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

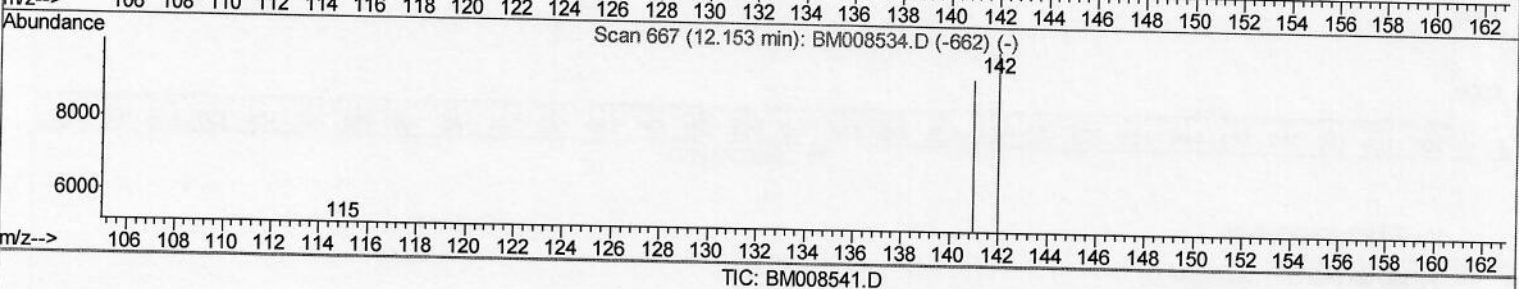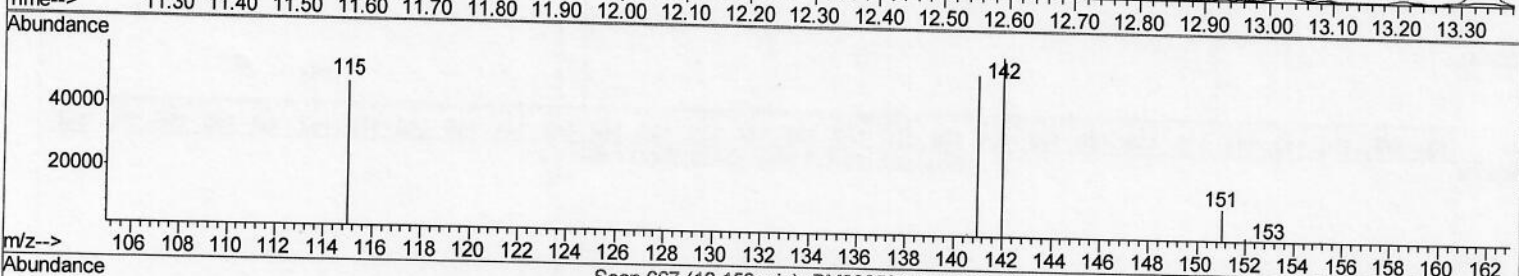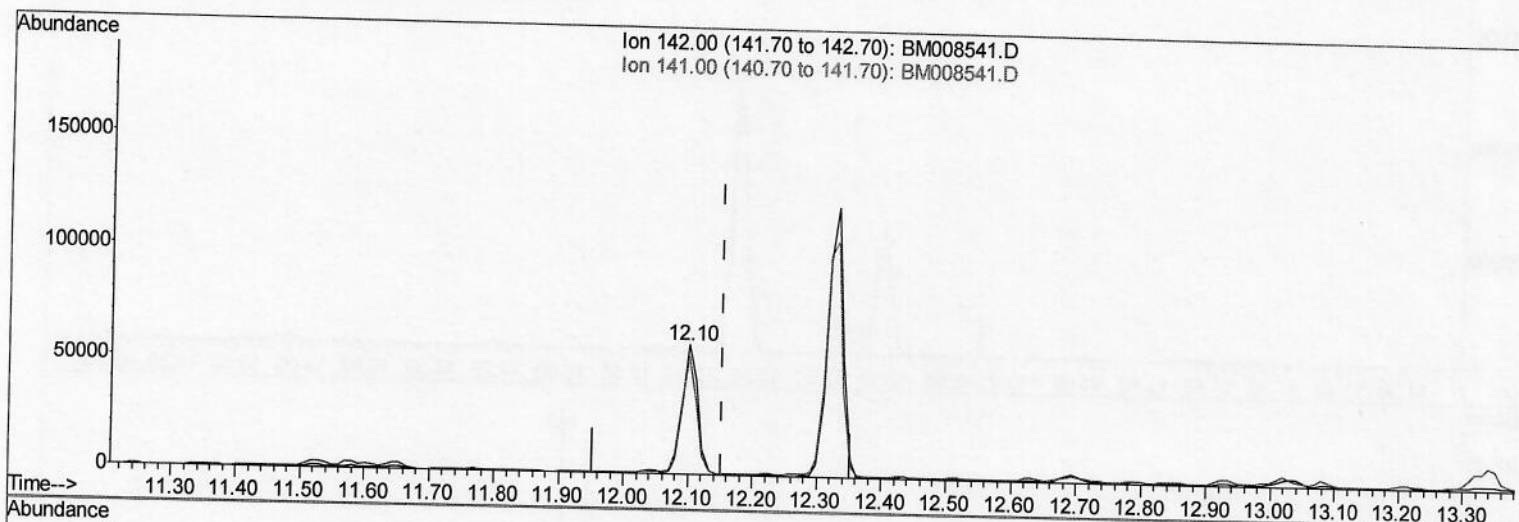

TIC: BM008541.D

(5) 2-Methylnaphthalene

12.101min (-0.052) 1.57ng/ul m

response 96730

Ion	Exp%	Act%
142.00	100	100
141.00	90.70	192.80#
0.00	0.00	0.00
0.00	0.00	0.00

> 9.7
 12/22/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:01:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

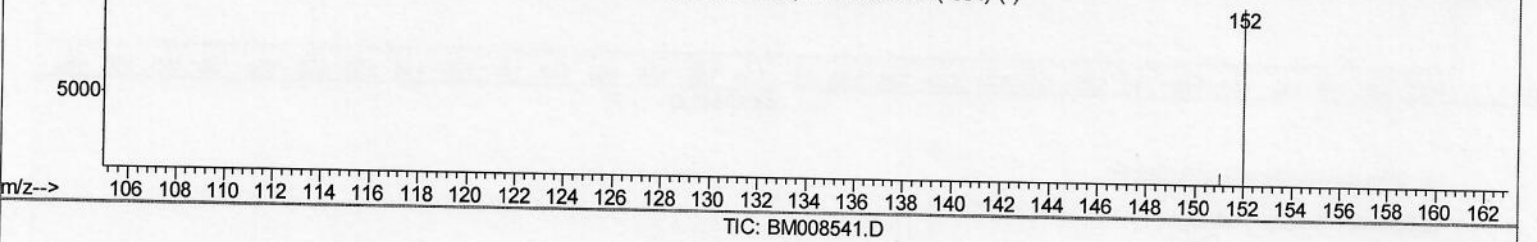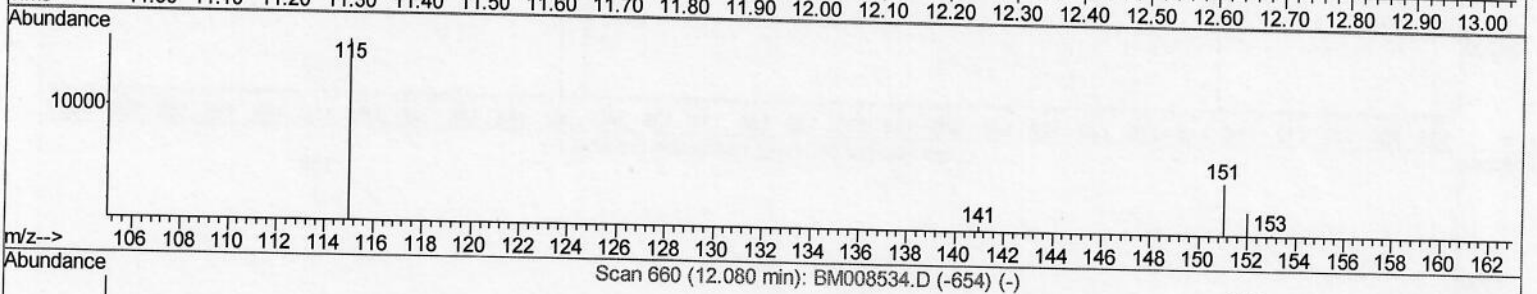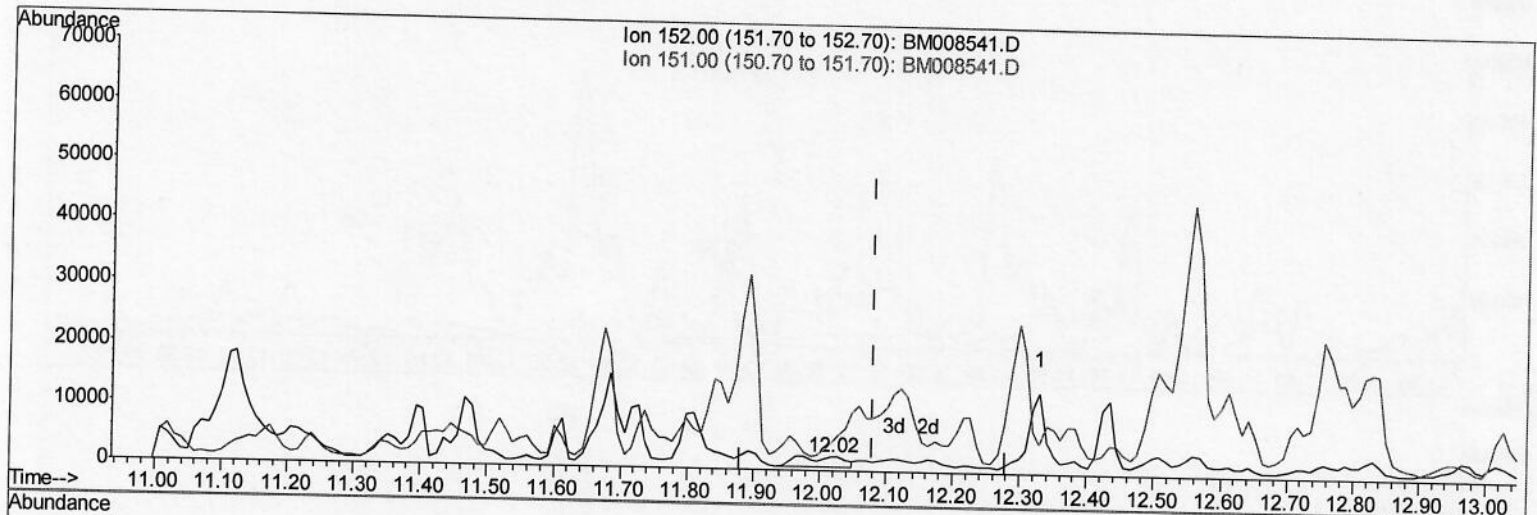

(4) 2-Methylnaphthalene-d10 (SURR)

12.018min (-0.062) 0.18ng/ul m

response 9077

Ion	Exp%	Act%
152.00	100	100
151.00	19.30	180.25#
0.00	0.00	0.00
0.00	0.00	0.00

> 5.7
 12/22/2016

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:01:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

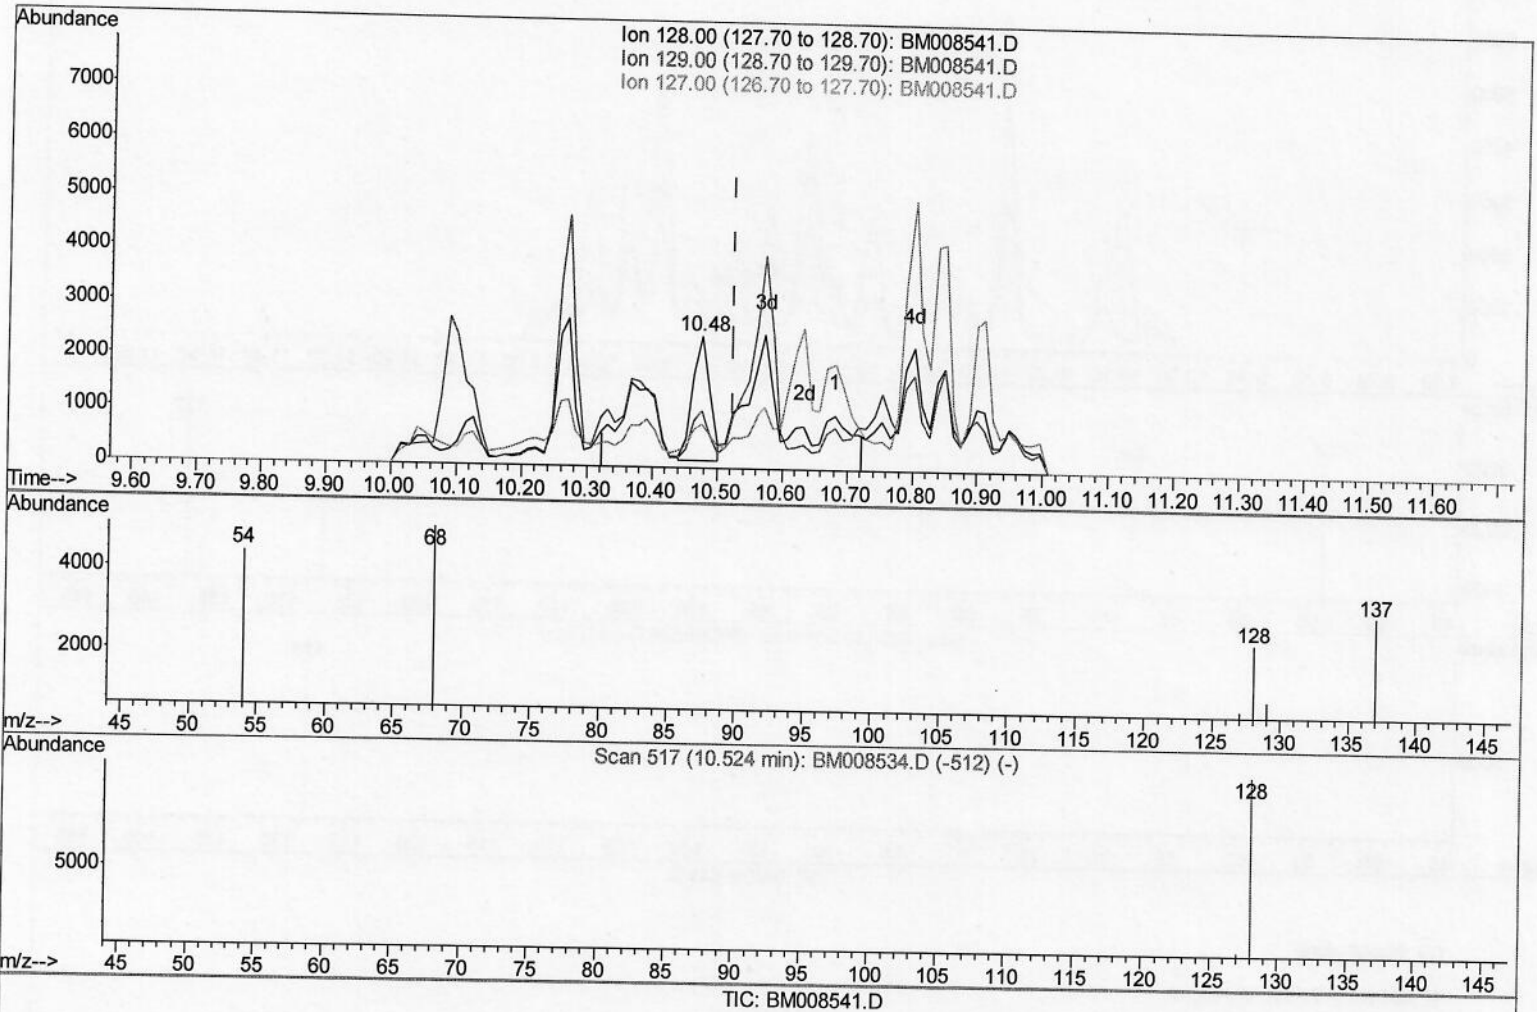

(3) Naphthalene

10.476min (-0.048) 0.05ng/ul m

response 4200

Ion	Exp%	Act%
128.00	100	100
129.00	14.10	42.90#
127.00	16.00	33.35#
0.00	0.00	0.00

> 5.7
 12/22/2016

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:01:03 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

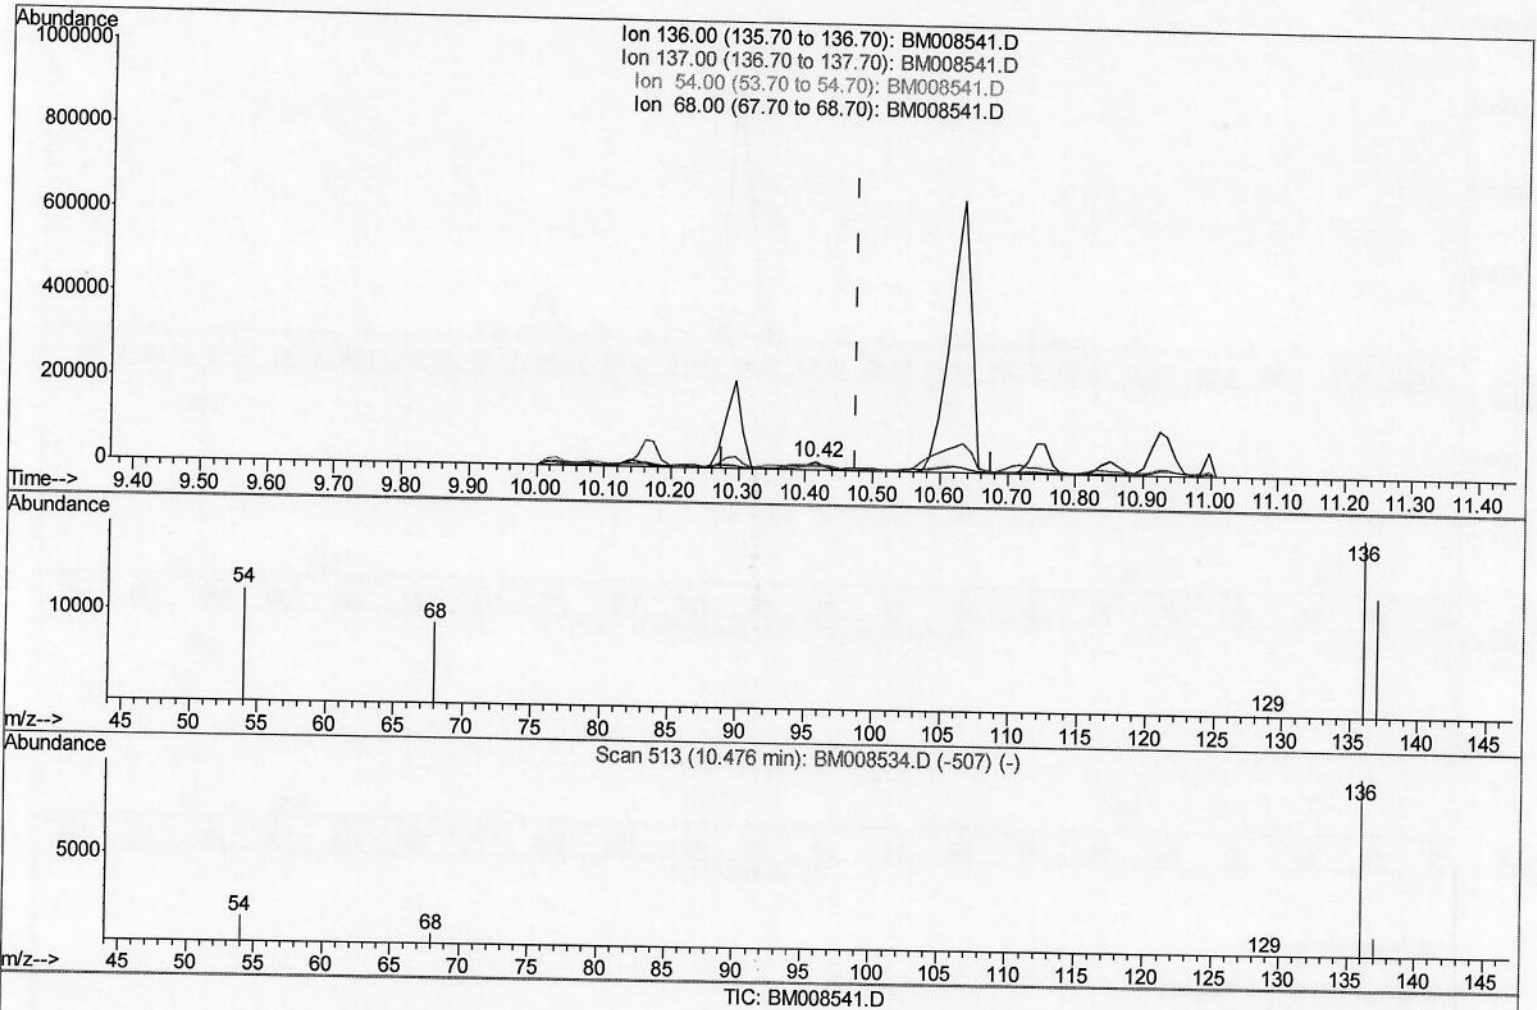

(2) Naphthalene-d8 (I)

10.415min (-0.060) 0.40ng/ul m

response 32465

Ion	Exp%	Act%
136.00	100	100
137.00	13.90	67.49#
54.00	15.50	63.95#
68.00	9.90	46.17#

79.7
 12/22/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122116\
 Data File : BM008541.D
 Acq On : 22 Dec 2016 05:37
 Operator : UM/SJ
 Sample : H6039-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DA8T3

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:59 PM

Quant Time: Dec 22 11:00:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

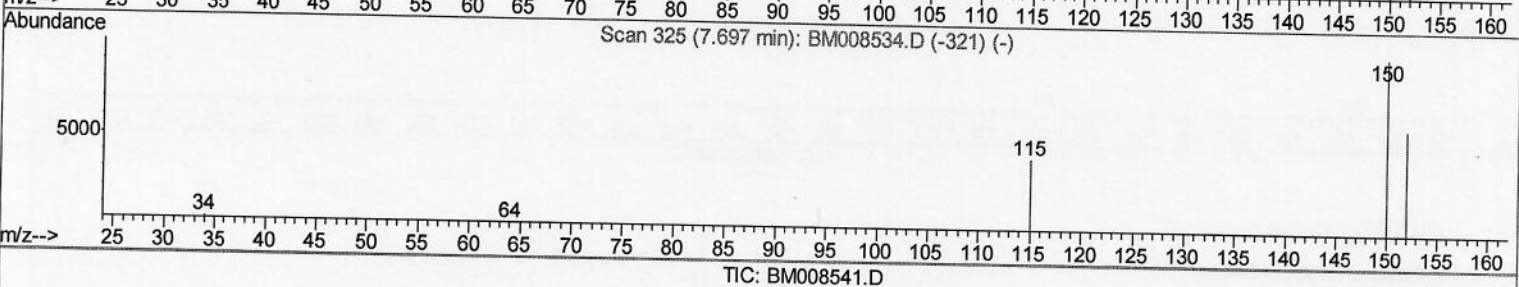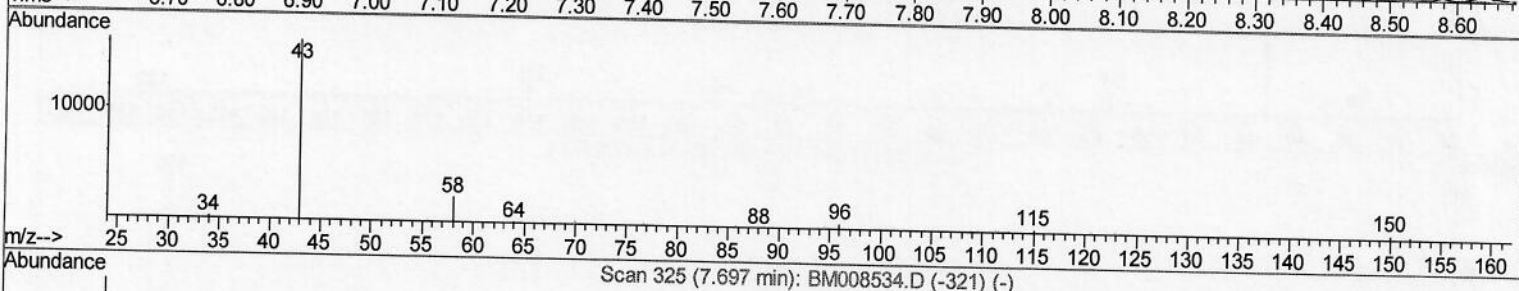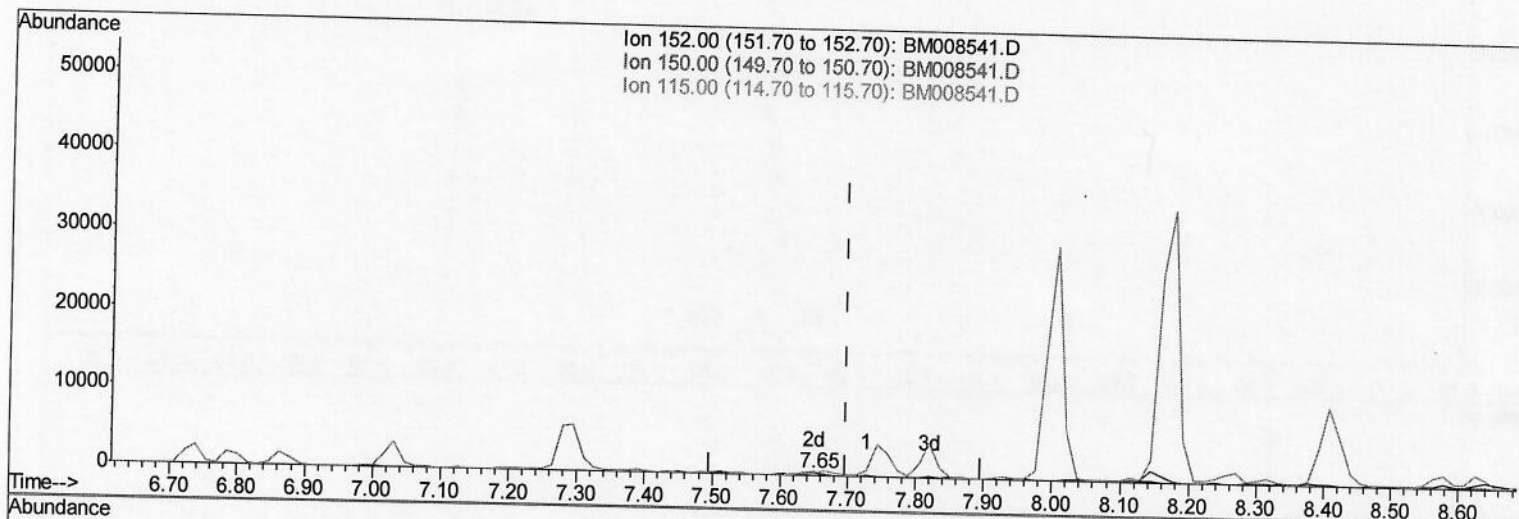

(1) 1,4-Dichlorobenzene-d4 (I)

7.650min (-0.046) 0.40ng/ul m

response 509

Ion Exp% Act%

152.00 100 100

150.00 143.40 137.61

115.00 64.90 109.48#

0.00 0.00 0.00

> 5.1
 12/22/2016