

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
 Data File : BM008528.D
 Acq On : 21 Dec 2016 21:48
 Operator : UM/SJ
 Sample : H5995-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA865

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:12 PM

Quant Time: Dec 22 01:24:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 00:24:45 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	418	0.40	ng/ul	-0.09
2) Naphthalene-d8	10.42	136	1370	0.40	ng/ul	-0.08
6) Acenaphthene-d10	14.28	164	856	0.40	ng/ul	-0.05
10) Phenanthrene-d10	17.04	188	1681m	0.40	ng/ul	-0.05
16) Chrysene-d12	21.26	240	1507	0.40	ng/ul	-0.02
20) Perylene-d12	23.48	264	1361m	0.40	ng/ul	-0.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	1059	0.50	ng/ul	-0.07
14) Fluoranthene-d10	19.08	212	2262m	0.49	ng/ul	-0.04
Target Compounds						
5) 2-Methylnaphthalene	12.11	142	140	0.05	ng/ul	Qvalue 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008528.D
Acq On : 21 Dec 2016 21:48
Operator : UM/SJ
Sample : H5995-04
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DA865

Manual Integrations
APPROVED

Sohil
12/22/2016 12:36:12 PM

Quant Time: Dec 22 01:24:49 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 00:24:45 2016
Response via : Initial Calibration

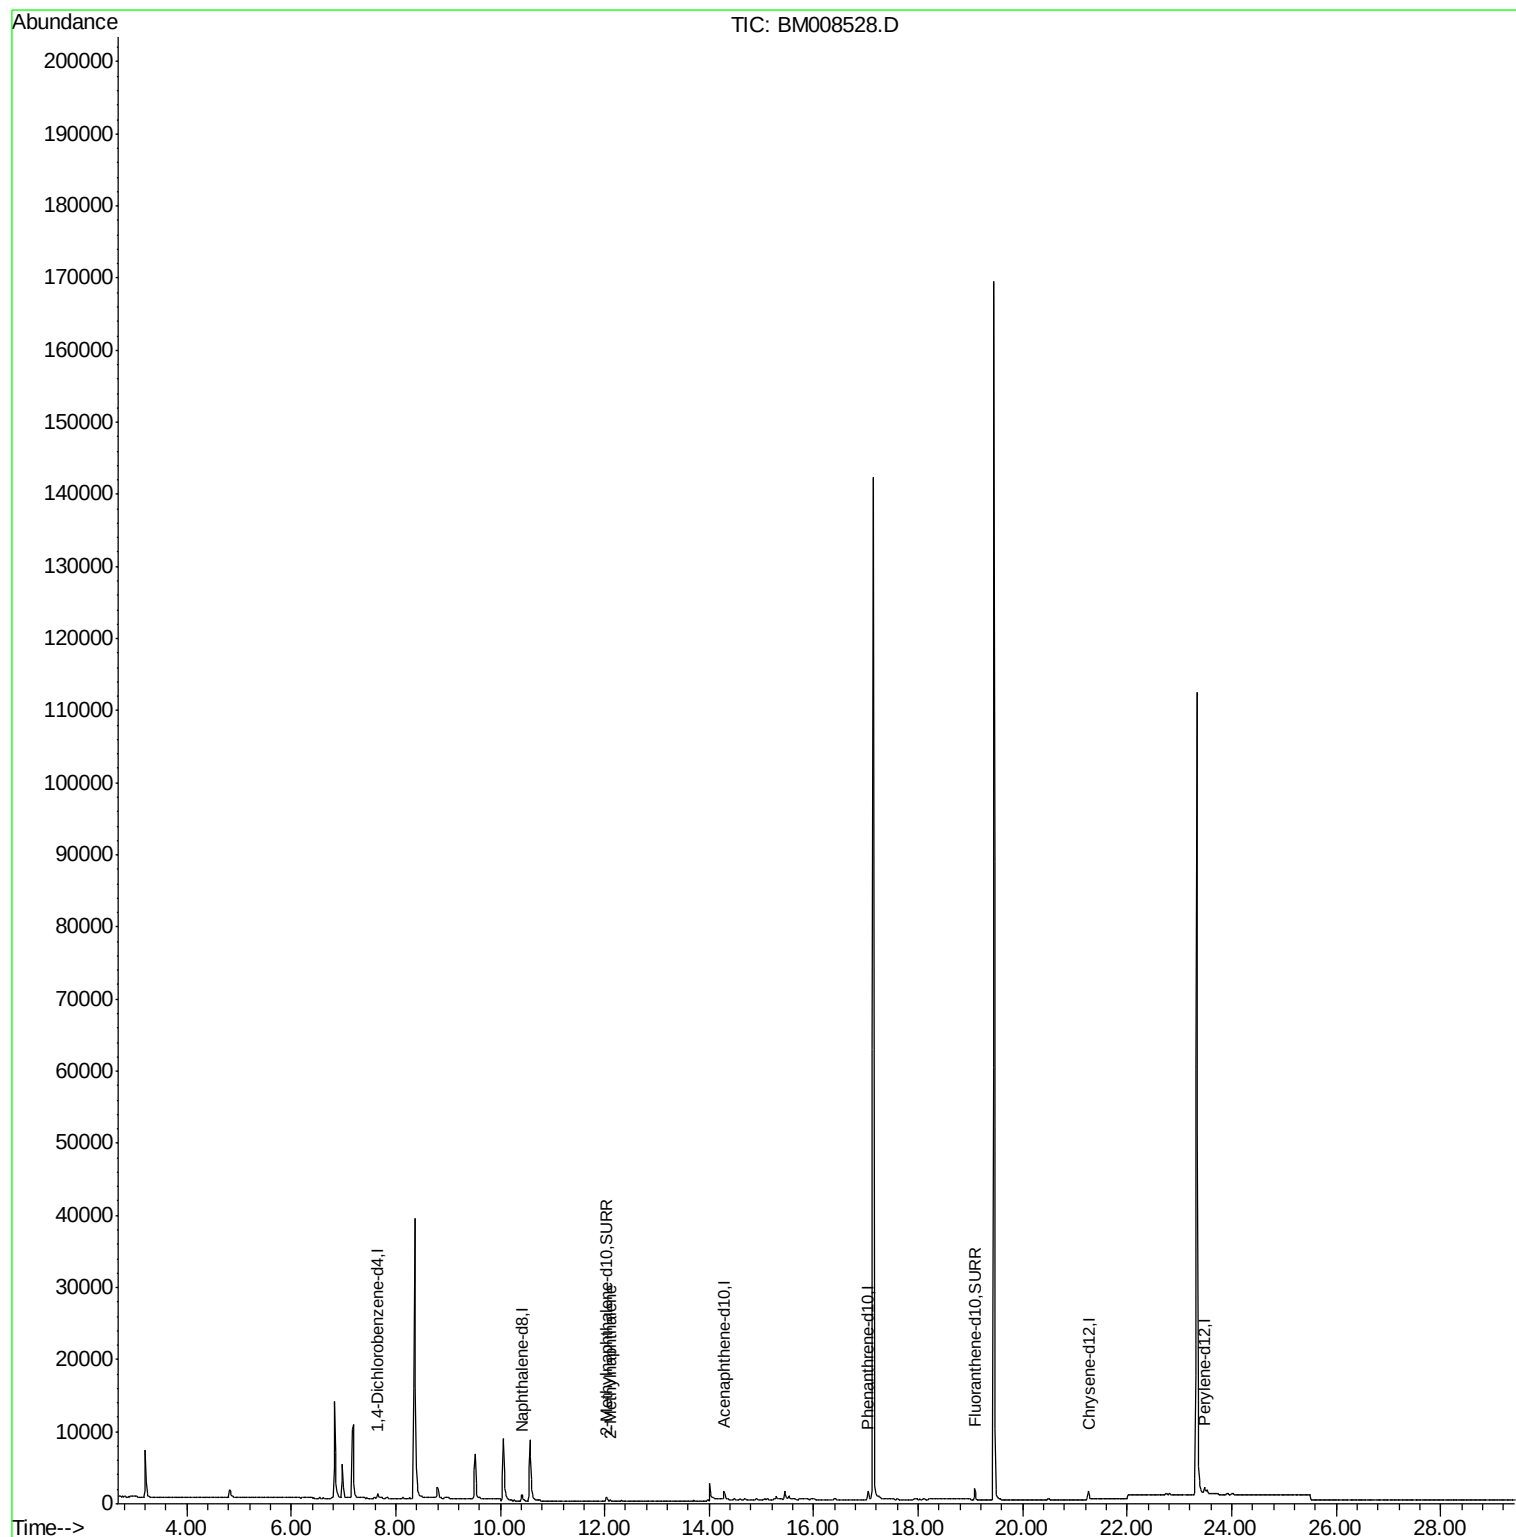

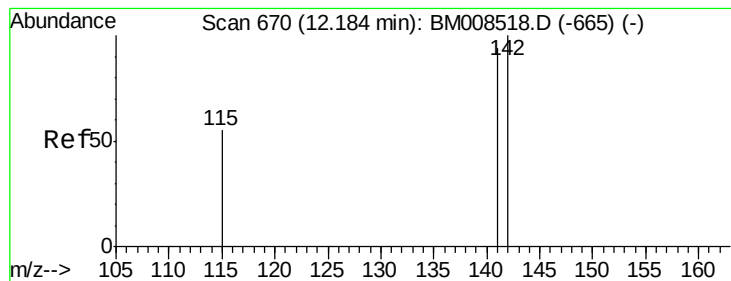

#5

2-Methylnaphthalene

Concen: 0.05 ng/ul

RT: 12.11 min Scan# 663

Delta R.T. -0.07 min

Lab File: BM008528.D

Acq: 21 Dec 2016 21:48

Instrument :

BNA_M

ClientSampleId :

DA865

Tgt Ion:142 Resp: 140

Ion Ratio Lower Upper

142 100

141 98.6 72.6 108.8

Manual Integrations

APPROVED

Sohil

12/22/2016 12:36:12 PM

