

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
 Data File : BM008542.D
 Acq On : 22 Dec 2016 06:13
 Operator : UM/SJ
 Sample : H6039-20
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8T4

Manual Integrations
 APPROVED

Sohil
 12/22/2016 12:36:36 PM

Quant Time: Dec 22 11:16:00 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:22:34 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	424	0.40	ng/ul	-0.05
2) Naphthalene-d8	10.42	136	1449m	0.40	ng/ul	-0.06
6) Acenaphthene-d10	14.28	164	1648m	0.40	ng/ul	-0.03
10) Phenanthrene-d10	17.04	188	2184m	0.40	ng/ul	-0.03
16) Chrysene-d12	21.25	240	1583m	0.40	ng/ul	-0.01
20) Perylene-d12	23.47	264	1347m	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	1154m	0.52	ng/ul	-0.07
14) Fluoranthene-d10	19.08	212	1805m	0.30	ng/ul	-0.02
Target Compounds						
3) Naphthalene	10.46	128	151282	37.11	ng/ul	93
5) 2-Methylnaphthalene	12.08	142	60349	21.99	ng/ul	100
8) Acenaphthene	14.35	153	10715m	1.91	ng/ul	
9) Fluorene	15.34	166	22231m	3.47	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122116\
Data File : BM008542.D
Acq On : 22 Dec 2016 06:13
Operator : UM/SJ
Sample : H6039-20
Misc :
ALS Vial : 34 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DA8T4

Manual Integrations
APPROVED

Sohil
12/22/2016 12:36:36 PM

Quant Time: Dec 22 11:16:00 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 02:22:34 2016
Response via : Initial Calibration

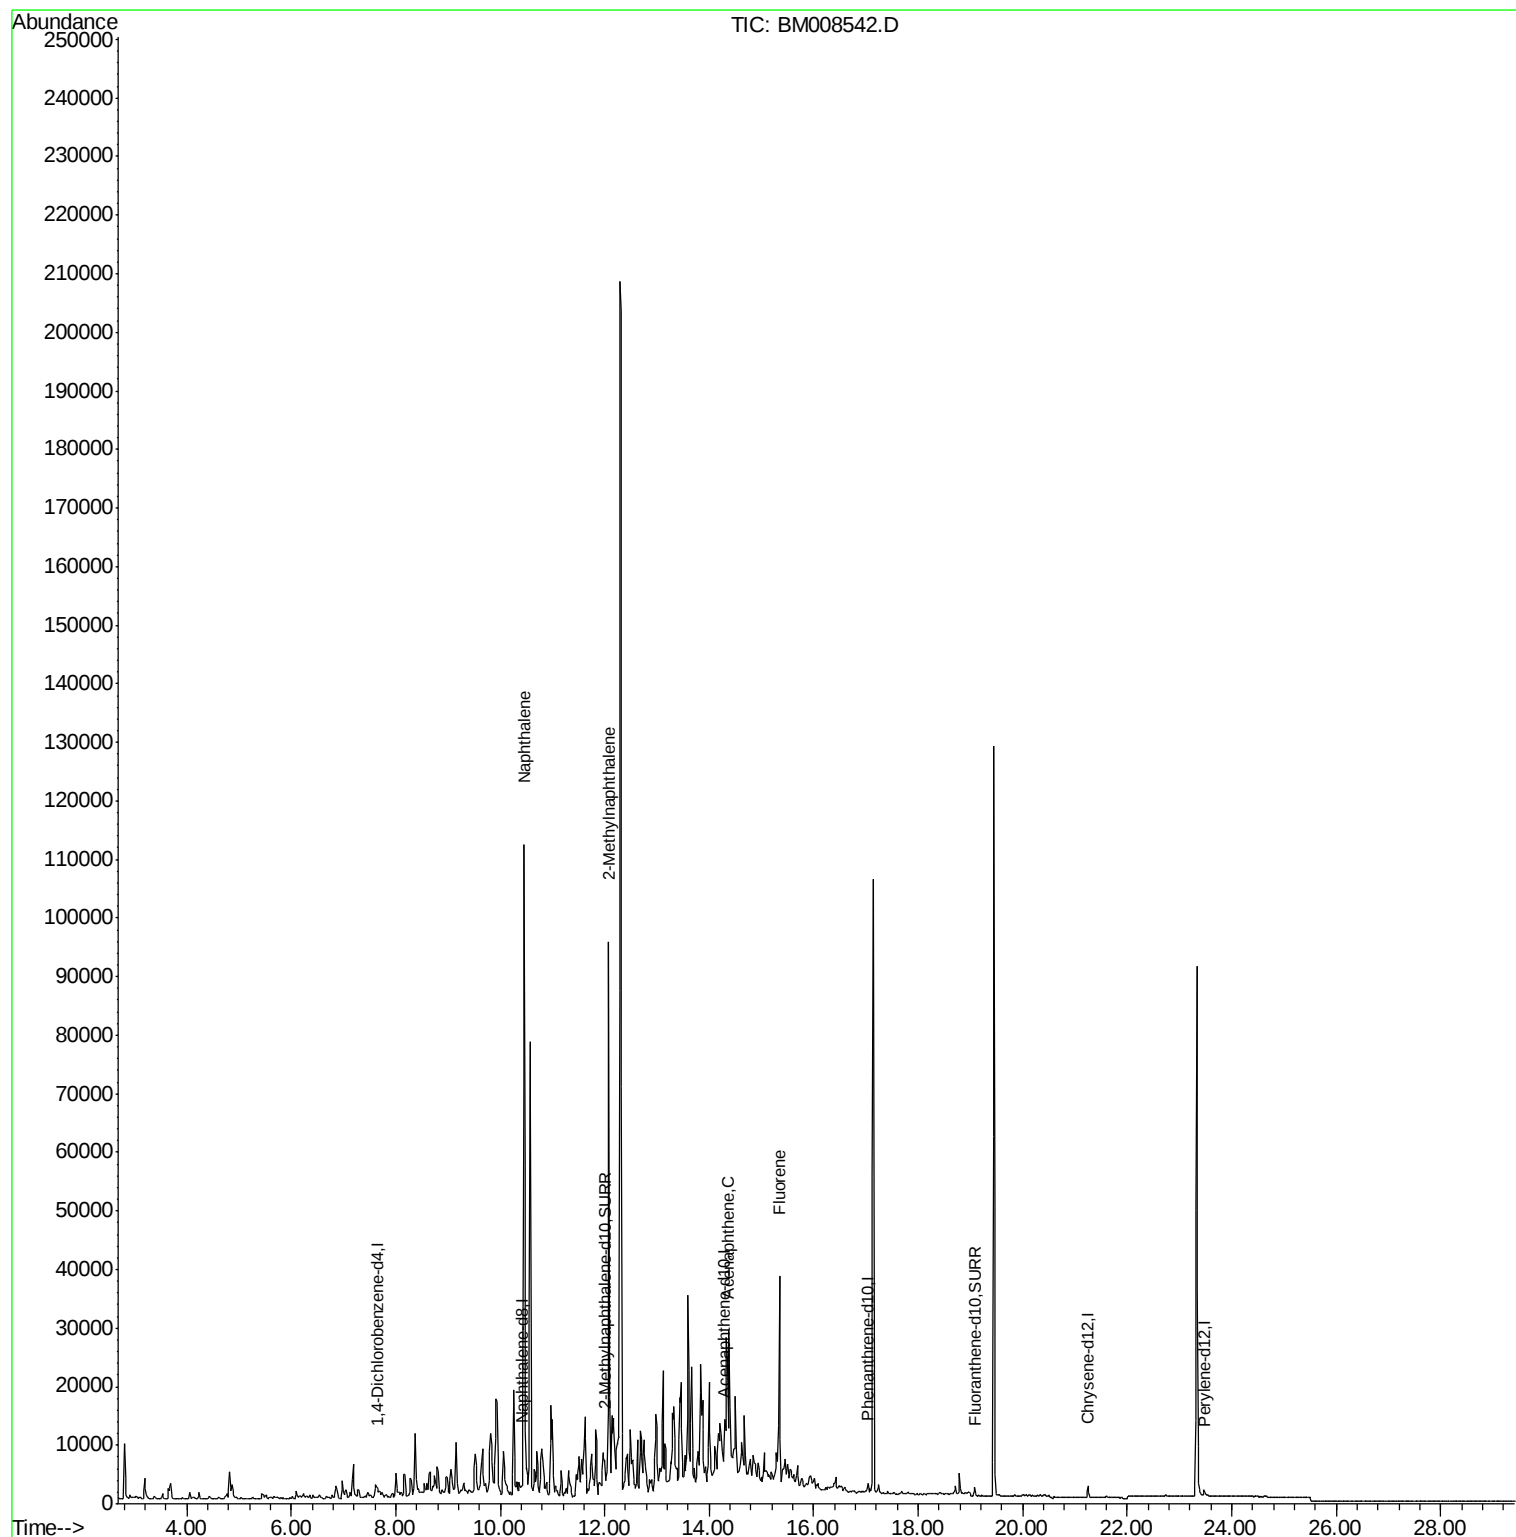

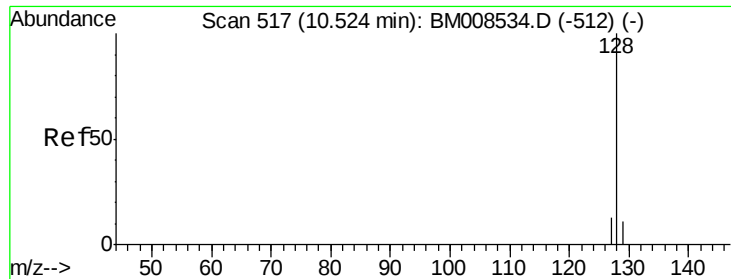

#3

Naphthalene

Concen: 37.11 ng/ul

RT: 10.46 min Scan# 512

Delta R.T. -0.06 min

Lab File: BM008542.D

Acq: 22 Dec 2016 06:13

Instrument :

BNA_M





ClientSampleId :

DA8T4

Tgt Ion:	128	Resp:	151282
Ion Ratio		Lower	Upper
128	100		
129	11.3	11.3	16.9
127	12.9	12.8	19.2

Manual Integrations
APPROVED

Sohil
12/22/2016 12:36:36 PM

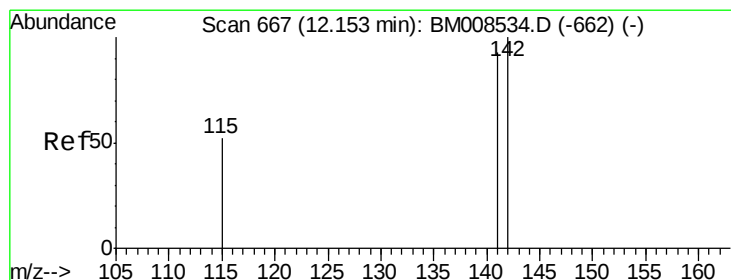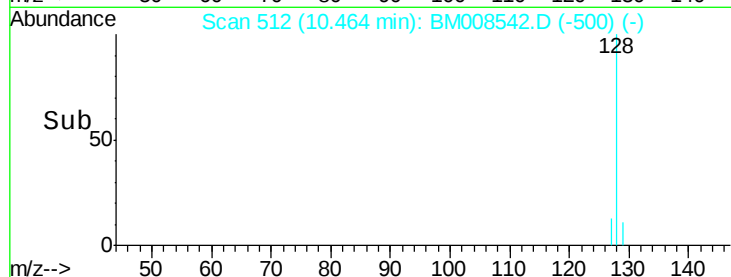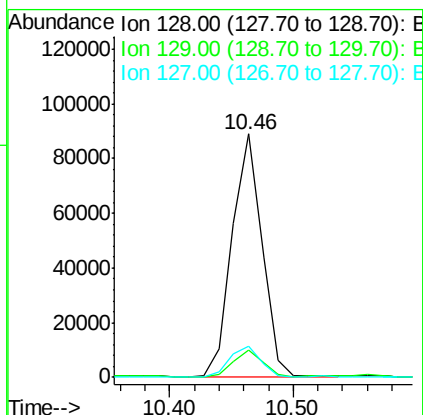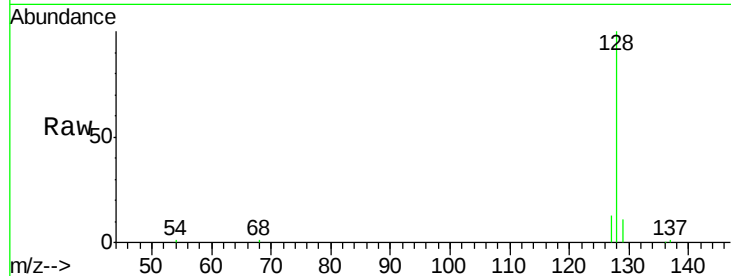

#5

2-Methylnaphthalene

Concen: 21.99 ng/ul




RT: 12.08 min Scan# 660


Delta R.T. -0.07 min

Lab File: BM008542.D

Acq: 22 Dec 2016 06:13

Tgt Ion:	142	Resp:	60349
Ion Ratio		Lower	Upper
142	100		
141	90.4	72.6	108.8

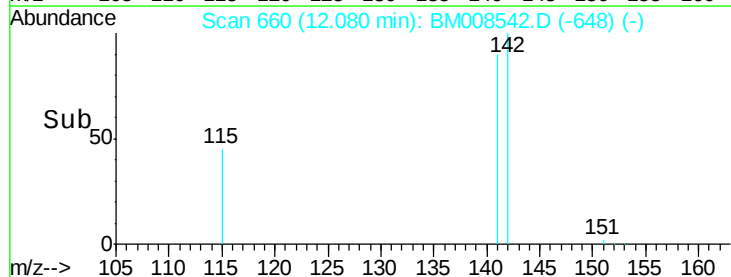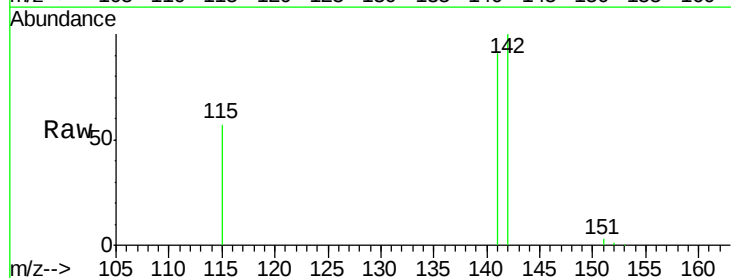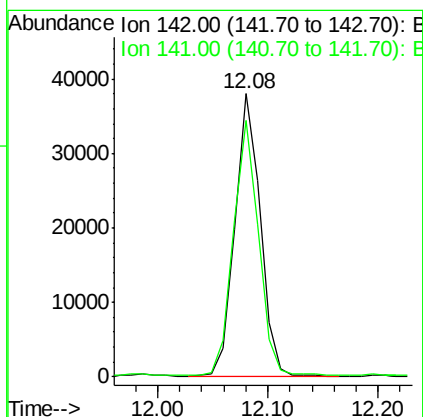

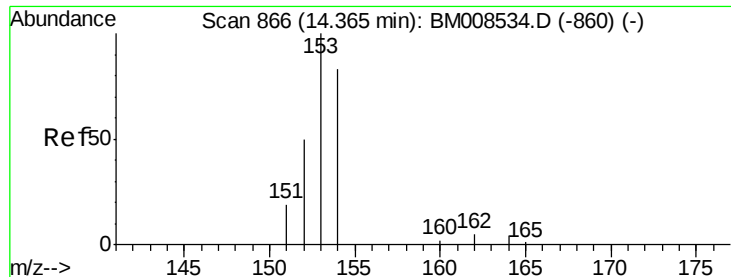

#8

Acenaphthene





Concen: 1.91 ng/ul m
RT: 14.35 min Scan# 865
Delta R.T. -0.02 min
Lab File: BM008542.D
Acq: 22 Dec 2016 06:13

Instrument :
BNA_M
ClientSampleId :
DA8T4

Tgt Ion	Ratio	Lower	Upper
153	100		
152	44.0	40.3	60.5
154	97.1	71.4	107.2

Manual Integrations
APPROVED

Sohil
12/22/2016 12:36:36 PM

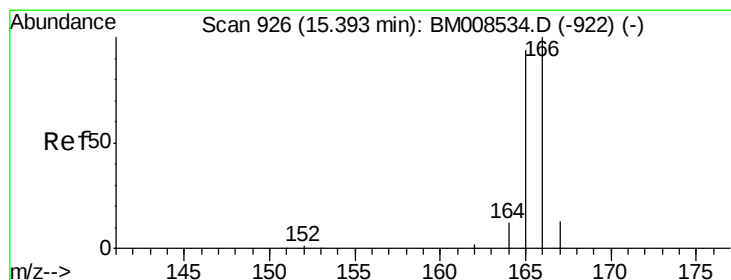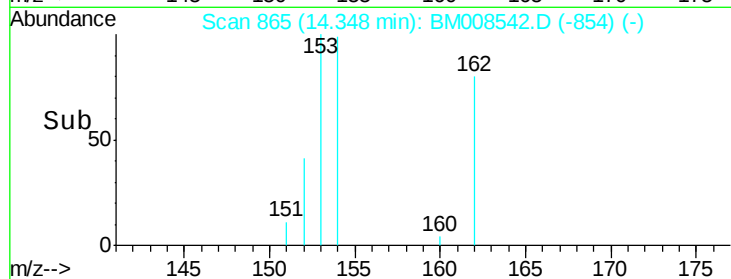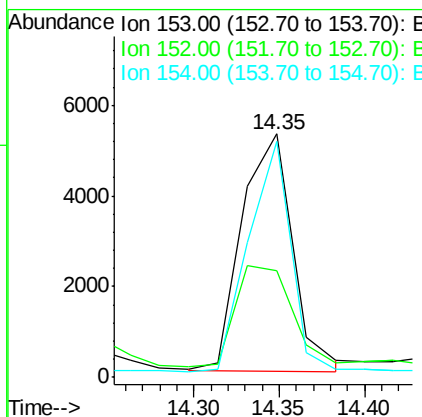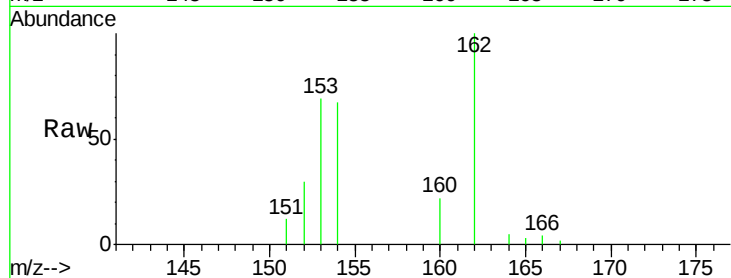

#9

Fluorene

Concen: 3.47 ng/ul m
RT: 15.34 min Scan# 923
Delta R.T. -0.05 min
Lab File: BM008542.D
Acq: 22 Dec 2016 06:13

Tgt Ion	Ratio	Lower	Upper
166	100		
165	101.9	73.4	110.2
167	14.1	14.6	22.0

