

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043503.D
 Acq On : 21 Dec 2023 15:23
 Operator : MA/JU
 Sample : 05912-14
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3D6

Quant Time: Dec 21 22:38:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 15 22:09:25 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	170269	20.000	ng/u1	-0.02
20) Naphthalene-d8	10.780	136	733485	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.604	164	392950	20.000	ng/u1	-0.02
64) Phenanthrene-d10	17.351	188	756223	20.000	ng/u1	-0.01
79) Chrysene-d12	21.527	240	596741	20.000	ng/u1	-0.01
88) Perylene-d12	23.944	264	714013	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	20162	3.848	ng/uL	-0.01
4) Pyridine-d5	3.804	84	133765	8.871	ng/u1	0.00
7) Phenol-d5	7.134	99	100037	5.165	ng/u1	-0.02
9) Bis-(2-Chloroethyl)eth...	7.310	67	388051	31.634	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.498	132	312674	21.142	ng/u1	-0.02
15) 4-Methylphenol-d8	8.681	113	191102	12.714	ng/u1	-0.02
21) Nitrobenzene-d5	9.145	128	210647	29.683	ng/u1	-0.02
24) 2-Nitrophenol-d4	9.869	143	27079	3.693	ng/u1	-0.02
28) 2,4-Dichlorophenol-d3	10.398	165	286585	22.140	ng/u1	-0.02
31) 4-Chloroaniline-d4	10.927	131	515958	27.095	ng/u1	-0.02
46) Dimethylphthalate-d6	14.027	166	1152012	32.567	ng/u1	-0.01
49) Acenaphthylene-d8	14.304	160	1329801	31.690	ng/u1	-0.02
54) 4-Nitrophenol-d4	14.839	143	246	0.037	ng/u1	0.02
60) Fluorene-d10	15.598	176	1014769	34.692	ng/u1	-0.02
65) 4,6-Dinitro-2-methylph...	15.733	200	157	0.031	ng/u1	0.00
73) Anthracene-d10	17.451	188	1756034	41.405	ng/u1	-0.01
81) Pyrene-d10	19.739	212	1810382	38.427	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.791	264	1874235	42.537	ng/u1	-0.01
Target Compounds						
35) 4-Chloro-3-methylphenol	12.069	107	25331	1.717	ng/u1	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043503.D
Acq On : 21 Dec 2023 15:23
Operator : MA/JU
Sample : 05912-14
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3D6

Quant Time: Dec 21 22:38:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 15 22:09:25 2023
Response via : Initial Calibration

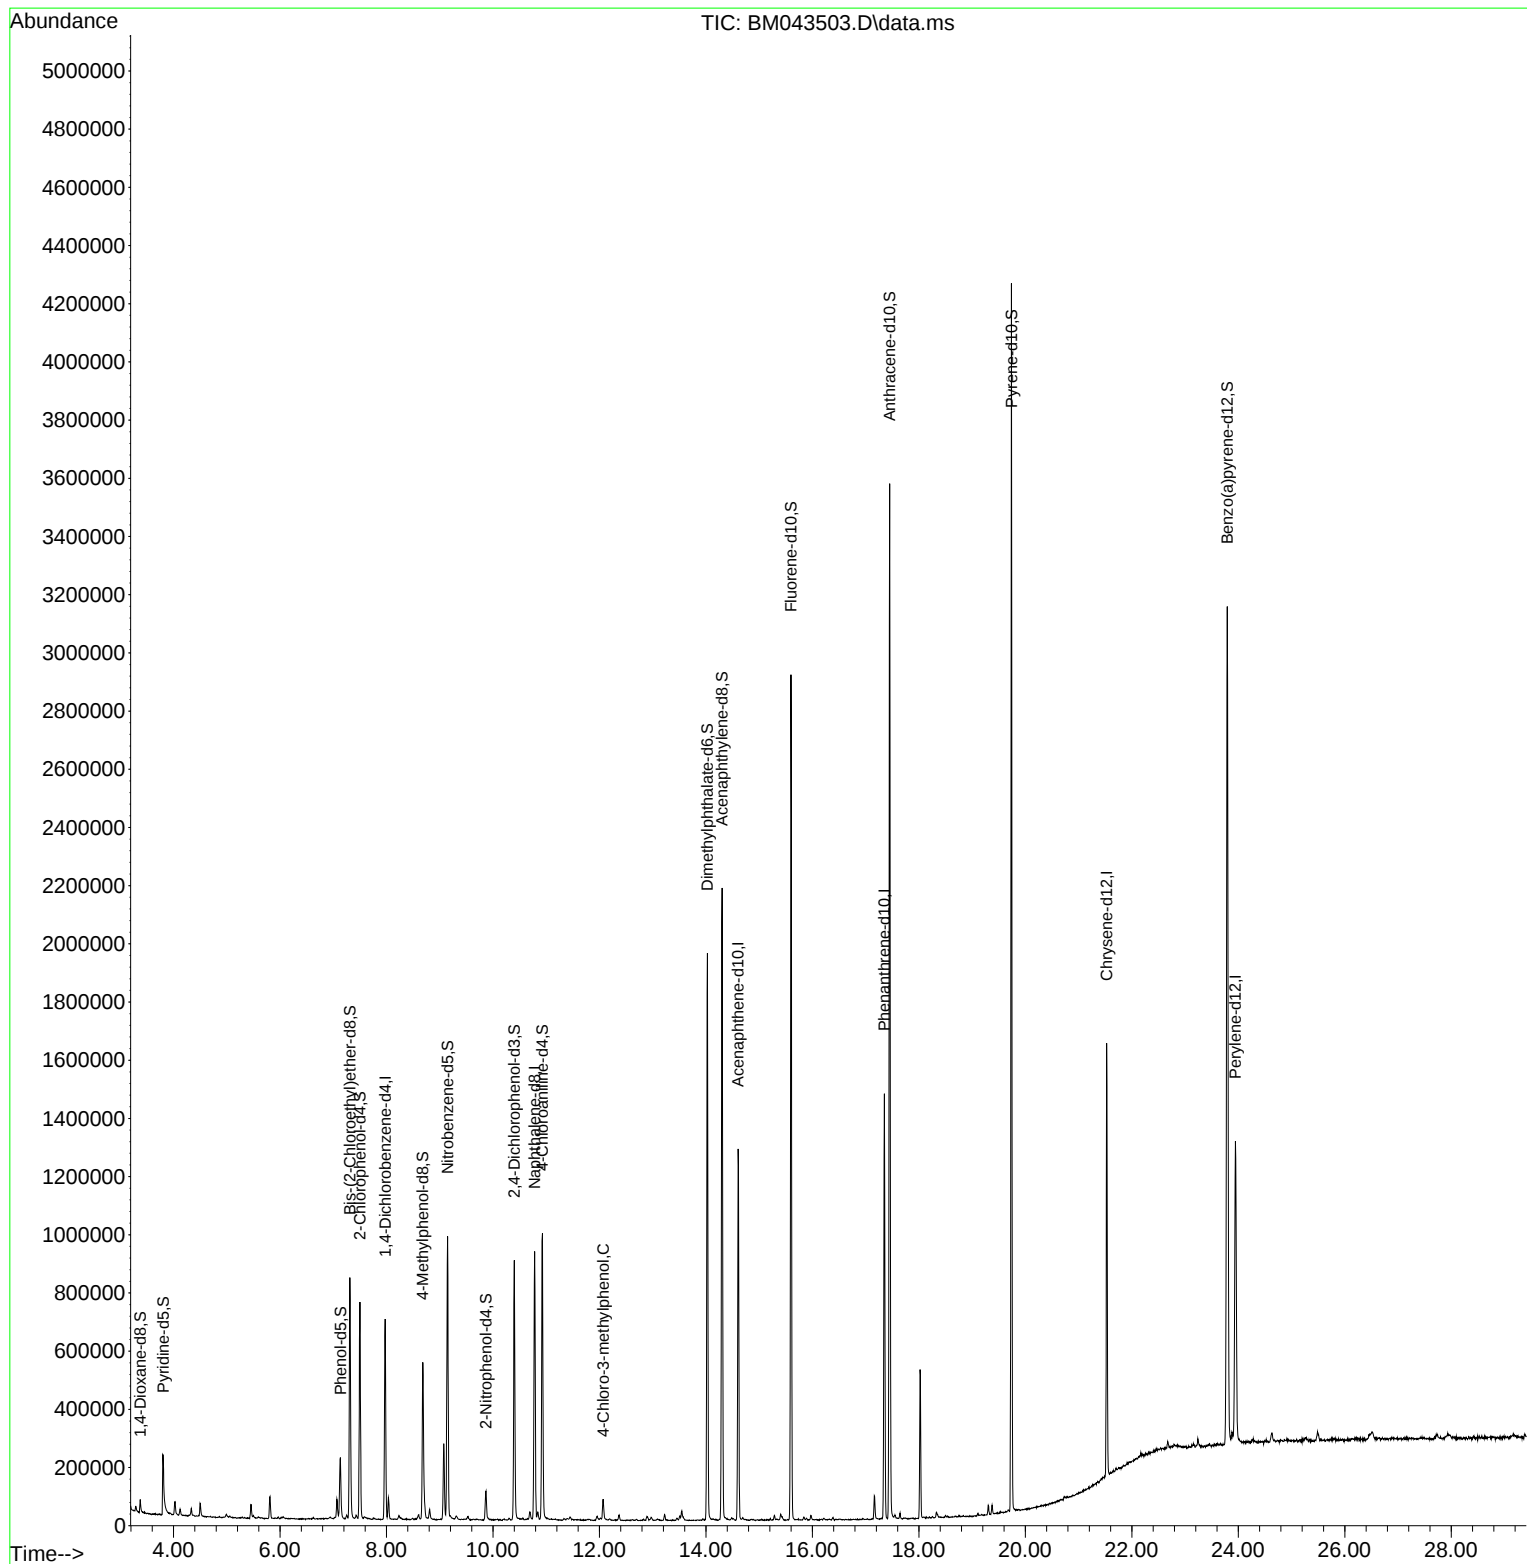

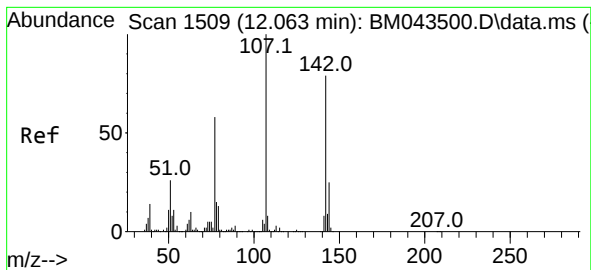

#35
 4-Chloro-3-methylphenol
 Concen: 1.717 ng/ul
 RT: 12.069 min Scan# 11
 Delta R.T. -0.012 min
 Lab File: BM043503.D
 Acq: 21 Dec 2023 15:23

Instrument :
 BNA_M
 ClientSampleId :
 BH3D6

Tgt Ion	Ratio	Lower	Upper
107	100		
144	25.3	20.3	30.5
142	73.6	64.3	96.5

