

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043538.D
 Acq On : 22 Dec 2023 14:07
 Operator : MA/JU
 Sample : 05927-05
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGWA5

Quant Time: Dec 22 14:40:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 21 21:59:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	201220	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	856745	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.604	164	453875	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.357	188	745117	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	713611	20.000	ng/ul	0.00
88) Perylene-d12	23.944	264	815742	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	27038	4.367	ng/uL	0.00
4) Pyridine-d5	3.799	84	205013	11.505	ng/ul	0.00
7) Phenol-d5	7.128	99	187445	8.189	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.304	67	538456	37.143	ng/ul	0.00
11) 2-Chlorophenol-d4	7.492	132	472972	27.062	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	320830	18.062	ng/ul	0.00
21) Nitrobenzene-d5	9.139	128	283228	34.169	ng/ul	0.00
24) 2-Nitrophenol-d4	9.863	143	262370	30.634	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.392	165	461205	30.505	ng/ul	0.00
31) 4-Chloroaniline-d4	10.922	131	658639	29.611	ng/ul	0.00
46) Dimethylphthalate-d6	14.021	166	1521300	37.234	ng/ul	0.00
49) Acenaphthylene-d8	14.298	160	1786414	36.857	ng/ul	0.00
54) 4-Nitrophenol-d4	14.810	143	49267	6.371	ng/ul	0.00
60) Fluorene-d10	15.598	176	1322966	39.157	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.715	200	145455	29.516	ng/ul	0.00
73) Anthracene-d10	17.457	188	1904861	45.584	ng/ul	0.00
81) Pyrene-d10	19.739	212	2073803	36.809	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.791	264	2009418	39.918	ng/ul	0.00
Target Compounds						
					Qvalue	
34) Caprolactam	11.739	113	9495	2.025	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043538.D
Acq On : 22 Dec 2023 14:07
Operator : MA/JU
Sample : 05927-05
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGWA5

Quant Time: Dec 22 14:40:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 21 21:59:32 2023
Response via : Initial Calibration

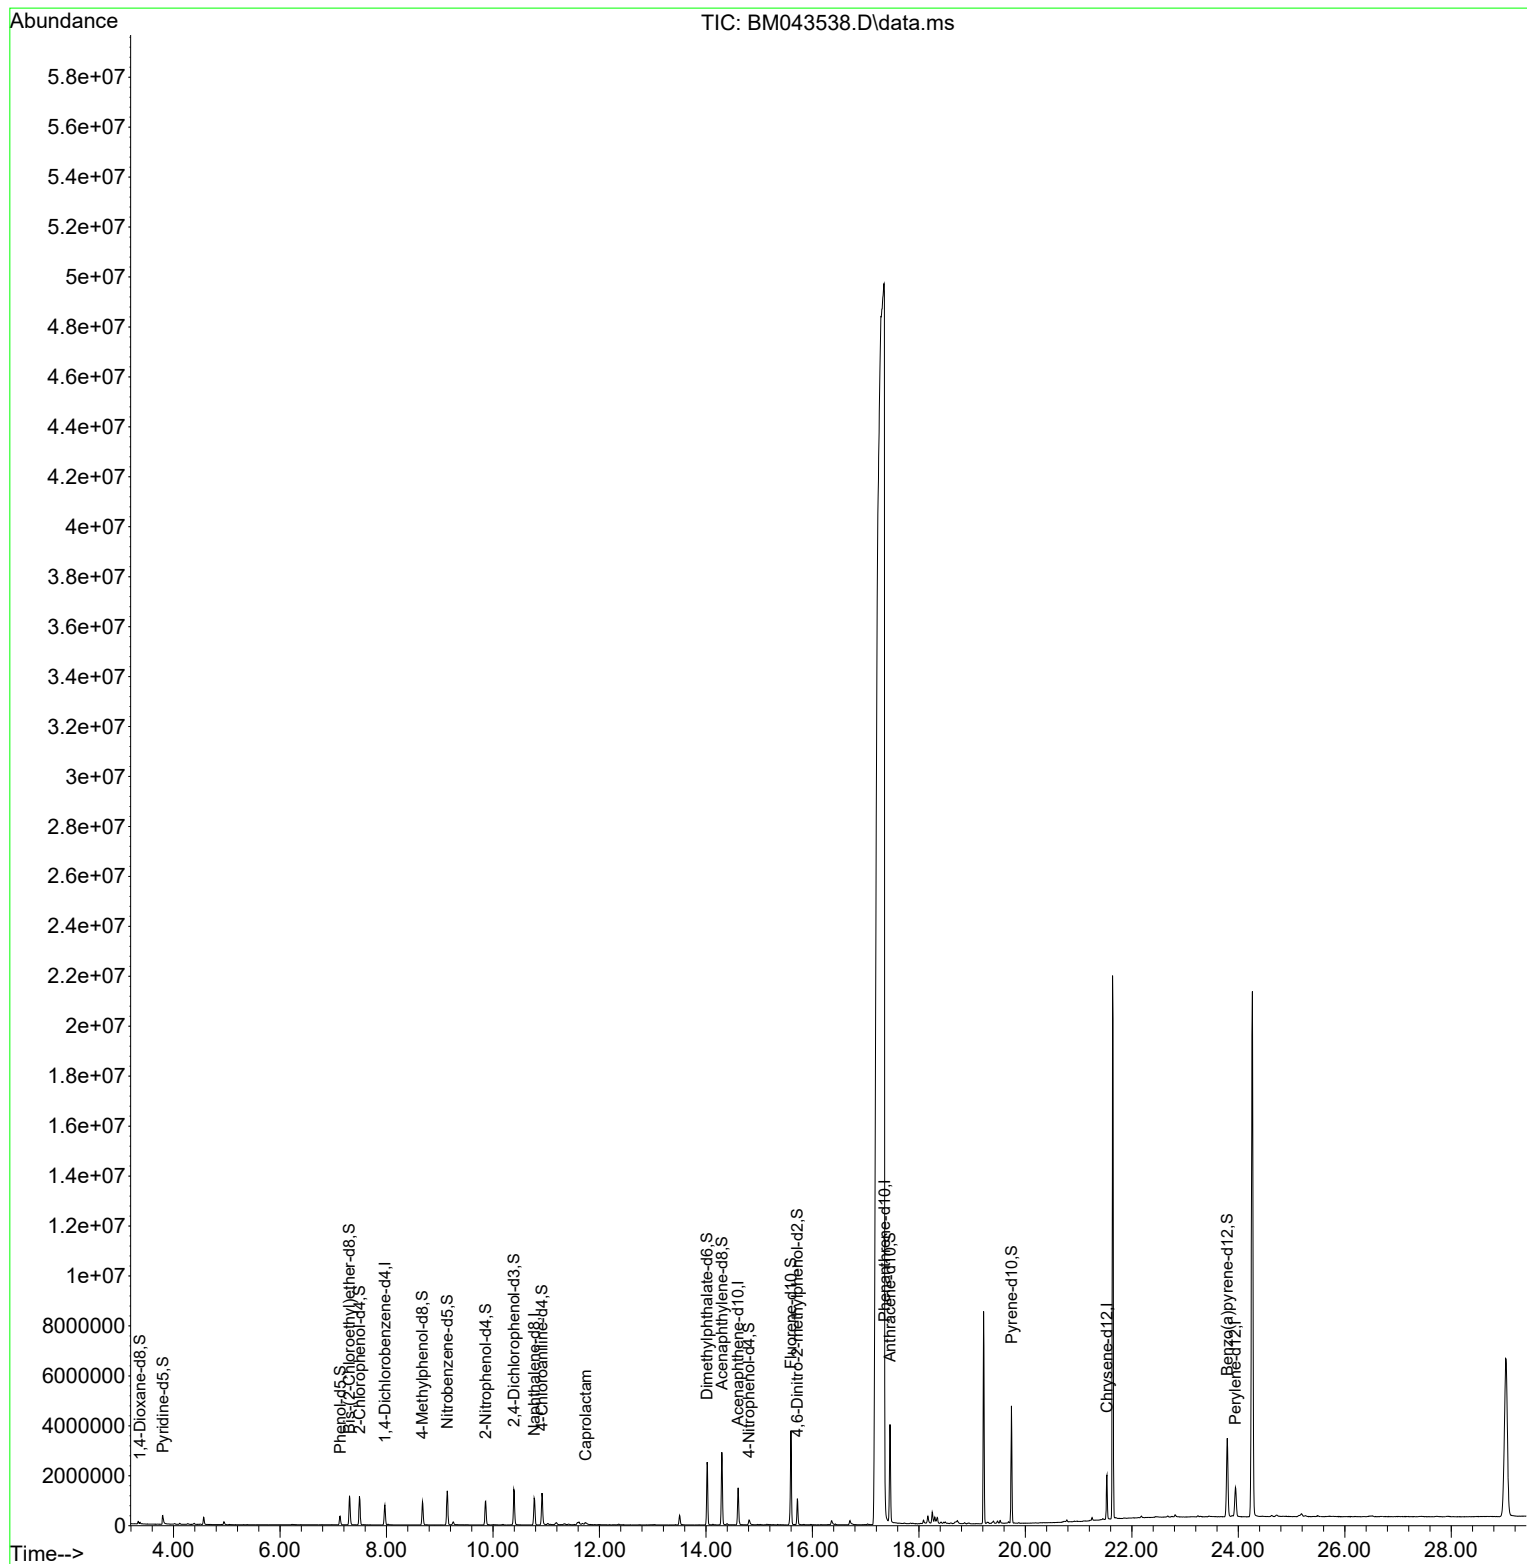

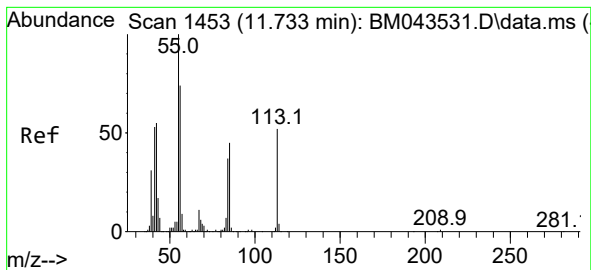

#34
Caprolactam
Concen: 2.025 ng/ul
RT: 11.739 min Scan# 14
Delta R.T. 0.006 min
Lab File: BM043538.D
Acq: 22 Dec 2023 14:07

Instrument :
BNA_M
ClientSampleId :
BGWA5

Tgt Ion:	113	Resp:	9495
Ion	Ratio	Lower	Upper
113	100		
55	299.7	148.9	223.3#
56	187.3	111.4	167.2#

