

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043540.D
 Acq On : 22 Dec 2023 15:23
 Operator : MA/JU
 Sample : 05927-08
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGWA8

Quant Time: Dec 22 16:04:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 21 21:59:32 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	246420	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	1047397	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.604	164	556321	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	1068034	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	828187	20.000	ng/ul	0.00
88) Perylene-d12	23.939	264	965540	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	27366	3.609	ng/uL	0.00
4) Pyridine-d5	3.799	84	137914	6.320	ng/ul	0.00
7) Phenol-d5	7.128	99	138893	4.955	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.310	67	465300	26.209	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	390231	18.232	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	245368	11.280	ng/ul	0.00
21) Nitrobenzene-d5	9.140	128	244143	24.092	ng/ul	0.00
24) 2-Nitrophenol-d4	9.863	143	224596	21.450	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.392	165	367790	19.898	ng/ul	0.00
31) 4-Chloroaniline-d4	10.922	131	592810	21.800	ng/ul	0.00
46) Dimethylphthalate-d6	14.022	166	1286055	25.680	ng/ul	0.00
49) Acenaphthylene-d8	14.298	160	1493916	25.146	ng/ul	0.00
54) 4-Nitrophenol-d4	14.810	143	37995	4.008	ng/ul	0.00
60) Fluorene-d10	15.598	176	1146234	27.679	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.716	200	139900	19.806	ng/ul	0.00
73) Anthracene-d10	17.445	188	1850470	30.894	ng/ul	0.00
81) Pyrene-d10	19.733	212	1941903	29.700	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.786	264	1899460	31.879	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.063	107	26513	1.258	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043540.D
Acq On : 22 Dec 2023 15:23
Operator : MA/JU
Sample : 05927-08
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGWA8


Quant Time: Dec 22 16:04:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 21 21:59:32 2023
Response via : Initial Calibration

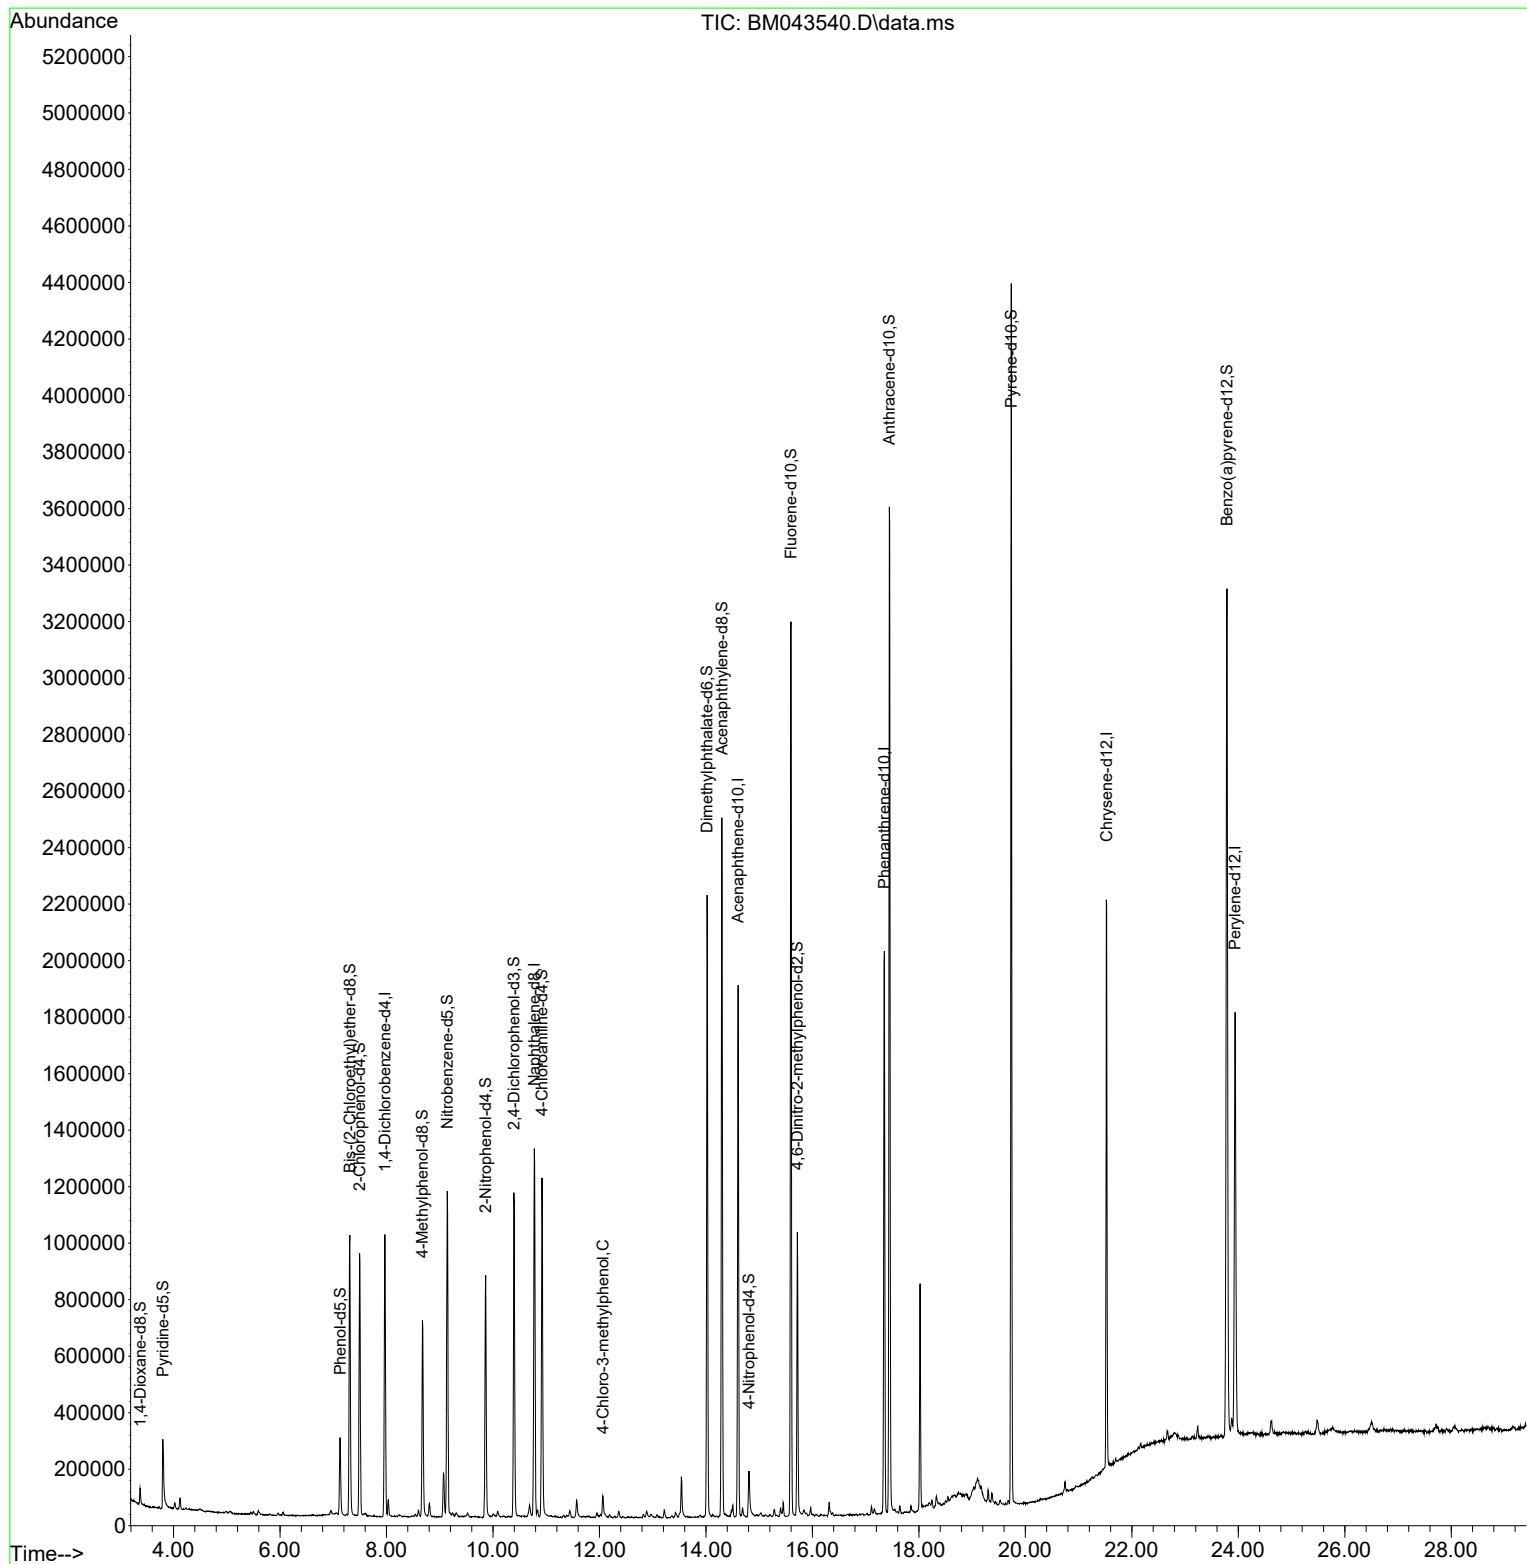

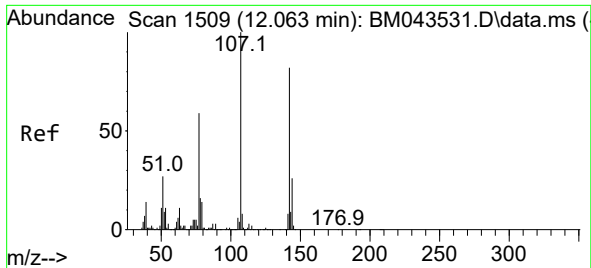

#35
 4-Chloro-3-methylphenol
 Concen: 1.258 ng/ul
 RT: 12.063 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BM043540.D
 Acq: 22 Dec 2023 15:23

Instrument :
 BNA_M
 ClientSampleId :
 BGWA8

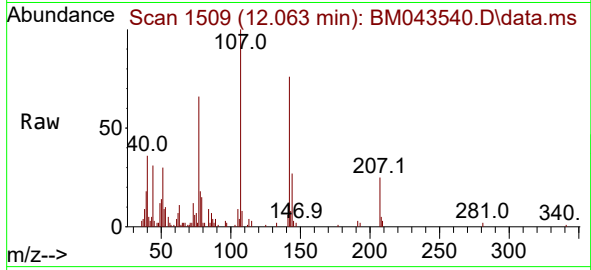

Tgt Ion:	107	Resp:	26513
Ion	Ratio	Lower	Upper
107	100		
144	27.0	20.3	30.5
142	76.2	64.3	96.5

