

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043501.D
 Acq On : 21 Dec 2023 14:11
 Operator : MA/JU
 Sample : PB157922BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK922

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043501.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	28	32	43	rVB	81873	116267	2.53%	0.206%
2	3.793	100	103	130	rBV	948038	1571697	34.16%	2.786%
3	4.122	156	159	165	rVB	15457	21752	0.47%	0.039%
4	7.134	664	671	688	rVB	1127462	1817600	39.51%	3.222%
5	7.310	694	701	715	rBV	882249	1406363	30.57%	2.493%
6	7.498	726	733	744	rBV	1085765	1738519	37.79%	3.082%
7	7.975	806	814	824	rBV	852803	1381451	30.03%	2.449%
8	8.681	927	934	946	rBV	1298375	2080145	45.21%	3.687%
9	9.145	1005	1013	1022	rBV	1031813	1683136	36.58%	2.983%
10	9.863	1127	1135	1149	rBV	749363	1282465	27.87%	2.273%
11	10.398	1218	1226	1242	rBV	1162107	1931601	41.98%	3.424%
12	10.780	1283	1291	1298	rBV	1148043	1944858	42.27%	3.447%
13	10.928	1305	1316	1338	rBV	1206678	2196683	47.75%	3.894%
14	11.974	1489	1494	1495	rBV5	3130	4824	0.10%	0.009%
15	12.369	1556	1561	1569	rVB2	17886	33454	0.73%	0.059%
16	12.445	1569	1574	1578	rBV3	10275	18497	0.40%	0.033%
17	12.663	1607	1611	1616	rVB6	4904	8422	0.18%	0.015%
18	13.451	1741	1745	1750	rBV6	4984	7723	0.17%	0.014%
19	13.510	1750	1755	1760	rVB4	11280	19064	0.41%	0.034%
20	13.921	1821	1825	1830	rBV8	2847	5718	0.12%	0.010%
21	14.027	1836	1843	1853	rBV	1874356	2678729	58.22%	4.748%
22	14.304	1883	1890	1900	rBV	2185442	3292912	71.57%	5.837%
23	14.604	1934	1941	1948	rBV	1546937	2331584	50.68%	4.133%
24	14.668	1948	1952	1959	rVB2	31194	48241	1.05%	0.086%
25	14.804	1969	1975	2000	rBV	917015	1557002	33.84%	2.760%
26	15.010	2005	2010	2017	rVB	21621	39257	0.85%	0.070%
27	15.598	2100	2110	2117	rBV	2790174	3961849	86.11%	7.022%
28	15.651	2117	2119	2124	rVV	31203	42581	0.93%	0.075%
29	15.721	2124	2131	2143	rVV	736800	1092883	23.75%	1.937%
30	15.839	2146	2151	2155	rVV3	16156	29182	0.63%	0.052%
31	15.898	2157	2161	2167	rVV8	3645	8460	0.18%	0.015%
32	15.951	2167	2170	2173	rVB5	3698	4916	0.11%	0.009%
33	16.380	2239	2243	2246	rVB6	3558	5636	0.12%	0.010%
34	17.168	2374	2377	2384	rVB8	5757	8674	0.19%	0.015%
35	17.351	2401	2408	2413	rBV	1863787	2609955	56.73%	4.626%
36	17.392	2413	2415	2419	rVV	81928	97076	2.11%	0.172%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043501.D
 Acq On : 21 Dec 2023 14:11
 Operator : MA/JU
 Sample : PB157922BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK922

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	17.451	2419	2425	2442	rVB	3001820	4242749	92.22%	7.520%
38	17.745	2472	2475	2477	rBV4	3812	5455	0.12%	0.010%
39	18.245	2555	2560	2564	rBV8	6893	13335	0.29%	0.024%
40	18.433	2587	2592	2594	rBV5	5979	9549	0.21%	0.017%
41	18.721	2638	2641	2645	rBV6	2904	6047	0.13%	0.011%
42	19.303	2736	2740	2747	rVB3	29585	39517	0.86%	0.070%
43	19.374	2747	2752	2754	rBV	29470	41243	0.90%	0.073%
44	19.403	2754	2757	2763	rVB	32479	42820	0.93%	0.076%
45	19.739	2808	2814	2823	rBV	3406562	4507154	97.96%	7.989%
46	21.527	3113	3118	3128	rBV	1987537	2581562	56.11%	4.576%
47	22.121	3216	3219	3224	rVB2	66926	84791	1.84%	0.150%
48	22.744	3322	3325	3331	rVB2	125462	180594	3.93%	0.320%
49	23.450	3441	3445	3454	rVB	131184	243294	5.29%	0.431%
50	23.785	3495	3502	3513	rBV2	2394599	4600815	100.00%	8.155%
51	23.944	3522	3529	3539	rVB	1339598	2739372	59.54%	4.856%




Sum of corrected areas: 56417473

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043501.D
Acq On : 21 Dec 2023 14:11
Operator : MA/JU
Sample : PB157922BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

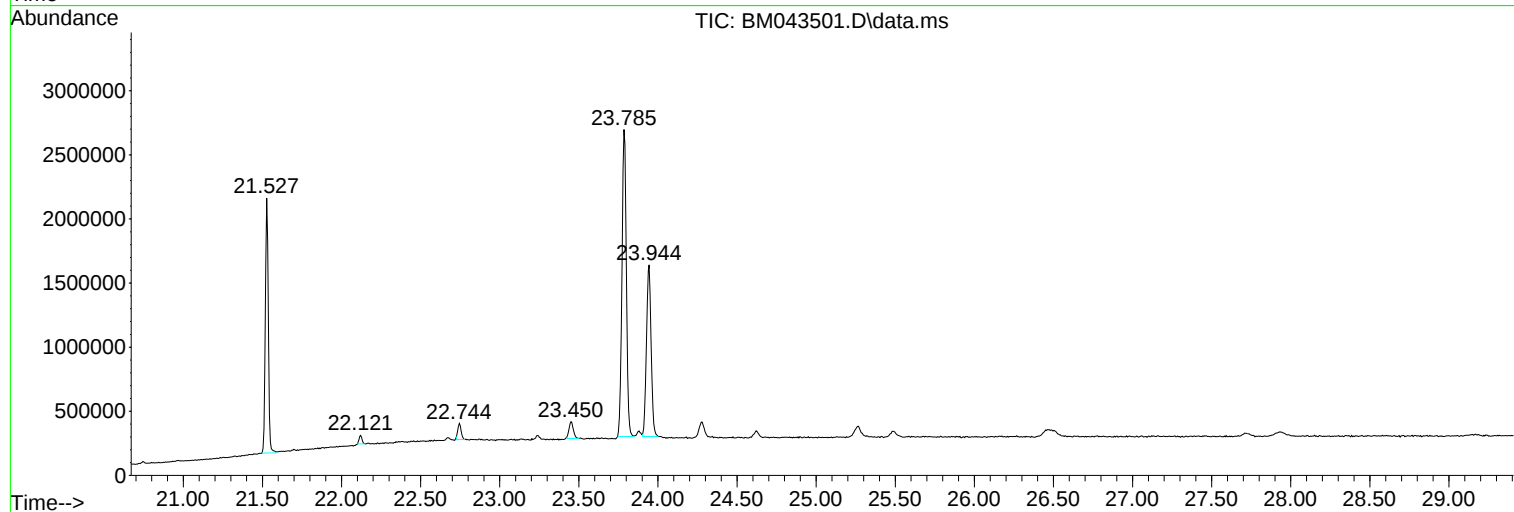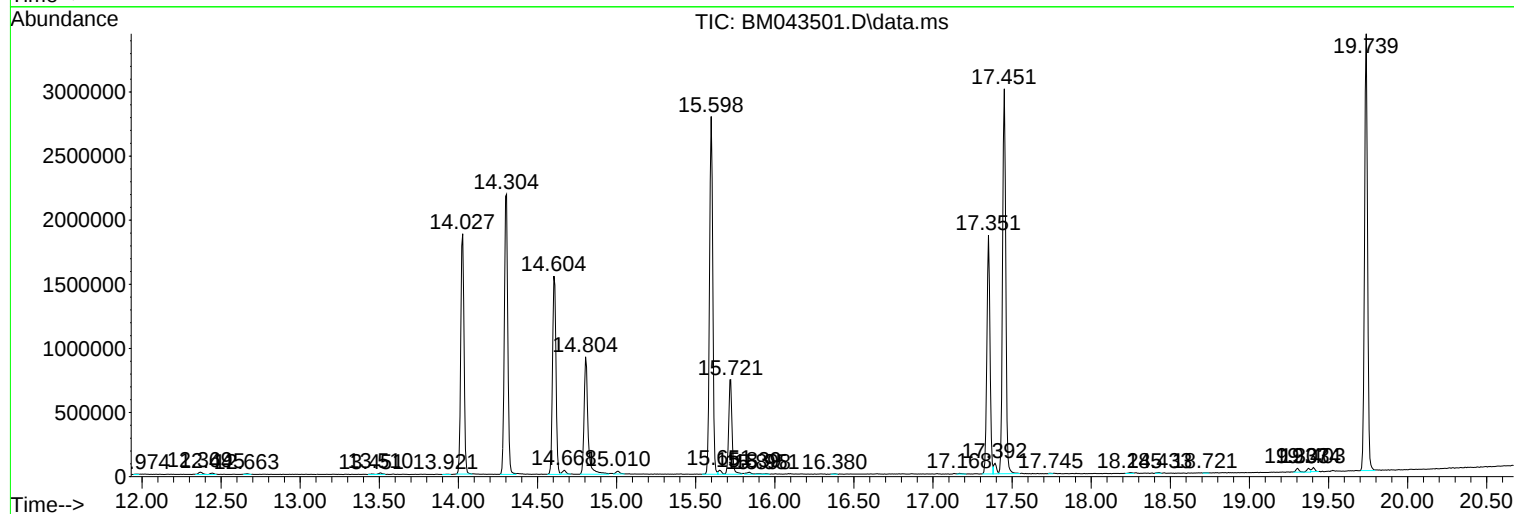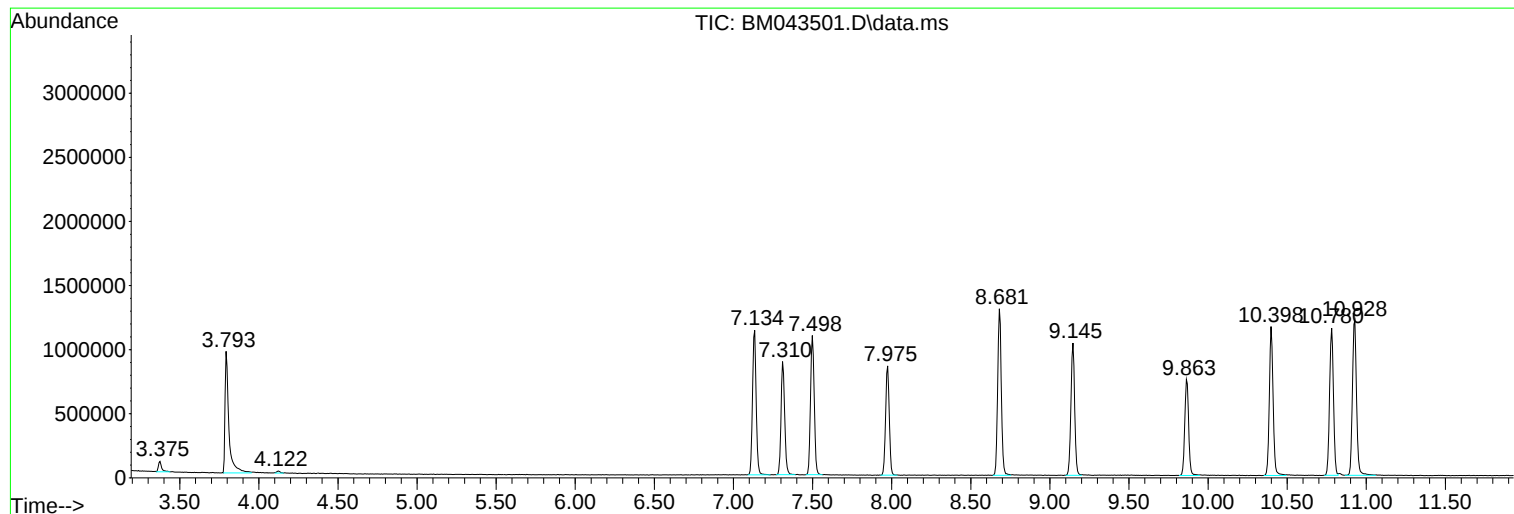

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043501.D
Acq On : 21 Dec 2023 14:11
Operator : MA/JU
Sample : PB157922BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043501.D
Acq On : 21 Dec 2023 14:11
Operator : MA/JU
Sample : PB157922BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------