

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043502.D
 Acq On : 21 Dec 2023 14:47
 Operator : MA/JU
 Sample : PB157924BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK924

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043502.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	28	32	41	rBV	76529	109584	2.34%	0.210%
2	3.793	99	103	124	rBV	905753	1464315	31.21%	2.803%
3	4.122	156	159	163	rBV3	13987	17189	0.37%	0.033%
4	7.134	664	671	684	rBV	1066910	1720369	36.67%	3.293%
5	7.310	695	701	714	rBV	822652	1331549	28.38%	2.549%
6	7.498	726	733	748	rBV	1031337	1637298	34.90%	3.134%
7	7.975	807	814	822	rBV	682205	1090172	23.24%	2.087%
8	8.681	927	934	945	rBV	1239884	1974331	42.08%	3.779%
9	9.145	1004	1013	1026	rBV	966937	1604721	34.21%	3.072%
10	9.863	1128	1135	1150	rBV	701761	1211027	25.81%	2.318%
11	10.398	1216	1226	1239	rBV	1084664	1820681	38.81%	3.485%
12	10.780	1281	1291	1298	rBV	935340	1569616	33.46%	3.005%
13	10.833	1298	1300	1305	rVB	13019	15339	0.33%	0.029%
14	10.927	1308	1316	1332	rBV	1173407	2085133	44.45%	3.992%
15	12.369	1556	1561	1568	rVB3	16422	29163	0.62%	0.056%
16	12.439	1568	1573	1578	rBV4	9281	16291	0.35%	0.031%
17	12.657	1608	1610	1617	rVB4	5928	8016	0.17%	0.015%
18	13.451	1741	1745	1750	rBV6	4249	7389	0.16%	0.014%
19	13.504	1750	1754	1760	rVV2	11677	19577	0.42%	0.037%
20	14.027	1836	1843	1853	rBV	1875067	2620381	55.86%	5.016%
21	14.304	1882	1890	1905	rBV	2083558	3168462	67.54%	6.065%
22	14.604	1934	1941	1948	rBV	1251091	1898243	40.46%	3.634%
23	14.668	1948	1952	1959	rVB2	28096	46358	0.99%	0.089%
24	14.804	1969	1975	1995	rBV	929560	1545644	32.95%	2.959%
25	15.010	2005	2010	2014	rVB	18205	28331	0.60%	0.054%
26	15.598	2103	2110	2117	rBV	2746268	3848470	82.03%	7.367%
27	15.651	2117	2119	2124	rVB	28175	36438	0.78%	0.070%
28	15.715	2124	2130	2140	rBV	749062	1087314	23.18%	2.081%
29	15.839	2147	2151	2154	rVB5	12419	19742	0.42%	0.038%
30	17.033	2350	2354	2357	rVB5	4110	5061	0.11%	0.010%
31	17.174	2375	2378	2382	rVB4	4026	5823	0.12%	0.011%
32	17.351	2401	2408	2413	rBV	1528833	2147964	45.79%	4.112%
33	17.392	2413	2415	2419	rVV	74636	91434	1.95%	0.175%
34	17.451	2419	2425	2438	rVB2	2969346	4177380	89.05%	7.997%
35	17.639	2453	2457	2462	rBV7	4186	6871	0.15%	0.013%
36	18.427	2586	2591	2596	rBV6	7225	13179	0.28%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043502.D
Acq On : 21 Dec 2023 14:47
Operator : MA/JU
Sample : PB157924BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK924

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	18.727	2640	2642	2647	rBV6	3986	7612	0.16%	0.015%
38	19.303	2736	2740	2745	rBV3	27488	41336	0.88%	0.079%
39	19.374	2748	2752	2755	rVV	28191	40415	0.86%	0.077%
40	19.403	2755	2757	2762	rVB	31963	35582	0.76%	0.068%
41	19.739	2808	2814	2826	rBV	3474221	4528868	96.54%	8.670%
42	21.527	3113	3118	3128	rBV	1678971	2128703	45.38%	4.075%
43	23.791	3495	3503	3513	rBV2	2326307	4691307	100.00%	8.981%
44	23.944	3522	3529	3539	rVB	1172455	2285530	48.72%	4.375%




Sum of corrected areas: 52238208

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043502.D
Acq On : 21 Dec 2023 14:47
Operator : MA/JU
Sample : PB157924BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK924

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

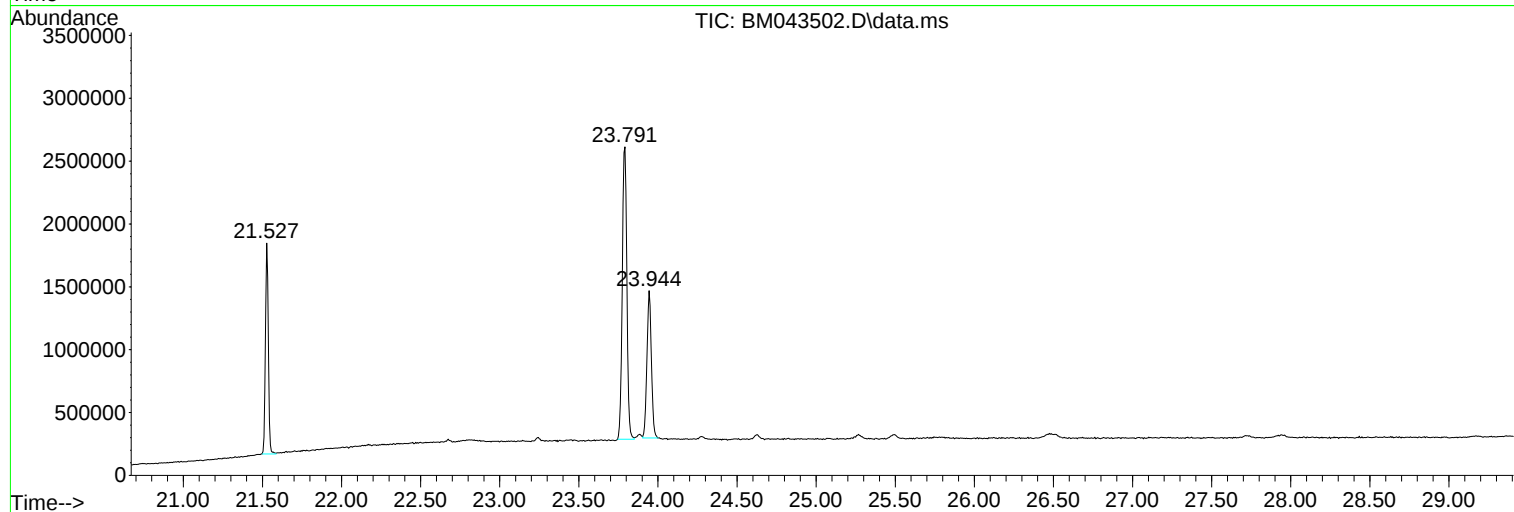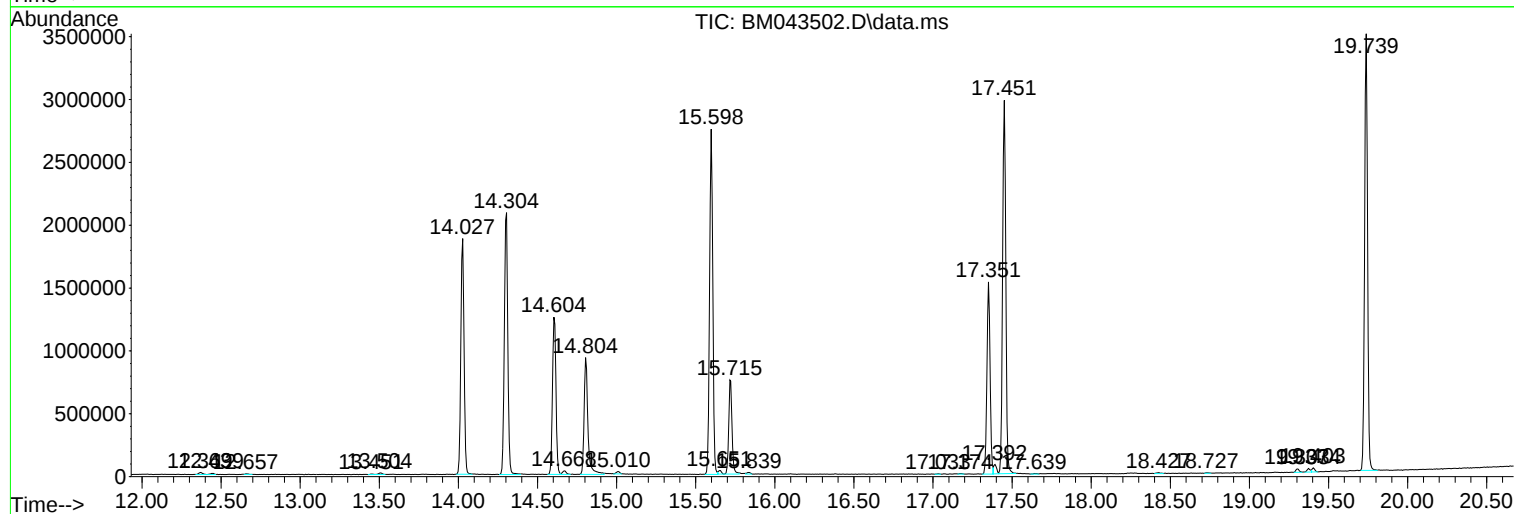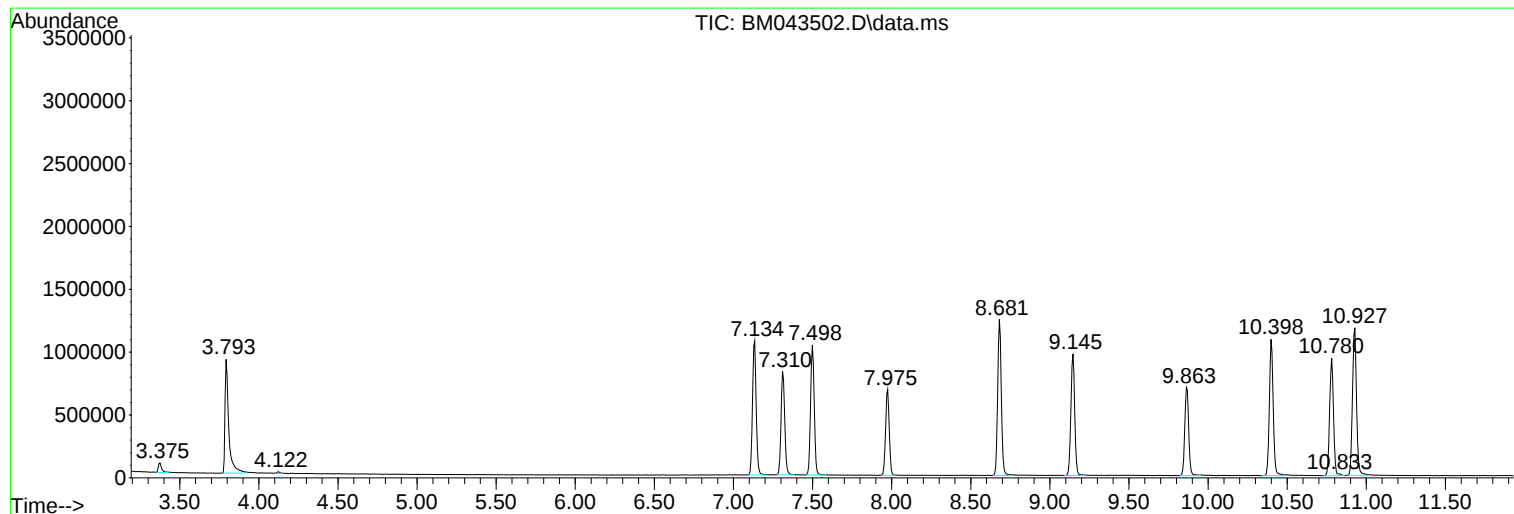

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043502.D
Acq On : 21 Dec 2023 14:47
Operator : MA/JU
Sample : PB157924BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK924

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043502.D
Acq On : 21 Dec 2023 14:47
Operator : MA/JU
Sample : PB157924BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK924

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc