

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043504.D
 Acq On : 21 Dec 2023 15:59
 Operator : MA/JU
 Sample : 05912-15
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3P4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	28	32	44	rVB	62263	92390	1.20%	0.141%
2	3.799	101	104	119	rBV	299902	524437	6.83%	0.802%
3	4.022	138	142	151	rVB2	25561	44979	0.59%	0.069%
4	4.122	154	159	167	rVB2	16797	24555	0.32%	0.038%
5	5.057	314	318	323	rVB6	7332	11181	0.15%	0.017%
6	7.134	664	671	683	rVB	277324	458279	5.97%	0.701%
7	7.310	694	701	712	rBV	1173882	1891323	24.64%	2.892%
8	7.498	726	733	743	rBV	1092340	1719924	22.41%	2.630%
9	7.587	743	748	750	rVB5	5549	8251	0.11%	0.013%
10	7.975	805	814	821	rBV	669490	1091419	14.22%	1.669%
11	8.040	821	825	832	rVB6	8758	15560	0.20%	0.024%
12	8.681	927	934	947	rBV	777176	1250014	16.29%	1.911%
13	9.145	1004	1013	1025	rBV	1404708	2336267	30.44%	3.572%
14	9.245	1025	1030	1036	rVV2	21072	39463	0.51%	0.060%
15	9.522	1072	1077	1083	rVB4	11165	20445	0.27%	0.031%
16	9.863	1128	1135	1145	rBV	1027968	1724450	22.47%	2.637%
17	10.398	1216	1226	1240	rBV	1461639	2415000	31.46%	3.693%
18	10.781	1283	1291	1299	rBV	952562	1582500	20.62%	2.420%
19	10.928	1307	1316	1329	rBV	1297990	2291872	29.86%	3.504%
20	12.016	1497	1501	1508	rVB4	6752	13460	0.18%	0.021%
21	12.198	1528	1532	1539	rBV8	3930	8715	0.11%	0.013%
22	12.369	1555	1561	1566	rBV2	25361	45992	0.60%	0.070%
23	13.427	1737	1741	1748	rBV7	5002	8419	0.11%	0.013%
24	13.504	1751	1754	1760	rVV2	19149	30273	0.39%	0.046%
25	13.574	1763	1766	1772	rBV6	5452	8665	0.11%	0.013%
26	14.027	1833	1843	1858	rBV	2844352	3961685	51.62%	6.057%
27	14.304	1882	1890	1902	rBV	3169668	4836842	63.02%	7.395%
28	14.604	1934	1941	1949	rBV	1295373	1920559	25.02%	2.937%
29	14.716	1957	1960	1966	rVB8	4711	8511	0.11%	0.013%
30	14.810	1969	1976	1991	rBV	208951	414804	5.40%	0.634%
31	15.027	2008	2013	2020	rVB7	11815	23234	0.30%	0.036%
32	15.357	2065	2069	2074	rBV	12350	16666	0.22%	0.025%
33	15.598	2102	2110	2123	rBV	4340265	6088347	79.32%	9.309%
34	15.721	2124	2131	2141	rVV	1345737	1899595	24.75%	2.904%
35	15.833	2147	2150	2155	rVB4	17634	28902	0.38%	0.044%
36	16.380	2239	2243	2250	rVB3	14139	19048	0.25%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043504.D
 Acq On : 21 Dec 2023 15:59
 Operator : MA/JU
 Sample : 05912-15
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3P4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	17.351	2401	2408	2415	rBV	1545803	2137147	27.84%	3.268%
38	17.451	2418	2425	2438	rVV2	4828410	6769149	88.19%	10.350%
39	17.645	2454	2458	2465	rVB5	6995	9201	0.12%	0.014%
40	18.021	2516	2522	2527	rBV9	9258	16309	0.21%	0.025%
41	18.245	2555	2560	2567	rBV3	52526	77012	1.00%	0.118%
42	18.327	2572	2574	2579	rVB3	9691	10396	0.14%	0.016%
43	19.304	2736	2740	2746	rBV2	45112	63713	0.83%	0.097%
44	19.374	2748	2752	2756	rBV	44122	62022	0.81%	0.095%
45	19.521	2774	2777	2783	rBV4	31761	45659	0.59%	0.070%
46	19.680	2801	2804	2807	rBV4	11029	12997	0.17%	0.020%
47	19.739	2808	2814	2821	rBV	5737546	7329487	95.49%	11.207%
48	21.250	3068	3071	3075	rBV5	27775	37245	0.49%	0.057%
49	21.527	3113	3118	3124	rBV	1594255	2036935	26.54%	3.114%
50	23.791	3495	3503	3513	rBV2	4065071	7675450	100.00%	11.736%
51	23.944	3523	3529	3541	rVB	1097193	2244054	29.24%	3.431%




Sum of corrected areas: 65402802

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043504.D
Acq On : 21 Dec 2023 15:59
Operator : MA/JU
Sample : 05912-15
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3P4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

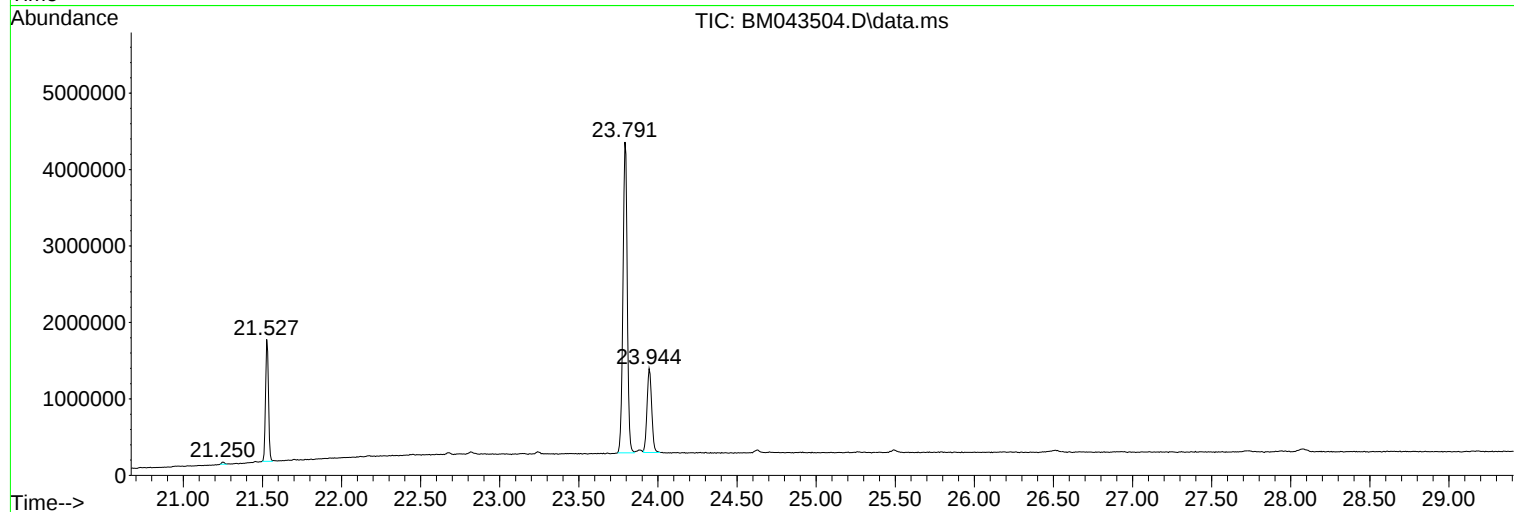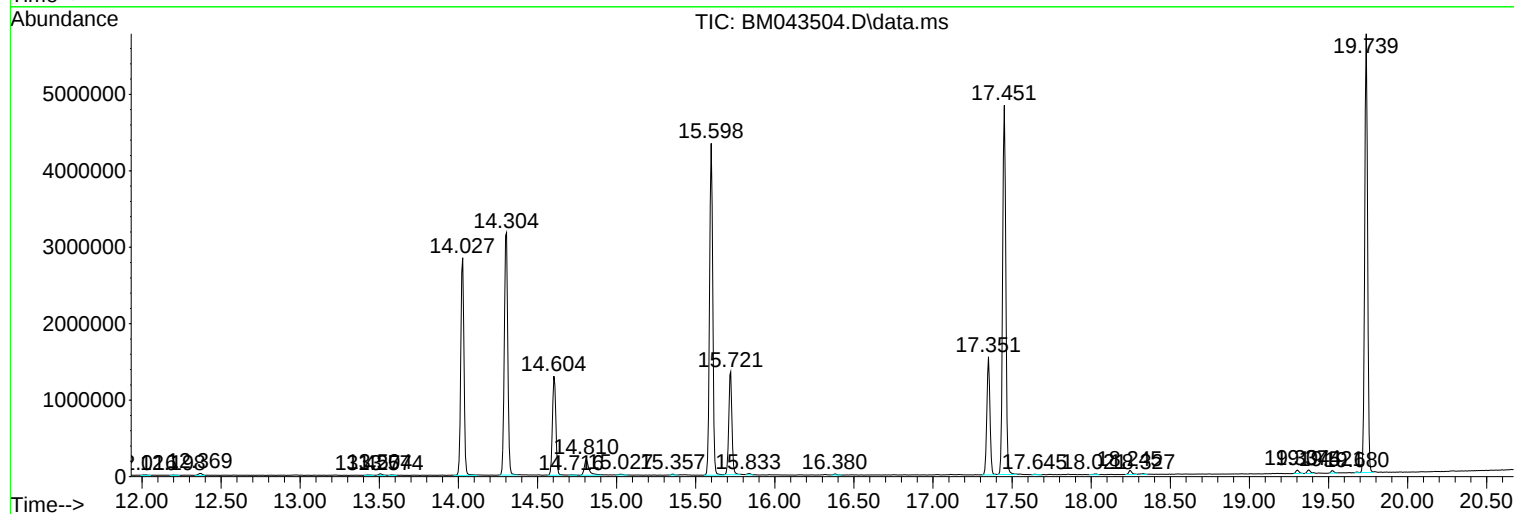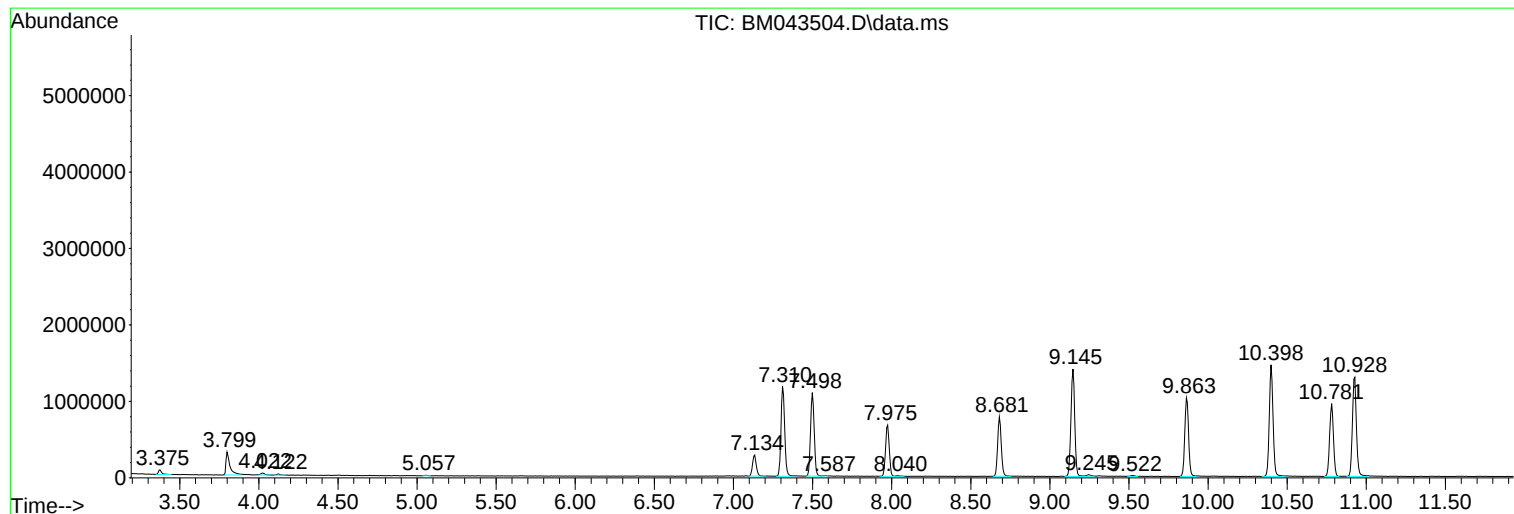

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043504.D
Acq On : 21 Dec 2023 15:59
Operator : MA/JU
Sample : 05912-15
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3P4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043504.D
Acq On : 21 Dec 2023 15:59
Operator : MA/JU
Sample : 05912-15
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3P4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc