

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043506.D
 Acq On : 21 Dec 2023 17:11
 Operator : MA/JU
 Sample : 05912-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043506.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	28	32	37	rBV	47870	62401	1.13%	0.123%
2	3.799	101	104	116	rBV	209204	376150	6.81%	0.742%
3	4.028	140	143	151	rVB	19613	27347	0.50%	0.054%
4	4.122	156	159	164	rVB	15221	20289	0.37%	0.040%
5	7.128	665	670	681	rBV	179127	309256	5.60%	0.610%
6	7.310	694	701	714	rBV	826982	1329230	24.07%	2.621%
7	7.499	726	733	743	rBV	743020	1177344	21.32%	2.321%
8	7.975	806	814	822	rBV	819749	1331974	24.12%	2.626%
9	8.681	927	934	943	rBV	517306	840664	15.22%	1.657%
10	9.146	1005	1013	1025	rBV	968771	1615572	29.25%	3.185%
11	9.522	1073	1077	1085	rVB4	9068	16420	0.30%	0.032%
12	9.863	1128	1135	1146	rBV	675754	1123559	20.34%	2.215%
13	10.398	1218	1226	1240	rBV	924840	1597034	28.92%	3.149%
14	10.781	1282	1291	1301	rBV	1114296	1871744	33.89%	3.690%
15	10.928	1307	1316	1334	rBV	899754	1674488	30.32%	3.301%
16	11.587	1423	1428	1430	rBV5	4381	6516	0.12%	0.013%
17	12.022	1499	1502	1506	rVB3	4935	6850	0.12%	0.014%
18	12.198	1528	1532	1537	rVB6	7312	12056	0.22%	0.024%
19	12.369	1555	1561	1569	rBV3	16974	32775	0.59%	0.065%
20	13.228	1702	1707	1710	rBV7	5043	6507	0.12%	0.013%
21	13.434	1735	1742	1747	rBV2	13168	19283	0.35%	0.038%
22	13.510	1749	1755	1760	rBV	21788	35300	0.64%	0.070%
23	13.581	1763	1767	1774	rBV8	3457	7384	0.13%	0.015%
24	14.028	1836	1843	1851	rBV	1786622	2559818	46.35%	5.047%
25	14.298	1882	1889	1905	rBV	2122280	3198068	57.91%	6.305%
26	14.604	1934	1941	1951	rBV	1502675	2224773	40.28%	4.386%
27	14.810	1969	1976	1987	rBV2	117922	247776	4.49%	0.489%
28	15.028	2006	2013	2018	rVB9	7859	17446	0.32%	0.034%
29	15.598	2102	2110	2124	rBV	2903065	4122047	74.64%	8.127%
30	15.716	2124	2130	2145	rVV	878666	1250250	22.64%	2.465%
31	15.839	2147	2151	2156	rVB5	12732	18250	0.33%	0.036%
32	16.380	2239	2243	2247	rBV6	9647	13387	0.24%	0.026%
33	16.627	2280	2285	2291	rBV6	3890	7771	0.14%	0.015%
34	17.169	2373	2377	2383	rVB3	12465	22680	0.41%	0.045%
35	17.351	2401	2408	2418	rBV	1719872	2458789	44.52%	4.848%
36	17.451	2418	2425	2440	rBV	3430937	4859478	87.99%	9.581%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043506.D
Acq On : 21 Dec 2023 17:11
Operator : MA/JU
Sample : 05912-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3M8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	18.033	2520	2524	2527	rVB6	6137	7916	0.14%	0.016%
38	18.245	2552	2560	2569	rBV2	72320	115181	2.09%	0.227%
39	18.733	2641	2643	2647	rBV5	4702	5988	0.11%	0.012%
40	19.304	2736	2740	2743	rBV2	32188	40968	0.74%	0.081%
41	19.374	2748	2752	2755	rBV	32307	45451	0.82%	0.090%
42	19.527	2774	2778	2785	rBV4	26828	42943	0.78%	0.085%
43	19.674	2800	2803	2807	rBV6	9833	13150	0.24%	0.026%
44	19.739	2807	2814	2821	rBV	3956635	5291962	95.82%	10.434%
45	21.251	3067	3071	3078	rBV3	98649	155181	2.81%	0.306%
46	21.527	3113	3118	3126	rBV	1841012	2390612	43.29%	4.713%
47	23.792	3495	3503	3513	rBV2	2879044	5522893	100.00%	10.889%
48	23.945	3523	3529	3539	rVB	1323428	2587457	46.85%	5.101%


Sum of corrected areas: 50720378

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043506.D
Acq On : 21 Dec 2023 17:11
Operator : MA/JU
Sample : 05912-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3M8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

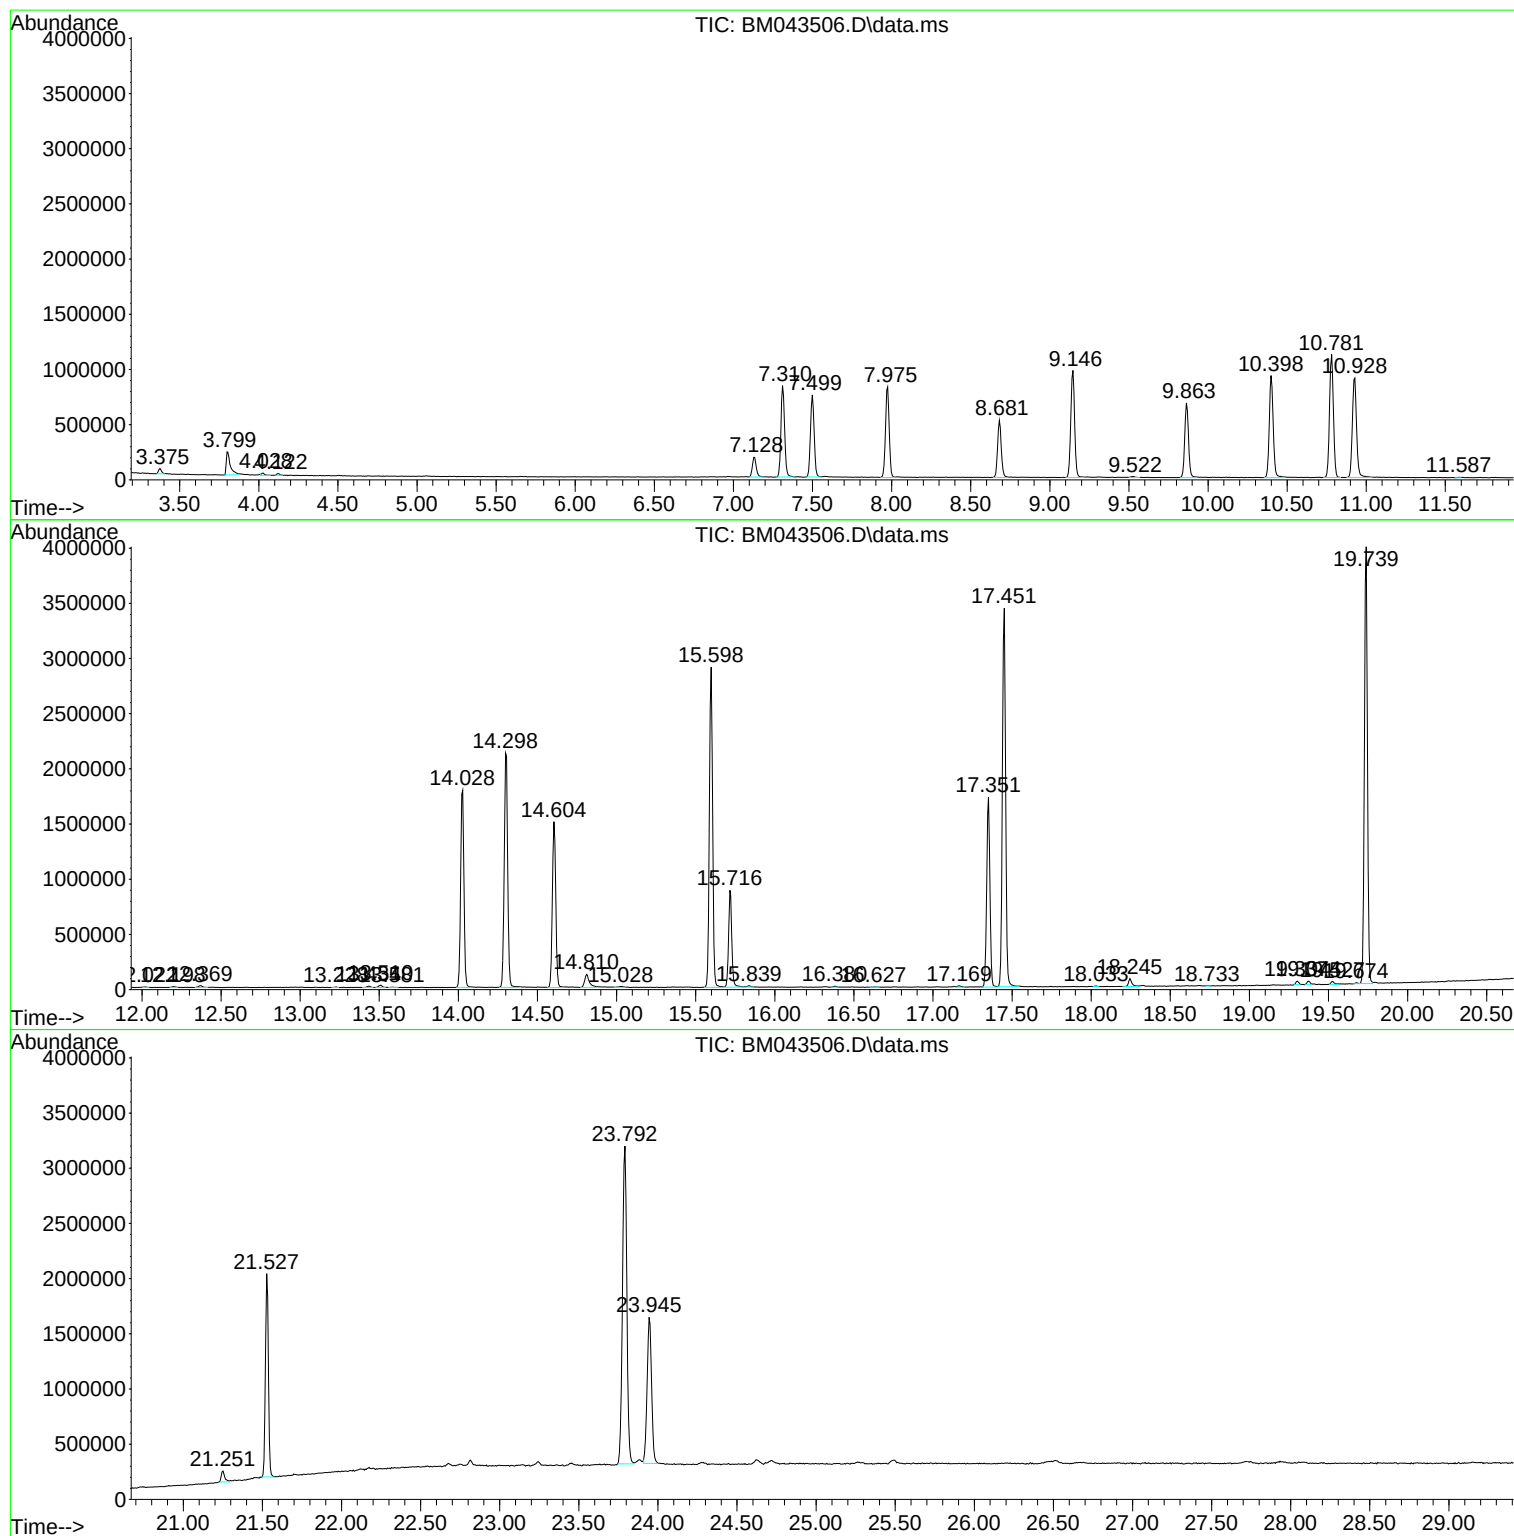

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043506.D
Acq On : 21 Dec 2023 17:11
Operator : MA/JU
Sample : 05912-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3M8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043506.D
Acq On : 21 Dec 2023 17:11
Operator : MA/JU
Sample : 05912-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3M8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc