

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043507.D
 Acq On : 21 Dec 2023 17:47
 Operator : MA/JU
 Sample : 05912-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3M9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043507.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	28	32	37	rBV	50599	66356	1.21%	0.131%
2	3.799	102	104	119	rBV	208400	384178	6.99%	0.757%
3	4.028	138	143	147	rVB	18220	29693	0.54%	0.058%
4	4.122	155	159	167	rVB	15328	24353	0.44%	0.048%
5	5.058	314	318	321	rBV3	5749	7697	0.14%	0.015%
6	7.134	664	671	683	rVB	206544	349475	6.36%	0.688%
7	7.310	694	701	713	rBV	891065	1413851	25.73%	2.785%
8	7.499	726	733	744	rBV	820015	1306746	23.78%	2.574%
9	7.975	807	814	821	rBV	711977	1178479	21.45%	2.322%
10	8.681	927	934	947	rBV	591364	960969	17.49%	1.893%
11	9.145	1005	1013	1022	rBV	1035768	1719403	31.30%	3.387%
12	9.234	1027	1028	1034	rVB5	4217	5967	0.11%	0.012%
13	9.516	1072	1076	1083	rVB7	6480	12481	0.23%	0.025%
14	9.863	1127	1135	1145	rBV	744338	1238774	22.55%	2.440%
15	10.398	1219	1226	1239	rBV	1048562	1759927	32.03%	3.467%
16	10.781	1283	1291	1301	rBV	982321	1654237	30.11%	3.259%
17	10.928	1308	1316	1330	rBV	1020546	1835220	33.40%	3.615%
18	12.198	1528	1532	1538	rVB7	5851	10418	0.19%	0.021%
19	12.369	1552	1561	1568	rBV2	19154	39473	0.72%	0.078%
20	13.428	1738	1741	1746	rBV4	7531	10886	0.20%	0.021%
21	13.510	1750	1755	1762	rBV4	18377	32940	0.60%	0.065%
22	14.028	1836	1843	1857	rBV	1986753	2852570	51.92%	5.620%
23	14.298	1879	1889	1901	rBV	2245320	3459091	62.96%	6.814%
24	14.604	1933	1941	1949	rBV	1314159	1957770	35.63%	3.857%
25	14.810	1970	1976	1991	rBV	132817	274546	5.00%	0.541%
26	15.033	2007	2014	2020	rVB	9382	18963	0.35%	0.037%
27	15.357	2064	2069	2072	rBV2	8408	14093	0.26%	0.028%
28	15.598	2102	2110	2124	rBV	3141962	4393509	79.97%	8.655%
29	15.716	2124	2130	2145	rVV	873971	1274829	23.20%	2.511%
30	15.833	2147	2150	2157	rVB7	13967	20839	0.38%	0.041%
31	16.316	2227	2232	2239	rVV10	4167	8913	0.16%	0.018%
32	16.380	2239	2243	2249	rVB5	12023	18713	0.34%	0.037%
33	16.474	2254	2259	2264	rBV8	2581	5680	0.10%	0.011%
34	17.033	2350	2354	2358	rVB7	4424	6567	0.12%	0.013%
35	17.110	2363	2367	2370	rBV6	5385	7127	0.13%	0.014%
36	17.168	2374	2377	2383	rVB4	9764	13836	0.25%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043507.D
 Acq On : 21 Dec 2023 17:47
 Operator : MA/JU
 Sample : 05912-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	17.351	2401	2408	2418	rBV	1509792	2160786	39.33%	4.257%
38	17.451	2418	2425	2437	rBV2	3350800	4782422	87.05%	9.421%
39	17.651	2455	2459	2461	rBV5	4094	5802	0.11%	0.011%
40	17.857	2490	2494	2497	rBV6	6404	7364	0.13%	0.015%
41	18.245	2555	2560	2566	rBV2	55724	79359	1.44%	0.156%
42	19.304	2736	2740	2744	rBV2	35516	48579	0.88%	0.096%
43	19.374	2748	2752	2756	rBV	27960	43745	0.80%	0.086%
44	19.521	2774	2777	2781	rBV5	21183	30190	0.55%	0.059%
45	19.739	2807	2814	2822	rBV	4030153	5170417	94.11%	10.186%
46	21.251	3068	3071	3077	rVB4	56688	73984	1.35%	0.146%
47	21.527	3113	3118	3126	rBV	1679438	2157151	39.26%	4.250%
48	23.792	3495	3503	3514	rBV	2870352	5494102	100.00%	10.823%
49	23.945	3523	3529	3539	rVB	1169302	2338589	42.57%	4.607%




Sum of corrected areas: 50761059

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043507.D
Acq On : 21 Dec 2023 17:47
Operator : MA/JU
Sample : 05912-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3M9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

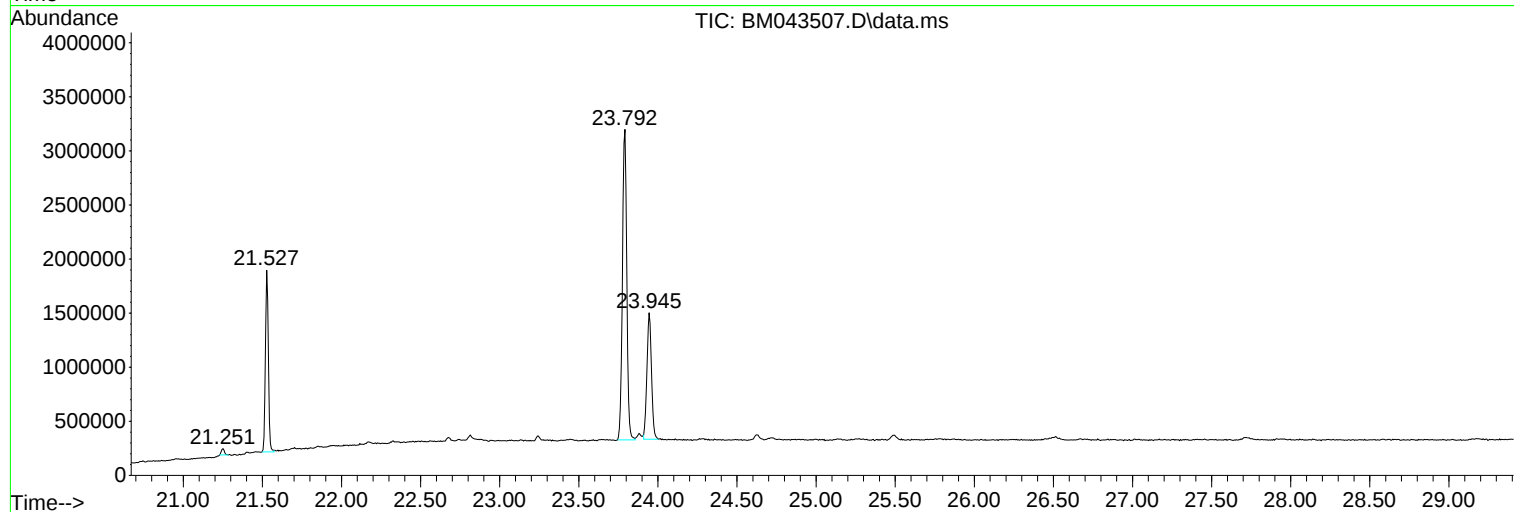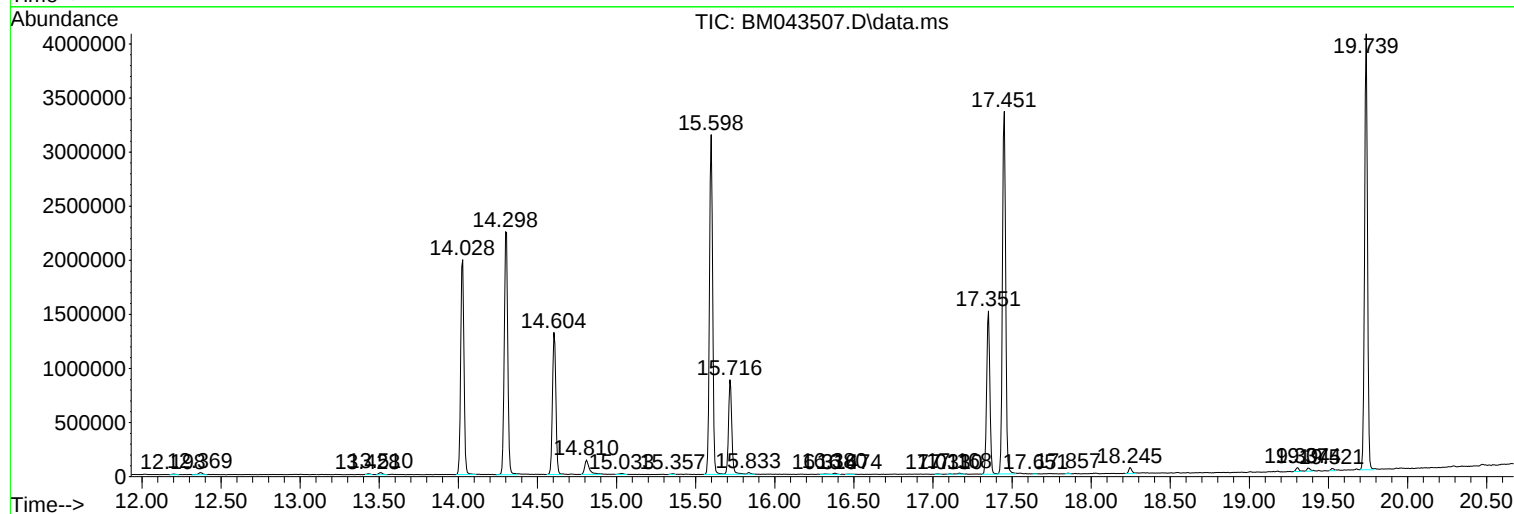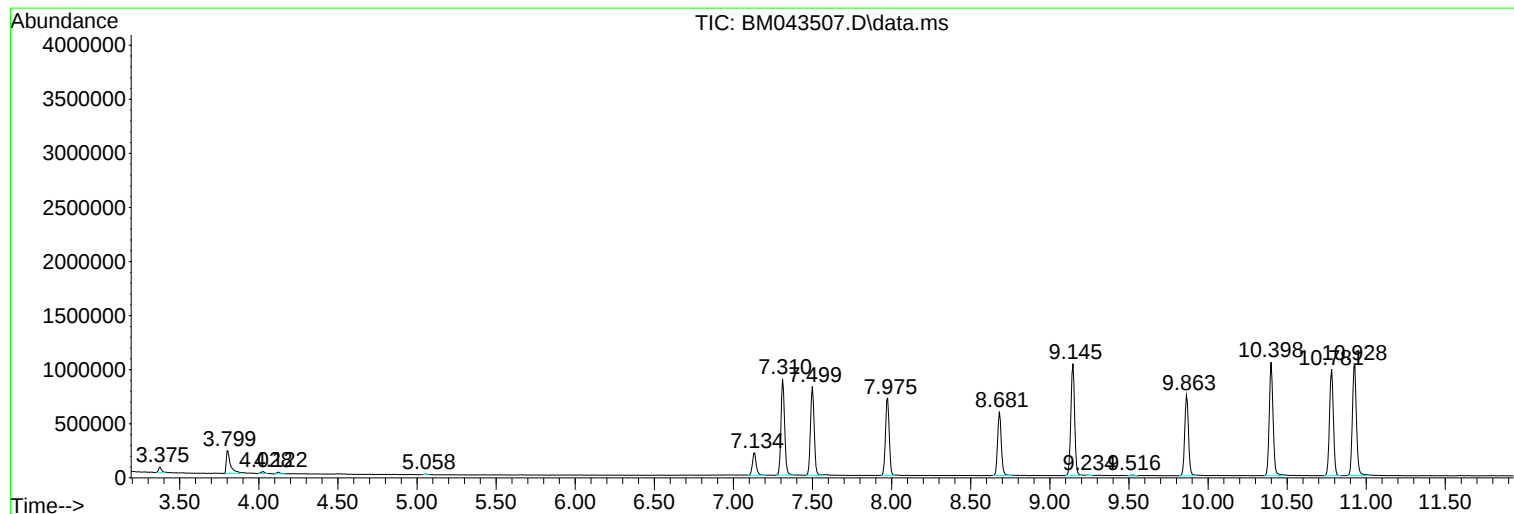

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043507.D
Acq On : 21 Dec 2023 17:47
Operator : MA/JU
Sample : 05912-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3M9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043507.D
Acq On : 21 Dec 2023 17:47
Operator : MA/JU
Sample : 05912-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3M9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------