

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043509.D
 Acq On : 21 Dec 2023 18:59
 Operator : MA/JU
 Sample : 05912-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3N7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043509.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	29	32	40	rVB	49279	68302	1.28%	0.139%
2	3.805	101	105	120	rBV	168718	302266	5.64%	0.615%
3	4.022	139	142	148	rVB3	17366	28795	0.54%	0.059%
4	4.122	157	159	165	rVB	15199	17781	0.33%	0.036%
5	5.052	315	317	321	rVB5	6683	8784	0.16%	0.018%
6	7.134	664	671	679	rBV	192163	319589	5.97%	0.650%
7	7.310	692	701	716	rBV	801358	1289422	24.08%	2.624%
8	7.498	726	733	743	rBV	725641	1174846	21.94%	2.391%
9	7.975	806	814	824	rBV	708075	1165718	21.77%	2.372%
10	8.681	926	934	950	rBV	564989	926812	17.30%	1.886%
11	9.145	1005	1013	1023	rBV	959458	1578527	29.47%	3.213%
12	9.245	1027	1030	1035	rVV6	9093	15784	0.29%	0.032%
13	9.310	1038	1041	1045	rVB6	4461	6565	0.12%	0.013%
14	9.528	1074	1078	1080	rVB4	6787	7148	0.13%	0.015%
15	9.863	1127	1135	1146	rBV	672988	1127744	21.06%	2.295%
16	10.292	1205	1208	1211	rBV5	3417	6065	0.11%	0.012%
17	10.398	1218	1226	1237	rBV	954732	1610601	30.07%	3.278%
18	10.781	1283	1291	1301	rBV	985435	1674892	31.27%	3.409%
19	10.922	1307	1315	1331	rBV	827898	1509259	28.18%	3.072%
20	12.022	1498	1502	1507	rVB	5853	8257	0.15%	0.017%
21	12.198	1529	1532	1536	rVB5	5153	6862	0.13%	0.014%
22	12.369	1554	1561	1567	rVB3	17118	30945	0.58%	0.063%
23	13.222	1703	1706	1712	rBV6	4890	8169	0.15%	0.017%
24	13.428	1738	1741	1748	rVB7	8034	12913	0.24%	0.026%
25	13.510	1748	1755	1761	rBV2	24023	42533	0.79%	0.087%
26	13.586	1764	1768	1773	rVB7	5716	8814	0.16%	0.018%
27	14.022	1835	1842	1852	rBV	1808705	2621890	48.95%	5.336%
28	14.298	1879	1889	1904	rBV2	2087678	3191170	59.58%	6.495%
29	14.604	1933	1941	1950	rBV	1405213	2090359	39.03%	4.254%
30	14.810	1969	1976	1986	rBV2	134322	270824	5.06%	0.551%
31	15.022	2008	2012	2020	rVB10	11312	23004	0.43%	0.047%
32	15.357	2064	2069	2072	rBV4	4585	6178	0.12%	0.013%
33	15.598	2102	2110	2122	rBV	2884158	4027935	75.21%	8.198%
34	15.716	2124	2130	2140	rBV	787435	1128839	21.08%	2.297%
35	15.839	2147	2151	2156	rVB5	14394	21472	0.40%	0.044%
36	16.380	2240	2243	2250	rVB8	8476	14794	0.28%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043509.D
 Acq On : 21 Dec 2023 18:59
 Operator : MA/JU
 Sample : 05912-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3N7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	16.751	2303	2306	2312	rBV7	6810	9871	0.18%	0.020%
38	17.027	2350	2353	2357	rVB6	4557	7133	0.13%	0.015%
39	17.163	2368	2376	2383	rBV	56581	85612	1.60%	0.174%
40	17.263	2389	2393	2398	rBV6	3118	5953	0.11%	0.012%
41	17.351	2401	2408	2418	rVV	1629773	2356422	44.00%	4.796%
42	17.451	2418	2425	2446	rVB	3221333	4634801	86.54%	9.433%
43	18.027	2519	2523	2528	rVB8	3702	7021	0.13%	0.014%
44	18.245	2554	2560	2566	rBV	63938	93688	1.75%	0.191%
45	18.327	2569	2574	2578	rVB	16237	24333	0.45%	0.050%
46	19.304	2736	2740	2744	rBV2	33693	44690	0.83%	0.091%
47	19.374	2747	2752	2755	rBV	32208	45673	0.85%	0.093%
48	19.521	2774	2777	2784	rBV4	30625	45244	0.84%	0.092%
49	19.680	2801	2804	2807	rBV5	12495	15559	0.29%	0.032%
50	19.739	2808	2814	2821	rBV	3862103	5022352	93.77%	10.222%
51	21.251	3067	3071	3076	rBV3	67648	98741	1.84%	0.201%
52	21.527	3113	3118	3127	rBV2	1792358	2356765	44.00%	4.797%
53	23.792	3495	3503	3514	rBV2	2784652	5355803	100.00%	10.900%
54	23.944	3522	3529	3540	rVB	1286585	2571310	48.01%	5.233%




Sum of corrected areas: 49134829

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043509.D
Acq On : 21 Dec 2023 18:59
Operator : MA/JU
Sample : 05912-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3N7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

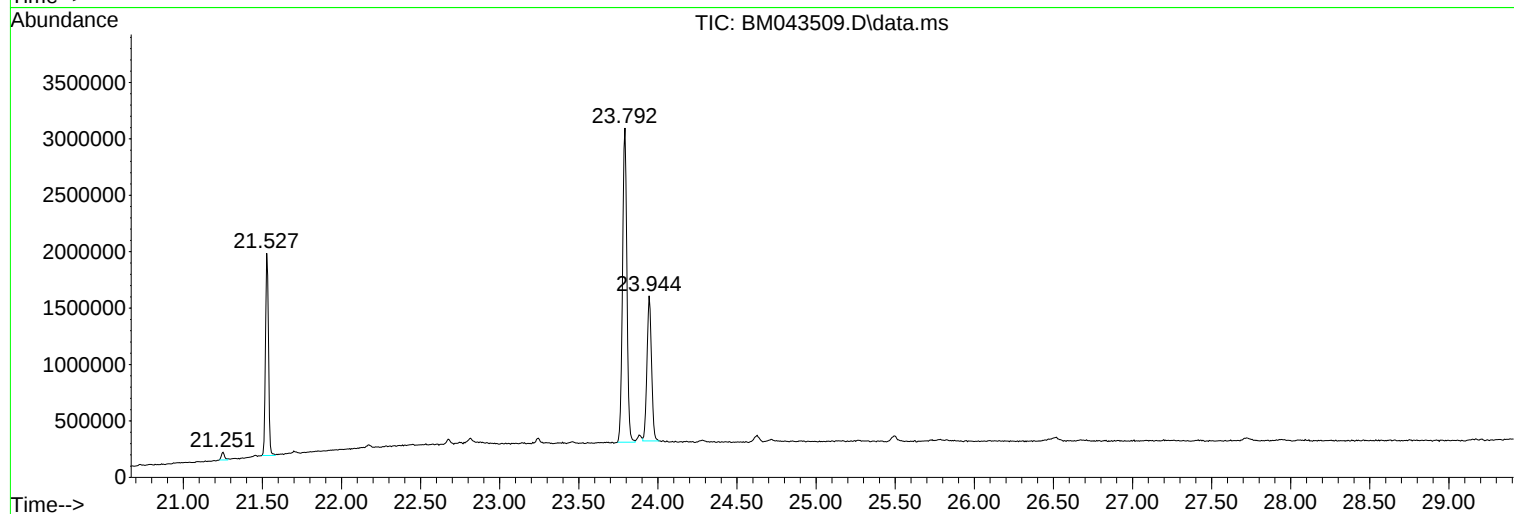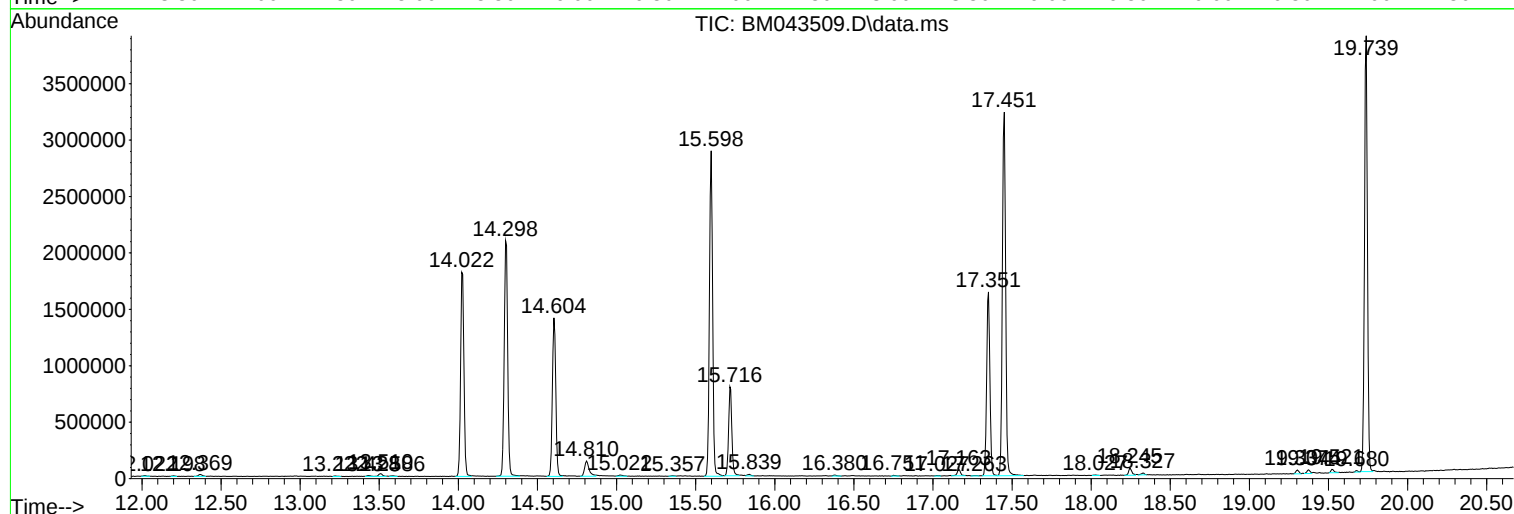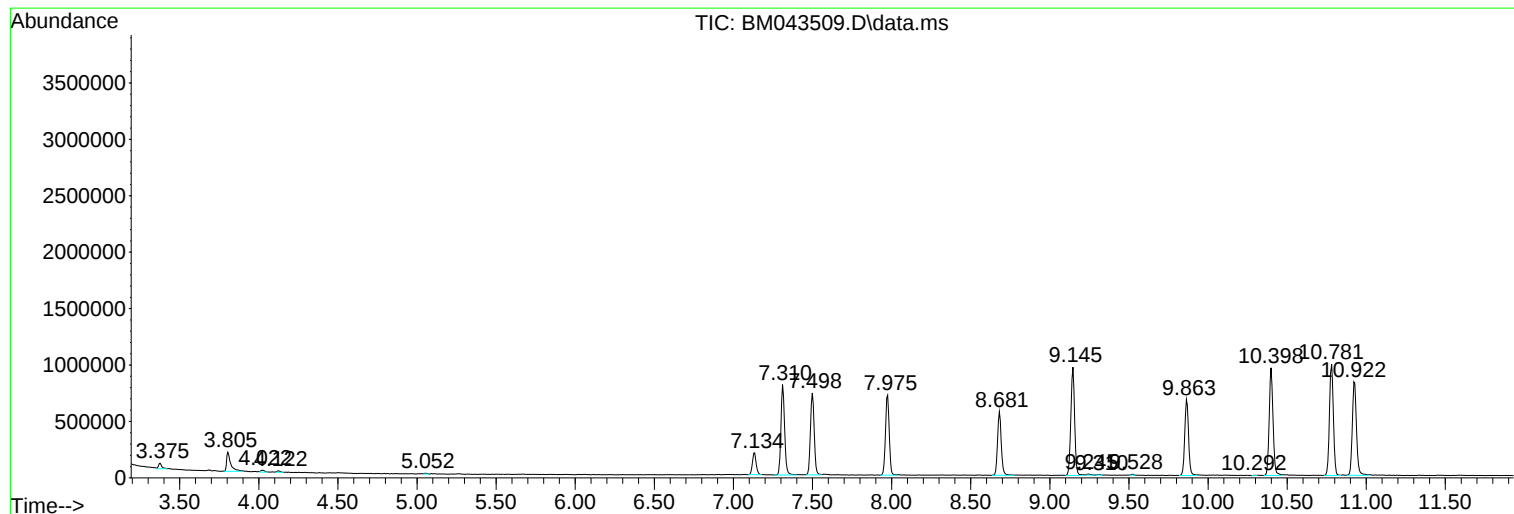

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043509.D
Acq On : 21 Dec 2023 18:59
Operator : MA/JU
Sample : 05912-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3N7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043509.D
Acq On : 21 Dec 2023 18:59
Operator : MA/JU
Sample : 05912-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3N7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc