

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043513.D
 Acq On : 21 Dec 2023 21:23
 Operator : MA/JU
 Sample : PB157941BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK941

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	28	31	42	rVB	89390	123778	2.34%	0.212%
2	3.793	100	103	123	rBV	1048047	1647142	31.12%	2.816%
3	4.122	155	159	163	rBV	16936	22079	0.42%	0.038%
4	7.128	664	670	680	rBV	1197102	1922478	36.33%	3.287%
5	7.310	694	701	713	rBV	923048	1488774	28.13%	2.545%
6	7.499	724	733	744	rBV	1154511	1860715	35.16%	3.181%
7	7.969	806	813	822	rBV	803720	1304065	24.64%	2.230%
8	8.681	927	934	946	rBV	1387278	2221381	41.98%	3.798%
9	9.146	1004	1013	1024	rBV	1085391	1793461	33.89%	3.066%
10	9.863	1127	1135	1146	rBV	832494	1371919	25.92%	2.346%
11	9.969	1151	1153	1159	rVB6	2791	6401	0.12%	0.011%
12	10.398	1217	1226	1243	rBV	1190988	2056458	38.86%	3.516%
13	10.781	1283	1291	1298	rBV	1094041	1837690	34.73%	3.142%
14	10.828	1298	1299	1305	rVB	14318	16929	0.32%	0.029%
15	10.922	1307	1315	1331	rBV	1286513	2311335	43.68%	3.952%
16	12.369	1556	1561	1569	rBV	20966	33716	0.64%	0.058%
17	12.445	1569	1574	1579	rVB2	10290	18943	0.36%	0.032%
18	12.657	1606	1610	1616	rVB5	6025	9435	0.18%	0.016%
19	13.451	1740	1745	1749	rVV7	6460	12790	0.24%	0.022%
20	13.510	1749	1755	1764	rVB2	19632	34009	0.64%	0.058%
21	14.022	1836	1842	1852	rBV	2009918	2821440	53.31%	4.824%
22	14.298	1882	1889	1905	rBV	2338477	3457703	65.34%	5.912%
23	14.604	1935	1941	1948	rBV	1496762	2166889	40.95%	3.705%
24	14.669	1948	1952	1957	rVB	31285	45284	0.86%	0.077%
25	14.804	1969	1975	1992	rBV	1048507	1675474	31.66%	2.865%
26	15.010	2004	2010	2017	rVB	22774	41764	0.79%	0.071%
27	15.598	2100	2110	2116	rBV	3026967	4178965	78.97%	7.145%
28	15.651	2116	2119	2124	rVV	31541	51882	0.98%	0.089%
29	15.716	2124	2130	2144	rVV	854065	1250722	23.63%	2.138%
30	15.839	2146	2151	2155	rVB6	15346	28621	0.54%	0.049%
31	16.010	2175	2180	2183	rBV6	2931	5536	0.10%	0.009%
32	16.086	2191	2193	2203	rVB10	4263	7567	0.14%	0.013%
33	16.710	2295	2299	2302	rBV4	3706	5794	0.11%	0.010%
34	17.033	2349	2354	2357	rVB7	3401	6098	0.12%	0.010%
35	17.169	2375	2377	2380	rVB4	5388	5624	0.11%	0.010%
36	17.351	2400	2408	2413	rBV	1721956	2464225	46.56%	4.213%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043513.D
 Acq On : 21 Dec 2023 21:23
 Operator : MA/JU
 Sample : PB157941BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK941

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	17.392	2413	2415	2419	rVV	82669	96039	1.81%	0.164%
38	17.451	2419	2425	2437	rVB	3081429	4475268	84.56%	7.651%
39	18.251	2554	2561	2563	rBV5	9615	18139	0.34%	0.031%
40	18.280	2563	2566	2568	rVB4	4842	6525	0.12%	0.011%
41	18.421	2587	2590	2595	rVB5	9244	9160	0.17%	0.016%
42	19.163	2712	2716	2717	rBV4	5976	6513	0.12%	0.011%
43	19.304	2735	2740	2744	rBV3	32064	46689	0.88%	0.080%
44	19.374	2747	2752	2754	rVV	28733	41035	0.78%	0.070%
45	19.404	2754	2757	2761	rVB	34432	43945	0.83%	0.075%
46	19.533	2774	2779	2783	rBV8	7446	16268	0.31%	0.028%
47	19.739	2807	2814	2826	rBV	3683849	4953286	93.60%	8.469%
48	21.527	3113	3118	3128	rBV	1930788	2492951	47.11%	4.262%
49	23.792	3495	3503	3514	rBV	2779796	5292123	100.00%	9.048%
50	23.945	3522	3529	3540	rVB	1301701	2684143	50.72%	4.589%




Sum of corrected areas: 58489170

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043513.D
Acq On : 21 Dec 2023 21:23
Operator : MA/JU
Sample : PB157941BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK941

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

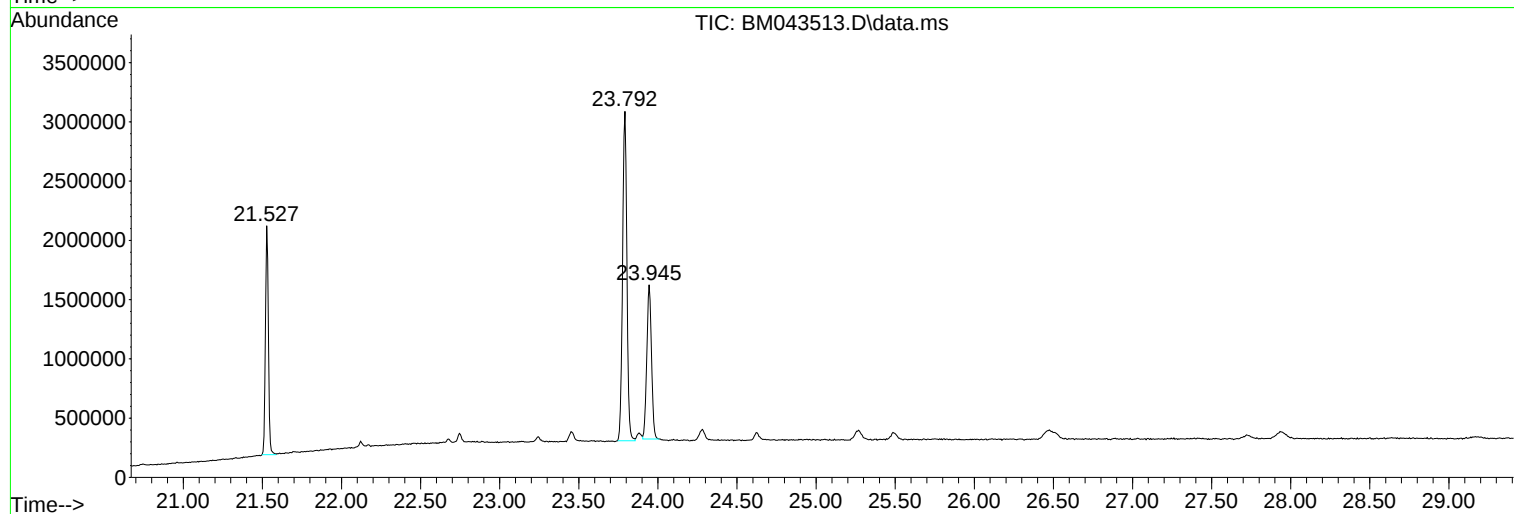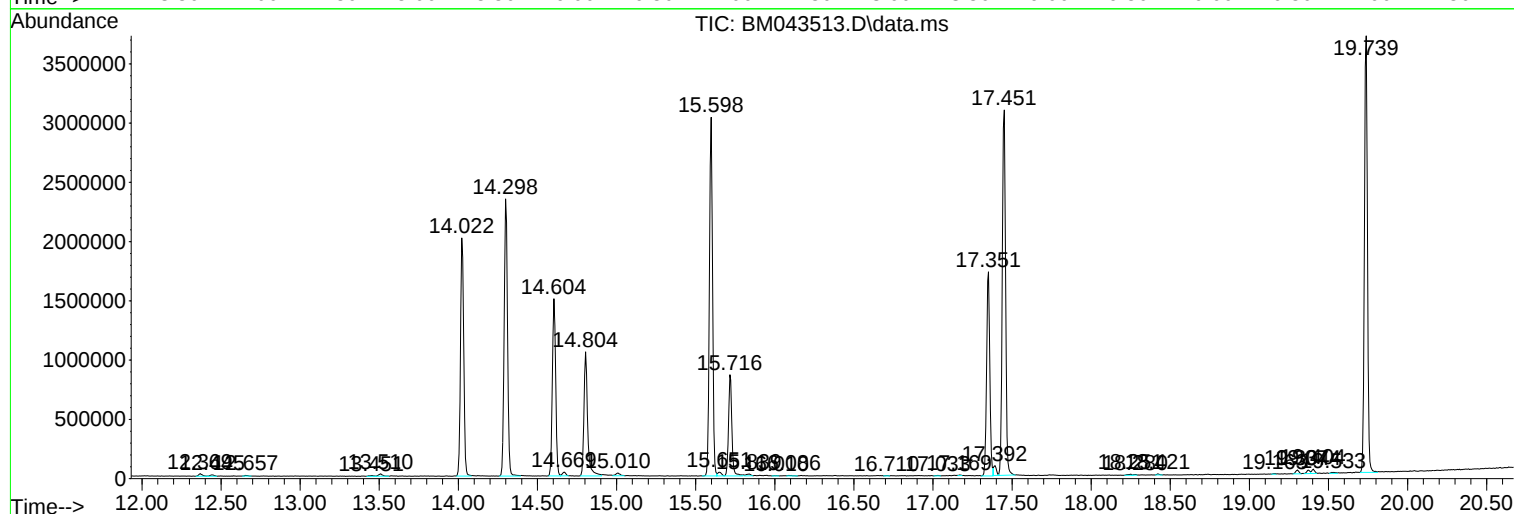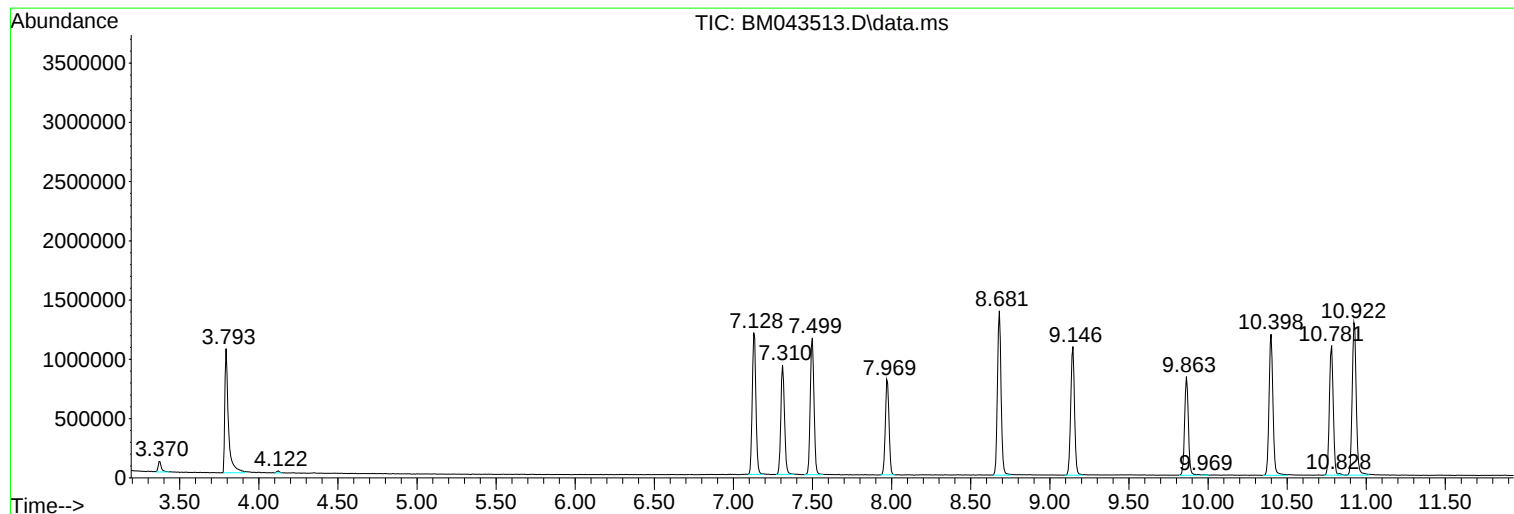

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043513.D
Acq On : 21 Dec 2023 21:23
Operator : MA/JU
Sample : PB157941BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK941

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043513.D
Acq On : 21 Dec 2023 21:23
Operator : MA/JU
Sample : PB157941BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK941

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------