

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043516.D
 Acq On : 21 Dec 2023 23:47
 Operator : MA/JU
 Sample : PB157939BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK939

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	28	31	39	rBV	86686	114335	2.24%	0.186%
2	3.793	100	103	130	rBV	1054737	1696967	33.24%	2.758%
3	4.122	155	159	165	rVB	21605	28921	0.57%	0.047%
4	5.658	417	420	425	rBV6	3081	6349	0.12%	0.010%
5	7.128	663	670	683	rBV	1234628	1963174	38.46%	3.191%
6	7.310	692	701	711	rBV	939964	1522102	29.82%	2.474%
7	7.499	725	733	745	rBV	1175506	1887425	36.98%	3.067%
8	7.969	806	813	822	rBV	995773	1626869	31.87%	2.644%
9	8.681	927	934	948	rBV	1383978	2260288	44.28%	3.673%
10	9.063	997	999	1004	rBV6	2878	5226	0.10%	0.008%
11	9.146	1004	1013	1020	rBV	1067395	1806366	35.39%	2.936%
12	9.863	1126	1135	1146	rBV	829542	1371782	26.87%	2.229%
13	10.398	1217	1226	1242	rBV	1209985	2065592	40.47%	3.357%
14	10.781	1283	1291	1298	rBV	1331491	2286791	44.80%	3.716%
15	10.922	1307	1315	1330	rBV	1324630	2327418	45.59%	3.782%
16	12.369	1556	1561	1568	rVB3	17559	32495	0.64%	0.053%
17	12.445	1568	1574	1576	rBV4	10988	18140	0.36%	0.029%
18	12.663	1606	1611	1618	rVB9	6229	12884	0.25%	0.021%
19	13.504	1749	1754	1760	rVV4	14757	24956	0.49%	0.041%
20	13.575	1763	1766	1772	rVB6	3825	5529	0.11%	0.009%
21	14.022	1836	1842	1855	rBV	1962523	2822173	55.29%	4.587%
22	14.298	1882	1889	1899	rBV	2376470	3474643	68.07%	5.647%
23	14.604	1934	1941	1948	rBV	1892019	2722742	53.34%	4.425%
24	14.669	1948	1952	1957	rVB2	31142	47855	0.94%	0.078%
25	14.804	1969	1975	1996	rBV	1010392	1685657	33.02%	2.739%
26	15.010	2004	2010	2016	rVB	21248	35914	0.70%	0.058%
27	15.598	2103	2110	2116	rBV	2998089	4172660	81.74%	6.781%
28	15.651	2116	2119	2125	rVV	32970	48856	0.96%	0.079%
29	15.716	2125	2130	2143	rVV	865976	1224865	24.00%	1.991%
30	15.833	2143	2150	2157	rVB8	15128	33102	0.65%	0.054%
31	17.169	2374	2377	2382	rVB5	6240	7065	0.14%	0.011%
32	17.351	2401	2408	2413	rBV	2113189	3051404	59.78%	4.959%
33	17.392	2413	2415	2419	rVV	86416	103855	2.03%	0.169%
34	17.451	2419	2425	2439	rVV2	3043468	4467272	87.52%	7.260%
35	18.427	2586	2591	2595	rBV7	8053	11774	0.23%	0.019%
36	18.727	2636	2642	2643	rBV6	4818	8301	0.16%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043516.D
Acq On : 21 Dec 2023 23:47
Operator : MA/JU
Sample : PB157939BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK939

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	19.304	2736	2740	2744	rBV3	30922	39235	0.77%	0.064%
38	19.374	2748	2752	2754	rVV	28286	38975	0.76%	0.063%
39	19.404	2754	2757	2764	rVB	33048	45833	0.90%	0.074%
40	19.739	2807	2814	2829	rBV	3703652	4916131	96.31%	7.990%
41	21.527	3113	3118	3129	rBV	2419104	3056360	59.88%	4.967%
42	23.786	3495	3502	3512	rBV2	2670615	5104550	100.00%	8.296%
43	23.945	3522	3529	3542	rVB	1619036	3348779	65.60%	5.442%




Sum of corrected areas: 61531610

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043516.D
Acq On : 21 Dec 2023 23:47
Operator : MA/JU
Sample : PB157939BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK939

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

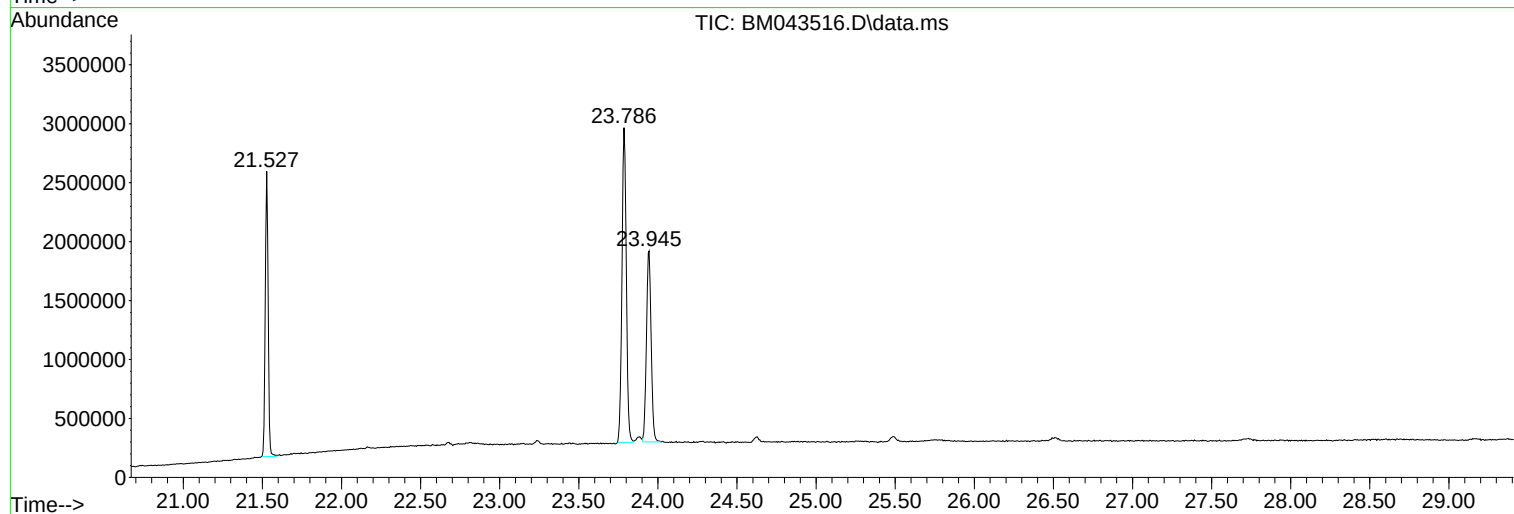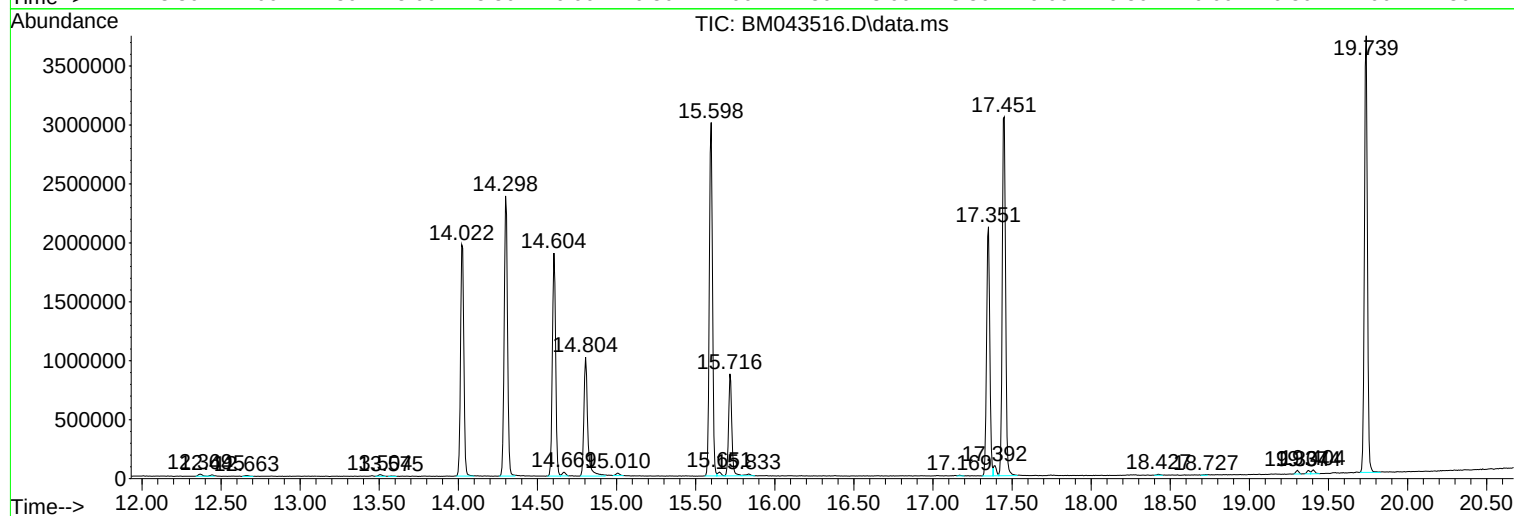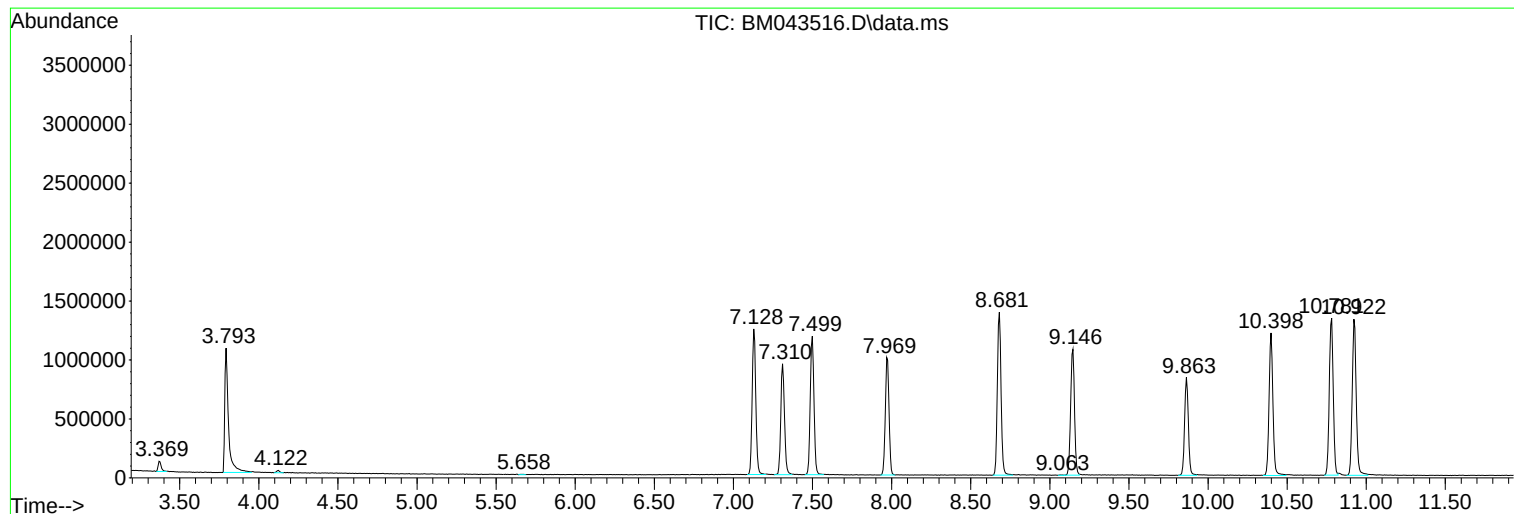

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043516.D
Acq On : 21 Dec 2023 23:47
Operator : MA/JU
Sample : PB157939BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK939

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043516.D
Acq On : 21 Dec 2023 23:47
Operator : MA/JU
Sample : PB157939BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK939

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc