

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043526.D
 Acq On : 22 Dec 2023 05:47
 Operator : MA/JU
 Sample : 05912-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3L2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	28	32	40	rVB	51622	76226	1.40%	0.143%
2	3.799	101	104	119	rBV	265515	463167	8.52%	0.867%
3	4.028	139	143	148	rVB	16199	24854	0.46%	0.047%
4	4.122	155	159	163	rBV	16313	25244	0.46%	0.047%
5	4.575	232	236	244	rVB	25804	43519	0.80%	0.081%
6	4.951	296	300	306	rBV5	12717	20913	0.38%	0.039%
7	5.051	315	317	320	rBV3	4995	5475	0.10%	0.010%
8	7.128	664	670	680	rVB	203924	339946	6.25%	0.637%
9	7.310	694	701	710	rBV	865620	1397397	25.70%	2.617%
10	7.498	725	733	742	rBV	792407	1295876	23.83%	2.426%
11	7.969	806	813	823	rBV	765683	1254255	23.07%	2.349%
12	8.328	870	874	877	rBV6	3980	6830	0.13%	0.013%
13	8.681	926	934	946	rBV	570395	944705	17.37%	1.769%
14	9.145	1005	1013	1020	rBV	1005979	1690553	31.09%	3.165%
15	9.863	1127	1135	1149	rBV	750740	1247063	22.93%	2.335%
16	10.398	1217	1226	1243	rBV	1002560	1762523	32.41%	3.300%
17	10.780	1283	1291	1299	rBV	1019936	1771112	32.57%	3.316%
18	10.922	1307	1315	1328	rBV	1041552	1843600	33.90%	3.452%
19	11.604	1430	1431	1436	rVB5	6325	6620	0.12%	0.012%
20	12.010	1495	1500	1504	rBV6	5281	9539	0.18%	0.018%
21	12.192	1525	1531	1537	rBV6	4602	11374	0.21%	0.021%
22	12.369	1554	1561	1568	rBV4	16664	30747	0.57%	0.058%
23	13.433	1739	1742	1747	rVB5	4988	8329	0.15%	0.016%
24	13.510	1747	1755	1759	rBV3	23808	42891	0.79%	0.080%
25	13.586	1764	1768	1772	rVB6	4072	7181	0.13%	0.013%
26	14.021	1835	1842	1856	rBV	1981074	2782296	51.17%	5.210%
27	14.298	1881	1889	1900	rBV	2316199	3348884	61.59%	6.271%
28	14.604	1933	1941	1949	rBV	1479489	2137766	39.31%	4.003%
29	14.810	1970	1976	1988	rBV	139920	280798	5.16%	0.526%
30	15.033	2010	2014	2019	rVB6	5891	11275	0.21%	0.021%
31	15.598	2103	2110	2124	rBV	2899271	4185034	76.96%	7.836%
32	15.715	2124	2130	2144	rVV	910673	1301120	23.93%	2.436%
33	15.833	2147	2150	2155	rVB5	13768	21023	0.39%	0.039%
34	16.321	2226	2233	2237	rBV7	6088	13347	0.25%	0.025%
35	16.380	2238	2243	2249	rVB6	11564	15457	0.28%	0.029%
36	16.898	2326	2331	2336	rBV9	4147	8465	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043526.D
 Acq On : 22 Dec 2023 05:47
 Operator : MA/JU
 Sample : 05912-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3L2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	17.162	2368	2376	2385	rBV	1488708	1925758	35.41%	3.606%
38	17.351	2401	2408	2418	rVV	1709503	2414022	44.39%	4.520%
39	17.451	2418	2425	2439	rVV	3242809	4816533	88.58%	9.019%
40	17.704	2465	2468	2470	rBV3	5981	7864	0.14%	0.015%
41	18.033	2520	2524	2527	rBV5	14524	20142	0.37%	0.038%
42	18.245	2556	2560	2567	rVB2	37700	54119	1.00%	0.101%
43	18.327	2572	2574	2578	rVV4	6670	7261	0.13%	0.014%
44	19.303	2736	2740	2743	rVB2	30876	35207	0.65%	0.066%
45	19.374	2748	2752	2756	rBV2	30771	38635	0.71%	0.072%
46	19.521	2774	2777	2781	rBV5	20363	25159	0.46%	0.047%
47	19.674	2800	2803	2807	rVB5	13229	18500	0.34%	0.035%
48	19.733	2807	2813	2821	rBV	4164458	5346363	98.32%	10.011%
49	21.527	3112	3118	3127	rBV	1723640	2345622	43.14%	4.392%
50	23.786	3494	3502	3512	rBV2	2853881	5437768	100.00%	10.182%
51	23.938	3521	3528	3538	rVB	1189476	2477879	45.57%	4.640%




Sum of corrected areas: 53406236

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043526.D
Acq On : 22 Dec 2023 05:47
Operator : MA/JU
Sample : 05912-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3L2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

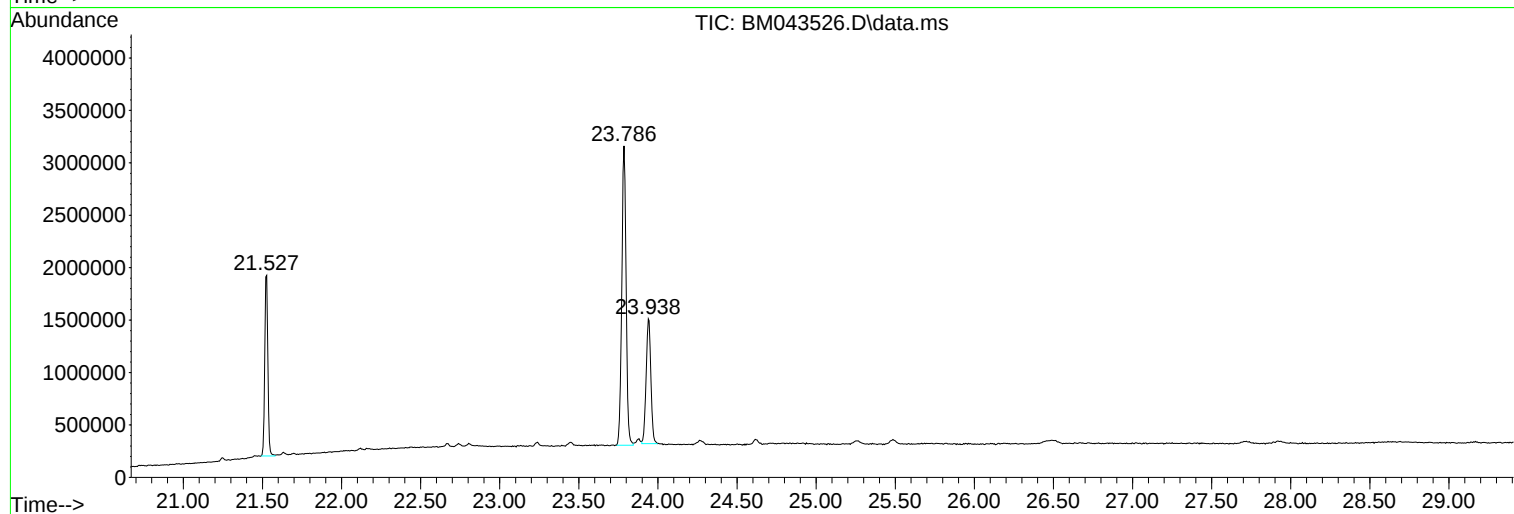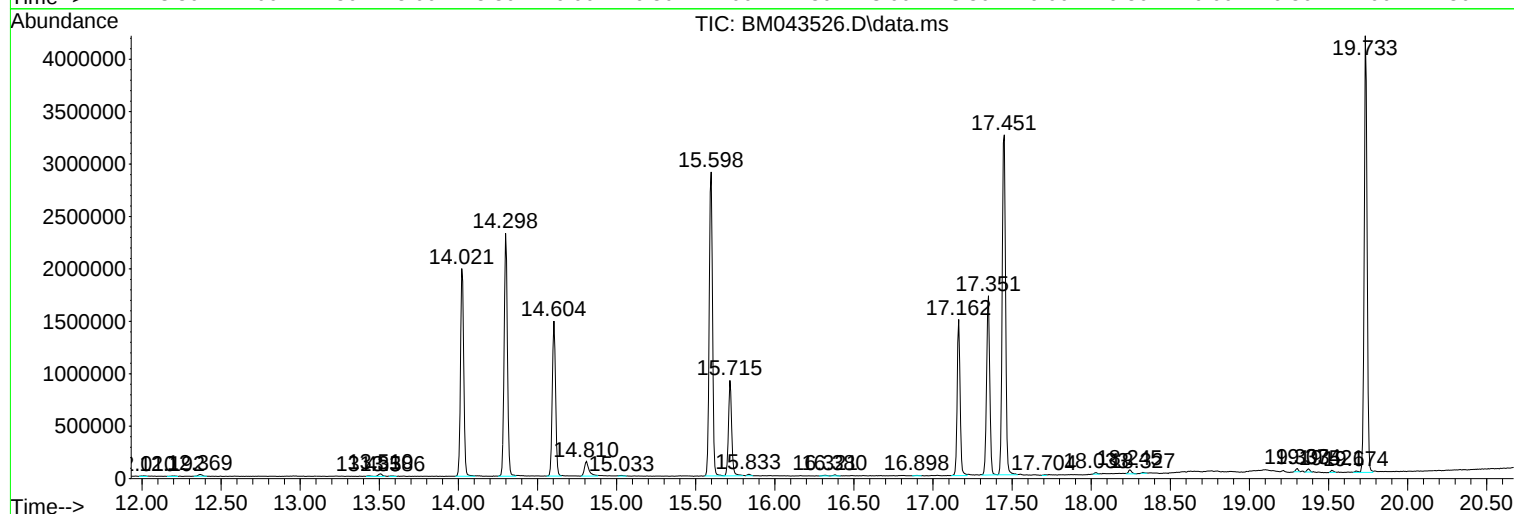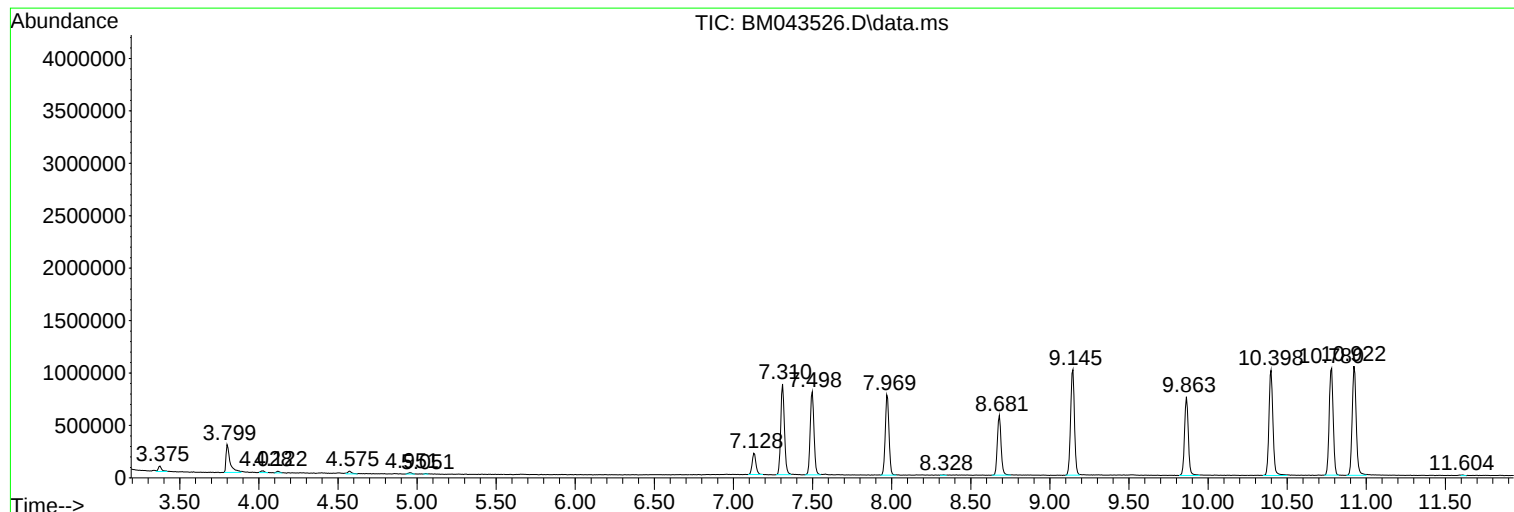

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043526.D
Acq On : 22 Dec 2023 05:47
Operator : MA/JU
Sample : 05912-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3L2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzenesulfonamide, N-butyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.162	15.95 ng/ul	1925760	Phenanthrene-d10	17.351

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	94
2			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	91
3			N-(2-Cyano-ethyl)-benzenesulfona...	210	C9H10N2O2S	002619-21-8	74
4			2-propenoic acid, 2-methyl-, 2-[...	269	C12H15NO4S	1000401-71-8	74
5			N-Benzenesulfonyloxy-2,2-bis(tri...	335	C10H7F6NO3S	055734-41-3	64

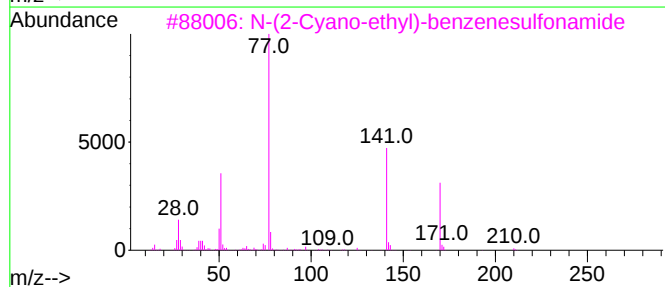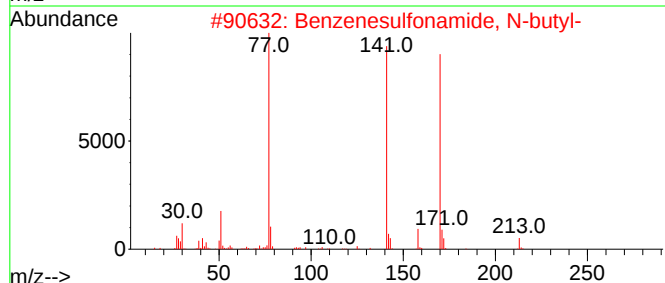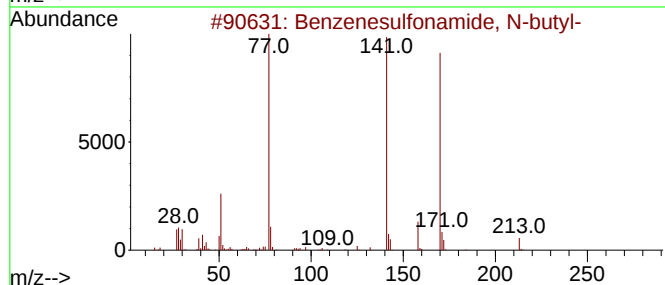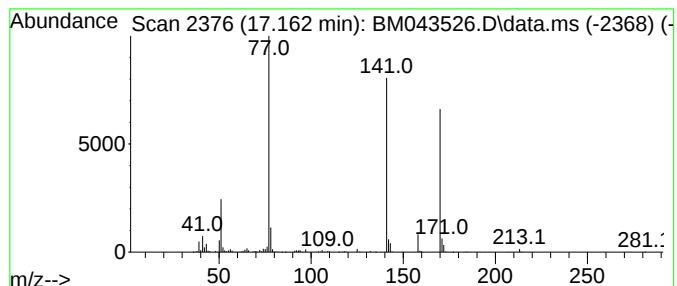

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043526.D
Acq On : 22 Dec 2023 05:47
Operator : MA/JU
Sample : 05912-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3L2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzenesulfonam...	17.162	15.9	ng/ul	1925760	4	17.351	2414020	20.0