

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043533.D
 Acq On : 22 Dec 2023 10:53
 Operator : MA/JU
 Sample : PB157969BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK969

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	28	31	38	rVB	77849	99501	2.32%	0.200%
2	3.793	100	103	131	rBV	924911	1494663	34.91%	3.004%
3	4.122	155	159	165	rVB	17644	24252	0.57%	0.049%
4	4.534	227	229	234	rVB5	4751	5914	0.14%	0.012%
5	7.128	663	670	681	rBV	1094473	1700409	39.72%	3.418%
6	7.310	694	701	711	rBV	807613	1314878	30.71%	2.643%
7	7.498	725	733	742	rBV	978957	1609319	37.59%	3.235%
8	7.969	806	813	824	rVB	793559	1256821	29.36%	2.526%
9	8.234	854	858	860	rVB5	4273	5587	0.13%	0.011%
10	8.316	869	872	876	rBV6	3066	5535	0.13%	0.011%
11	8.681	925	934	945	rBV	1150715	1900554	44.39%	3.820%
12	9.139	1003	1012	1023	rVV	914927	1559781	36.43%	3.135%
13	9.451	1061	1065	1068	rBV6	2452	4316	0.10%	0.009%
14	9.863	1127	1135	1147	rVV	705699	1157542	27.04%	2.327%
15	10.398	1218	1226	1245	rBV	977795	1761237	41.14%	3.540%
16	10.775	1282	1290	1298	rBV	1039022	1737126	40.58%	3.491%
17	10.922	1308	1315	1333	rBV	1119833	1980254	46.25%	3.980%
18	12.010	1496	1500	1508	rVB8	4136	10049	0.23%	0.020%
19	12.374	1553	1562	1567	rBV3	15465	30900	0.72%	0.062%
20	13.504	1749	1754	1763	rBV5	15202	28603	0.67%	0.057%
21	14.021	1834	1842	1853	rBV	1593082	2309957	53.96%	4.643%
22	14.298	1882	1889	1904	rBV	1956596	2867564	66.98%	5.764%
23	14.604	1933	1941	1949	rBV	1356265	2016433	47.10%	4.053%
24	14.804	1968	1975	1993	rBV	771066	1321144	30.86%	2.655%
25	15.598	2099	2110	2122	rBV	2329276	3450190	80.59%	6.935%
26	15.715	2124	2130	2144	rVV	668830	946742	22.11%	1.903%
27	15.833	2147	2150	2157	rVB8	12265	18134	0.42%	0.036%
28	16.327	2230	2234	2236	rBV5	4080	4959	0.12%	0.010%
29	16.380	2239	2243	2247	rVB7	7023	9641	0.23%	0.019%
30	16.809	2313	2316	2322	rVB8	2933	5049	0.12%	0.010%
31	17.021	2351	2352	2358	rVB6	5159	4906	0.11%	0.010%
32	17.127	2366	2370	2373	rBV6	4485	7786	0.18%	0.016%
33	17.351	2401	2408	2417	rBV	1534244	2237660	52.27%	4.498%
34	17.445	2418	2424	2436	rBV2	2507489	3656982	85.42%	7.350%
35	18.009	2517	2520	2521	rBV3	4517	4436	0.10%	0.009%
36	18.062	2526	2529	2530	rBV3	4059	4424	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043533.D
Acq On : 22 Dec 2023 10:53
Operator : MA/JU
Sample : PB157969BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK969

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	18.256	2555	2562	2565	rBV8	8947	17605	0.41%	0.035%
38	19.303	2737	2740	2744	rVB5	25907	34811	0.81%	0.070%
39	19.374	2747	2752	2757	rBV	21531	37381	0.87%	0.075%
40	19.521	2775	2777	2778	rBV2	8237	7448	0.17%	0.015%
41	19.733	2807	2813	2822	rBV	2920076	3996405	93.35%	8.032%
42	21.527	3113	3118	3126	rBV	1716797	2283176	53.33%	4.589%
43	23.785	3495	3502	3514	rBV	2202428	4281216	100.00%	8.605%
44	23.938	3522	3528	3543	rVB	1220033	2541795	59.37%	5.109%




Sum of corrected areas: 49753085

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043533.D
Acq On : 22 Dec 2023 10:53
Operator : MA/JU
Sample : PB157969BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK969

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

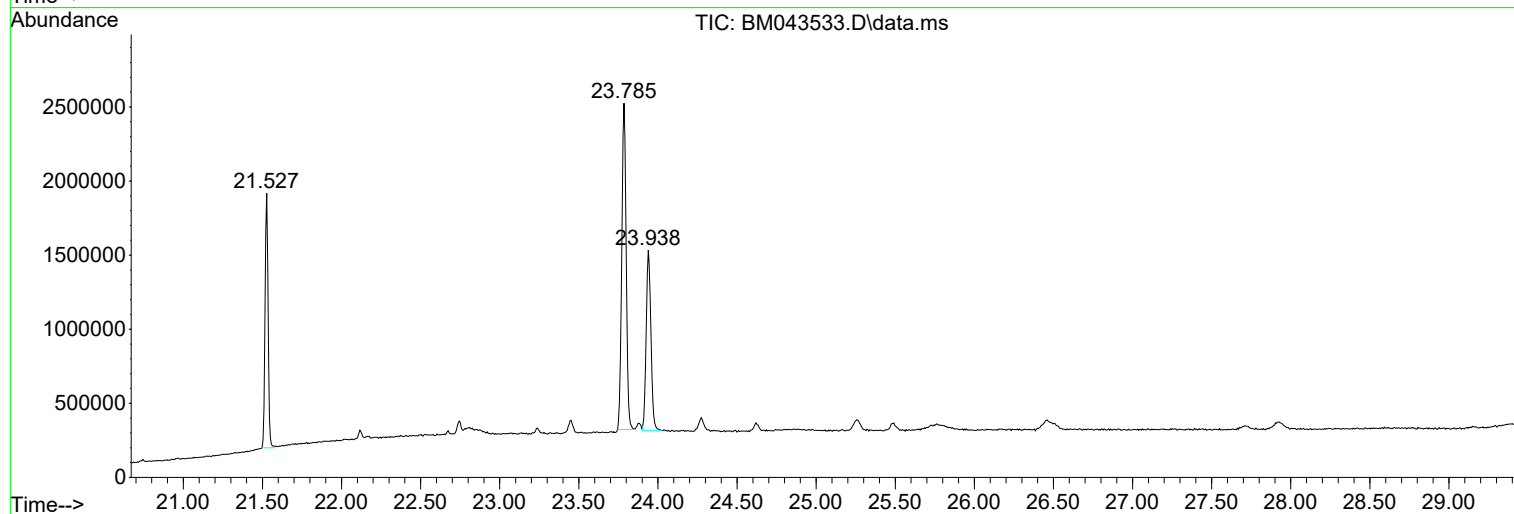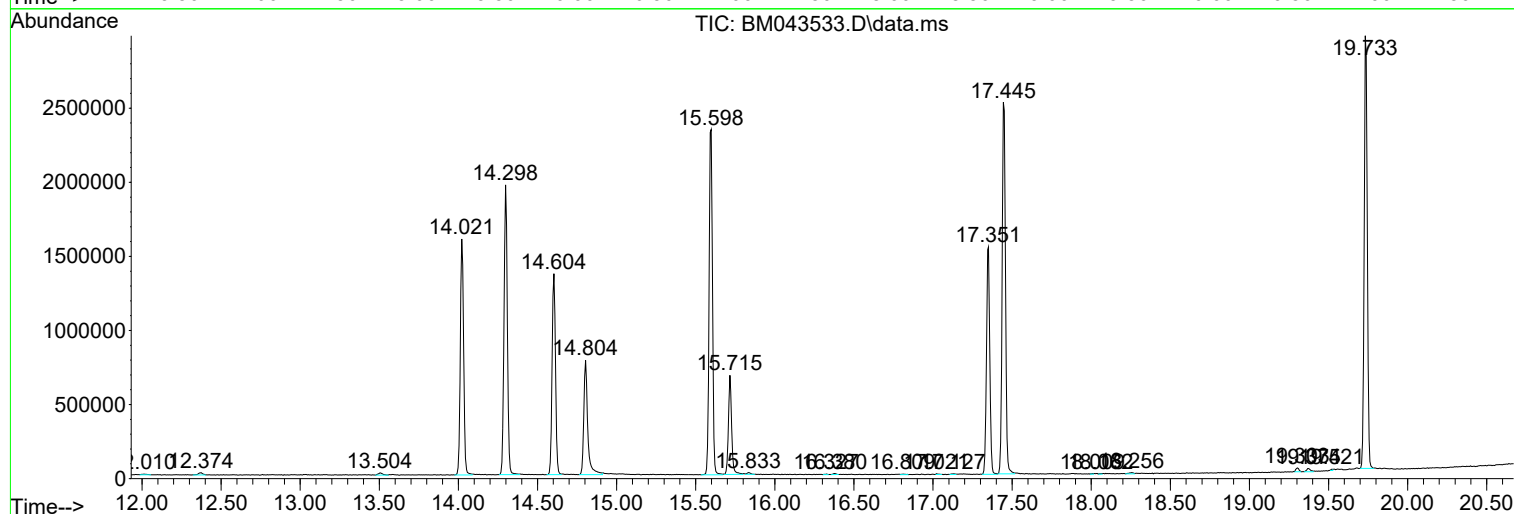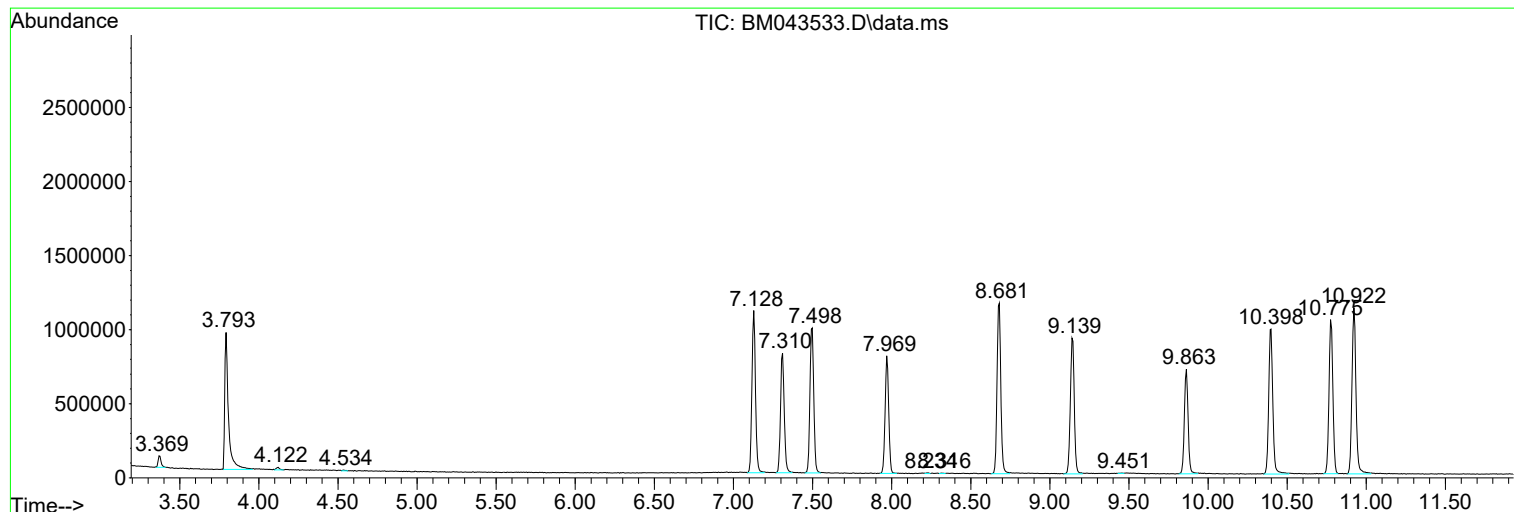

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043533.D
Acq On : 22 Dec 2023 10:53
Operator : MA/JU
Sample : PB157969BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK969

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043533.D
Acq On : 22 Dec 2023 10:53
Operator : MA/JU
Sample : PB157969BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK969

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc