

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043539.D
 Acq On : 22 Dec 2023 14:48
 Operator : MA/JU
 Sample : 05927-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGWA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043539.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	28	31	38	rVB	74007	92415	1.67%	0.153%
2	3.798	100	104	116	rBV	279947	472201	8.52%	0.784%
3	4.022	138	142	145	rVB2	23510	32575	0.59%	0.054%
4	4.116	155	158	163	rVB	18991	23541	0.42%	0.039%
5	5.045	314	316	321	rVB4	8280	12660	0.23%	0.021%
6	5.657	415	420	423	rBV6	5494	9110	0.16%	0.015%
7	7.128	663	670	677	rBV	281631	458354	8.27%	0.761%
8	7.304	693	700	713	rBV	1045577	1672198	30.16%	2.775%
9	7.492	724	732	742	rBV	991651	1592519	28.72%	2.643%
10	7.969	804	813	823	rBV	1094995	1744744	31.47%	2.896%
11	8.675	926	933	943	rBV	765489	1239032	22.34%	2.056%
12	9.139	1005	1012	1024	rBV	1223769	2006551	36.19%	3.330%
13	9.245	1024	1030	1036	rBV	34455	61864	1.12%	0.103%
14	9.522	1074	1077	1080	rVB3	7261	9320	0.17%	0.015%
15	9.863	1127	1135	1143	rBV	872900	1472693	26.56%	2.444%
16	10.098	1171	1175	1181	rVB8	3302	6056	0.11%	0.010%
17	10.392	1218	1225	1244	rBV	1219773	2111433	38.08%	3.504%
18	10.775	1282	1290	1298	rBV	1444097	2455746	44.29%	4.076%
19	10.922	1307	1315	1333	rBV	1211787	2177352	39.27%	3.614%
20	11.957	1484	1491	1492	rBV7	4236	5970	0.11%	0.010%
21	12.192	1528	1531	1536	rVB6	4011	6795	0.12%	0.011%
22	12.369	1555	1561	1566	rVB2	22381	36881	0.67%	0.061%
23	12.521	1582	1587	1594	rVV2	7358	16153	0.29%	0.027%
24	12.574	1594	1596	1601	rVB6	4750	6062	0.11%	0.010%
25	13.427	1736	1741	1745	rVV7	6060	10462	0.19%	0.017%
26	13.504	1748	1754	1761	rBV2	22054	39586	0.71%	0.066%
27	13.580	1763	1767	1775	rVB10	5821	12938	0.23%	0.021%
28	14.021	1831	1842	1858	rBV	2422019	3411558	61.52%	5.662%
29	14.298	1879	1889	1897	rBV2	2742859	3925965	70.80%	6.516%
30	14.604	1934	1941	1949	rBV	1925684	2869445	51.75%	4.762%
31	14.704	1957	1958	1966	rVB7	5372	10395	0.19%	0.017%
32	14.810	1970	1976	1987	rBV	169097	330784	5.97%	0.549%
33	15.021	2006	2012	2020	rVB10	15881	34875	0.63%	0.058%
34	15.598	2099	2110	2120	rBV	3537449	5036177	90.82%	8.358%
35	15.715	2124	2130	2145	rVV	1035618	1461596	26.36%	2.426%
36	15.833	2147	2150	2156	rVB6	18327	30165	0.54%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
 Data File : BM043539.D
 Acq On : 22 Dec 2023 14:48
 Operator : MA/JU
 Sample : 05927-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGWA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	16.157	2199	2205	2209	rBV8	3404	5689	0.10%	0.009%
38	16.321	2229	2233	2235	rBV5	5049	5677	0.10%	0.009%
39	16.380	2240	2243	2247	rVB6	11123	14260	0.26%	0.024%
40	16.751	2304	2306	2310	rBV4	3935	6158	0.11%	0.010%
41	17.033	2349	2354	2357	rVB7	5863	7992	0.14%	0.013%
42	17.162	2371	2376	2382	rBV	86372	116915	2.11%	0.194%
43	17.351	2400	2408	2418	rBV	2147185	3029578	54.64%	5.028%
44	17.451	2418	2425	2444	rVB	3721130	5451025	98.30%	9.047%
45	18.027	2519	2523	2524	rBV4	9356	10551	0.19%	0.018%
46	18.245	2555	2560	2568	rBV	107826	157470	2.84%	0.261%
47	18.321	2571	2573	2575	rBV3	6138	7424	0.13%	0.012%
48	19.303	2736	2740	2744	rVB	39231	51119	0.92%	0.085%
49	19.374	2748	2752	2755	rBV	38824	50709	0.91%	0.084%
50	19.521	2773	2777	2785	rBV3	77063	117214	2.11%	0.195%
51	19.674	2800	2803	2807	rBV4	13983	17402	0.31%	0.029%
52	19.739	2807	2814	2821	rBV	4082247	5545020	100.00%	9.203%
53	21.250	3068	3071	3079	rVB6	38794	64014	1.15%	0.106%
54	21.527	3113	3118	3129	rBV	2113732	2639887	47.61%	4.381%
55	23.785	3495	3502	3513	rVB	2738654	5300973	95.60%	8.798%
56	23.938	3522	3528	3538	rVB	1340208	2759907	49.77%	4.580%




Sum of corrected areas: 60255155

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043539.D
Acq On : 22 Dec 2023 14:48
Operator : MA/JU
Sample : 05927-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGWA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

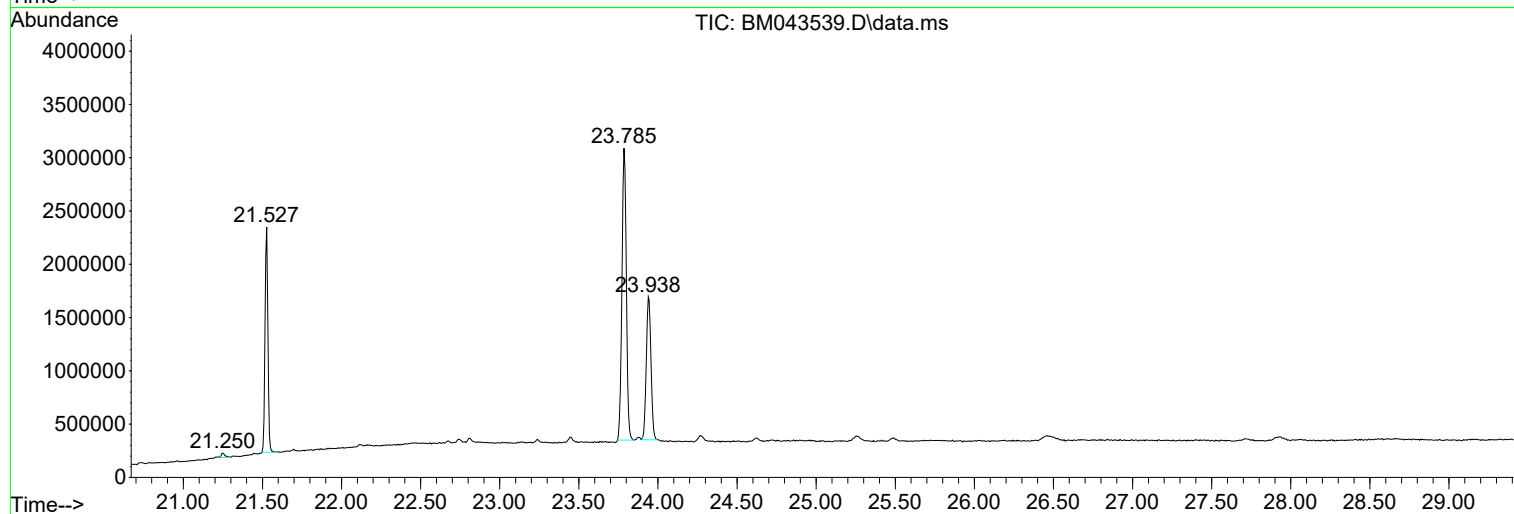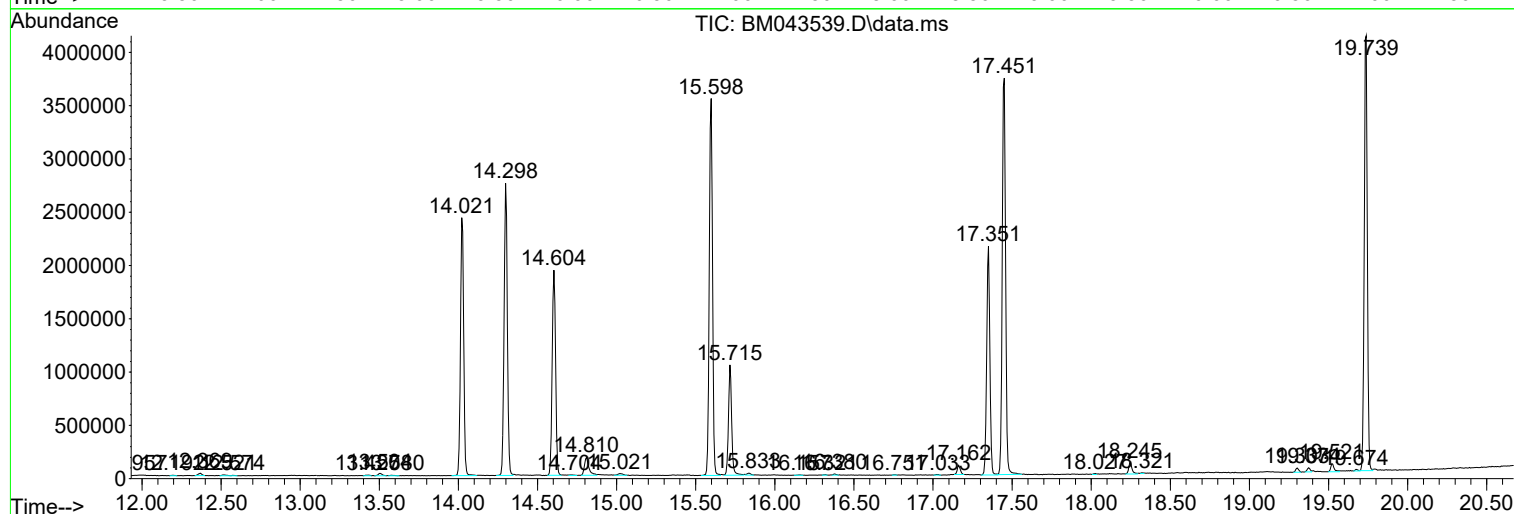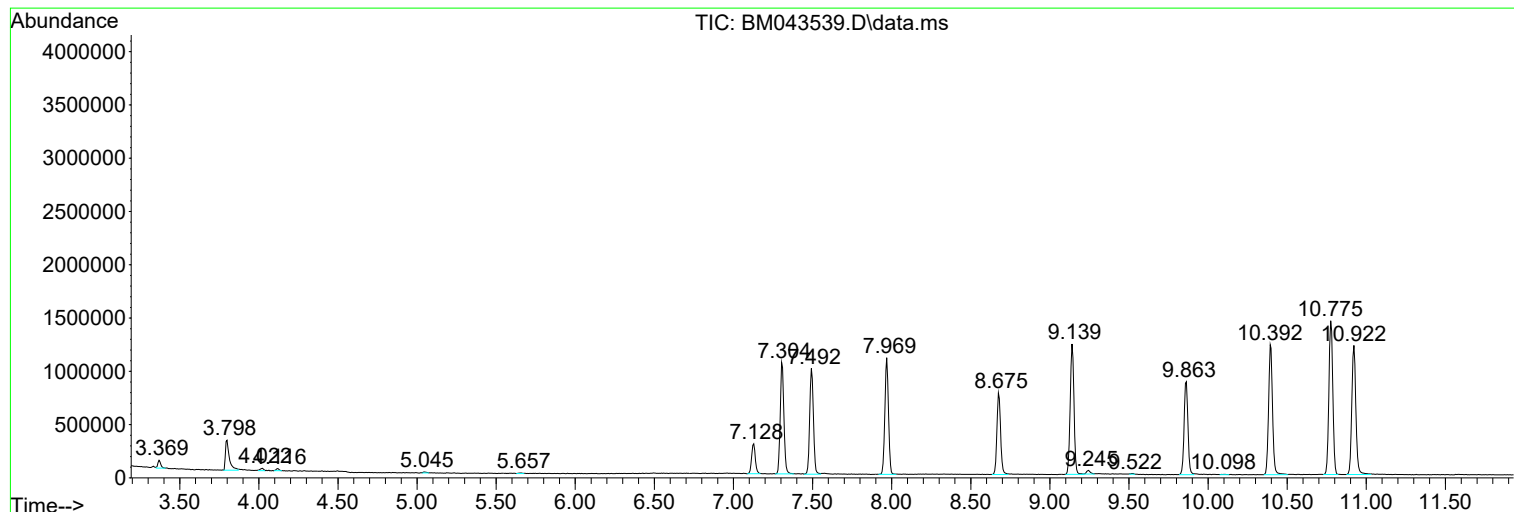

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043539.D
Acq On : 22 Dec 2023 14:48
Operator : MA/JU
Sample : 05927-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGWA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122123\
Data File : BM043539.D
Acq On : 22 Dec 2023 14:48
Operator : MA/JU
Sample : 05927-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGWA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc