


Data Path : Z:\HPCHEM1\BNA M\DATA\BM122215\
Data File : BM003701.D
Acq On : 22 Dec 2015 08:40
Operator : UM/SJ
Sample : DFTPP63
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP63

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM121915.M
Title : SVOA CALIBRATION
Last Update : Wed Dec 23 00:25:10 2015

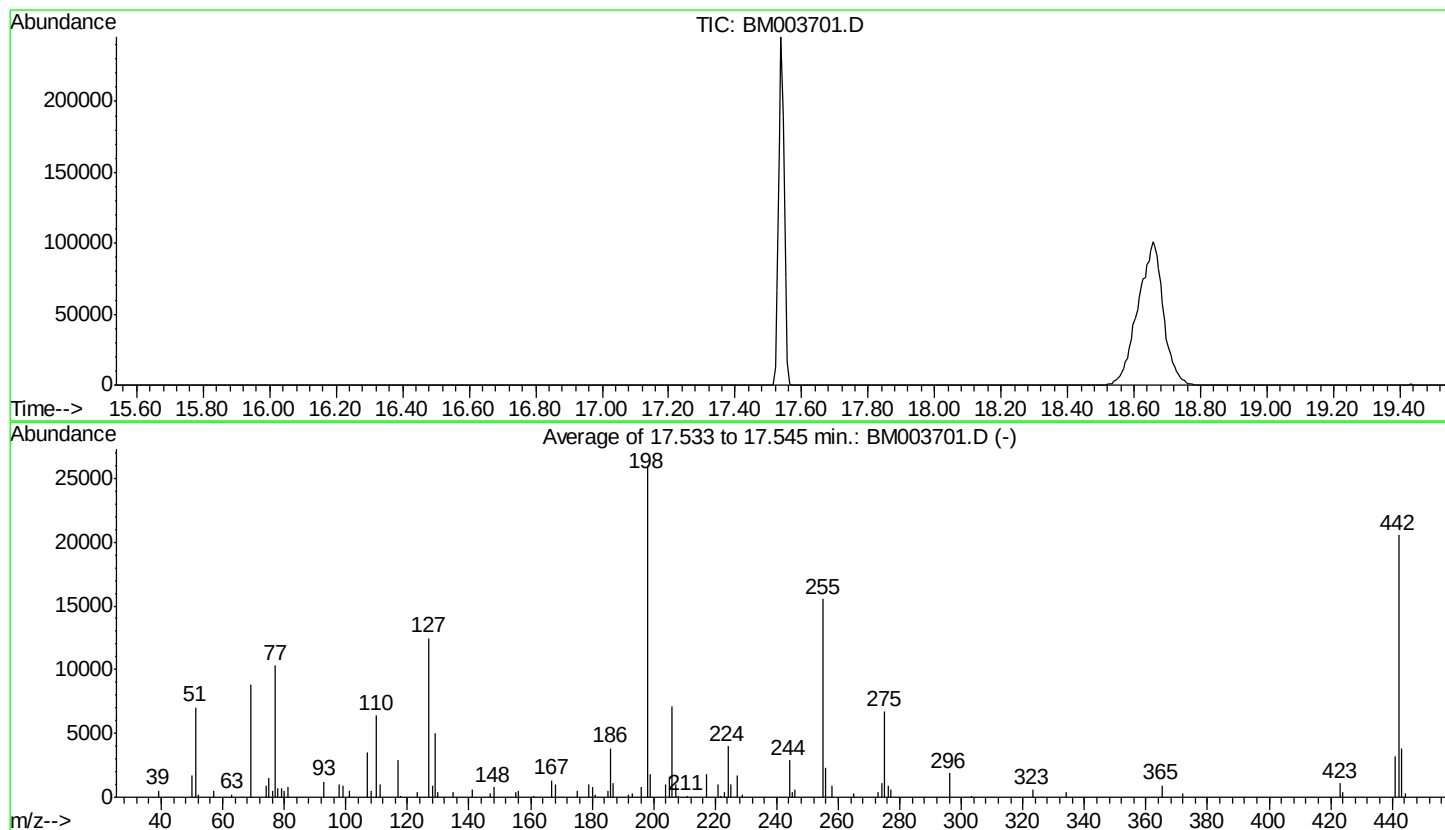

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	7029	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.0	8827	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	12442	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25989	PASS
199	198	5	9	6.9	1801	PASS
275	198	10	60	25.7	6692	PASS
365	198	1	100	3.5	916	PASS
441	443	0.01	100	83.7	3231	PASS
442	198	50	100	79.0	20525	PASS
443	442	15	24	18.8	3859	PASS

m/z

Abundance

Instrument :

BNA_M

ClientSampleId :

DFTPP63

m/z	Abundance
39.00	498.0
50.10	1677.0
51.10	7080.0
52.00	353.0
57.00	543.0
63.00	302.0
69.00	8572.0
74.00	960.0
75.00	1446.0
76.10	483.0
77.10	10265.0
78.00	725.0
79.00	705.0
80.00	467.0
81.00	786.0
93.00	1189.0
98.00	932.0
99.00	970.0
101.00	437.0
107.00	3150.0
108.00	530.0
110.00	5881.0
111.00	931.0
117.00	2766.0
123.00	353.0
127.00	11639.0
128.00	786.0
129.00	4640.0
130.00	362.0
135.00	378.0
141.00	596.0
147.00	359.0
148.00	658.0
155.00	375.0
156.00	503.0
167.00	1109.0
168.00	1035.0
175.10	410.0
179.00	822.0
180.00	674.0
185.00	443.0
186.00	3357.0
187.00	1015.0
193.10	324.0
196.00	647.0
198.00	22656.0
199.00	1591.0
204.00	844.0
205.00	1409.0
206.10	6083.0
207.10	859.0
217.00	1457.0
221.10	723.0
223.10	337.0
224.10	3173.0
225.10	800.0
227.00	1387.0
244.10	2394.0
245.00	338.0
246.00	482.0
255.10	12355.0
256.10	1834.0
258.00	779.0
273.00	330.0
274.10	850.0
275.10	5267.0
276.00	645.0
277.00	450.0
296.00	1339.0
323.10	468.0
334.10	315.0
365.00	588.0
423.10	745.0
424.10	337.0
441.10	2041.0
442.10	13815.0
443.10	2654.0

Instrument :
BNA_M
ClientSampleId :
DFTPP63

m/z	Abundance
39.00	683.0
50.10	2153.0
51.10	8369.0
52.00	405.0
57.00	632.0
63.00	416.0
69.00	10821.0
74.10	1102.0
75.00	1789.0
76.10	605.0
77.10	12353.0
78.10	907.0
79.00	862.0
80.00	690.0
81.00	921.0
93.00	1497.0
98.00	1191.0
99.00	1080.0
101.00	600.0
107.00	4220.0
108.00	626.0
110.00	7824.0
111.00	1173.0
117.00	3559.0
117.90	300.0
123.00	405.0
127.00	15260.0
128.00	1140.0
129.00	6008.0
130.00	600.0
135.00	509.0
141.00	746.0
147.00	412.0
148.00	918.0
155.00	476.0
156.00	674.0
161.00	368.0
167.00	1754.0
168.00	1174.0
175.00	633.0
179.00	1180.0
180.00	960.0
181.00	385.0
185.00	536.0
186.00	4627.0
187.00	1307.0
192.00	365.0
193.00	427.0
196.00	928.0
198.00	31216.0
199.00	2182.0
204.00	1126.0
205.10	2006.0
206.10	8749.0
207.10	1224.0
208.00	315.0
210.90	341.0
217.00	2212.0
221.00	1191.0
221.80	308.0
223.00	510.0
224.10	4934.0
225.00	1272.0
227.00	1965.0
229.00	385.0
244.10	3585.0
245.10	432.0
246.00	712.0
255.10	18584.0
256.00	2813.0
258.10	1128.0
265.00	444.0
273.00	527.0
274.00	1367.0
275.10	7979.0
276.10	1194.0
277.00	769.0
296.00	2344.0
303.10	307.0
323.10	668.0
334.10	526.0
365.10	1113.0
372.10	412.0
423.10	1305.0
424.10	472.0
441.10	3726.0
442.20	23512.0
443.20	4618.0
444.10	451.0

Instrument :
BNA_M
ClientSampleId :
DFTPP63

m/z	Abundance
39.00	405.0
50.00	1370.0
51.10	5638.0
57.00	430.0
69.00	7088.0
74.10	702.0
75.00	1149.0
76.10	391.0
77.10	8351.0
78.00	595.0
79.00	637.0
80.00	356.0
81.00	623.0
93.00	1031.0
98.00	753.0
98.90	626.0
101.00	389.0
107.00	3119.0
108.00	462.0
110.00	5417.0
111.00	767.0
117.00	2498.0
123.00	336.0
127.00	10428.0
128.00	785.0
129.00	4453.0
130.00	346.0
135.00	344.0
140.90	613.0
148.00	716.0
155.00	309.0
156.00	480.0
167.00	1173.0
168.00	769.0
175.00	505.0
179.00	885.0
180.00	671.0
181.00	322.0
185.00	457.0
186.10	3486.0
187.00	939.0
191.90	384.0
193.00	306.0
196.00	721.0
198.00	24096.0
199.00	1632.0
204.00	913.0
205.10	1537.0
206.10	6565.0
207.10	976.0
217.00	1748.0
221.00	981.0
223.00	404.0
224.10	3800.0
225.00	997.0
227.00	1743.0
228.90	352.0
244.10	2748.0
245.10	318.0
246.10	675.0
255.10	15656.0
256.10	2384.0
258.00	883.0
265.00	422.0
273.00	446.0
274.10	1176.0
275.10	6831.0
276.00	936.0
277.00	646.0
296.00	1976.0
323.10	568.0
334.00	425.0
365.10	1047.0
372.10	355.0
423.10	1243.0
424.10	390.0
441.10	3926.0
442.10	24248.0
443.10	4307.0
444.10	330.0

Instrument :
BNA_M
ClientSampleId :
DFTPP63