

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
Data File : BM008565.D
Acq On : 22 Dec 2016 20:50
Operator : UM/SJ
Sample : H5938-11DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:24:51 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:50:04 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DA831DL

Manual Integrations
APPROVED

umangi
12/23/2016 6:11:37 PM

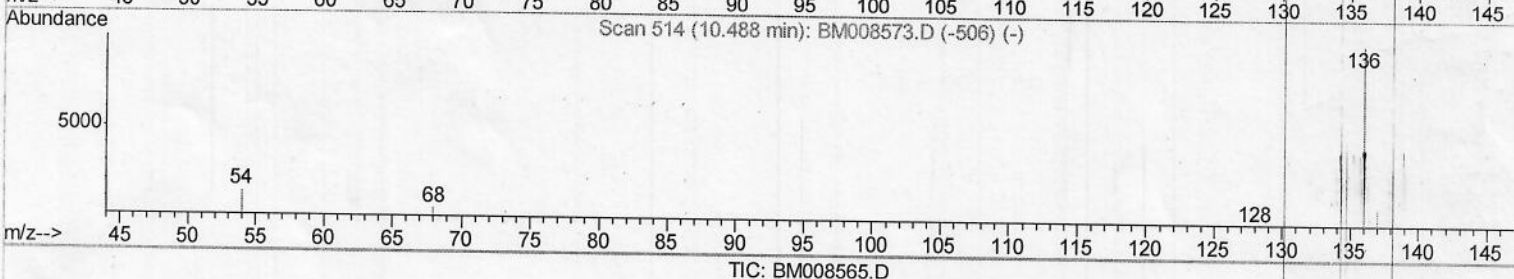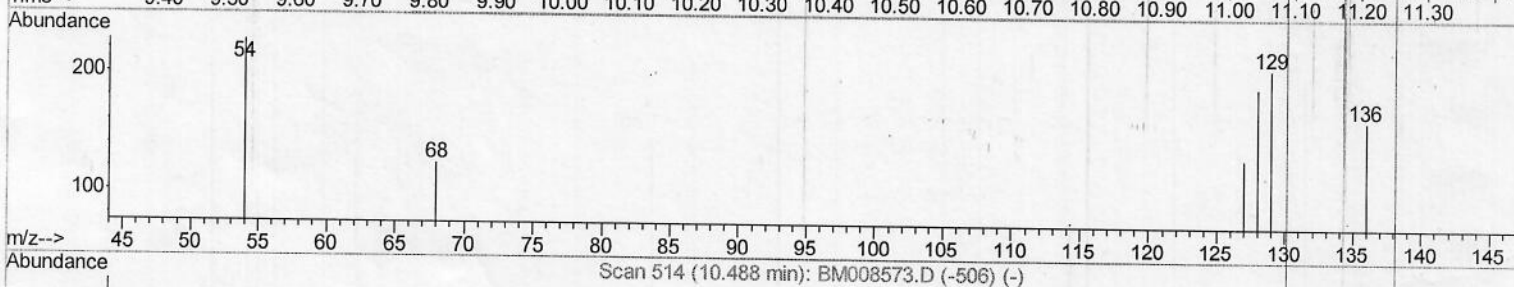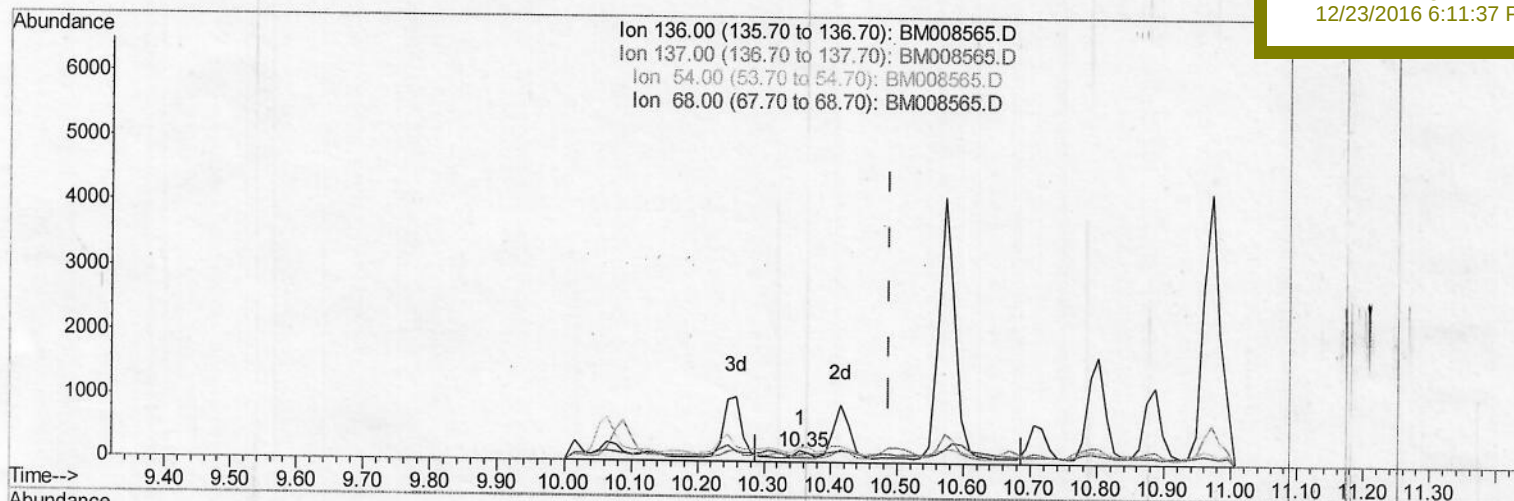

(2) Naphthalene-d8 (I)

10.355min (-0.133) 0.40ng/ul

response 177

Ion	Exp%	Act%
136.00	100	100
137.00	13.90	45.12#
54.00	15.50	138.41#
68.00	9.90	75.61#

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
Data File : BM008565.D
Acq On : 22 Dec 2016 20:50
Operator : UM/SJ
Sample : H5938-11DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:24:51 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:50:04 2016
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DA831DL

Manual Integrations

APPROVED

umangi

12/23/2016 6:11:37 PM

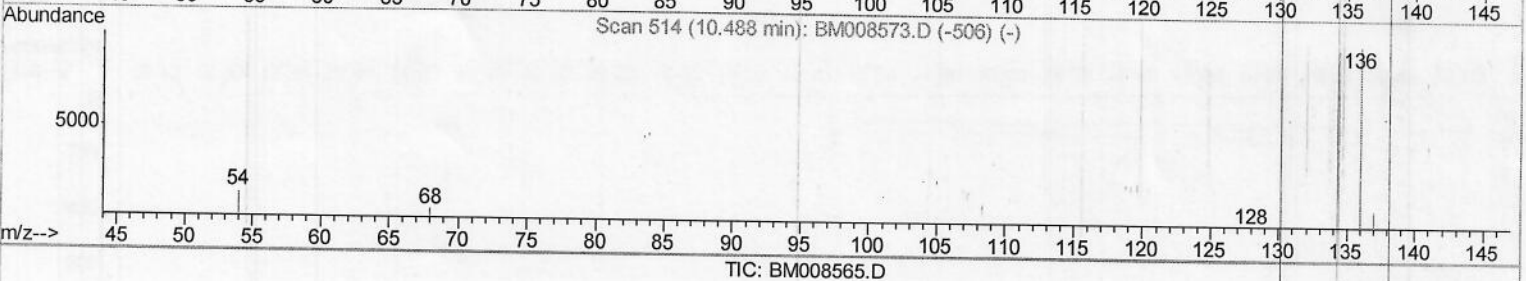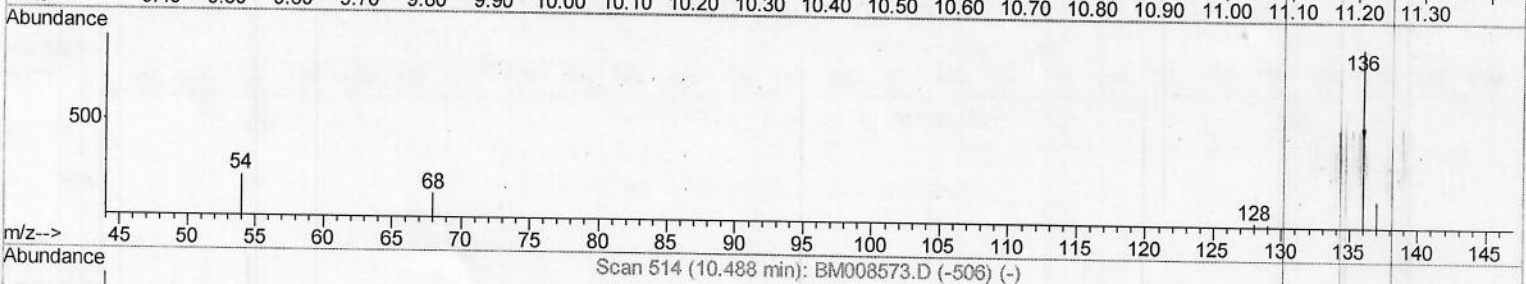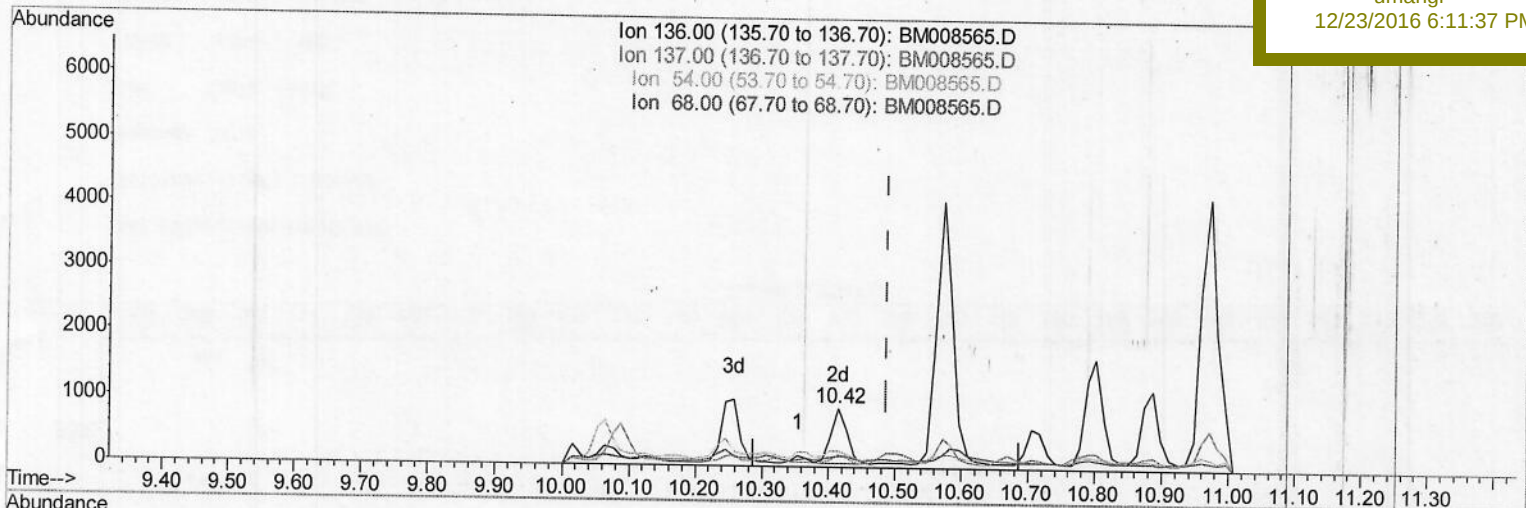

(2) Naphthalene-d8 (I)

10.415min (-0.073) 0.40ng/ul m

response 1454

Ion	Exp%	Act%
136.00	100	100
137.00	13.90	20.58#
54.00	15.50	27.36#
68.00	9.90	18.69#

S.J
12/23/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:25:22 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 Client Sampled :
 DA831DL

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

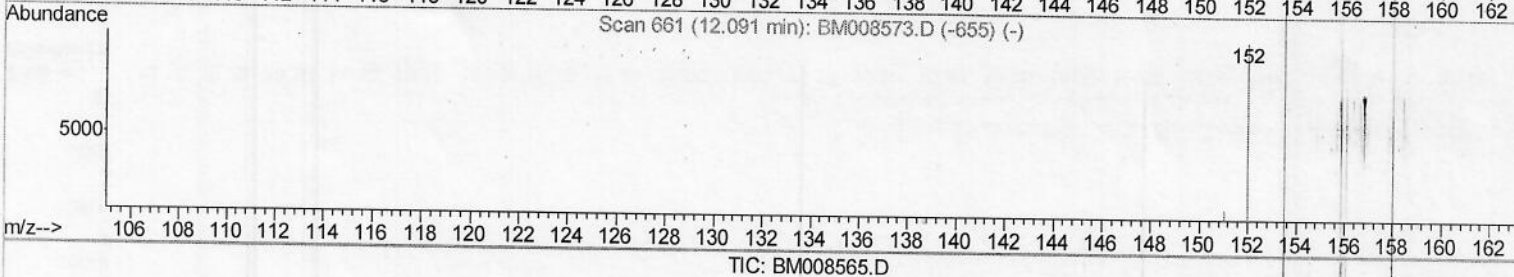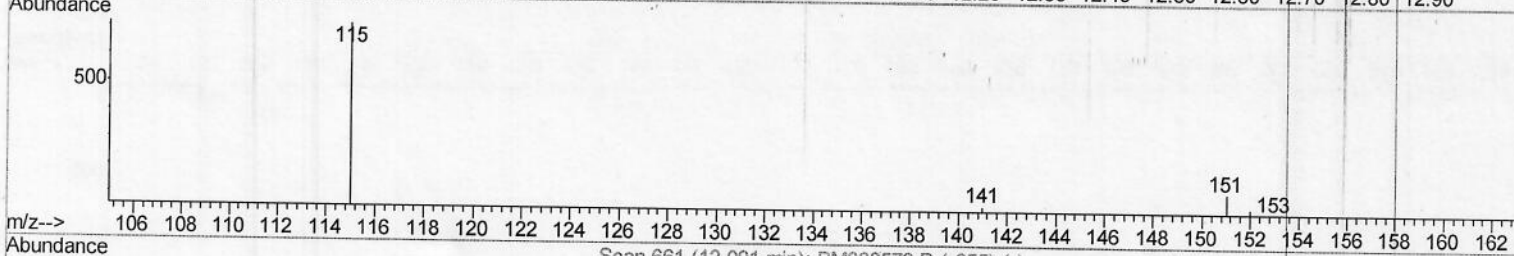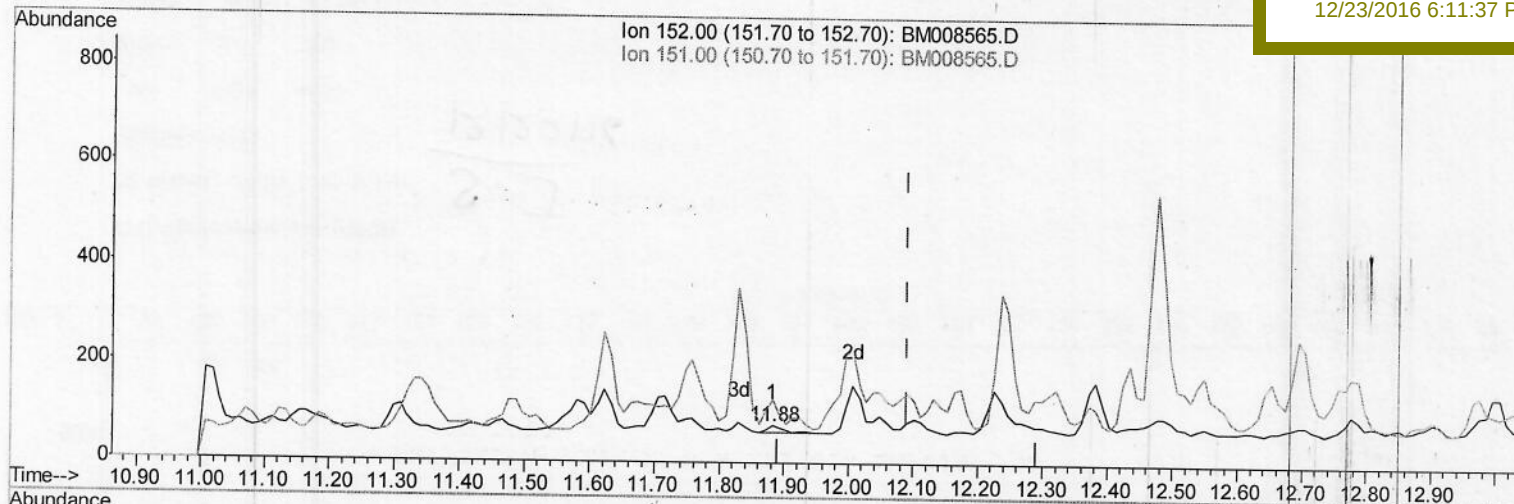

(4) 2-Methylnaphthalene-d10 (SURR)

11.882min (-0.208) 0.01ng/ul

response 32

Ion	Exp%	Act%
152.00	100	100
151.00	19.30	362.50#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:25:22 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA831DL

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

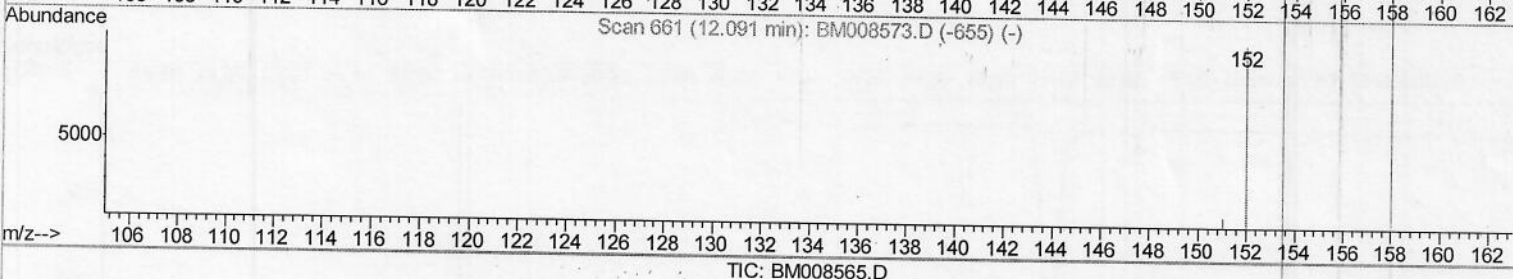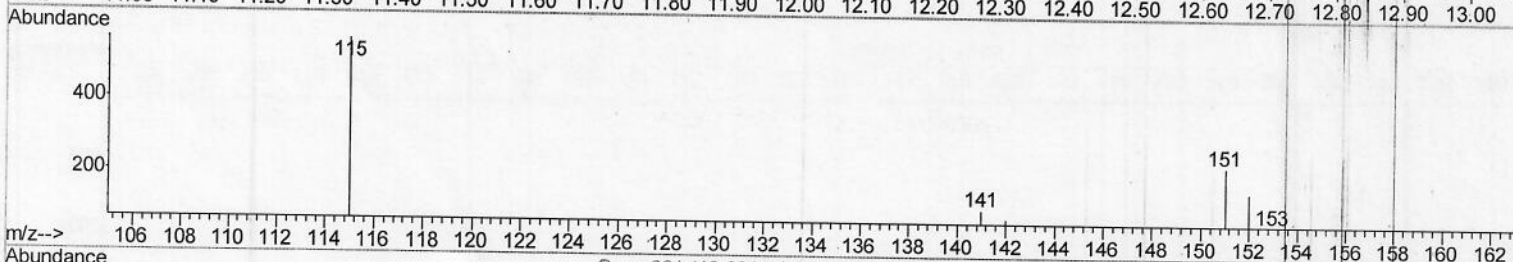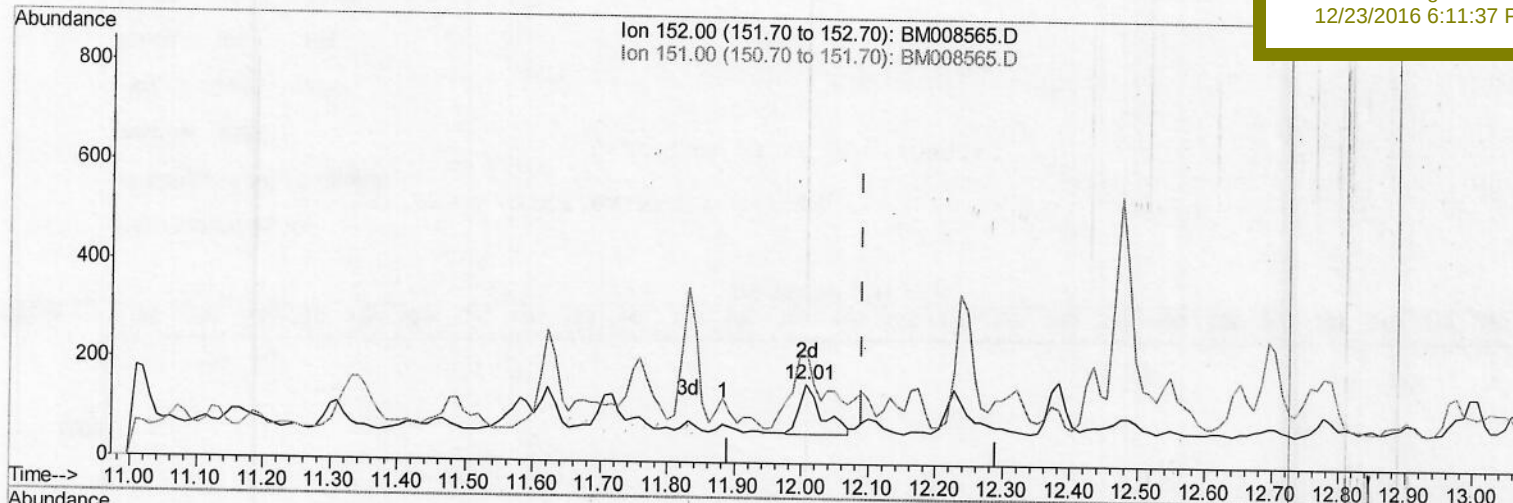

(4) 2-Methylnaphthalene-d10 (SURR)

12.007min (-0.083) 0.10ng/ul m

response 230

Ion	Exp%	Act%
152.00	100	100
151.00	19.30	50.43#
0.00	0.00	0.00
0.00	0.00	0.00

SJ
 12/23/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:25:22 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA831DL

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

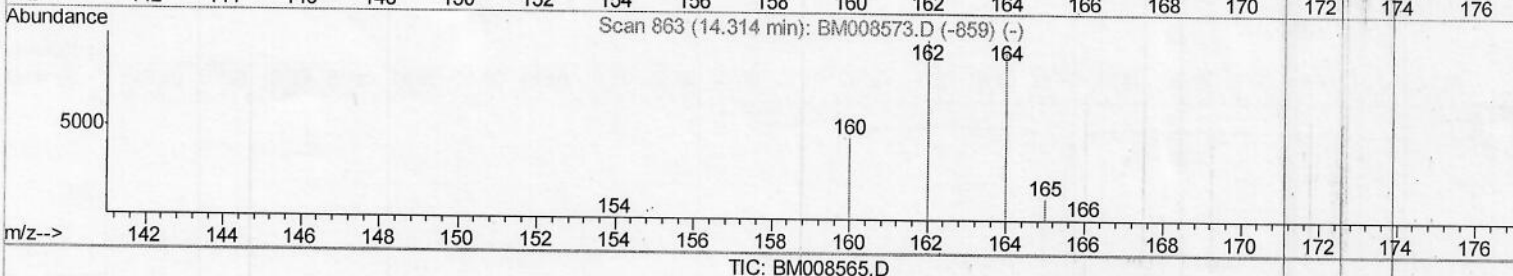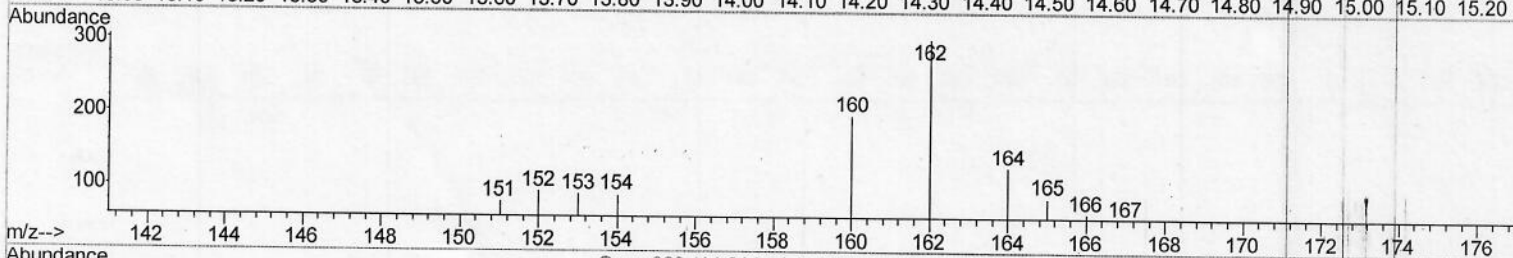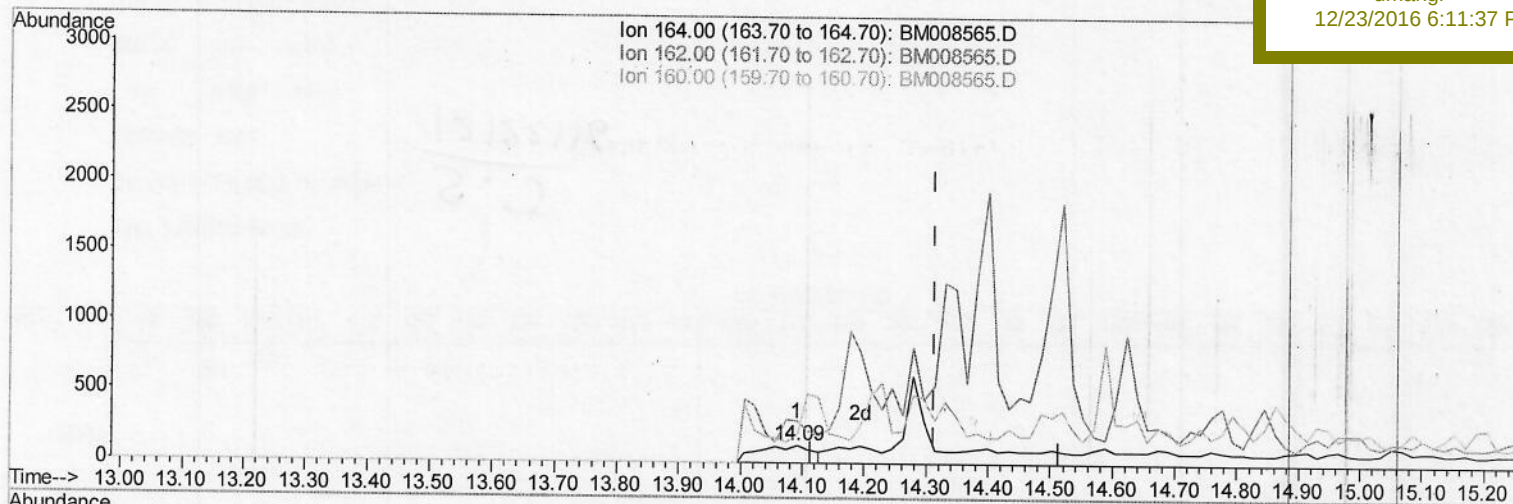

(6) Acenaphthene-d10 (I)

14.091min (-0.223) 0.40ng/ul

response 718

Ion	Exp%	Act%
164.00	100	100
162.00	98.60	237.50#
160.00	48.80	155.47#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
Data File : BM008565.D
Acq On : 22 Dec 2016 20:50
Operator : UM/SJ
Sample : H5938-11DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:25:22 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:50:04 2016
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DA831DL

Manual Integrations

APPROVED

umangi

12/23/2016 6:11:37 PM

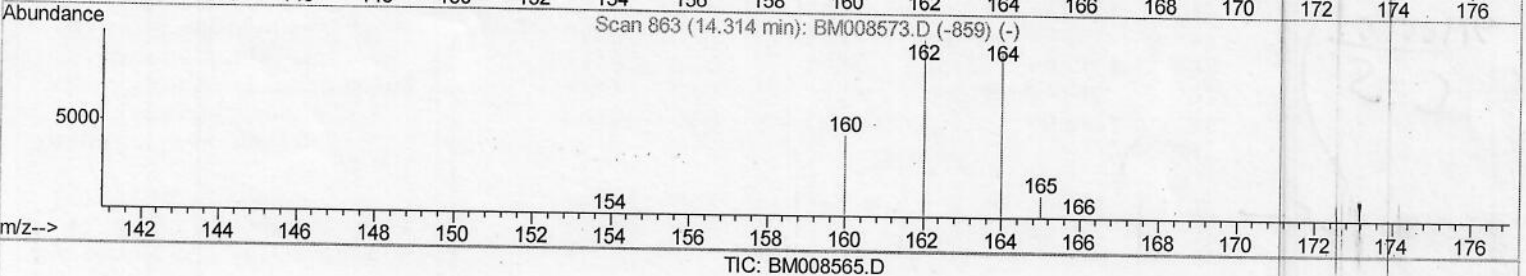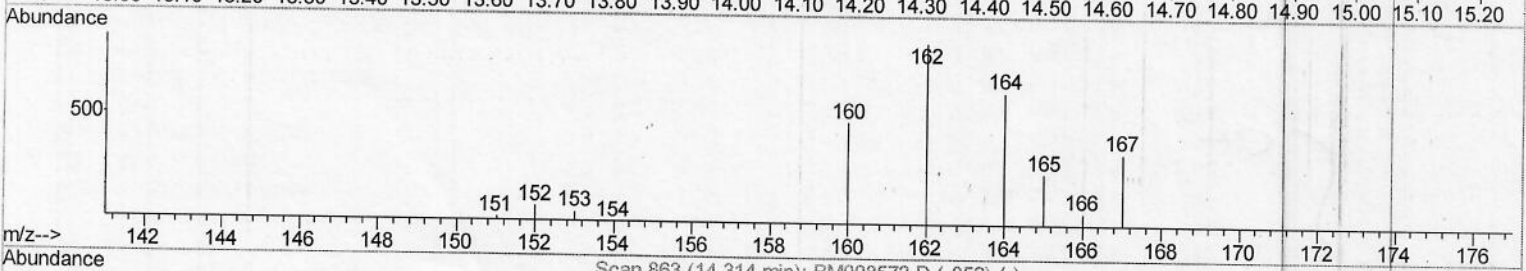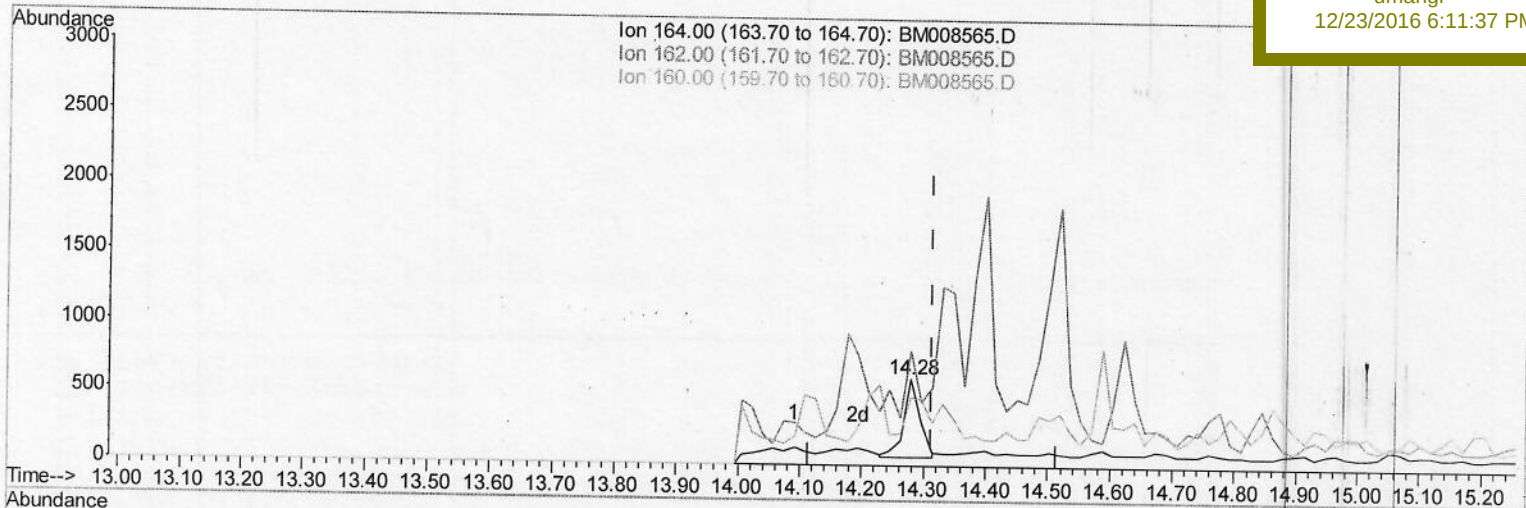

TIC: BM008565.D

(6) Acenaphthene-d10 (I)

14.280min (-0.034) 0.40ng/ul m

response 993

Ion	Exp%	Act%
164.00	100	100
162.00	98.60	133.17#
160.00	48.80	79.13#
0.00	0.00	0.00

S.J
12/23/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:28:02 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 Client Sampled :
 DA831DL

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

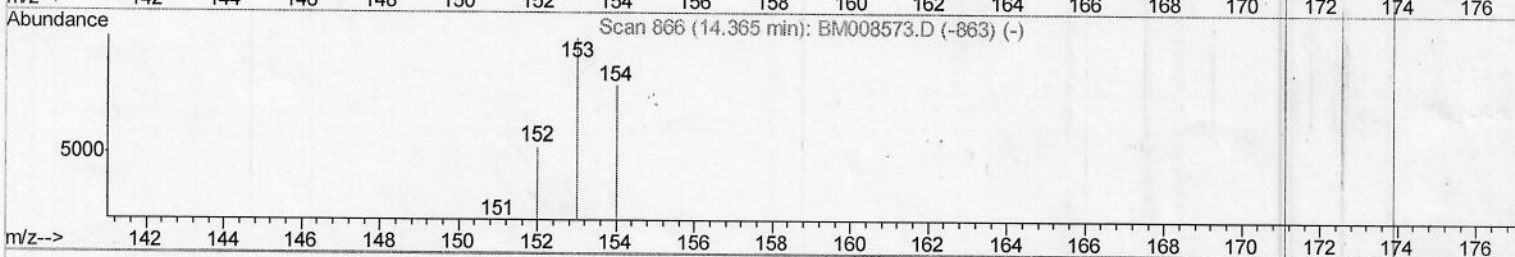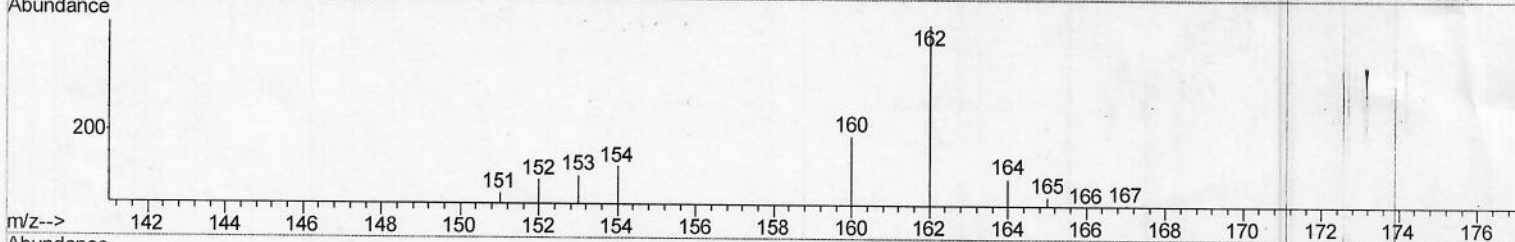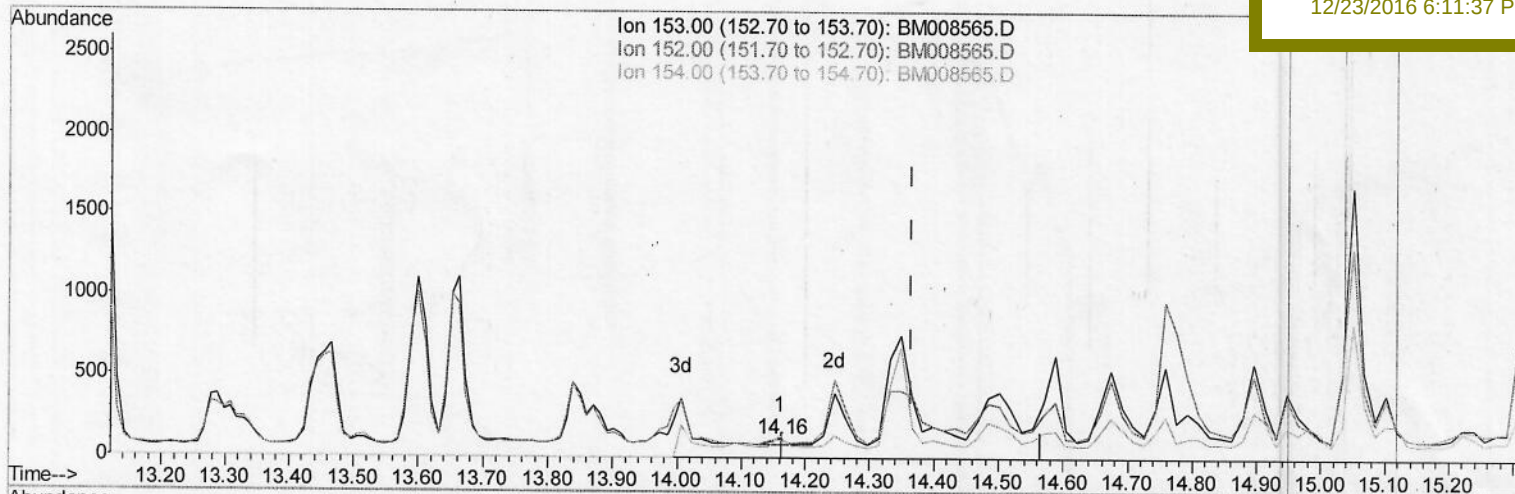

TIC: BM008565.D

(8) Acenaphthene (C)

14.160min (-0.206) 0.02ng/ul

response 77

Ion	Exp%	Act%
153.00	100	100
152.00	50.40	93.33#
154.00	89.30	114.17#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:28:02 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA831DL

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

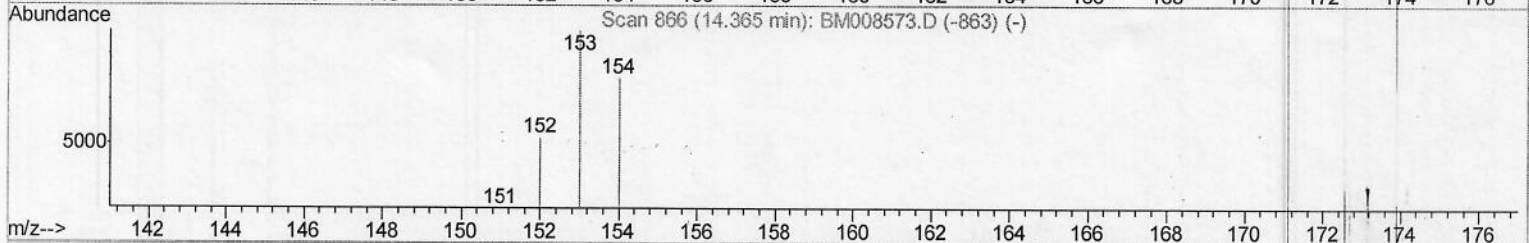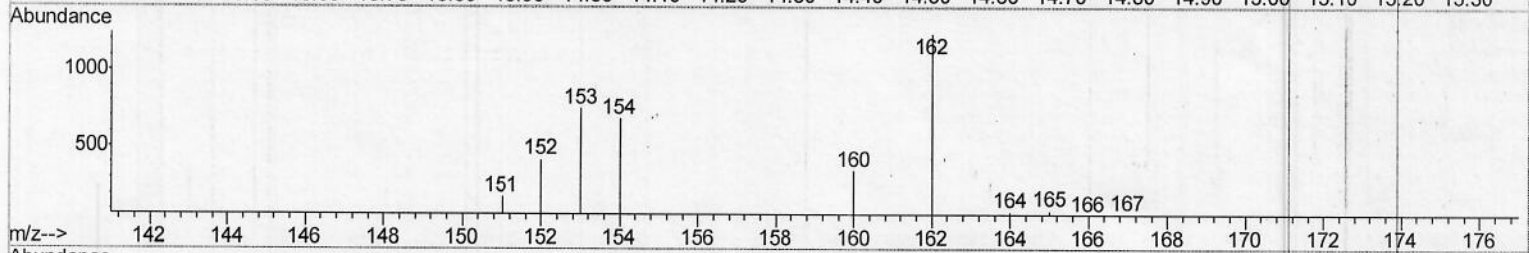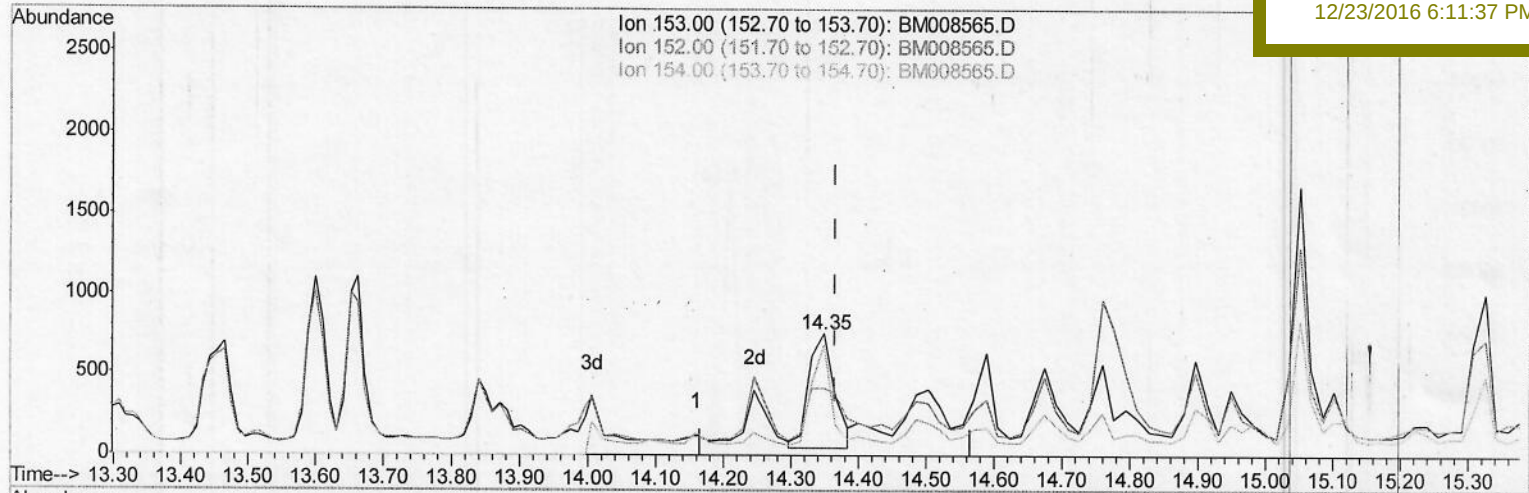

TIC: BM008565.D

(8) Acenaphthene (C)

14.348min (-0.017) 0.54ng/ul m

response 1818

Ion	Exp%	Act%
153.00	100	100
152.00	50.40	55.26
154.00	89.30	90.95
0.00	0.00	0.00

S.J
 12/23/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:28:02 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampled :
 DA831DL

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

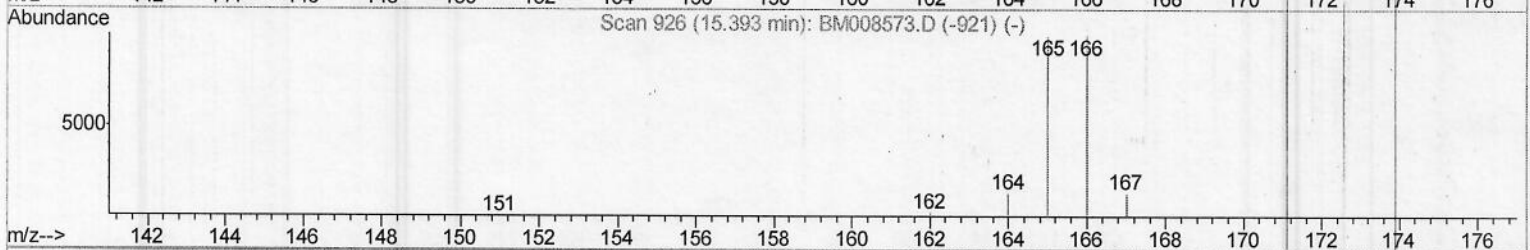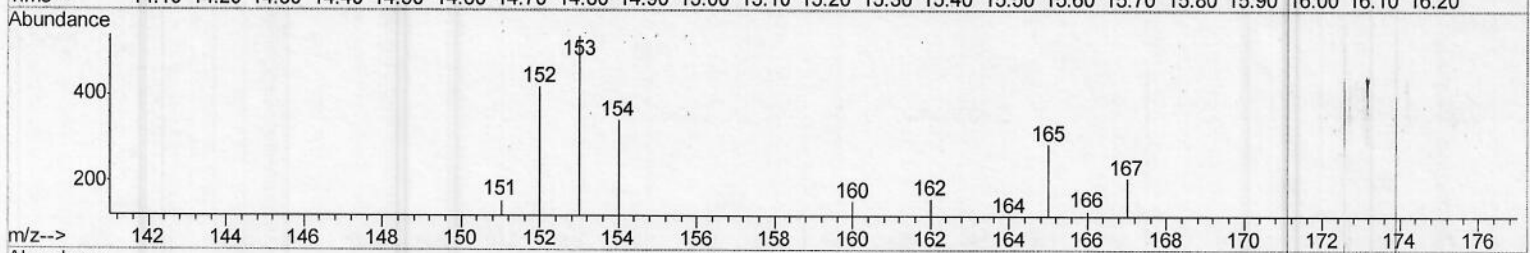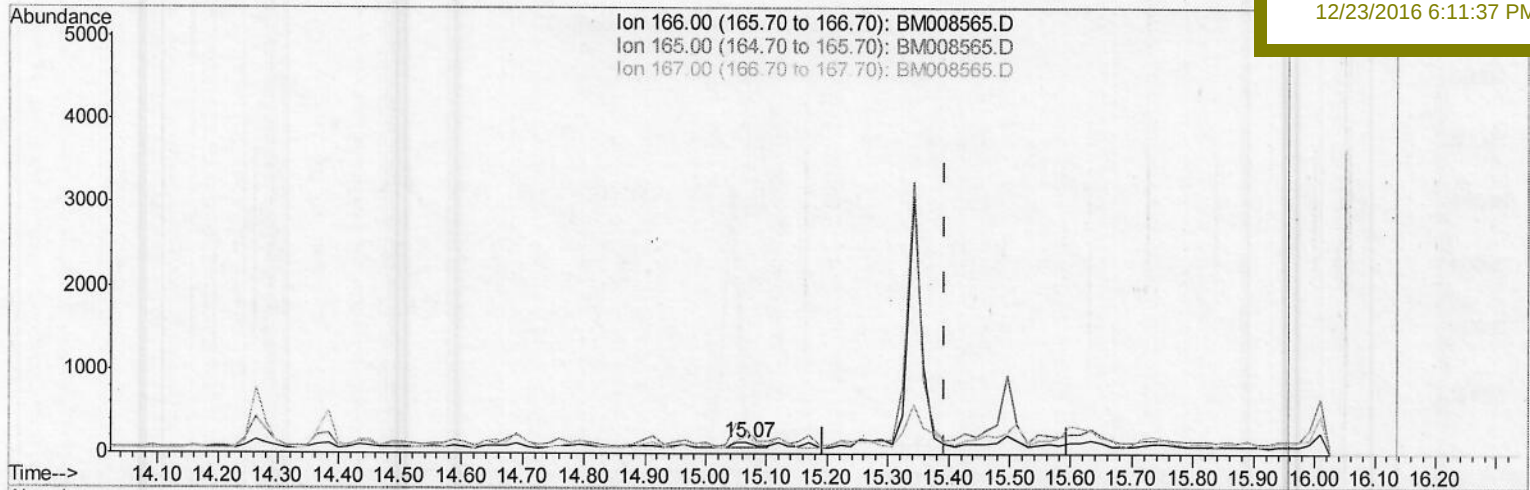

TIC: BM008565.D

(9) Fluorene

15.068min (-0.325) 0.04ng/ul

response 144

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	214.93#
167.00	18.30	155.97#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:28:02 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5" POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 Client Sampled :
 DA831DL

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

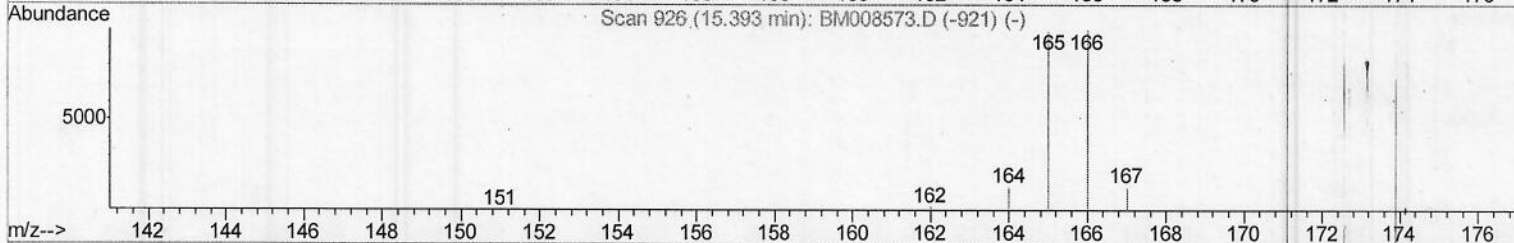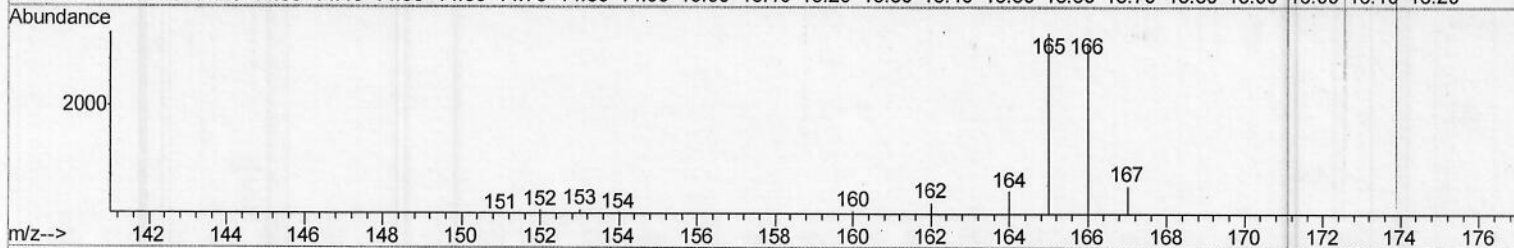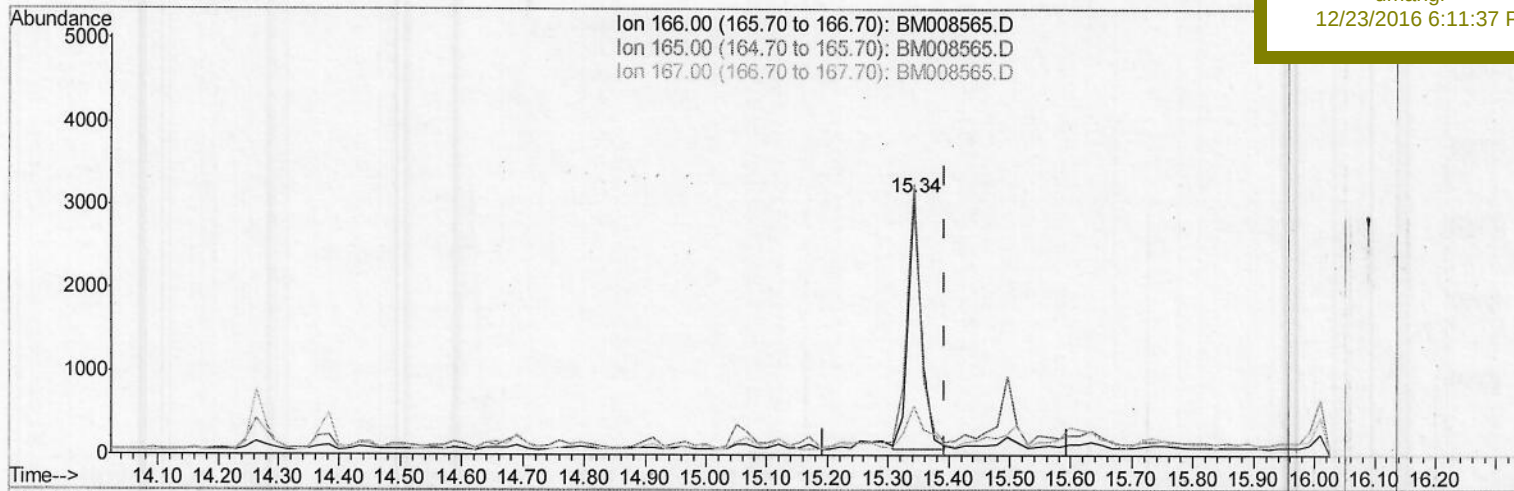

TIC: BM008565.D

(9) Fluorene

15.342min (-0.051) 1.21ng/ul m

response 4683

S.J.
12/23/2016

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	105.01
167.00	18.30	19.30
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:28:02 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA831DL

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

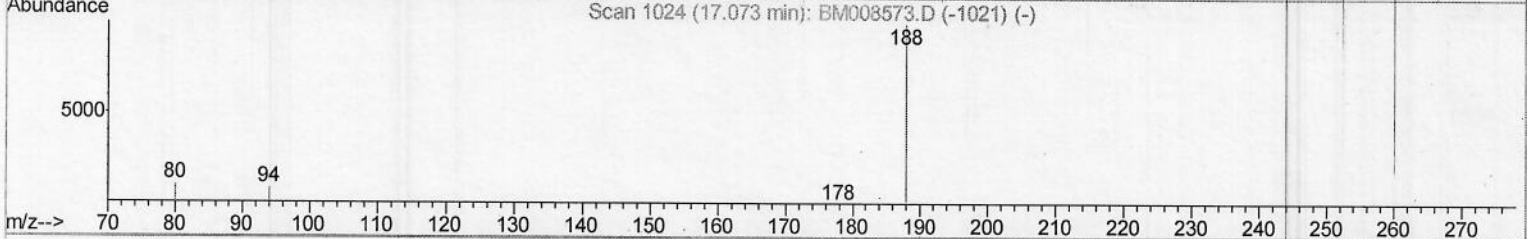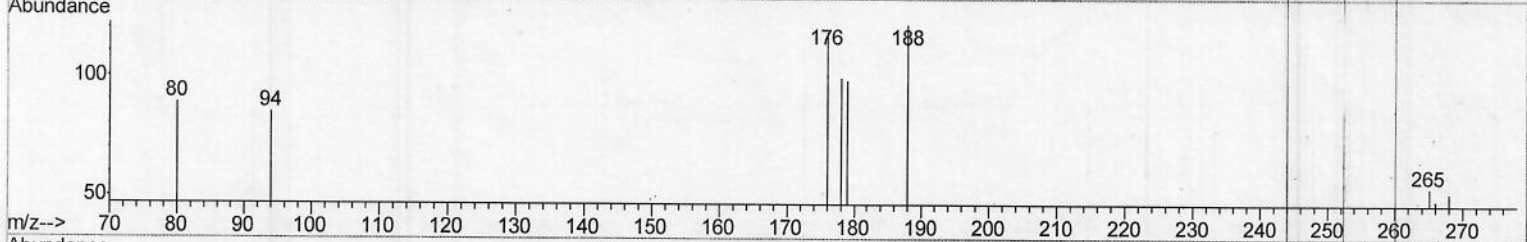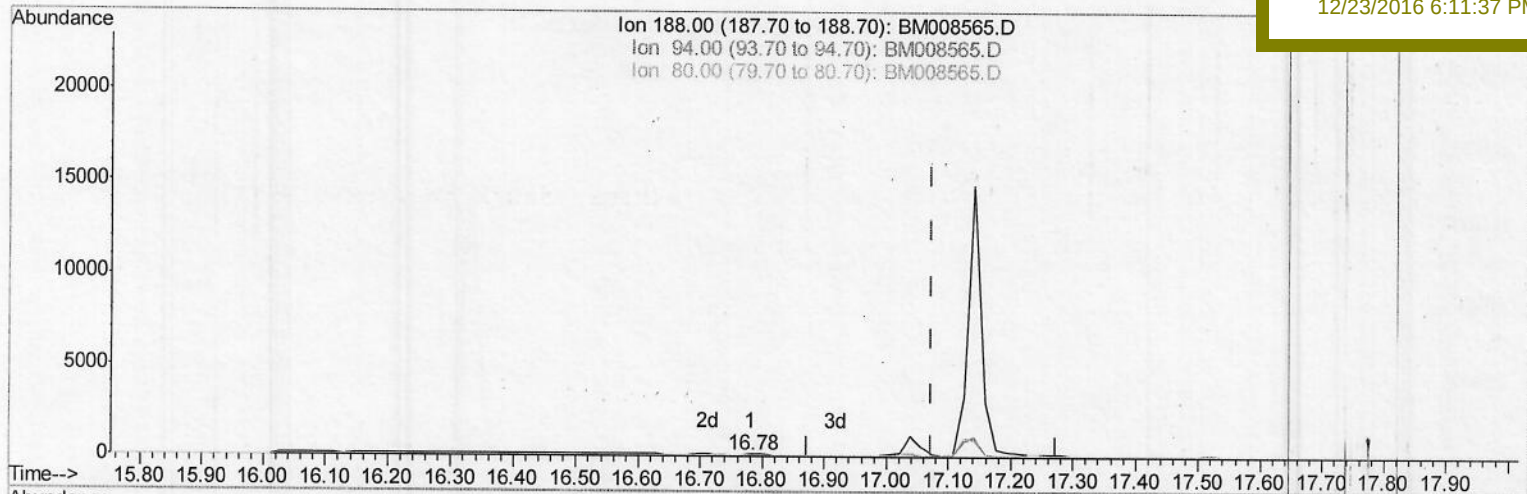

(10) Phenanthrene-d10 (I)
 16.781min (-0.292) 0.40ng/ul
 response 64

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	69.67#
80.00	11.80	72.95#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:28:02 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :

BNA_M

Client Sample ID :




DA831DL

Manual Integrations

APPROVED

umangi

12/23/2016 6:11:37 PM

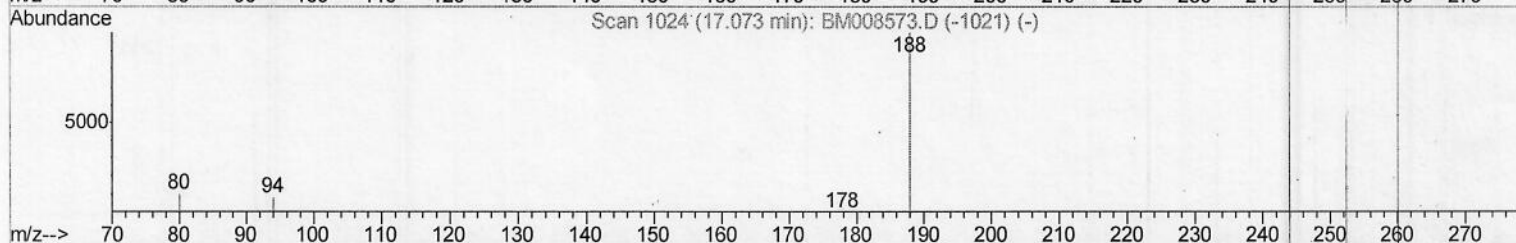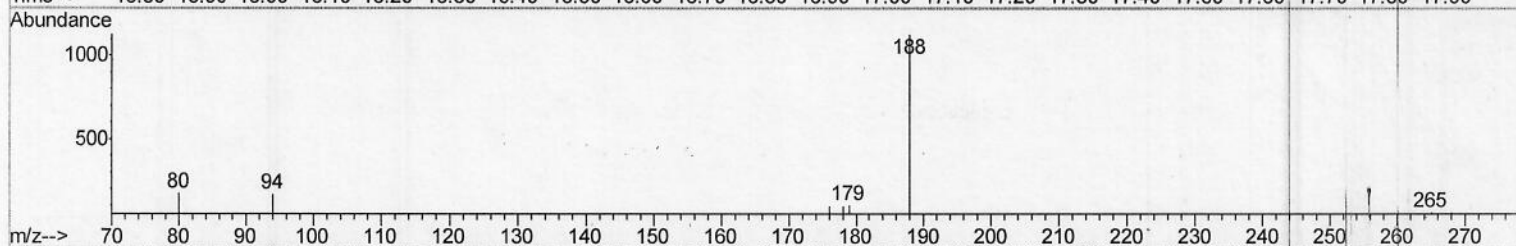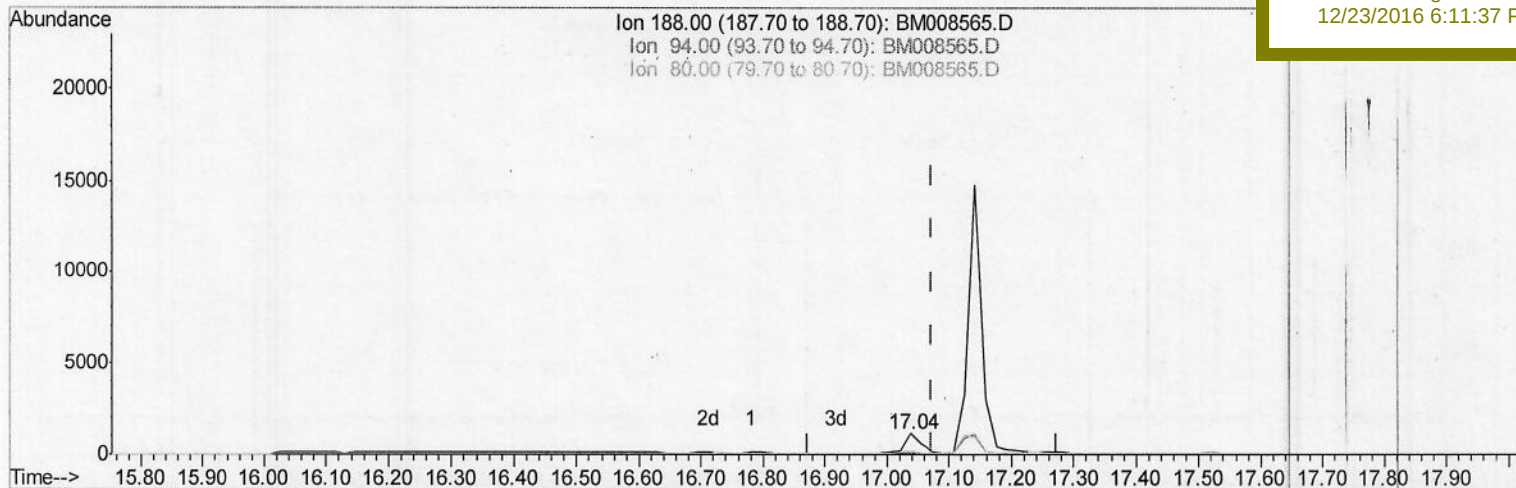

TIC: BM008565.D

(10) Phenanthrene-d10 (I)

17.039min (-0.034) 0.40ng/ul m

response 1745

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	14.74#
80.00	11.80	15.45#
0.00	0.00	0.00

S.J
 12/23/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:30:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA831DL

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

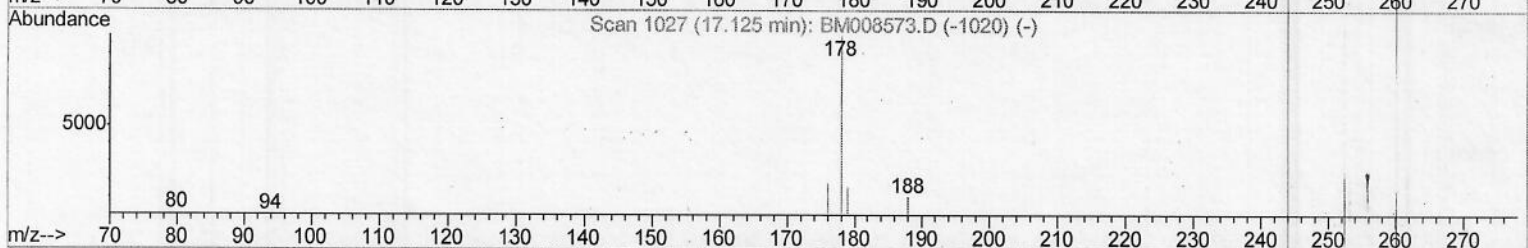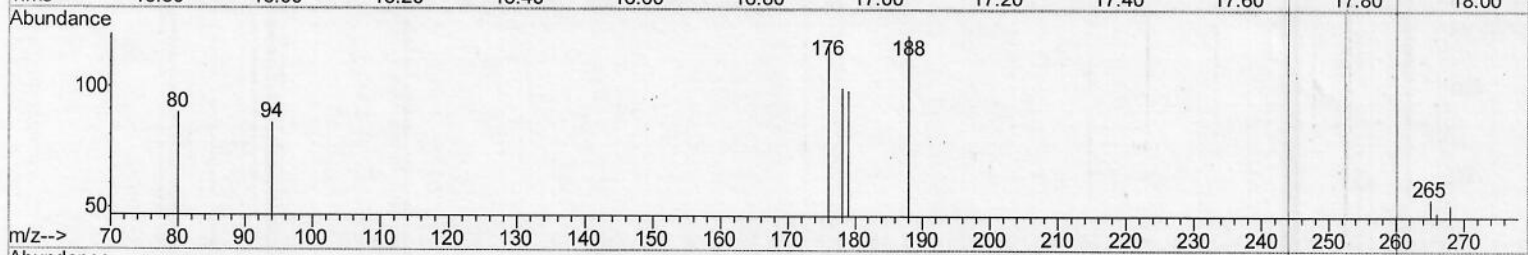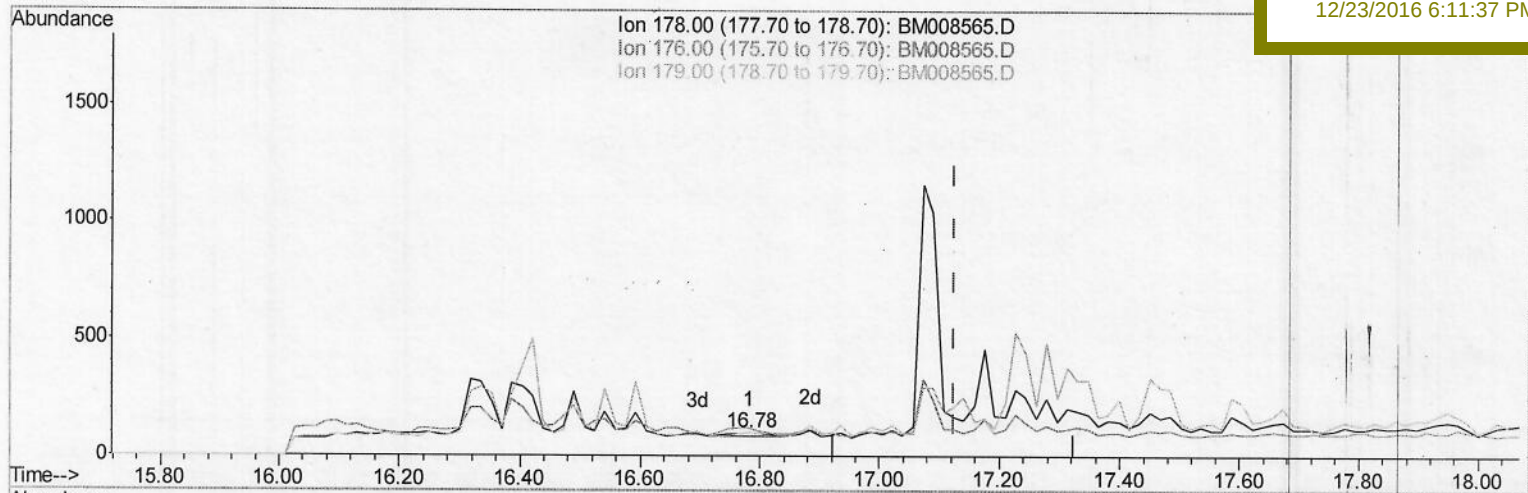

TIC: BM008565.D

(12) Phenanthrene

16.781min (-0.343) 0.01ng/ul

response 59

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	119.00#
179.00	17.00	99.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:30:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
ClientSampleId :
 DA831DL

Manual Integrations
APPROVED

umangi
 12/23/2016 6:11:37 PM

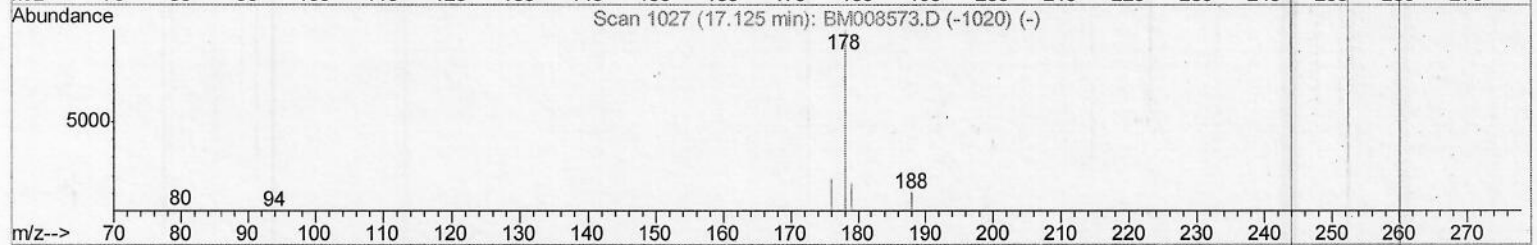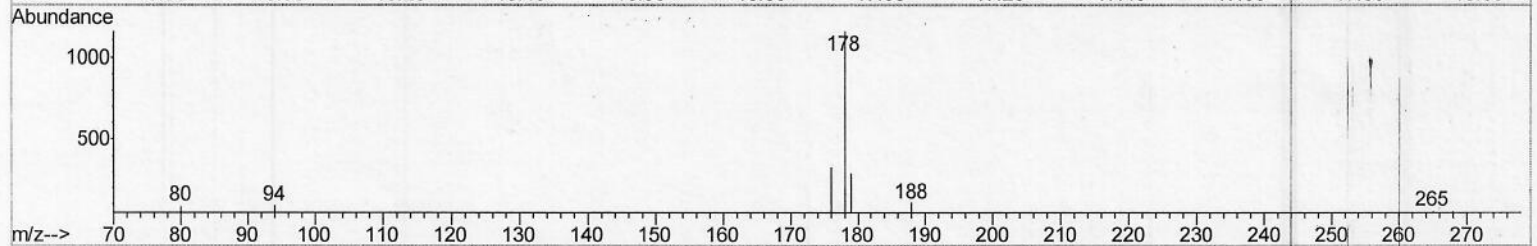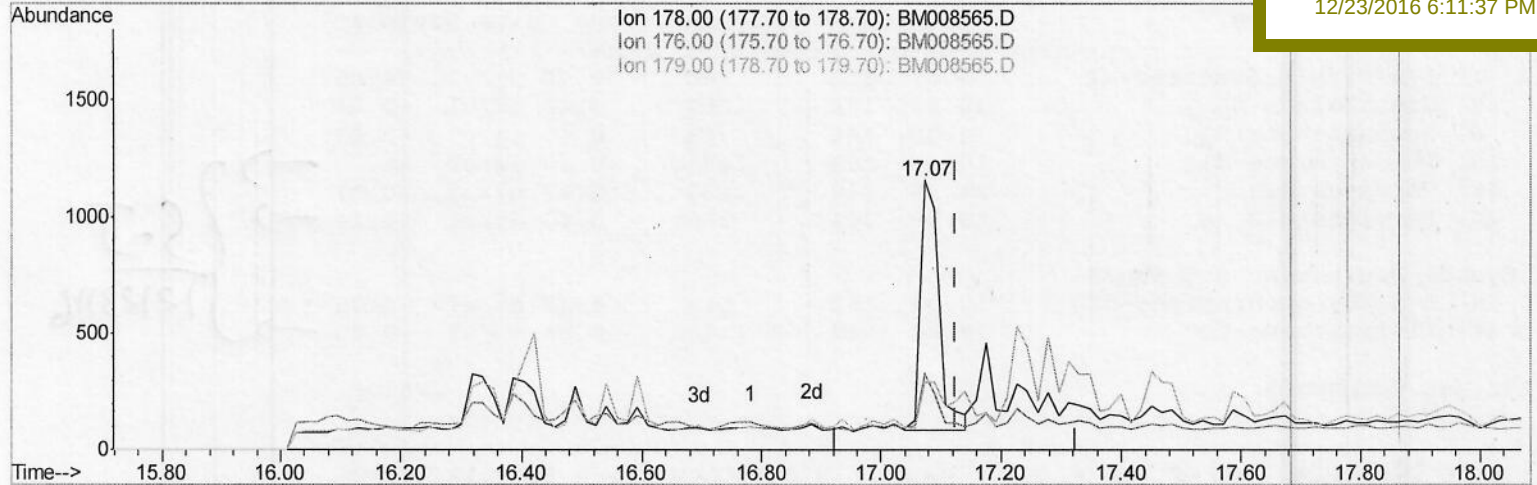

TIC: BM008565.D

(12) Phenanthrene

17.073min (-0.052) 0.45ng/ul m

response 2387

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	28.55#
179.00	17.00	25.26#
0.00	0.00	0.00

S.J
12/23/2016

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:30:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DA831DL

Manual Integrations

APPROVED

umangi

12/23/2016 6:11:37 PM

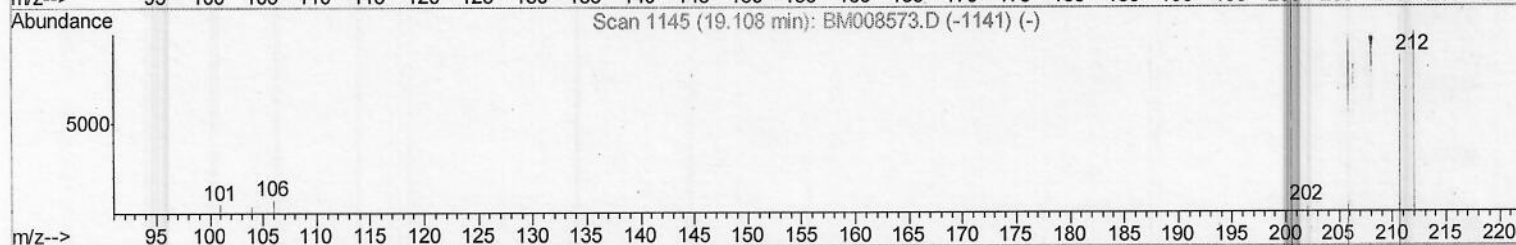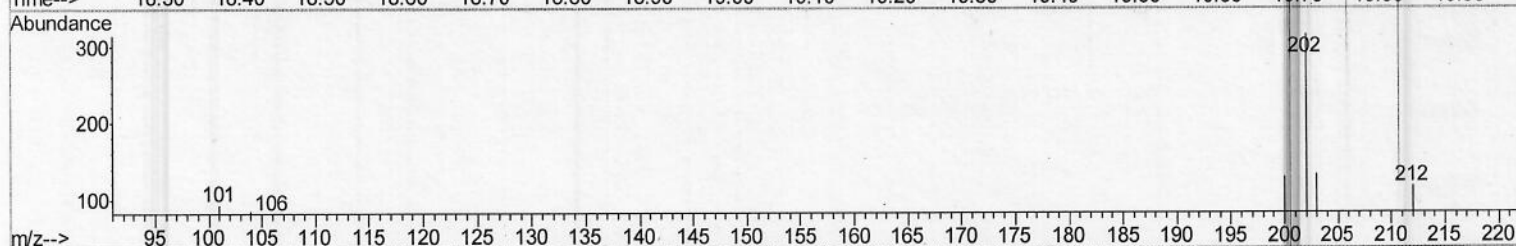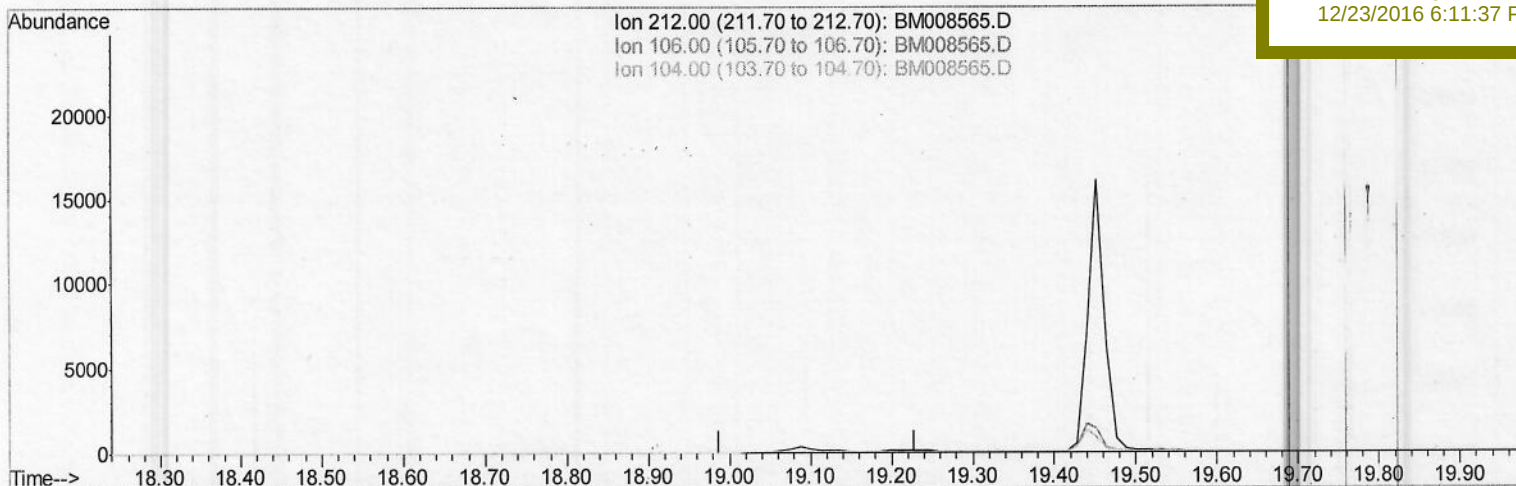

TIC: BM008565.D

(14) Fluoranthene-d10 (SURR)

19.108min (-19.108) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA831DL

Quant Time: Dec 23 10:30:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

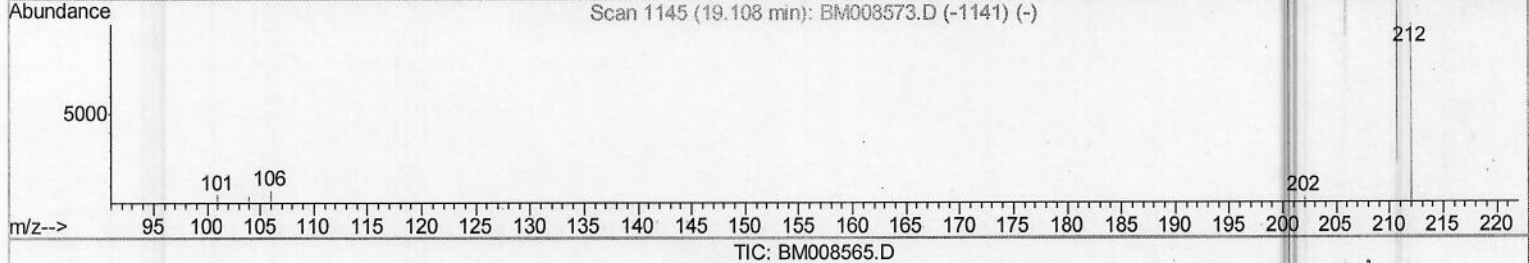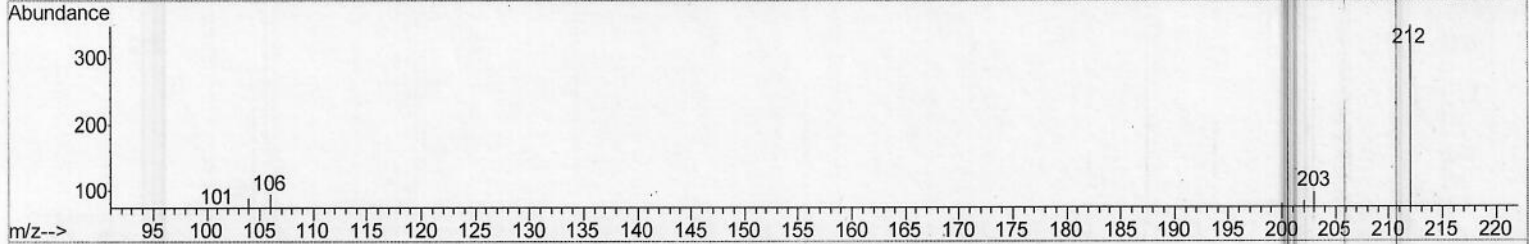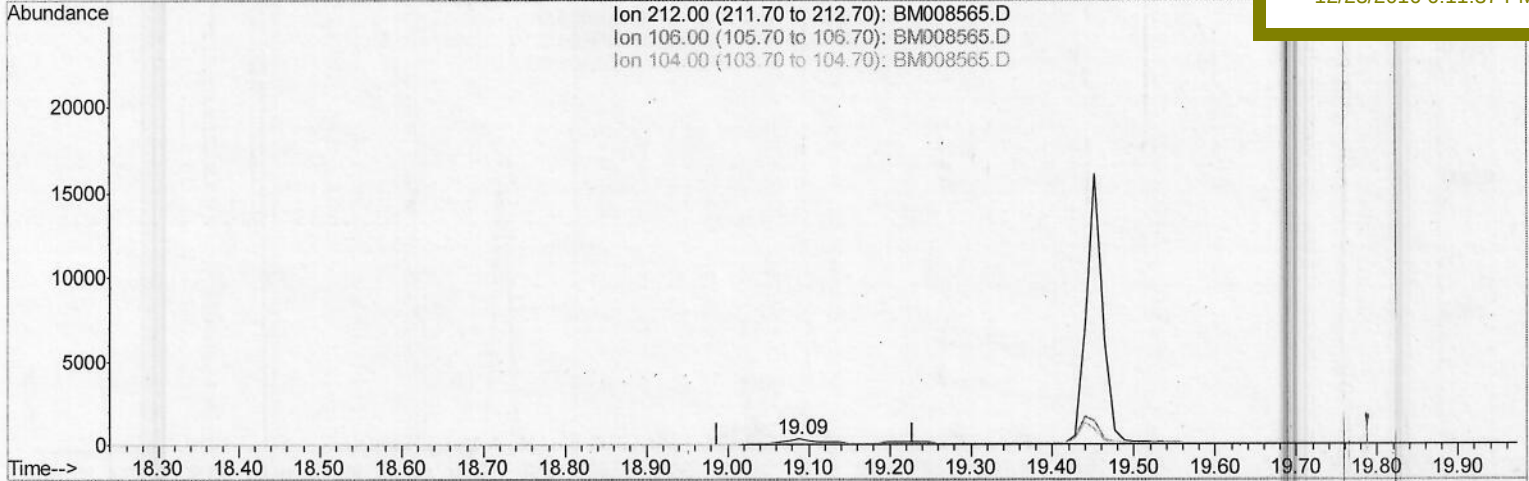

(14) Fluoranthene-d10 (SURR)

19.089min (-0.019) 0.08ng/ul m

response 390

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

SJ
 12/23/2016

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:30:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :

BNA_M




Client Sampled :

DA831DL

Manual Integrations
 APPROVED

umangi

12/23/2016 6:11:37 PM

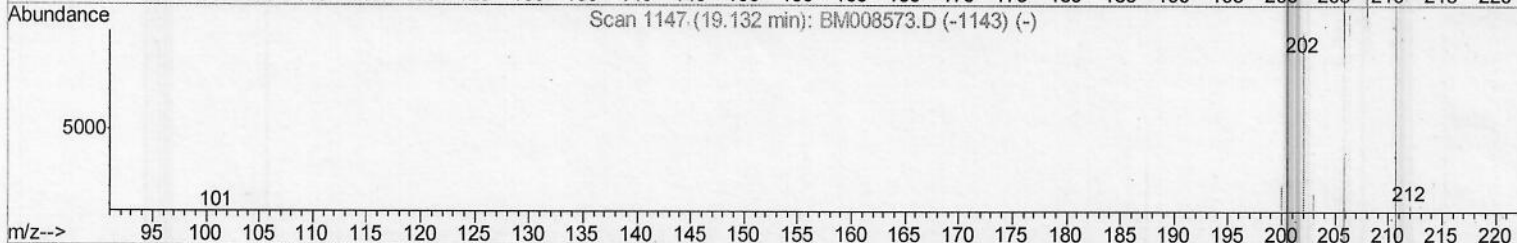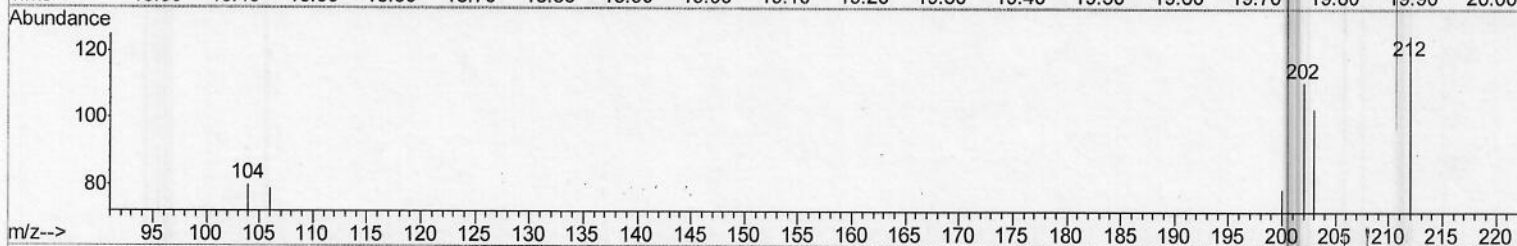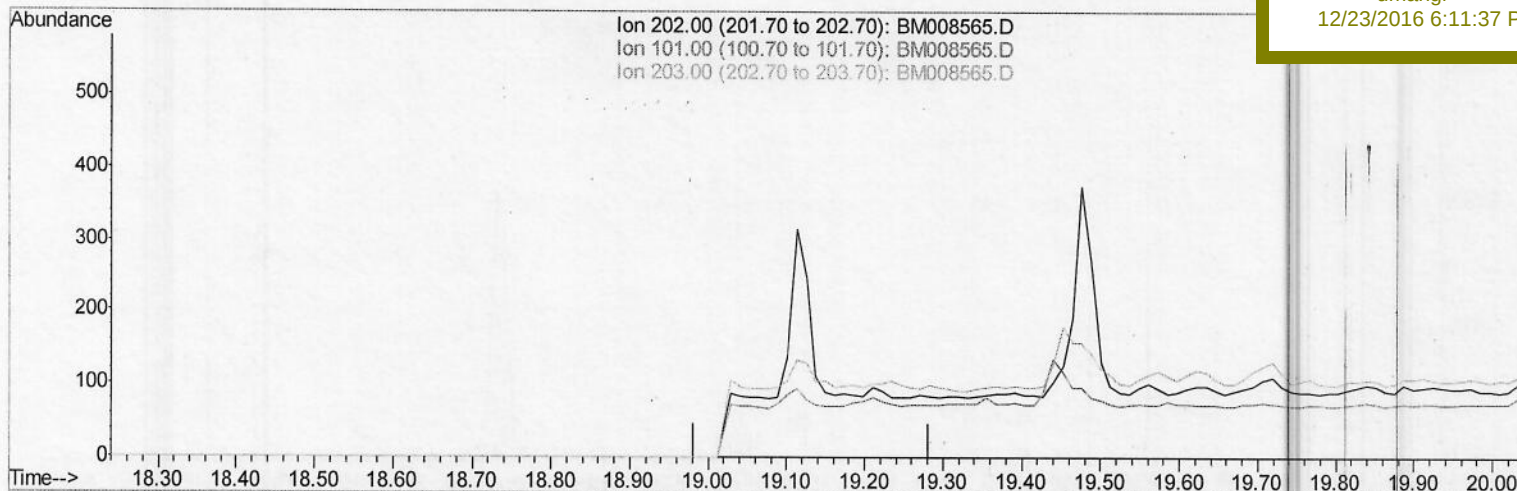

TIC: BM008565.D

(15) Fluoranthene (C)

19.132min (-19.132) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	10.30	0.00
203.00	19.50	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:30:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA831DL

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

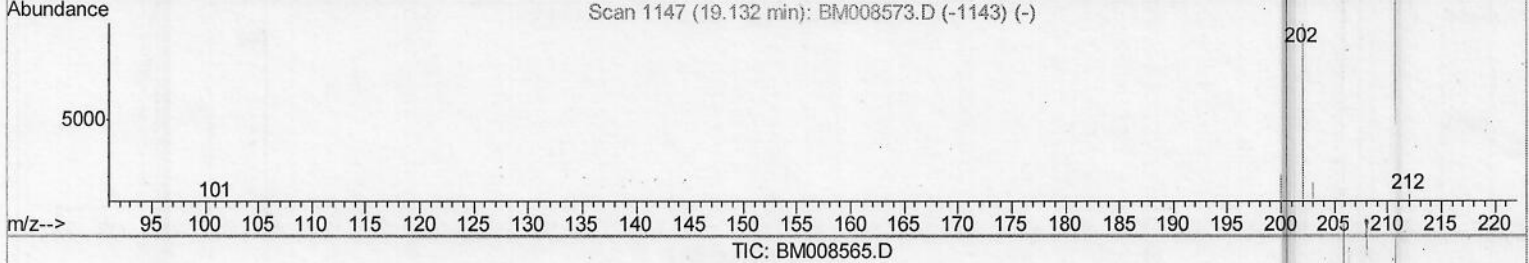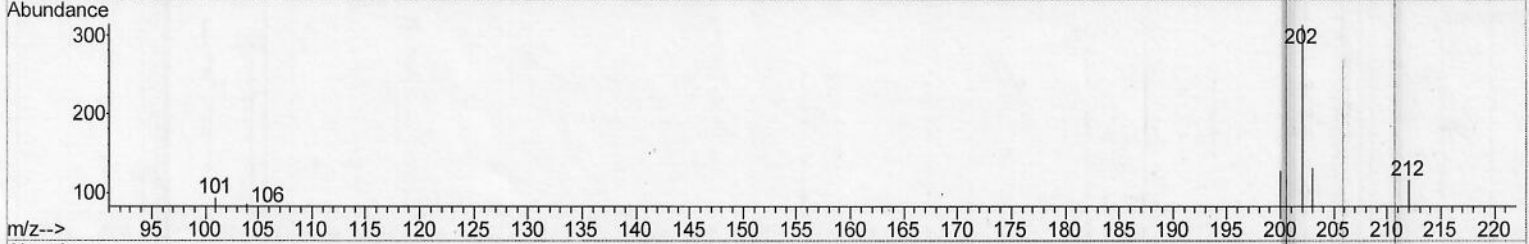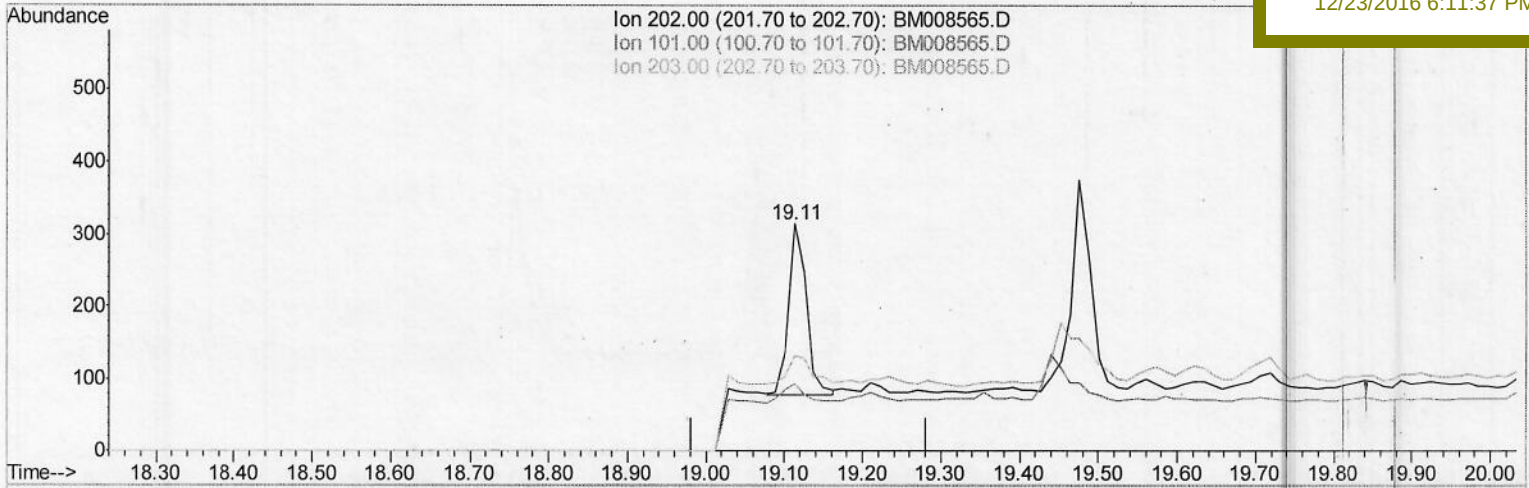

(15) Fluoranthene (C)

19.113min (-0.019) 0.06ng/ul m

response 375

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	29.62
203.00	19.50	42.04#
0.00	0.00	0.00

S-J
 12/23/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
Data File : BM008565.D
Acq On : 22 Dec 2016 20:50
Operator : UM/SJ
Sample : H5938-11DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:30:13 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:50:04 2016
Response via : Initial Calibration

Instrument :
BNA_M
Client Sampled :
DA831DL

Manual Integrations
APPROVED

umangi
12/23/2016 6:11:37 PM

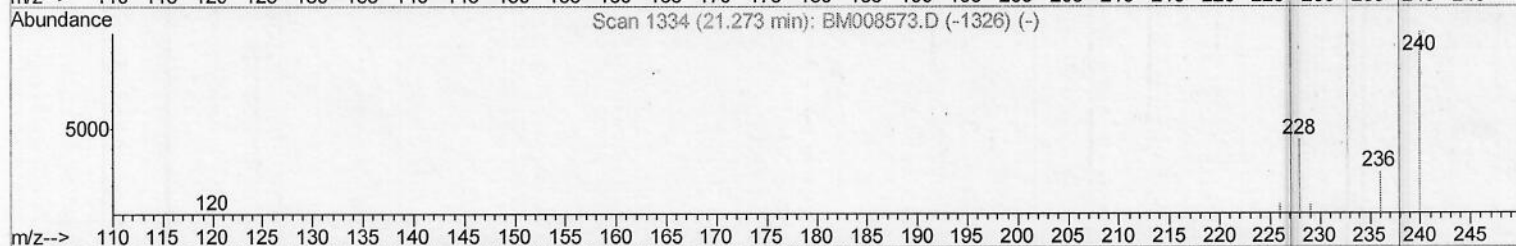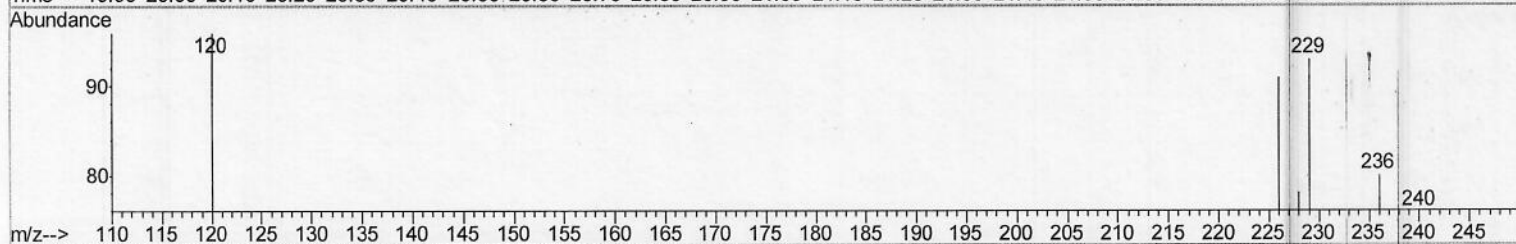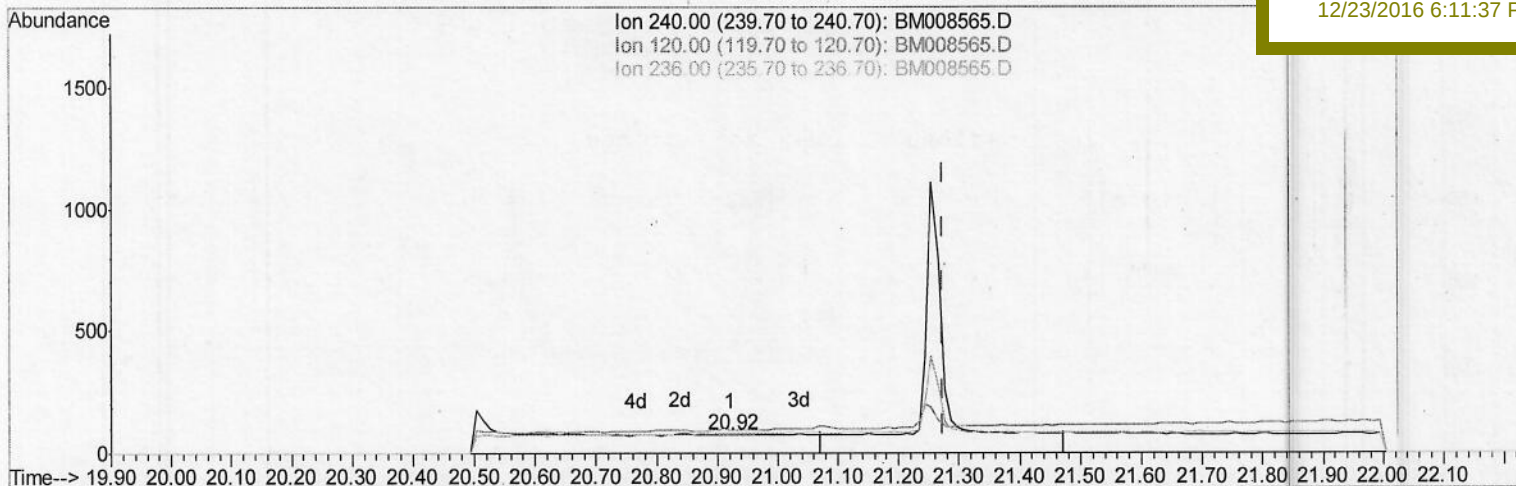

TIC: BM008565.D

(16) Chrysene-d12 (I)

20.922min (-0.351) 0.40ng/ul

response 6

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	126.32#
236.00	34.90	105.26#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
Data File : BM008565.D
Acq On : 22 Dec 2016 20:50
Operator : UM/SJ
Sample : H5938-11DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:30:13 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:50:04 2016
Response via : Initial Calibration

Instrument :

BNA_M




Client Sampled :

DA831DL

Manual Integrations
APPROVED

umangi

12/23/2016 6:11:37 PM

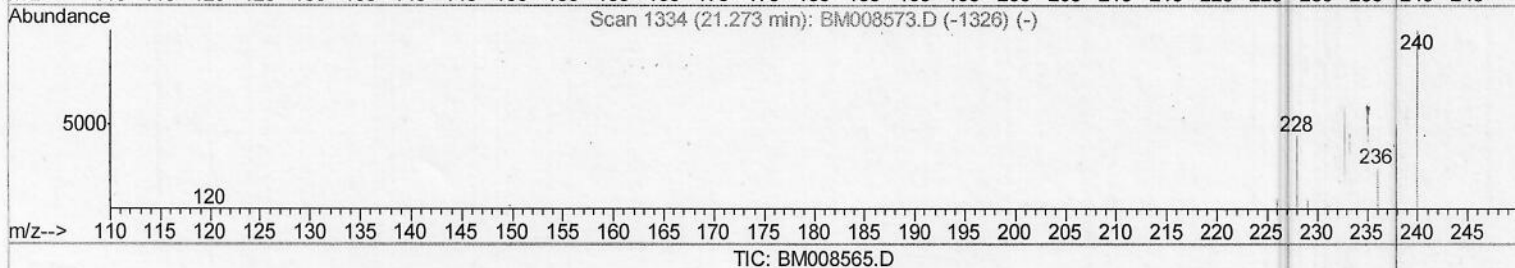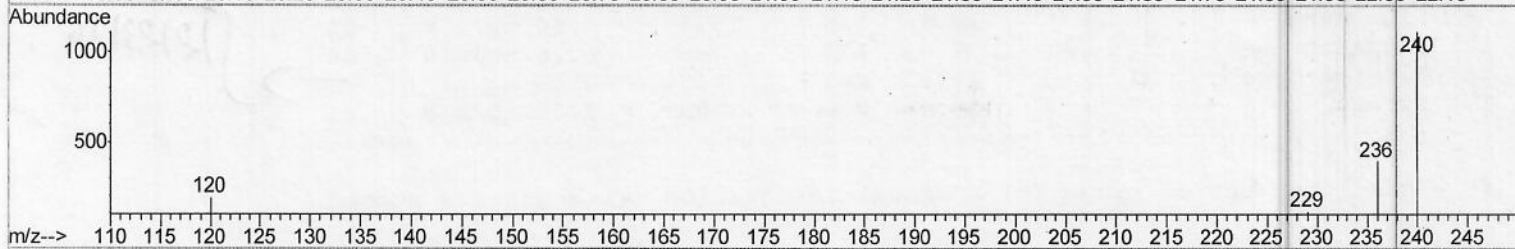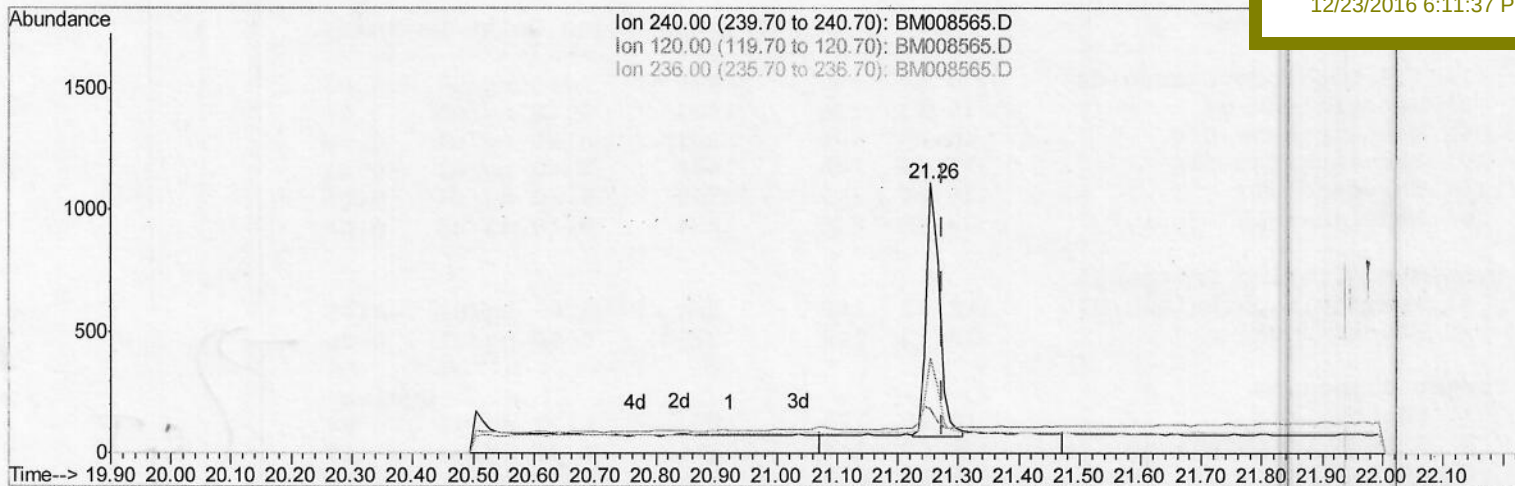

(16) Chrysene-d12 (I)

21.255min (-0.018) 0.40ng/ul m

response 1523

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	16.85
236.00	34.90	35.50
0.00	0.00	0.00

S.J
12/23/2016

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

DA831DL

Quant Time: Dec 23 10:32:01 2016

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Dec 23 05:50:04 2016




Response via : Initial Calibration

Manual Integrations

APPROVED

umangi

12/23/2016 6:11:37 PM

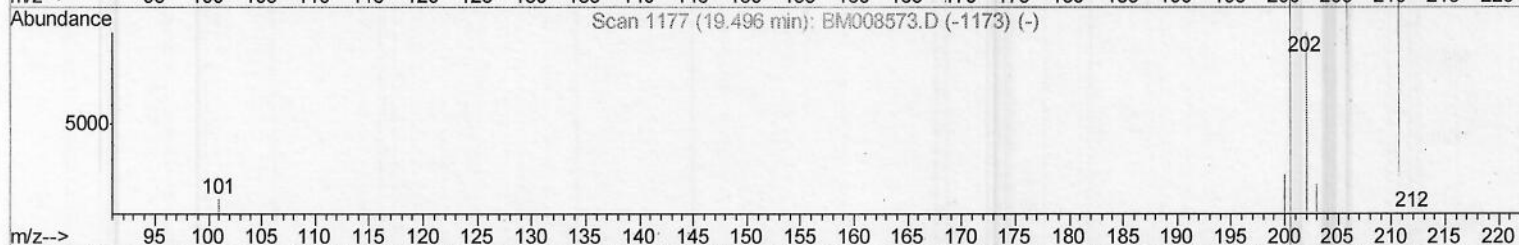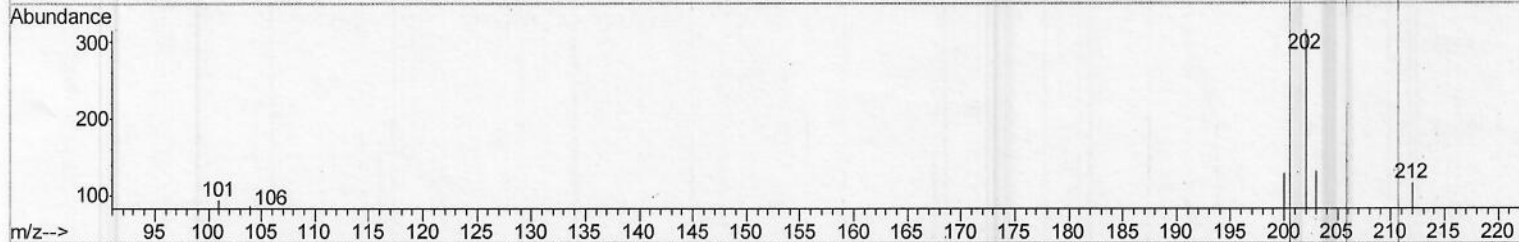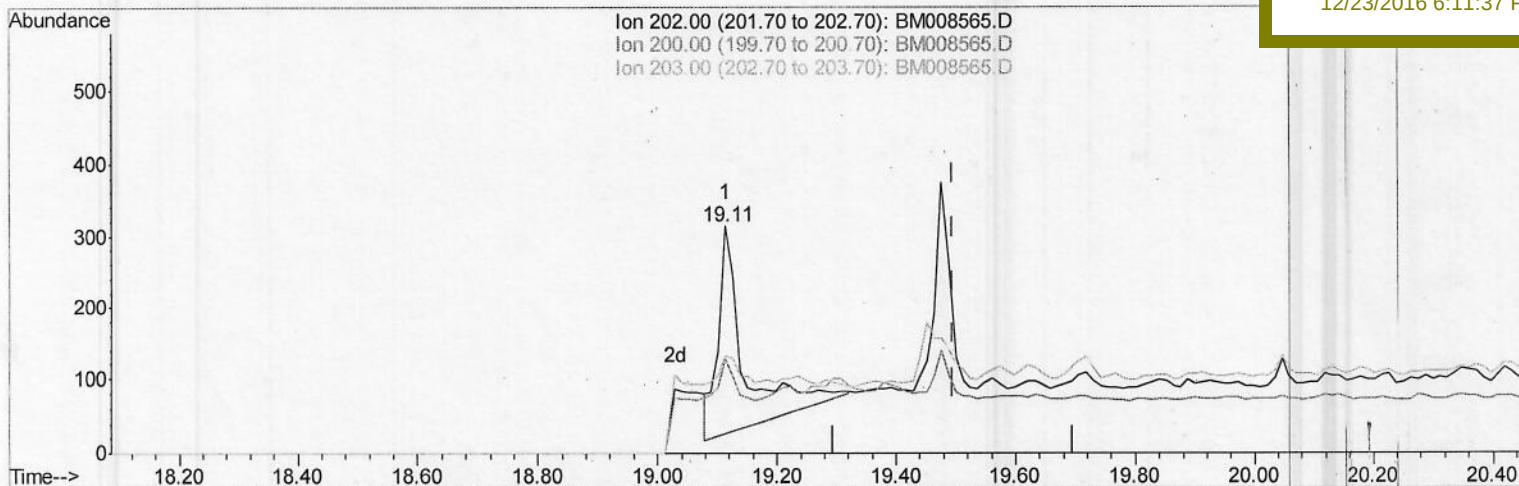

(17) Pyrene

19.113min (-0.382) 0.15ng/ul

response 868

Ion	Exp%	Act%
202.00	100	100
200.00	22.80	40.76#
203.00	19.50	42.04#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 DA831DL

Quant Time: Dec 23 10:32:01 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

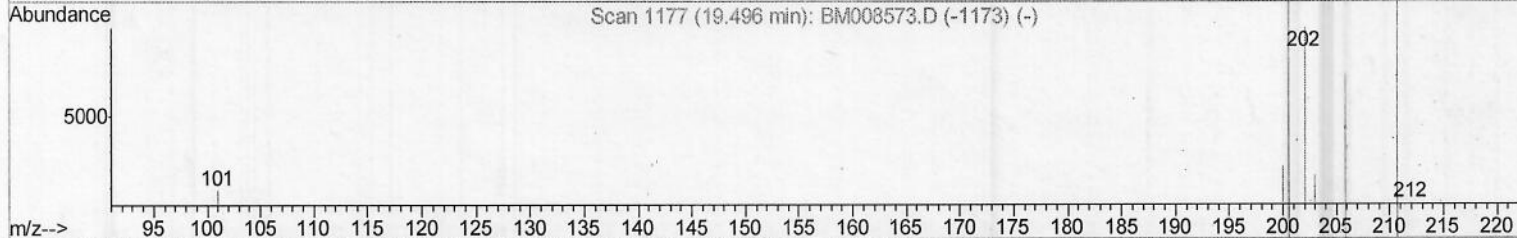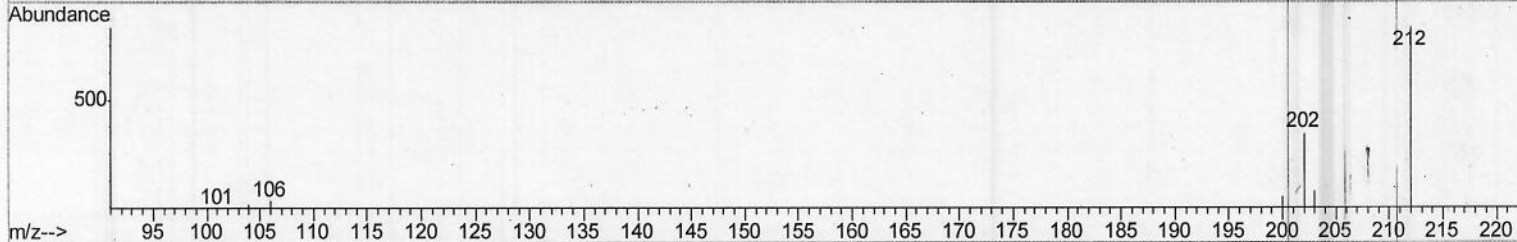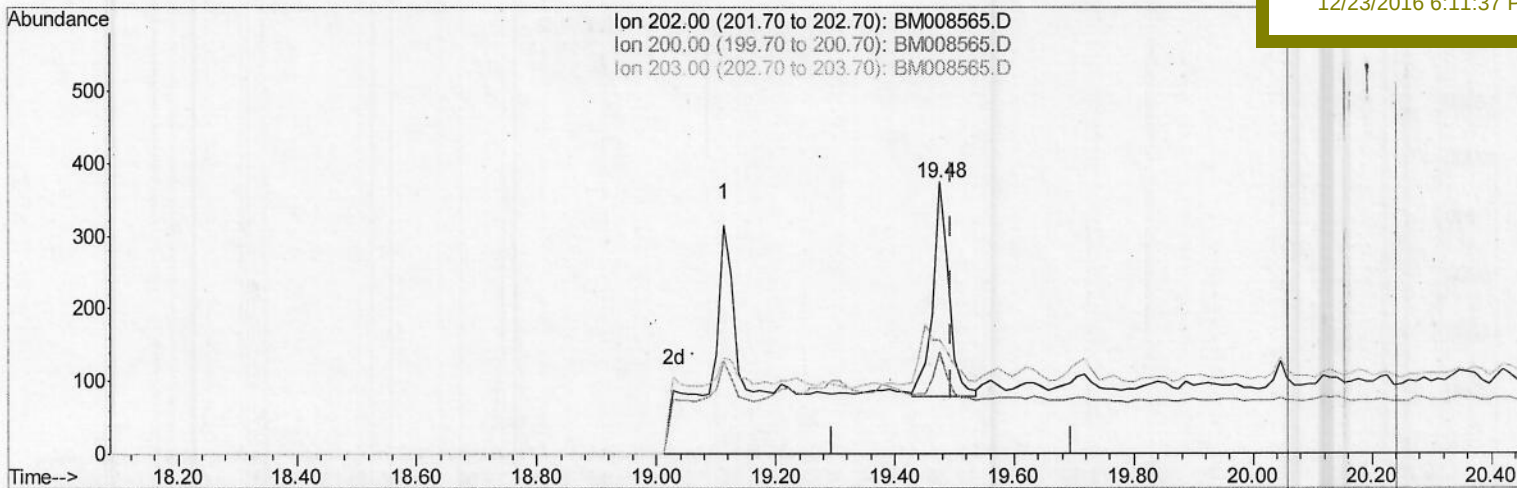

TIC: BM008565.D

(17) Pyrene

19.476min (-0.019) 0.09ng/ul m

response 547

Ion	Exp%	Act%
202.00	100	100
200.00	22.80	37.43#
203.00	19.50	41.98#
0.00	0.00	0.00

S.J
 12/23/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:32:01 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA831DL

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

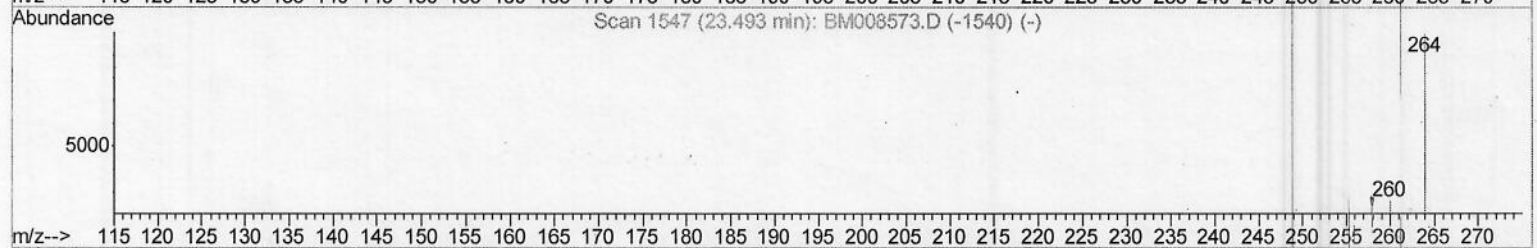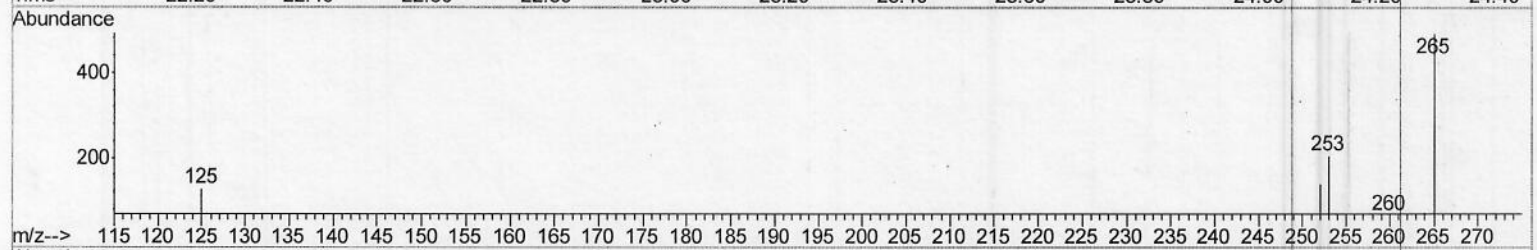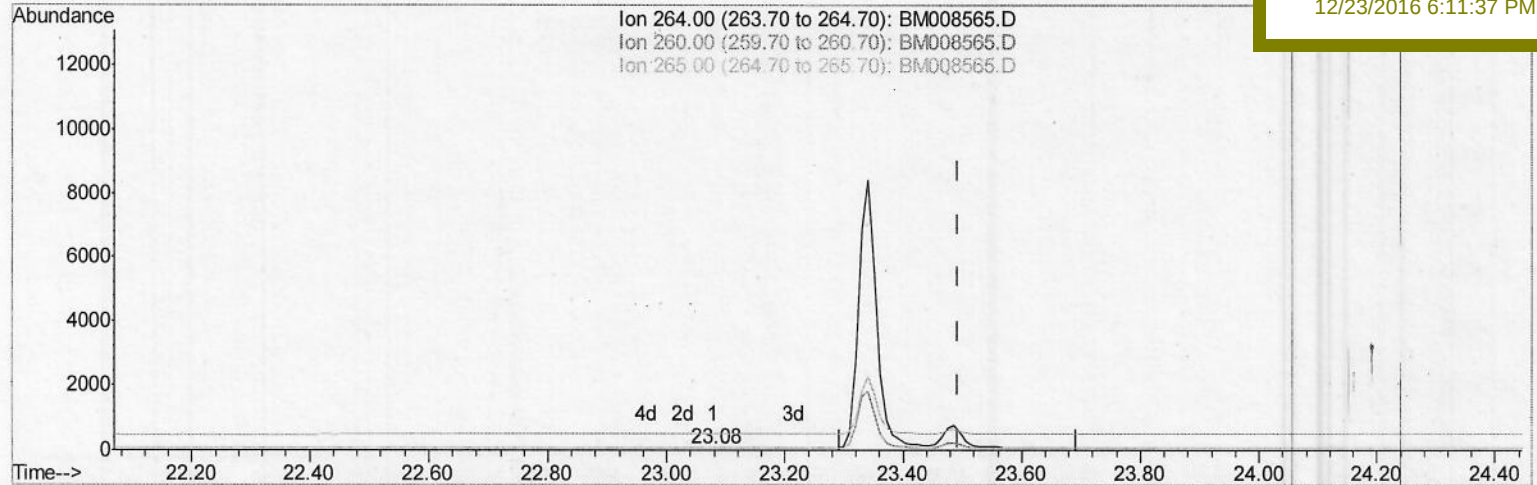

TIC: BM008565.D

(20) Perylene-d12 (I)

23.079min (-0.414) 0.40ng/ul

response 8

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	97.14#
265.00	103.50	704.29#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:32:01 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :

BNA_M

Client Sample ID :




DA831DL

Manual Integrations

APPROVED

umangi

12/23/2016 6:11:37 PM

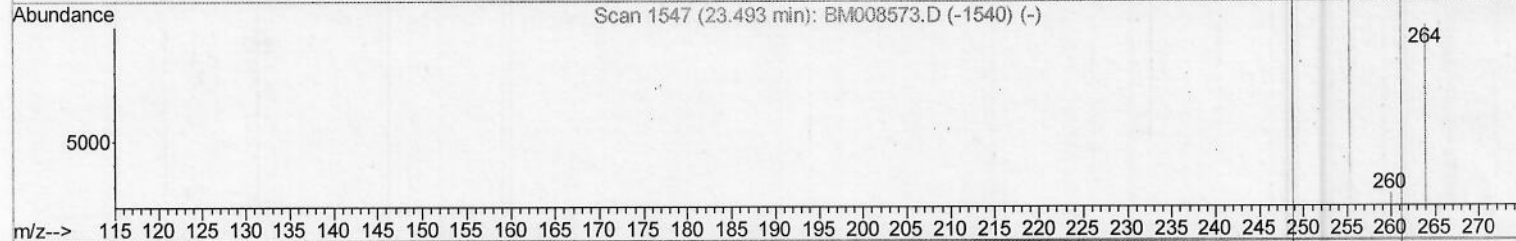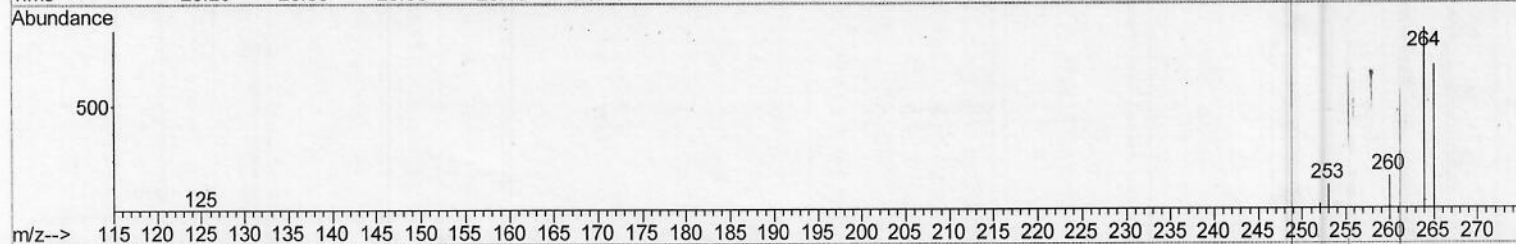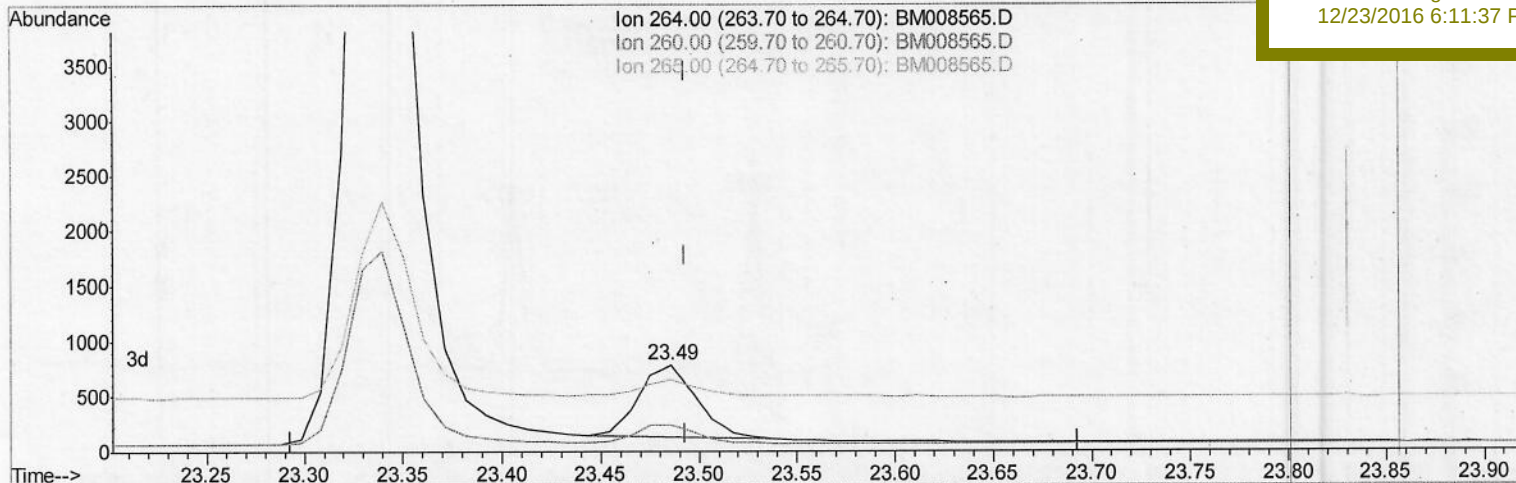

TIC: BM008565.D

(20) Perylene-d12 (I)

23.486min (-0.007) 0.40ng/ul m

response 1333

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	30.61
265.00	103.50	82.40#
0.00	0.00	0.00

S.J
12/23/2016

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
 Data File : BM008565.D
 Acq On : 22 Dec 2016 20:50
 Operator : UM/SJ
 Sample : H5938-11DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:32:57 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 05:50:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 Client Sampled :
 DA831DL

Manual Integrations
 APPROVED

umangi
 12/23/2016 6:11:37 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	441	0.40	ng/ul	-0.08
2) Naphthalene-d8	10.42	136	1454m	0.40	ng/ul	-0.07 →
6) Acenaphthene-d10	14.28	164	993m	0.40	ng/ul	-0.03 →
10) Phenanthrene-d10	17.04	188	1745m	0.40	ng/ul	-0.03 →
16) Chrysene-d12	21.26	240	1523m	0.40	ng/ul	-0.02 →
20) Perylene-d12	23.49	264	1333m	0.40	ng/ul	0.00 →

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.01	152	230m	0.10	ng/ul	-0.08 →
14) Fluoranthene-d10	19.09	212	390m	0.08	ng/ul	-0.02 →

Target Compounds

						Qvalue
3) Naphthalene	10.46	128	28822	7.05	ng/ul	94
5) 2-Methylnaphthalene	12.08	142	34138	12.40	ng/ul	99
8) Acenaphthene	14.35	153	1818m	0.54	ng/ul	→
9) Fluorene	15.34	166	4683m	1.21	ng/ul	→
12) Phenanthrene	17.07	178	2387m	0.45	ng/ul	→
15) Fluoranthene	19.11	202	375m	0.06	ng/ul	→
17) Pyrene	19.48	202	547m	0.09	ng/ul	→

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122216\
Data File : BM008565.D
Acq On : 22 Dec 2016 20:50
Operator : UM/SJ
Sample : H5938-11DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 23 10:32:57 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:50:04 2016
Response via : Initial Calibration

Instrument :
BNA_M
Client Sample ID :
DA831DL

Manual Integrations
APPROVED

umangi
12/23/2016 6:11:37 PM

