

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
 Data File : BM038205.D
 Acq On : 22 Dec 2022 19:26
 Operator : CG/JU
 Sample : PB149721BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK721

Quant Time: Dec 23 01:48:57 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 23:36:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.043	152	4990	0.400	ng/ul	0.00
4) Naphthalene-d8	10.856	136	15417	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.666	164	8504	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.405	188	16647	0.400	ng/ul	0.00
17) Chrysene-d12	21.574	240	9930	0.400	ng/ul	0.00
23) Perylene-d12	24.024	264	10224	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.398	96	25641	5.052	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.435	152	6624	0.292	ng/ul	0.00
18) Fluoranthene-d10	19.427	212	11483	0.308	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.789	202	2081	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.863	252	3434	0.087	ng/ul#	8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
Data File : BM038205.D
Acq On : 22 Dec 2022 19:26
Operator : CG/JU
Sample : PB149721BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Quant Time: Dec 23 01:48:57 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 23:36:45 2022
Response via : Initial Calibration




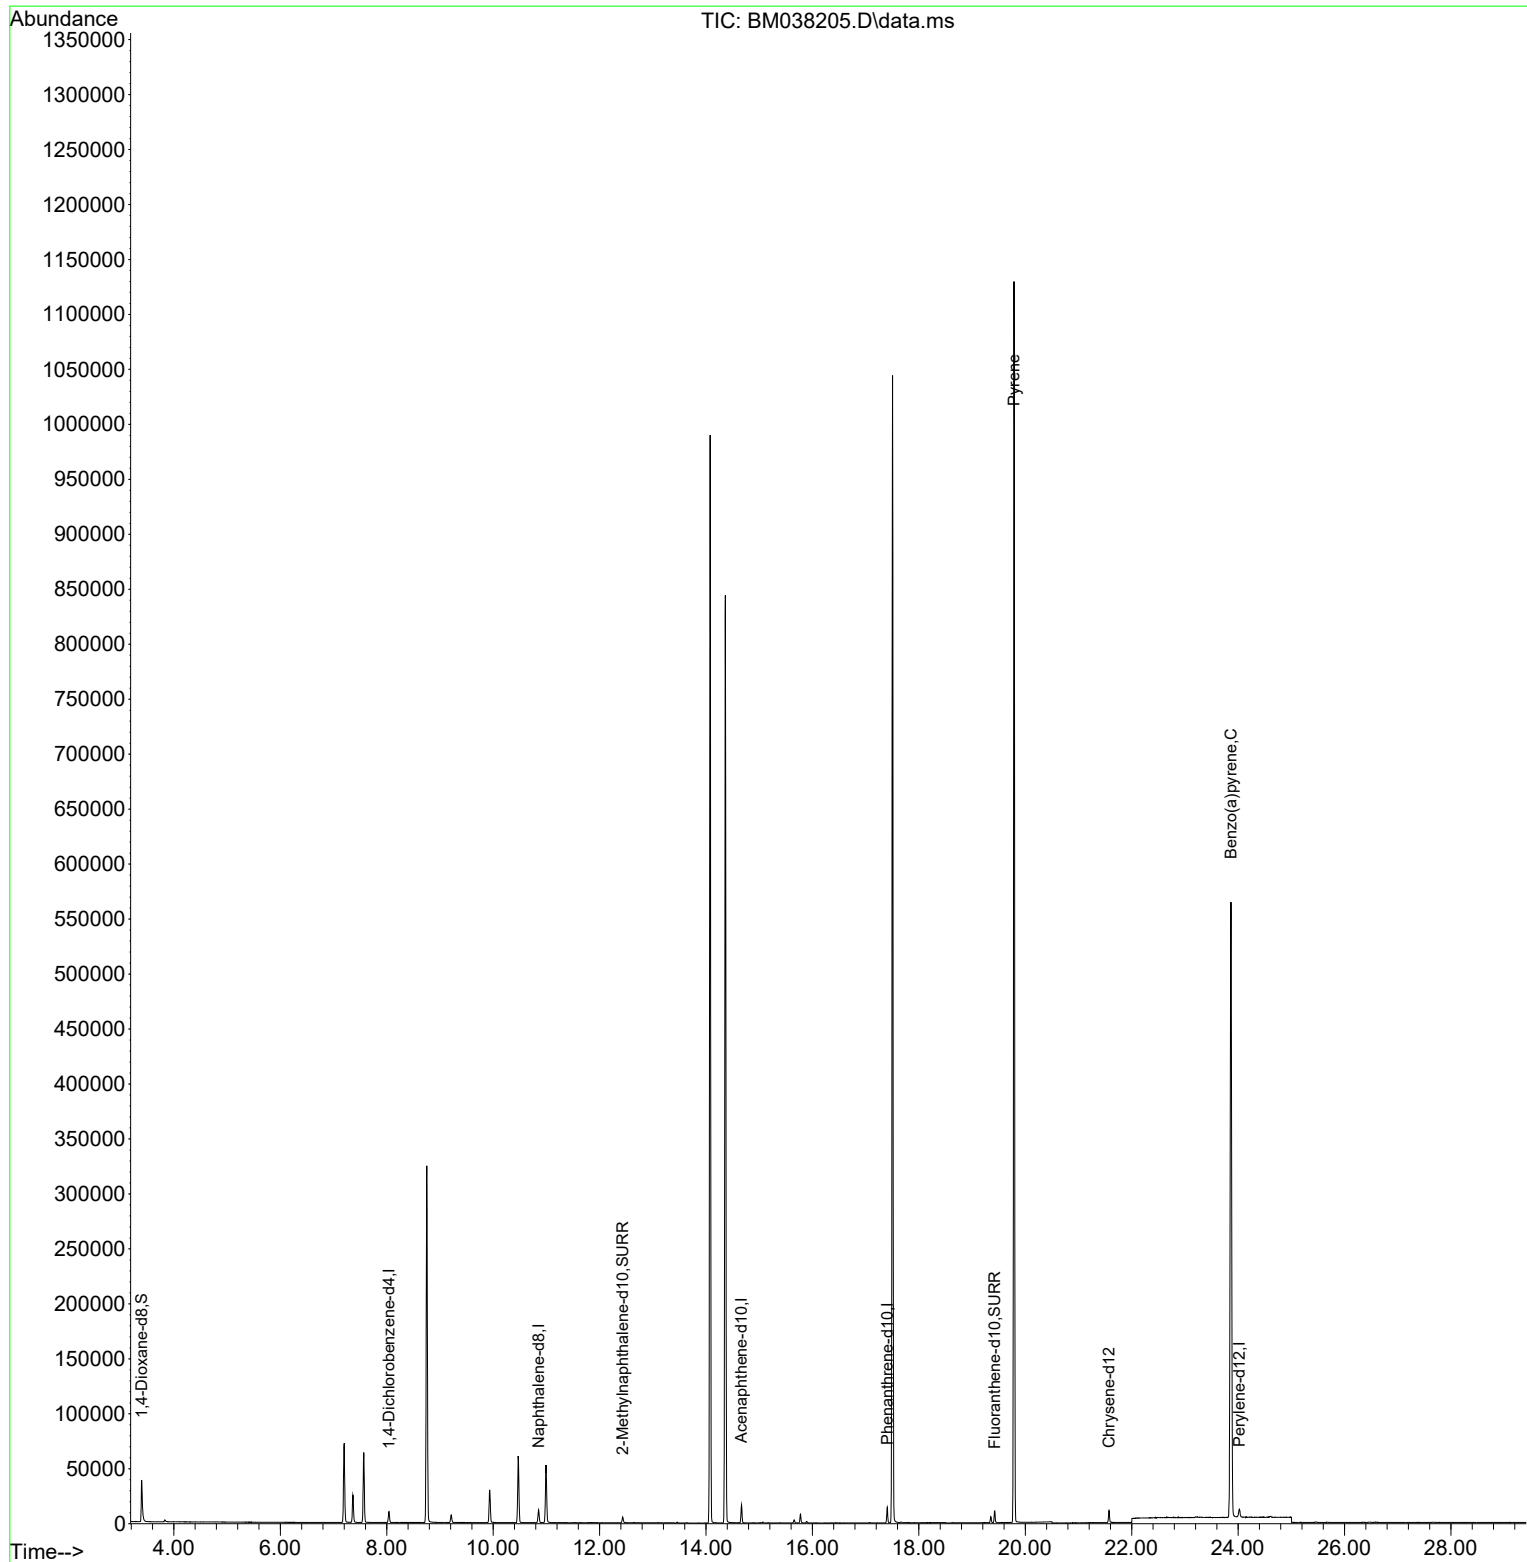


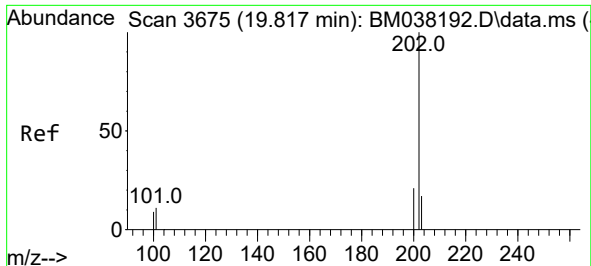

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.789 min Scan# 3081
Delta R.T. -0.028 min
Lab File: BM038205.D
Acq: 22 Dec 2022 19:26

Instrument :
BNA_M
ClientSampleId :
SBLK721

Tgt Ion:202 Resp: 2081
Ion Ratio Lower Upper
202 100
101 132.7 8.9 13.3#
100 962.9 7.4 11.0#

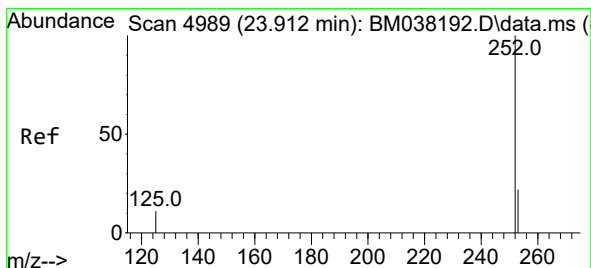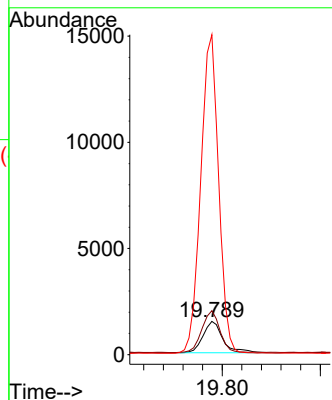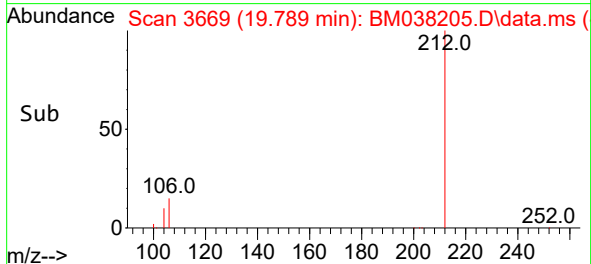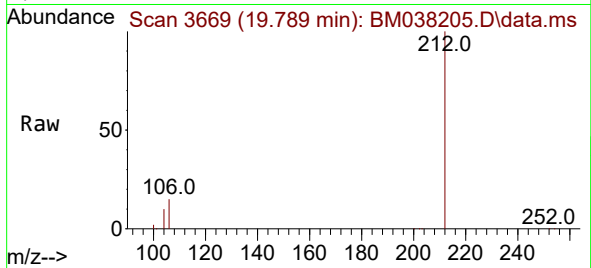

#26
Benzo(a)pyrene
Concen: 0.087 ng/ul
RT: 23.863 min Scan# 4972
Delta R.T. -0.049 min
Lab File: BM038205.D
Acq: 22 Dec 2022 19:26

Tgt Ion:252 Resp: 3434
Ion Ratio Lower Upper
252 100
253 64.0 24.2 36.4#
125 84.7 17.3 25.9#

