

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
 Data File : BM038237.D
 Acq On : 23 Dec 2022 17:54
 Operator : CG/JU
 Sample : PB149780BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 23 23:24:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 23:36:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.038	152	4176	0.400	ng/ul	0.00
4) Naphthalene-d8	10.851	136	12383	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.662	164	6874	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.405	188	13616	0.400	ng/ul	0.00
17) Chrysene-d12	21.574	240	8414	0.400	ng/ul	0.00
23) Perylene-d12	24.023	264	8844	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	23239	5.471	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.429	152	5534	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.422	212	9798	0.310	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.789	202	1927	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.866	252	3165	0.093	ng/ul#	14


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
Data File : BM038237.D
Acq On : 23 Dec 2022 17:54
Operator : CG/JU
Sample : PB149780BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 23 23:24:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 23:36:45 2022
Response via : Initial Calibration




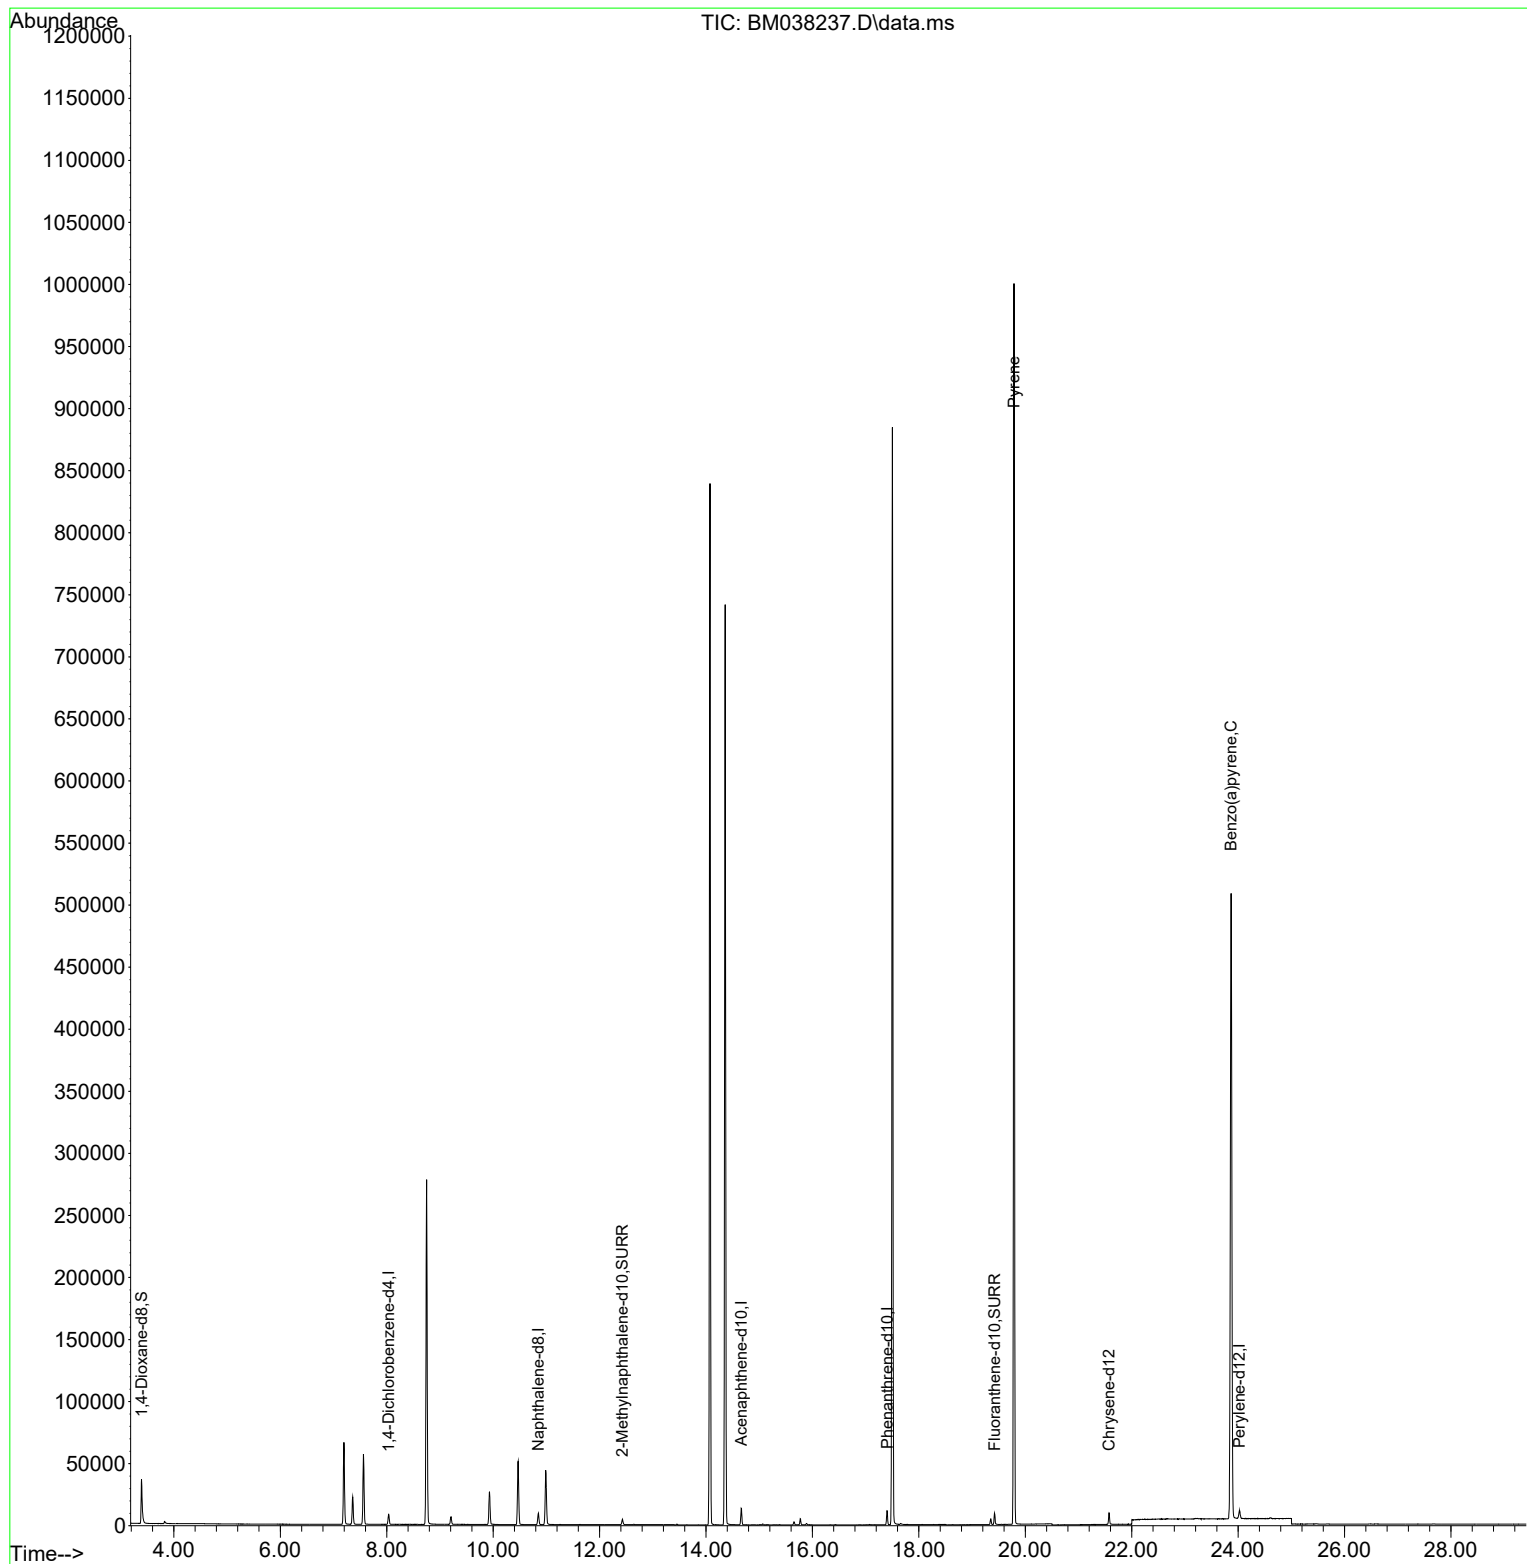


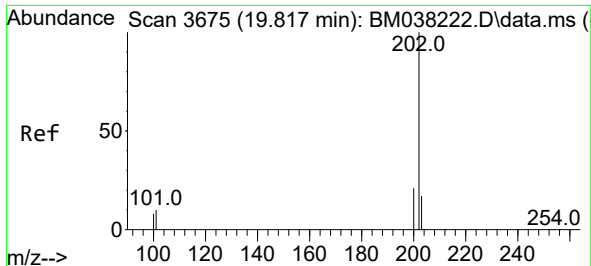

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.789 min Scan# 3669
Delta R.T. -0.028 min
Lab File: BM038237.D
Acq: 23 Dec 2022 17:54

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 1927
Ion Ratio Lower Upper
202 100
101 132.0 8.9 13.3#
100 937.7 7.4 11.0#

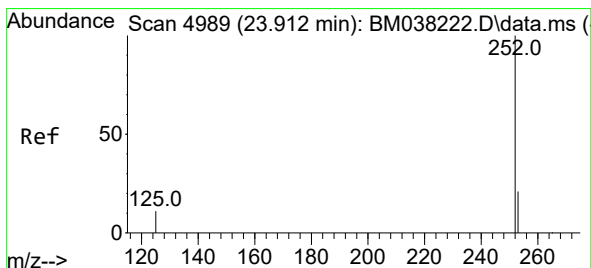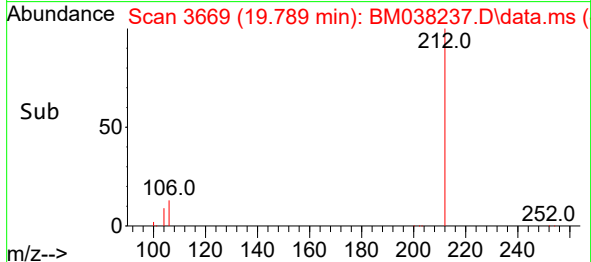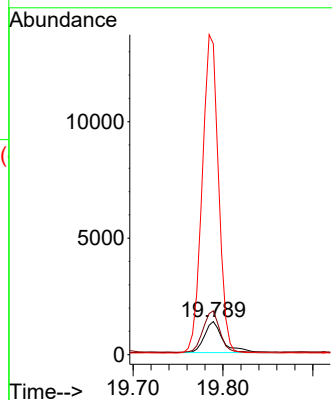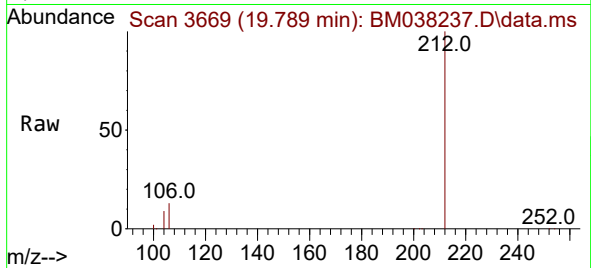

#26
Benzo(a)pyrene
Concen: 0.093 ng/ul
RT: 23.866 min Scan# 4973
Delta R.T. -0.047 min
Lab File: BM038237.D
Acq: 23 Dec 2022 17:54

Tgt Ion:252 Resp: 3165
Ion Ratio Lower Upper
252 100
253 64.7 24.2 36.4#
125 76.9 17.3 25.9#

