

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
 Data File : BM038238.D
 Acq On : 23 Dec 2022 18:31
 Operator : CG/JU
 Sample : N6014-17
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 23 23:24:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 23:36:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	3882	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136	11519	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.661	164	6369	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.405	188	12437	0.400	ng/ul	0.00
17) Chrysene-d12	21.574	240	8025	0.400	ng/ul	# 0.00
23) Perylene-d12	24.023	264	8128	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	14944	3.784	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.429	152	4298	0.253	ng/ul	0.00
18) Fluoranthene-d10	19.422	212	7830	0.260	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.900	128	1376	0.041	ng/ul#	85
7) 2-Methylnaphthalene	12.500	142	601	0.029	ng/ul	99
8) 1-Methylnaphthalene	12.720	142	444	0.021	ng/ul	94
10) Acenaphthylene	14.384	152	2772	0.079	ng/ul#	89
11) Acenaphthene	14.726	153	619	0.025	ng/ul	94
12) Fluorene	15.707	166	555	0.020	ng/ul#	88
15) Phenanthrene	17.447	178	12546	0.301	ng/ul	100
16) Anthracene	17.535	178	3482	0.087	ng/ul#	91
19) Fluoranthene	19.454	202	36303	0.826	ng/ul	100
20) Pyrene	19.817	202	34154	0.769	ng/ul	98
21) Benzo(a)anthracene	21.556	228	17367	0.493	ng/ul	97
22) Chrysene	21.612	228	19626	0.573	ng/ul	97
24) Benzo(b)fluoranthene	23.275	252	30392	0.845	ng/ul	99
26) Benzo(a)pyrene	23.915	252	18620	0.593	ng/ul	98
27) Indeno(1,2,3-cd)pyrene	26.582	276	15612	0.359	ng/ul#	90
28) Dibenzo(a,h)anthracene	26.592	278	3909	0.116	ng/ul#	51
29) Benzo(g,h,i)perylene	27.377	276	15775	0.431	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
Data File : BM038238.D
Acq On : 23 Dec 2022 18:31
Operator : CG/JU
Sample : N6014-17
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Dec 23 23:24:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 23:36:45 2022
Response via : Initial Calibration

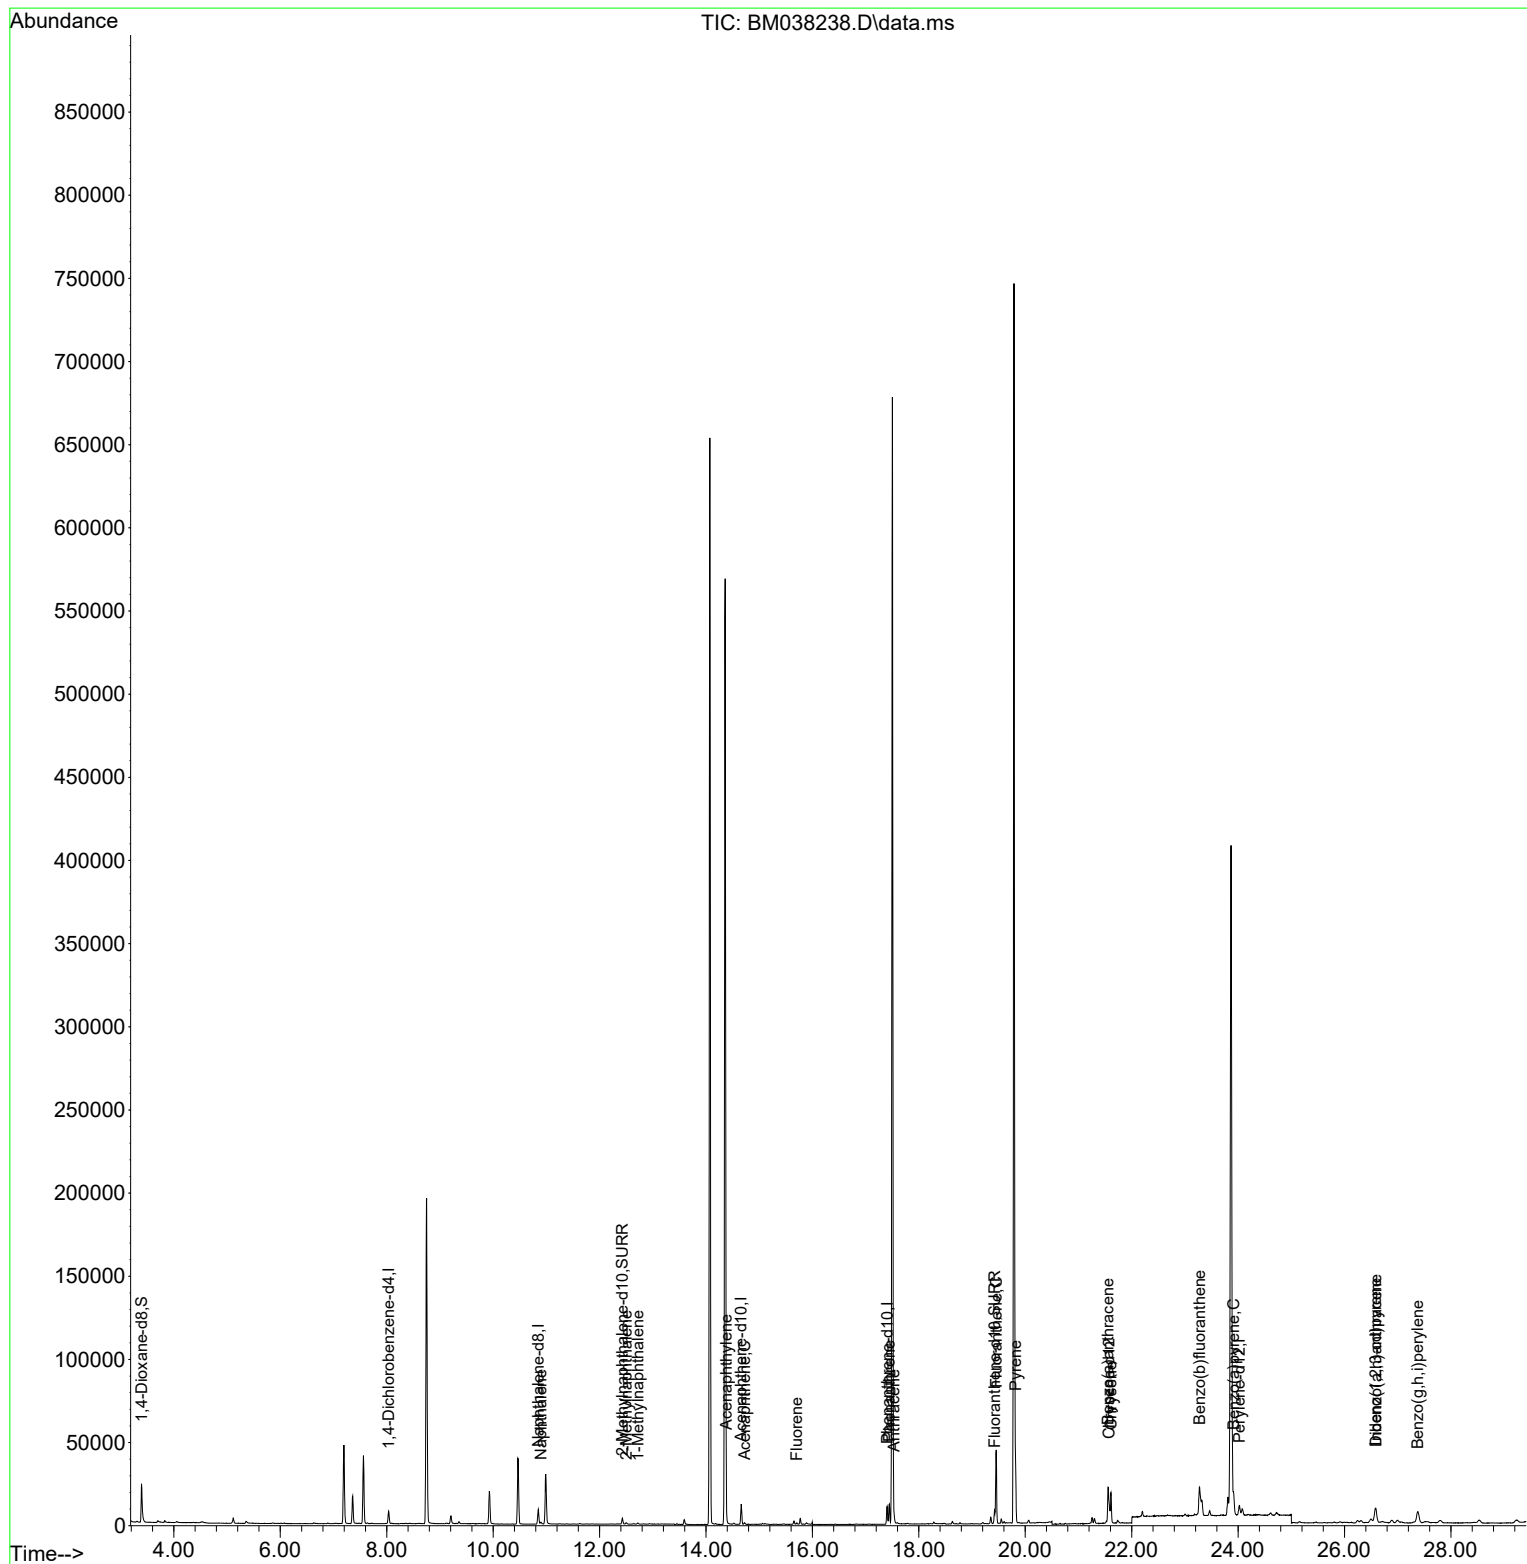



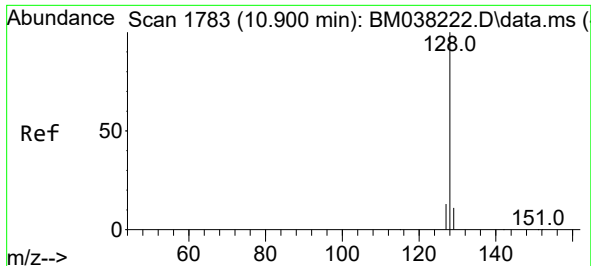


#5
Naphthalene
Concen: 0.041 ng/ul
RT: 10.900 min Scan# 1783
Delta R.T. -0.005 min
Lab File: BM038238.D
Acq: 23 Dec 2022 18:31

Instrument :
BNA_M
ClientSampleId :







Tgt Ion:128 Resp: 1376
Ion Ratio Lower Upper
128 100
129 18.0 9.4 14.0#
127 19.2 10.7 16.1#

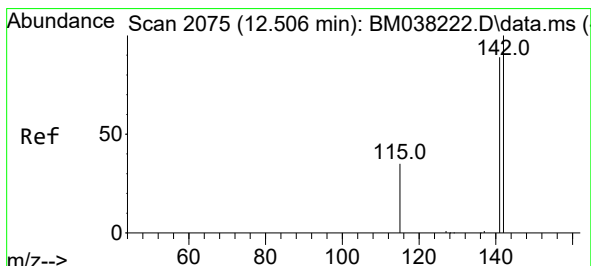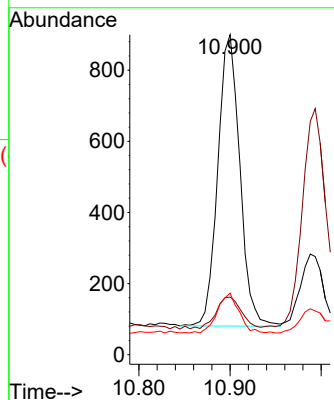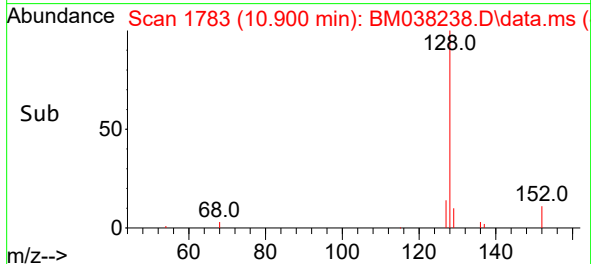

#7
2-Methylnaphthalene
Concen: 0.029 ng/ul
RT: 12.500 min Scan# 2074
Delta R.T. -0.005 min
Lab File: BM038238.D
Acq: 23 Dec 2022 18:31

Tgt Ion:142 Resp: 601
Ion Ratio Lower Upper
142 100
141 90.7 71.9 107.9

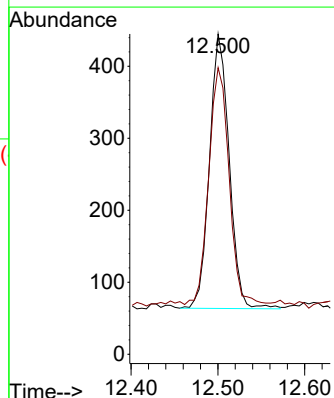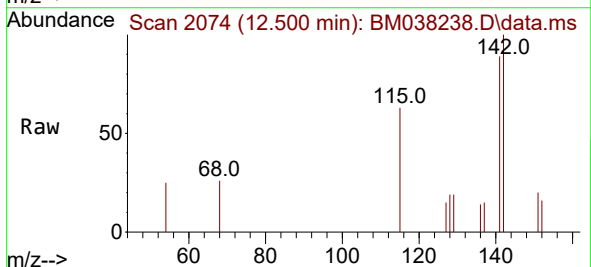



#8

1-Methylnaphthalene

Concen: 0.021 ng/ul

RT: 12.720 min Scan# 2114

Delta R.T. -0.005 min


Lab File: BM038238.D

Acq: 23 Dec 2022 18:31

Instrument :

BNA_M

ClientSampleId :






Tgt Ion:142 Resp: 444

Ion Ratio Lower Upper

142 100

141 99.1 74.7 112.1

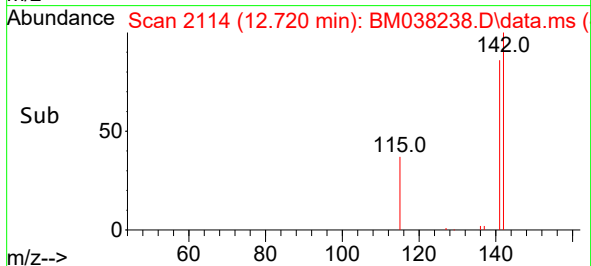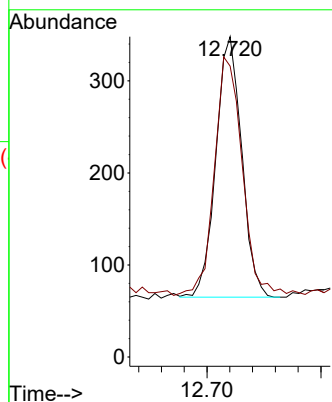

#10

Acenaphthylene

Concen: 0.079 ng/ul

RT: 14.384 min Scan# 2450

Delta R.T. -0.005 min

Lab File: BM038238.D

Acq: 23 Dec 2022 18:31




Tgt Ion:152 Resp: 2772


Ion Ratio Lower Upper

152 100

151 25.0 16.2 24.2#

153 18.2 10.7 16.1#

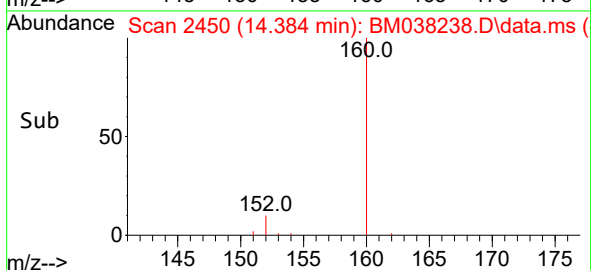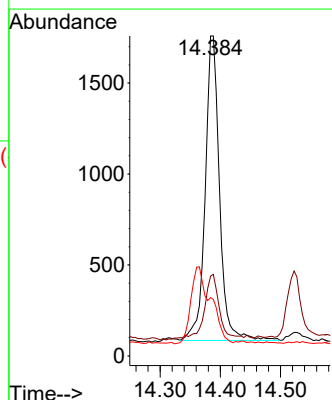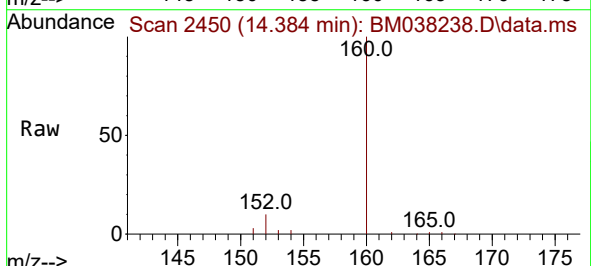



#11

Acenaphthene

Concen: 0.025 ng/ul

RT: 14.726 min Scan# 2

Delta R.T. -0.005 min


Lab File: BM038238.D

Acq: 23 Dec 2022 18:31

Instrument :

BNA_M

ClientSampleId :

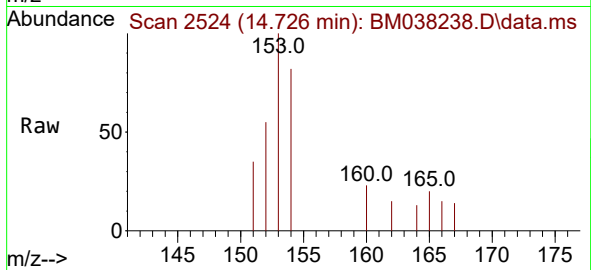




Tgt Ion:153 Resp: 619

Ion Ratio Lower Upper

153 100

152 54.6 39.4 59.0

154 82.3 69.0 103.4

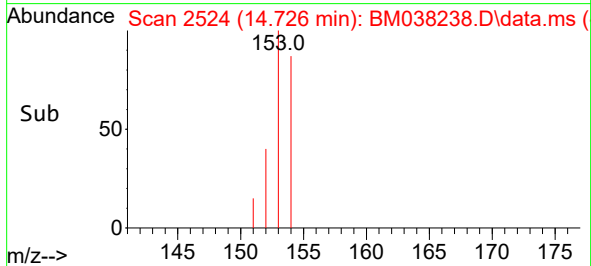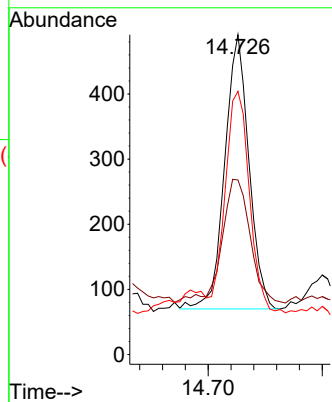

#12

Fluorene

Concen: 0.020 ng/ul

RT: 15.707 min Scan# 2736

Delta R.T. -0.005 min

Lab File: BM038238.D

Acq: 23 Dec 2022 18:31




Tgt Ion:166 Resp: 555


Ion Ratio Lower Upper

166 100

165 106.8 79.0 118.6

167 28.7 11.0 16.6#


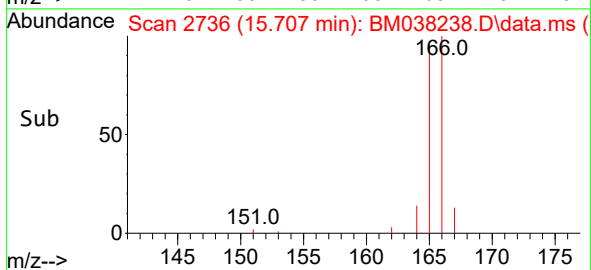
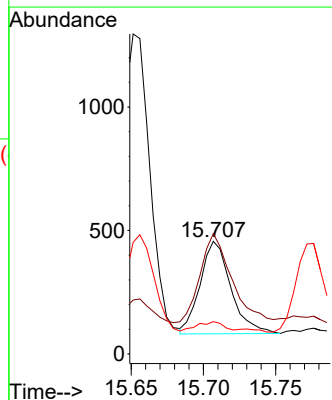
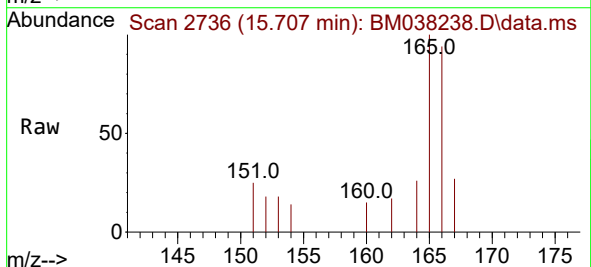


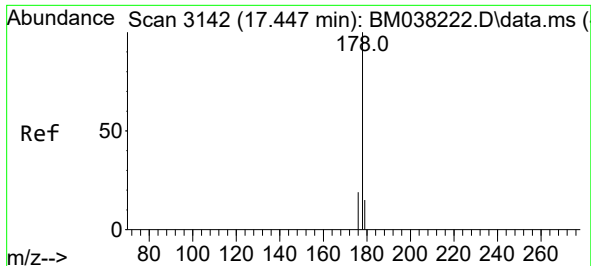

#15
Phenanthrene
Concen: 0.301 ng/ul
RT: 17.447 min Scan# 3142
Delta R.T. 0.000 min
Lab File: BM038238.D
Acq: 23 Dec 2022 18:31




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:178 Resp: 12546
Ion Ratio Lower Upper
178 100
179 16.5 13.0 19.4
176 20.4 16.2 24.4

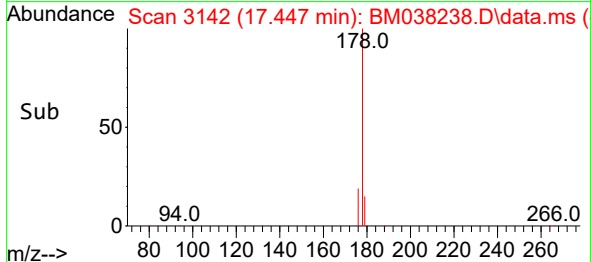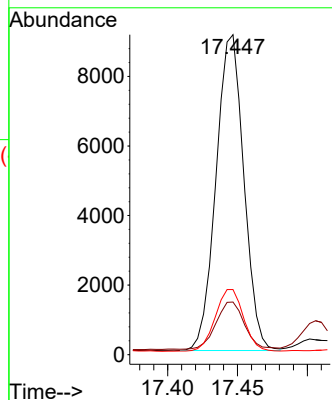

#16
Anthracene
Concen: 0.087 ng/ul
RT: 17.535 min Scan# 3163
Delta R.T. -0.004 min
Lab File: BM038238.D
Acq: 23 Dec 2022 18:31

Tgt Ion:178 Resp: 3482
Ion Ratio Lower Upper
178 100
179 20.6 13.0 19.6#
176 22.9 15.6 23.4


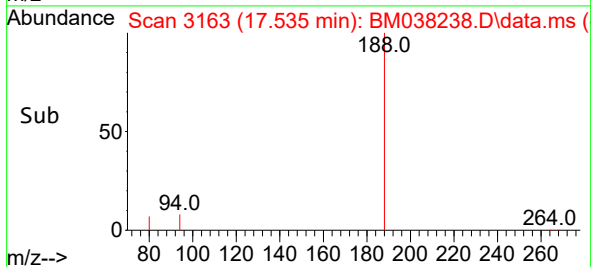
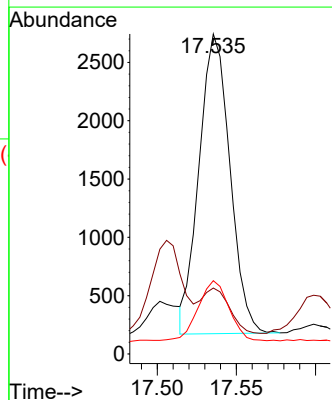
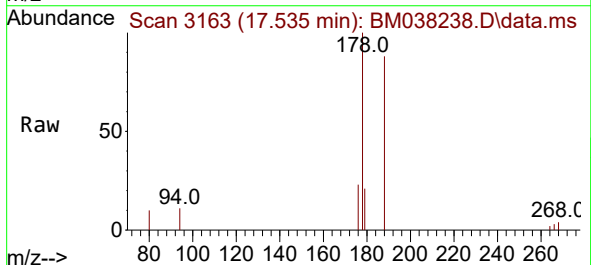




#19
Fluoranthene
Concen: 0.826 ng/ul
RT: 19.454 min Scan# 3597
Delta R.T. 0.000 min
Lab File: BM038238.D
Acq: 23 Dec 2022 18:31




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:202 Resp: 36303
Ion Ratio Lower Upper
202 100
101 9.4 7.5 11.3
100 6.8 5.6 8.4

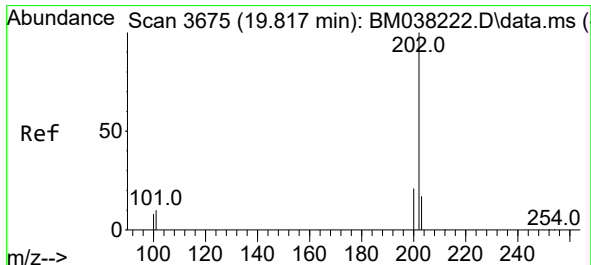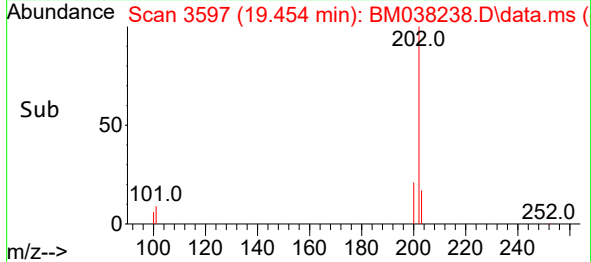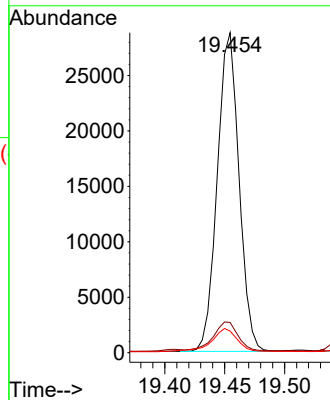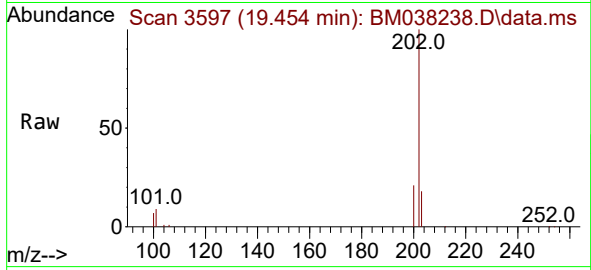

#20
Pyrene
Concen: 0.769 ng/ul
RT: 19.817 min Scan# 3675
Delta R.T. 0.000 min
Lab File: BM038238.D
Acq: 23 Dec 2022 18:31

Tgt Ion:202 Resp: 34154
Ion Ratio Lower Upper
202 100
101 10.1 8.9 13.3
100 8.6 7.4 11.0


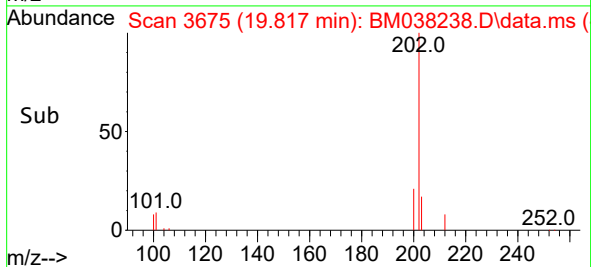
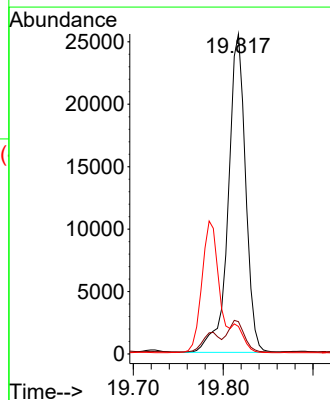
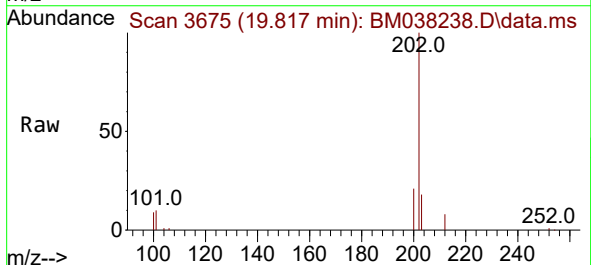


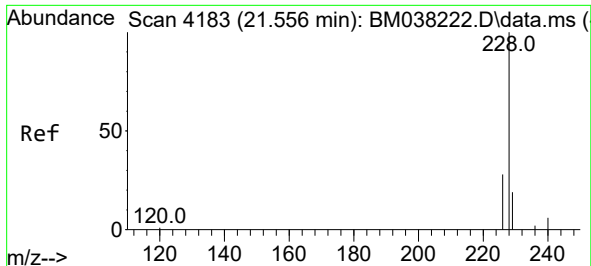

#21
Benzo(a)anthracene
Concen: 0.493 ng/ul
RT: 21.556 min Scan# 4183
Delta R.T. -0.003 min
Lab File: BM038238.D
Acq: 23 Dec 2022 18:31




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:228 Resp: 17367
Ion Ratio Lower Upper
228 100
229 21.3 15.5 23.3
226 29.0 22.2 33.2

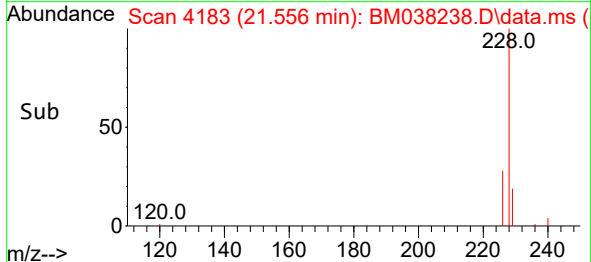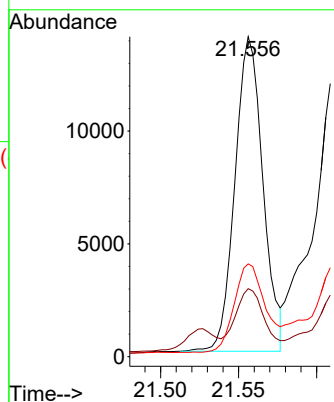

#22
Chrysene
Concen: 0.573 ng/ul
RT: 21.612 min Scan# 4202
Delta R.T. 0.000 min
Lab File: BM038238.D
Acq: 23 Dec 2022 18:31

Tgt Ion:228 Resp: 19626
Ion Ratio Lower Upper
228 100
226 32.2 25.0 37.4
229 22.8 16.0 24.0


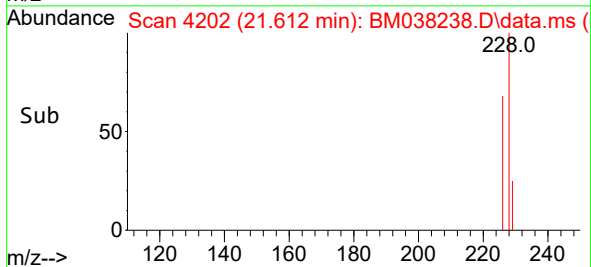
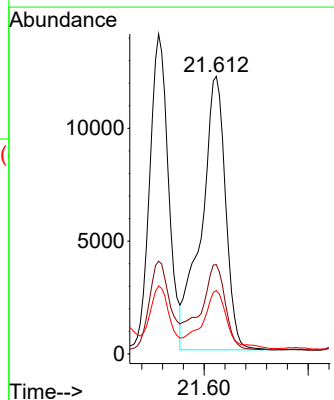
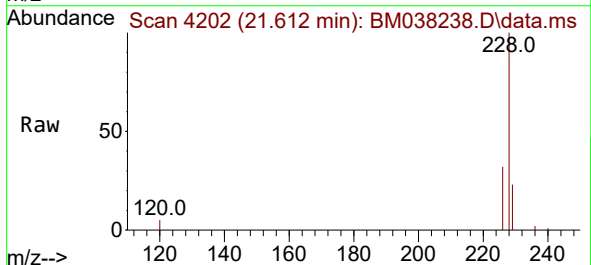


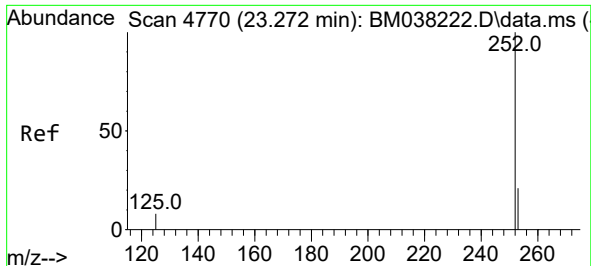

#24
Benzo(b)fluoranthene
Concen: 0.845 ng/ul
RT: 23.275 min Scan# 4770
Delta R.T. 0.003 min
Lab File: BM038238.D
Acq: 23 Dec 2022 18:31




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:252 Resp: 30392
Ion Ratio Lower Upper
252 100
253 27.9 0.0 56.0
125 17.8 0.0 36.6

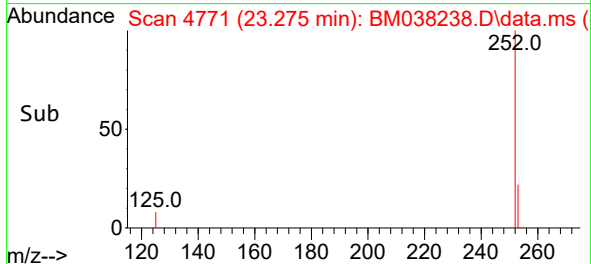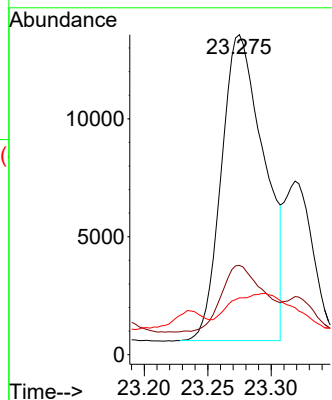

#26
Benzo(a)pyrene
Concen: 0.593 ng/ul
RT: 23.915 min Scan# 4990
Delta R.T. 0.003 min
Lab File: BM038238.D
Acq: 23 Dec 2022 18:31


Tgt Ion:252 Resp: 18620
Ion Ratio Lower Upper
252 100
253 30.1 24.2 36.4
125 20.0 17.3 25.9

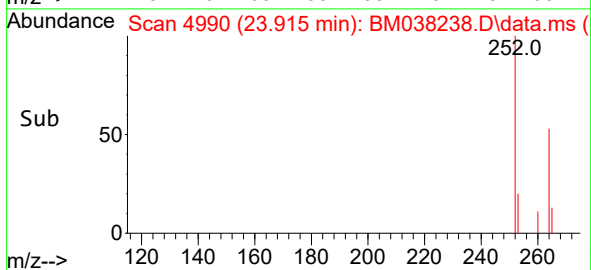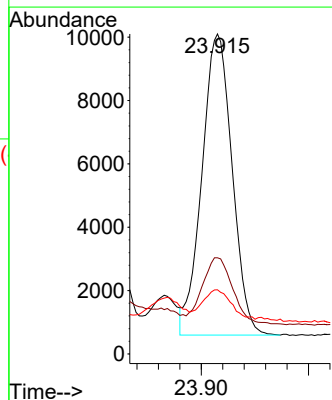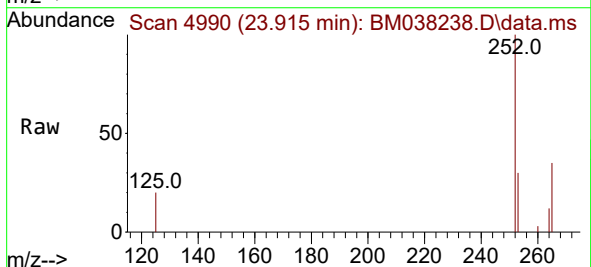



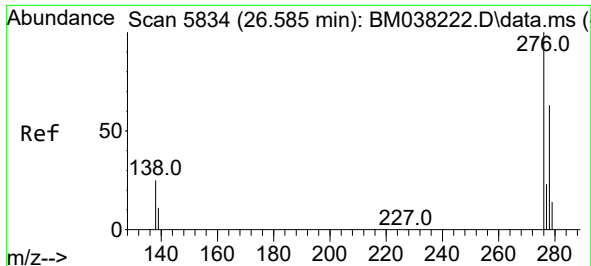


#27
 Indeno(1,2,3-cd)pyrene
 Concen: 0.359 ng/ul
 RT: 26.582 min Scan# 5833
 Delta R.T. 0.000 min
 Lab File: BM038238.D
 Acq: 23 Dec 2022 18:31

Instrument :
 BNA_M
 ClientSampleId :







Tgt Ion:276 Resp: 15612
 Ion Ratio Lower Upper
 276 100
 138 21.7 21.7 32.5#
 227 0.0 0.0 0.0

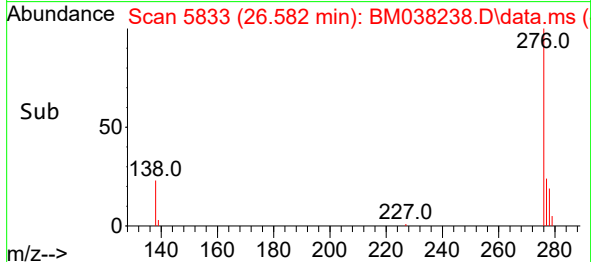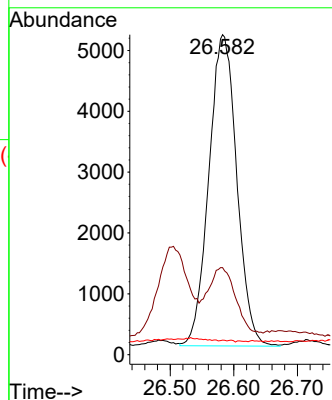

#28
 Dibenzo(a,h)anthracene
 Concen: 0.116 ng/ul
 RT: 26.592 min Scan# 5836
 Delta R.T. -0.003 min
 Lab File: BM038238.D
 Acq: 23 Dec 2022 18:31


Tgt Ion:278 Resp: 3909
 Ion Ratio Lower Upper
 278 100
 139 40.4 16.8 25.2#
 279 58.6 23.4 35.2#

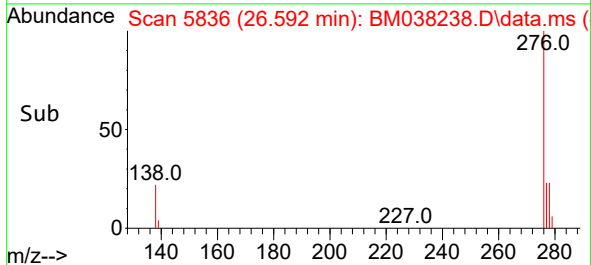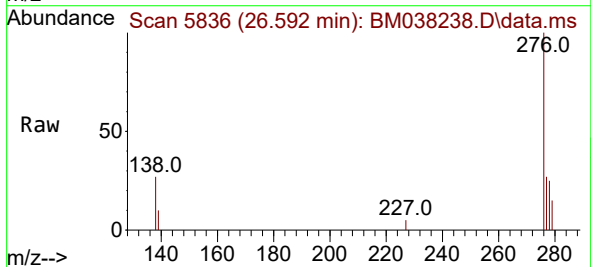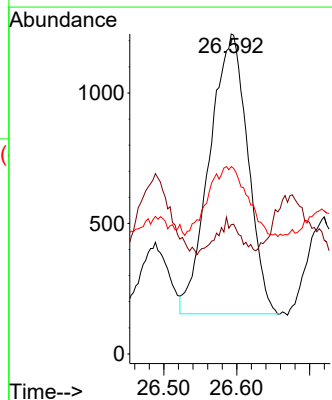



#29
 Benzo(g,h,i)perylene
 Concen: 0.431 ng/ul
 RT: 27.377 min Scan# 6070
 Delta R.T. 0.007 min
 Lab File: BM038238.D
 Acq: 23 Dec 2022 18:31

Instrument :
 BNA_M
 ClientSampleId :

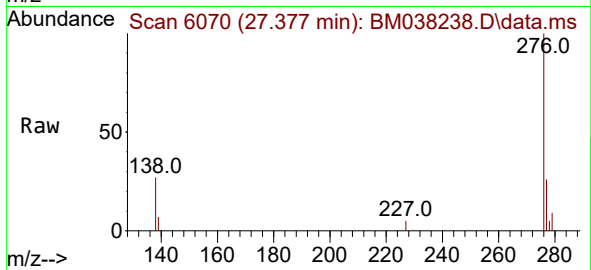

Tgt Ion:276 Resp: 15775
 Ion Ratio Lower Upper
 276 100
 138 27.3 20.8 31.2
 277 25.6 20.5 30.7

