

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
 Data File : BM038273.D
 Acq On : 24 Dec 2022 16:44
 Operator : CG/JU
 Sample : PB149811BL
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 25 02:56:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 24 05:23:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.030	152	3964	0.400	ng/ul	0.00
4) Naphthalene-d8	10.845	136	11961	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.657	164	6921	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.396	188	12875	0.400	ng/ul	0.00
17) Chrysene-d12	21.568	240	8820	0.400	ng/ul	0.00
23) Perylene-d12	24.015	264	8573	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	18461	4.578	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.423	152	4830	0.274	ng/ul	0.00
18) Fluoranthene-d10	19.417	212	8472	0.256	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.647	166	1863	0.063	ng/ul#	16
20) Pyrene	19.784	202	1591	0.033	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
Data File : BM038273.D
Acq On : 24 Dec 2022 16:44
Operator : CG/JU
Sample : PB149811BL
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Dec 25 02:56:38 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 24 05:23:31 2022
Response via : Initial Calibration

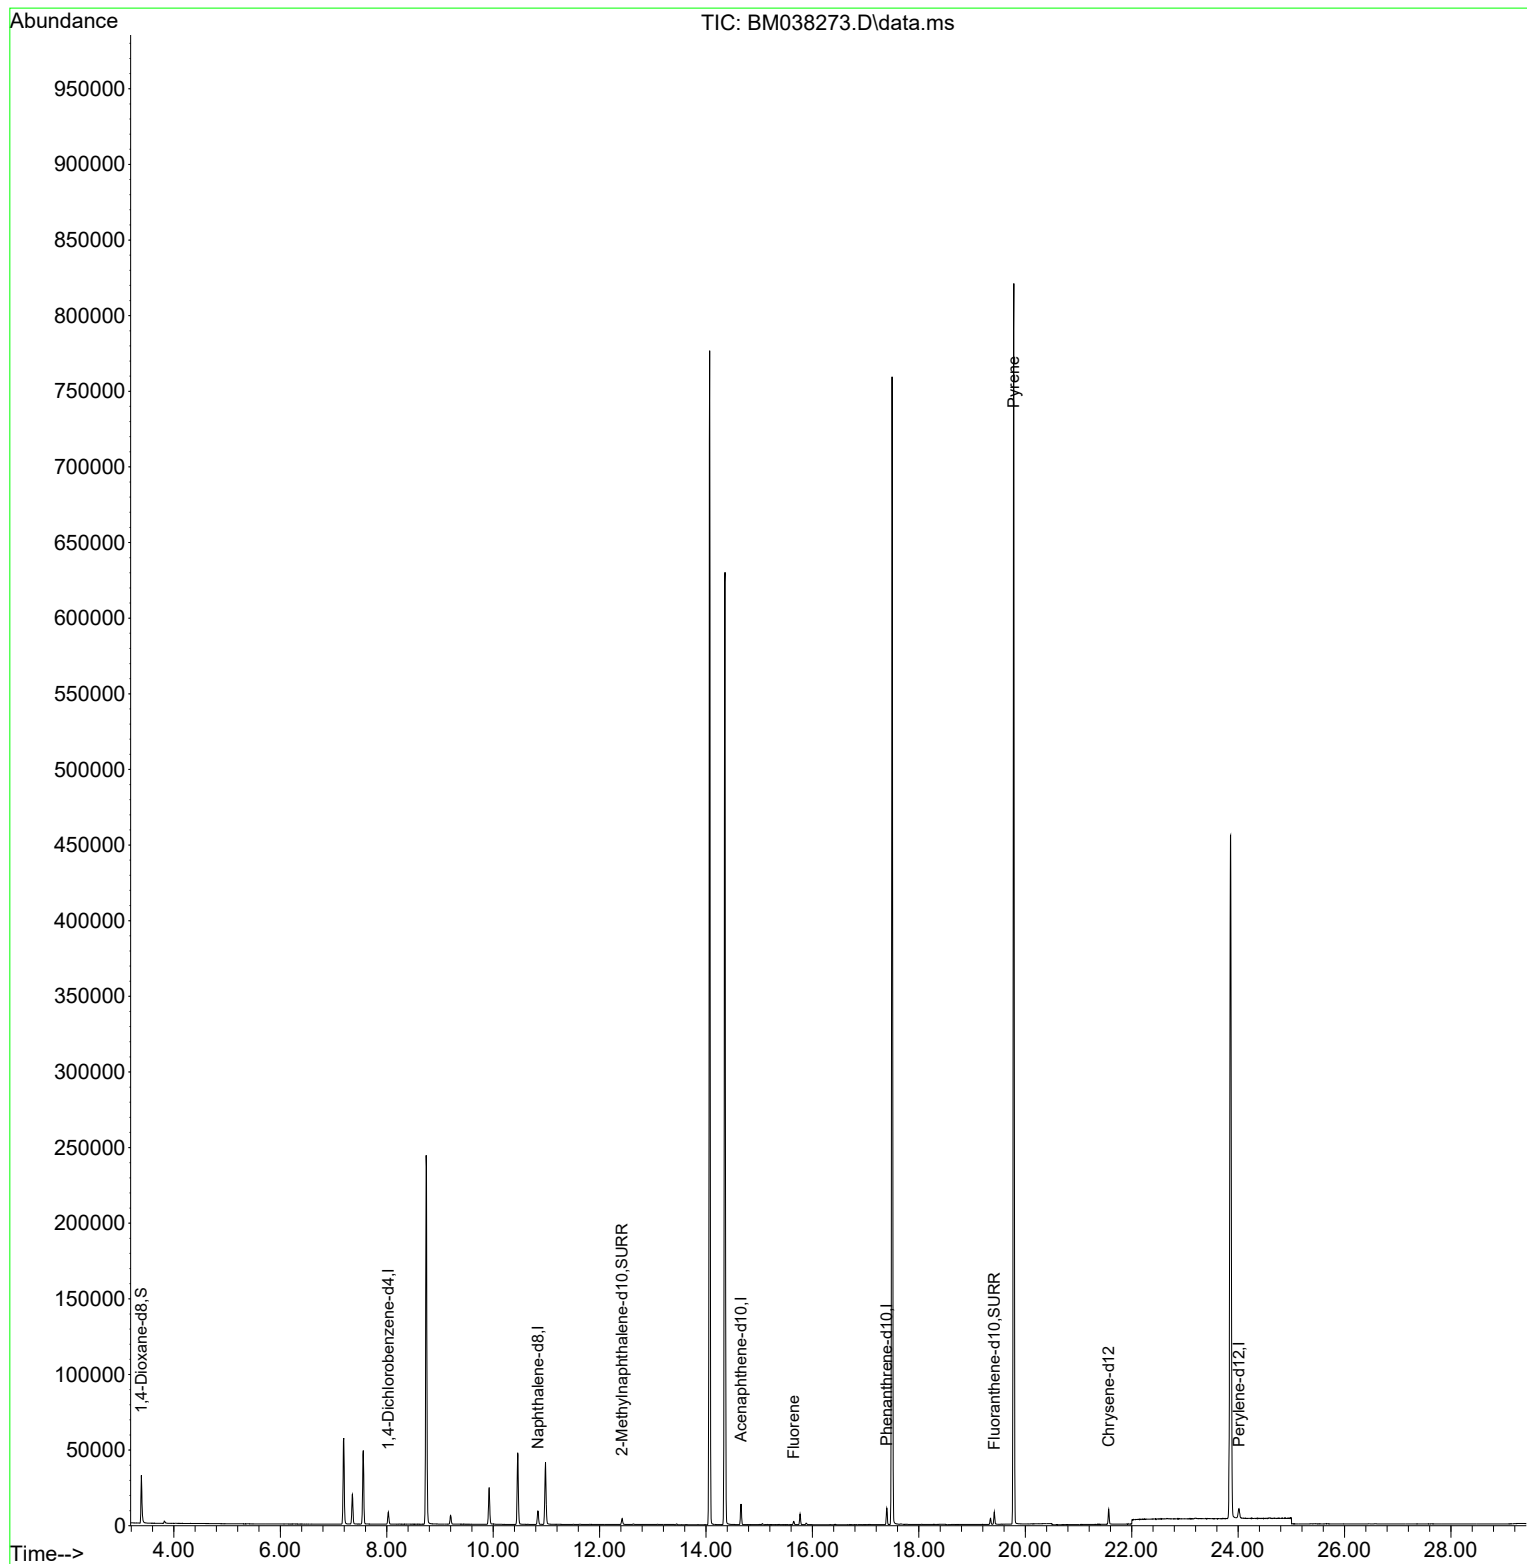



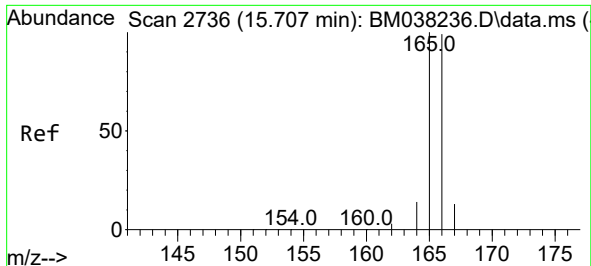


#12
Fluorene
Concen: 0.063 ng/ul
RT: 15.647 min Scan# 21
Delta R.T. -0.056 min
Lab File: BM038273.D
Acq: 24 Dec 2022 16:44

Instrument :
BNA_M
ClientSampleId :

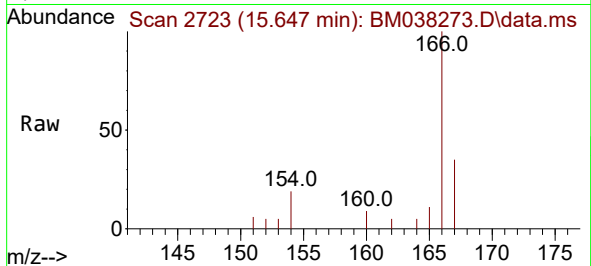

Tgt Ion:166 Resp: 1863
Ion Ratio Lower Upper
166 100
165 11.3 79.0 118.6#
167 34.7 11.0 16.6#

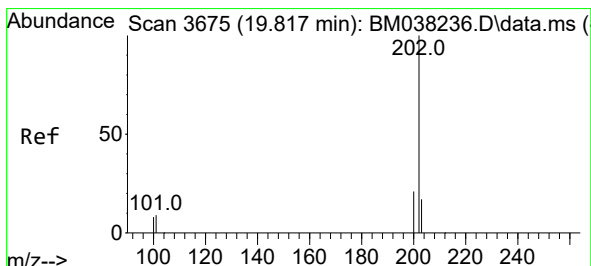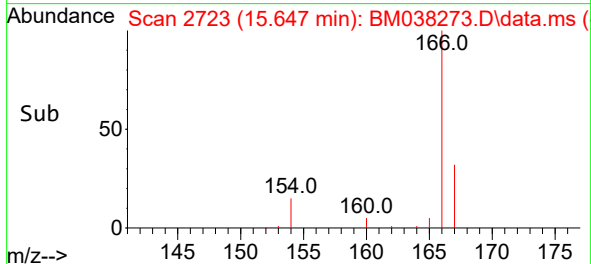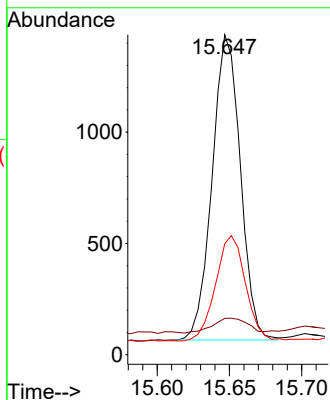

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.784 min Scan# 3668
Delta R.T. -0.028 min
Lab File: BM038273.D
Acq: 24 Dec 2022 16:44

Tgt Ion:202 Resp: 1591
Ion Ratio Lower Upper
202 100
101 132.0 8.9 13.3#
100 925.1 7.4 11.0#

