

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
 Data File : BM038274.D
 Acq On : 24 Dec 2022 17:20
 Operator : CG/JU
 Sample : N149785BL
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 25 02:56:43 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 24 05:23:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.030	152	4153	0.400	ng/ul	0.00
4) Naphthalene-d8	10.839	136	12637	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.657	164	7246	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.396	188	13327	0.400	ng/ul	0.00
17) Chrysene-d12	21.568	240	8855	0.400	ng/ul	0.00
23) Perylene-d12	24.012	264	8714	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	14195	3.360	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.423	152	3808	0.205	ng/ul	0.00
18) Fluoranthene-d10	19.417	212	6497	0.195	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.784	202	1250	0.025	ng/ul#	1
26) Benzo(a)pyrene	23.854	252	1986	0.059	ng/ul#	7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
Data File : BM038274.D
Acq On : 24 Dec 2022 17:20
Operator : CG/JU
Sample : N149785BL
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 25 02:56:43 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 24 05:23:31 2022
Response via : Initial Calibration

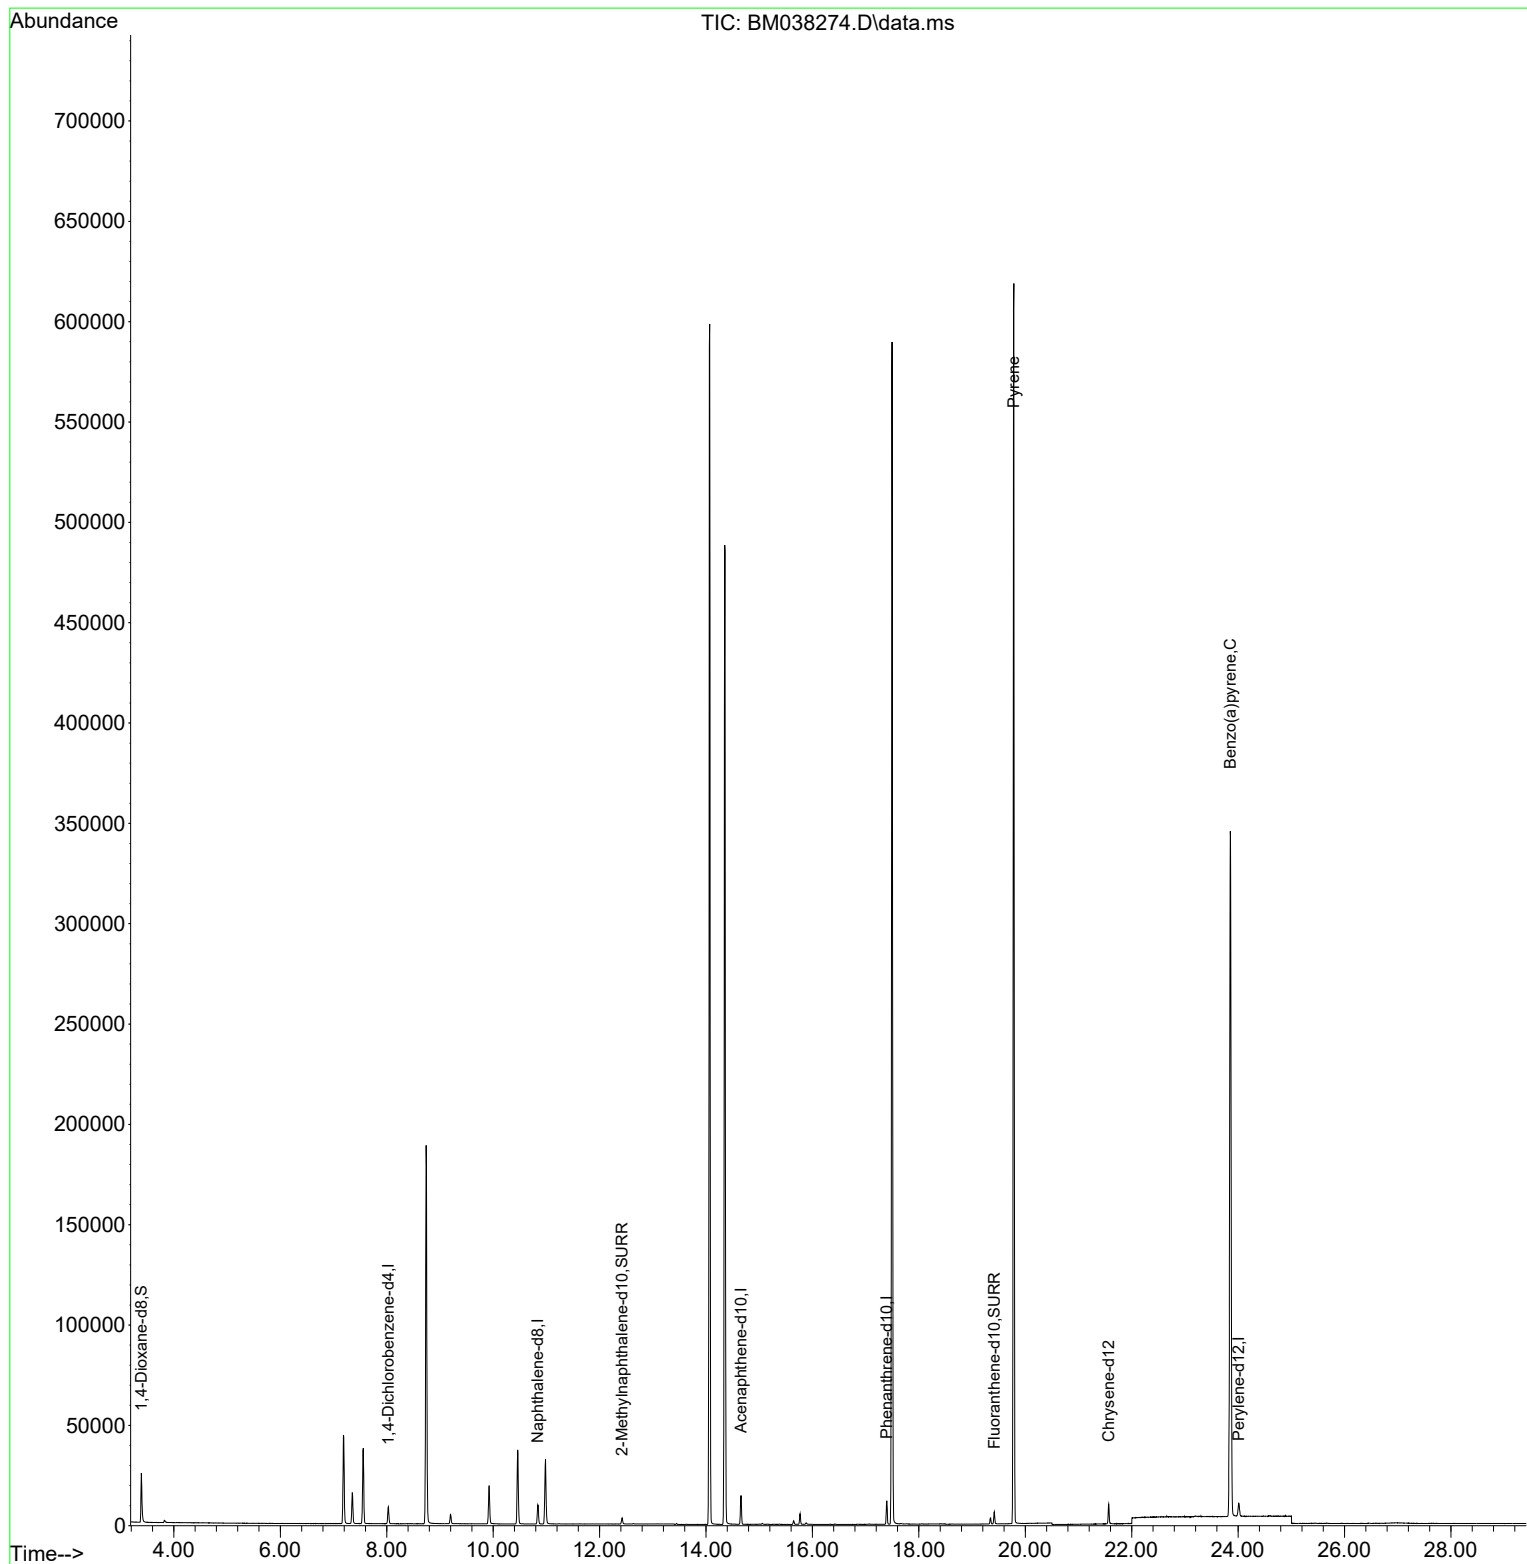

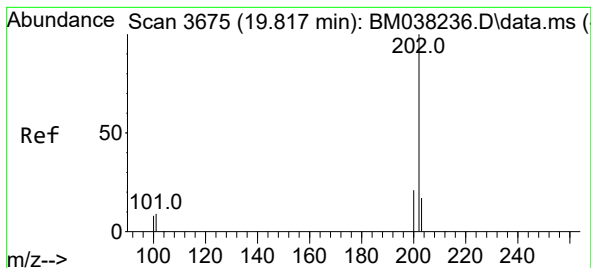

#20

Pyrene

Concen: 0.025 ng/ul

RT: 19.784 min Scan# 3

Delta R.T. -0.028 min

Lab File: BM038274.D

Acq: 24 Dec 2022 17:20

Instrument :

BNA_M

ClientSampleId :





Tgt Ion:202 Resp: 1250

Ion Ratio Lower Upper

202 100

101 138.0 8.9 13.3#

100 924.9 7.4 11.0#

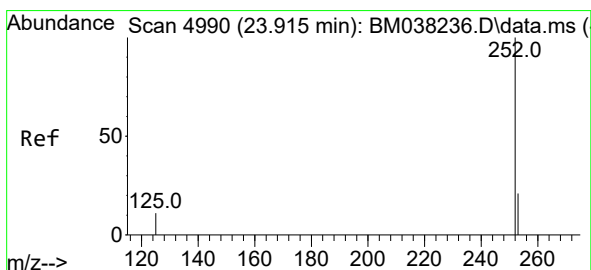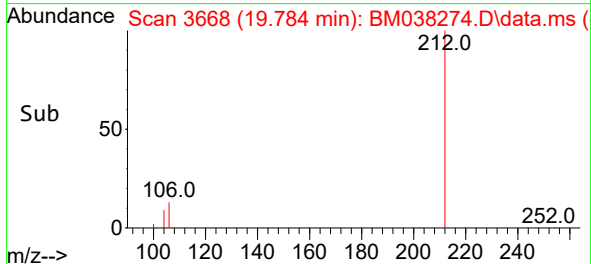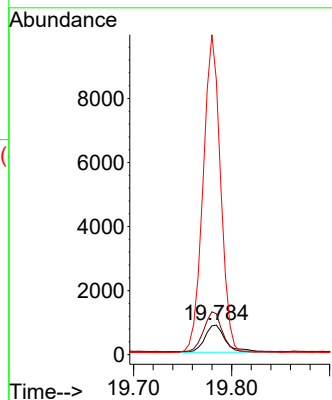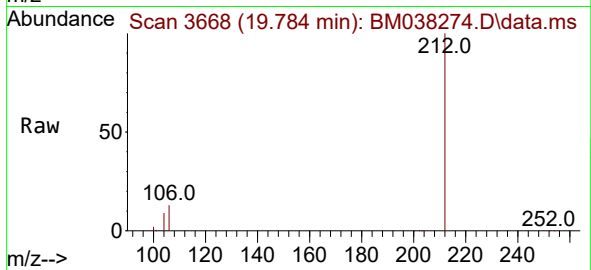

#26

Benzo(a)pyrene

Concen: 0.059 ng/ul

RT: 23.854 min Scan# 4969

Delta R.T. -0.053 min

Lab File: BM038274.D

Acq: 24 Dec 2022 17:20

Tgt Ion:252 Resp: 1986

Ion Ratio Lower Upper

252 100

253 70.5 24.2 36.4#

125 78.4 17.3 25.9#

