

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
 Data File : BM038279.D
 Acq On : 24 Dec 2022 20:20
 Operator : CG/JU
 Sample : N6016-03
 Misc :
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 25 02:57:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 24 05:23:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.030	152	4202	0.400	ng/ul	0.00
4) Naphthalene-d8	10.840	136	12247	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.657	164	6634	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.396	188	11634	0.400	ng/ul	0.00
17) Chrysene-d12	21.565	240	8194	0.400	ng/ul	0.00
23) Perylene-d12	24.012	264	8167	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	12242	2.864	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.423	152	3348	0.186	ng/ul	0.00
18) Fluoranthene-d10	19.417	212	5532	0.180	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.889	128	3648	0.102	ng/ul	95
7) 2-Methylnaphthalene	12.495	142	1036	0.046	ng/ul	93
8) 1-Methylnaphthalene	12.709	142	680	0.030	ng/ul	98
10) Acenaphthylene	14.379	152	6559	0.179	ng/ul	96
11) Acenaphthene	14.717	153	3145	0.120	ng/ul	98
12) Fluorene	15.702	166	2663	0.094	ng/ul#	98
15) Phenanthrene	17.438	178	46196	1.186	ng/ul	99
16) Anthracene	17.527	178	13481	0.361	ng/ul	98
19) Fluoranthene	19.445	202	116448	2.594	ng/ul	98
20) Pyrene	19.808	202	100878	2.224	ng/ul	97
21) Benzo(a)anthracene	21.547	228	78023	2.171	ng/ul	98
22) Chrysene	21.603	228	84439	2.414	ng/ul	98
24) Benzo(b)fluoranthene	23.263	252	152496	4.218	ng/ul	88
26) Benzo(a)pyrene	23.903	252	103654	3.286	ng/ul#	84
27) Indeno(1,2,3-cd)pyrene	26.562	276	82217	1.879	ng/ul#	89
28) Dibenzo(a,h)anthracene	26.575	278	21559	0.634	ng/ul	98
29) Benzo(g,h,i)perylene	27.360	276	74657	2.028	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
Data File : BM038279.D
Acq On : 24 Dec 2022 20:20
Operator : CG/JU
Sample : N6016-03
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Dec 25 02:57:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 24 05:23:31 2022
Response via : Initial Calibration

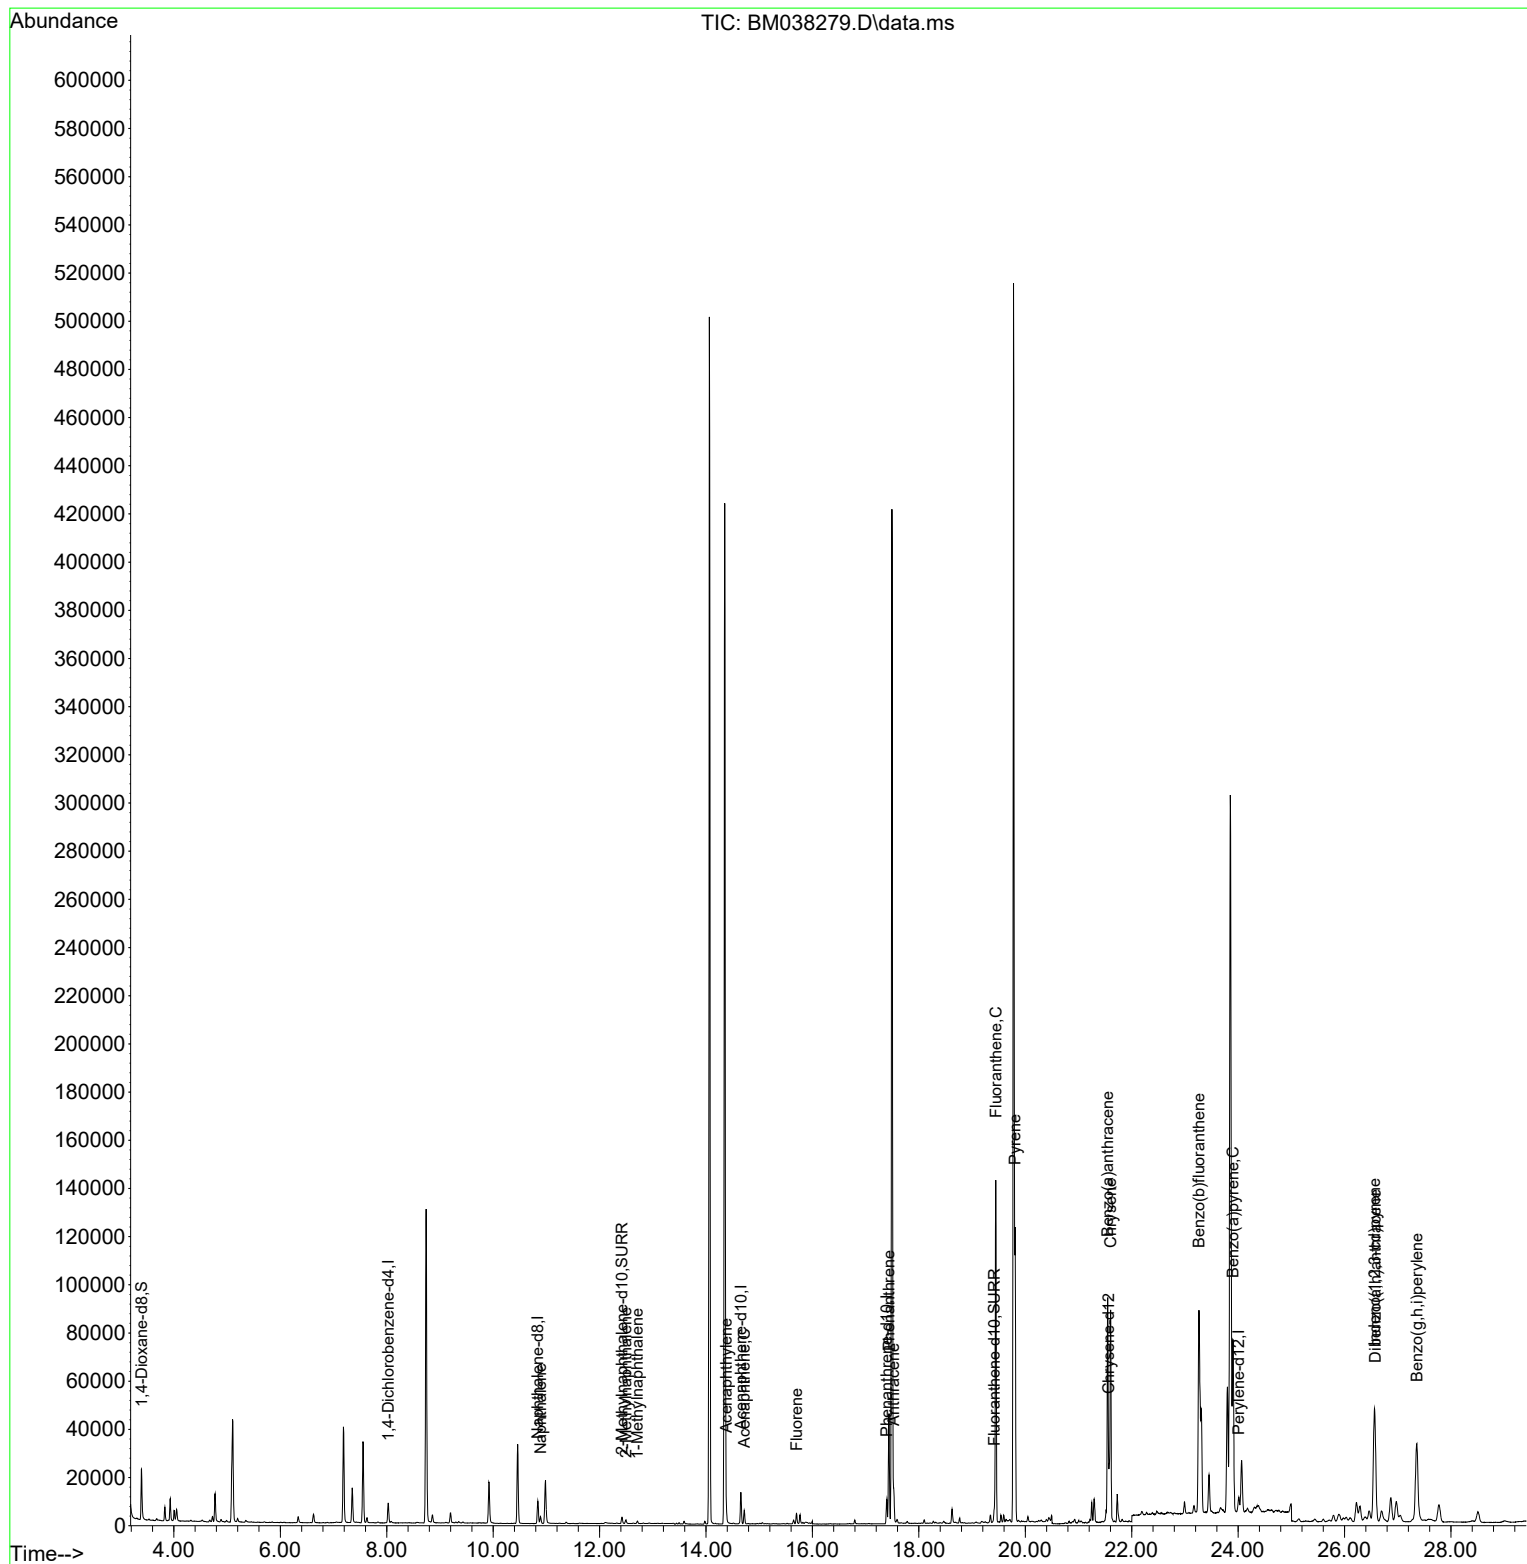



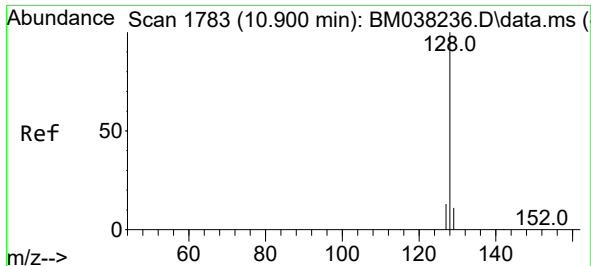


#5
Naphthalene
Concen: 0.102 ng/ul
RT: 10.889 min Scan# 1781
Delta R.T. -0.005 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20


Instrument :
BNA_M
ClientSampleId :





Tgt Ion:128 Resp: 3648
Ion Ratio Lower Upper
128 100
129 13.7 9.4 14.0
127 15.2 10.7 16.1

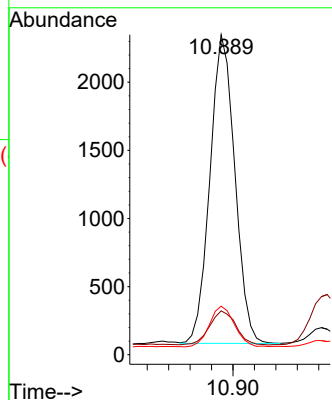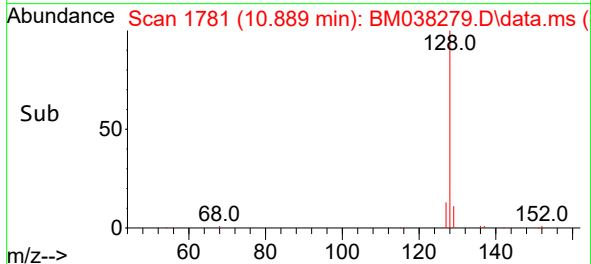


#7
2-Methylnaphthalene
Concen: 0.046 ng/ul
RT: 12.495 min Scan# 2073
Delta R.T. 0.000 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20

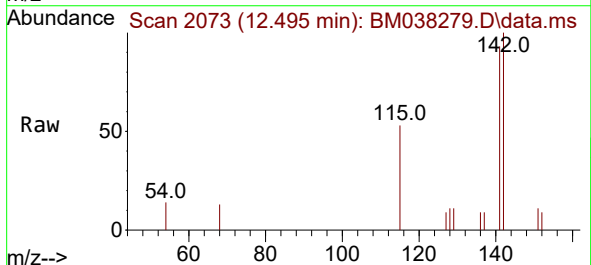

Tgt Ion:142 Resp: 1036
Ion Ratio Lower Upper
142 100
141 96.0 71.9 107.9



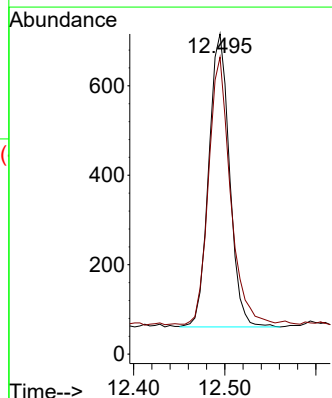
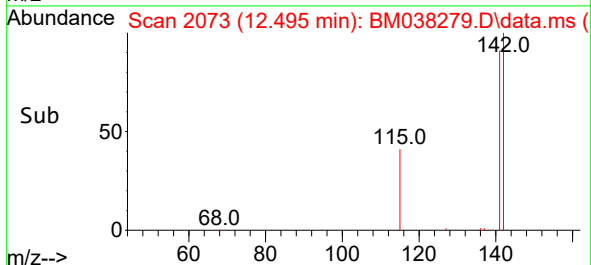


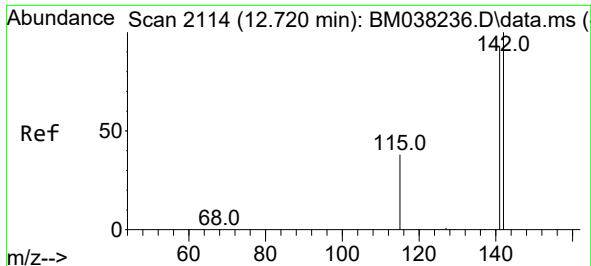

#8
1-Methylnaphthalene
Concen: 0.030 ng/ul
RT: 12.709 min Scan# 2112
Delta R.T. -0.005 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:142 Resp: 680
Ion Ratio Lower Upper
142 100
141 91.2 74.7 112.1

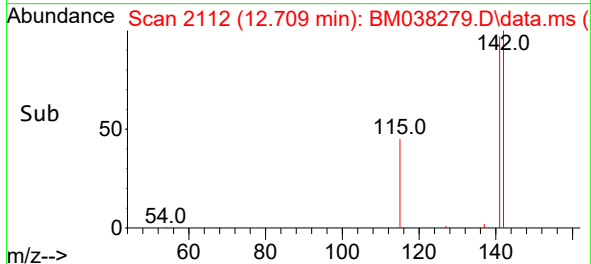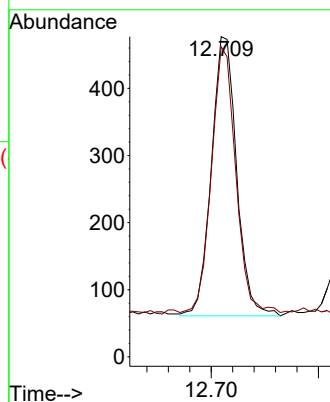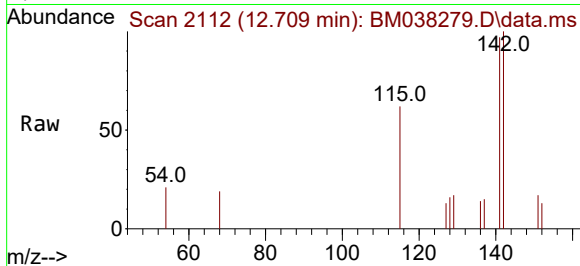

#10
Acenaphthylene
Concen: 0.179 ng/ul
RT: 14.379 min Scan# 2449
Delta R.T. 0.000 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20

Tgt Ion:152 Resp: 6559
Ion Ratio Lower Upper
152 100
151 21.8 16.2 24.2
153 15.2 10.7 16.1


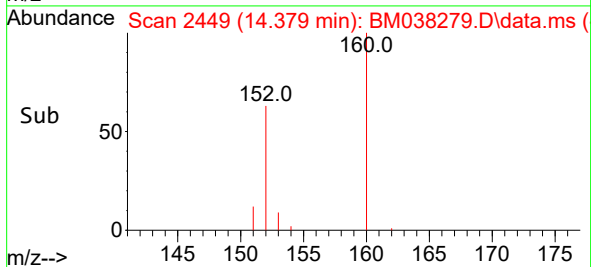
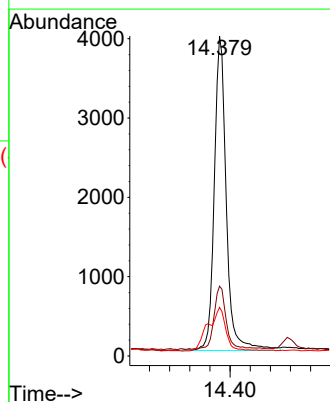
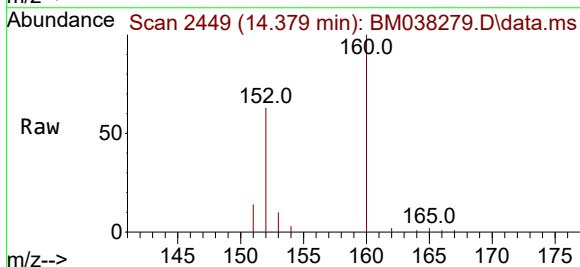


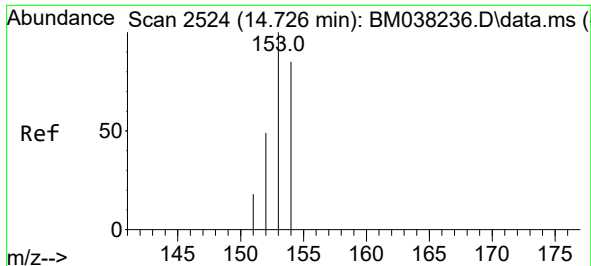

#11
Acenaphthene
Concen: 0.120 ng/ul
RT: 14.717 min Scan# 21
Delta R.T. -0.005 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:153 Resp: 3145
Ion Ratio Lower Upper
153 100
152 51.6 39.4 59.0
154 84.6 69.0 103.4

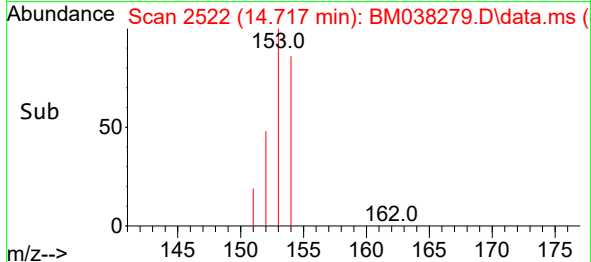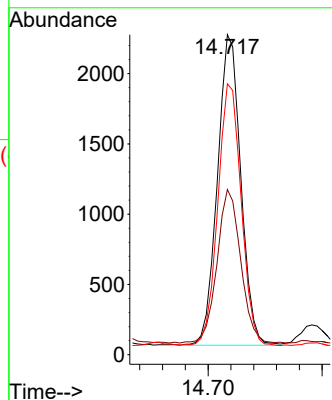

#12
Fluorene
Concen: 0.094 ng/ul
RT: 15.702 min Scan# 2735
Delta R.T. 0.000 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20


Tgt Ion:166 Resp: 2663
Ion Ratio Lower Upper
166 100
165 99.5 79.0 118.6
167 17.6 11.0 16.6#

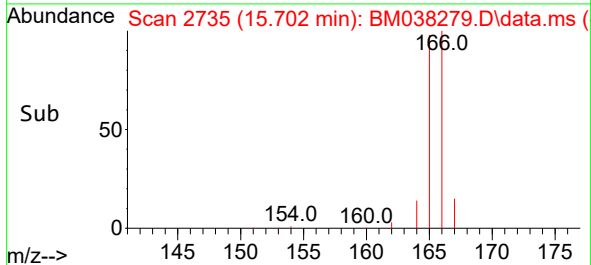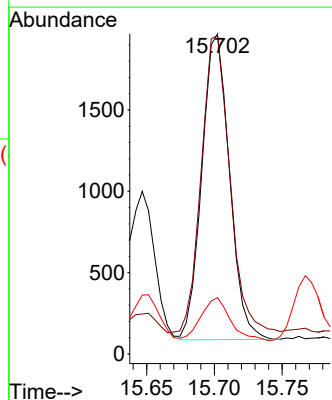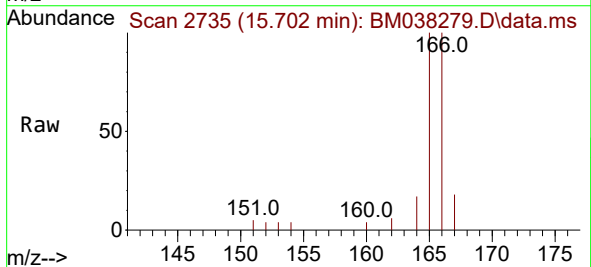



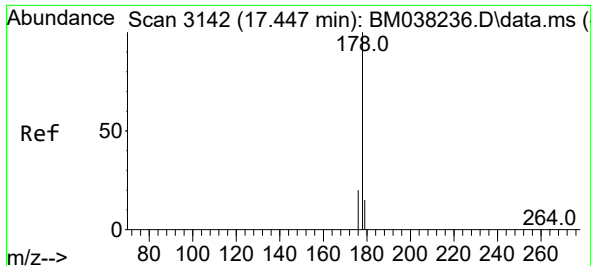


#15
Phenanthrene
Concen: 1.186 ng/ul
RT: 17.438 min Scan# 3140
Delta R.T. 0.000 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20

Instrument :
BNA_M
ClientSampleId :







Tgt Ion:178 Resp: 46196
Ion Ratio Lower Upper
178 100
179 15.5 13.0 19.4
176 20.1 16.2 24.4

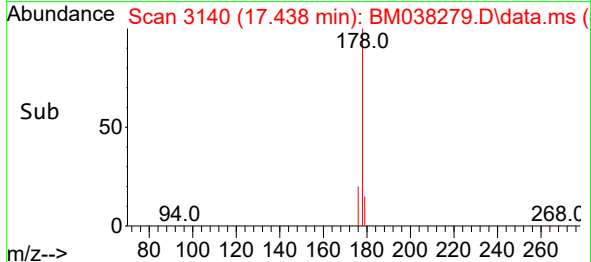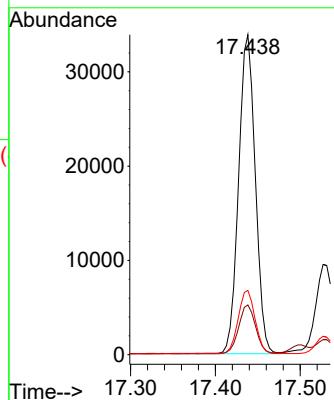

#16
Anthracene
Concen: 0.361 ng/ul
RT: 17.527 min Scan# 3161
Delta R.T. -0.004 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20

Tgt Ion:178 Resp: 13481
Ion Ratio Lower Upper
178 100
179 16.7 13.0 19.6
176 20.4 15.6 23.4


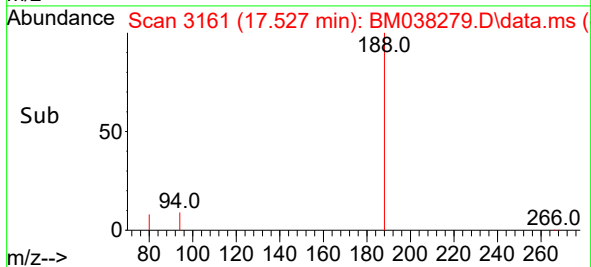
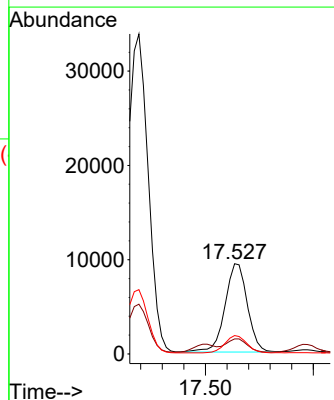
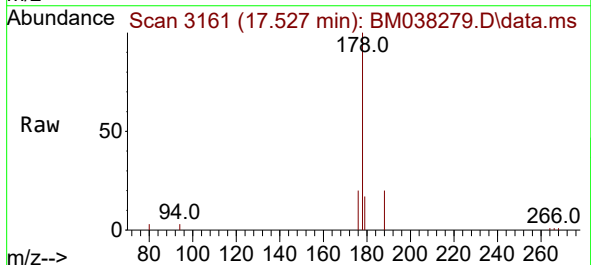


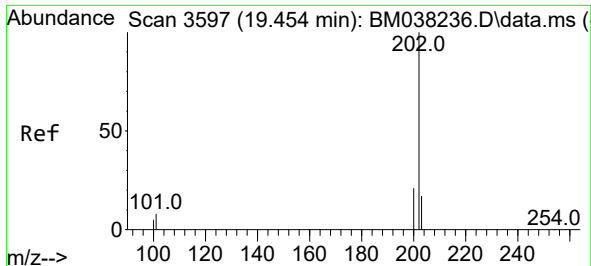

#19
Fluoranthene
Concen: 2.594 ng/ul
RT: 19.445 min Scan# 31
Delta R.T. -0.005 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:202 Resp: 116448
Ion Ratio Lower Upper
202 100
101 8.3 7.5 11.3
100 6.6 5.6 8.4

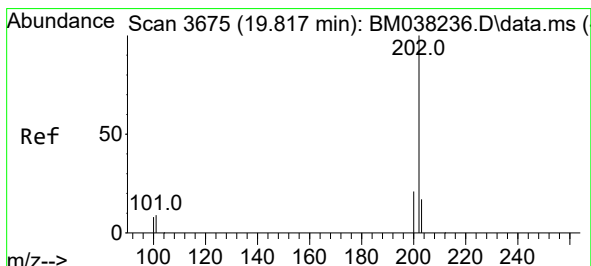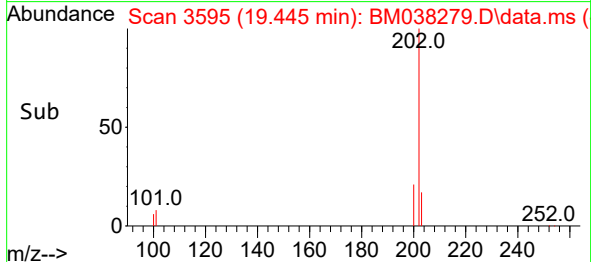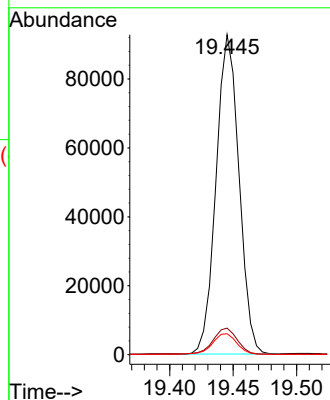

#20
Pyrene
Concen: 2.224 ng/ul
RT: 19.808 min Scan# 3673
Delta R.T. -0.005 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20

Tgt Ion:202 Resp: 100878
Ion Ratio Lower Upper
202 100
101 9.8 8.9 13.3
100 8.2 7.4 11.0

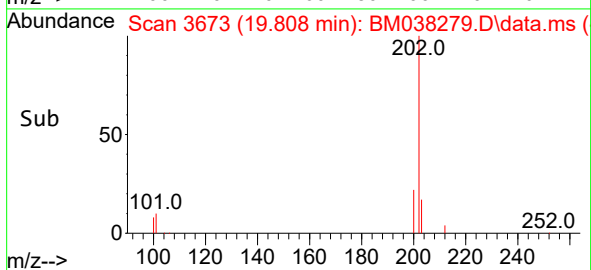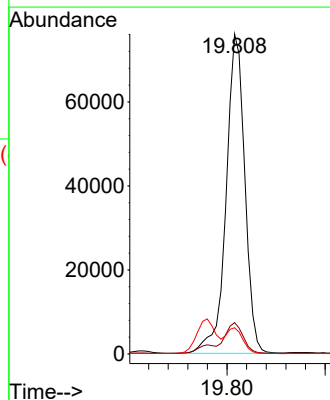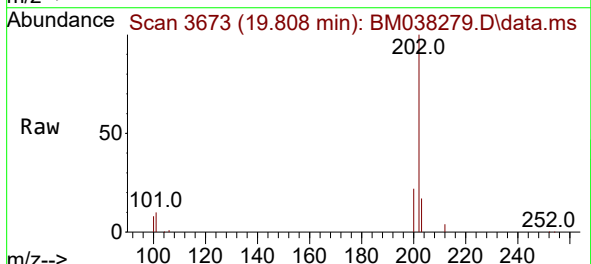



#21

Benzo(a)anthracene

Concen: 2.171 ng/ul

RT: 21.547 min Scan# 41

Delta R.T. -0.003 min


Lab File: BM038279.D

Acq: 24 Dec 2022 20:20

Instrument :

BNA_M

ClientSampleId :

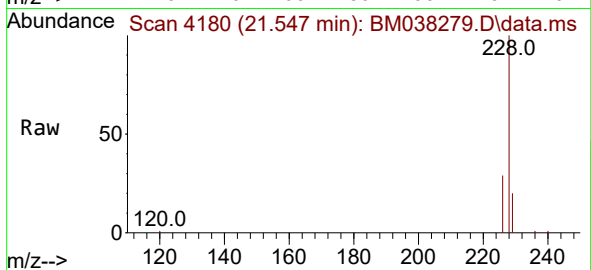




Tgt Ion:228 Resp: 78023

Ion Ratio Lower Upper

228 100

229 20.2 15.5 23.3

226 29.0 22.2 33.2

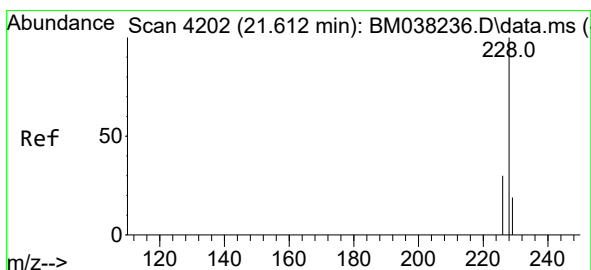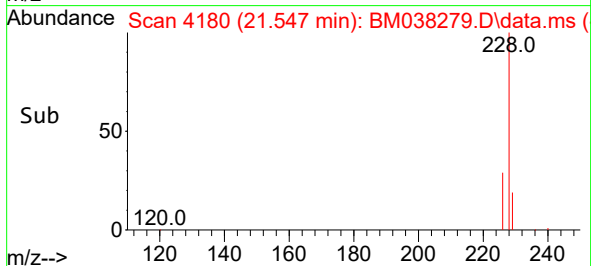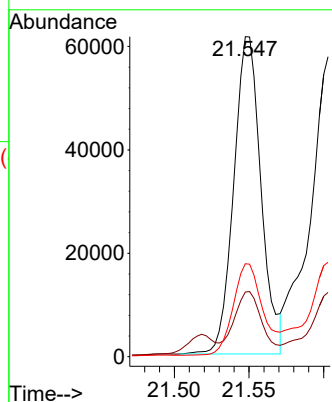

#22

Chrysene

Concen: 2.414 ng/ul

RT: 21.603 min Scan# 4199

Delta R.T. -0.003 min

Lab File: BM038279.D

Acq: 24 Dec 2022 20:20




Tgt Ion:228 Resp: 84439


Ion Ratio Lower Upper

228 100

226 31.5 25.0 37.4


229 21.4 16.0 24.0

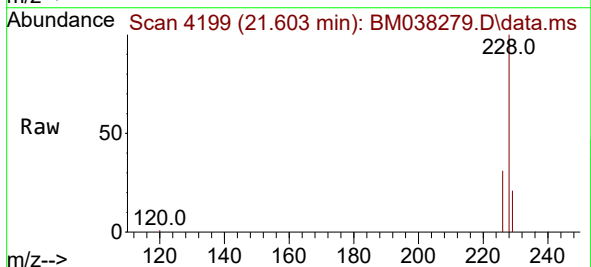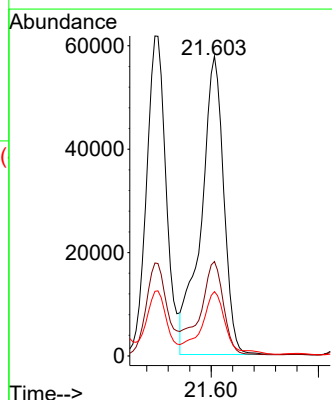






#24
Benzo(b)fluoranthene
Concen: 4.218 ng/ul
RT: 23.263 min Scan# 41
Delta R.T. -0.003 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20

Instrument :
BNA_M
ClientSampleId :







Tgt Ion:252 Resp: 152496
Ion Ratio Lower Upper
252 100
253 23.2 0.0 56.0
125 11.4 0.0 36.6

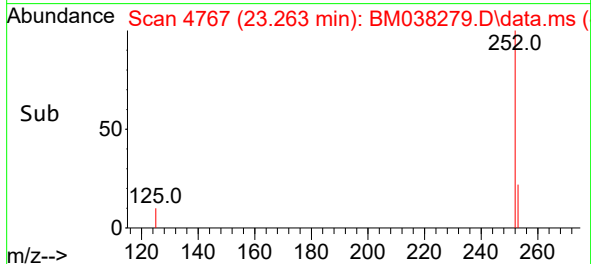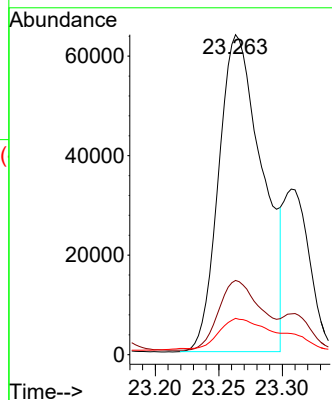

#26
Benzo(a)pyrene
Concen: 3.286 ng/ul
RT: 23.903 min Scan# 4986
Delta R.T. -0.003 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20

Tgt Ion:252 Resp: 103654
Ion Ratio Lower Upper
252 100
253 23.4 24.2 36.4#
125 12.0 17.3 25.9#

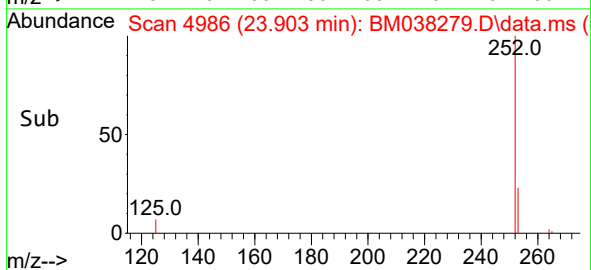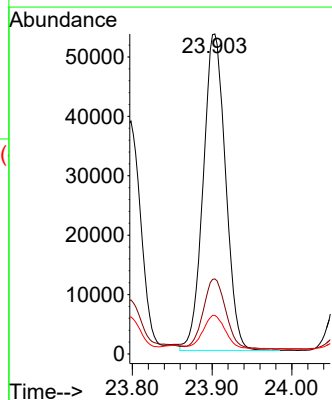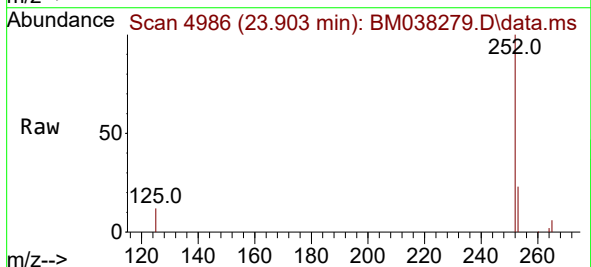

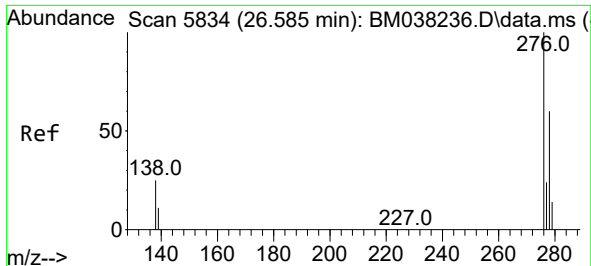

#27

Indeno(1,2,3-cd)pyrene

Concen: 1.879 ng/ul

RT: 26.562 min Scan# 5827

Delta R.T. -0.007 min

Lab File: BM038279.D

Acq: 24 Dec 2022 20:20

Instrument :

BNA_M

ClientSampleId :





Tgt Ion:276 Resp: 82217

Ion Ratio Lower Upper

276 100

138 21.1 21.7 32.5#

227 0.0 0.0 0.0

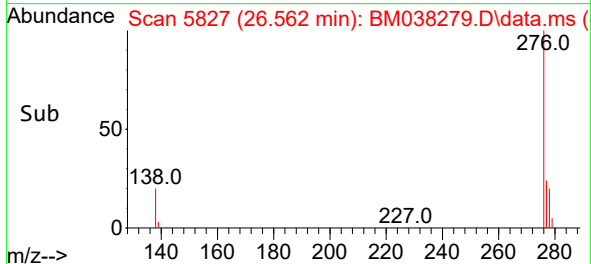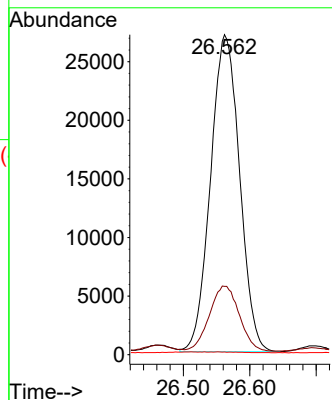

#28

Dibenzo(a,h)anthracene

Concen: 0.634 ng/ul

RT: 26.575 min Scan# 5831

Delta R.T. -0.013 min

Lab File: BM038279.D

Acq: 24 Dec 2022 20:20




Tgt Ion:278 Resp: 21559


Ion Ratio Lower Upper

278 100

139 19.8 16.8 25.2


279 30.5 23.4 35.2

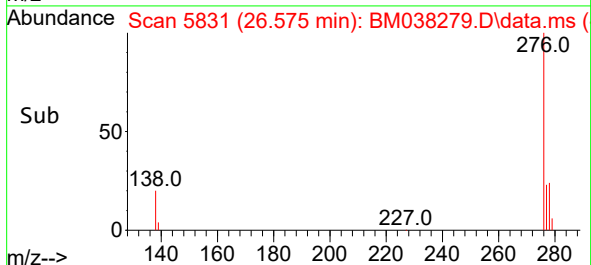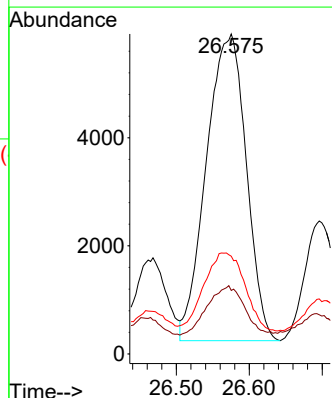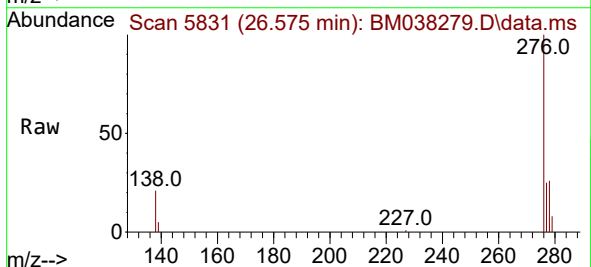



#29
Benzo(g,h,i)perylene
Concen: 2.028 ng/ul
RT: 27.360 min Scan# 6070
Delta R.T. 0.000 min
Lab File: BM038279.D
Acq: 24 Dec 2022 20:20

Instrument :
BNA_M
ClientSampleId :

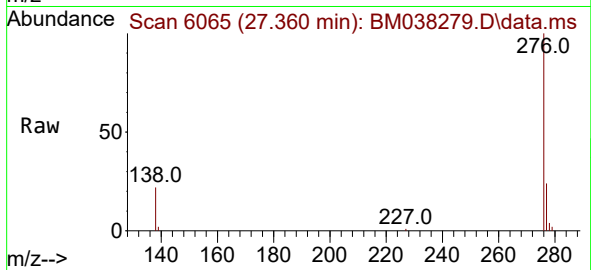

Tgt Ion:276 Resp: 74657
Ion Ratio Lower Upper
276 100
138 21.6 20.8 31.2
277 23.9 20.5 30.7

