

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
 Data File : BM038307.D
 Acq On : 25 Dec 2022 14:32
 Operator : CG/JU
 Sample : PB149813BL
 Misc :
 ALS Vial : 116 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 25 23:56:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 24 05:23:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.021	152	3252	0.400	ng/ul	0.00
4) Naphthalene-d8	10.834	136	10320	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.652	164	6046	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	12036	0.400	ng/ul	0.00
17) Chrysene-d12	21.568	240	7850	0.400	ng/ul	0.00
23) Perylene-d12	24.014	264	8100	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.385	96	13814	4.176	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.418	152	3821	0.252	ng/ul	0.00
18) Fluoranthene-d10	19.413	212	7164	0.243	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.423	88	85	0.026	ng/ul#	54
20) Pyrene	19.780	202	1416	0.033	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

BNA_M

ClientSampleId :


Quant Time: Dec 25 23:56:02 2022


Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Dec 24 05:23:31 2022


Response via : Initial Calibration





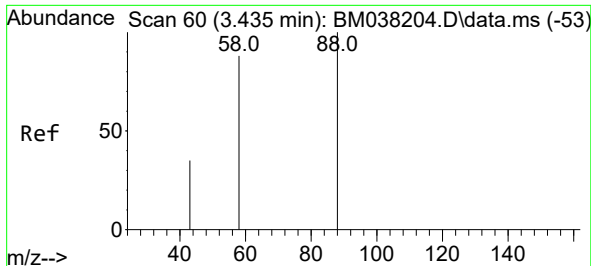


#2
1,4-Dioxane
Concen: 0.026 ng/ul
RT: 3.423 min Scan# 51
Delta R.T. -0.008 min
Lab File: BM038307.D
Acq: 25 Dec 2022 14:32


Instrument :
BNA_M
ClientSampleId :

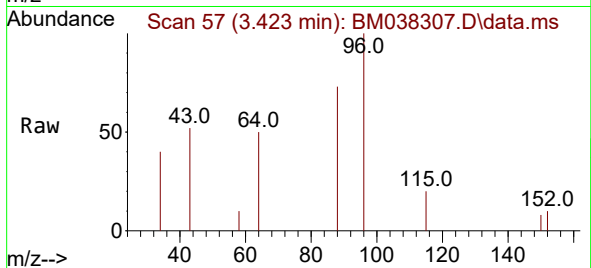

Tgt Ion: 88 Resp: 85
Ion Ratio Lower Upper
88 100
43 70.4 46.4 69.6#
58 13.9 56.9 85.3#

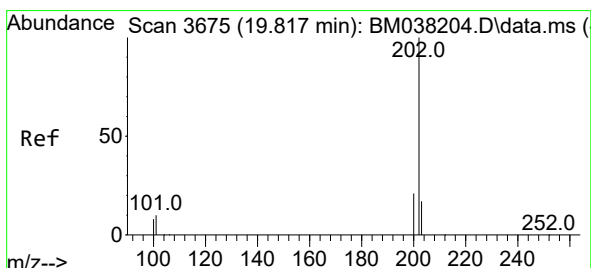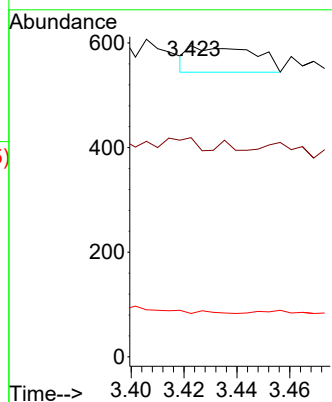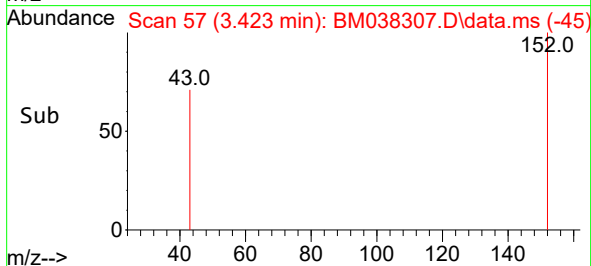

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.780 min Scan# 3667
Delta R.T. -0.033 min
Lab File: BM038307.D
Acq: 25 Dec 2022 14:32

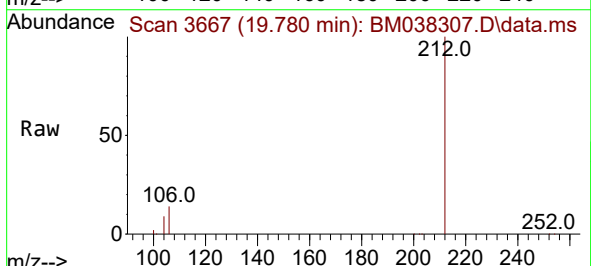

Tgt Ion: 202 Resp: 1416
Ion Ratio Lower Upper
202 100
101 147.6 8.9 13.3#
100 1088.1 7.4 11.0#

