

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
 Data File : BM038210.D
 Acq On : 22 Dec 2022 22:32
 Operator : CG/JU
 Sample : N6009-01DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBYG7DL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2022
 Supervised By :mohammad ahmed 12/23/2022

Quant Time: Dec 23 01:49:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 23:36:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.043	152	4508	0.400	ng/ul	0.00
4) Naphthalene-d8	10.856	136	14126	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.666	164	7837	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.405	188	15615	0.400	ng/ul	0.00
17) Chrysene-d12	21.574	240	9999	0.400	ng/ul	0.00
23) Perylene-d12	24.023	264	9848	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.398	96	4450	0.970	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	1336	0.064	ng/ul	0.00
18) Fluoranthene-d10	19.422	212	2652	0.071	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.906	128	5363	0.130	ng/ul	97
7) 2-Methylnaphthalene	12.506	142	1003	0.039	ng/ul	97
10) Acenaphthylene	14.388	152	5056	0.117	ng/ul	96
15) Phenanthrene	17.447	178	10538	0.202	ng/ul	99
16) Anthracene	17.540	178	3398	0.068	ng/ul#	92
19) Fluoranthene	19.455	202	31889	0.582	ng/ul	100
20) Pyrene	19.817	202	25628m	0.463	ng/ul	
21) Benzo(a)anthracene	21.556	228	17329	0.395	ng/ul	95
22) Chrysene	21.609	228	17787	0.417	ng/ul	98
24) Benzo(b)fluoranthene	23.272	252	26789	0.615	ng/ul	99
25) Benzo(k)fluoranthene	23.316	252	8319m	0.199	ng/ul	
26) Benzo(a)pyrene	23.912	252	15381	0.404	ng/ul	99
27) Indeno(1,2,3-cd)pyrene	26.579	276	12924	0.245	ng/ul#	91
28) Dibenzo(a,h)anthracene	26.585	278	3250	0.079	ng/ul#	49
29) Benzo(g,h,i)perylene	27.370	276	11727	0.264	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
Data File : BM038210.D
Acq On : 22 Dec 2022 22:32
Operator : CG/JU
Sample : N6009-01DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DBYG7DL

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2022
Supervised By :mohammad ahmed 12/23/2022


Quant Time: Dec 23 01:49:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 23:36:45 2022
Response via : Initial Calibration

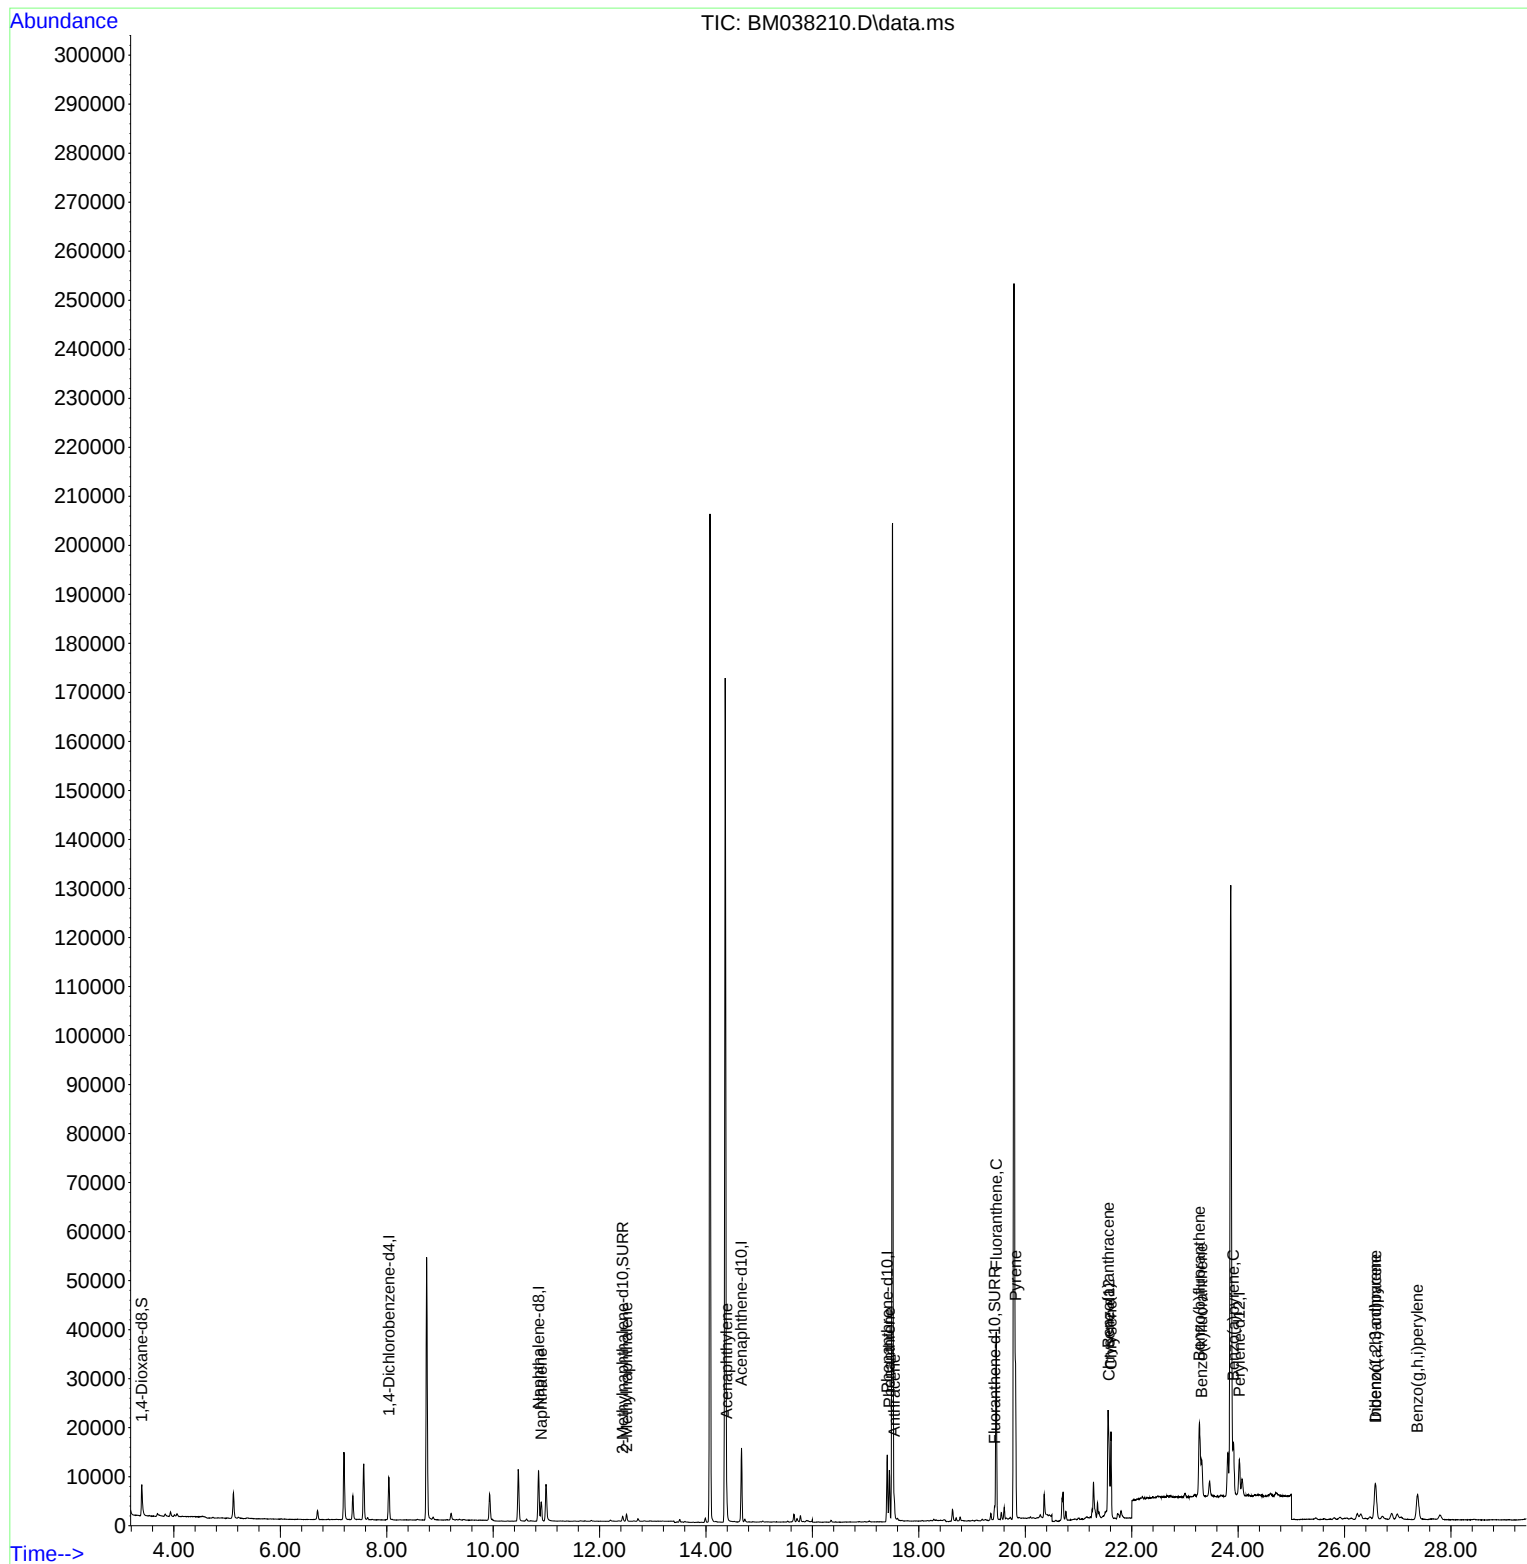



#5
Naphthalene
Concen: 0.130 ng/ul
RT: 10.906 min Scan# 1784
Delta R.T. 0.000 min
Lab File: BM038210.D
Acq: 22 Dec 2022 22:32




Instrument :
BNA_M
ClientSampleId :
DBYG7DL

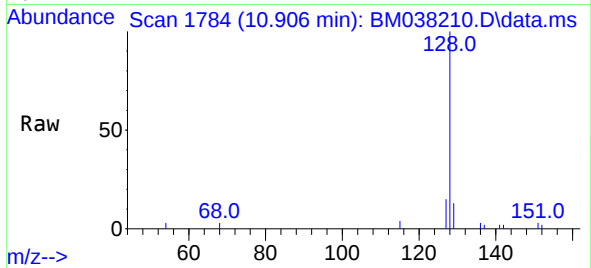


Tgt Ion:128 Resp: 536
Ion Ratio Lower Upper
128 100
129 13.1 9.4 14.0
127 14.6 10.7 16.1

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/23/2022
Supervised By :mohammad ahmed 12/23/2022

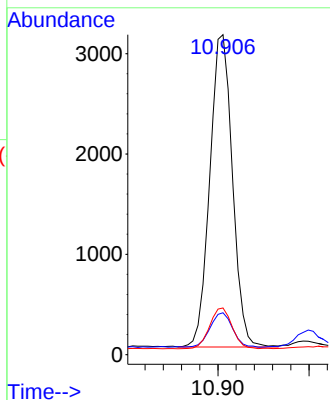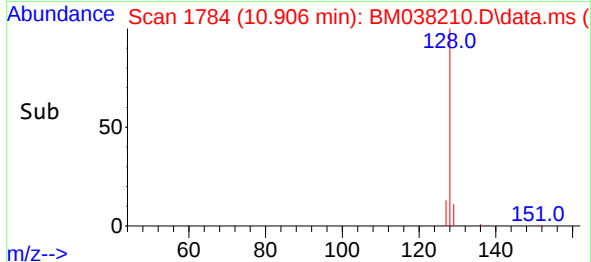


#7
2-Methylnaphthalene
Concen: 0.039 ng/ul
RT: 12.506 min Scan# 2075
Delta R.T. 0.000 min
Lab File: BM038210.D
Acq: 22 Dec 2022 22:32

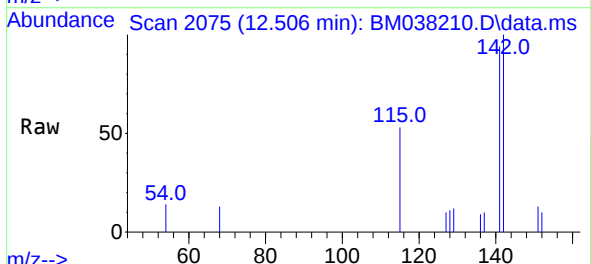


Tgt Ion:142 Resp: 1003
Ion Ratio Lower Upper
142 100
141 92.4 71.9 107.9

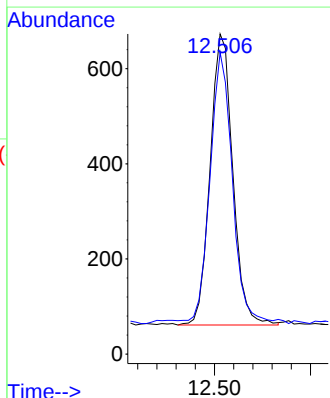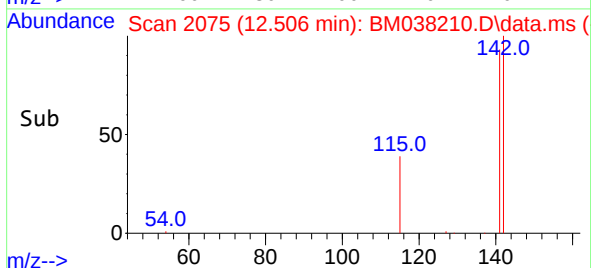



#10
Acenaphthylene
Concen: 0.117 ng/ul
RT: 14.388 min Scan# 2451
Delta R.T. 0.000 min
Lab File: BM038210.D
Acq: 22 Dec 2022 22:32




Instrument :
BNA_M
ClientSampleId :
DBYG7DL

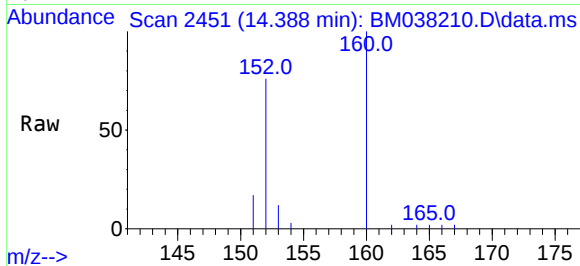


Tgt Ion:152 Resp: 5050
Ion Ratio Lower Upper
152 100
151 22.1 16.2 24.2
153 15.3 10.7 16.1

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/23/2022
Supervised By :mohammad ahmed 12/23/2022

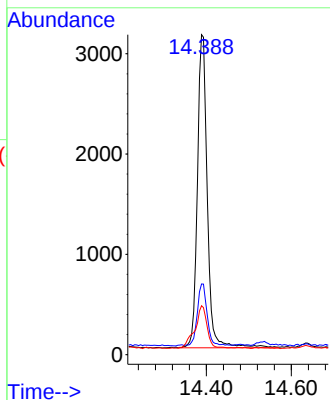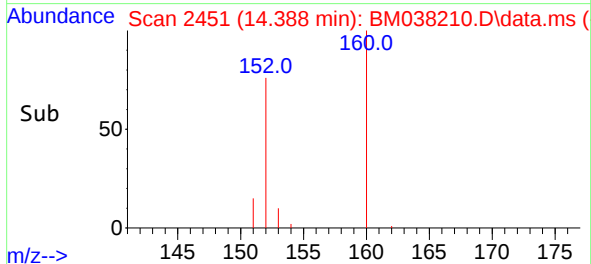


#15
Phenanthrene
Concen: 0.202 ng/ul
RT: 17.447 min Scan# 3142
Delta R.T. 0.000 min
Lab File: BM038210.D
Acq: 22 Dec 2022 22:32

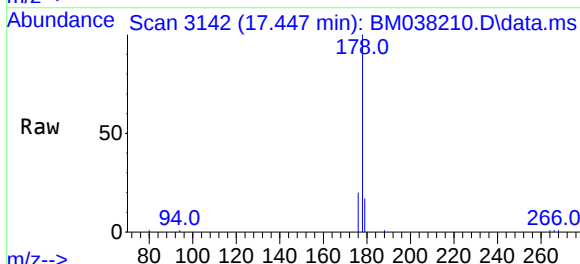


Tgt Ion:178 Resp: 10538
Ion Ratio Lower Upper
178 100
179 17.0 13.0 19.4
176 20.4 16.2 24.4

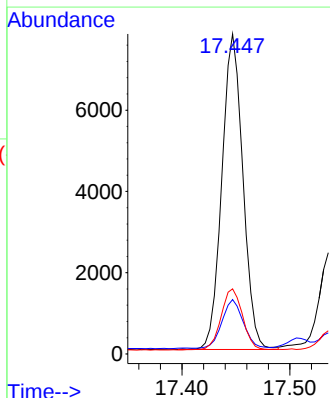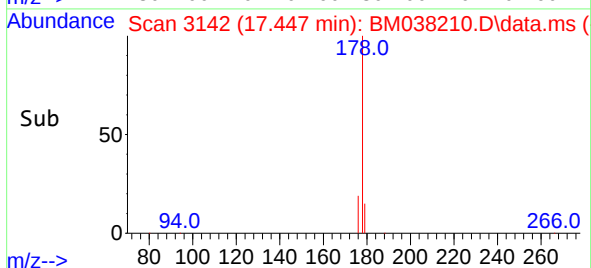



#16
 Anthracene
 Concen: 0.068 ng/ul
 RT: 17.540 min Scan# 3164
 Delta R.T. 0.000 min
 Lab File: BM038210.D
 Acq: 22 Dec 2022 22:32




Instrument :
 BNA_M
 ClientSampleId :
 DBYG7DL




Tgt Ion:178 Resp: 3398
 Ion Ratio Lower Upper
 178 100
 179 21.1 13.0 19.6
 176 22.0 15.6 23.4

Manual Integrations
 APPROVED



Reviewed By :Jagrut Upadhyay 12/23/2022
 Supervised By :mohammad ahmed 12/23/2022

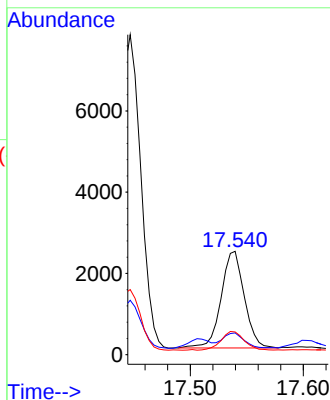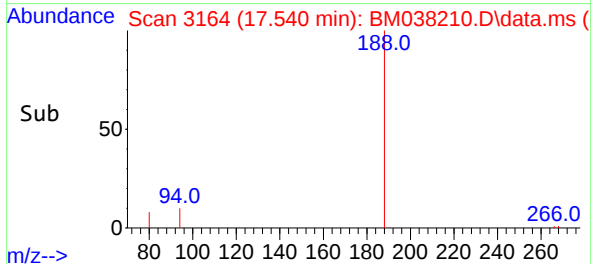


#19
 Fluoranthene
 Concen: 0.582 ng/ul
 RT: 19.455 min Scan# 3597
 Delta R.T. 0.000 min
 Lab File: BM038210.D
 Acq: 22 Dec 2022 22:32

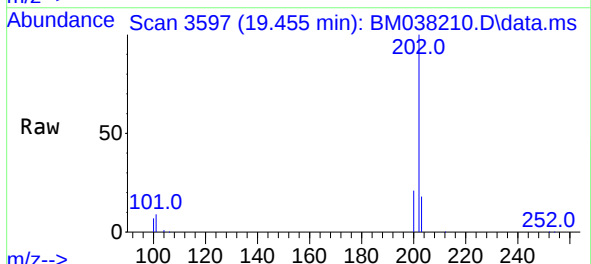


Tgt Ion:202 Resp: 31889
 Ion Ratio Lower Upper
 202 100
 101 9.2 7.5 11.3
 100 6.9 5.6 8.4

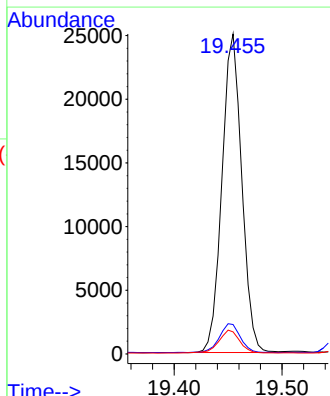



#20
Pyrene
Concen: 0.463 ng/ul m
RT: 19.817 min Scan# 3675
Delta R.T. 0.000 min
Lab File: BM038210.D
Acq: 22 Dec 2022 22:32




Instrument :
BNA_M
ClientSampleId :
DBYG7DL

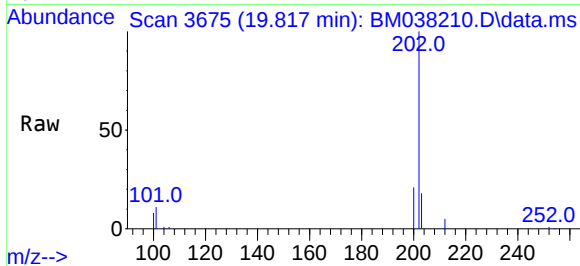


Tgt Ion:202 Resp: 25628
Ion Ratio Lower Upper
202 100
101 10.7 8.9 13.3
100 8.4 7.4 11.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/23/2022
Supervised By :mohammad ahmed 12/23/2022

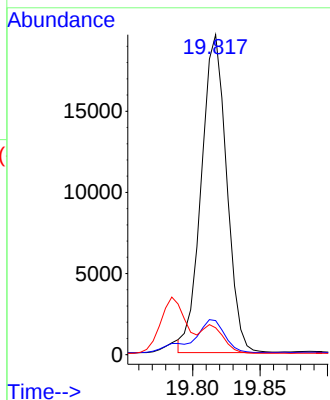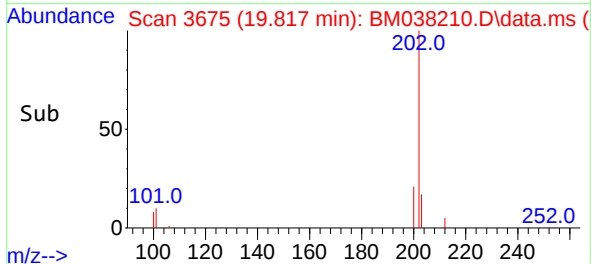


#21
Benzo(a)anthracene
Concen: 0.395 ng/ul
RT: 21.556 min Scan# 4183
Delta R.T. -0.003 min
Lab File: BM038210.D
Acq: 22 Dec 2022 22:32

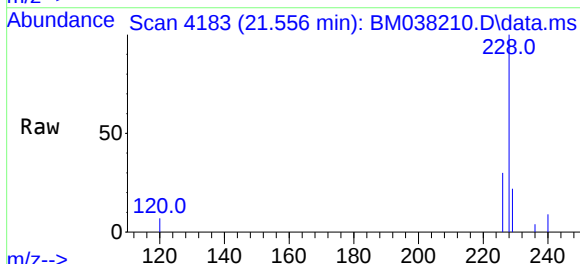


Tgt Ion:228 Resp: 17329
Ion Ratio Lower Upper
228 100
229 22.5 15.5 23.3
226 29.8 22.2 33.2

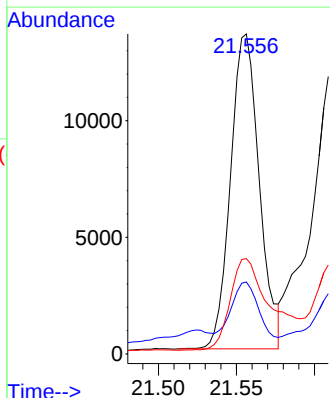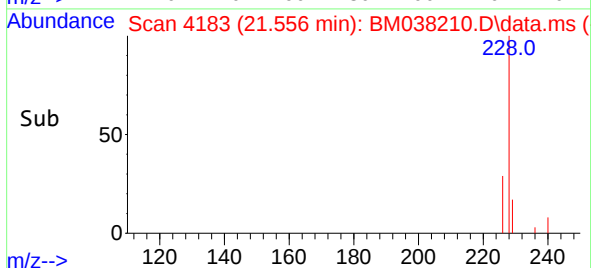



#22
Chrysene
Concen: 0.417 ng/ul
RT: 21.609 min Scan# 41
Delta R.T. -0.003 min
Lab File: BM038210.D
Acq: 22 Dec 2022 22:32




Instrument :
BNA_M
ClientSampleId :
DBYG7DL

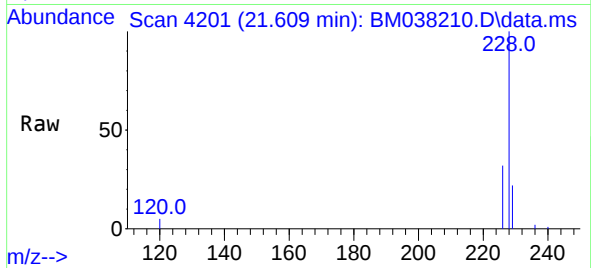


Tgt Ion:228 Resp: 1778
Ion Ratio Lower Upper
228 100
226 32.1 25.0 37.4
229 21.7 16.0 24.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/23/2022
Supervised By :mohammad ahmed 12/23/2022

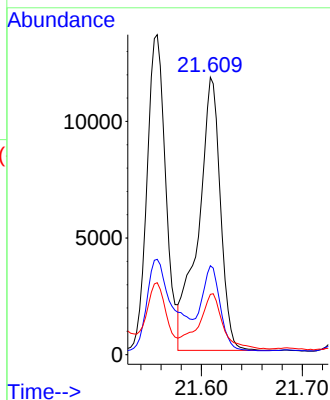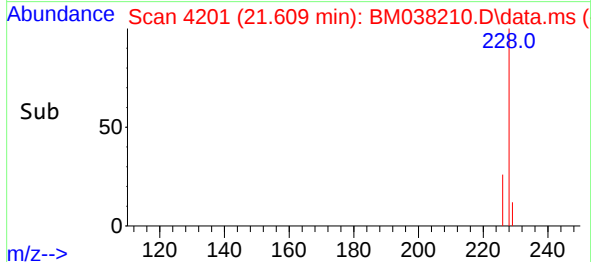


#24
Benzo(b)fluoranthene
Concen: 0.615 ng/ul
RT: 23.272 min Scan# 4770
Delta R.T. 0.000 min
Lab File: BM038210.D
Acq: 22 Dec 2022 22:32

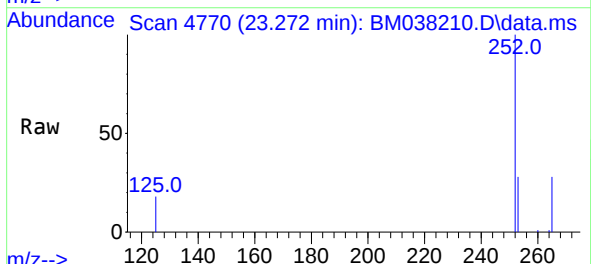

Tgt Ion:252 Resp: 26789
Ion Ratio Lower Upper
252 100
253 28.3 0.0 56.0
125 17.9 0.0 36.6

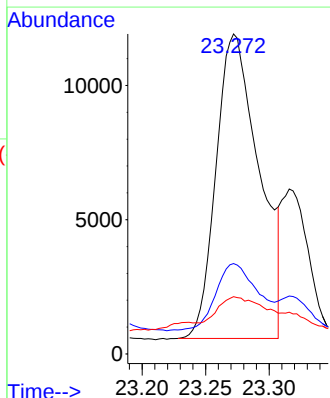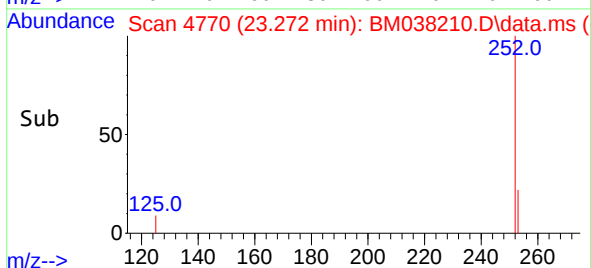



#25

Benzo(k)fluoranthene

Concen: 0.199 ng/ul m

RT: 23.316 min Scan# 4

Delta R.T. -0.006 min

Lab File: BM038210.D

Acq: 22 Dec 2022 22:32

Instrument :

BNA_M

ClientSampleId :

DBYG7DL





Tgt Ion:252 Resp: 8319

Ion	Ratio	Lower	Upper
252	100		
253	35.1	22.5	33.7
125	25.3	14.4	21.6

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2022
Supervised By :mohammad ahmed 12/23/2022

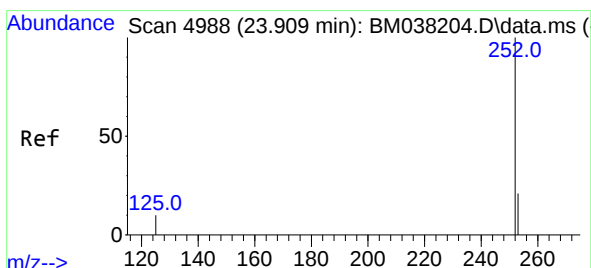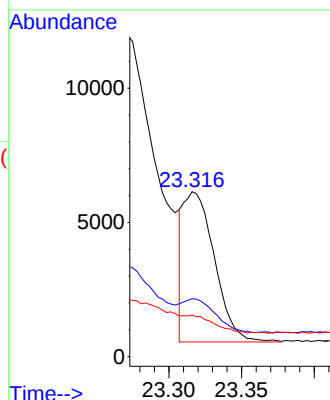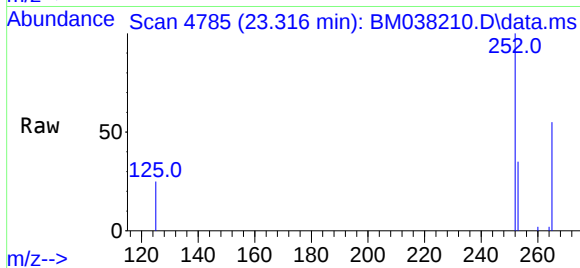

#26

Benzo(a)pyrene

Concen: 0.404 ng/ul

RT: 23.912 min Scan# 4989




Delta R.T. 0.000 min


Lab File: BM038210.D

Acq: 22 Dec 2022 22:32

Tgt Ion:252 Resp: 15381


Ion	Ratio	Lower	Upper
252	100		
253	31.2	24.2	36.4
125	21.7	17.3	25.9

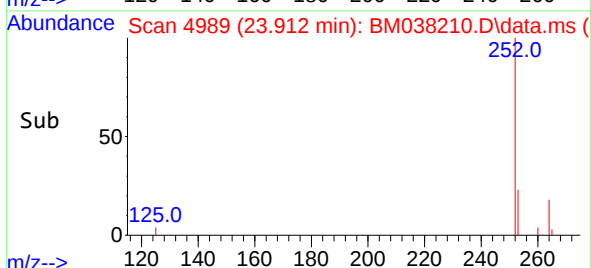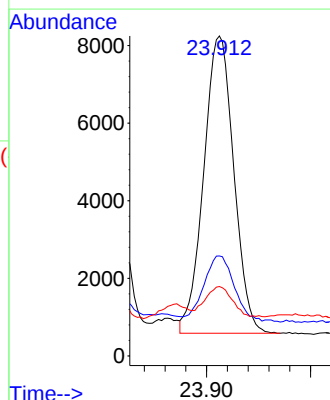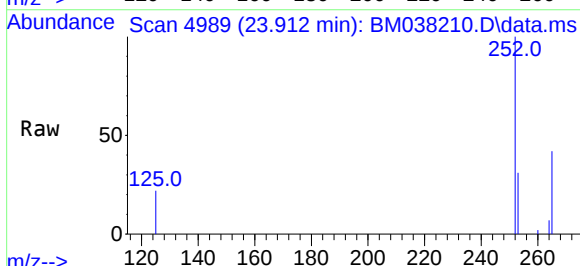



#27
Indeno(1,2,3-cd)pyrene
Concen: 0.245 ng/ul
RT: 26.579 min Scan# 5832
Delta R.T. -0.003 min
Lab File: BM038210.D
Acq: 22 Dec 2022 22:32




Instrument :
BNA_M
ClientSampleId :
DBYG7DL




Tgt Ion:276 Resp: 12924
Ion Ratio Lower Upper
276 100
138 22.4 21.7 32.5
227 0.2 0.0 0.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/23/2022
Supervised By :mohammad ahmed 12/23/2022

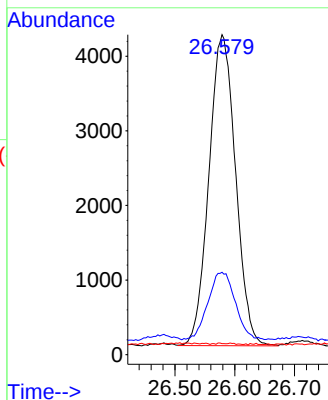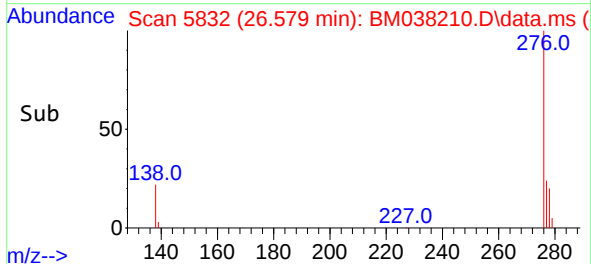


#28
Dibenzo(a,h)anthracene
Concen: 0.079 ng/ul
RT: 26.585 min Scan# 5834
Delta R.T. -0.010 min
Lab File: BM038210.D
Acq: 22 Dec 2022 22:32

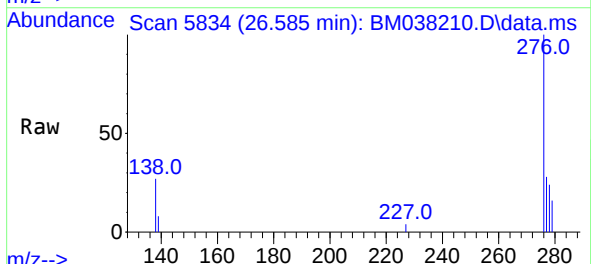


Tgt Ion:278 Resp: 3250
Ion Ratio Lower Upper
278 100
139 35.3 16.8 25.2#
279 64.8 23.4 35.2#

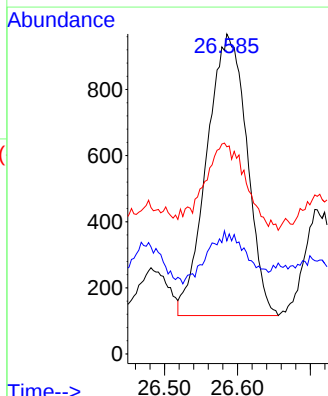



#29
Benzo(g,h,i)perylene
Concen: 0.264 ng/ul
RT: 27.370 min Scan# 6069
Delta R.T. 0.000 min
Lab File: BM038210.D
Acq: 22 Dec 2022 22:32

Instrument :
BNA_M
ClientSampleId :
DBYG7DL

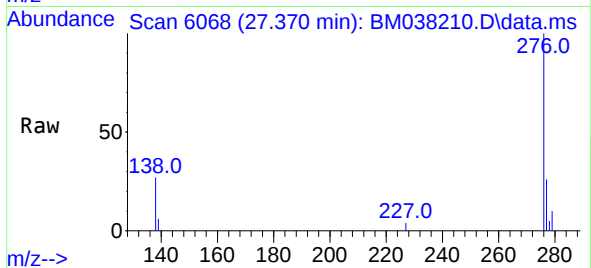

Tgt Ion:276 Resp: 1172
Ion Ratio Lower Upper
276 100
138 27.1 20.8 31.2
277 26.0 20.5 30.7

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2022
Supervised By :mohammad ahmed 12/23/2022

