

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
 Data File : BM038297.D
 Acq On : 25 Dec 2022 07:41
 Operator : CG/JU
 Sample : N6016-20
 Misc :
 ALS Vial : 106 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBYE3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

Quant Time: Dec 25 23:54:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 24 05:23:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.026	152	3122	0.400	ng/ul	0.00
4) Naphthalene-d8	10.840	136	9179	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.652	164	5476	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	11012	0.400	ng/ul	0.00
17) Chrysene-d12	21.565	240	8420	0.400	ng/ul	0.00
23) Perylene-d12	24.012	264	7521	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	8634	2.719	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.418	152	2571	0.190	ng/ul	0.00
18) Fluoranthene-d10	19.413	212	5880	0.186	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.434	178	3466	0.094	ng/ul	92
19) Fluoranthene	19.445	202	9332	0.202	ng/ul#	76
20) Pyrene	19.808	202	7959m	0.171	ng/ul	
21) Benzo(a)anthracene	21.551	228	4653	0.126	ng/ul#	91
22) Chrysene	21.603	228	5456	0.152	ng/ul#	91
24) Benzo(b)fluoranthene	23.263	252	8858	0.266	ng/ul	83
25) Benzo(k)fluoranthene	23.310	252	2819m	0.088	ng/ul	
26) Benzo(a)pyrene	23.904	252	5640	0.194	ng/ul#	82
27) Indeno(1,2,3-cd)pyrene	26.562	276	4863	0.121	ng/ul#	80
28) Dibenzo(a,h)anthracene	26.569	278	1210	0.039	ng/ul#	1
29) Benzo(g,h,i)perylene	27.353	276	4865	0.144	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122222\
Data File : BM038297.D
Acq On : 25 Dec 2022 07:41
Operator : CG/JU
Sample : N6016-20
Misc :
ALS Vial : 106 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DBYE3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022


Quant Time: Dec 25 23:54:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 24 05:23:31 2022
Response via : Initial Calibration

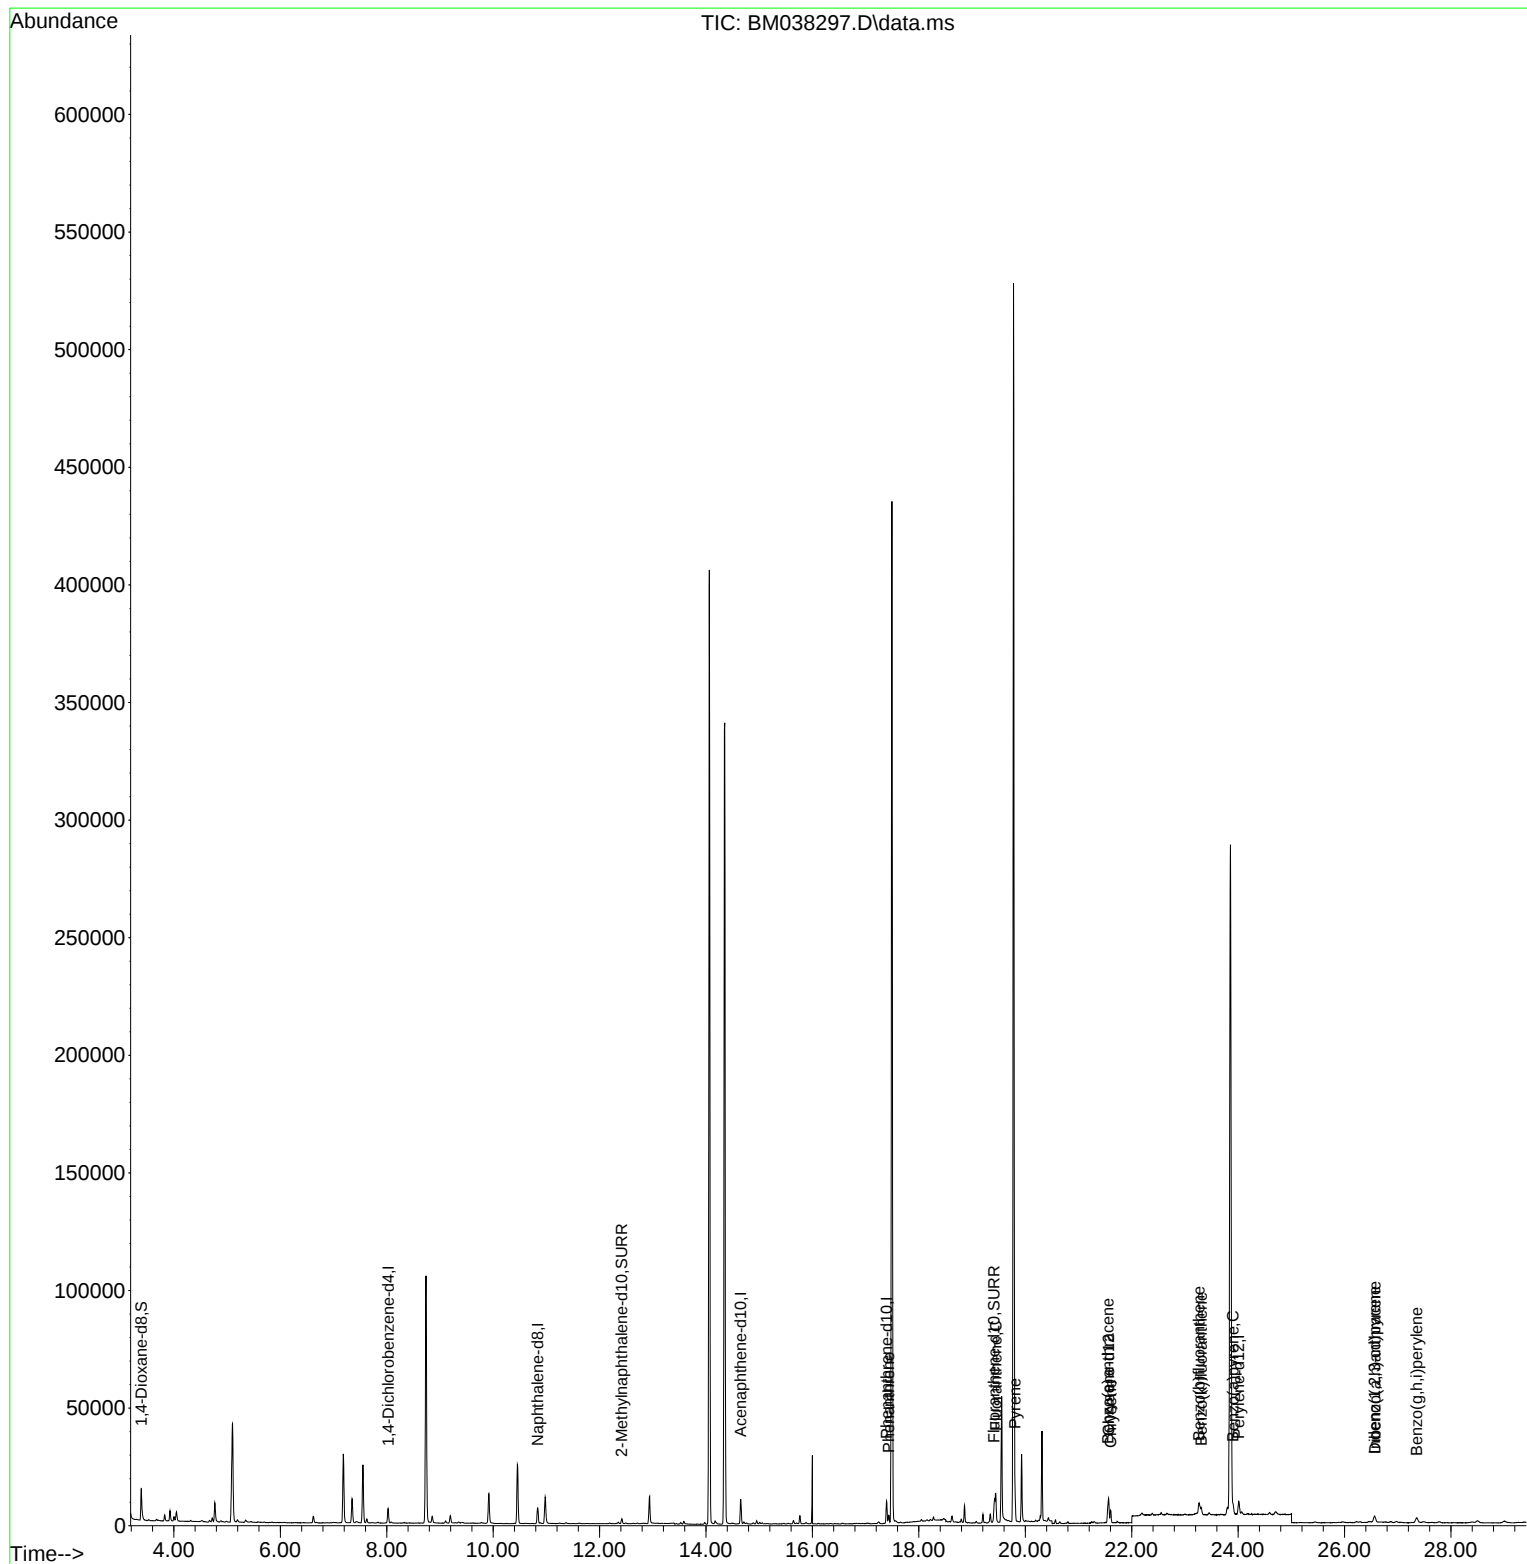

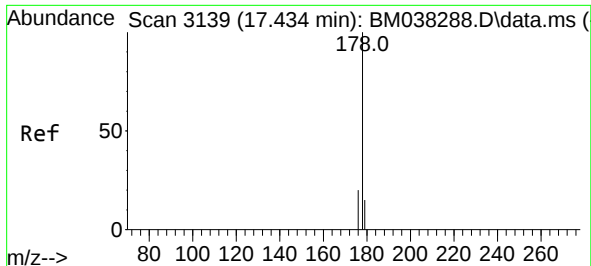

#15
Phenanthrene
Concen: 0.094 ng/ul
RT: 17.434 min Scan# 3139
Delta R.T. -0.004 min
Lab File: BM038297.D
Acq: 25 Dec 2022 07:41




Instrument :
BNA_M
ClientSampleId :
DBYE3

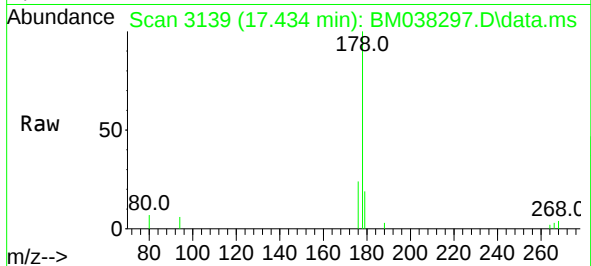

Tgt Ion:178 Resp: 3460
Ion Ratio Lower Upper
178 100
179 19.4 13.0 19.4
176 23.8 16.2 24.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

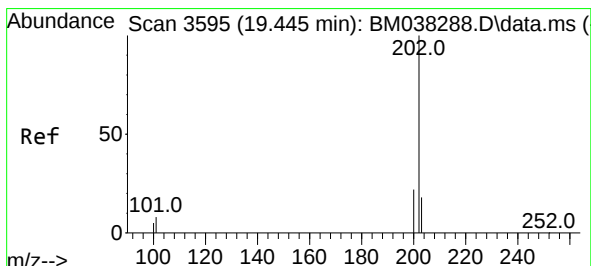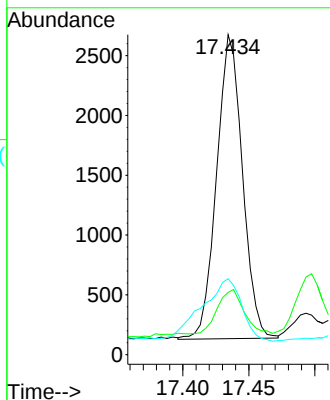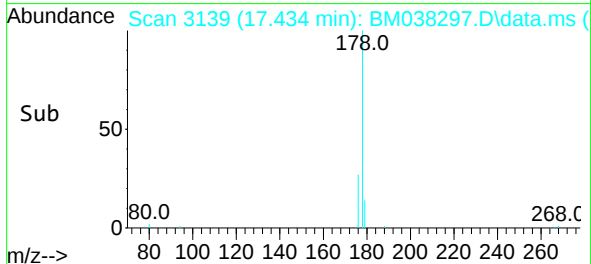

#19
Fluoranthene
Concen: 0.202 ng/ul
RT: 19.445 min Scan# 3595
Delta R.T. -0.004 min
Lab File: BM038297.D
Acq: 25 Dec 2022 07:41


Tgt Ion:202 Resp: 9332
Ion Ratio Lower Upper
202 100
101 19.2 7.5 11.3#
100 14.2 5.6 8.4#

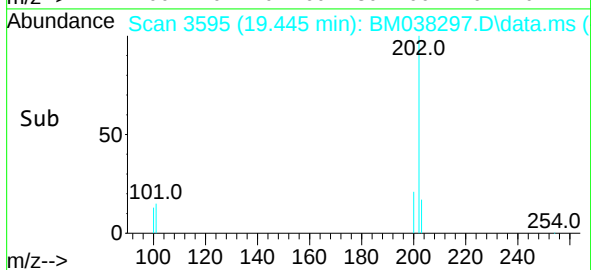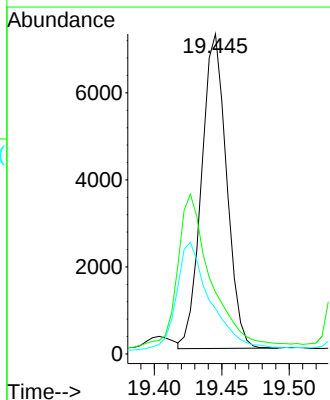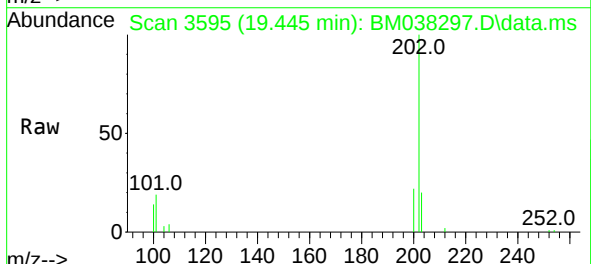



#20
Pyrene
Concen: 0.171 ng/ul m
RT: 19.808 min Scan# 3673
Delta R.T. -0.004 min
Lab File: BM038297.D
Acq: 25 Dec 2022 07:41




Instrument :
BNA_M
ClientSampleId :
DBYE3




Tgt Ion:202 Resp: 7959
Ion Ratio Lower Upper
202 100
101 13.8 8.9 13.3#
100 10.1 7.4 11.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

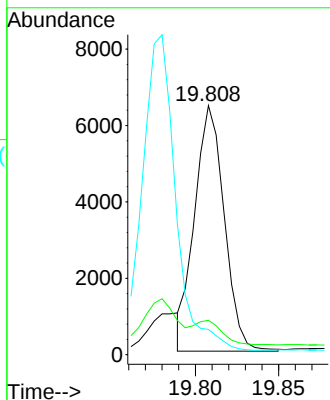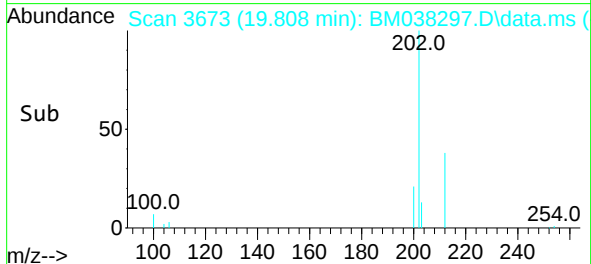


#21
Benzo(a)anthracene
Concen: 0.126 ng/ul
RT: 21.551 min Scan# 4181
Delta R.T. 0.000 min
Lab File: BM038297.D
Acq: 25 Dec 2022 07:41

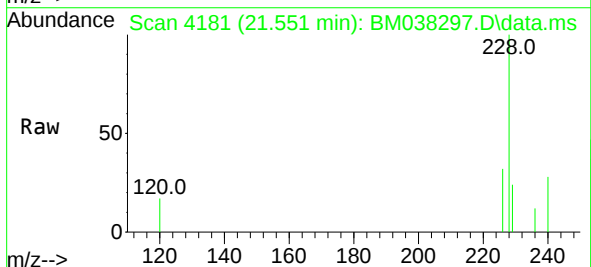


Tgt Ion:228 Resp: 4653
Ion Ratio Lower Upper
228 100
229 23.6 15.5 23.3#
226 31.9 22.2 33.2

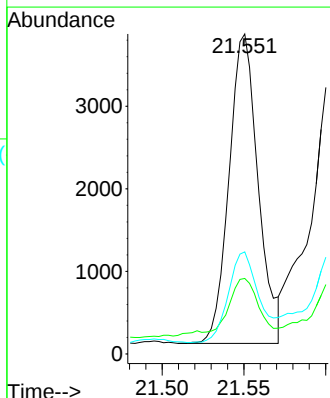

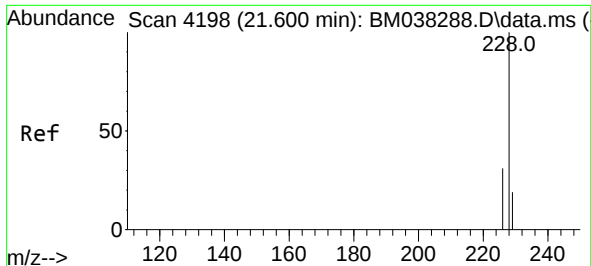

#22
Chrysene
Concen: 0.152 ng/ul
RT: 21.603 min Scan# 4198
Delta R.T. -0.003 min
Lab File: BM038297.D
Acq: 25 Dec 2022 07:41




Instrument :
BNA_M
ClientSampleId :
DBYE3



Tgt Ion:228 Resp: 5450
Ion Ratio Lower Upper
228 100
226 34.5 25.0 37.4
229 25.9 16.0 24.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

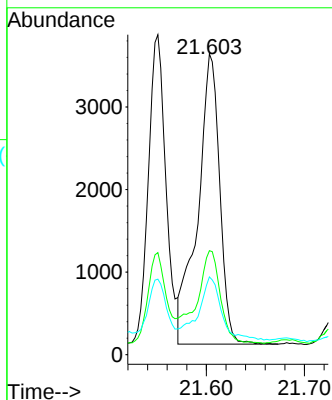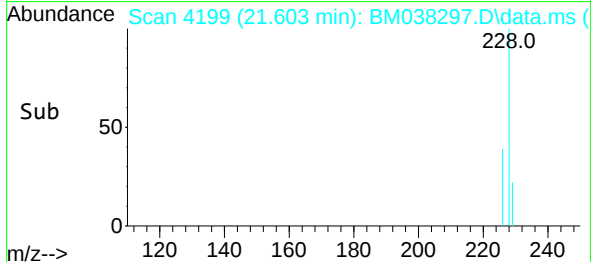

#24
Benzo(b)fluoranthene
Concen: 0.266 ng/ul
RT: 23.263 min Scan# 4767
Delta R.T. -0.003 min
Lab File: BM038297.D
Acq: 25 Dec 2022 07:41

Tgt Ion:252 Resp: 8858
Ion Ratio Lower Upper
252 100
253 36.0 0.0 56.0
125 27.6 0.0 36.6

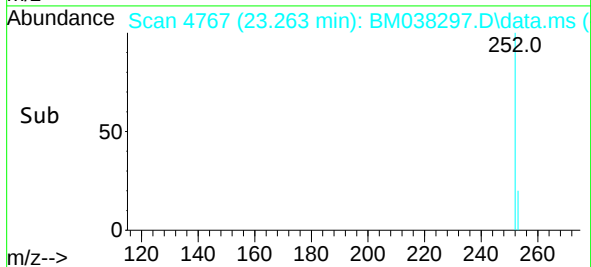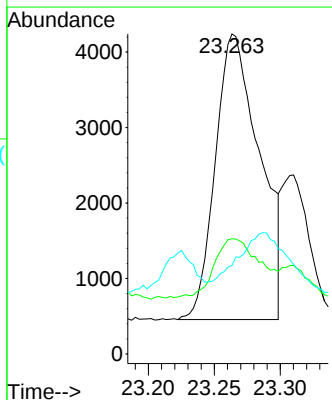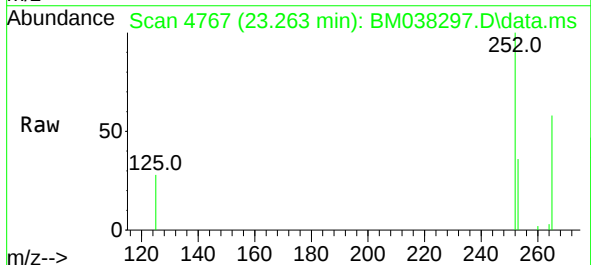

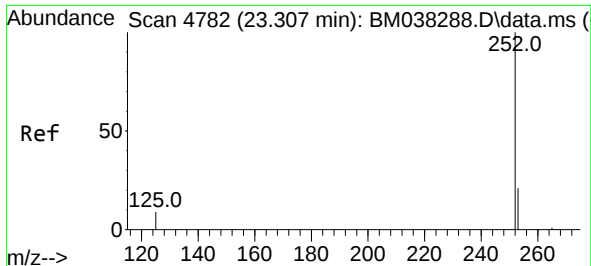

#25

Benzo(k)fluoranthene

Concen: 0.088 ng/ul m

RT: 23.310 min Scan# 4

Delta R.T. -0.003 min

Lab File: BM038297.D

Acq: 25 Dec 2022 07:41

Instrument :

BNM

ClientSampleId :

DBYE3

Tgt Ion:252 Resp: 2819

Ion Ratio Lower Upper

252 100

253 49.4 22.5 33.7





125 49.9 14.4 21.6

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 12/26/2022

Supervised By :Sohil Jodhani 12/26/2022

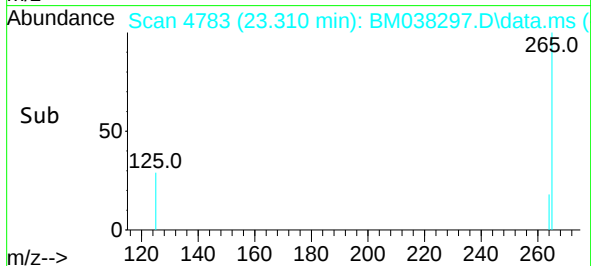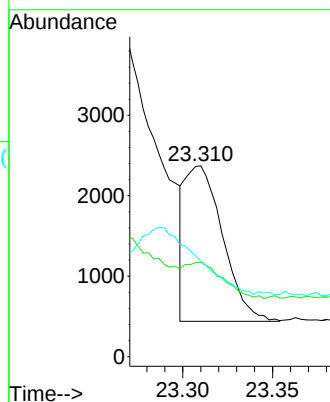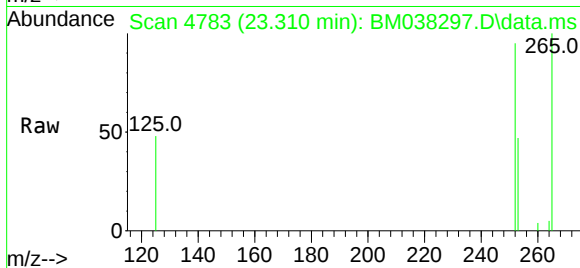

#26

Benzo(a)pyrene

Concen: 0.194 ng/ul

RT: 23.904 min Scan# 4986

Delta R.T. -0.003 min

Lab File: BM038297.D

Acq: 25 Dec 2022 07:41




Tgt Ion:252 Resp: 5640


Ion Ratio Lower Upper

252 100

253 39.6 24.2 36.4#


125 30.7 17.3 25.9#

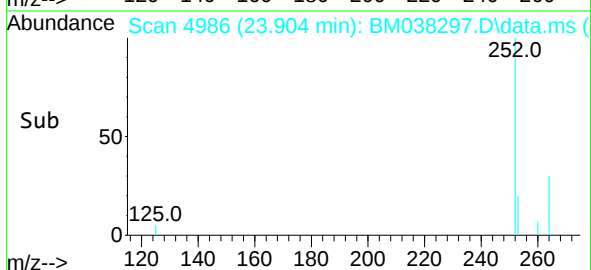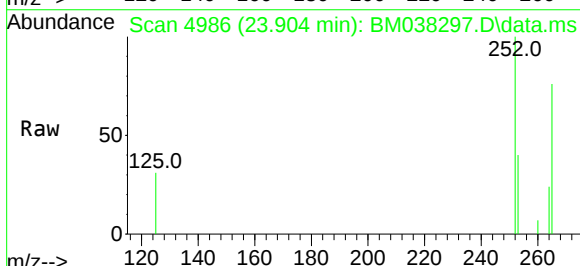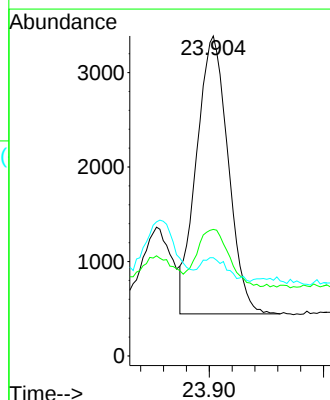

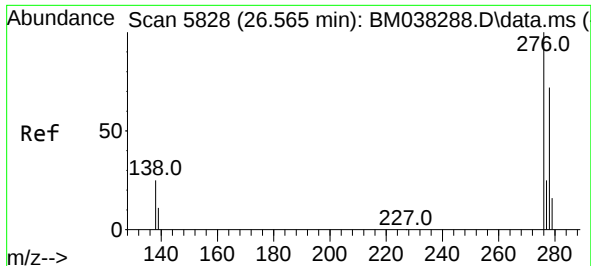

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.121 ng/ul
RT: 26.562 min Scan# 5827
Delta R.T. -0.007 min
Lab File: BM038297.D
Acq: 25 Dec 2022 07:41




Instrument :
BNA_M
ClientSampleId :
DBYE3




Tgt Ion:276 Resp: 486
Ion Ratio Lower Upper
276 100
138 16.5 21.7 32.5
227 0.0 0.0 0.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

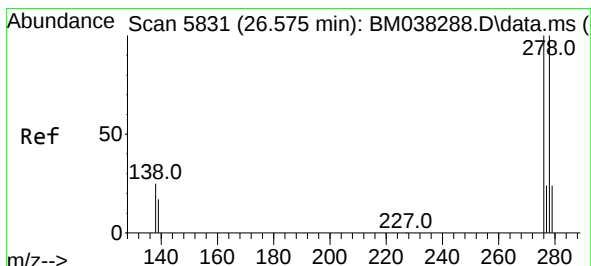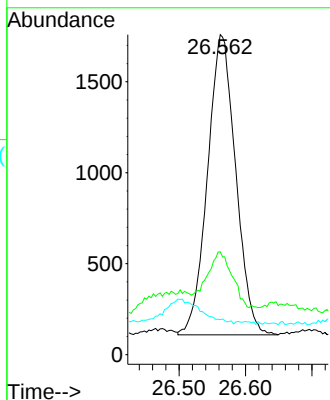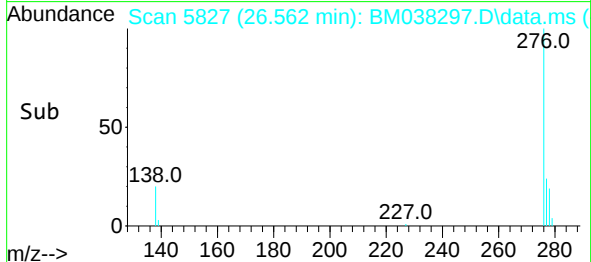


#28
Dibenzo(a,h)anthracene
Concen: 0.039 ng/ul
RT: 26.569 min Scan# 5829
Delta R.T. -0.020 min
Lab File: BM038297.D
Acq: 25 Dec 2022 07:41

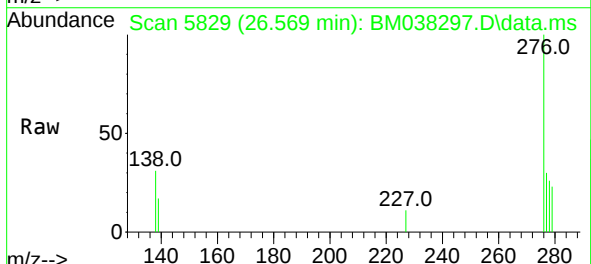


Tgt Ion:278 Resp: 1210
Ion Ratio Lower Upper
278 100
139 65.4 16.8 25.2#
279 92.0 23.4 35.2#

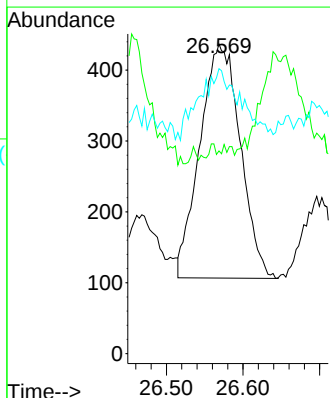



#29
Benzo(g,h,i)perylene
Concen: 0.144 ng/ul
RT: 27.353 min Scan# 6063
Delta R.T. -0.007 min
Lab File: BM038297.D
Acq: 25 Dec 2022 07:41

Instrument :
BNA_M
ClientSampleId :
DBYE3



Tgt Ion:276 Resp: 486
Ion Ratio Lower Upper
276 100
138 32.7 20.8 31.2
277 30.4 20.5 30.7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

