

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122315\
 Data File : BM003709.D
 Acq On : 22 Dec 2015 15:45
 Operator : UM/SJ
 Sample : PB87153BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB87153BL

Quant Time: Dec 22 23:31:31 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 18:52:47 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	39070	20.00	ng	-0.03
21) Naphthalene-d8	10.48	136	172441	20.00	ng	-0.04
38) Acenaphthene-d10	14.35	164	72898	20.00	ng	-0.03
63) Phenanthrene-d10	17.09	188	154386	20.00	ng	-0.03
75) Chrysene-d12	21.30	240	154660	20.00	ng	-0.02
86) Perylene-d12	23.54	264	148218	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	263797	120.04	ng	-0.02
7) Phenol-d6	6.87	99	291366	95.48	ng	-0.02
23) Nitrobenzene-d5	8.85	82	194951	70.10	ng	-0.03
41) 2,4,6-Tribromophenol	15.84	330	73278	100.65	ng	-0.03
44) 2-Fluorobiphenyl	12.96	172	409042	76.45	ng	-0.03
78) Terphenyl-d14	19.73	244	481708	73.45	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122315\
Data File : BM003709.D
Acq On : 22 Dec 2015 15:45
Operator : UM/SJ
Sample : PB87153BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB87153BL

Quant Time: Dec 22 23:31:31 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

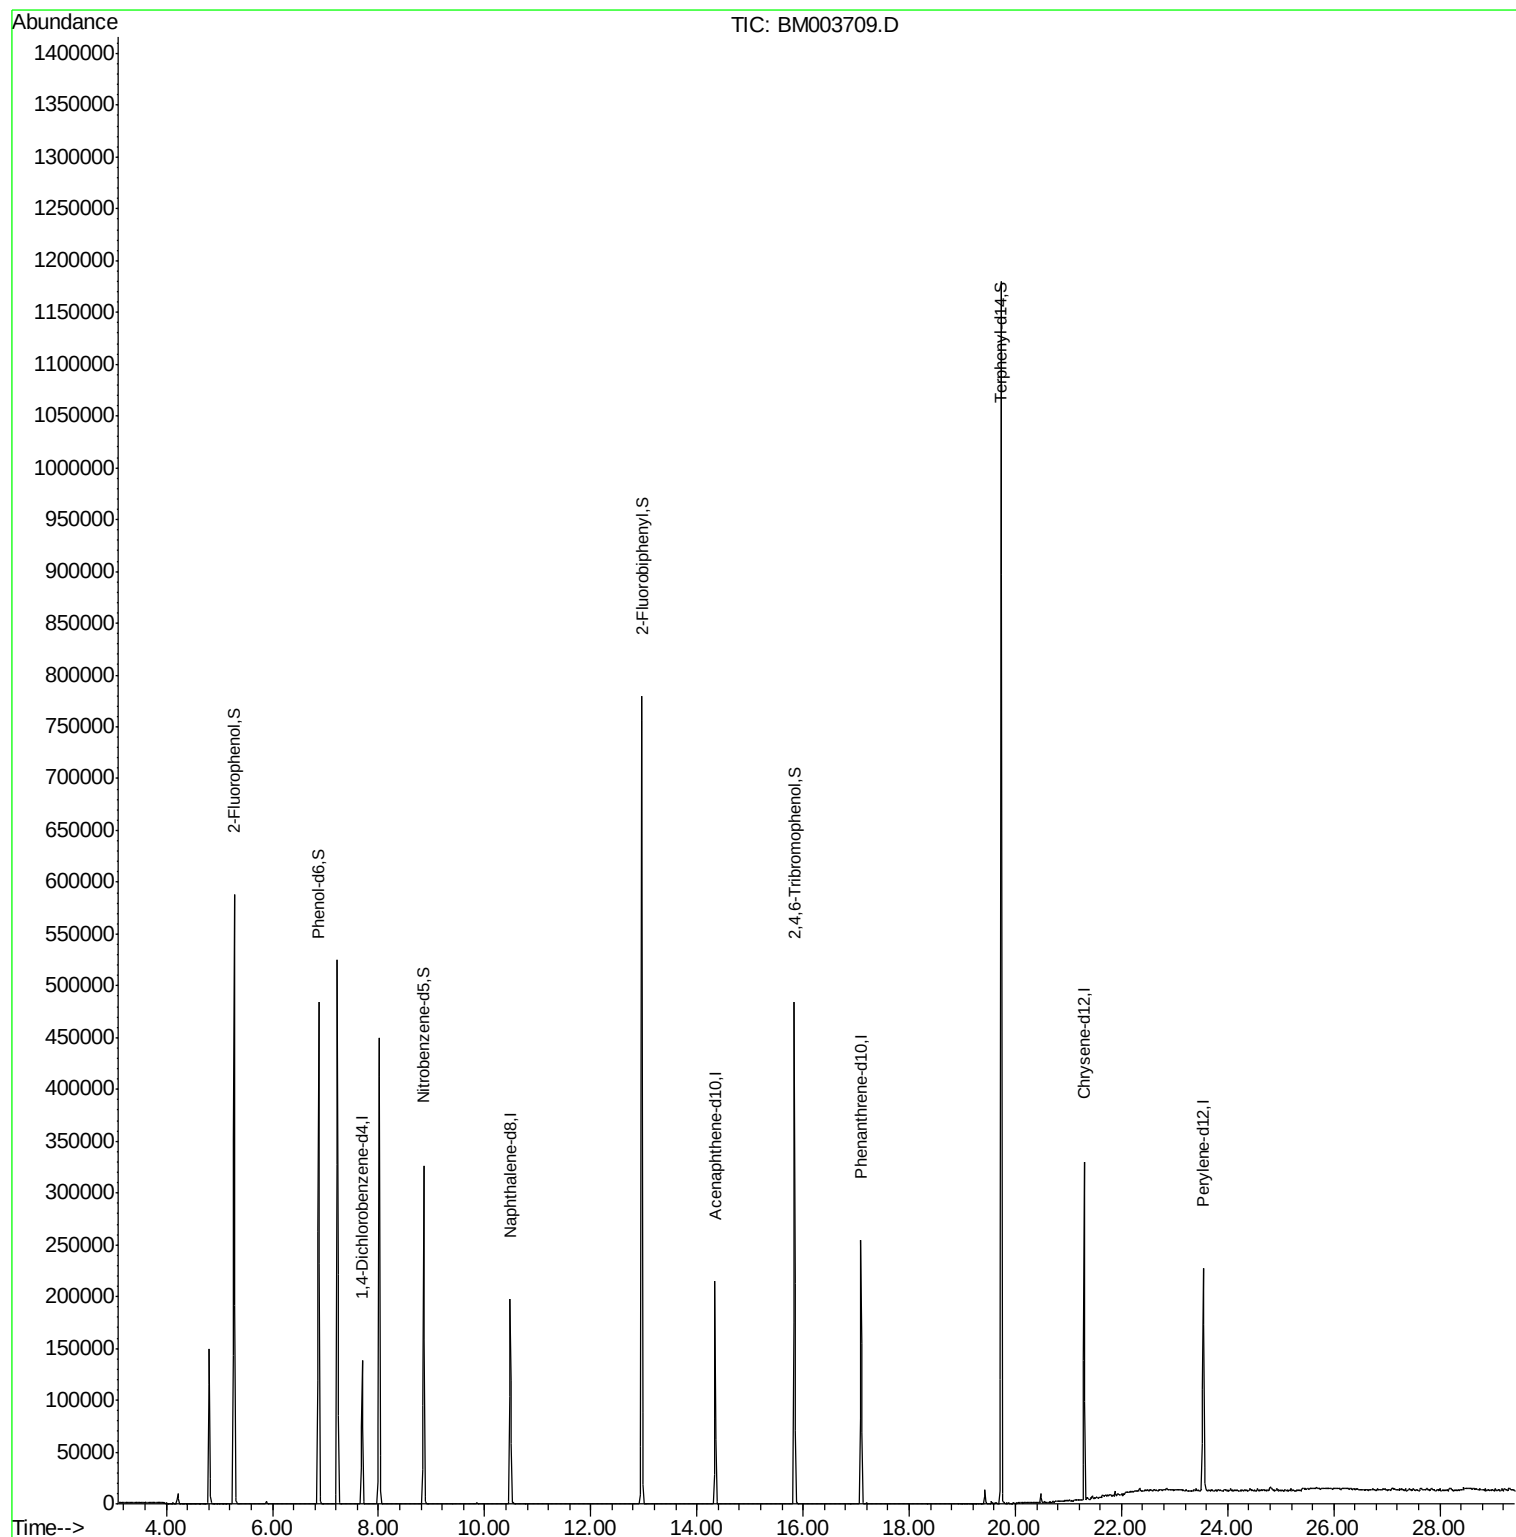


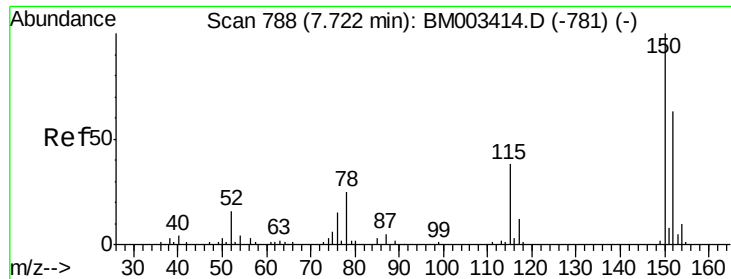




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.69 min Scan# 783
 Delta R.T. -0.03 min
 Lab File: BM003709.D
 Acq: 22 Dec 2015 15:45

Instrument :
 BNA_M
 ClientSampleId :
 PB87153BL

Tgt Ion:152 Resp: 39070
 Ion Ratio Lower Upper
 152 100
 150 158.6 119.5 179.3
 115 61.0 43.0 64.4

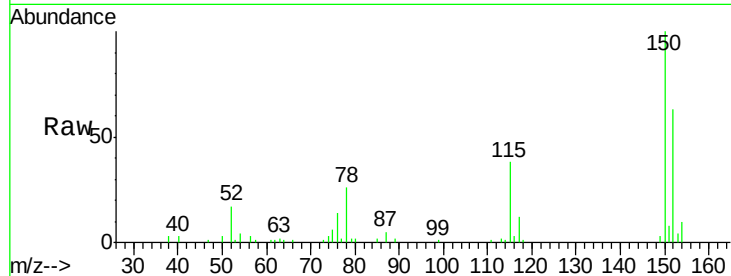


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

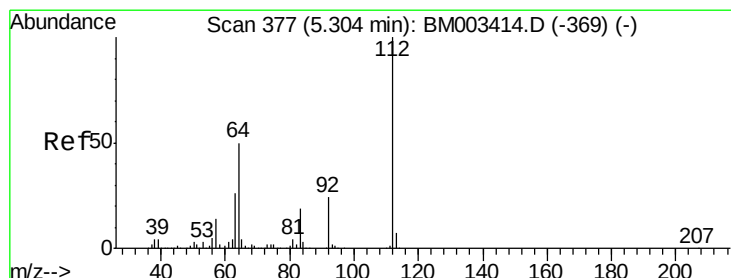
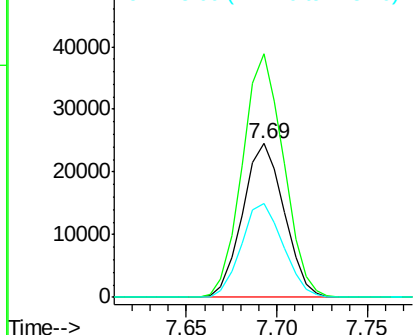



#5
 2-Fluorophenol
 Concen: 120.04 ng
 RT: 5.28 min Scan# 373
 Delta R.T. -0.02 min
 Lab File: BM003709.D
 Acq: 22 Dec 2015 15:45

Tgt Ion:112 Resp: 263797
 Ion Ratio Lower Upper
 112 100
 64 51.8 38.6 57.8
 63 26.7 19.3 28.9

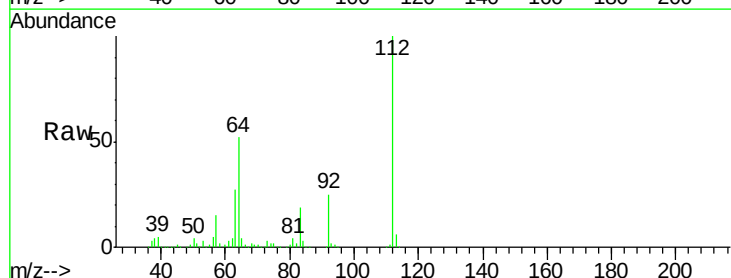

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BM0
 Ion 63.00 (62.70 to 63.70): BM0

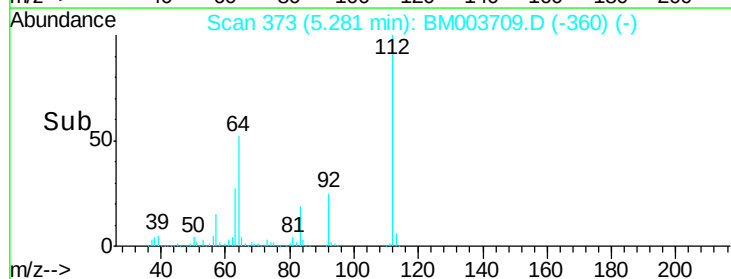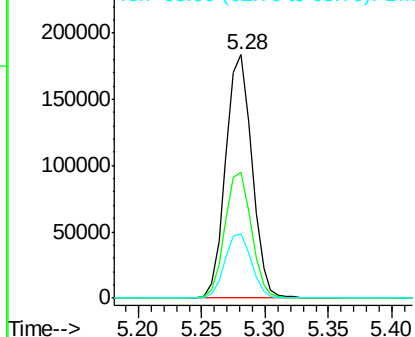



#7

Phenol-d6

Concen: 95.48 ng

RT: 6.87 min Scan# 643

Delta R.T. -0.02 min

Lab File: BM003709.D

Acq: 22 Dec 2015 15:45

Instrument :

BNA_M

ClientSampleId :

PB87153BL


Tgt Ion: 99 Resp: 291366

Ion Ratio Lower Upper

99 100

42 14.3 11.0 16.4




71 33.9 23.4 35.2

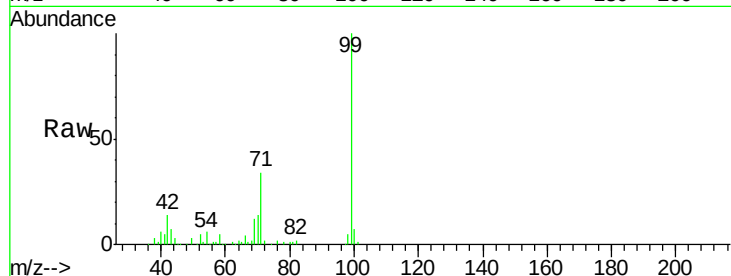

Abundance Ion 99.00 (98.70 to 99.70): BM003709.D (-630) (-)

Ion 42.00 (41.70 to 42.70): BM003709.D (-630) (-)

Ion 71.00 (70.70 to 71.70): BM003709.D (-630) (-)

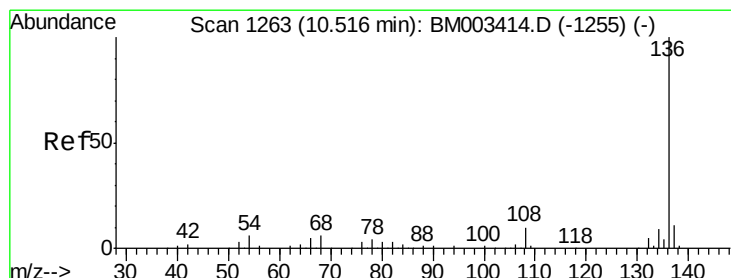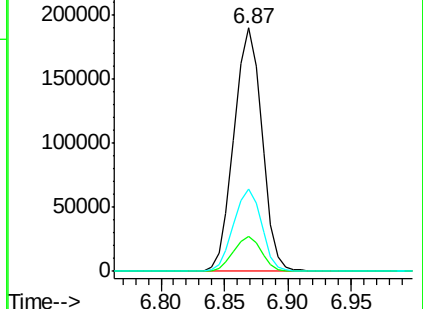

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.48 min Scan# 1257

Delta R.T. -0.04 min

Lab File: BM003709.D

Acq: 22 Dec 2015 15:45

Tgt Ion: 136 Resp: 172441


Ion Ratio Lower Upper

136 100

137 11.3 8.7 13.1

54 6.7 4.6 6.8

68 5.6 3.7 5.5#


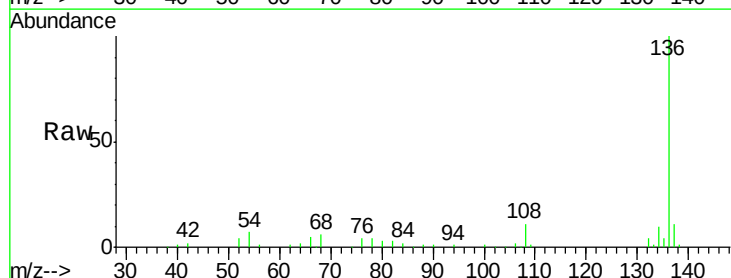



Abundance Ion 136.00 (135.70 to 136.70): BM003709.D (-1246) (-)

Ion 137.00 (136.70 to 137.70): BM003709.D (-1246) (-)

Ion 54.00 (53.70 to 54.70): BM003709.D (-1246) (-)

Ion 68.00 (67.70 to 68.70): BM003709.D (-1246) (-)

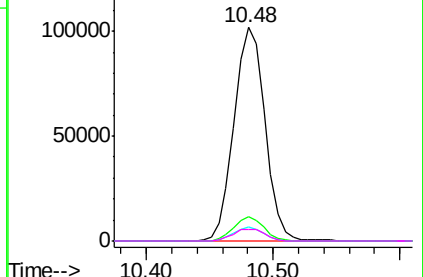







#23
 Nitrobenzene-d5
 Concen: 70.10 ng
 RT: 8.85 min Scan# 980
 Delta R.T. -0.03 min
 Lab File: BM003709.D
 Acq: 22 Dec 2015 15:45

Instrument :
 BNA_M
 ClientSampleId :
 PB87153BL

Tgt Ion: 82 Resp: 194951
 Ion Ratio Lower Upper
 82 100
 128 45.0 32.8 49.2
 54 41.8 40.6 60.8

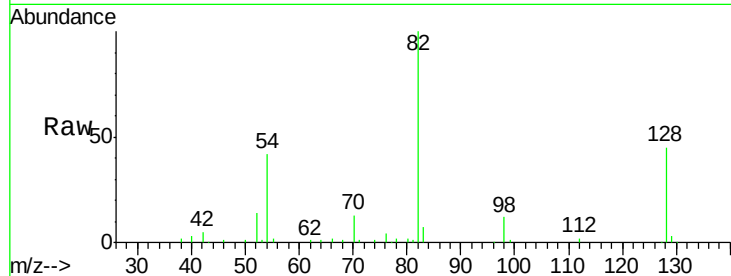


Abundance Ion 82.00 (81.70 to 82.70): BM003709.D (-968) (-)
 Ion 128.00 (127.70 to 128.70): BM003709.D (-968) (-)
 Ion 54.00 (53.70 to 54.70): BM003709.D (-968) (-)

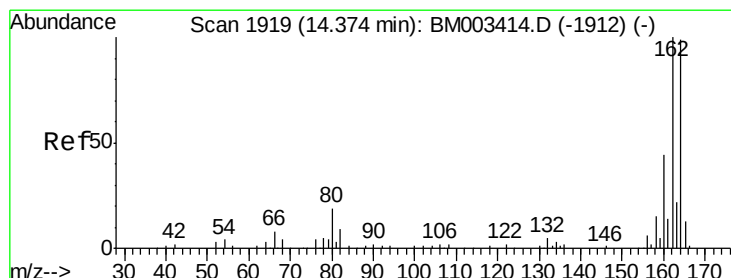
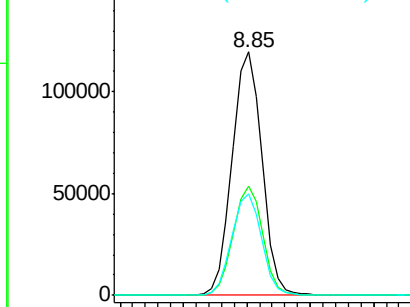



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.35 min Scan# 1914
 Delta R.T. -0.03 min
 Lab File: BM003709.D
 Acq: 22 Dec 2015 15:45

Tgt Ion: 164 Resp: 72898
 Ion Ratio Lower Upper
 164 100
 162 103.9 82.4 123.6
 160 46.6 35.8 53.6

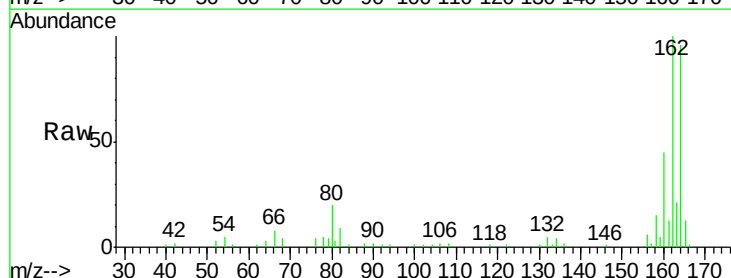

Abundance Ion 164.00 (163.70 to 164.70): BM003709.D (-1902) (-)
 Ion 162.00 (161.70 to 162.70): BM003709.D (-1902) (-)
 Ion 160.00 (159.70 to 160.70): BM003709.D (-1902) (-)




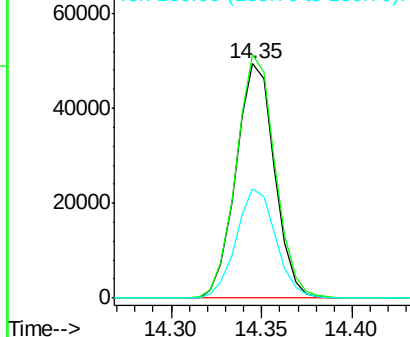




#41
 2,4,6-Tribromophenol
 Concen: 100.65 ng
 RT: 15.84 min Scan# 2168
 Delta R.T. -0.03 min
 Lab File: BM003709.D
 Acq: 22 Dec 2015 15:45




Instrument :
 BNA_M
 ClientSampleId :
 PB87153BL


Tgt Ion:330 Resp: 73278
 Ion Ratio Lower Upper
 330 100
 332 96.6 0.0 0.0#
 141 45.2 0.0 0.0#

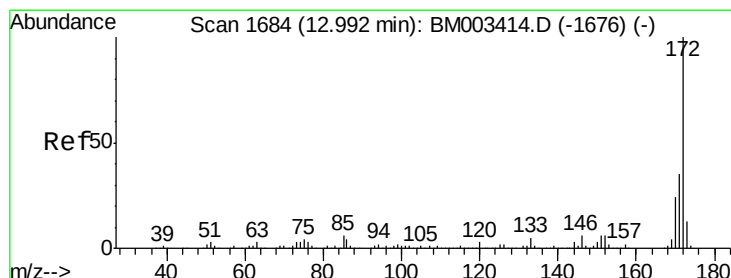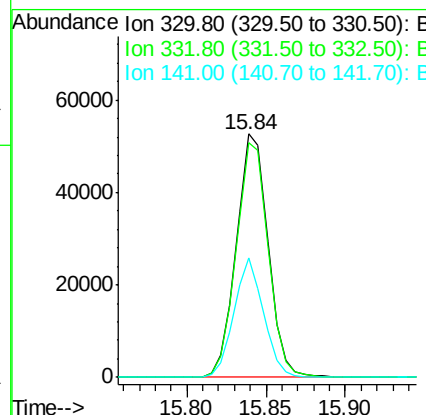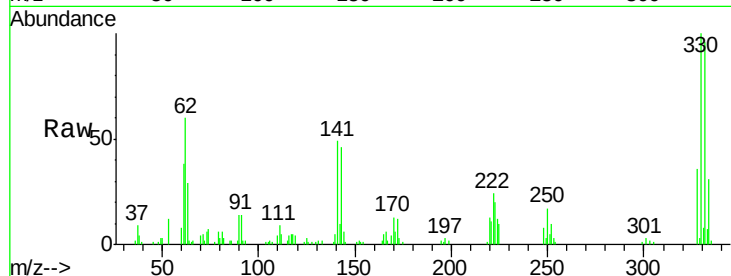

#44
 2-Fluorobiphenyl
 Concen: 76.45 ng
 RT: 12.96 min Scan# 1679
 Delta R.T. -0.03 min
 Lab File: BM003709.D
 Acq: 22 Dec 2015 15:45

Tgt Ion:172 Resp: 409042
 Ion Ratio Lower Upper
 172 100
 171 34.8 28.5 42.7
 170 23.1 18.8 28.2

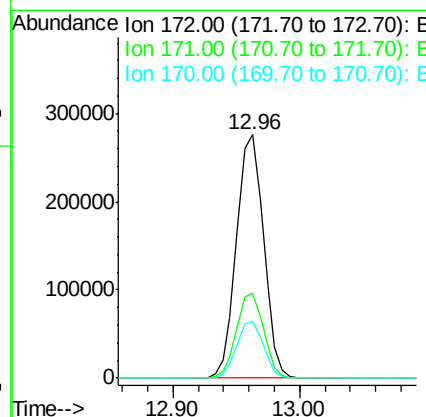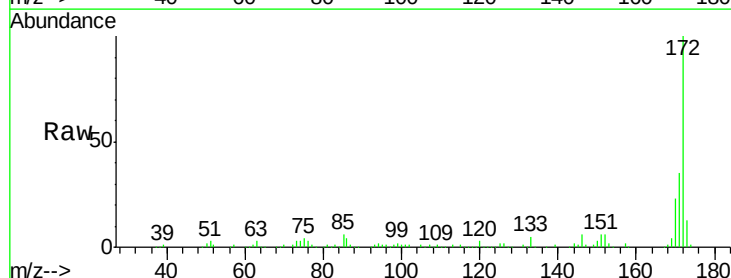


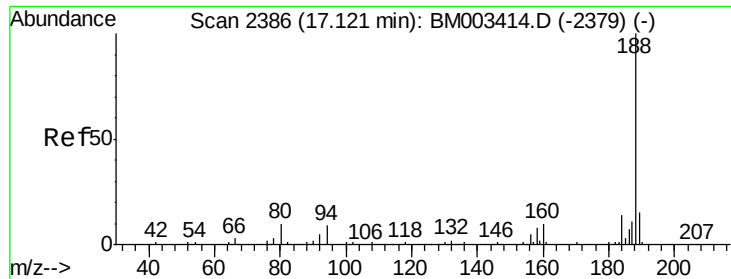




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.09 min Scan# 2381
Delta R.T. -0.03 min
Lab File: BM003709.D
Acq: 22 Dec 2015 15:45

Instrument :
BNA_M
ClientSampleId :
PB87153BL

Tgt Ion:188 Resp: 154386
Ion Ratio Lower Upper
188 100
94 9.6 8.7 13.1
80 10.5 9.3 13.9

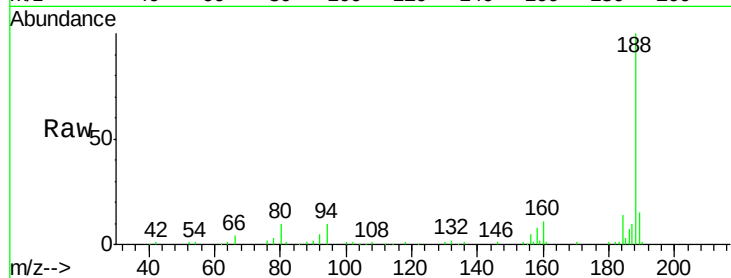


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

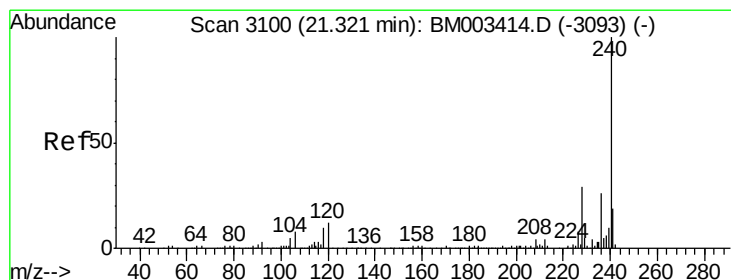
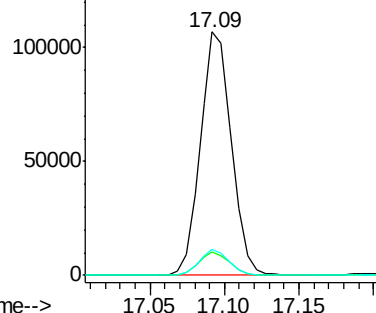



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.30 min Scan# 3096
Delta R.T. -0.02 min
Lab File: BM003709.D
Acq: 22 Dec 2015 15:45

Tgt Ion:240 Resp: 154660
Ion Ratio Lower Upper
240 100
120 11.7 8.2 12.2
236 25.8 20.0 30.0

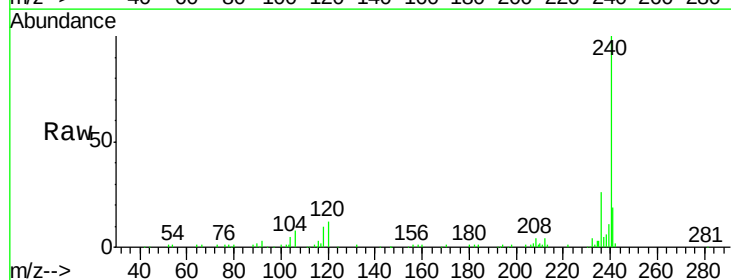

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

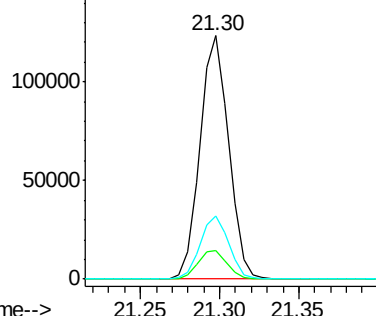

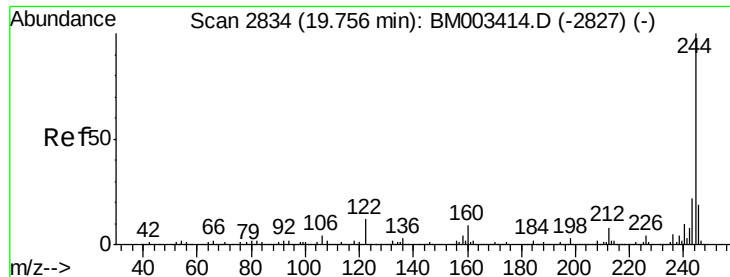

#78

Terphenyl-d14

Concen: 73.45 ng

RT: 19.73 min Scan# 2830

Delta R.T. -0.02 min

Lab File: BM003709.D

Acq: 22 Dec 2015 15:45

Instrument :

BNA_M

ClientSampleId :

PB87153BL


Tgt Ion:244 Resp: 481708

Ion Ratio Lower Upper

244 100

212 7.8 4.9 7.3#




122 12.2 6.2 9.4#

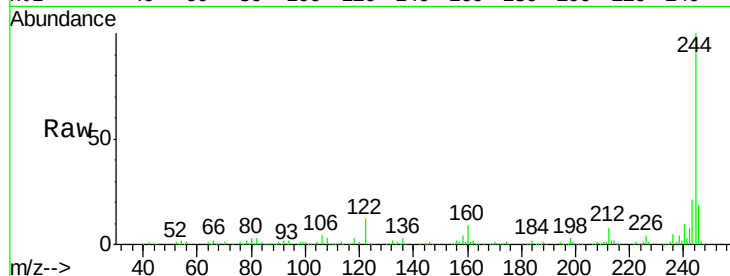

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

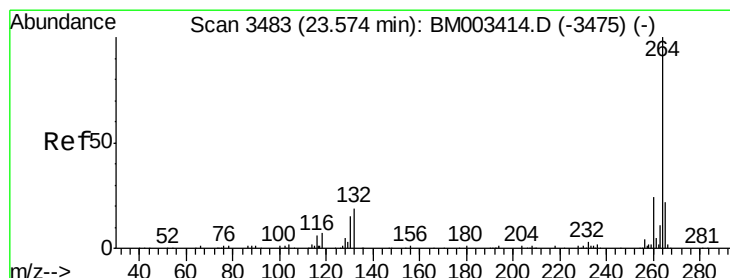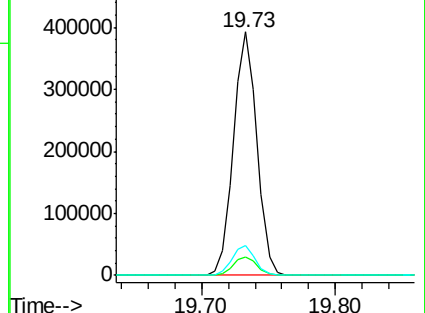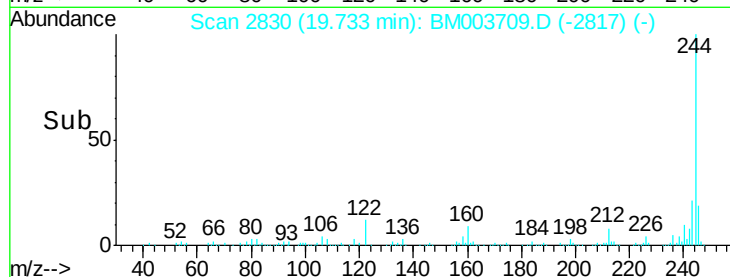

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.54 min Scan# 3477

Delta R.T. -0.04 min

Lab File: BM003709.D

Acq: 22 Dec 2015 15:45


Tgt Ion:264 Resp: 148218

Ion Ratio Lower Upper

264 100

260 23.4 18.6 27.8

265 21.1 17.3 25.9

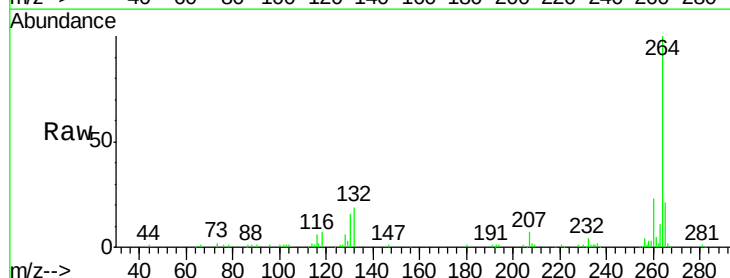

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

