

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122315\
 Data File : BM003712.D
 Acq On : 22 Dec 2015 17:34
 Operator : UM/SJ
 Sample : G4644-02RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 S8-0528

Quant Time: Dec 22 23:34:18 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 18:52:47 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	44686	20.00	ng	-0.03
21) Naphthalene-d8	10.48	136	160035	20.00	ng	-0.04
38) Acenaphthene-d10	14.35	164	77877	20.00	ng	-0.03
63) Phenanthrene-d10	17.09	188	199093	20.00	ng	-0.03
75) Chrysene-d12	21.29	240	171321	20.00	ng	-0.03
86) Perylene-d12	23.54	264	180953	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	152286	60.59	ng	-0.03
7) Phenol-d6	6.87	99	124990	35.81	ng	-0.02
23) Nitrobenzene-d5	8.85	82	263063	101.92	ng	-0.03
41) 2,4,6-Tribromophenol	15.84	330	136747	175.82	ng	-0.02
44) 2-Fluorobiphenyl	12.96	172	659948	115.46	ng	-0.03
78) Terphenyl-d14	19.73	244	650163	89.50	ng	-0.02


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122315\
Data File : BM003712.D
Acq On : 22 Dec 2015 17:34
Operator : UM/SJ
Sample : G4644-02RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
S8-0528

Quant Time: Dec 22 23:34:18 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

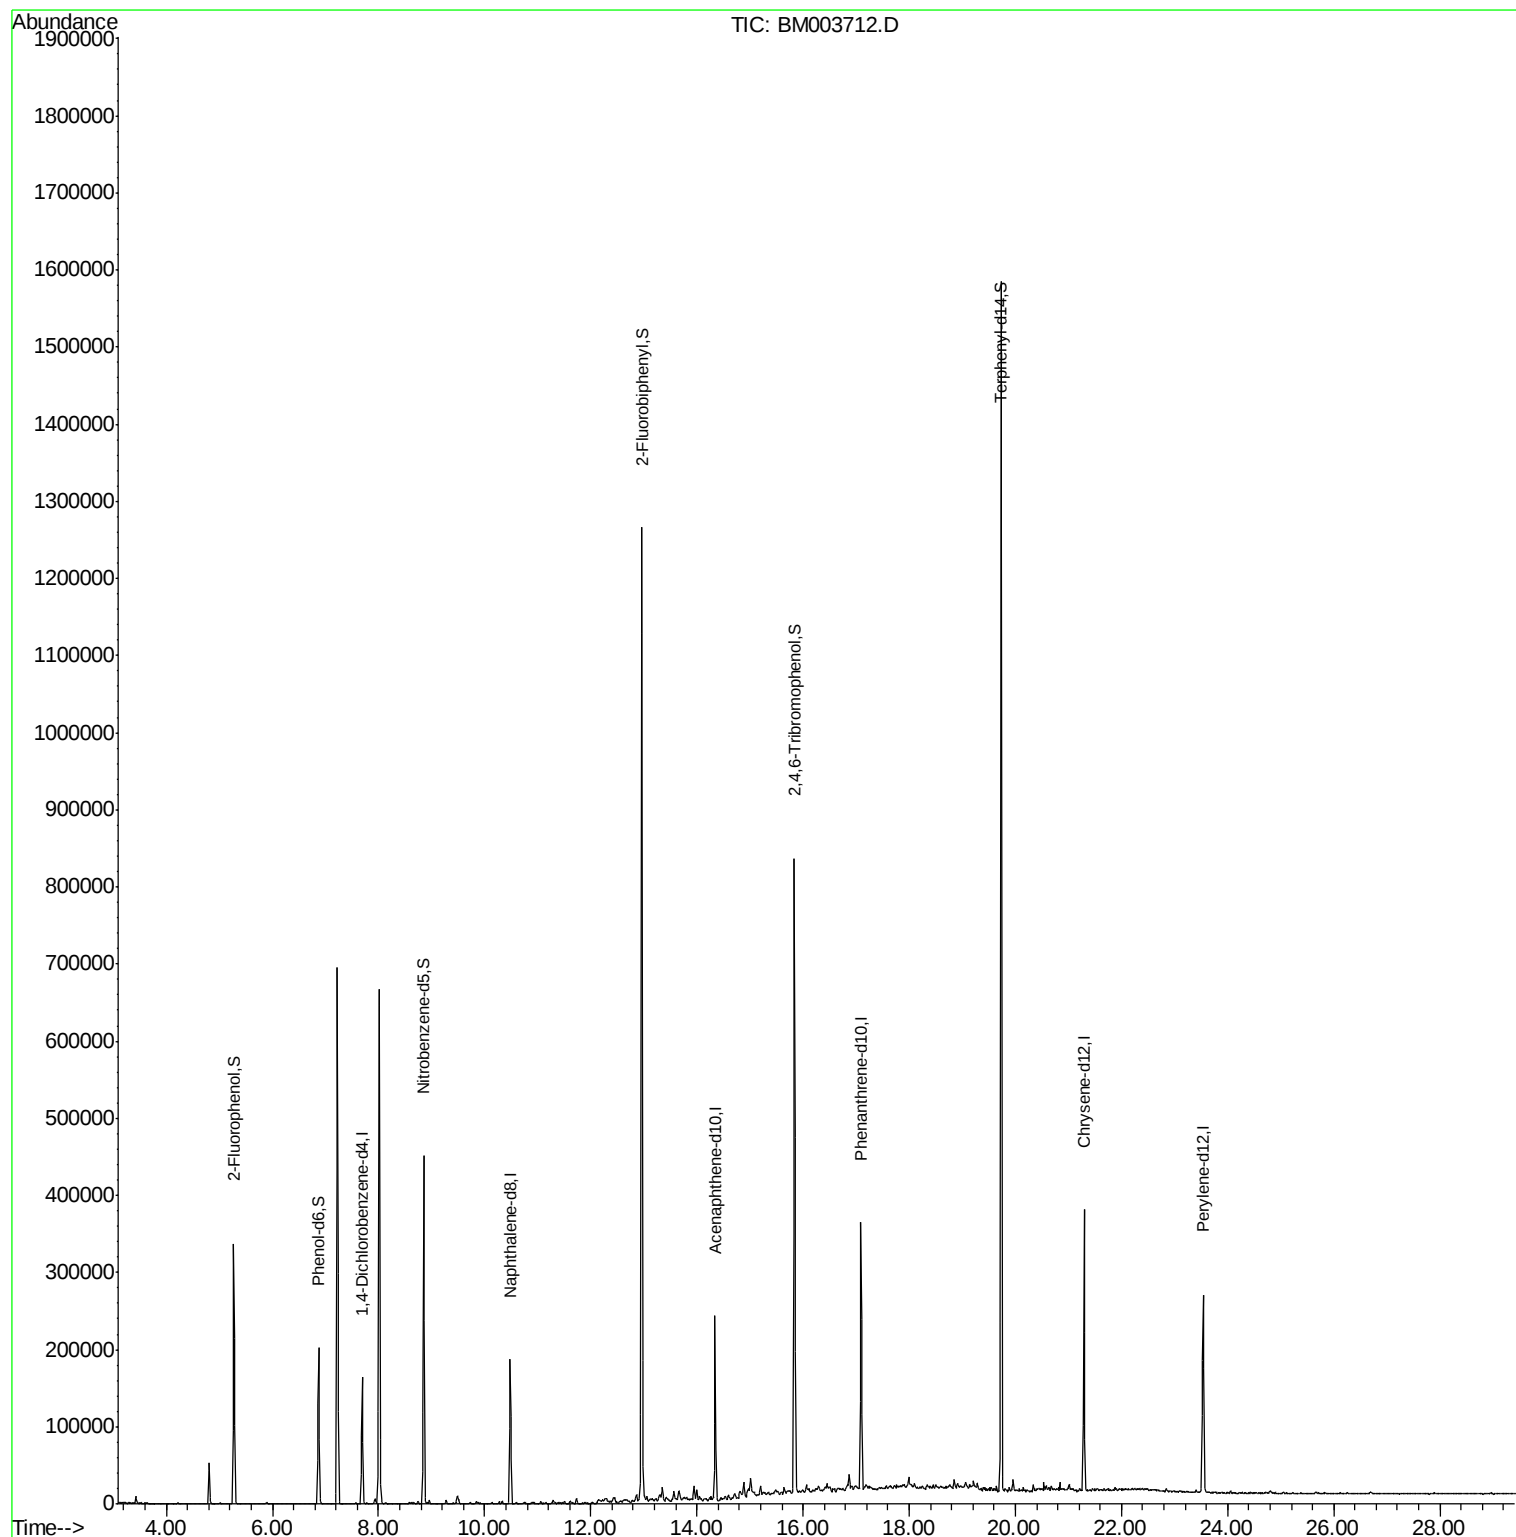




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.69 min Scan# 783
Delta R.T. -0.03 min
Lab File: BM003712.D
Acq: 22 Dec 2015 17:34

Instrument :
BNA_M
ClientSampleId :
S8-0528

Tgt Ion:152 Resp: 44686
Ion Ratio Lower Upper
152 100
150 158.4 119.5 179.3
115 60.7 43.0 64.4

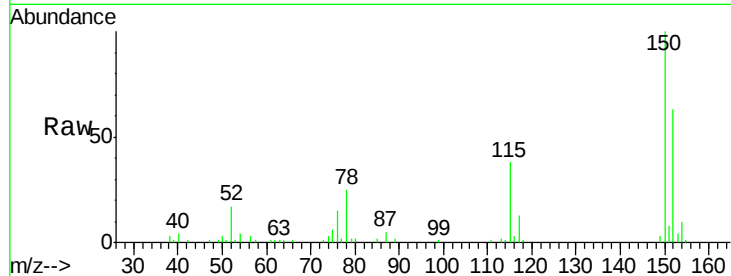


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

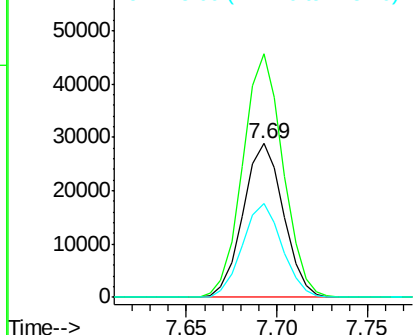



#5


2-Fluorophenol
Concen: 60.59 ng
RT: 5.28 min Scan# 372
Delta R.T. -0.03 min
Lab File: BM003712.D
Acq: 22 Dec 2015 17:34

Tgt Ion:112 Resp: 152286
Ion Ratio Lower Upper
112 100
64 54.3 38.6 57.8
63 28.4 19.3 28.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

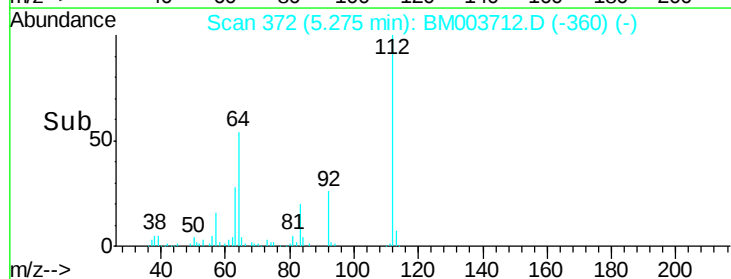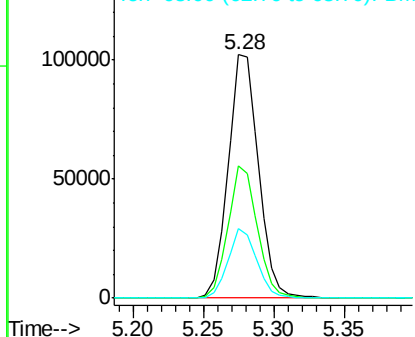



#7

Phenol-d6

Concen: 35.81 ng

RT: 6.87 min Scan# 643

Delta R.T. -0.02 min

Lab File: BM003712.D

Acq: 22 Dec 2015 17:34

Instrument :

BNA_M

ClientSampleId :

S8-0528


Tgt Ion: 99 Resp: 124990

Ion Ratio Lower Upper

99 100

42 14.2 11.0 16.4



71 33.2 23.4 35.2

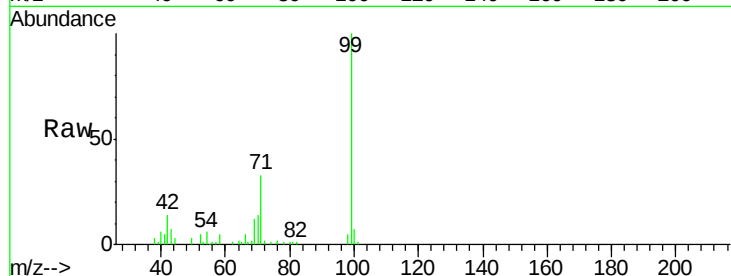

Abundance Ion 99.00 (98.70 to 99.70): BM003712.D (-630) (-)

Ion 42.00 (41.70 to 42.70): BM003712.D (-630) (-)

Ion 71.00 (70.70 to 71.70): BM003712.D (-630) (-)

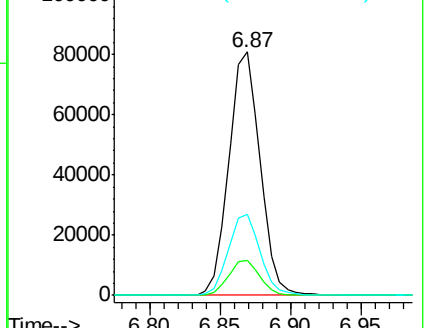

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.48 min Scan# 1257

Delta R.T. -0.04 min

Lab File: BM003712.D

Acq: 22 Dec 2015 17:34

Tgt Ion: 136 Resp: 160035


Ion Ratio Lower Upper

136 100

137 10.9 8.7 13.1

54 6.2 4.6 6.8

68 5.6 3.7 5.5#





Abundance Ion 136.00 (135.70 to 136.70): BM003712.D (-1246) (-)

Ion 137.00 (136.70 to 137.70): BM003712.D (-1246) (-)

Ion 54.00 (53.70 to 54.70): BM003712.D (-1246) (-)

Ion 68.00 (67.70 to 68.70): BM003712.D (-1246) (-)

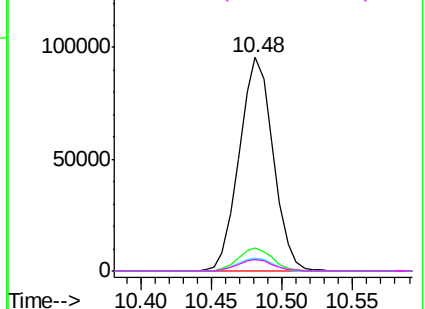







#23
 Nitrobenzene-d5
 Concen: 101.92 ng
 RT: 8.85 min Scan# 980
 Delta R.T. -0.03 min
 Lab File: BM003712.D
 Acq: 22 Dec 2015 17:34

Instrument :
 BNA_M
 ClientSampled :
 S8-0528

Tgt Ion: 82 Resp: 263063
 Ion Ratio Lower Upper
 82 100
 128 46.4 32.8 49.2
 54 41.1 40.6 60.8

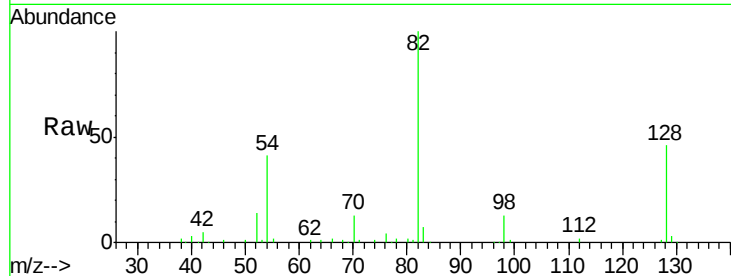


Abundance Ion 82.00 (81.70 to 82.70): BM003712.D (-968) (-)
 Ion 128.00 (127.70 to 128.70): BM003712.D (-968) (-)
 Ion 54.00 (53.70 to 54.70): BM003712.D (-968) (-)


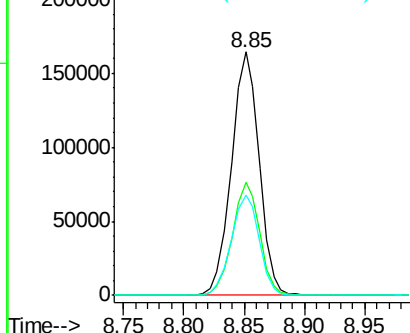


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.35 min Scan# 1914
 Delta R.T. -0.03 min
 Lab File: BM003712.D
 Acq: 22 Dec 2015 17:34

Tgt Ion: 164 Resp: 77877
 Ion Ratio Lower Upper
 164 100
 162 101.1 82.4 123.6
 160 45.2 35.8 53.6



Abundance Ion 164.00 (163.70 to 164.70): BM003712.D (-1902) (-)
 Ion 162.00 (161.70 to 162.70): BM003712.D (-1902) (-)
 Ion 160.00 (159.70 to 160.70): BM003712.D (-1902) (-)



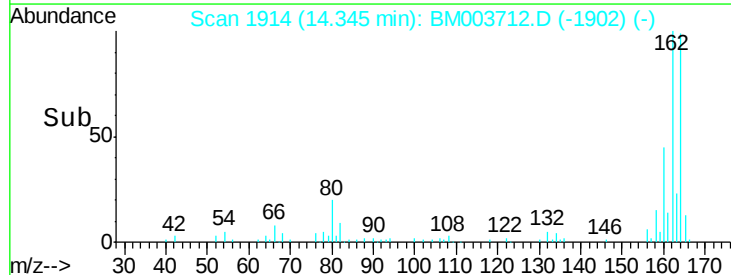
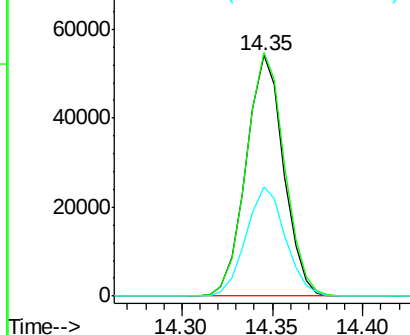




#41
 2,4,6-Tribromophenol
 Concen: 175.82 ng
 RT: 15.84 min Scan# 2169
 Delta R.T. -0.02 min
 Lab File: BM003712.D
 Acq: 22 Dec 2015 17:34




Instrument :
 BNA_M
 ClientSampleId :
 S8-0528


Tgt Ion:330 Resp: 136747
 Ion Ratio Lower Upper
 330 100
 332 96.2 0.0 0.0#
 141 44.1 0.0 0.0#

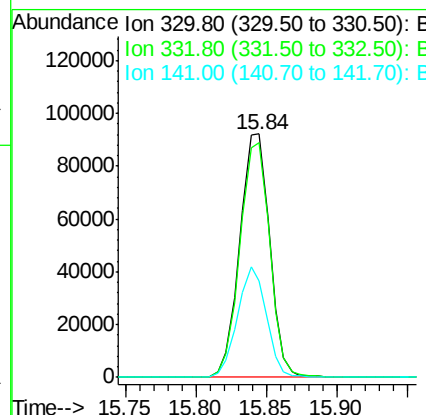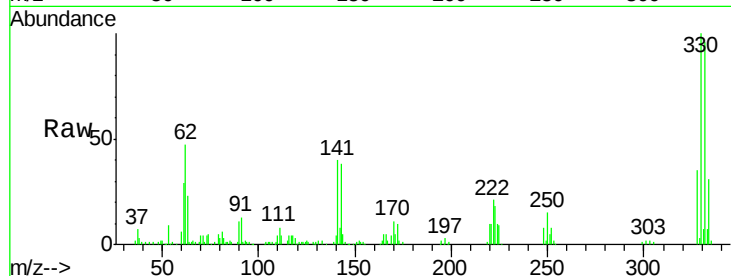

#44
 2-Fluorobiphenyl
 Concen: 115.46 ng
 RT: 12.96 min Scan# 1679
 Delta R.T. -0.03 min
 Lab File: BM003712.D
 Acq: 22 Dec 2015 17:34

Tgt Ion:172 Resp: 659948
 Ion Ratio Lower Upper
 172 100
 171 35.1 28.5 42.7
 170 23.3 18.8 28.2

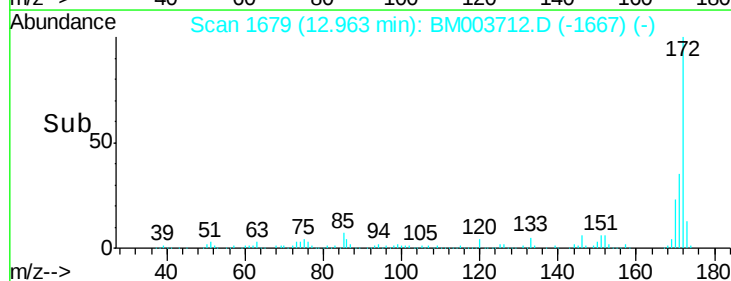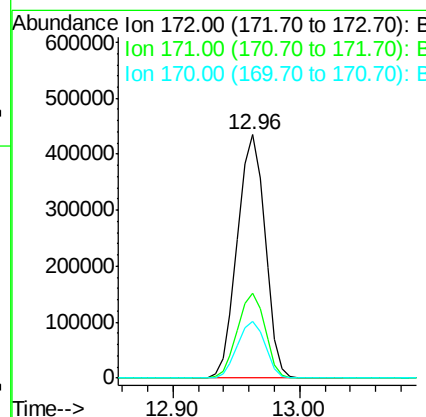



#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.09 min Scan# 2381

Delta R.T. -0.03 min

Lab File: BM003712.D

Acq: 22 Dec 2015 17:34

Instrument :

BNA_M

ClientSampleId :

S8-0528


Tgt Ion:188 Resp: 199093

Ion Ratio Lower Upper

188 100

94 10.0 8.7 13.1


80 10.8 9.3 13.9

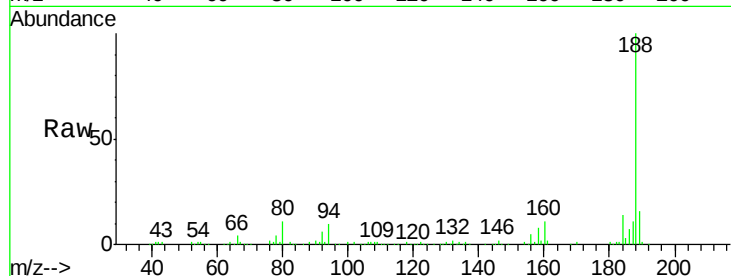



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

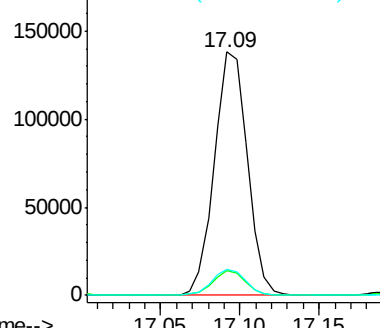

Time-->



#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.29 min Scan# 3095

Delta R.T. -0.03 min

Lab File: BM003712.D

Acq: 22 Dec 2015 17:34


Tgt Ion:240 Resp: 171321

Ion Ratio Lower Upper

240 100

120 11.7 8.2 12.2


236 25.9 20.0 30.0




Abundance Ion 240.00 (239.70 to 240.70): E


Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

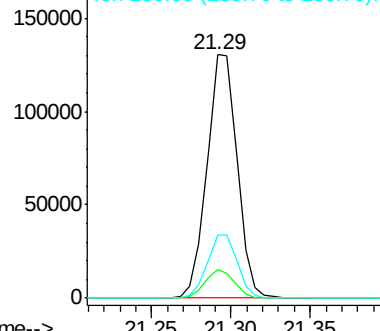

Time-->



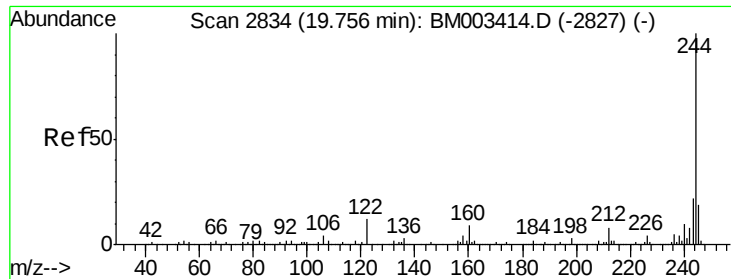

#78

Terphenyl-d14

Concen: 89.50 ng

RT: 19.73 min Scan# 2830

Delta R.T. -0.02 min

Lab File: BM003712.D

Acq: 22 Dec 2015 17:34

Instrument :

BNA_M

ClientSampleId :

S8-0528


Tgt Ion:244 Resp: 650163

Ion Ratio Lower Upper

244 100

212 7.9 4.9 7.3#




122 11.4 6.2 9.4#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

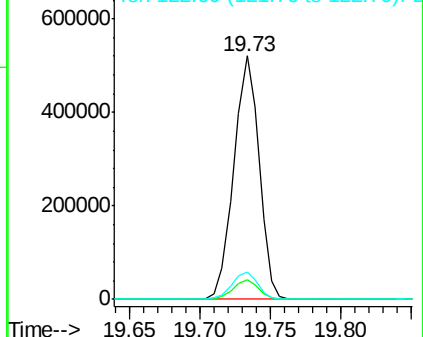

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.54 min Scan# 3477

Delta R.T. -0.04 min

Lab File: BM003712.D

Acq: 22 Dec 2015 17:34


Tgt Ion:264 Resp: 180953

Ion Ratio Lower Upper

264 100

260 24.2 18.6 27.8

265 21.6 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

