
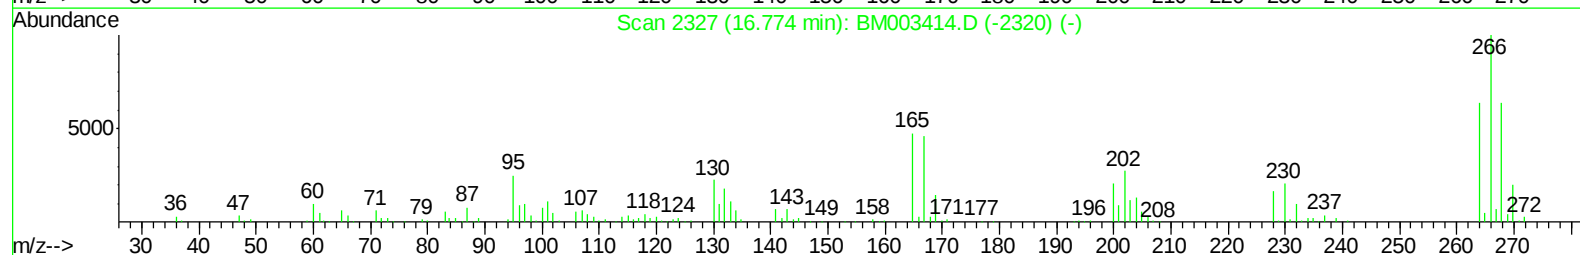
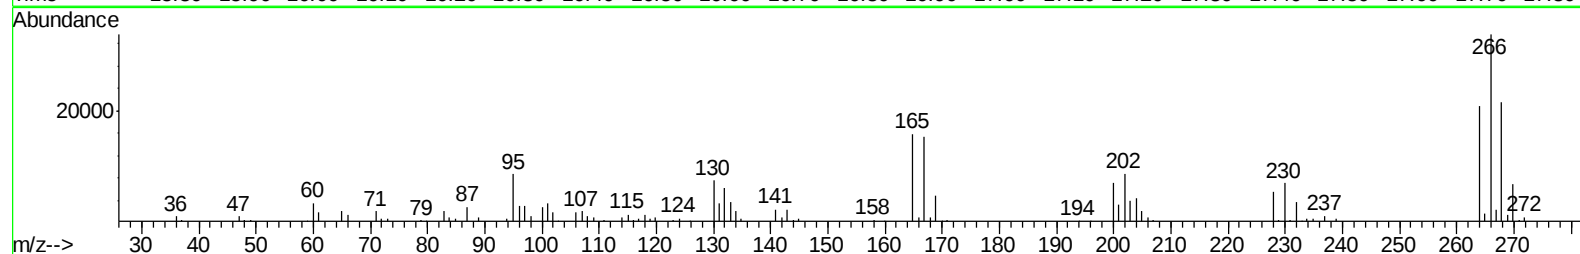


Data Path : Z:\HPCHEM1\BNA M\DATA\BM122315\
Data File : BM003724.D
Acq On : 23 Dec 2015 00:51
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 05:29:21 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

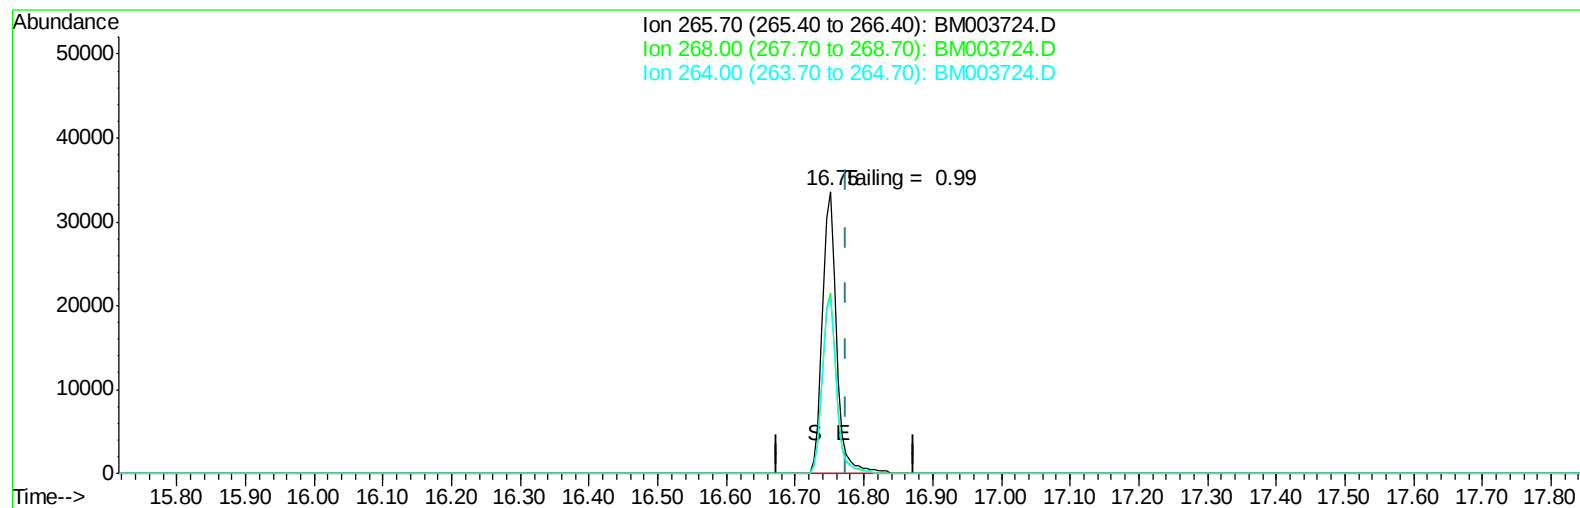

TIC: BM003724.D

(69) Pentachlorophenol (C)




16.751min (-0.023) 0.00ng

response 48062

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.27
264.00	61.20	62.22
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122315\
Data File : BM003724.D
Acq On : 23 Dec 2015 00:51
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 05:29:21 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

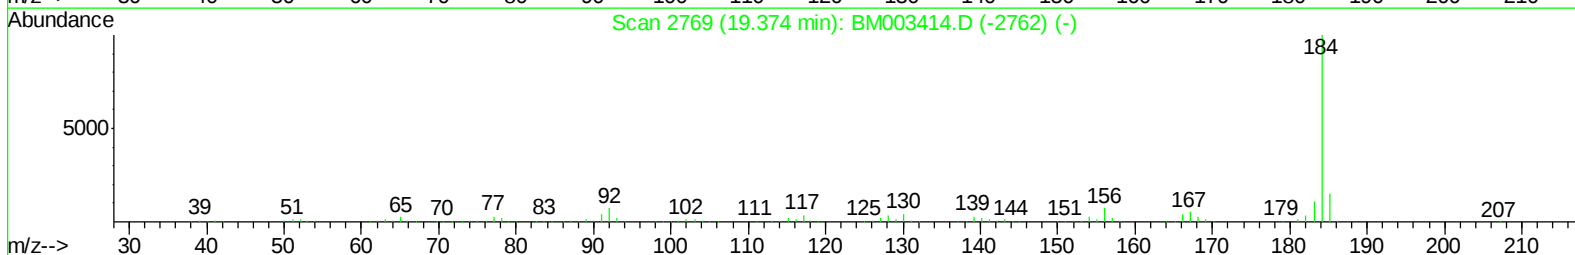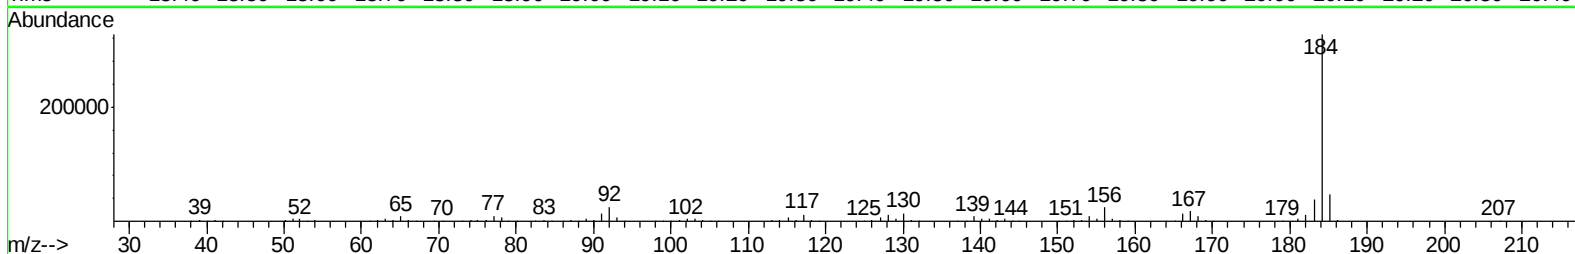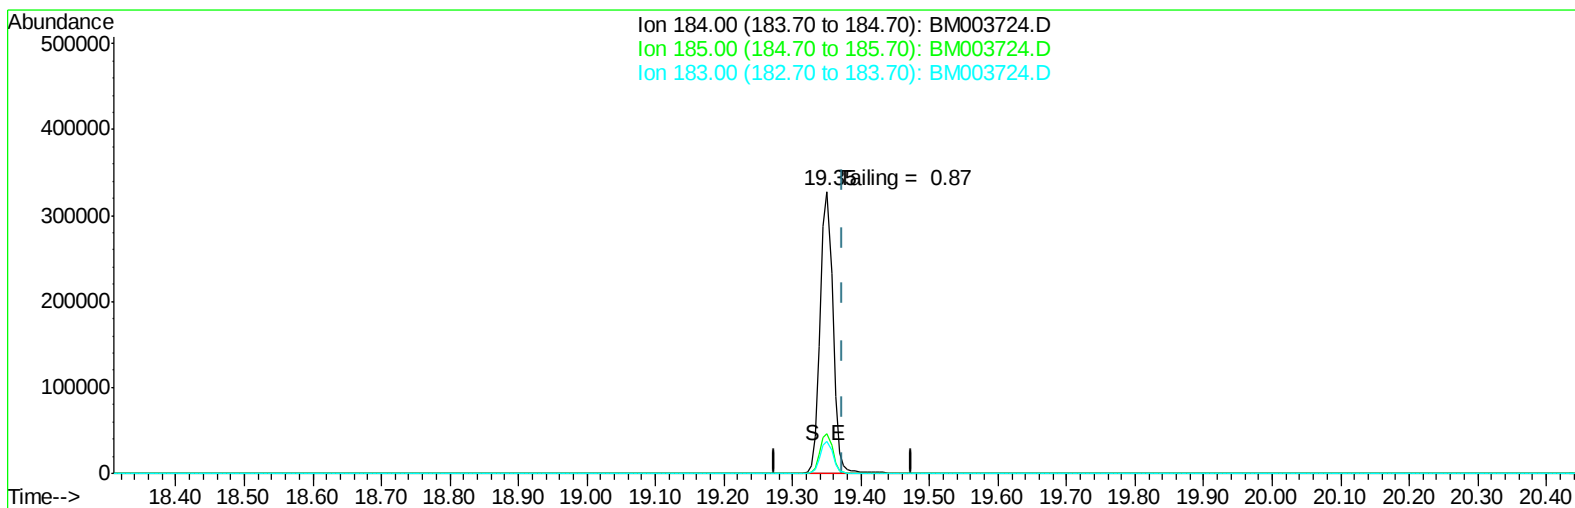

TIC: BM003724.D

(76) Benzidine

19.351min (-0.023) 0.00ng

response 419699

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.33
183.00	11.10	11.54
0.00	0.00	0.00