

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122315\
 Data File : BM003719.D
 Acq On : 22 Dec 2015 21:50
 Operator : UM/SJ
 Sample : G4913-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.810	287	293	307	rBV	152331	205735	11.66%	1.885%
2	5.281	367	373	385	rBB	691542	987866	55.99%	9.052%
3	6.869	636	643	659	rBB	656066	1004887	56.95%	9.208%
4	7.228	697	704	716	rBB	702998	1087491	61.64%	9.964%
5	7.692	777	783	789	rBB	116424	173569	9.84%	1.590%
6	8.010	831	837	845	rBB	549835	871794	49.41%	7.988%
7	8.851	973	980	993	rBB	391223	617369	34.99%	5.657%
8	10.480	1250	1257	1268	rBB	145988	235734	13.36%	2.160%
9	12.963	1672	1679	1691	rBB	966885	1416904	80.31%	12.983%
10	13.804	1816	1822	1831	rBB	114086	156399	8.86%	1.433%
11	14.345	1908	1914	1921	rBB2	186231	279313	15.83%	2.559%
12	15.839	2162	2168	2177	rBB	640880	868025	49.20%	7.953%
13	16.062	2202	2206	2217	rBB	16564	25859	1.47%	0.237%
14	17.092	2376	2381	2390	rVB	236718	321746	18.24%	2.948%
15	19.733	2824	2830	2835	rBV	1366561	1764397	100.00%	16.167%
16	21.292	3090	3095	3101	rBV	338015	419487	23.78%	3.844%
17	23.538	3470	3477	3486	rVB2	239596	437893	24.82%	4.012%
18	24.791	3687	3690	3698	rVB2	10009	18877	1.07%	0.173%
19	26.685	4007	4012	4019	rVB3	8149	20429	1.16%	0.187%


Sum of corrected areas: 10913774

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122315\
Data File : BM003719.D
Acq On : 22 Dec 2015 21:50
Operator : UM/SJ
Sample : G4913-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-2

Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

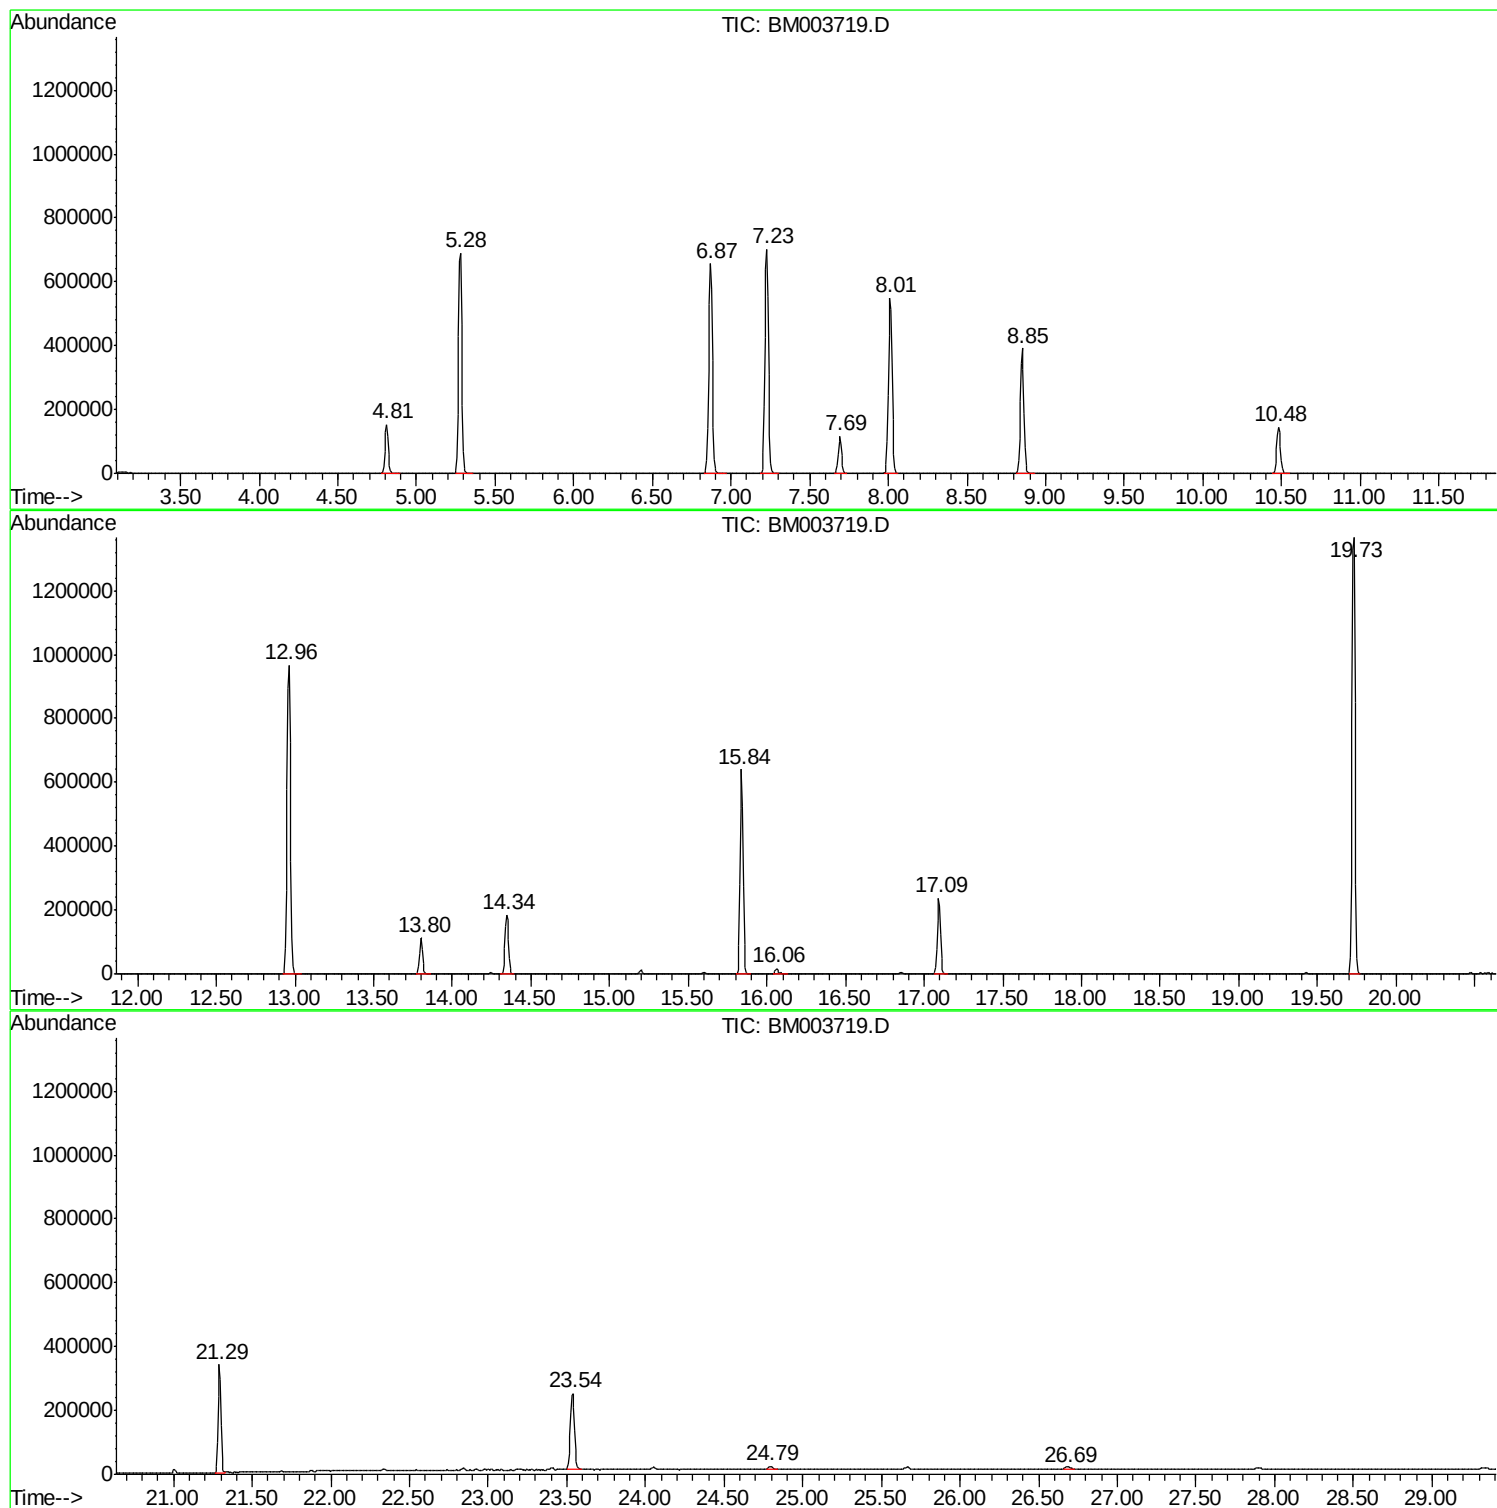

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122315\
Data File : BM003719.D
Acq On : 22 Dec 2015 21:50
Operator : UM/SJ
Sample : G4913-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-2










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.81	23.71 ng	205735	1,4-Dichlorobenzene-d4	7.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	17
3		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17
4		(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9
5		5-Hexen-2-one	98	C6H10O	000109-49-9	9

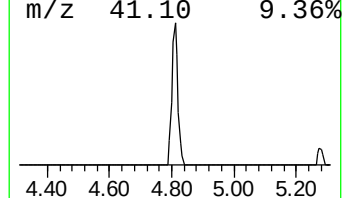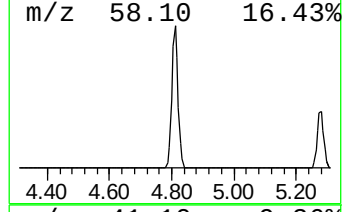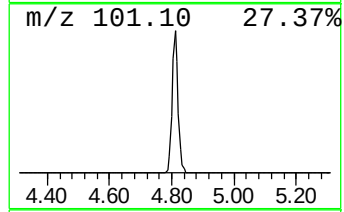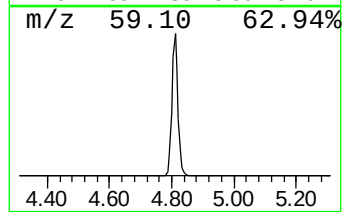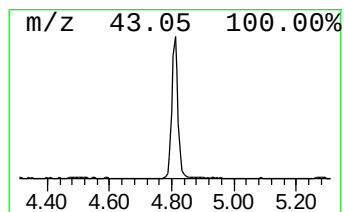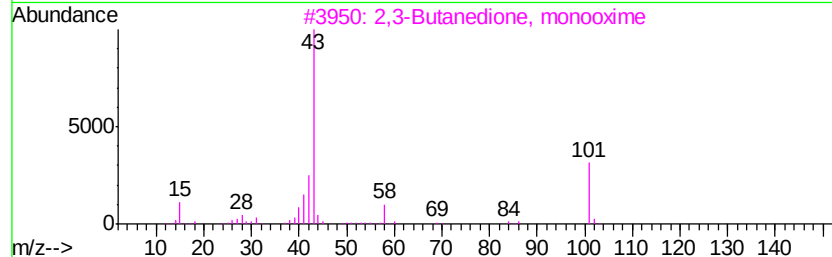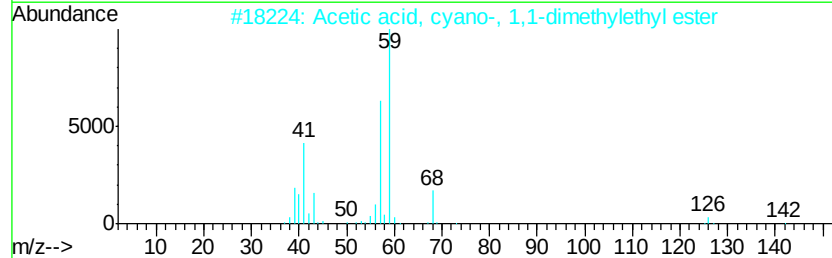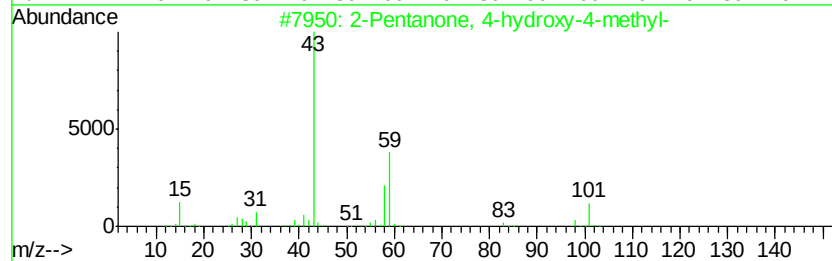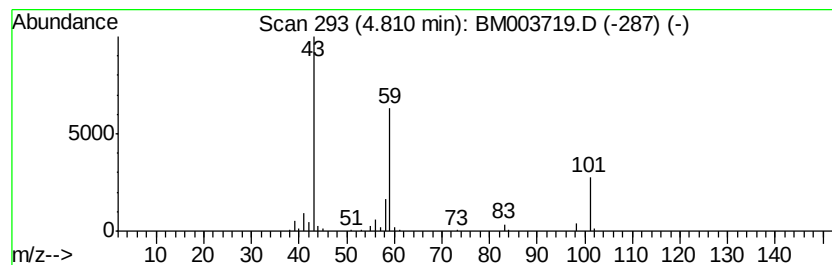

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122315\
Data File : BM003719.D
Acq On : 22 Dec 2015 21:50
Operator : UM/SJ
Sample : G4913-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-2










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.23 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.23	125.31 ng	1087490	1,4-Dichlorobenzene-d4	7.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
3		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

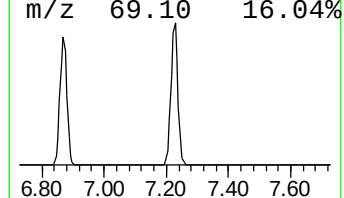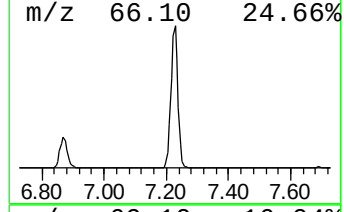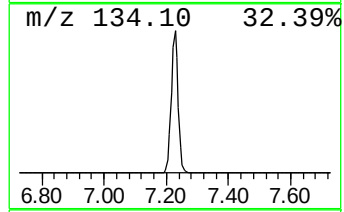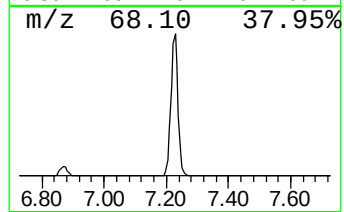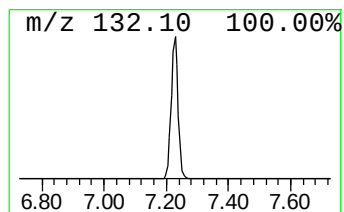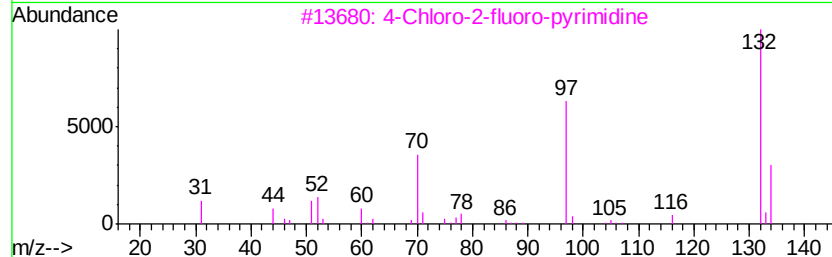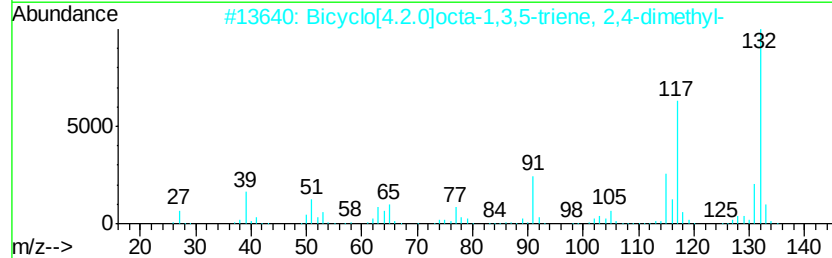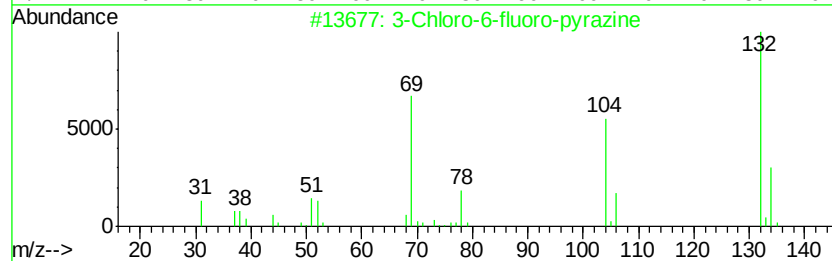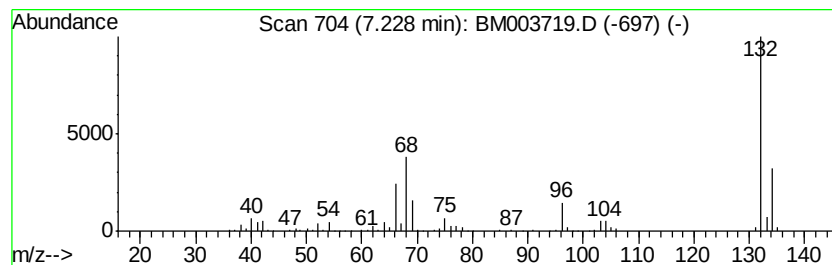

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122315\
Data File : BM003719.D
Acq On : 22 Dec 2015 21:50
Operator : UM/SJ
Sample : G4913-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.81	23.7	ng	205735	1	7.69	173569	20.0
unknown7.23	7.23	125.3	ng	1087490	1	7.69	173569	20.0