


Data Path : Z:\HPCHEM1\BNA M\DATA\BM122315\
 Data File : BM003706.D
 Acq On : 22 Dec 2015 13:54
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 09 18:52:47 2015

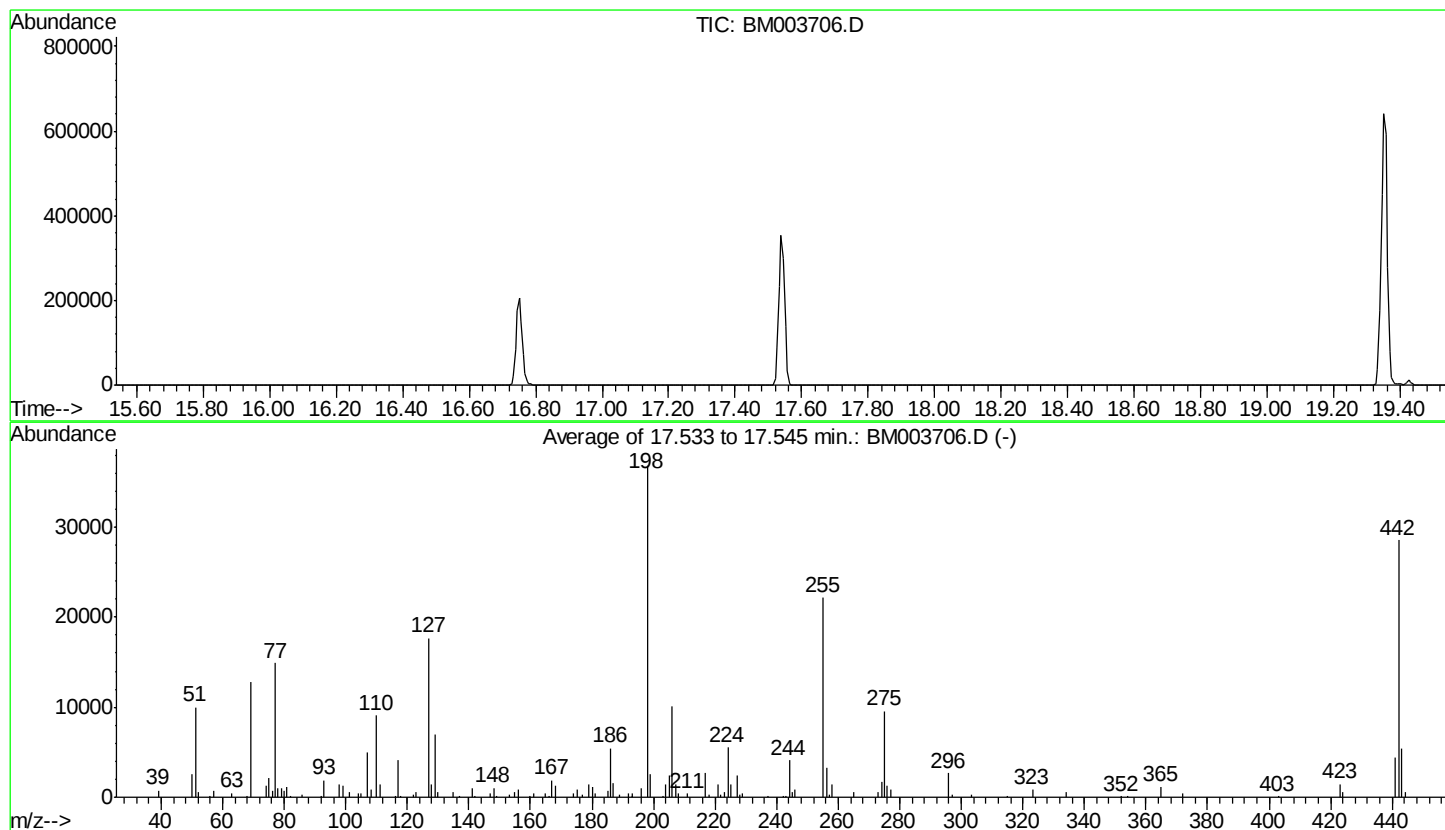

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	9964	PASS
68	69	0.00	2	0.8	101	PASS
69	198	0.00	100	34.8	12800	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	17642	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	36816	PASS
199	198	5	9	6.8	2517	PASS
275	198	10	60	25.9	9529	PASS
365	198	1	100	3.2	1189	PASS
441	442	0.01	24	15.6	4450	PASS
442	198	50	100	77.5	28546	PASS
443	442	15	24	19.2	5468	PASS