

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:58:42 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

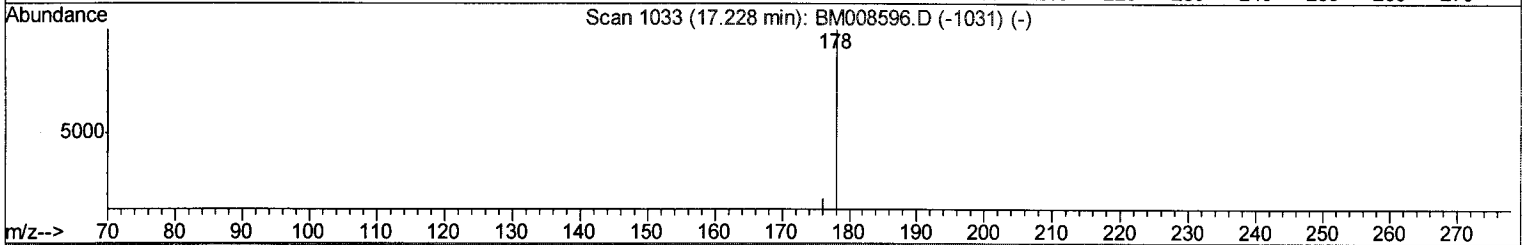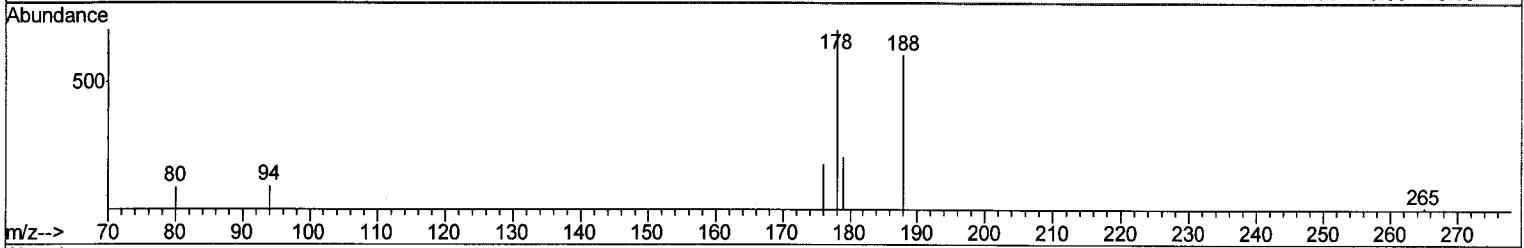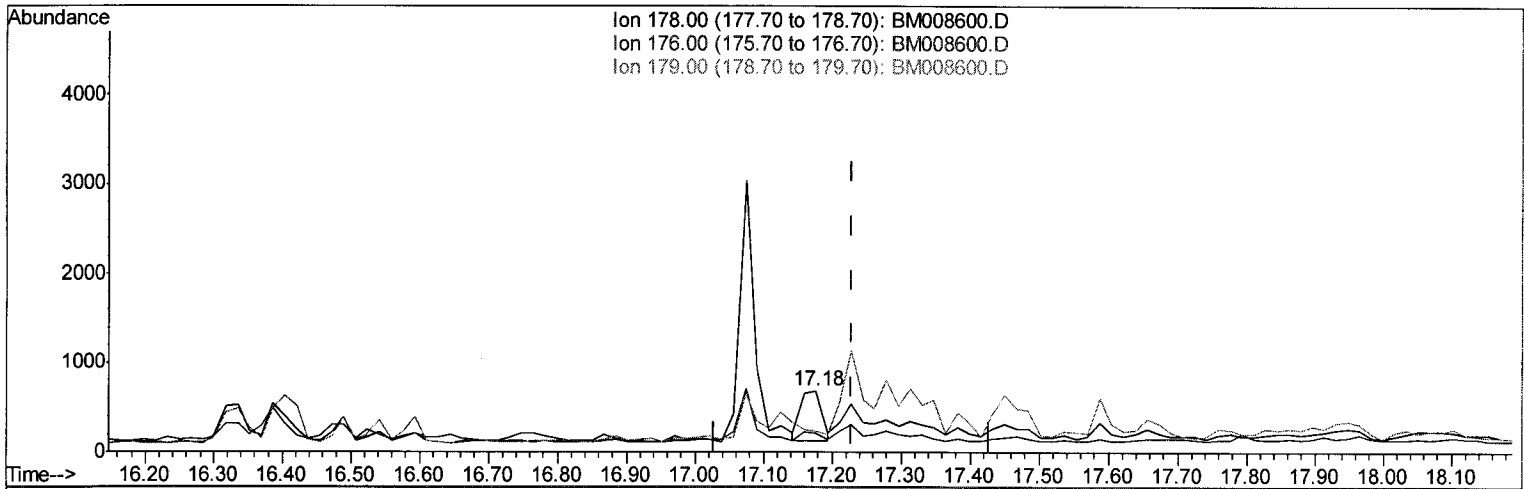

TIC: BM008600.D

(13) Anthracene

17.176min (-0.051) 0.16ng/ul m

response 1198

5.5
 12/27/2016

Ion	Exp%	Act%
178.00	100	100
176.00	22.60	30.88#
179.00	18.40	34.71#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Quant Time: Dec 23 23:58:42 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

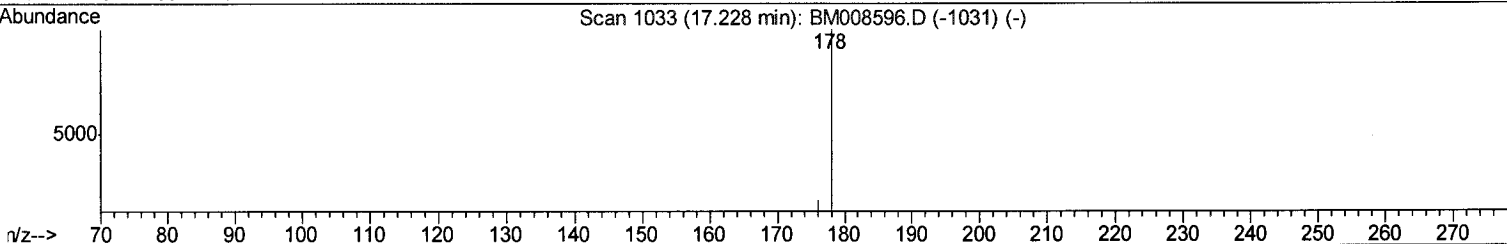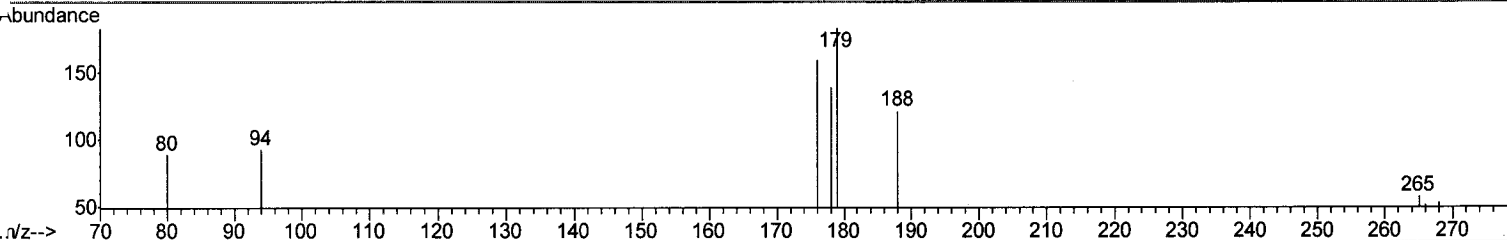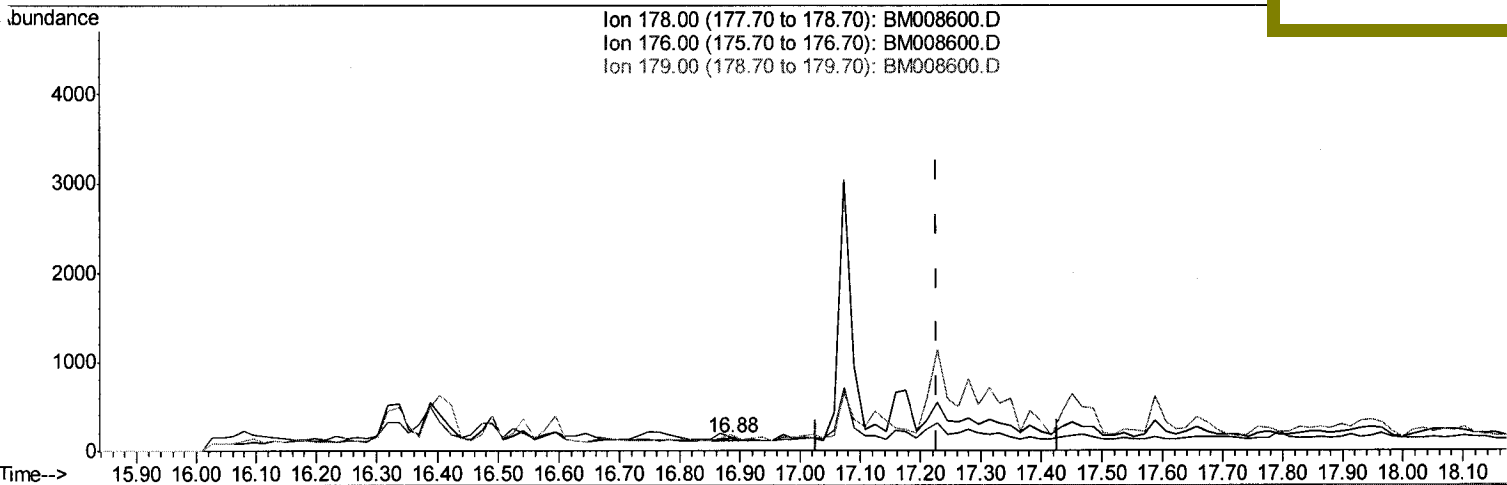

TIC: BM008600.D

(13) Anthracene

16.885min (-0.343) 0.01ng/ul

response 90

Ion	Exp%	Act%
178.00	100	100
176.00	22.60	114.39#
179.00	18.40	131.65#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:56:59 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

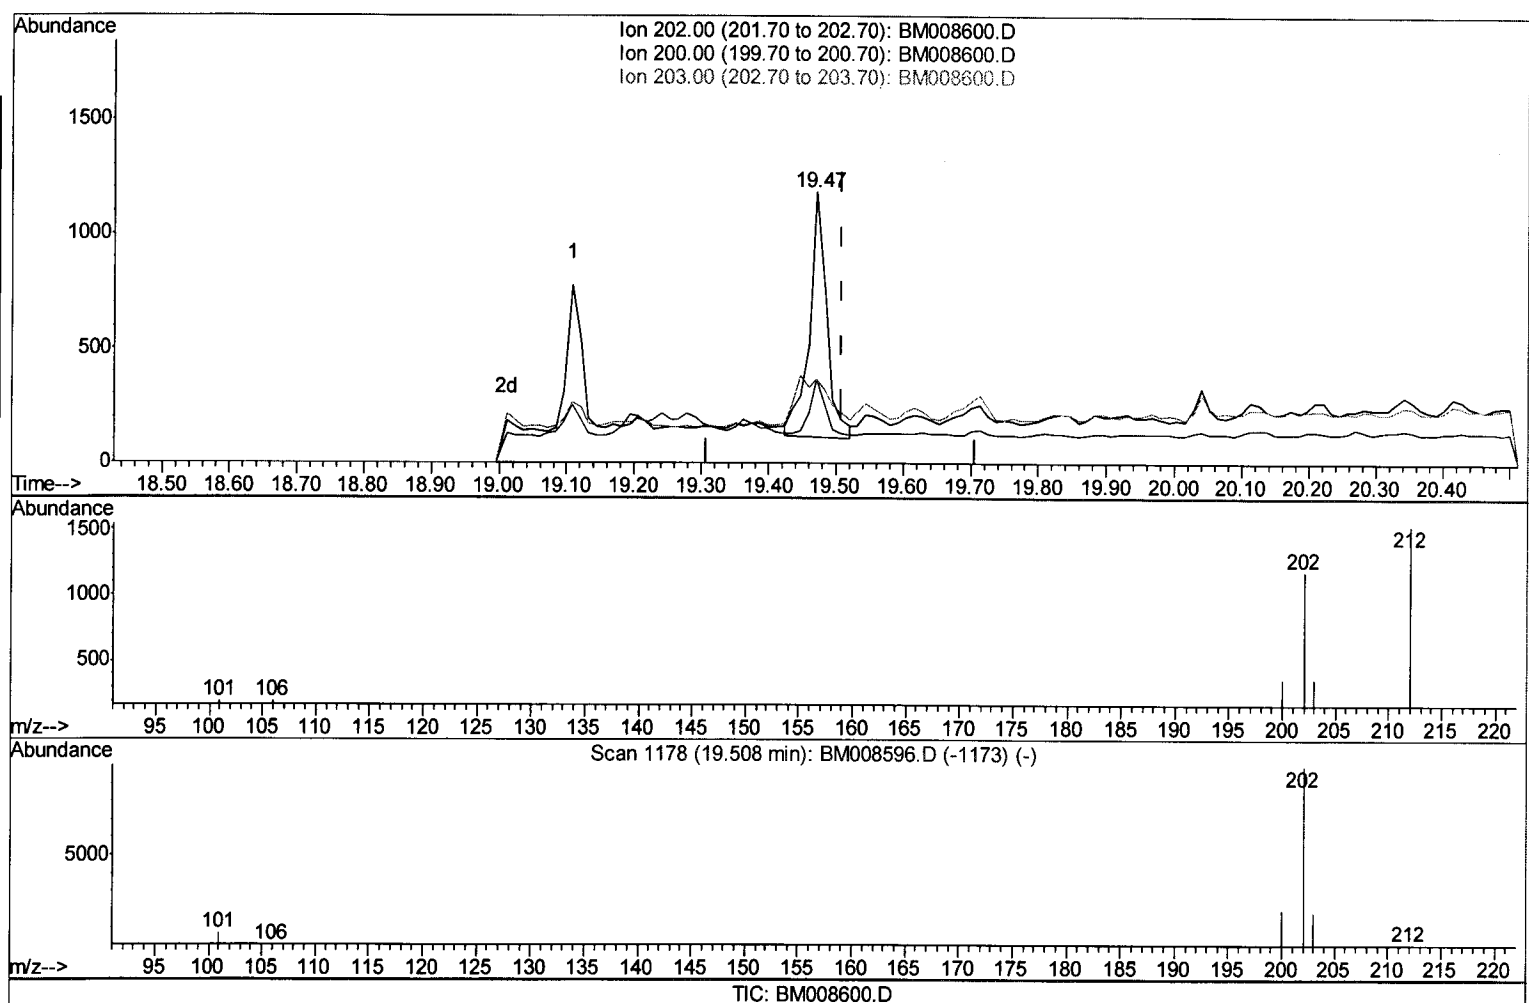

(17) Pyrene

19.471min (-0.036) 0.31ng/ul m

response 1964

Ion	Exp%	Act%
202.00	100	100
200.00	22.80	30.72#
203.00	19.50	30.80#
0.00	0.00	0.00

SS
 12/27/2016




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
Data File : BM008600.D
Acq On : 23 Dec 2016 17:57
Operator : UM/SJ
Sample : H6040-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8X0

Manual Integrations
APPROVED

sohil
12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:56:59 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 23:37:39 2016
Response via : Initial Calibration

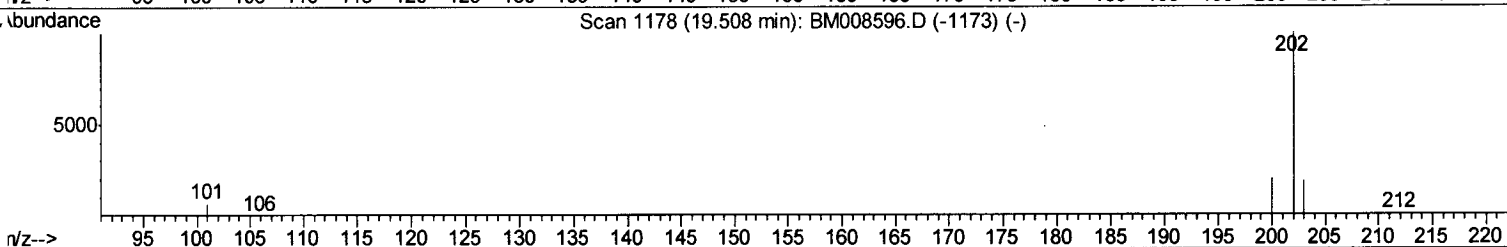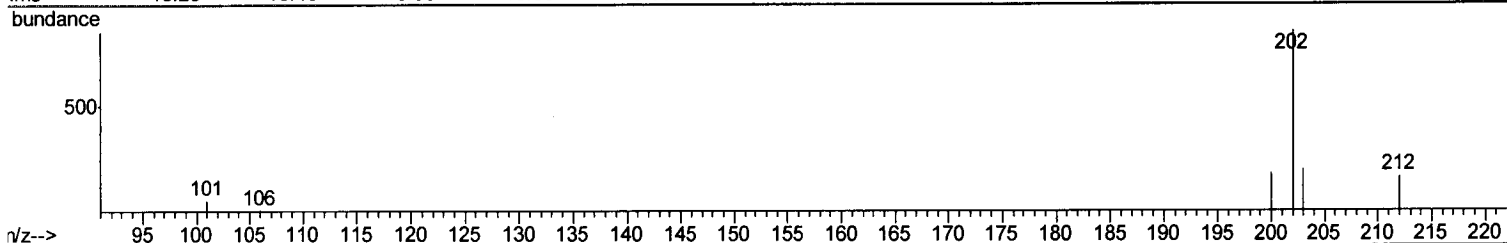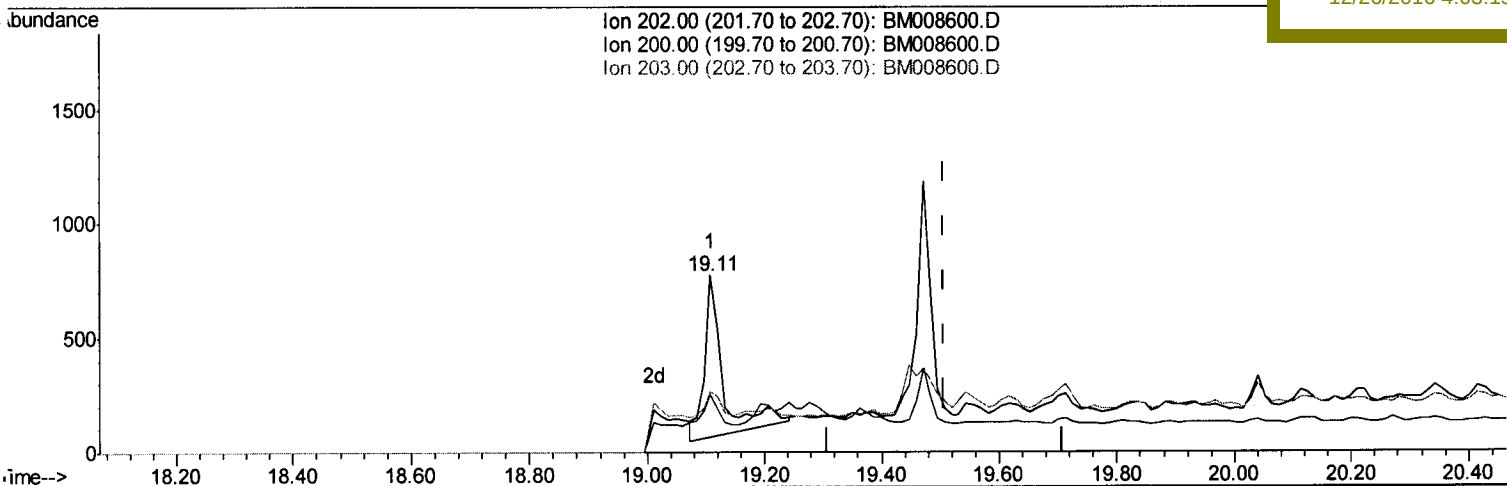

TIC: BM008600.D

(17) Pyrene

19.108min (-0.399) 0.24ng/ul

response 1537

Ion	Exp%	Act%
202.00	100	100
200.00	22.80	32.82#
203.00	19.50	34.37#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:56:59 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

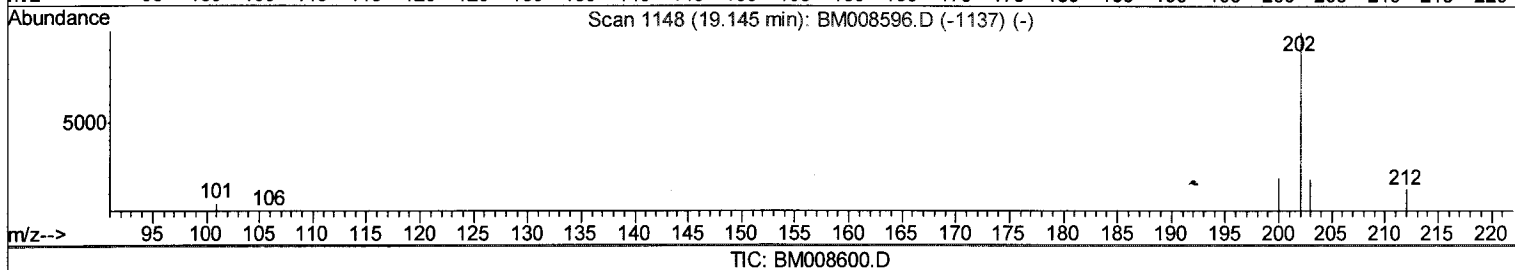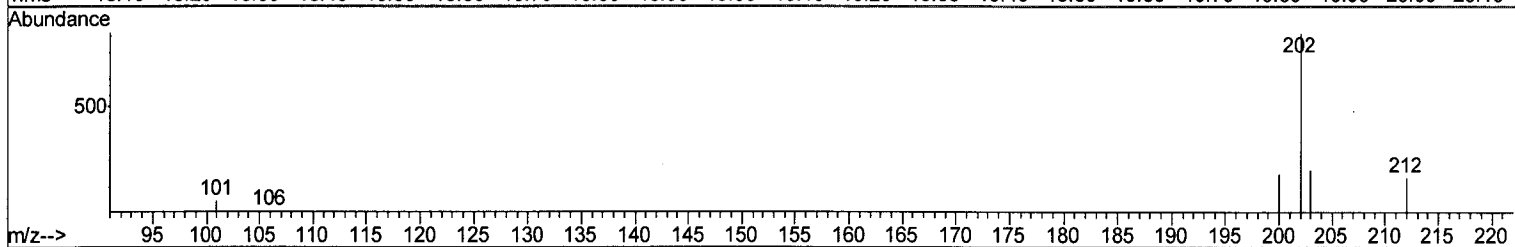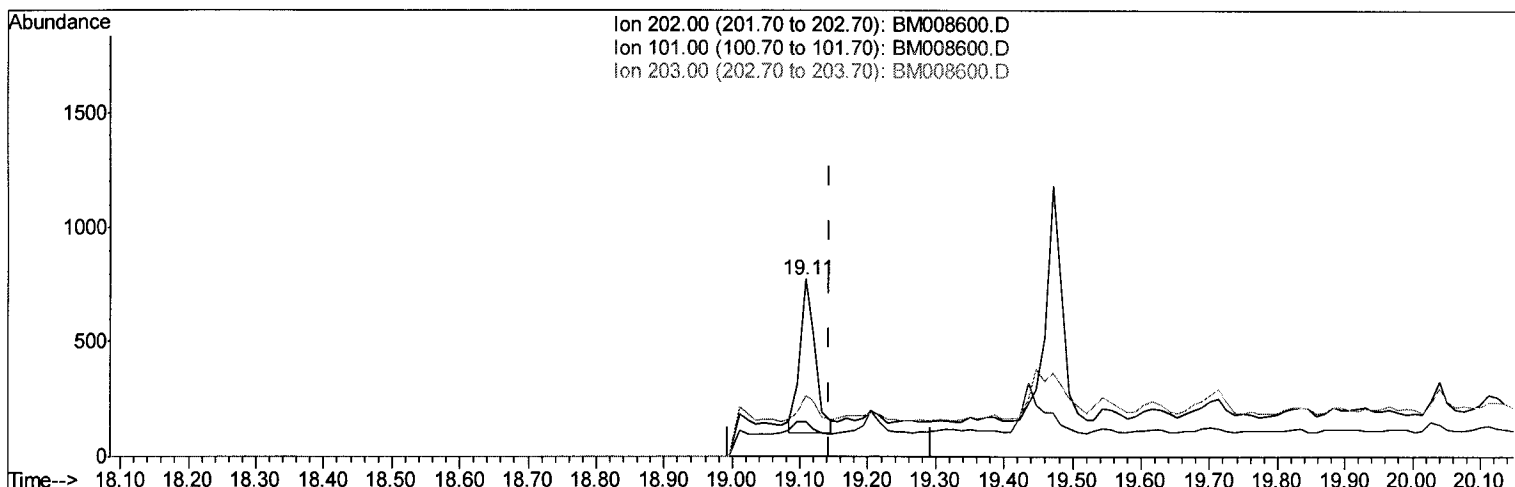

(15) Fluoranthene (C)

19.108min (-0.036) 0.11ng/ul m

response 1060

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	19.77
203.00	19.50	34.37
0.00	0.00	0.00

S.J.
 12/27/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DA8X0

Quant Time: Dec 23 23:56:59 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
 12/26/2016 4:03:15 PM

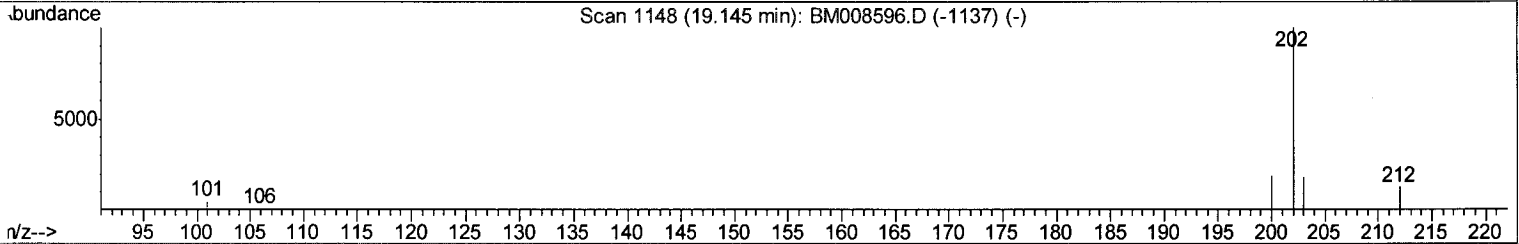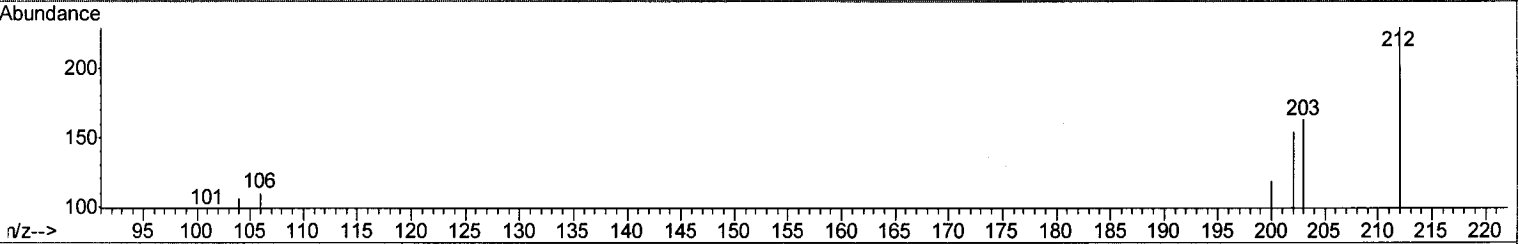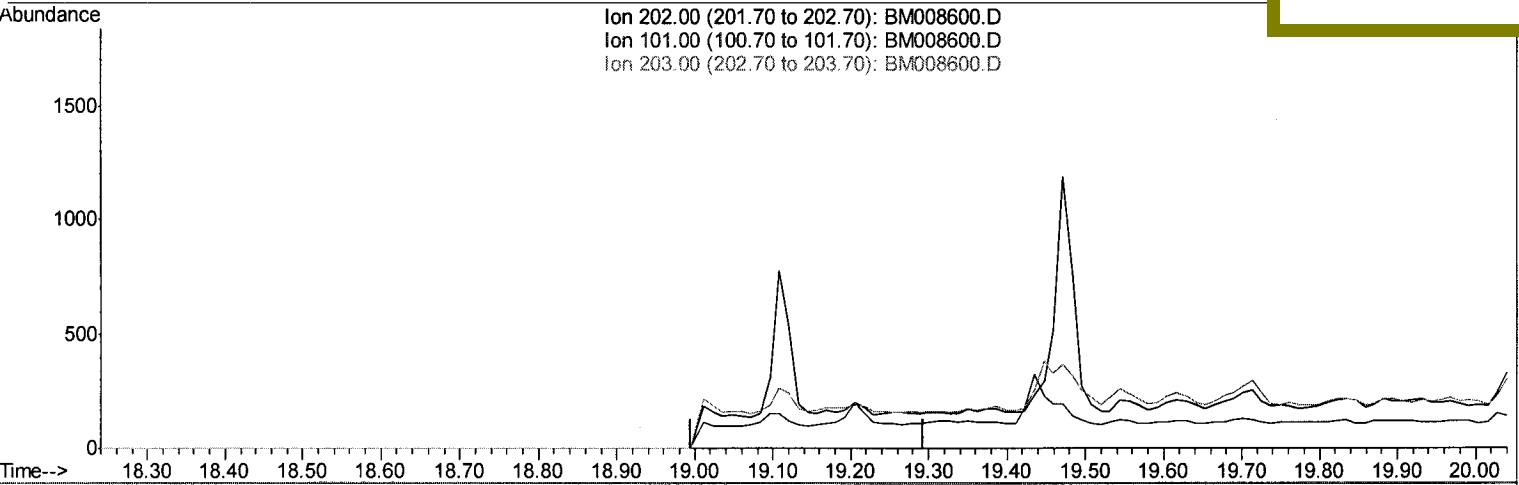

(15) Fluoranthene (C)

19.145min (-19.145) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	10.30	0.00
203.00	19.50	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:56:59 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

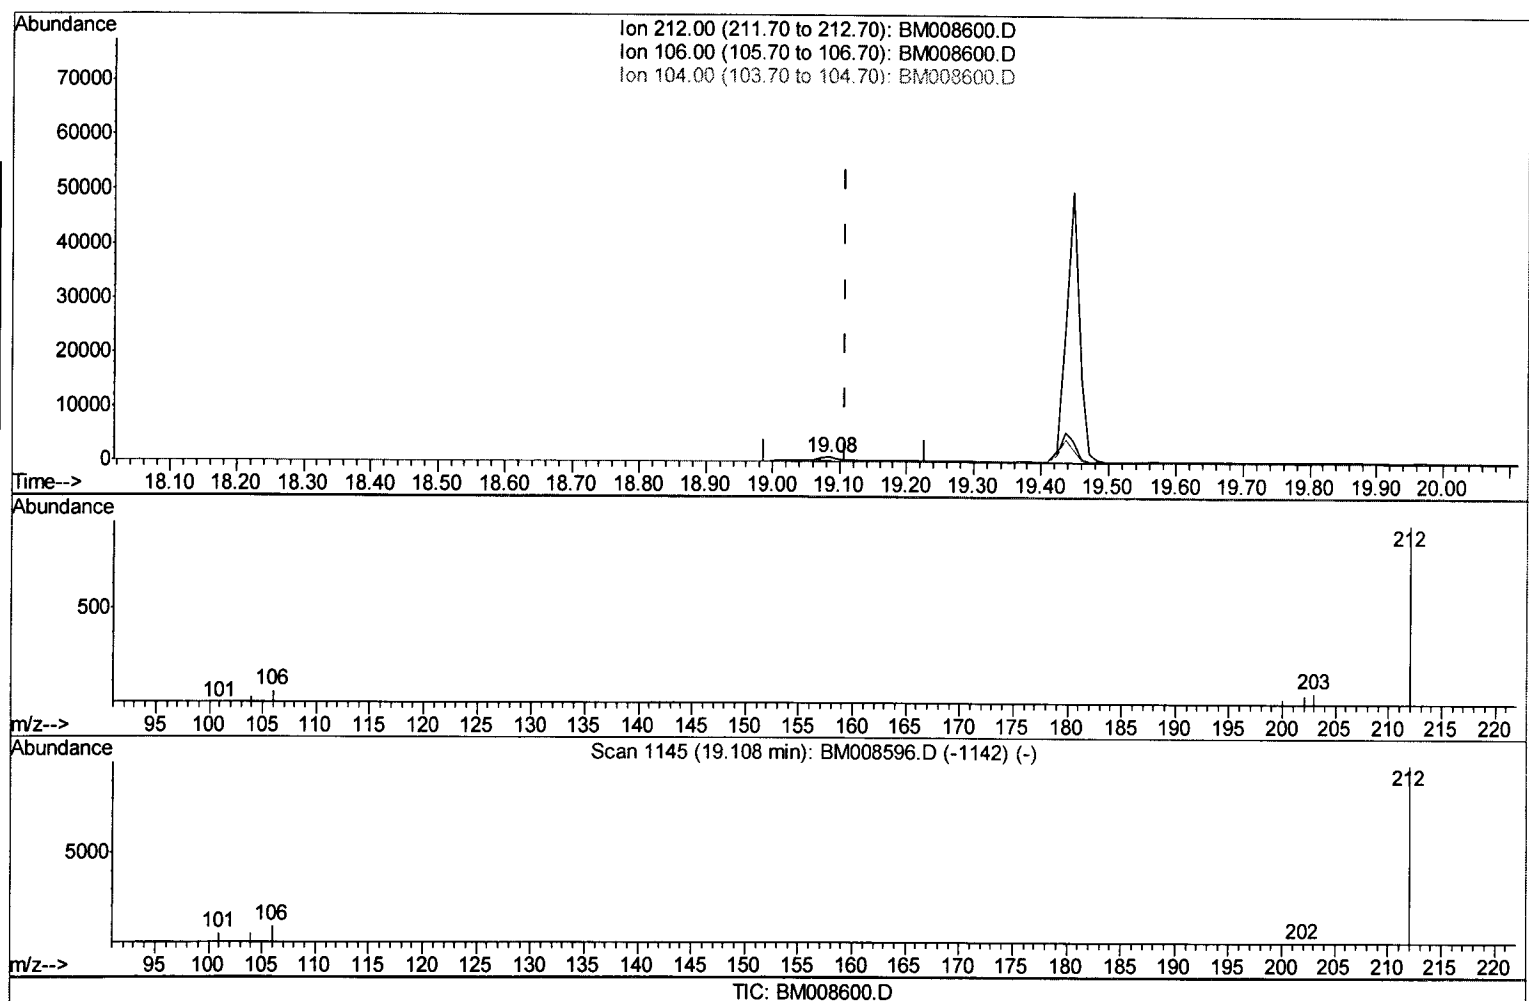

(14) Fluoranthene-d10 (SURR)

19.084min (-0.024) 0.26ng/ul m

response 1811

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

S.D.
 12/27/2016




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
Data File : BM008600.D
Acq On : 23 Dec 2016 17:57
Operator : UM/SJ
Sample : H6040-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8X0

Manual Integrations
APPROVED

sohil
12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:56:59 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 23:37:39 2016
Response via : Initial Calibration

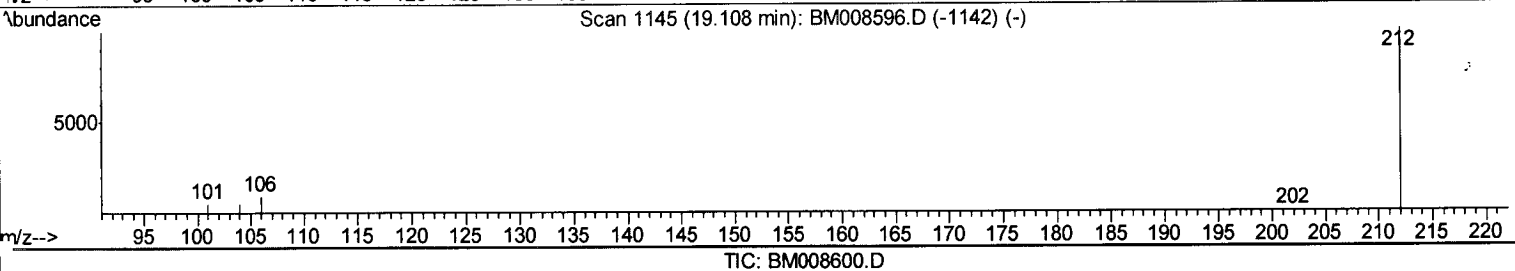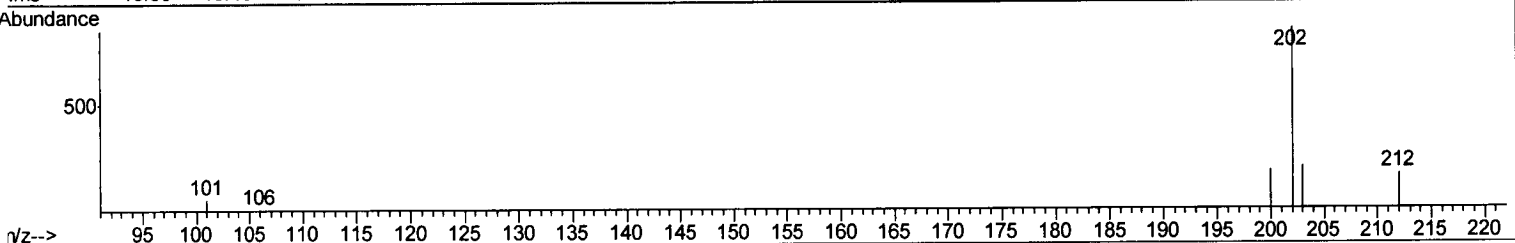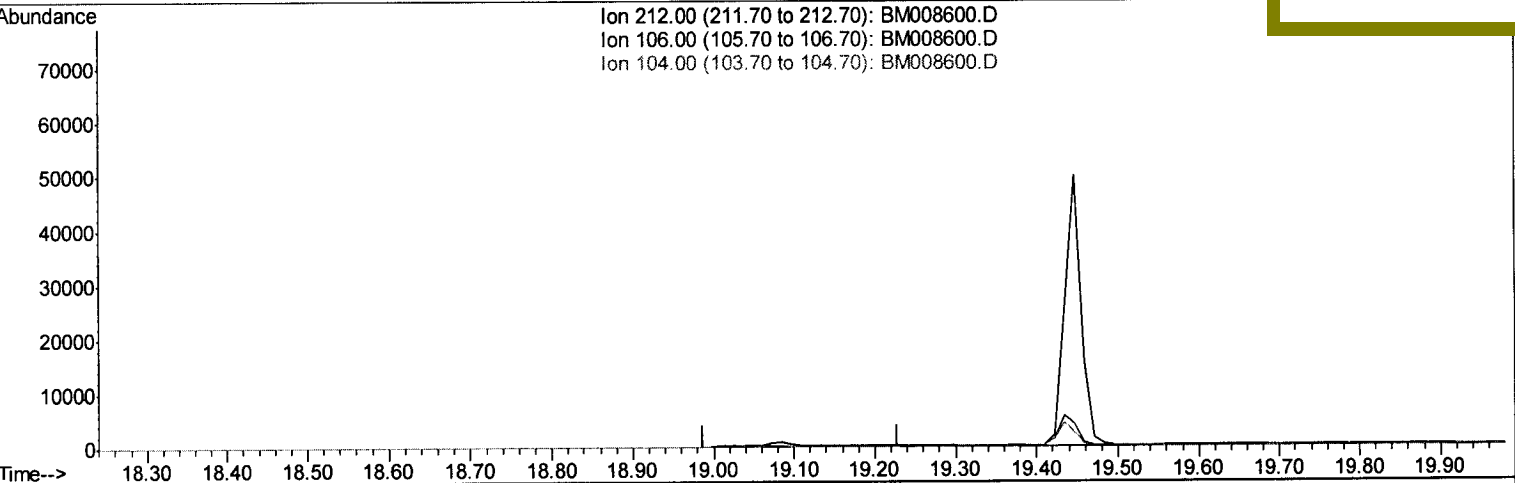

(14) Fluoranthene-d10 (SURR)

19.108min (-19.108) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:56:59 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

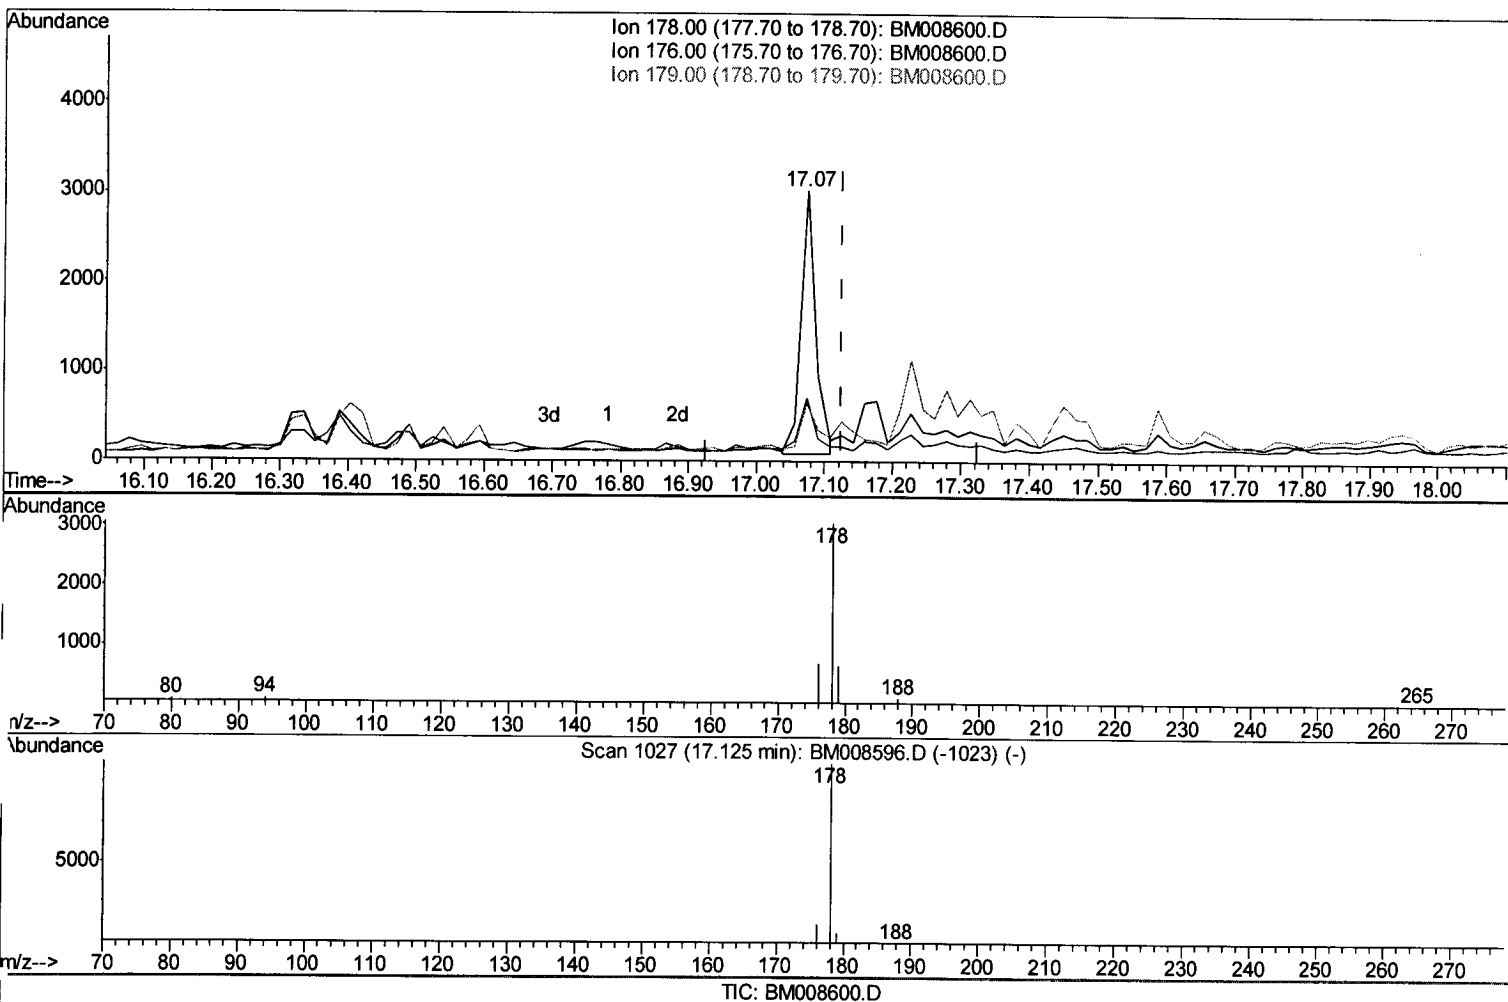

(12) Phenanthrene

17.073min (-0.051) 0.57ng/ul m

response 4449

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	22.97
179.00	17.00	21.56#
0.00	0.00	0.00

50
 12/27/2016




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
Data File : BM008600.D
Acq On : 23 Dec 2016 17:57
Operator : UM/SJ
Sample : H6040-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8X0

Manual Integrations
APPROVED

sohil
12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:56:59 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 23:37:39 2016
Response via : Initial Calibration

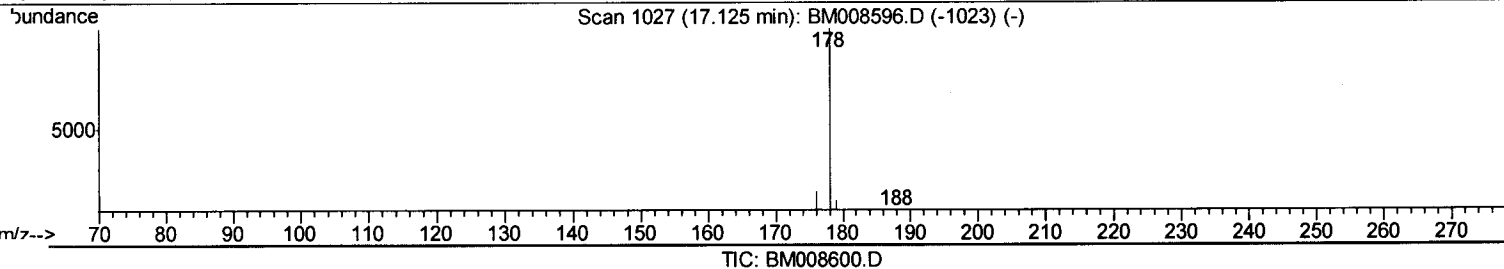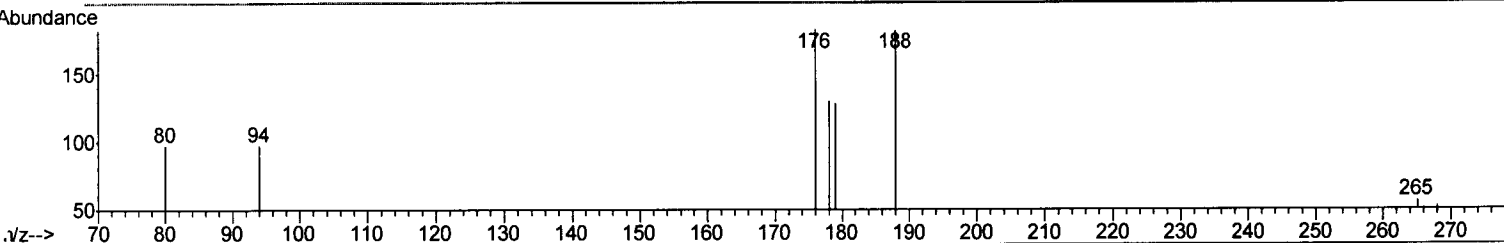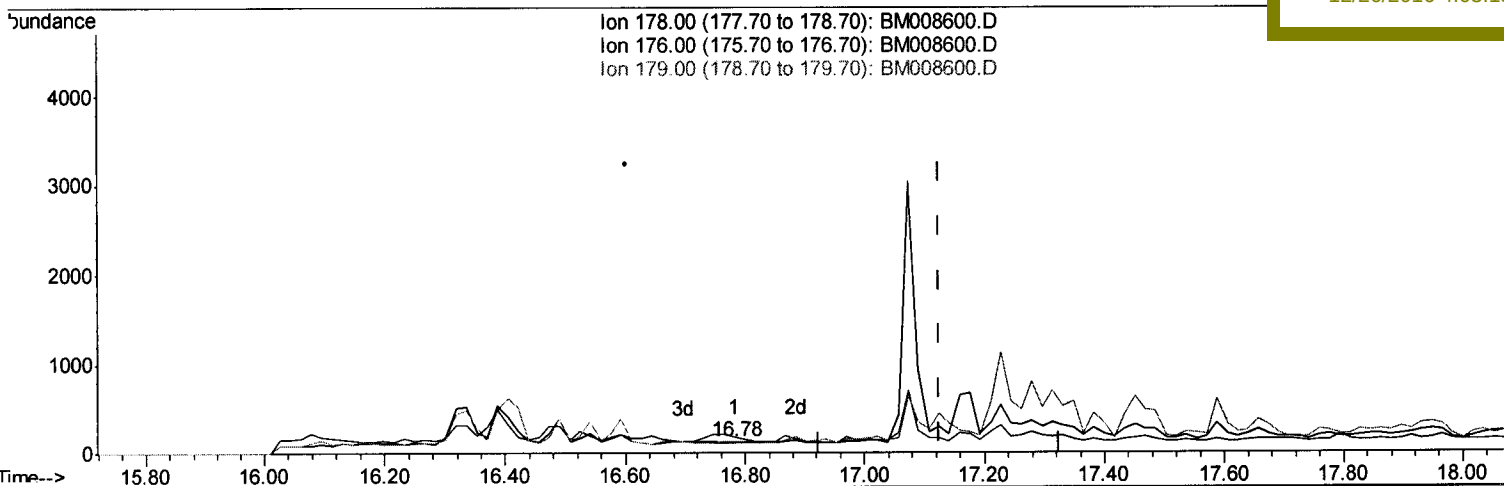

(12) Phenanthrene

16.782min (-0.343) 0.01ng/ul

response 87

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	140.77#
179.00	17.00	98.46#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:56:59 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

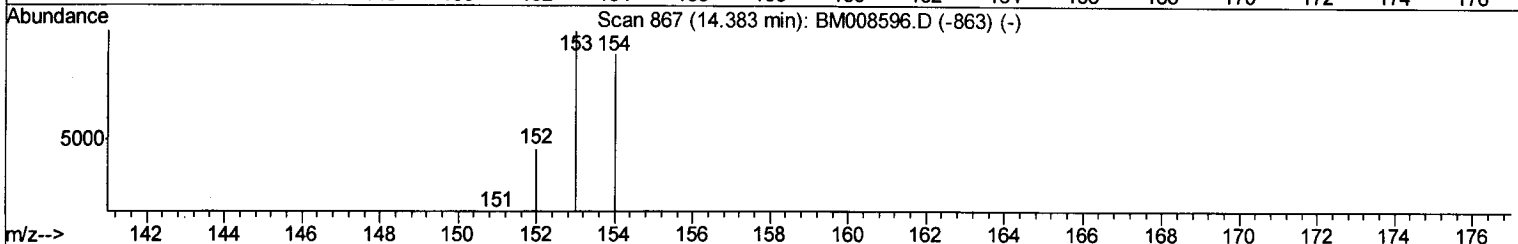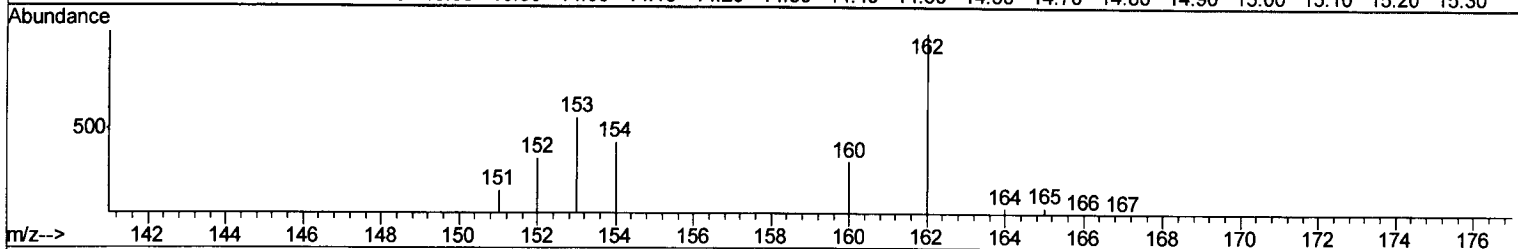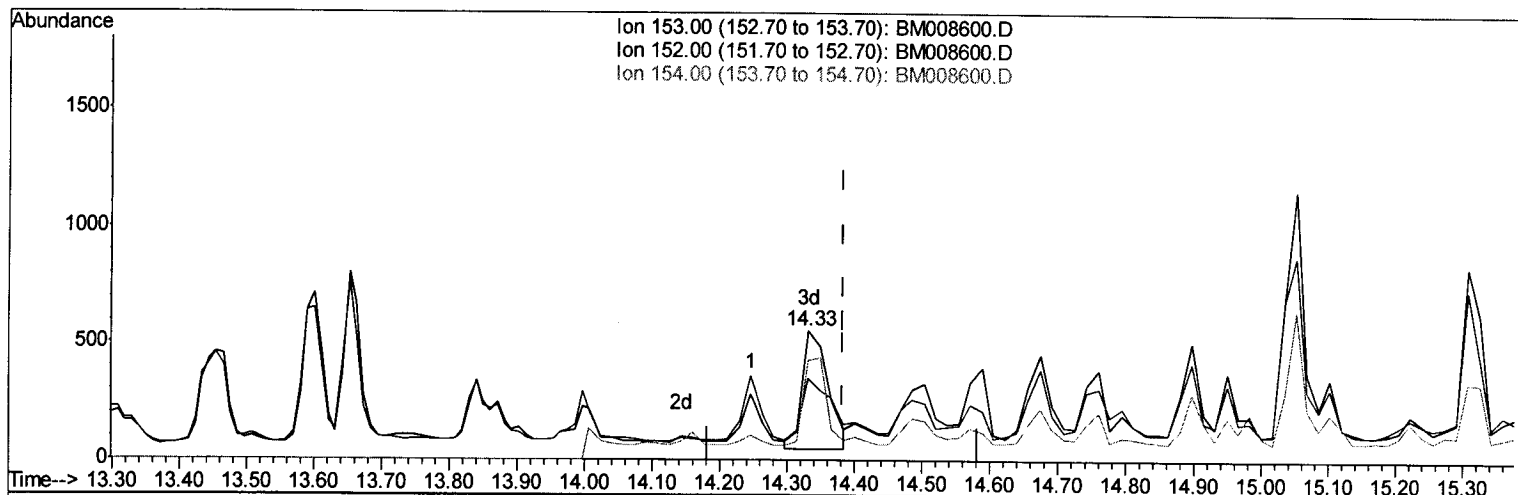

TIC: BM008600.D

(8) Acenaphthene (C)

14.331min (-0.051) 0.32ng/ul m

response 1348

Ion	Exp%	Act%
153.00	100	100
152.00	50.40	62.48#
154.00	89.30	77.02
0.00	0.00	0.00

SJ
 12/27/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
Data File : BM008600.D
Acq On : 23 Dec 2016 17:57
Operator : UM/SJ
Sample : H6040-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8X0

Manual Integrations
APPROVED

sohil
12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:56:59 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 23:37:39 2016
Response via : Initial Calibration

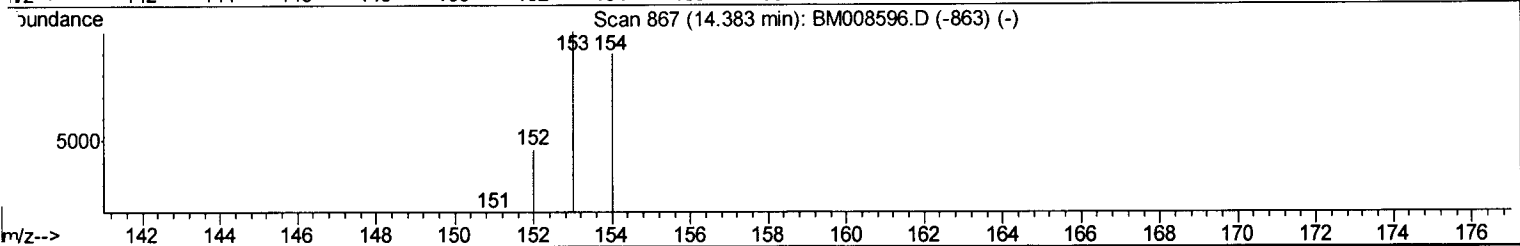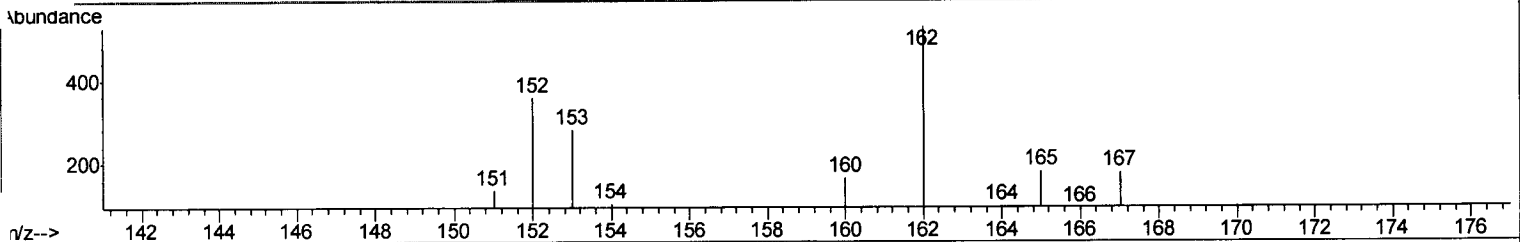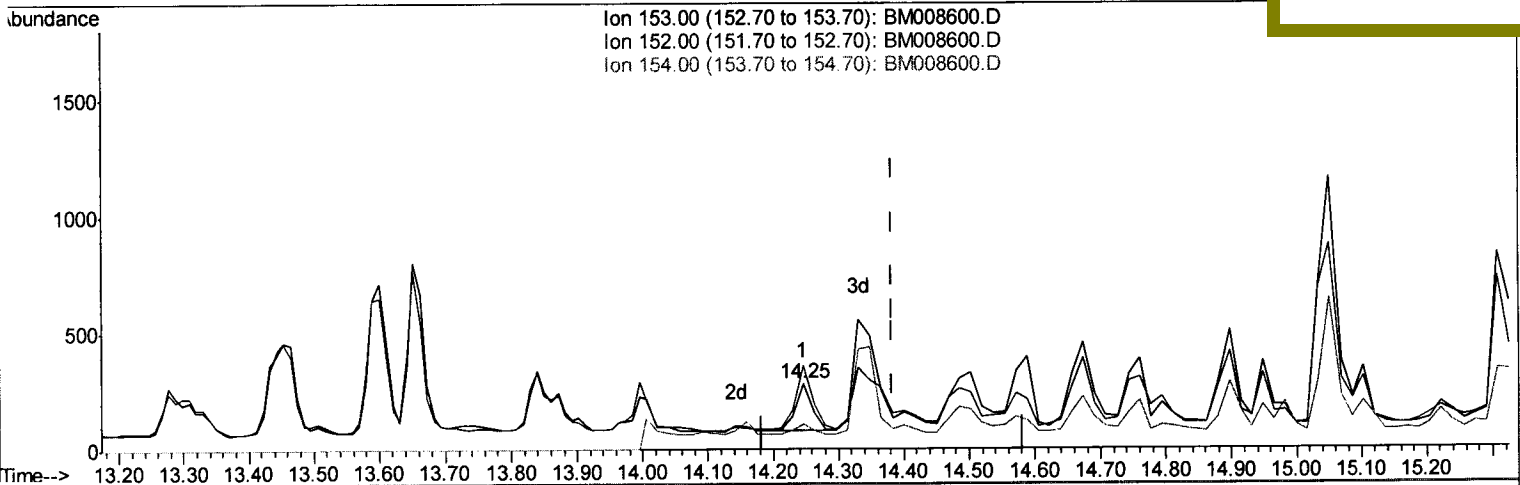

TIC: BM008600.D

(8) Acenaphthene (C)

14.246min (-0.137) 0.09ng/ul

response 372

Ion	Exp%	Act%
153.00	100	100
152.00	50.40	126.95#
154.00	89.30	37.23#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:41:37 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

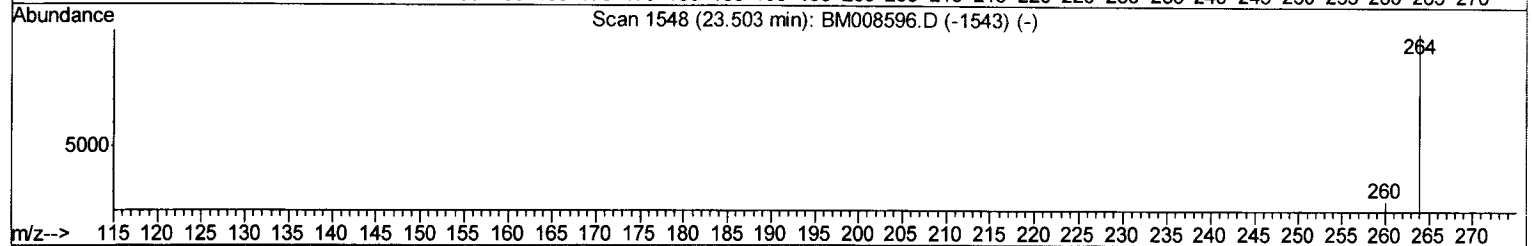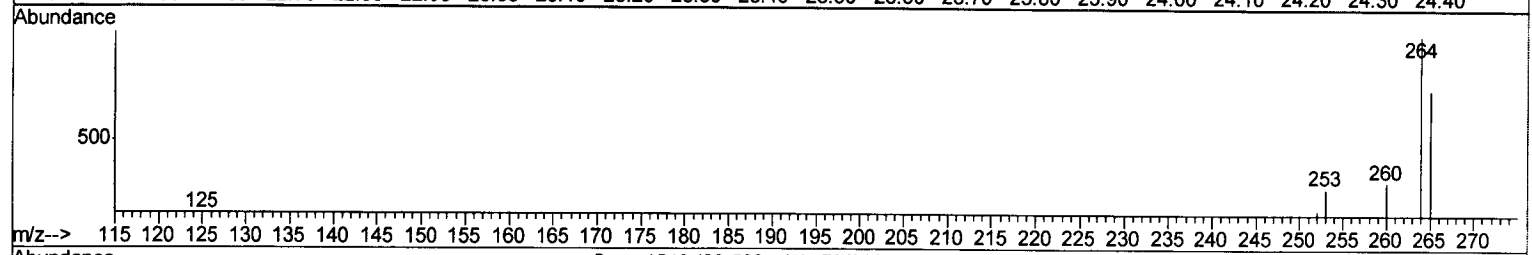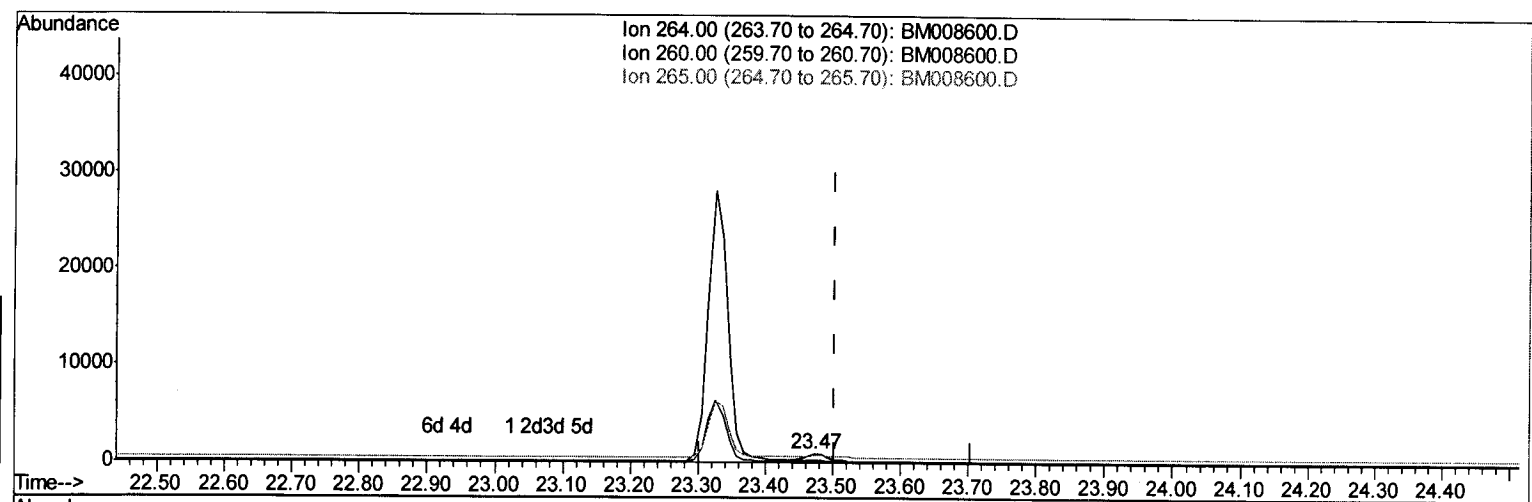

TIC: BM008600.D

(20) Perylene-d12 (I)

23.472min (-0.031) 0.40ng/ul m

response 1603

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	33.89
265.00	103.50	75.60#
0.00	0.00	0.00

5.5
 12/27/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:41:37 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

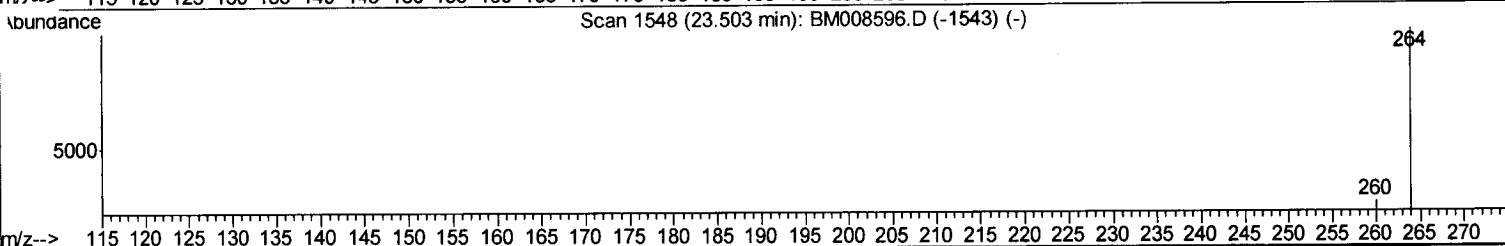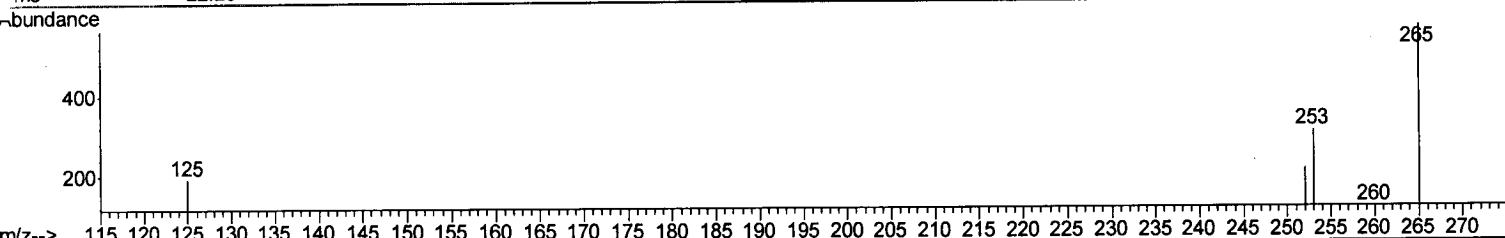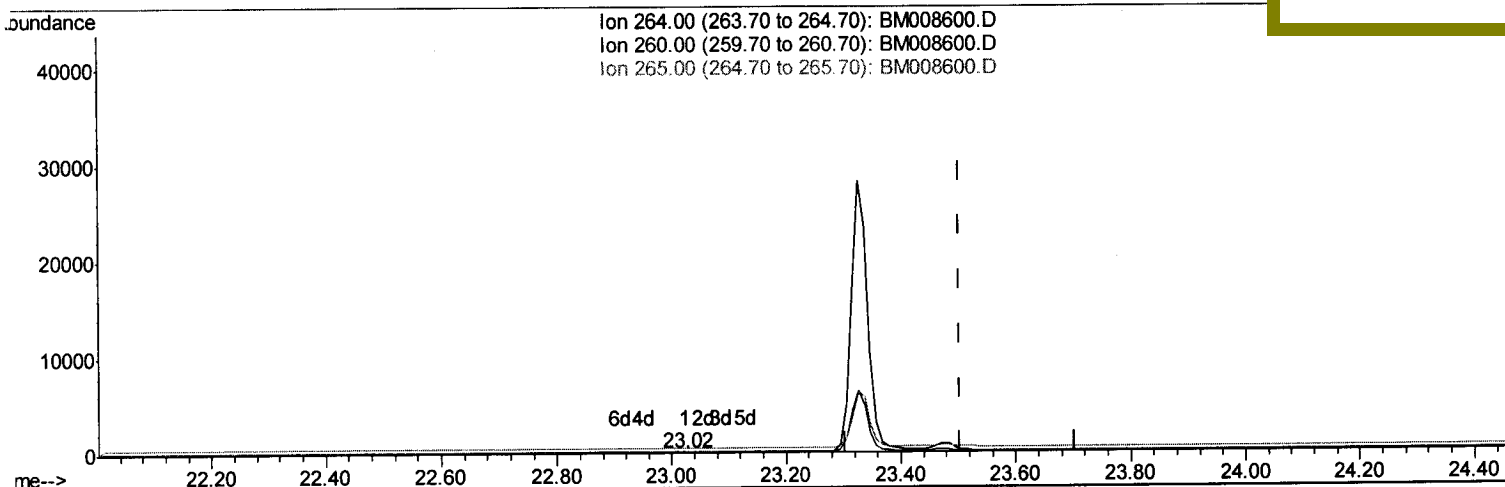

TIC: BM008600.D

(20) Perylene-d12 (I)

23.024min (-0.480) 0.40ng/ul

response 5

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	100.00#
265.00	103.50	487.93#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:41:37 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

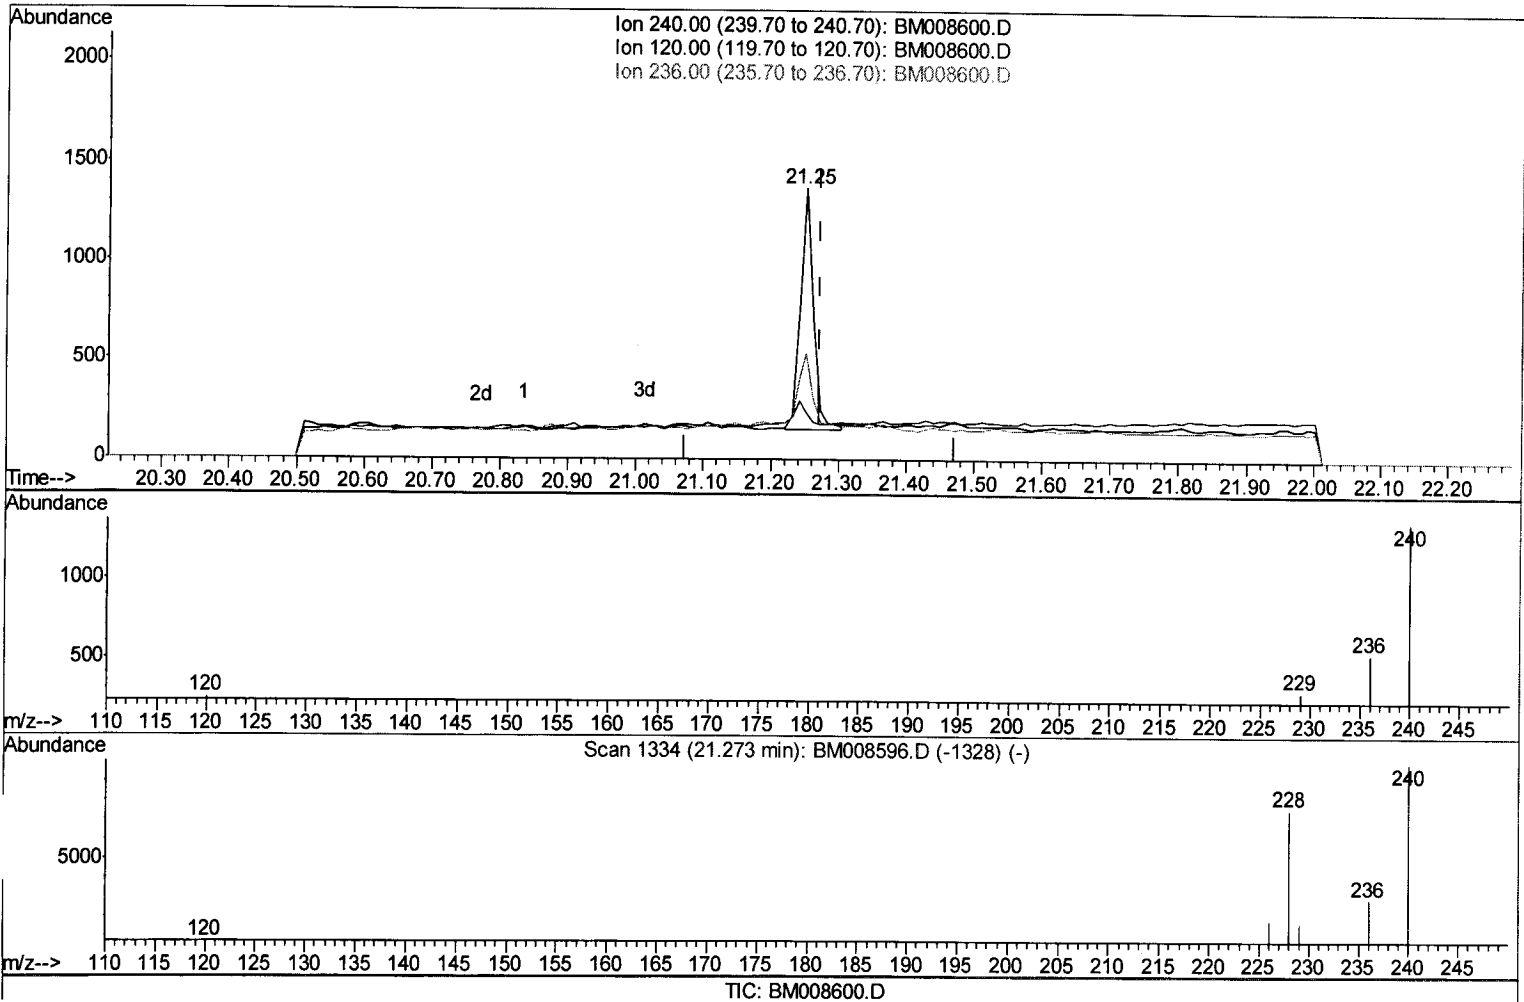

(16) Chrysene-d12 (I)

21.252min (-0.021) 0.40ng/ul m

response 1654

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	17.42
236.00	34.90	38.56
0.00	0.00	0.00

55.
 12/27/2016




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
Data File : BM008600.D
Acq On : 23 Dec 2016 17:57
Operator : UM/SJ
Sample : H6040-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8X0

Manual Integrations
APPROVED

sohil
12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:41:37 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 23:37:39 2016
Response via : Initial Calibration

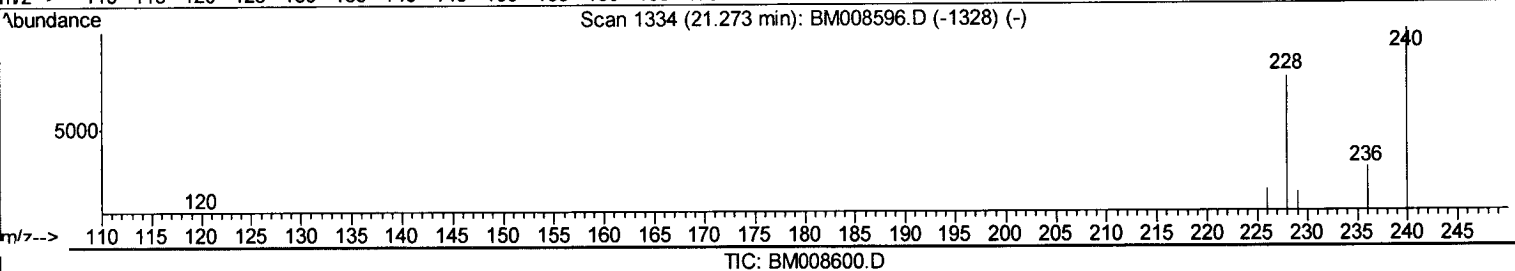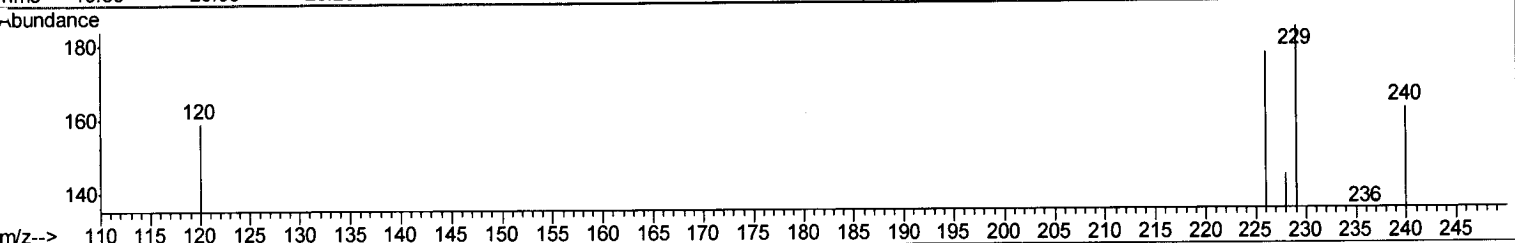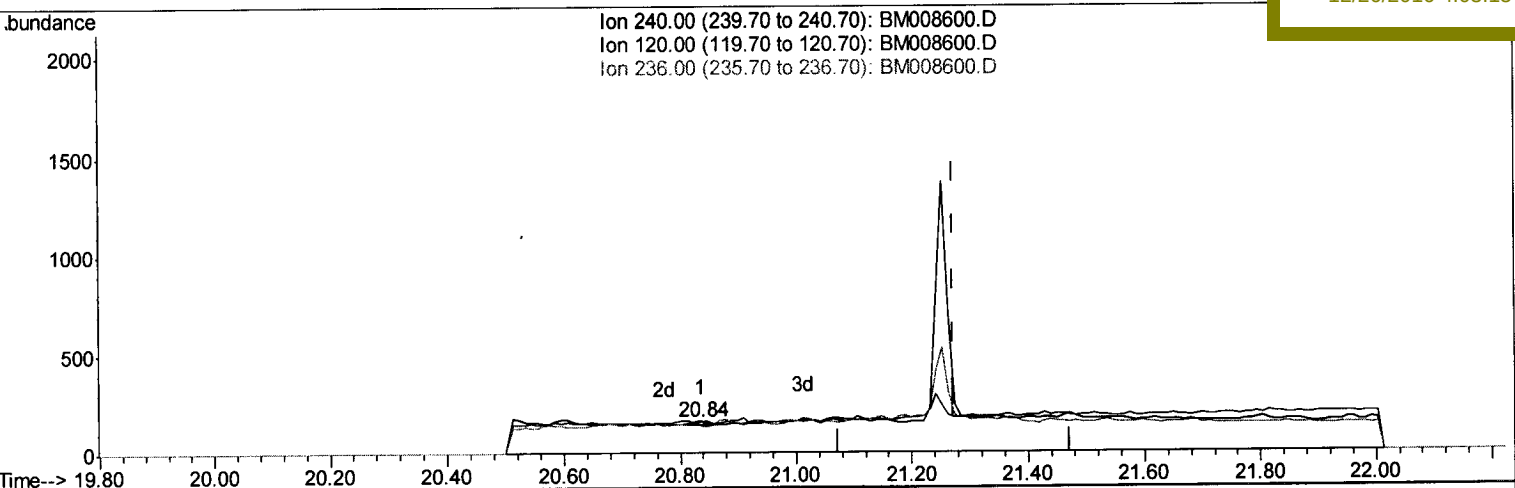

(16) Chrysene-d12 (I)

20.835min (-0.438) 0.40ng/ul

response 32

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	98.15#
236.00	34.90	83.33#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:41:37 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

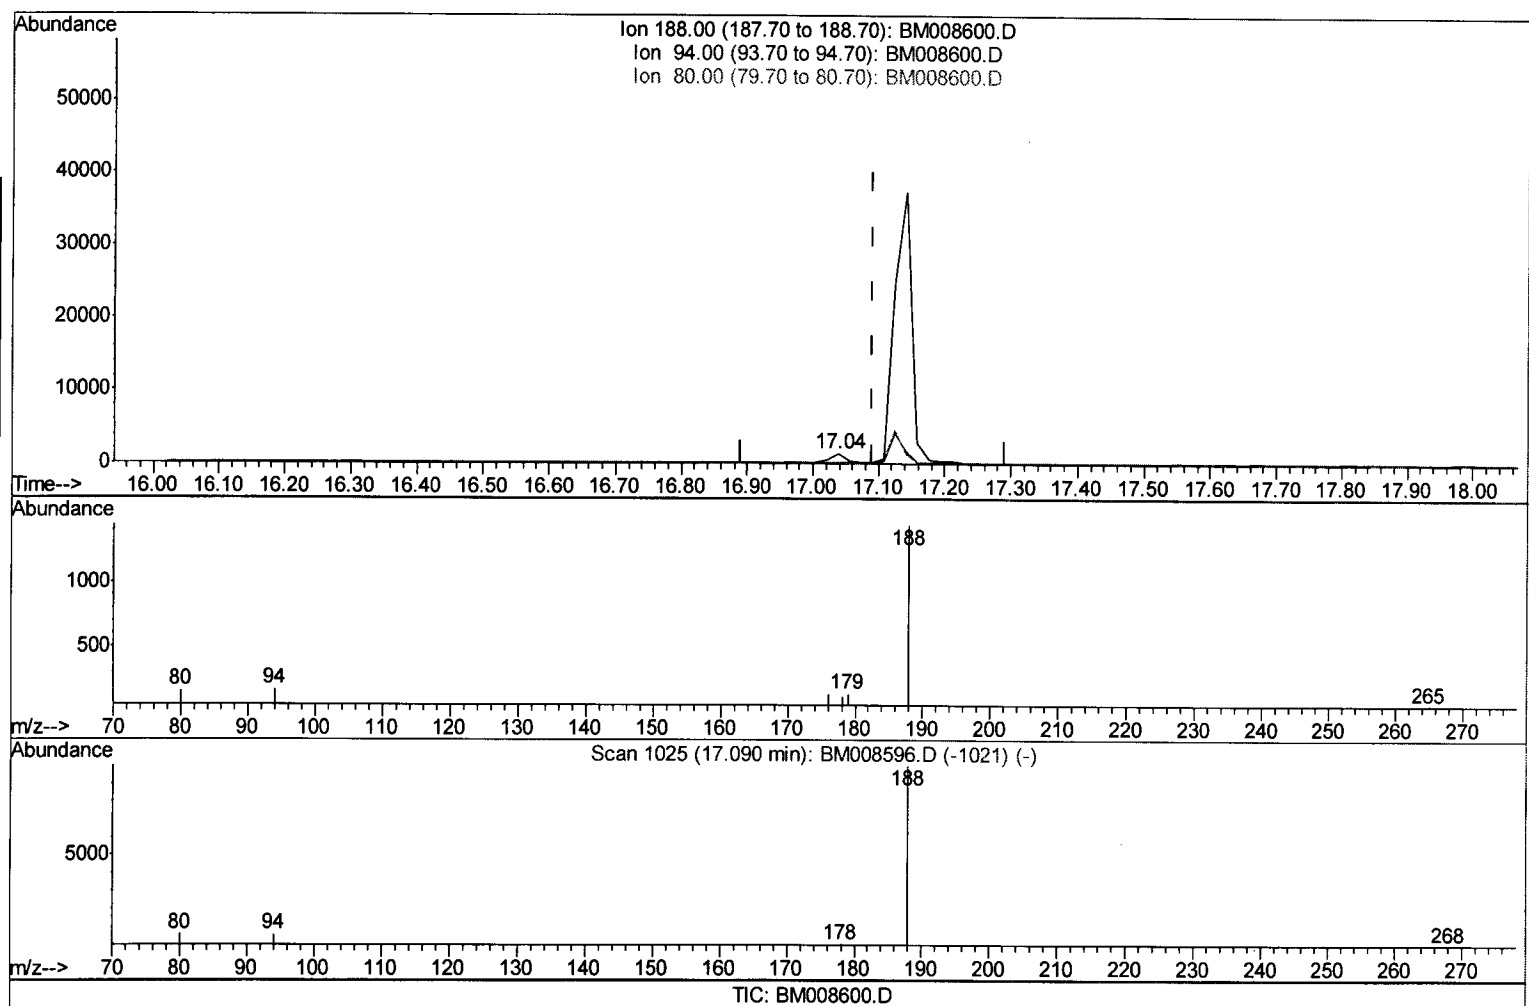

(10) Phenanthrene-d10 (I)

17.039min (-0.051) 0.40ng/ul m

response 2545

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.41
80.00	11.80	10.93
0.00	0.00	0.00

> 3.5
 12/27/2016

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:41:37 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

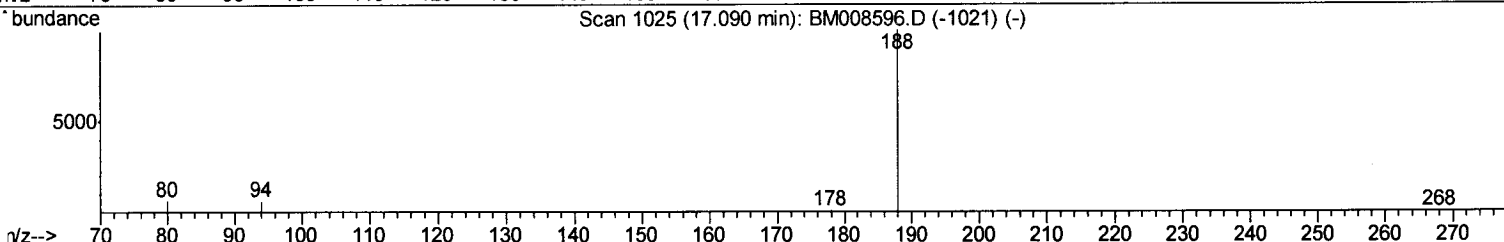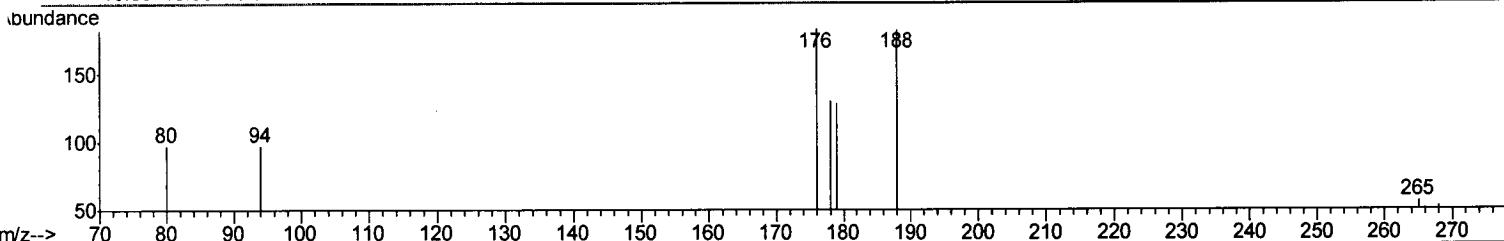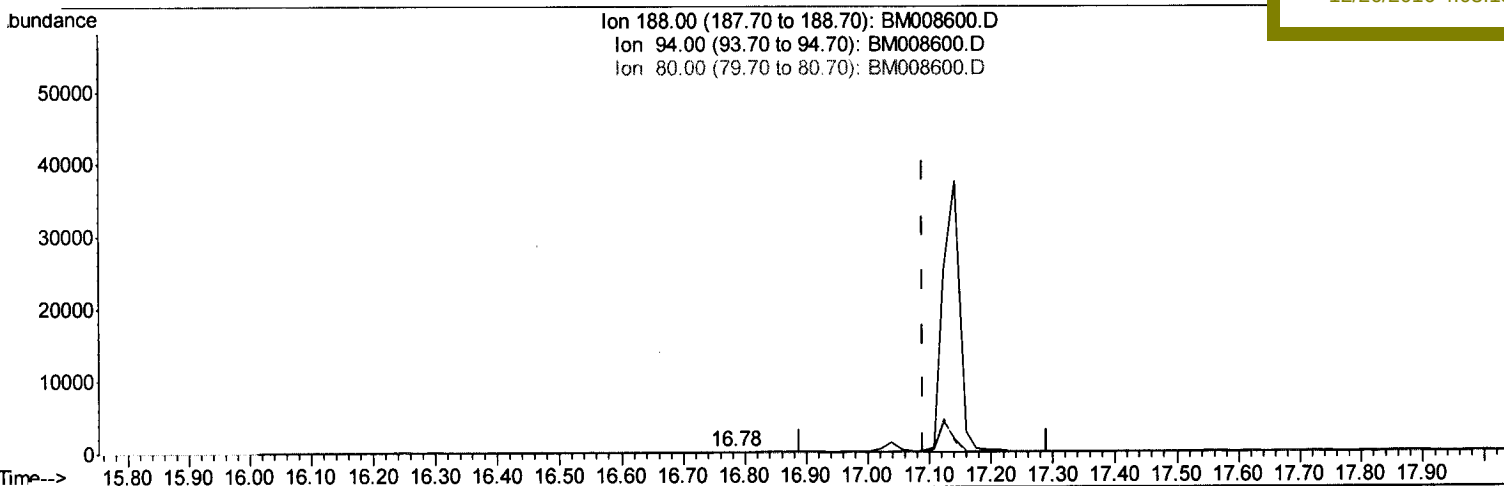

TIC: BM008600.D

(10) Phenanthrene-d10 (I)

16.782min (-0.309) 0.40ng/ul

response 208

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	53.30#
80.00	11.80	53.30#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
Data File : BM008600.D
Acq On : 23 Dec 2016 17:57
Operator : UM/SJ
Sample : H6040-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8X0

Manual Integrations
APPROVED

sohil
12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:41:37 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 23:37:39 2016
Response via : Initial Calibration

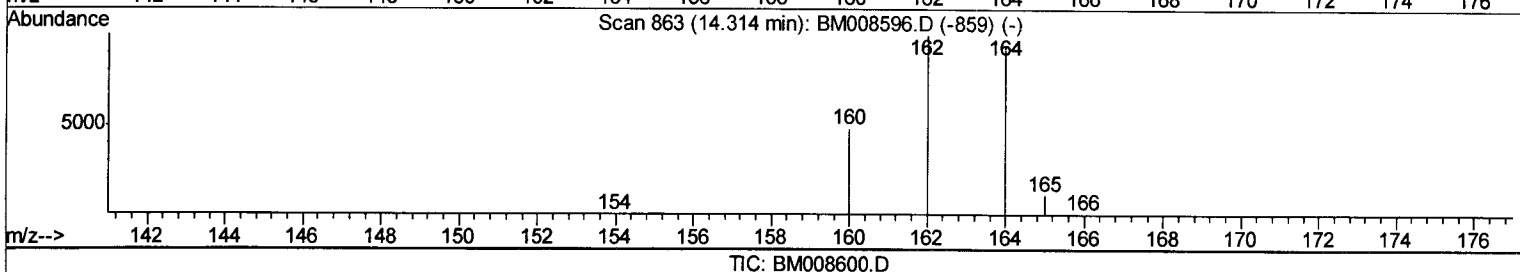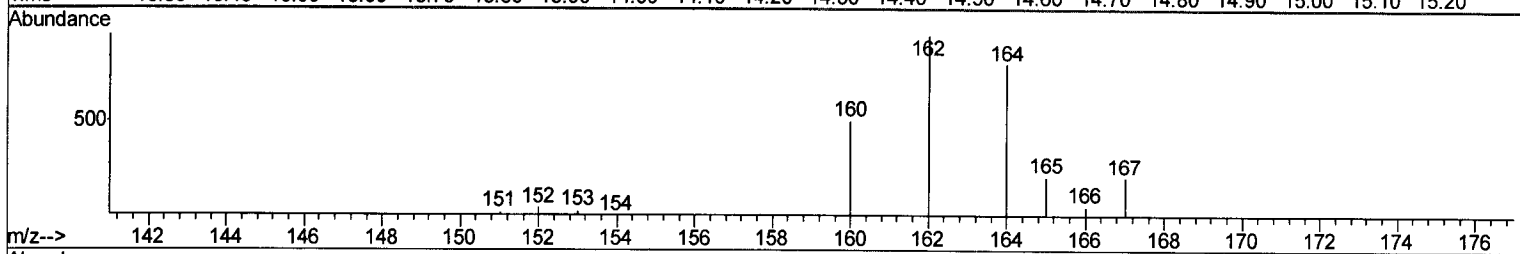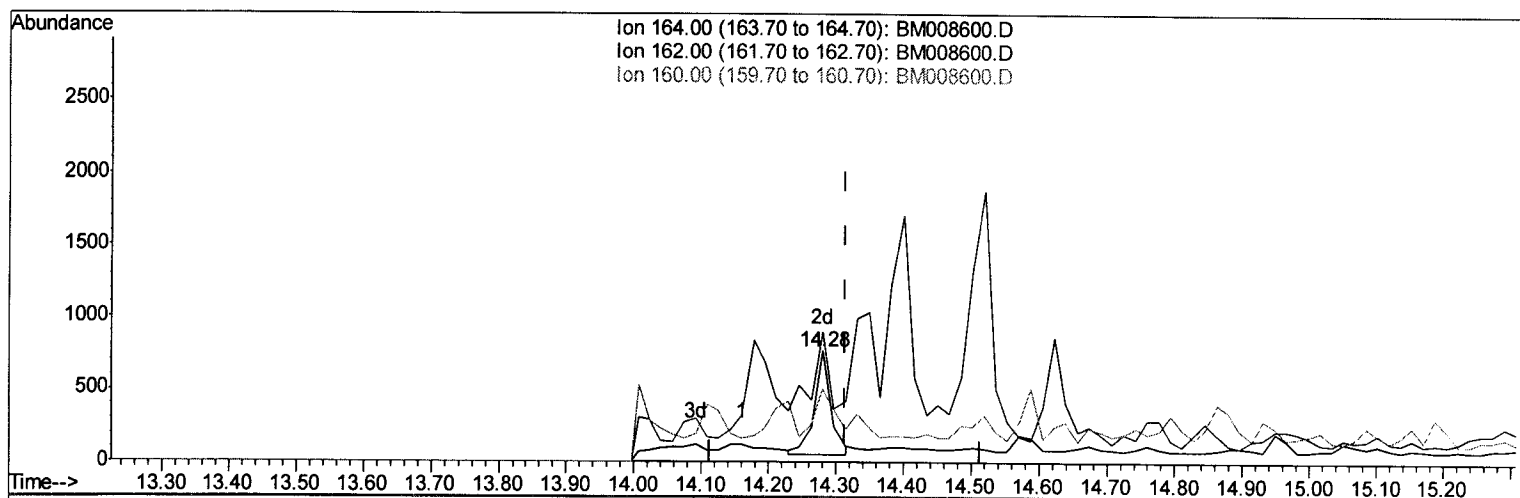

(6) Acenaphthene-d10 (I)

14.280min (-0.034) 0.40ng/ul m

response 1238

Ion	Exp%	Act%
164.00	100	100
162.00	98.60	117.19
160.00	48.80	65.23#
0.00	0.00	0.00

S.S.
12/27/2016




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
Data File : BM008600.D
Acq On : 23 Dec 2016 17:57
Operator : UM/SJ
Sample : H6040-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8X0

Manual Integrations
APPROVED

sohil
12/26/2016 4:03:15 PM

Quant Time: Dec 23 23:41:37 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 23:37:39 2016
Response via : Initial Calibration

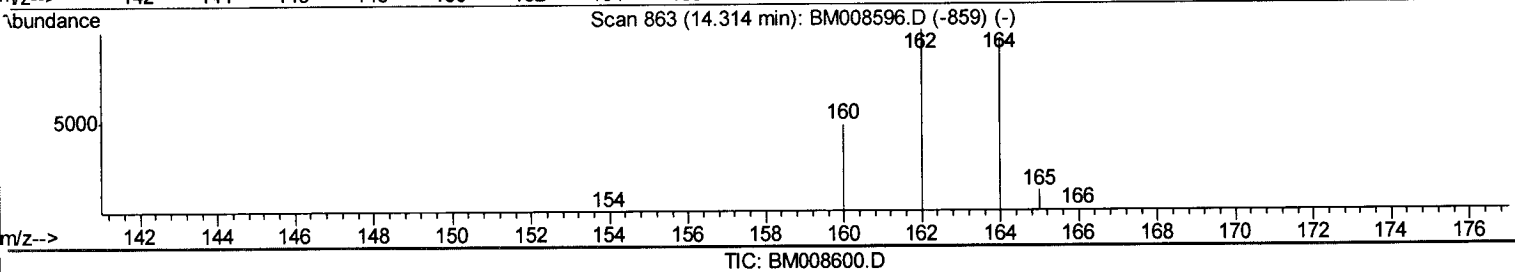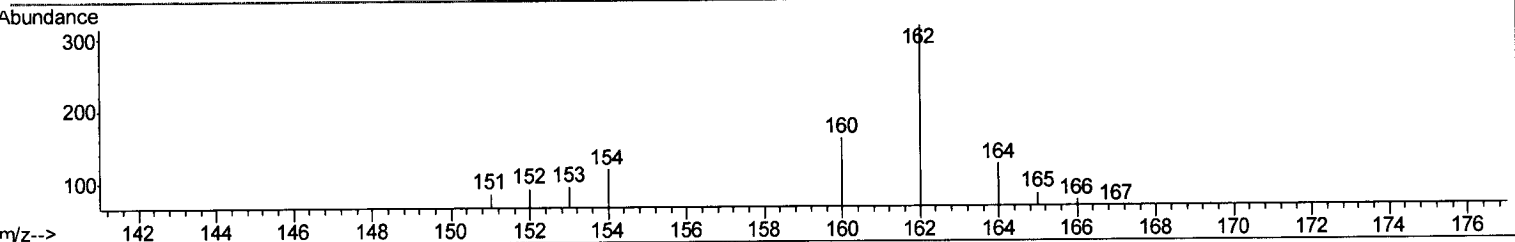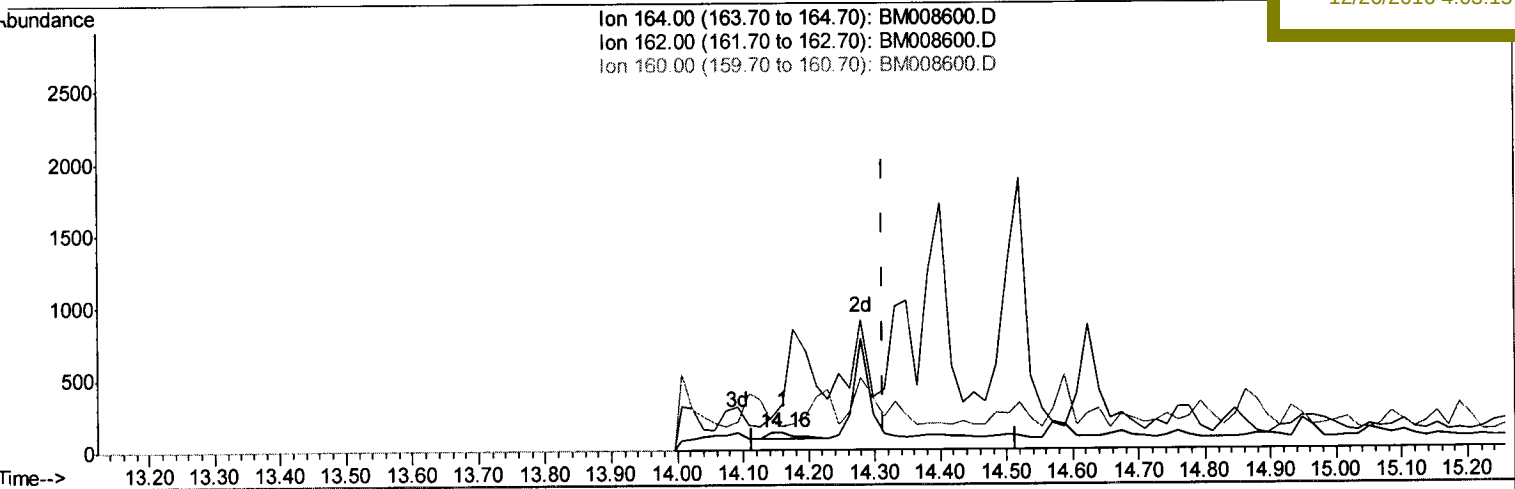

(6) Acenaphthene-d10 (I)

14.160min (-0.154) 0.40ng/ul

response 148

Ion	Exp%	Act%
164.00	100	100
162.00	98.60	256.91#
160.00	48.80	129.27#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 24 00:00:03 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	543	0.40	ng/ul	-0.09
2) Naphthalene-d8	10.42	136	1823	0.40	ng/ul	-0.08
6) Acenaphthene-d10	14.28	164	1238m	0.40	ng/ul	-0.03
10) Phenanthrene-d10	17.04	188	2545m	0.40	ng/ul	-0.05
16) Chrysene-d12	21.25	240	1654m	0.40	ng/ul	-0.02
20) Perylene-d12	23.47	264	1603m	0.40	ng/ul	-0.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	414	0.15	ng/ul	-0.09
14) Fluoranthene-d10	19.08	212	1811m	0.26	ng/ul	-0.02
Target Compounds						
3) Naphthalene	10.46	128	23164	4.52	ng/ul	95
5) 2-Methylnaphthalene	12.08	142	22253	6.45	ng/ul	99
8) Acenaphthene	14.33	153	1348m	0.32	ng/ul	
9) Fluorene	15.34	166	5664	1.18	ng/ul	96
12) Phenanthrene	17.07	178	4449m	0.57	ng/ul	
13) Anthracene	17.18	178	1198m	0.16	ng/ul	
15) Fluoranthene	19.11	202	1060m	0.11	ng/ul	
17) Pyrene	19.47	202	1964m	0.31	ng/ul	

S.S.
 12/27/2016

S.S.
 12/27/2016

S.S.
 12/27/2016

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122316\
 Data File : BM008600.D
 Acq On : 23 Dec 2016 17:57
 Operator : UM/SJ
 Sample : H6040-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0

Manual Integrations
 APPROVED

sohil
 12/26/2016 4:03:15 PM

Quant Time: Dec 24 00:00:03 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

