

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
 Data File : BM008605.D  
 Acq On : 23 Dec 2016 20:55  
 Operator : UM/SJ  
 Sample : H6069-06  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DA7J2

Manual Integrations  
 APPROVED

sohil  
 12/26/2016 4:03:28 PM

Quant Time: Dec 24 00:16:58 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 23 23:37:39 2016  
 Response via : Initial Calibration

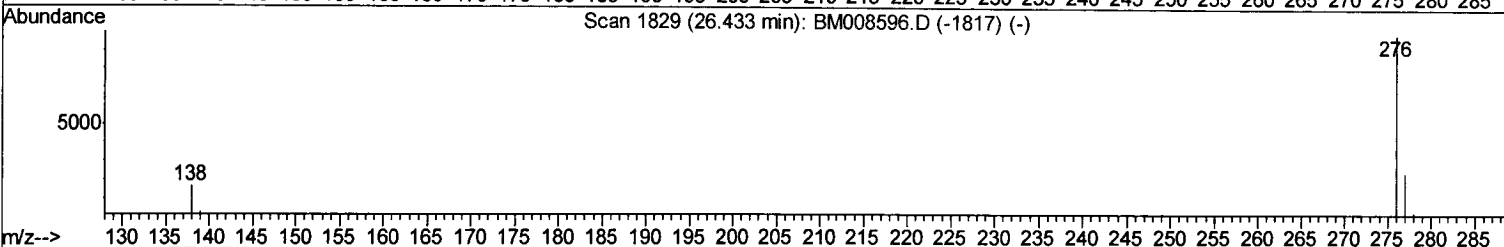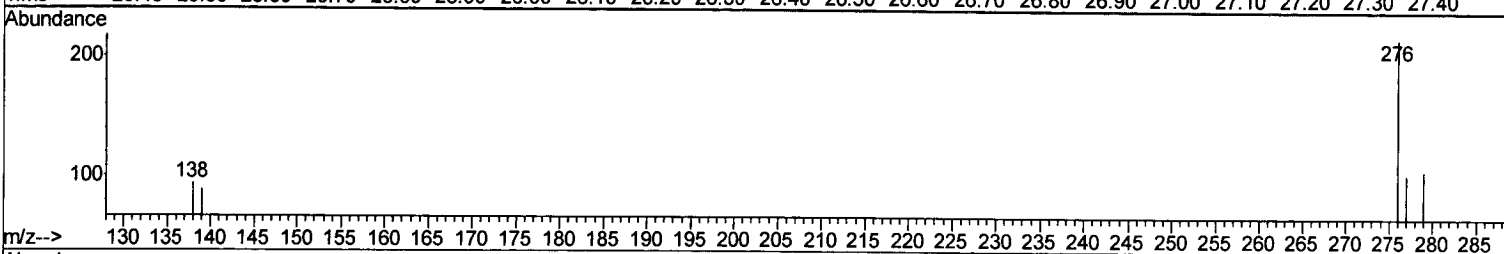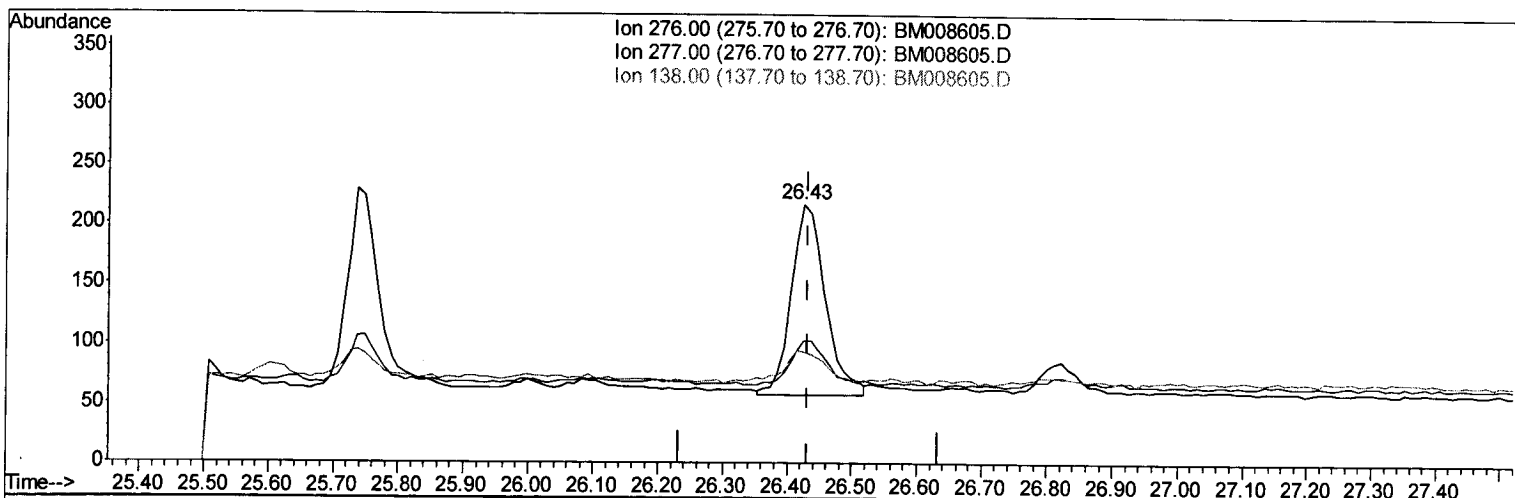

TIC: BM008605.D

(26) Benzo(g,h,i)perylene

26.426min (-0.007) 0.13ng/ul m

response 599

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 276.00 | 100   | 100    |
| 277.00 | 27.30 | 47.25# |
| 138.00 | 25.60 | 43.12# |
| 0.00   | 0.00  | 0.00   |

95  
 12/27/2016

## Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
Data File : BM008605.D  
Acq On : 23 Dec 2016 20:55  
Operator : UM/SJ  
Sample : H6069-06  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DA7J2

Manual Integrations  
APPROVED

sohil  
12/26/2016 4:03:28 PM

Quant Time: Dec 24 00:16:58 2016  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 23 23:37:39 2016  
Response via : Initial Calibration

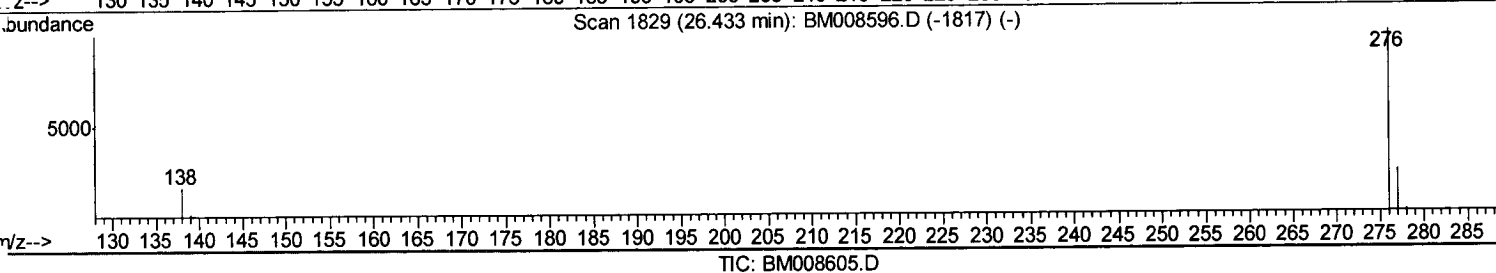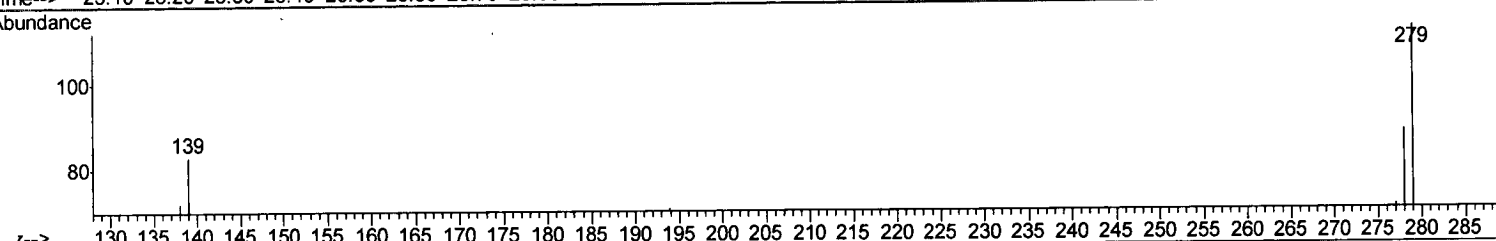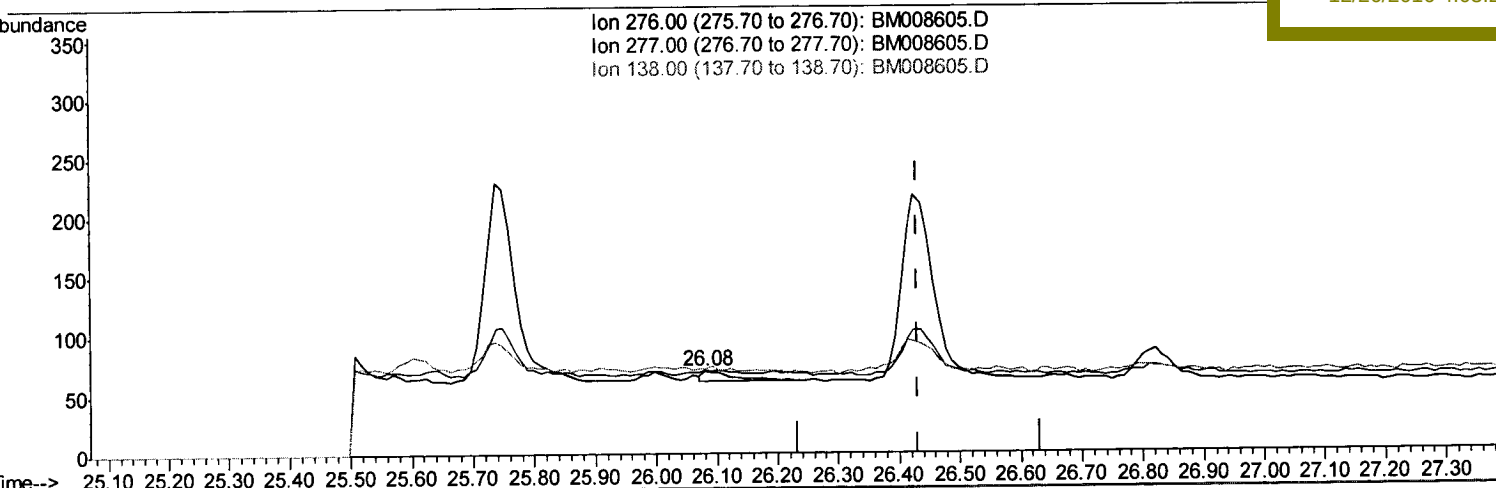

(26) Benzo(g,h,i)perylene

26.082min (-0.351) 0.01ng/ul

response 35

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 276.00 | 100   | 100     |
| 277.00 | 27.30 | 101.43# |
| 138.00 | 25.60 | 102.86# |
| 0.00   | 0.00  | 0.00    |

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
 Data File : BM008605.D  
 Acq On : 23 Dec 2016 20:55  
 Operator : UM/SJ  
 Sample : H6069-06  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DA7J2

Manual Integrations  
 APPROVED

sohil  
 12/26/2016 4:03:28 PM

Quant Time: Dec 24 00:16:58 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 23 23:37:39 2016  
 Response via : Initial Calibration

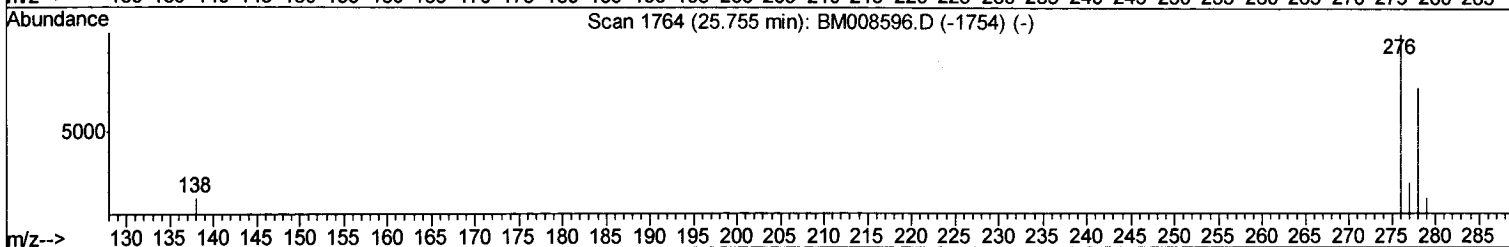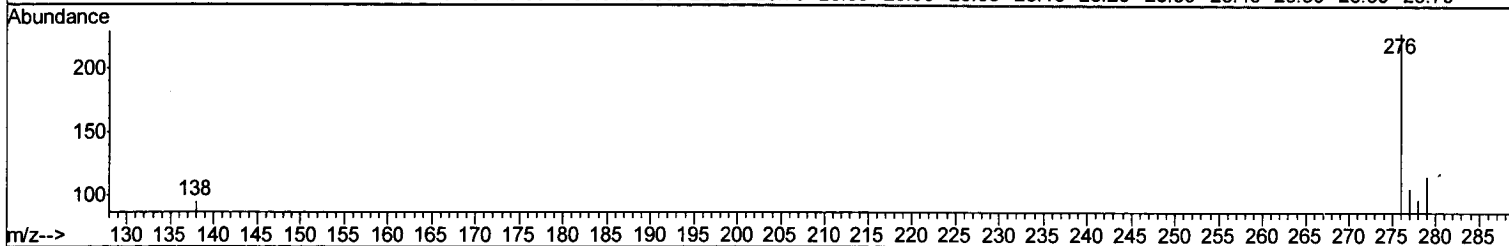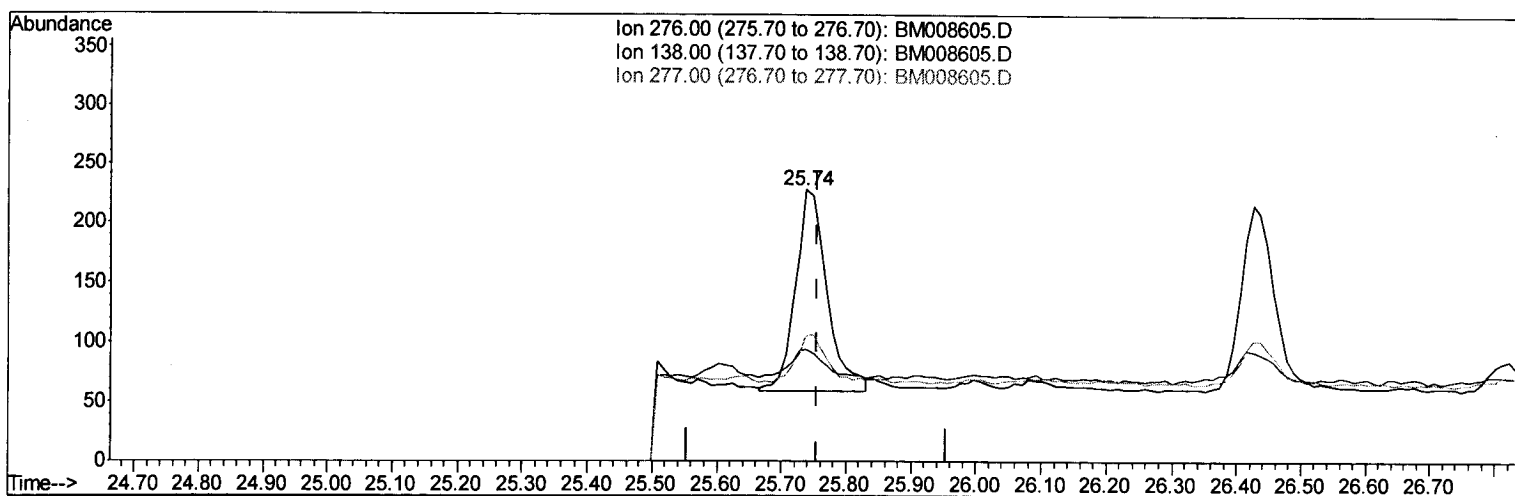

TIC: BM008605.D

(24) Indeno(1,2,3-cd)pyrene

25.738min (-0.018) 0.11ng/ul m

response 585

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 276.00 | 100   | 100    |
| 138.00 | 23.90 | 0.00#  |
| 277.00 | 24.50 | 71.45# |
| 0.00   | 0.00  | 0.00   |

S.I.  
 12/27/2016




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
Data File : BM008605.D  
Acq On : 23 Dec 2016 20:55  
Operator : UM/SJ  
Sample : H6069-06  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DA7J2

Manual Integrations  
APPROVED

sohil  
12/26/2016 4:03:28 PM

Quant Time: Dec 24 00:16:58 2016  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 23 23:37:39 2016  
Response via : Initial Calibration

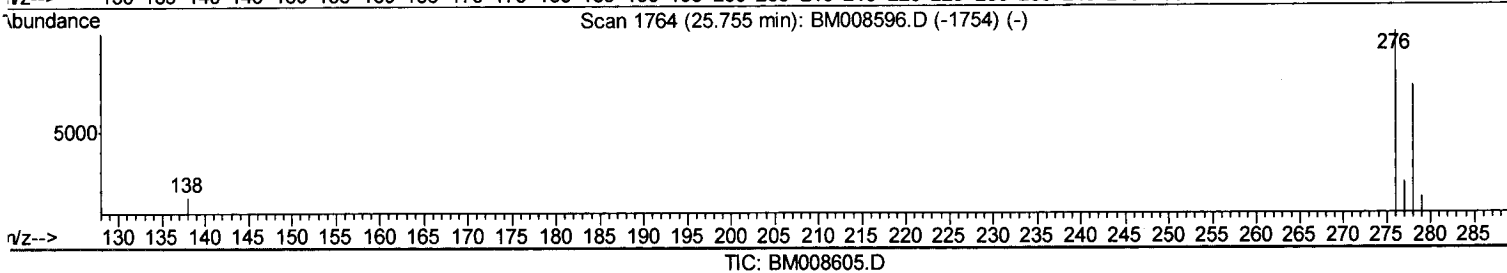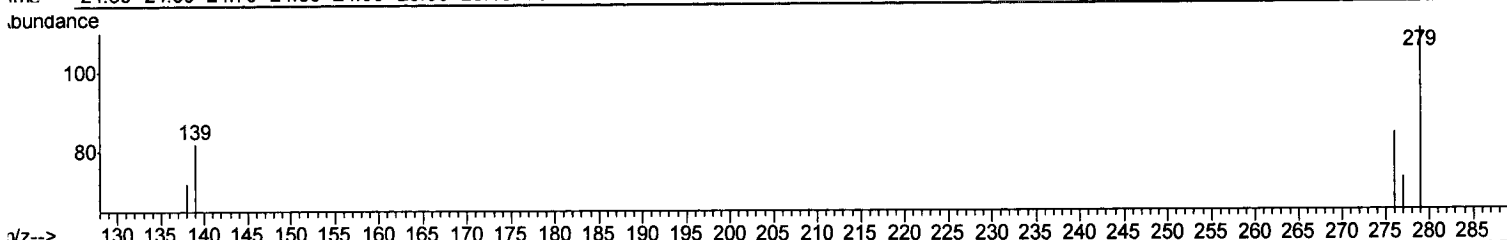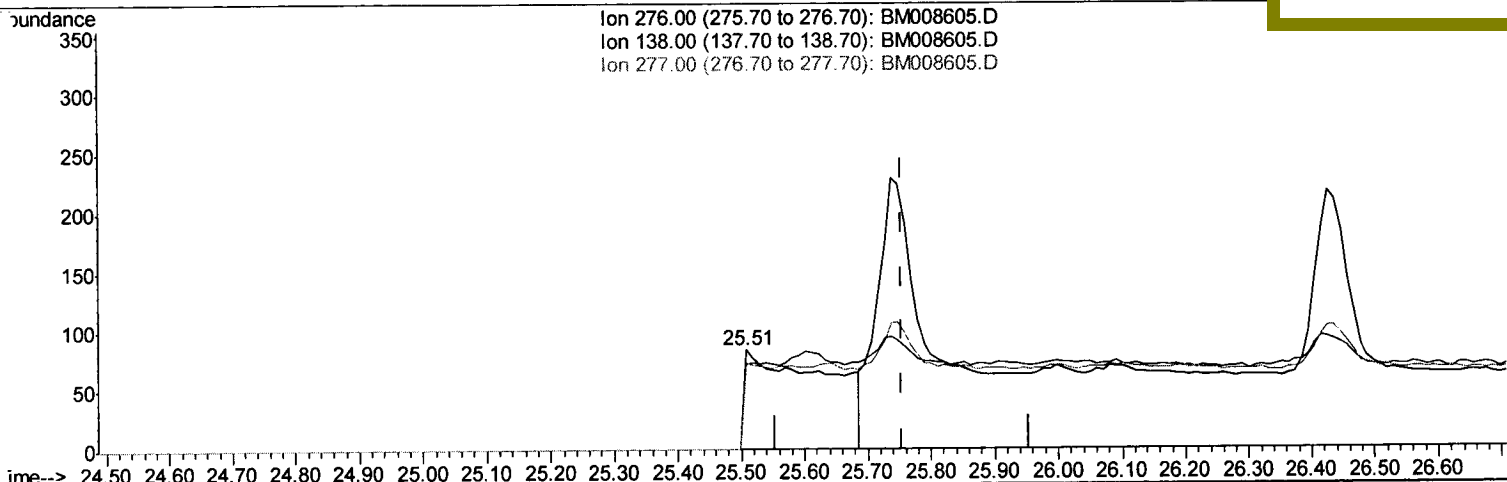

TIC: BM008605.D

(24) Indeno(1,2,3-cd)pyrene

25.508min (-0.247) 0.14ng/ul

response 756

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 276.00 | 100   | 100    |
| 138.00 | 23.90 | 0.00#  |
| 277.00 | 24.50 | 55.29# |
| 0.00   | 0.00  | 0.00   |

# Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\

Data File : BM008605.D

Acq On : 23 Dec 2016 20:55

Operator : UM/SJ

Sample : H6069-06

Misc :

ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 24 00:16:58 2016

Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Dec 23 23:37:39 2016

Response via : Initial Calibration

Instrument :

BNA\_M

ClientSampled :




DA7J2

Manual Integrations

APPROVED

sohil

12/26/2016 4:03:28 PM

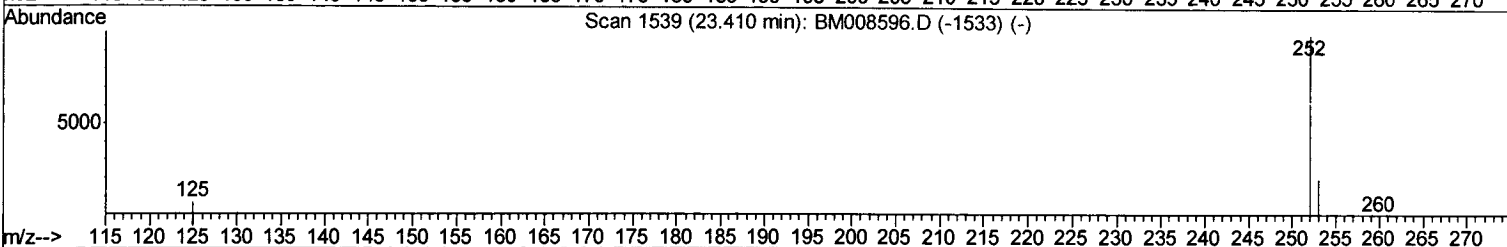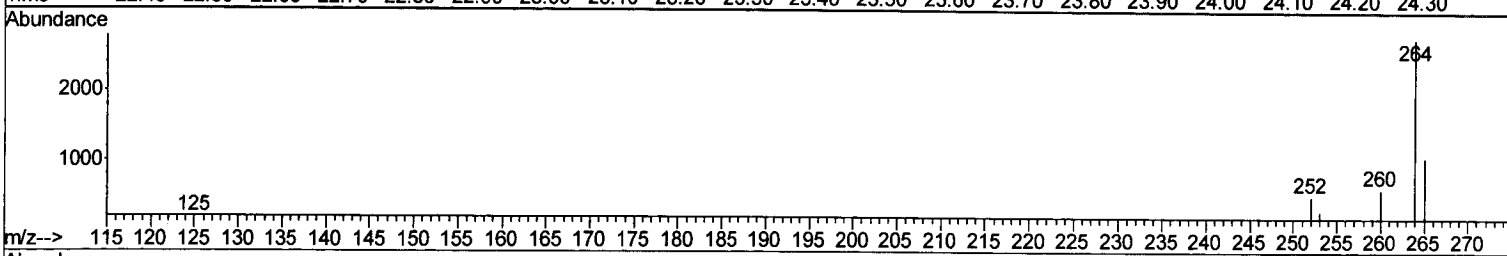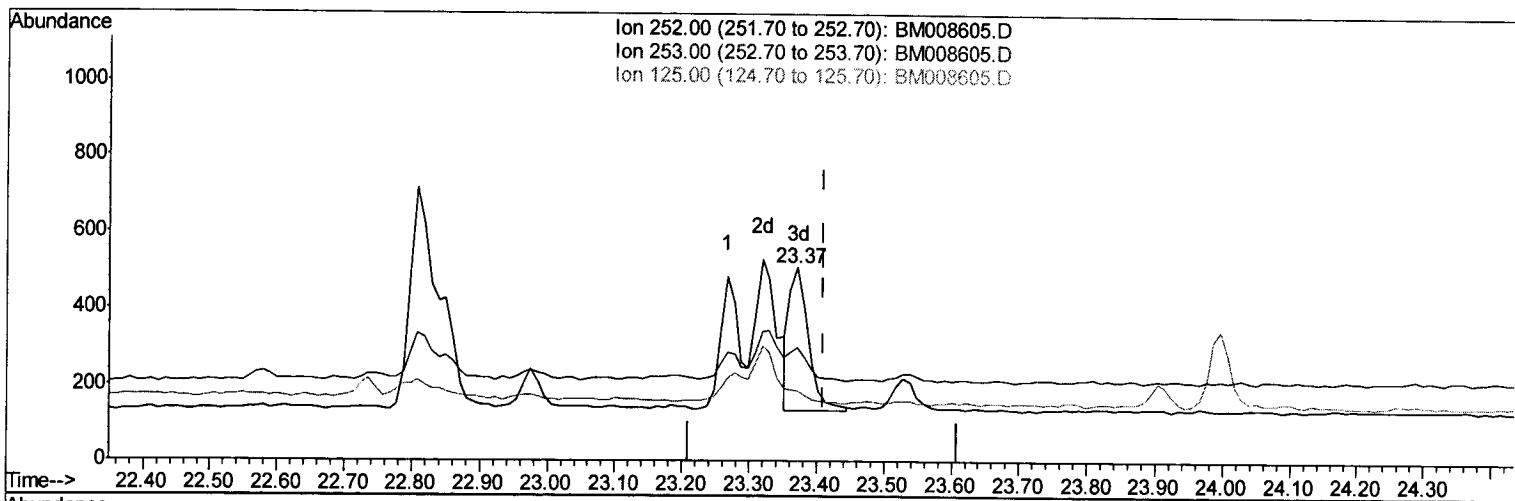

TIC: BM008605.D

(23) Benzo(a)pyrene (C)

23.371min (-0.038) 0.17ng/ul m 5.5  
12/27/2016

response 751

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 35.60 | 58.51# |
| 125.00 | 22.60 | 36.59# |
| 0.00   | 0.00  | 0.00   |




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
Data File : BM008605.D  
Acq On : 23 Dec 2016 20:55  
Operator : UM/SJ  
Sample : H6069-06  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DA7J2

Manual Integrations  
APPROVED

sohil  
12/26/2016 4:03:28 PM

Quant Time: Dec 24 00:16:58 2016  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 23 23:37:39 2016  
Response via : Initial Calibration

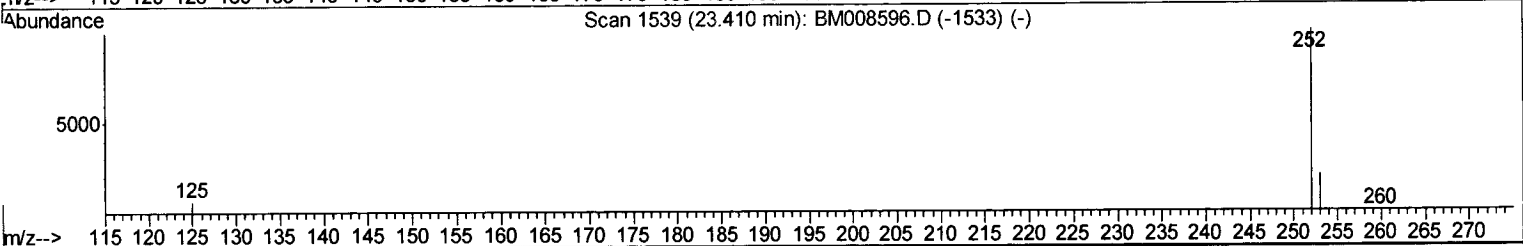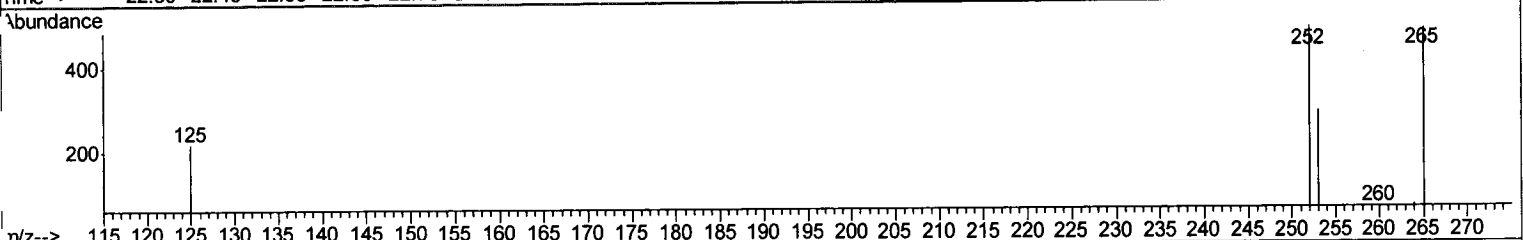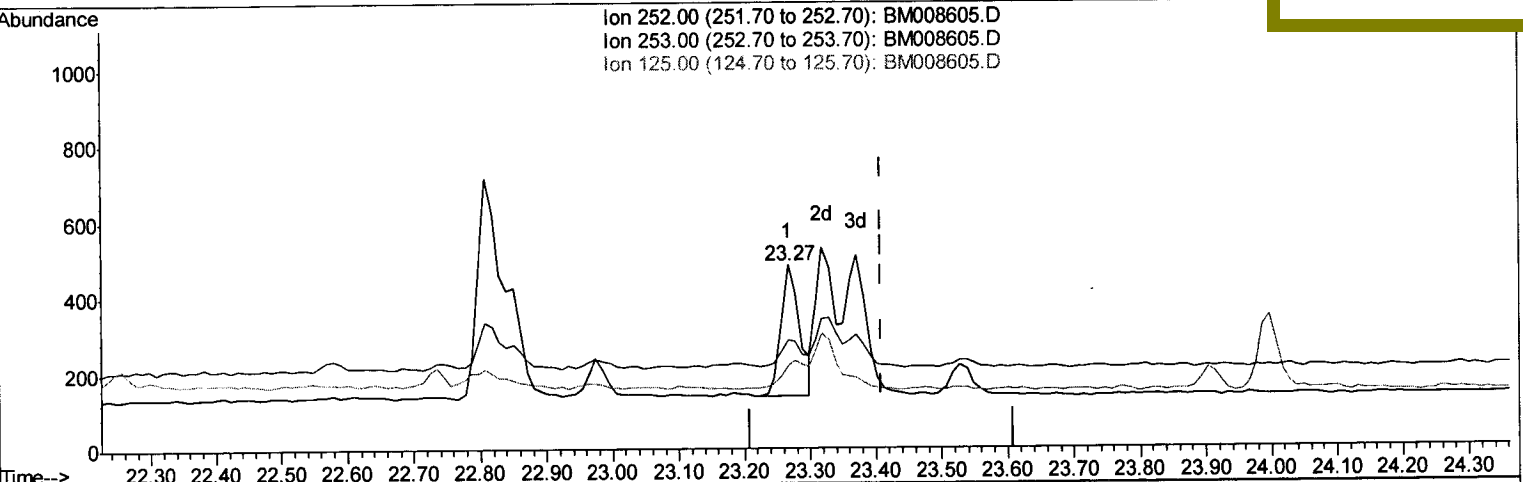

TIC: BM008605.D

(23) Benzo(a)pyrene (C)

23.267min (-0.143) 0.15ng/ul

response 684

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 35.60 | 59.38# |
| 125.00 | 22.60 | 44.74# |
| 0.00   | 0.00  | 0.00   |

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
 Data File : BM008605.D  
 Acq On : 23 Dec 2016 20:55  
 Operator : UM/SJ  
 Sample : H6069-06  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleID :  
 DA7J2

Manual Integrations  
 APPROVED

sohil  
 12/26/2016 4:03:28 PM

Quant Time: Dec 24 00:16:58 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 23 23:37:39 2016  
 Response via : Initial Calibration

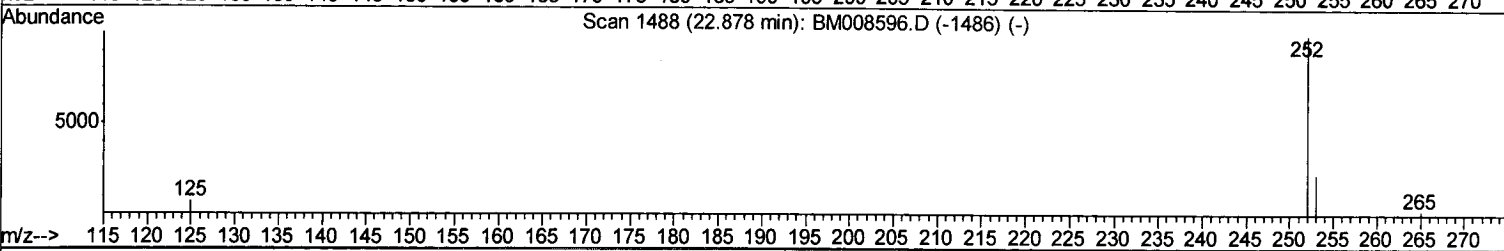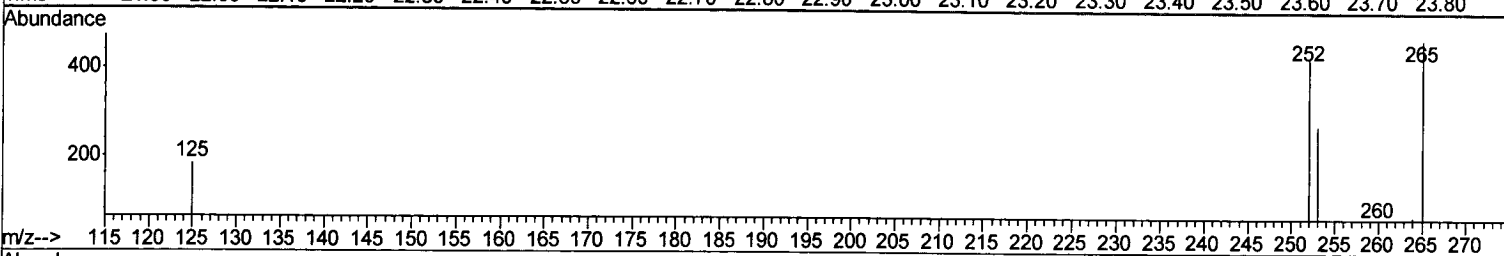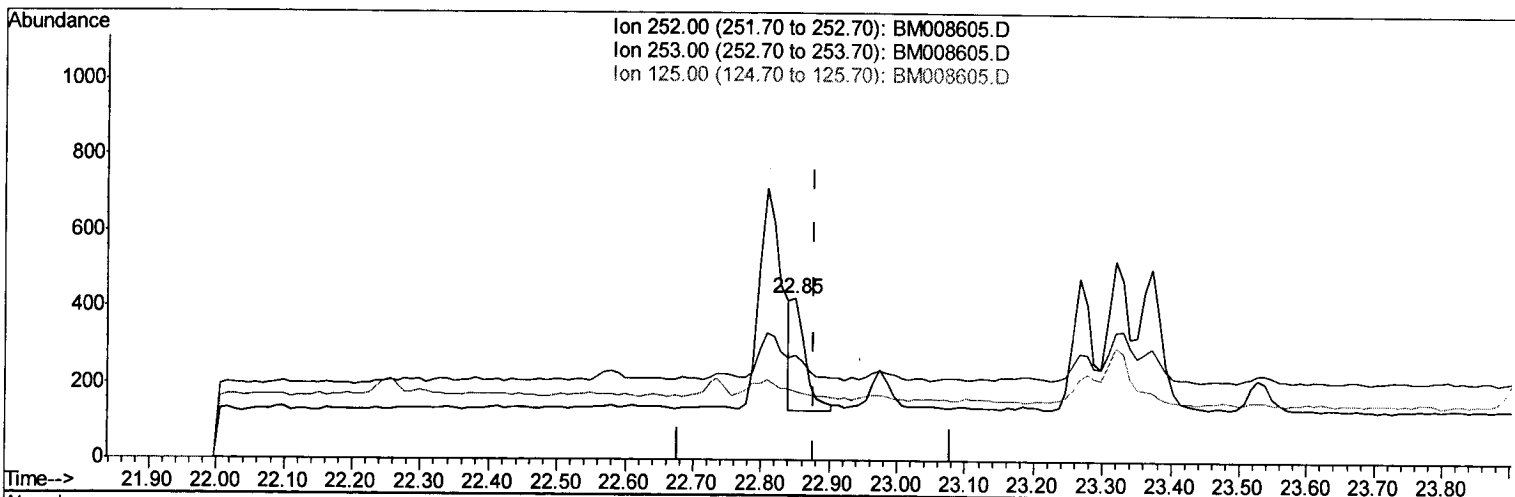

TIC: BM008605.D

(22) Benzo(k)fluoranthene

22.850min (-0.028) 0.08ng/ul m } 5.5  
 response 394 12/27/2016

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 30.60 | 64.87# |
| 125.00 | 17.10 | 43.09# |
| 0.00   | 0.00  | 0.00   |

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
 Data File : BM008605.D  
 Acq On : 23 Dec 2016 20:55  
 Operator : UM/SJ  
 Sample : H6069-06  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DA7J2

Manual Integrations  
 APPROVED

sohil  
 12/26/2016 4:03:28 PM

Quant Time: Dec 24 00:16:58 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 23 23:37:39 2016  
 Response via : Initial Calibration

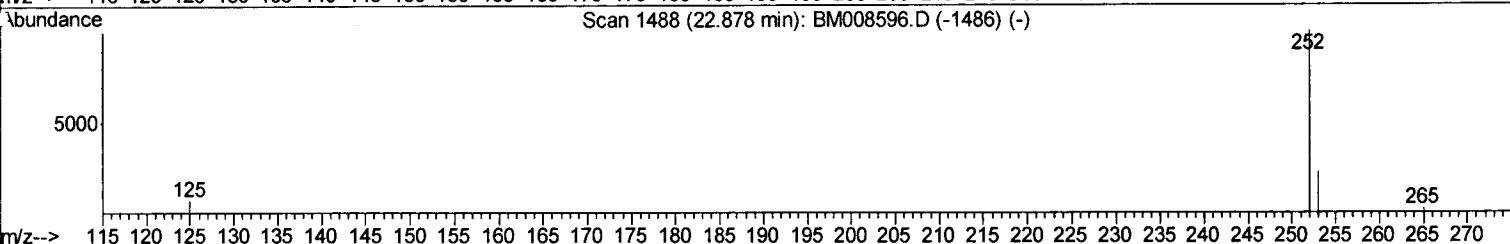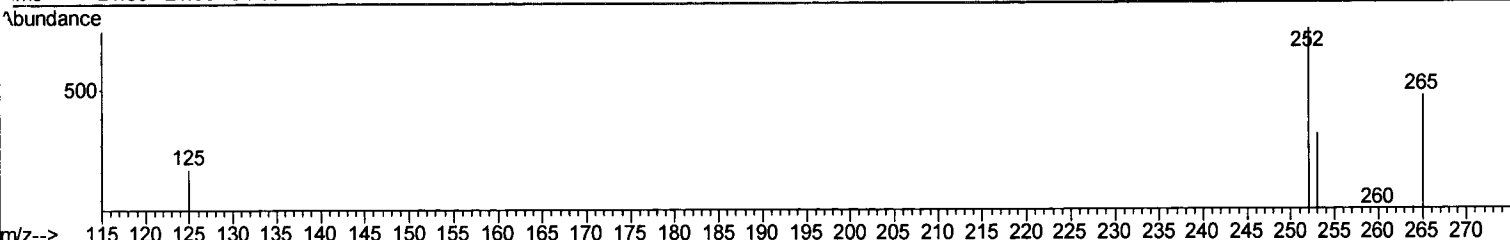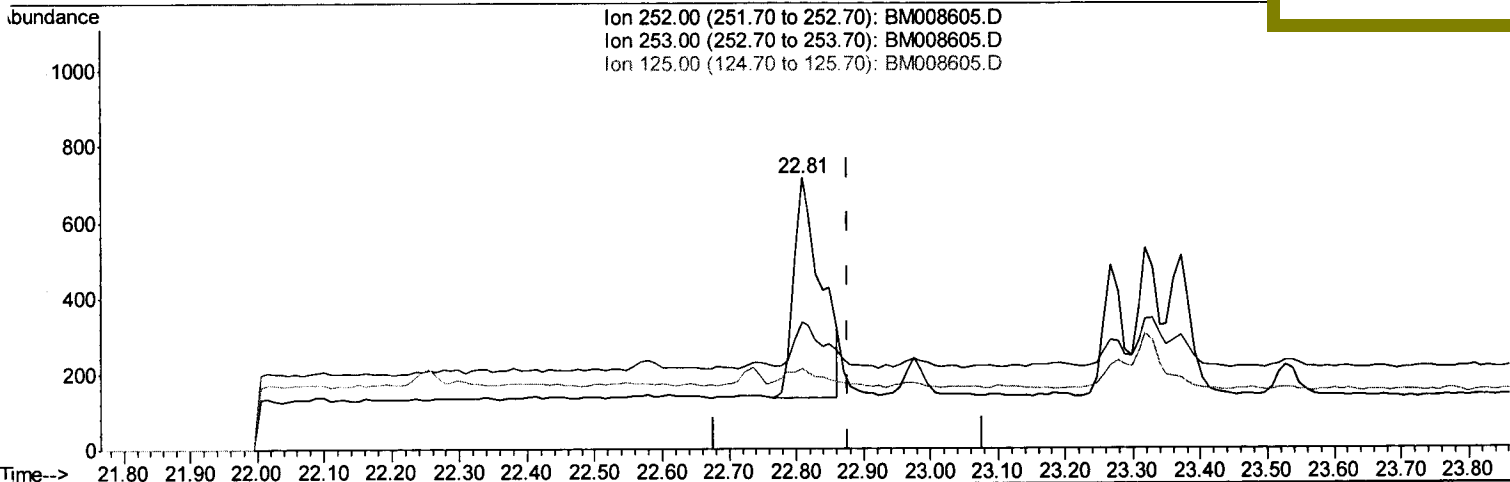

(22) Benzo(k)fluoranthene  
 22.808min (-0.070) 0.35ng/ul  
 response 1659

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 30.60 | 46.93# |
| 125.00 | 17.10 | 29.47# |
| 0.00   | 0.00  | 0.00   |

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
 Data File : BM008605.D  
 Acq On : 23 Dec 2016 20:55  
 Operator : UM/SJ  
 Sample : H6069-06  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DA7J2

Manual Integrations  
 APPROVED

sohil  
 12/26/2016 4:03:28 PM

Quant Time: Dec 24 00:16:58 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 23 23:37:39 2016  
 Response via : Initial Calibration

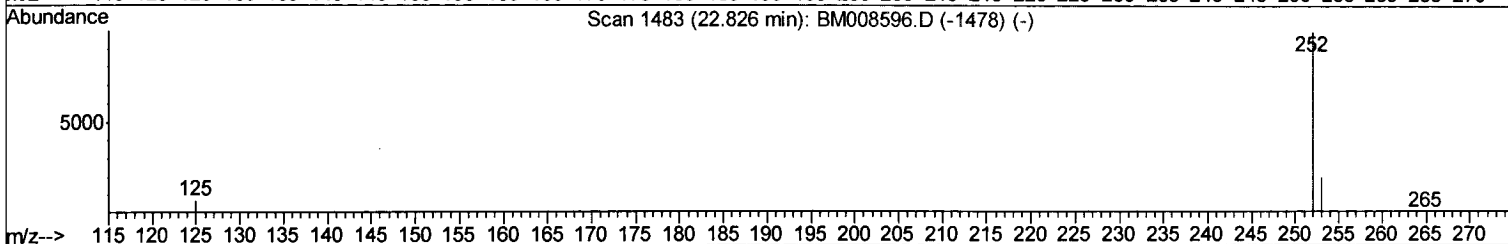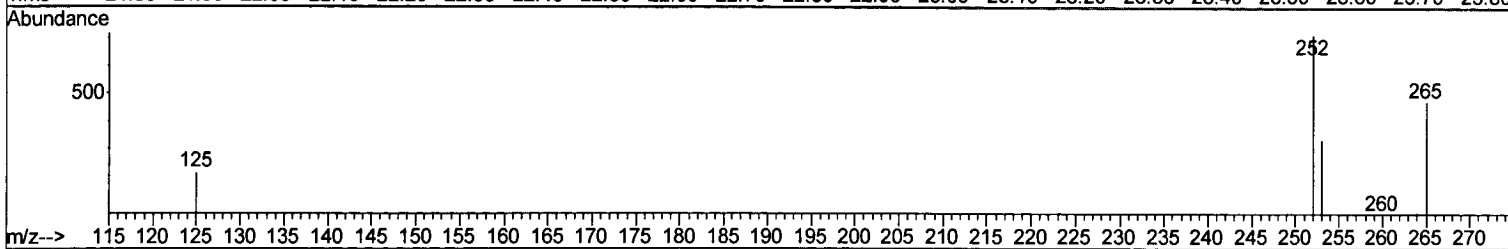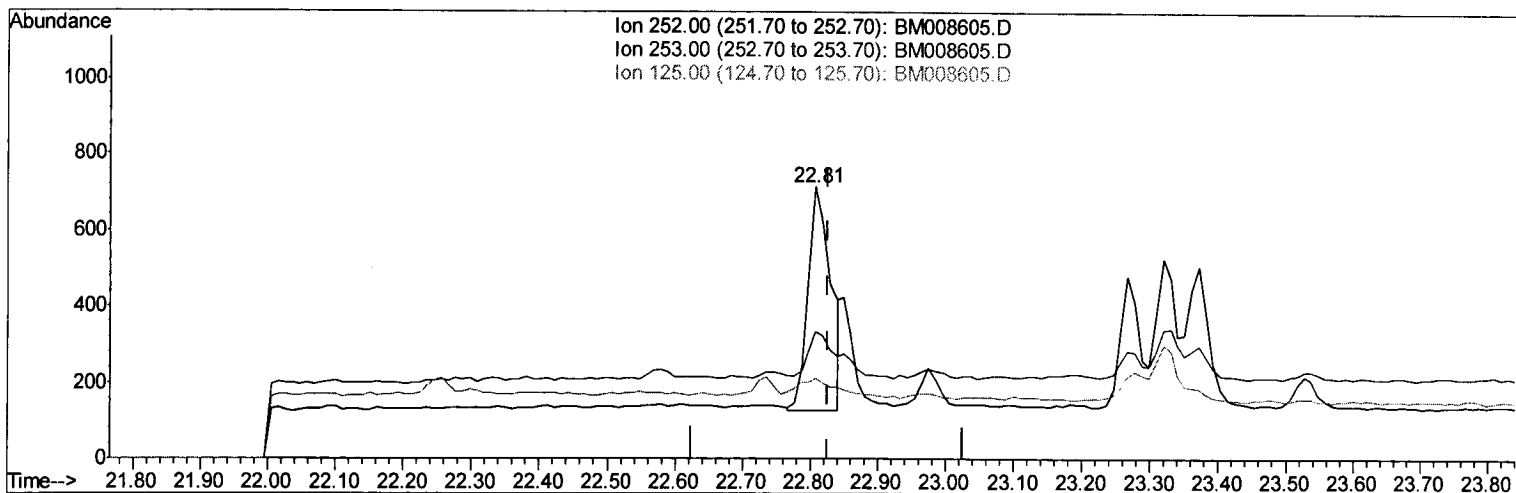

TIC: BM008605.D

(21) Benzo(b)fluoranthene

22.808min (-0.018) 0.29ng/ul m

response 1394

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 32.10 | 46.93 |
| 125.00 | 17.50 | 29.47 |
| 0.00   | 0.00  | 0.00  |

SJ  
 12/27/2016




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
Data File : BM008605.D  
Acq On : 23 Dec 2016 20:55  
Operator : UM/SJ  
Sample : H6069-06  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DA7J2

Manual Integrations  
APPROVED

sohil  
12/26/2016 4:03:28 PM

Quant Time: Dec 24 00:16:58 2016  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 23 23:37:39 2016  
Response via : Initial Calibration

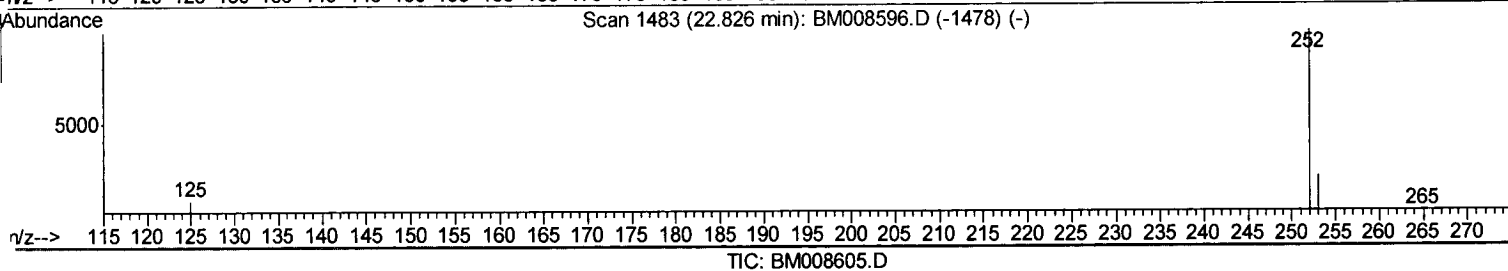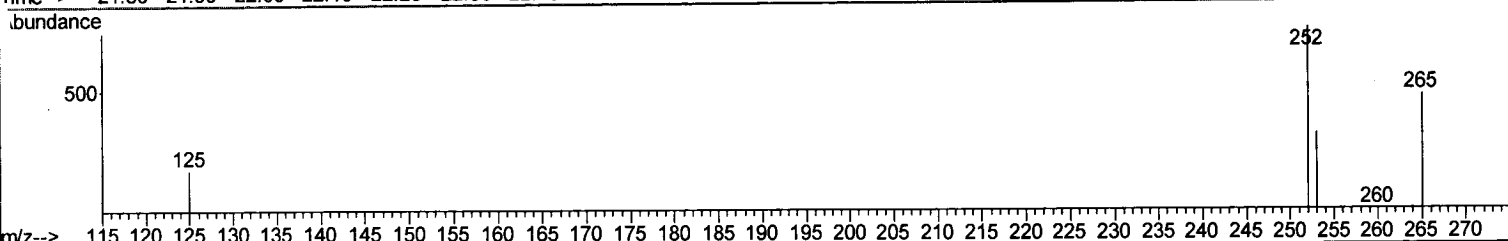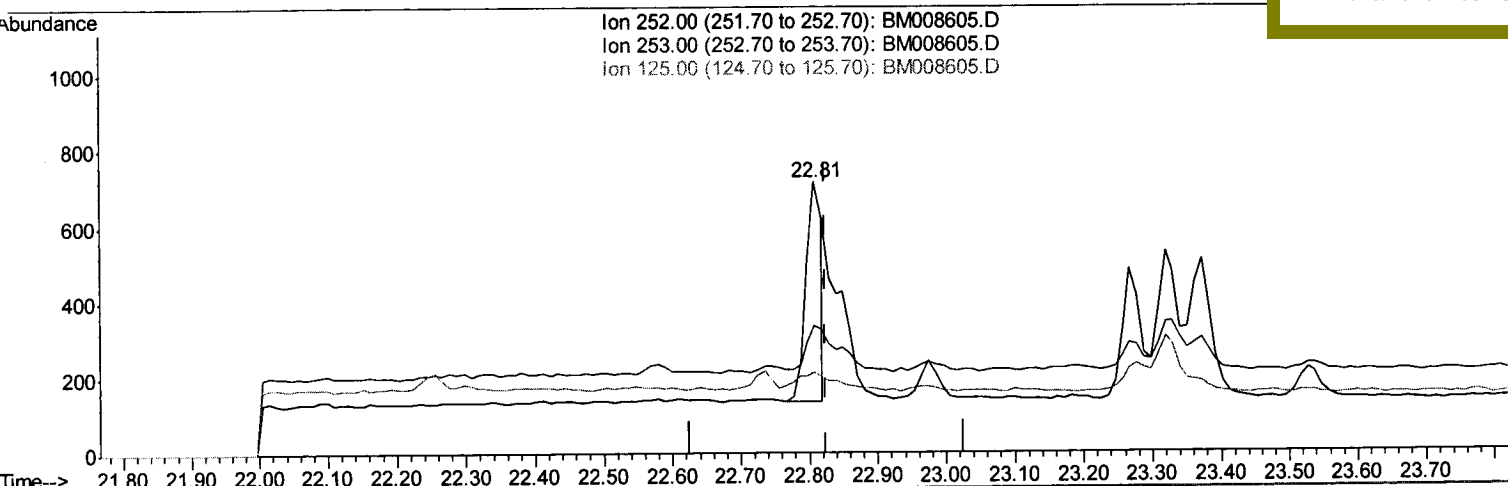

(21) Benzo(b)fluoranthene

22.808min (-0.018) 0.20ng/ul

response 976

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 32.10 | 46.93 |
| 125.00 | 17.50 | 29.47 |
| 0.00   | 0.00  | 0.00  |

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
 Data File : BM008605.D  
 Acq On : 23 Dec 2016 20:55  
 Operator : UM/SJ  
 Sample : H6069-06  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DA7J2

Manual Integrations  
 APPROVED

sohil  
 12/26/2016 4:03:28 PM

Quant Time: Dec 24 00:16:58 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 23 23:37:39 2016  
 Response via : Initial Calibration

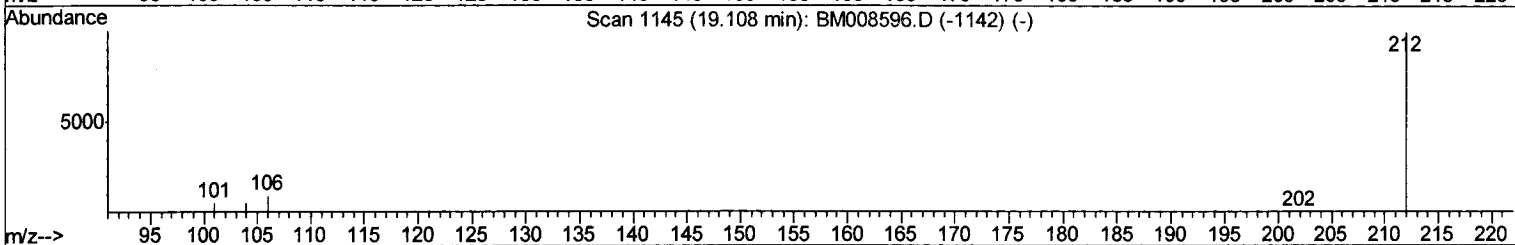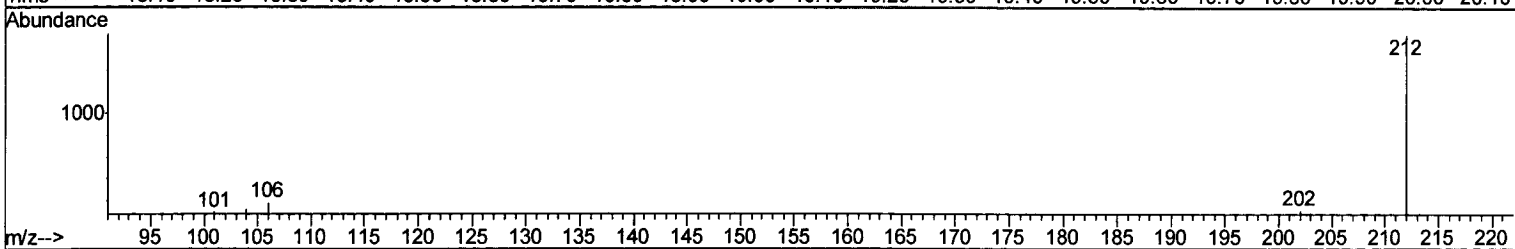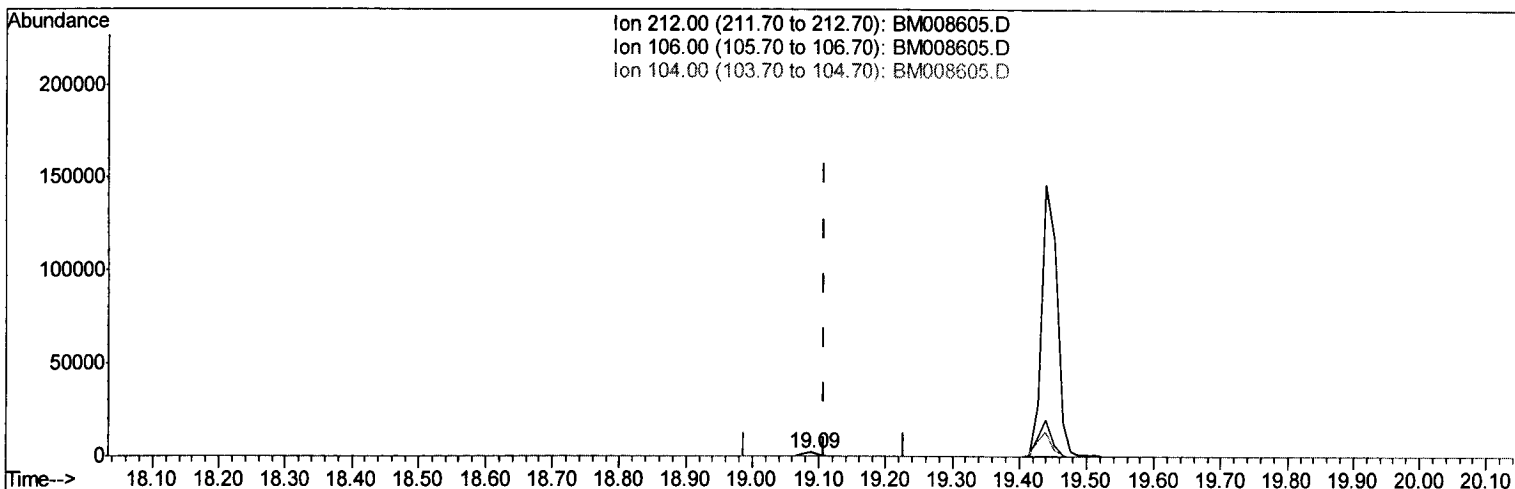

TIC: BM008605.D

(14) Fluoranthene-d10 (SURR)

19.089min (-0.019) 0.46ng/ul m

response 2651

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 212.00 | 100   | 100   |
| 106.00 | 18.30 | 8.07# |
| 104.00 | 15.60 | 4.94# |
| 0.00   | 0.00  | 0.00  |

> S.J.  
 12/27/2016

## Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
Data File : BM008605.D  
Acq On : 23 Dec 2016 20:55  
Operator : UM/SJ  
Sample : H6069-06  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DA7J2

Manual Integrations  
APPROVED

sohil  
12/26/2016 4:03:28 PM

Quant Time: Dec 24 00:16:58 2016  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 23 23:37:39 2016  
Response via : Initial Calibration

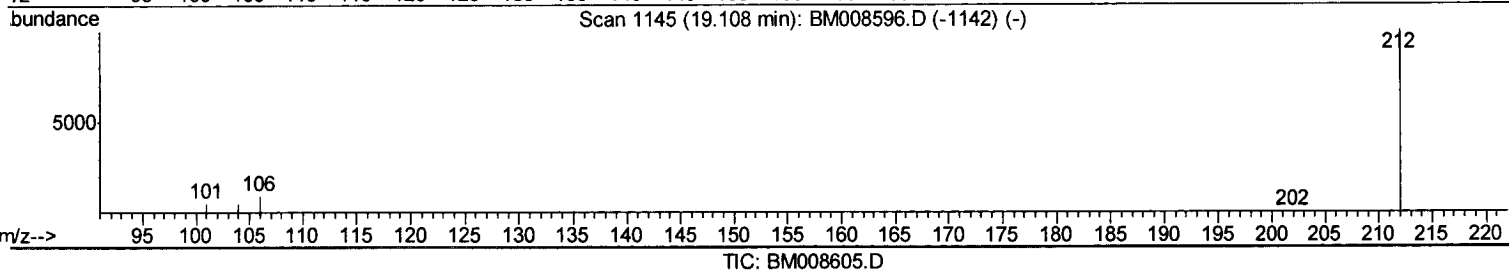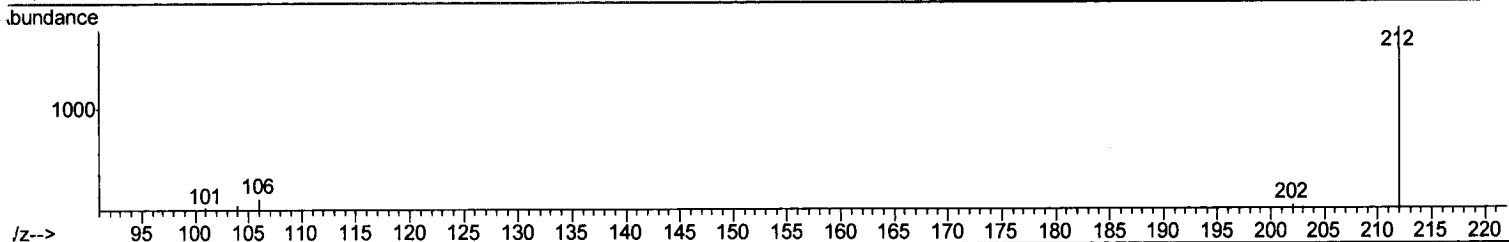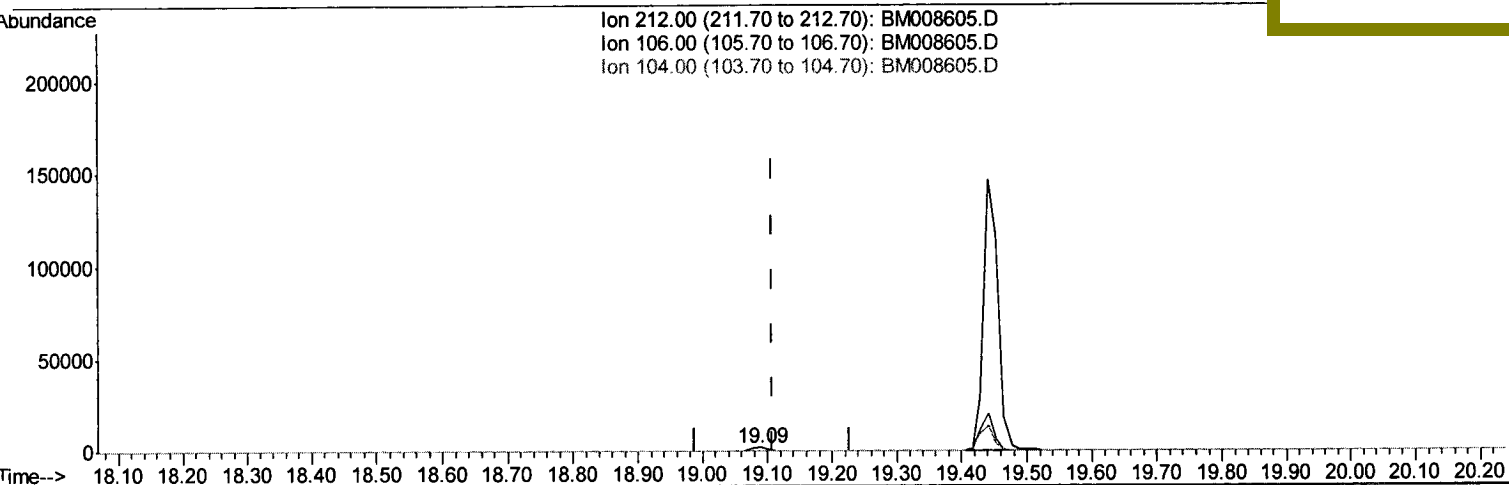

(14) Fluoranthene-d10 (SURR)

19.089min (-0.019) 0.42ng/ul

response 2465

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 212.00 | 100   | 100   |
| 106.00 | 18.30 | 8.68# |
| 104.00 | 15.60 | 5.31# |
| 0.00   | 0.00  | 0.00  |

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
 Data File : BM008605.D  
 Acq On : 23 Dec 2016 20:55  
 Operator : UM/SJ  
 Sample : H6069-06  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DA7J2

Manual Integrations  
 APPROVED

sohil  
 12/26/2016 4:03:28 PM

Quant Time: Dec 23 23:42:42 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 23 23:37:39 2016  
 Response via : Initial Calibration

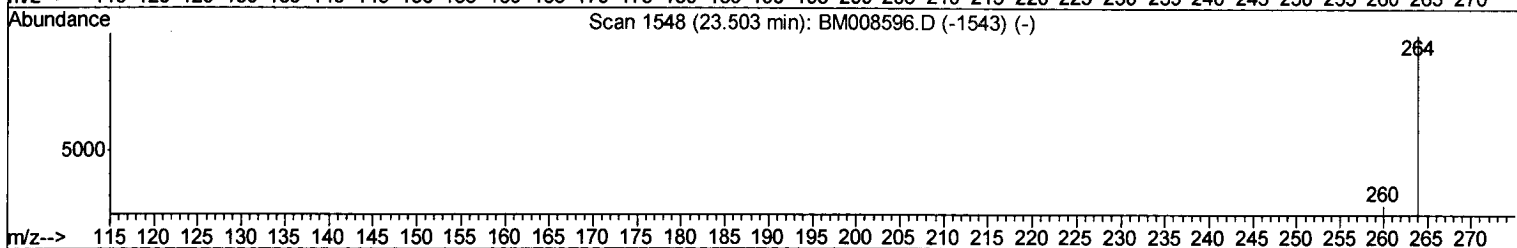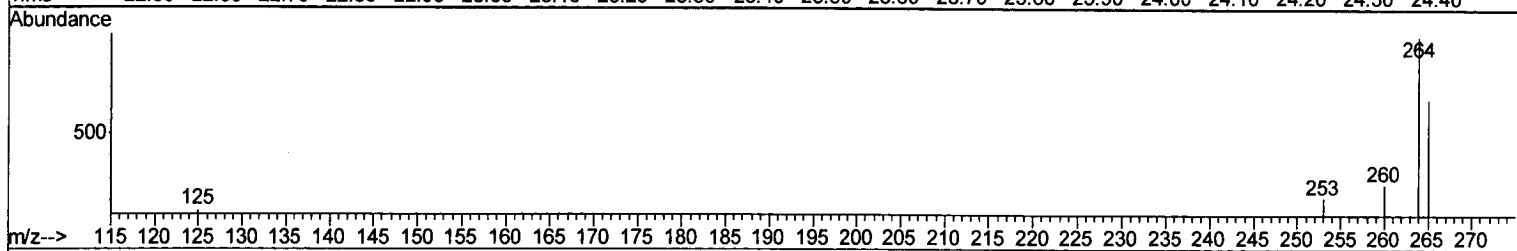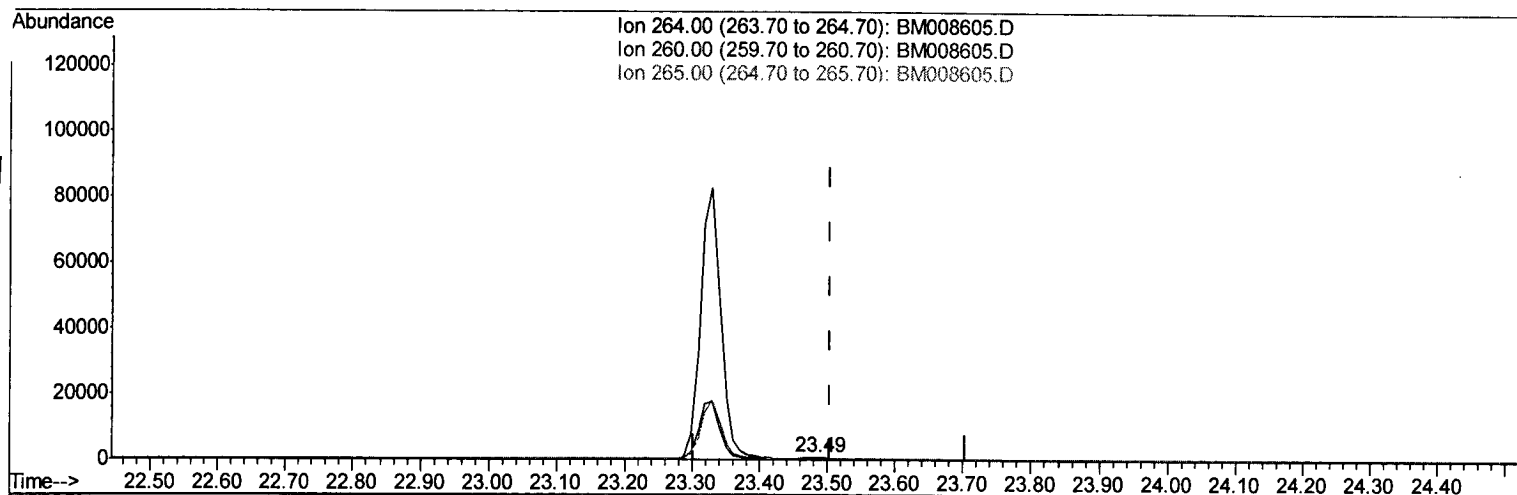

TIC: BM008605.D

(20) Perylene-d12 (I)

23.486min (-0.018) 0.40ng/ul m

response 1234

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100    | 100    |
| 260.00 | 30.10  | 29.30  |
| 265.00 | 103.50 | 70.59# |
| 0.00   | 0.00   | 0.00   |

5.5.  
 12/27/2016

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
 Data File : BM008605.D  
 Acq On : 23 Dec 2016 20:55  
 Operator : UM/SJ  
 Sample : H6069-06  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DA7J2

Manual Integrations  
 APPROVED

sohil  
 12/26/2016 4:03:28 PM

Quant Time: Dec 23 23:42:42 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 23 23:37:39 2016  
 Response via : Initial Calibration

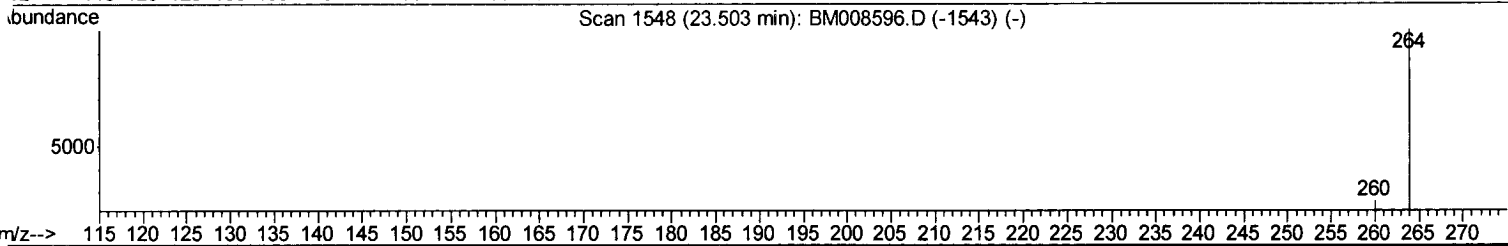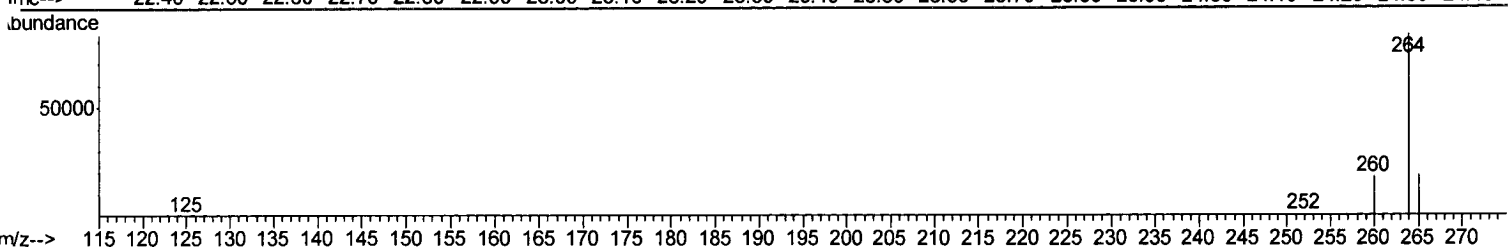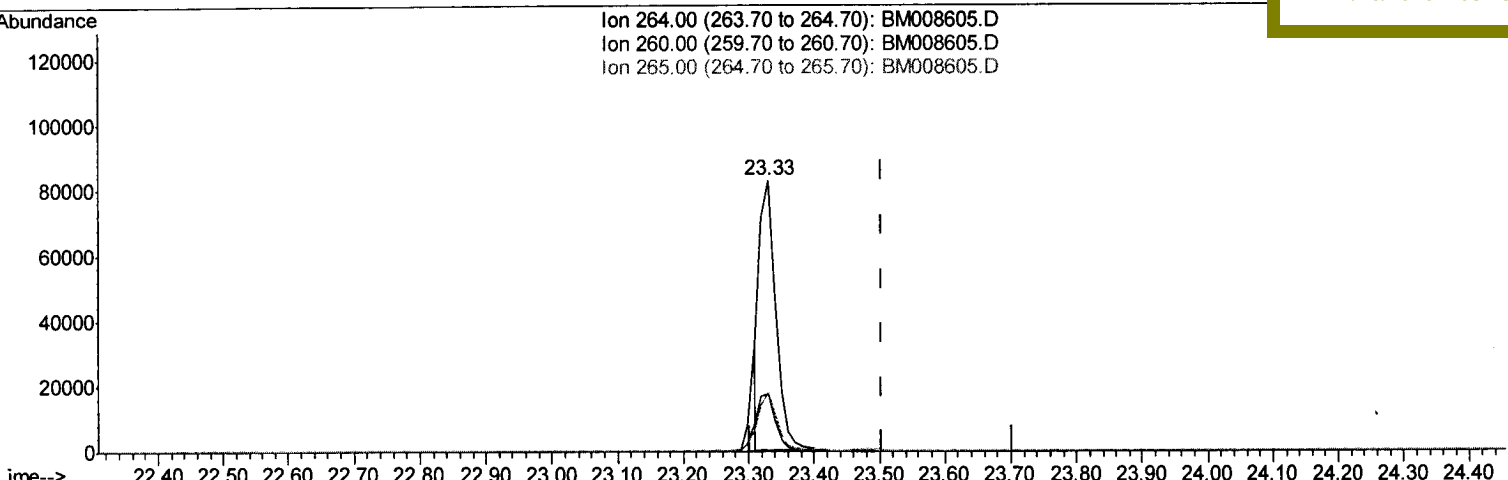

TIC: BM008605.D

(20) Perylene-d12 (I)

23.329min (-0.174) 0.40ng/ul

response 144762

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100    | 100    |
| 260.00 | 30.10  | 21.47# |
| 265.00 | 103.50 | 21.88# |
| 0.00   | 0.00   | 0.00   |

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
 Data File : BM008605.D  
 Acq On : 23 Dec 2016 20:55  
 Operator : UM/SJ  
 Sample : H6069-06  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DA7J2

Manual Integrations  
 APPROVED

sohil  
 12/26/2016 4:03:28 PM

Quant Time: Dec 23 23:42:42 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 23 23:37:39 2016  
 Response via : Initial Calibration

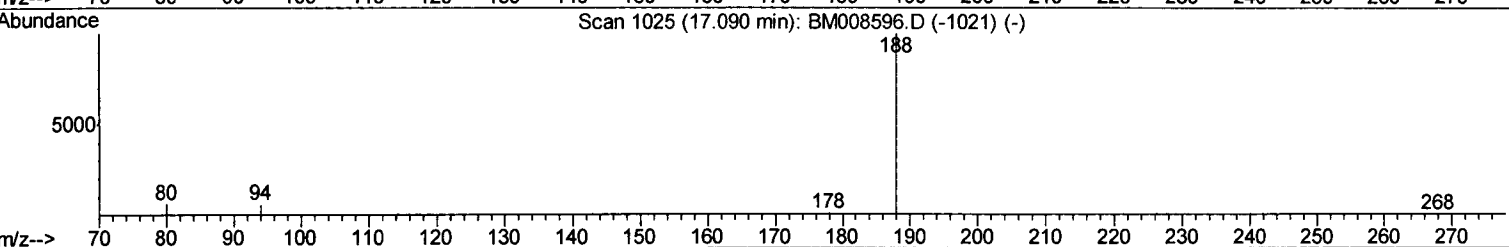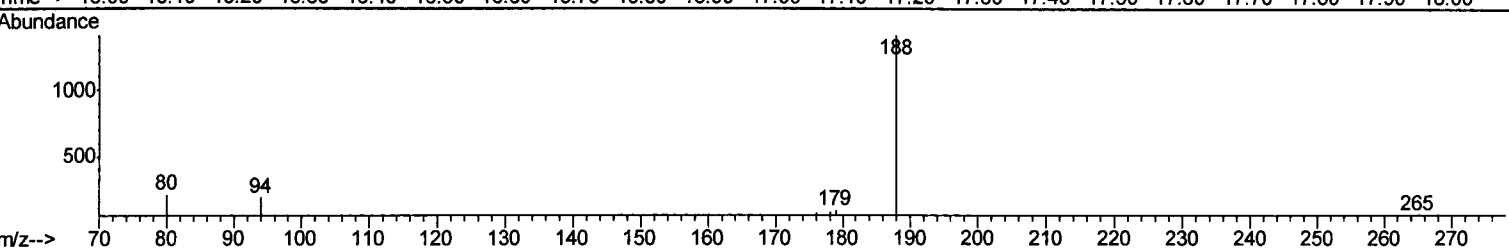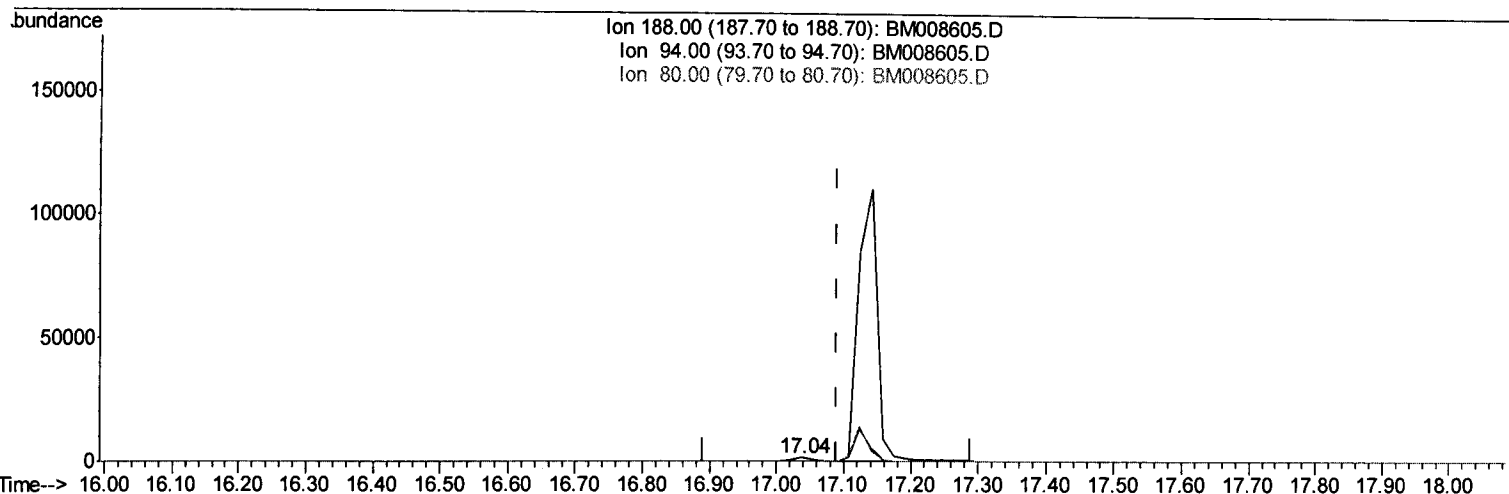

TIC: BM008605.D

(10) Phenanthrene-d10 (I)

17.039min (-0.052) 0.40ng/ul m

response 2107

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 188.00 | 100   | 100    |
| 94.00  | 11.00 | 13.05  |
| 80.00  | 11.80 | 14.82# |
| 0.00   | 0.00  | 0.00   |

S.J.  
 12/27/2016




Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
Data File : BM008605.D  
Acq On : 23 Dec 2016 20:55  
Operator : UM/SJ  
Sample : H6069-06  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DA7J2

Manual Integrations  
APPROVED

sohil  
12/26/2016 4:03:28 PM

Quant Time: Dec 23 23:42:42 2016  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 23 23:37:39 2016  
Response via : Initial Calibration

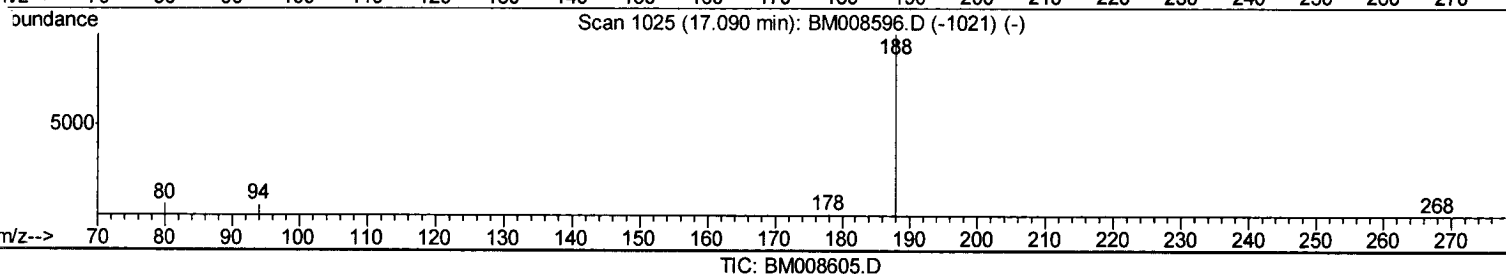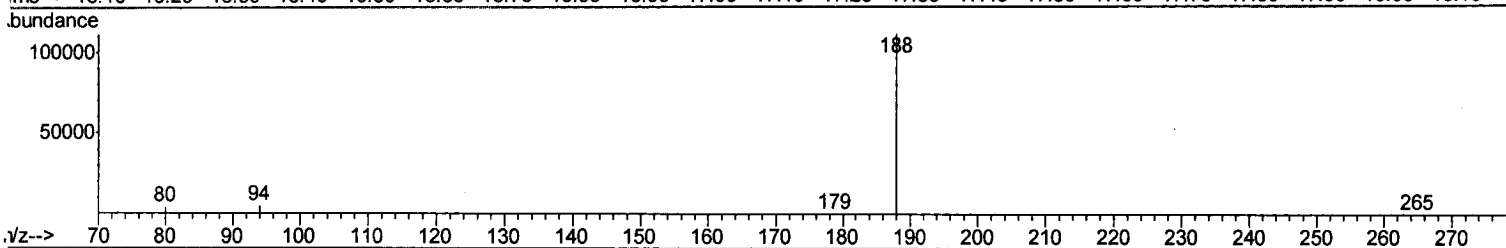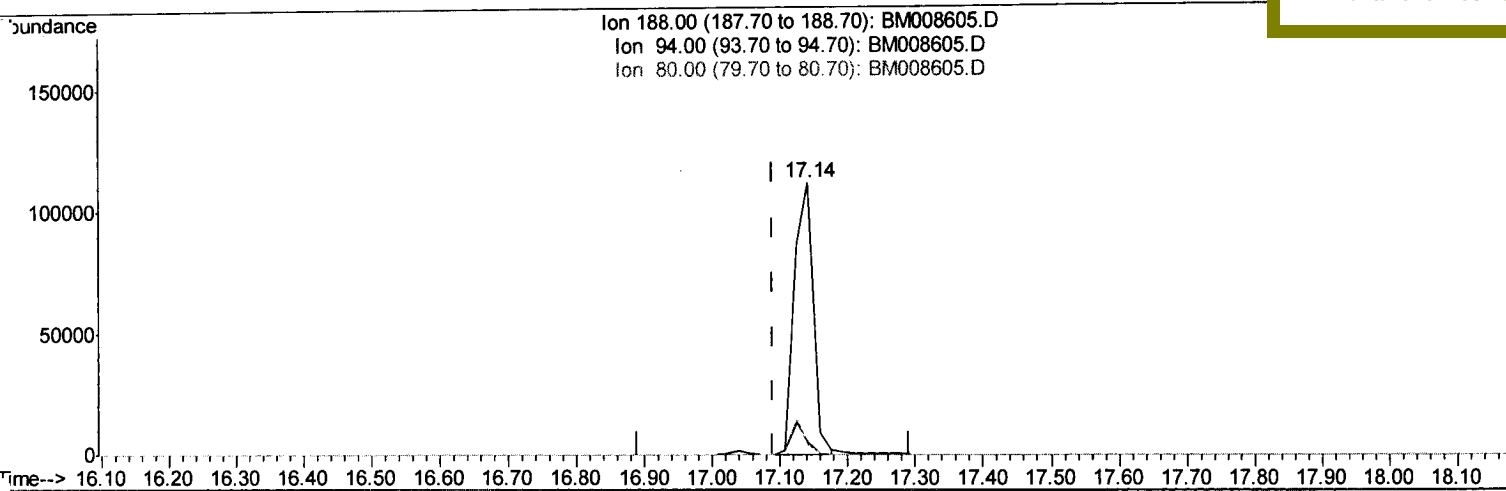

(10) Phenanthrene-d10 (I)

17.142min (+0.051) 0.40ng/ul

response 215826

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 188.00 | 100   | 100   |
| 94.00  | 11.00 | 4.34# |
| 80.00  | 11.80 | 3.53# |
| 0.00   | 0.00  | 0.00  |

a Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
 a File : BM008605.D  
 i On : 23 Dec 2016 20:55  
 rator : UM/SJ  
 mple : H6069-06  
 sc :  
 S Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA M  
 ClientSampleId :  
 DA7J2

Manual Integrations  
 APPROVED

sohil  
 12/26/2016 4:03:28 PM

ant Time: Dec 24 00:19:37 2016  
 ant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
 ant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 ast Update : Fri Dec 23 23:37:39 2016  
 sponse via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc | Units  | Dev(Min) |
|-----------------------------|-------|------|----------|------|--------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 7.65  | 152  | 451      | 0.40 | ng/ul  | -0.09    |
| 2) Naphthalene-d8           | 10.42 | 136  | 1581     | 0.40 | ng/ul  | -0.08    |
| 6) Acenaphthene-d10         | 14.28 | 164  | 1084     | 0.40 | ng/ul  | -0.03    |
| 10) Phenanthrene-d10        | 17.04 | 188  | 2107m    | 0.40 | ng/ul  | -0.05    |
| 16) Chrysene-d12            | 21.26 | 240  | 1679     | 0.40 | ng/ul  | -0.02    |
| 20) Perylene-d12            | 23.49 | 264  | 1234m    | 0.40 | ng/ul  | -0.02    |
| System Monitoring Compounds |       |      |          |      |        |          |
| 4) 2-Methylnaphthalene-d10  | 12.03 | 152  | 1093     | 0.45 | ng/ul  | -0.07    |
| 14) Fluoranthene-d10        | 19.09 | 212  | 2651m    | 0.46 | ng/ul  | -0.02    |
| Target Compounds            |       |      |          |      |        |          |
| 3) Naphthalene              | 10.46 | 128  | 1097     | 0.25 | ng/ul# | 86       |
| 5) 2-Methylnaphthalene      | 12.10 | 142  | 1153     | 0.39 | ng/ul  | 100      |
| 8) Acenaphthene             | 14.35 | 153  | 160      | 0.04 | ng/ul# | 85       |
| 12) Phenanthrene            | 17.07 | 178  | 2635     | 0.41 | ng/ul  | 99       |
| 15) Fluoranthene            | 19.11 | 202  | 2097     | 0.27 | ng/ul  | 95       |
| 17) Pyrene                  | 19.48 | 202  | 2291     | 0.35 | ng/ul# | 92       |
| 18) Benzo(a)anthracene      | 21.24 | 228  | 937      | 0.17 | ng/ul# | 79       |
| 19) Chrysene                | 21.30 | 228  | 1096     | 0.18 | ng/ul# | 81       |
| 21) Benzo(b)fluoranthene    | 22.81 | 252  | 1394m    | 0.29 | ng/ul  |          |
| 22) Benzo(k)fluoranthene    | 22.85 | 252  | 394m     | 0.08 | ng/ul  |          |
| 23) Benzo(a)pyrene          | 23.37 | 252  | 751m     | 0.17 | ng/ul  |          |
| 24) Indeno(1,2,3-cd)pyrene  | 25.74 | 276  | 585m     | 0.11 | ng/ul  |          |
| 26) Benzo(g,h,i)perylene    | 26.43 | 276  | 599m     | 0.13 | ng/ul  |          |

S.S.

12/27/2016

S.S.

12/27/2016

(#) = qualifier out of range (m) = manual integration (+) = signals summed

# Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM122316\  
 Data File : BM008605.D  
 Acq On : 23 Dec 2016 20:55  
 Operator : UM/SJ  
 Sample : H6069-06  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DA7J2

Manual Integrations  
 APPROVED

sohil  
 12/26/2016 4:03:28 PM

Quant Time: Dec 24 00:19:37 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM121916.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 23 23:37:39 2016  
 Response via : Initial Calibration

