
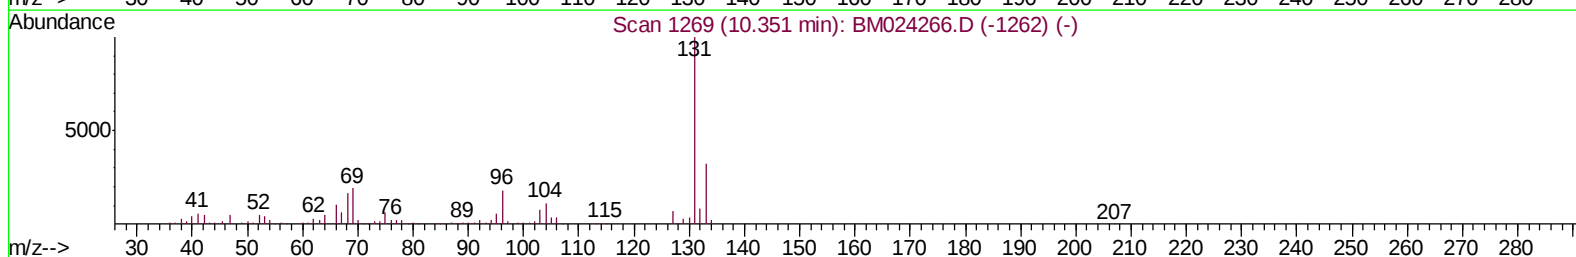
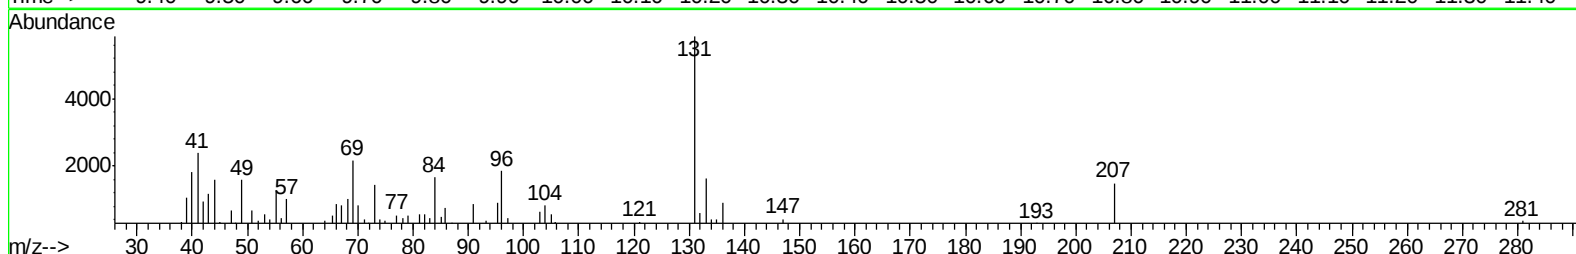


Data File : BM024268.D
Acq On : 24 Dec 2019 23:49
Operator : JU
Sample : K6240-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 25 03:36:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

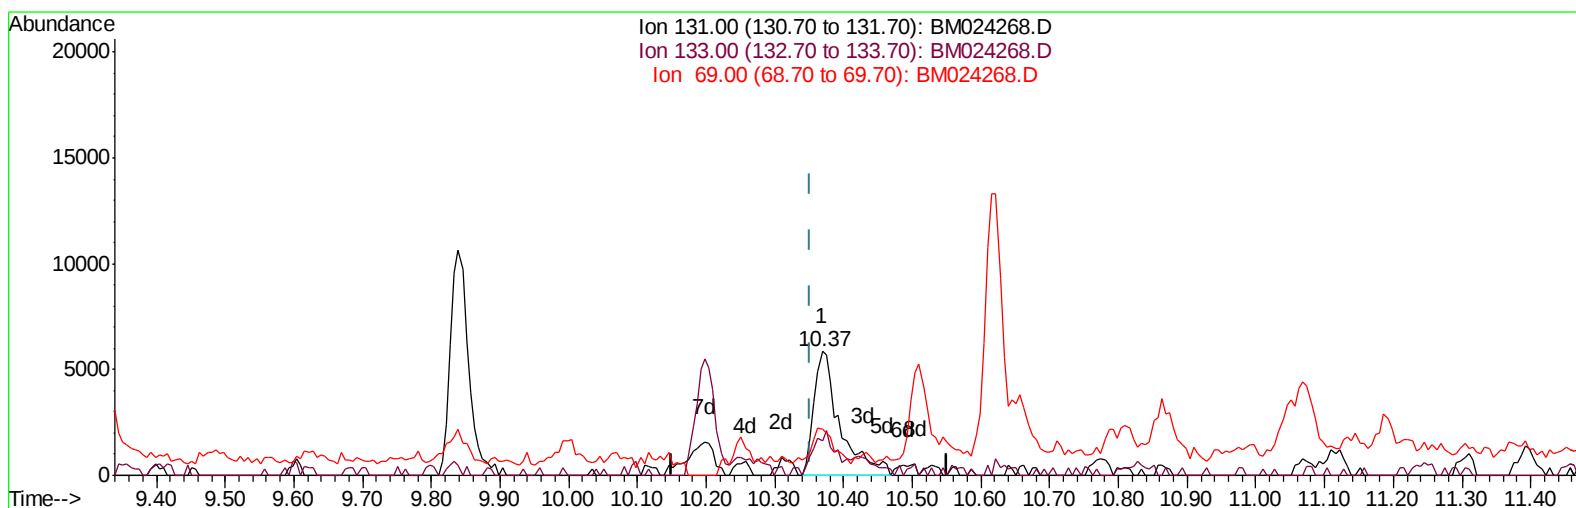

TIC: BM024268.D

(29) 4-Chloroaniline-d4 (S)

10.369min (+0.017) 0.62ng/ul m

response 15320

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	27.83
69.00	19.00	36.76#
0.00	0.00	0.00