
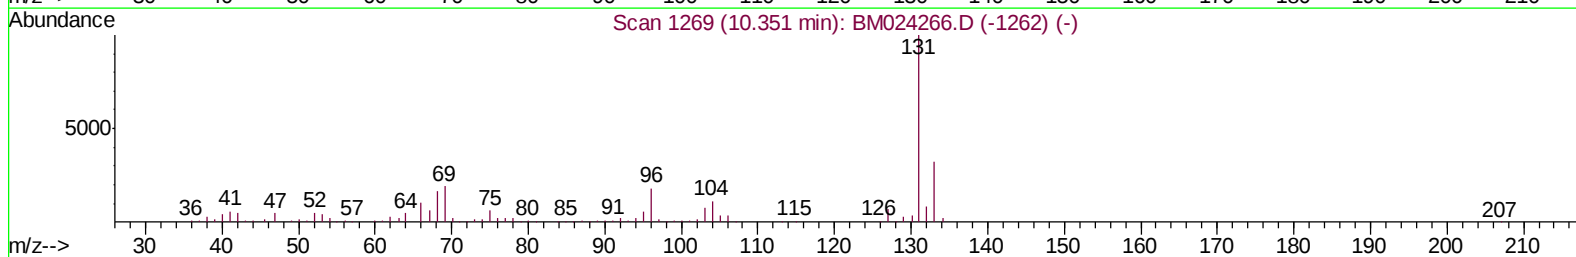
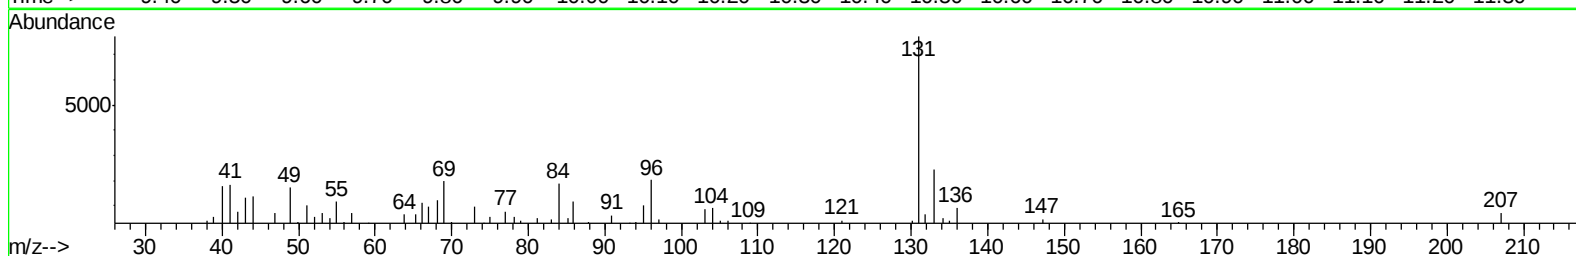


Data File : BM024270.D  
Acq On : 25 Dec 2019 01:01  
Operator : JU  
Sample : K6240-15  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 25 03:36:40 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM121719MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Dec 25 03:33:48 2019  
Response via : Initial Calibration

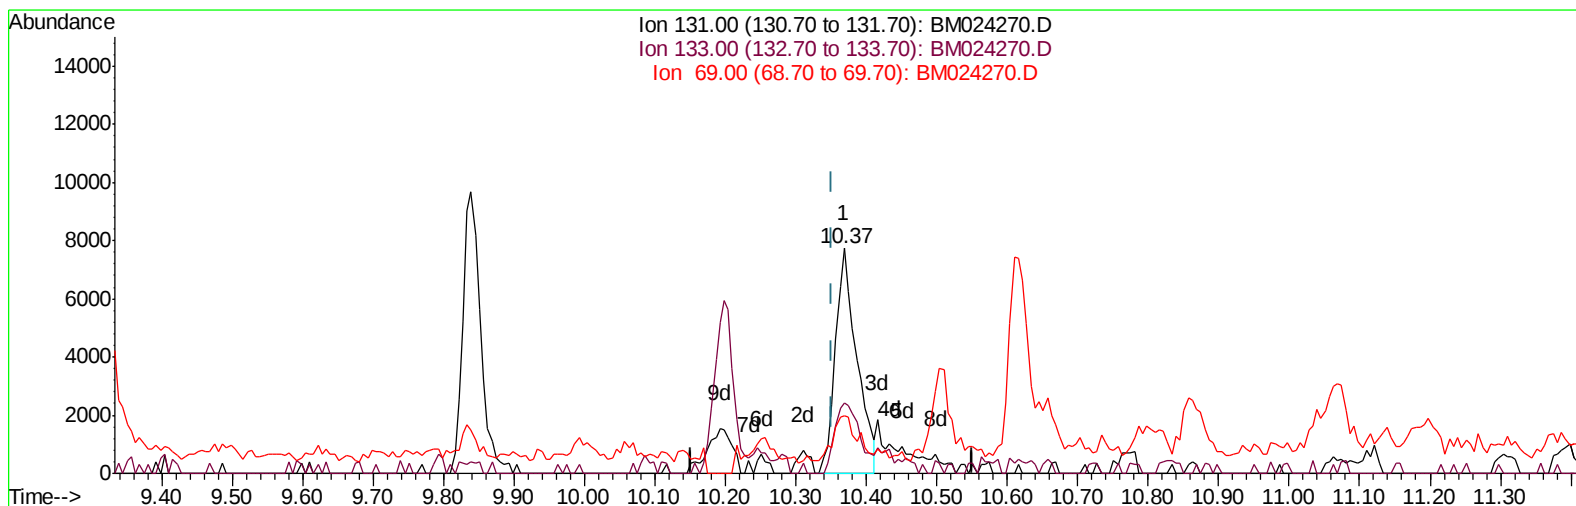

TIC: BM024270.D

(29) 4-Chloroaniline-d4 (S)  
10.369min (+0.017) 0.65ng/ul  
response 16285

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 131.00 | 100   | 100    |
| 133.00 | 32.50 | 31.38  |
| 69.00  | 19.00 | 25.42# |
| 0.00   | 0.00  | 0.00   |