
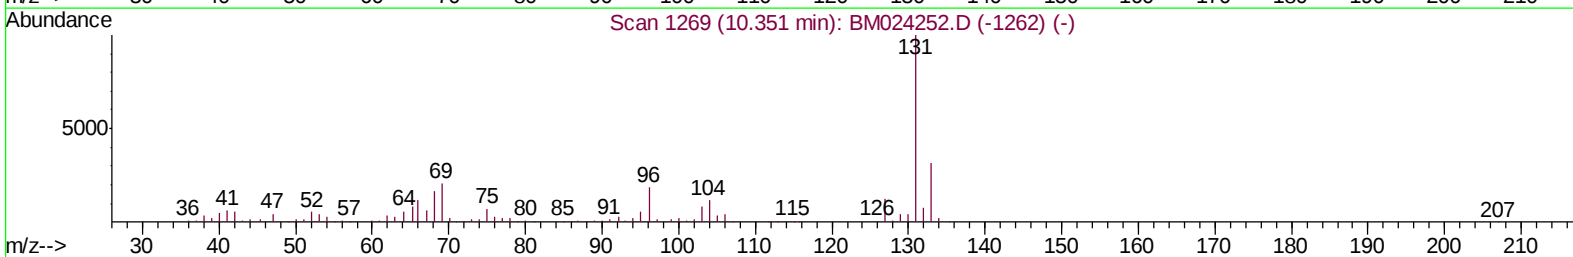
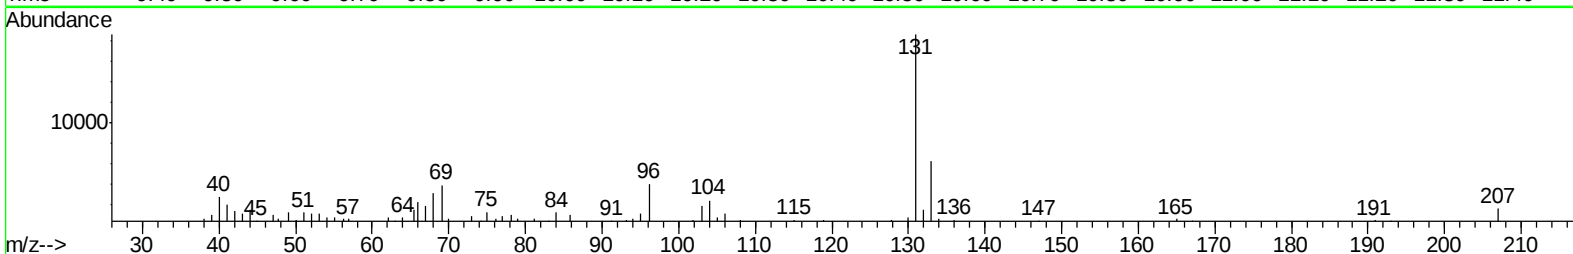


Data File : BM024260.D
Acq On : 24 Dec 2019 18:26
Operator : JU
Sample : K6240-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 25 02:51:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 02:48:28 2019
Response via : Initial Calibration

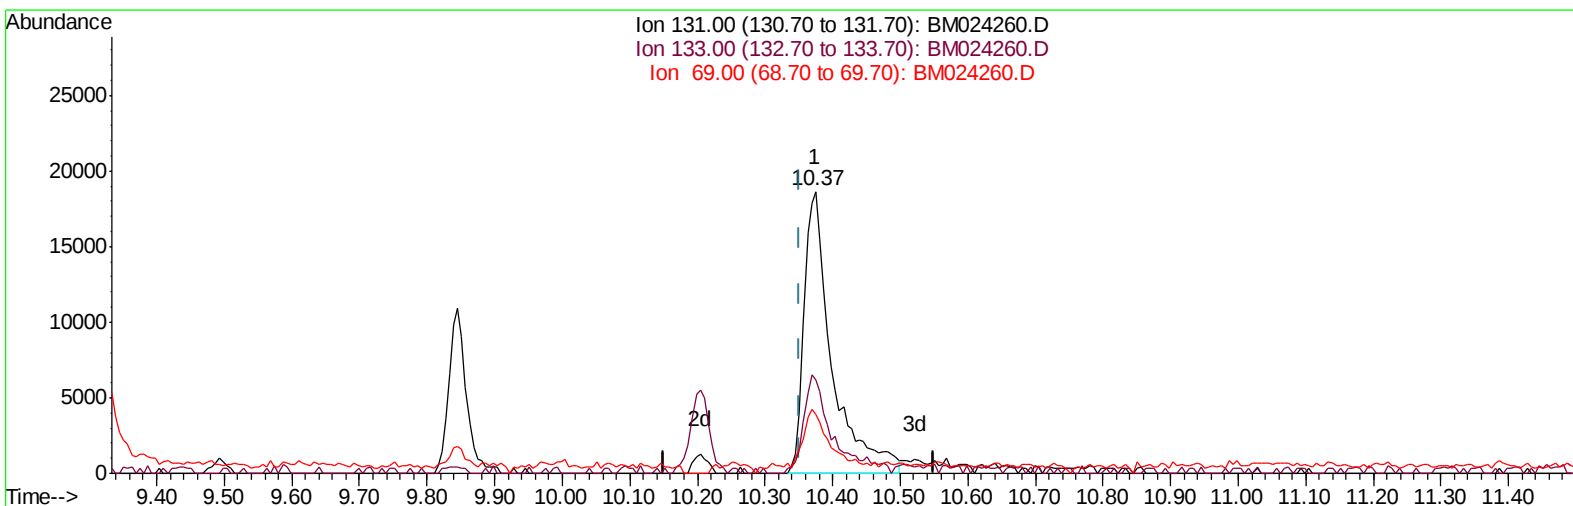

TIC: BM024260.D

(29) 4-Chloroaniline-d4 (S)

10.375min (+0.024) 2.27ng/ul m

response 53287

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	33.31
69.00	19.00	20.76
0.00	0.00	0.00