
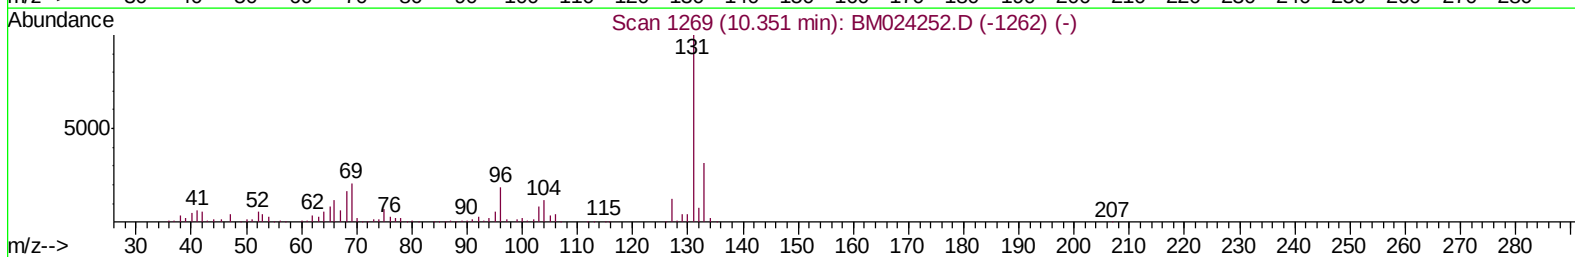
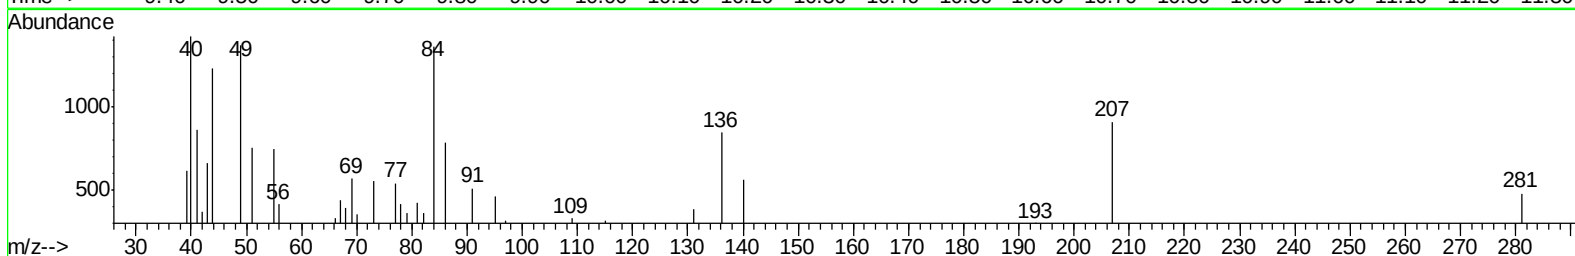


Data File : BM024262.D
Acq On : 24 Dec 2019 19:38
Operator : JU
Sample : K6240-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 25 02:51:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 02:48:28 2019
Response via : Initial Calibration

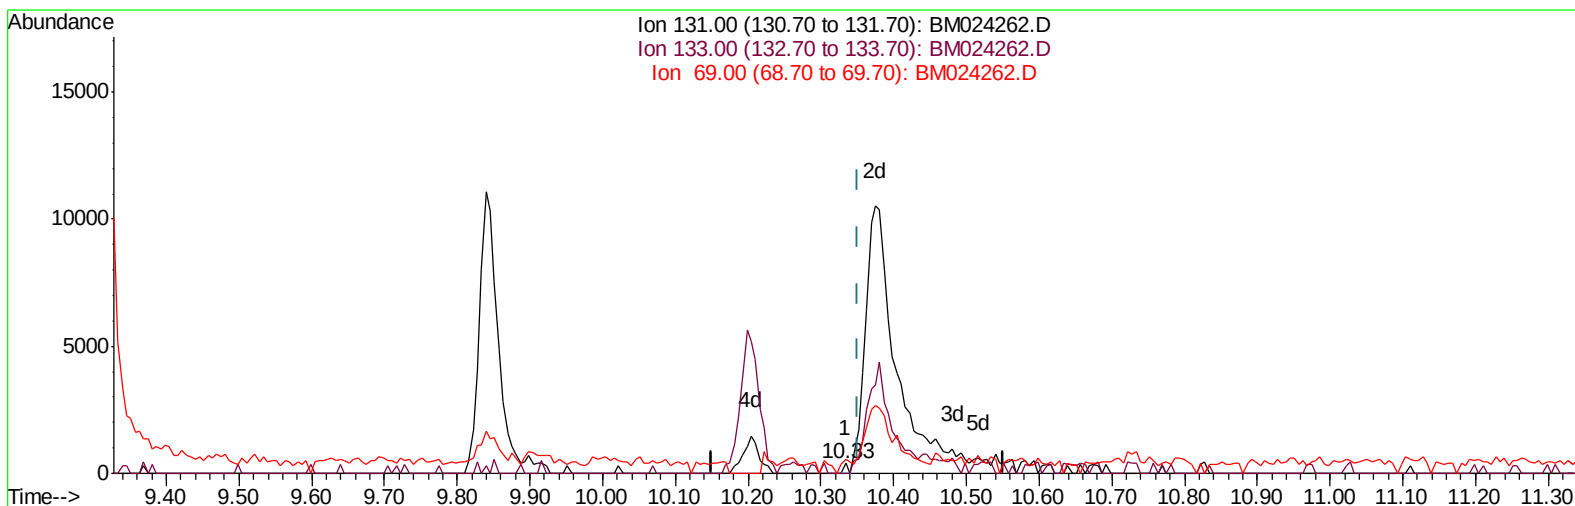

TIC: BM024262.D

(29) 4-Chloroaniline-d4 (S)
10.334min (-0.018) 0.01ng/ul
response 135

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	0.00#
69.00	19.00	147.78#
0.00	0.00	0.00