
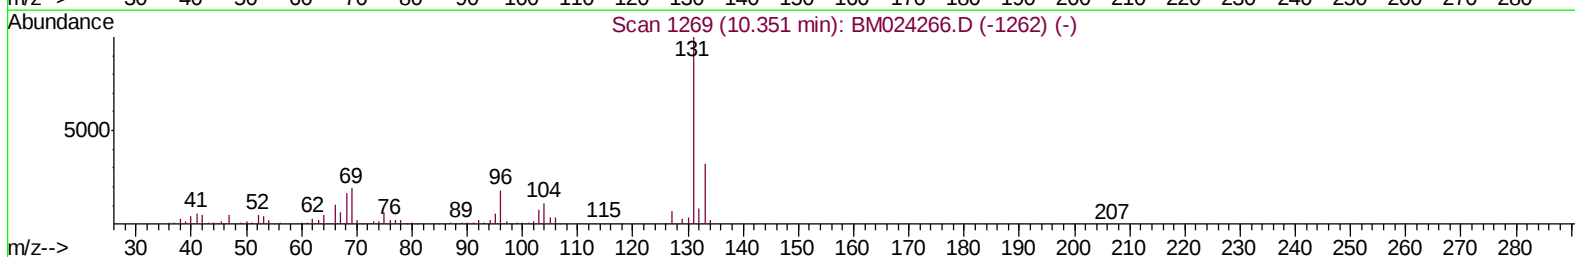
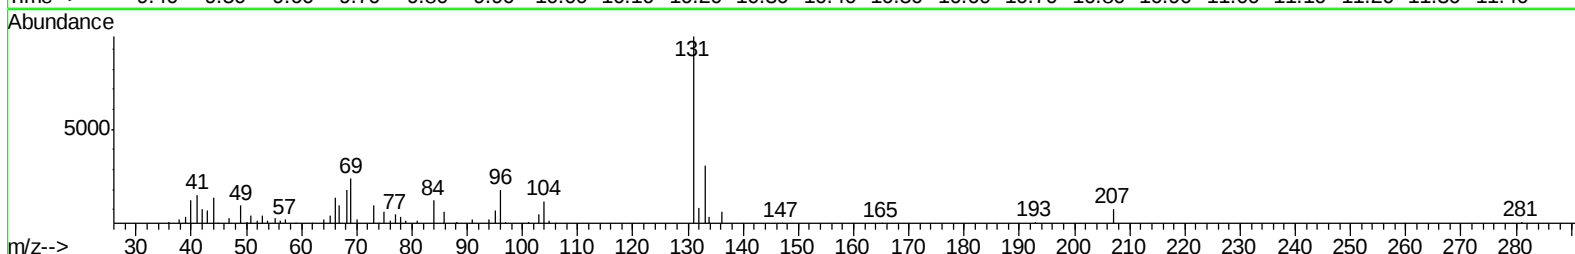


Data File : BM024271.D
Acq On : 25 Dec 2019 01:36
Operator : JU
Sample : K6240-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Dec 25 03:36:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

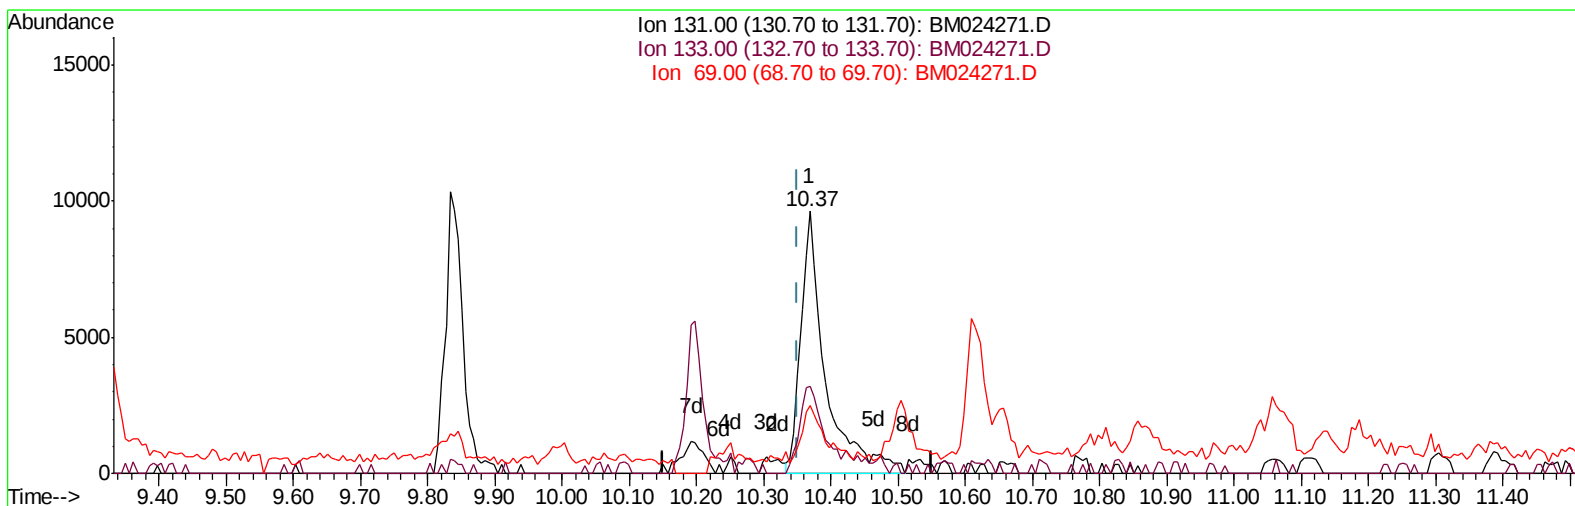

TIC: BM024271.D

(29) 4-Chloroaniline-d4 (S)

10.369min (+0.017) 1.12ng/ul m

response 24423

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	33.13
69.00	19.00	26.10#
0.00	0.00	0.00