
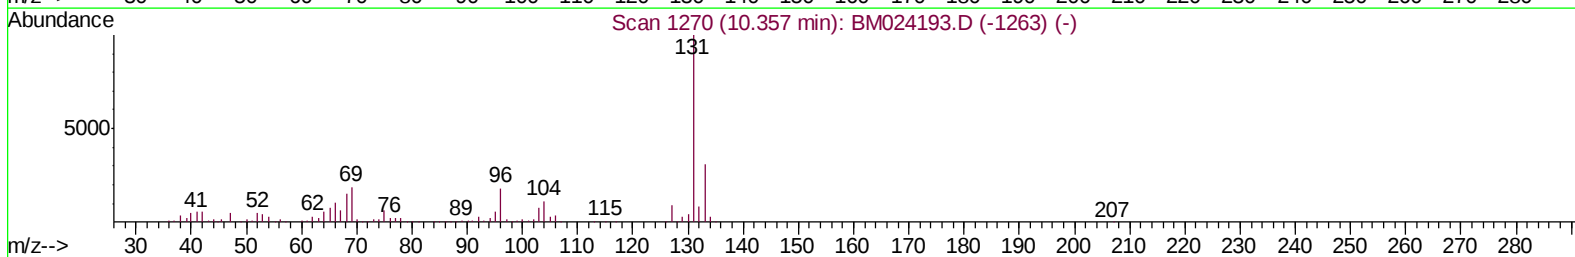
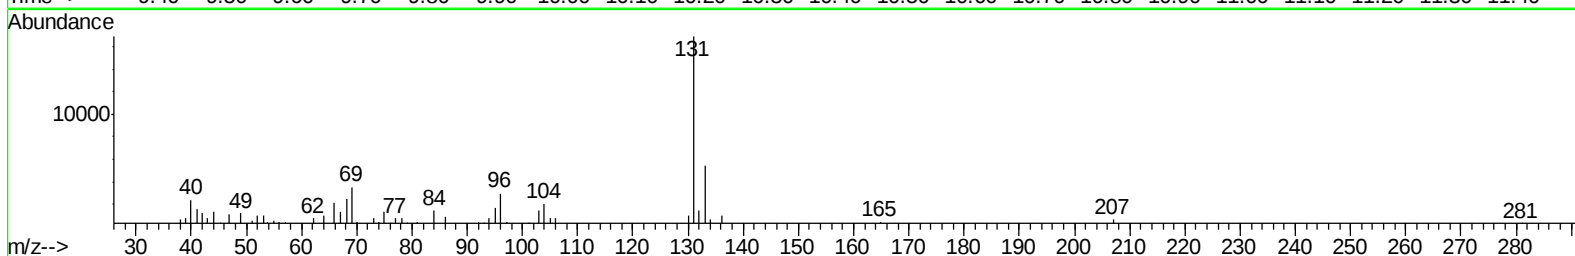


Data File : BM024276.D
Acq On : 25 Dec 2019 04:35
Operator : JU
Sample : K6240-22
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 25 06:35:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

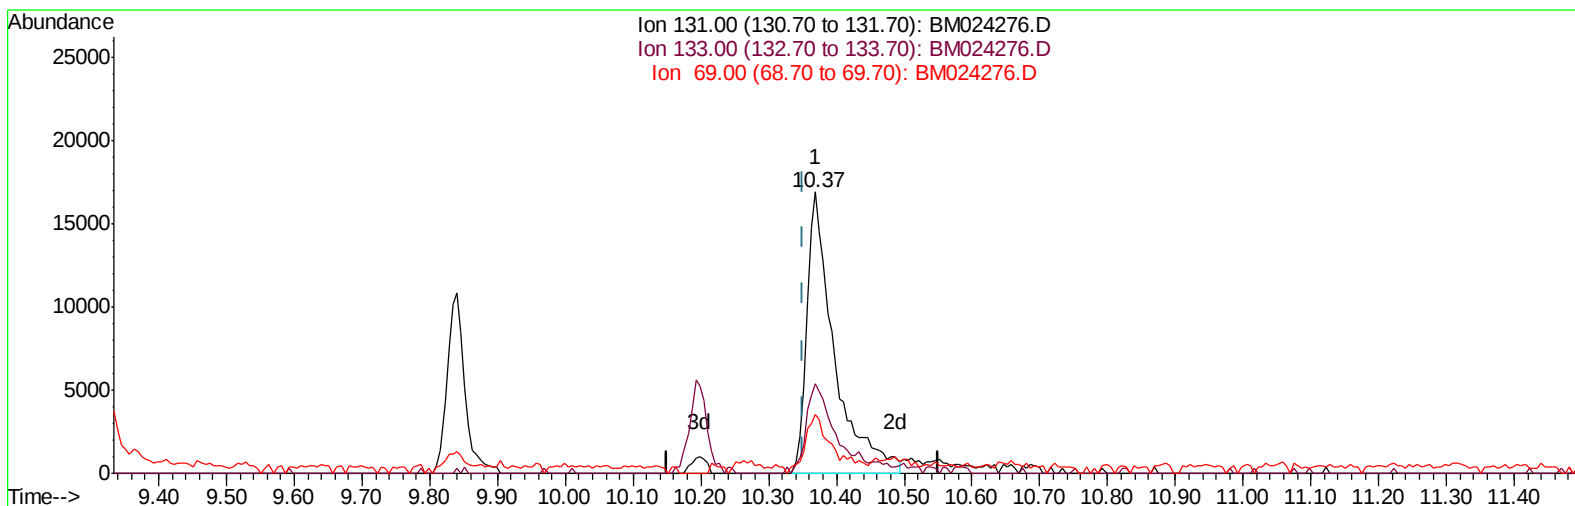

TIC: BM024276.D

(29) 4-Chloroaniline-d4 (S)

10.369min (+0.018) 2.07ng/ul m

response 47650

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	31.90
69.00	19.00	20.90
0.00	0.00	0.00