

Data File : BM024240.D
Acq On : 24 Dec 2019 06:20
Operator : JU
Sample : K6236-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFEZ1

Quant Time: Dec 24 07:33:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 05:54:49 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	259817	20.00	ng/ul	0.00
18) Naphthalene-d8	10.20	136	1125366	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	696462	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1401122	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	1236072	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	1455017	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.99	96	27961	4.75	ng/uL	0.00
5) Phenol-d5	6.63	99	532514	21.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	384214	26.04	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	428330	24.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	421104	20.94	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	202890	25.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	226540	25.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	412008	23.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	526576	25.08	ng/ul	0.00
44) Dimethylphthalate-d6	13.52	166	1347760	26.17	ng/ul	0.00
47) Acenaphthylene-d8	13.78	160	1590289	25.77	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	109268	11.82	ng/ul	0.00
58) Fluorene-d10	15.10	176	1175402	26.03	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	125261	14.65	ng/ul	0.00
71) Anthracene-d10	16.95	188	1694222	26.58	ng/ul	0.00
79) Pyrene-d10	19.26	212	1737003	29.50	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	1874317	25.93	ng/ul	0.00

Target Compounds					Qvalue
6) Phenol	6.65	94	75884	2.987 ng/ul	90
45) Dimethylphthalate	13.57	163	187212	3.498 ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM024240.D

Acq On : 24 Dec 2019 06:20

Operator : JU

Sample : K6236-08

Misc :

ALS Vial : 28 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

BFEZ1


Quant Time: Dec 24 07:33:23 2019


Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Dec 24 05:54:49 2019

Response via : Initial Calibration

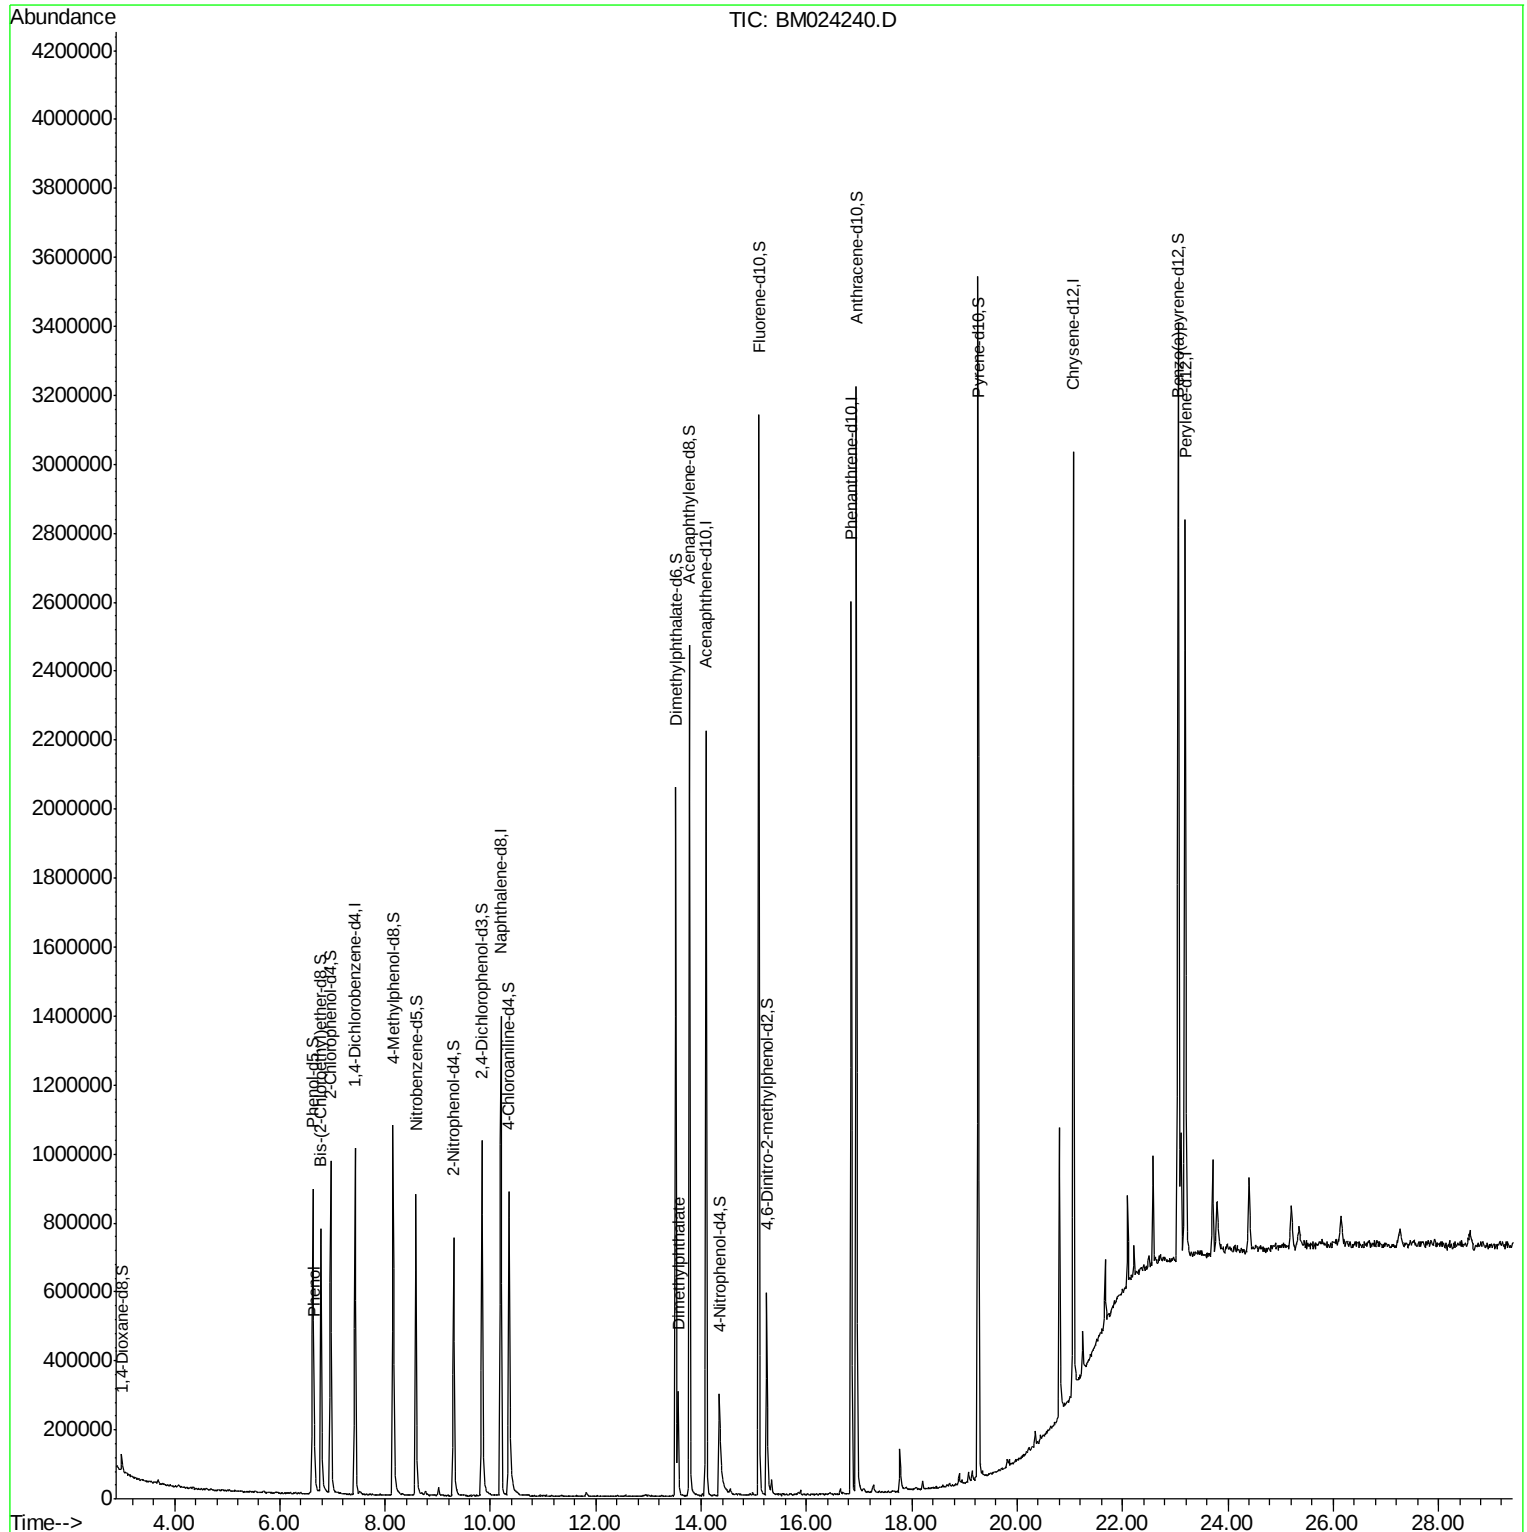

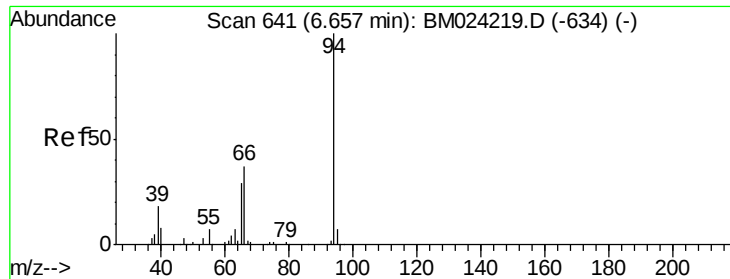

#6

Phenol

Concen: 2.987 ng/ul

RT: 6.65 min Scan# 640

Delta R.T. 0.00 min

Lab File: BM024240.D

Acq: 24 Dec 2019 06:20

Instrument :

BNA_M

ClientSampleId :

BFEZ1


Tgt Ion: 94 Resp: 75884

Ion Ratio Lower Upper

94 100

65 32.3 22.6 33.8




66 45.8 30.7 46.1

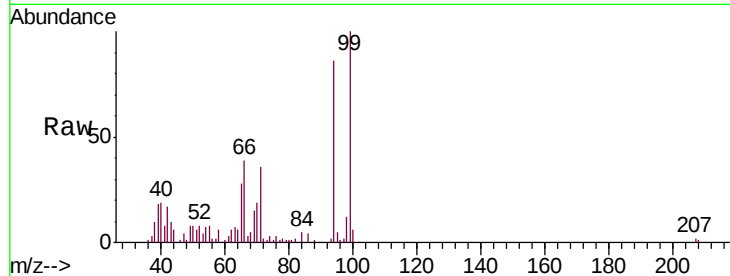

Abundance Ion 94.00 (93.70 to 94.70): BM024219.D (-634) (-)

Ion 65.00 (64.70 to 65.70): BM024219.D (-634) (-)

Ion 66.00 (65.70 to 66.70): BM024219.D (-634) (-)

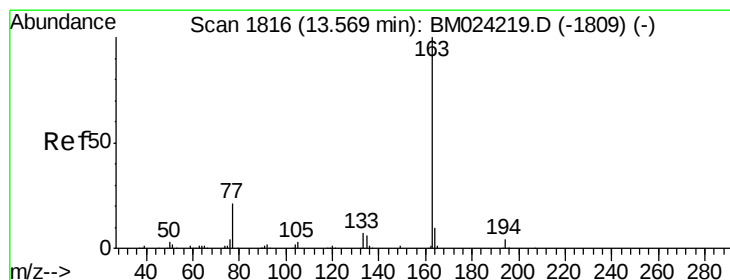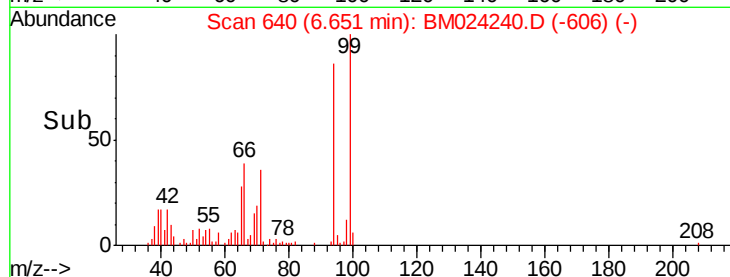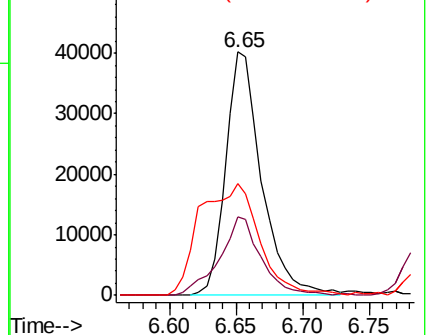

#45

Dimethylphthalate

Concen: 3.498 ng/ul

RT: 13.57 min Scan# 1816

Delta R.T. 0.00 min

Lab File: BM024240.D

Acq: 24 Dec 2019 06:20


Tgt Ion: 163 Resp: 187212

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 9.6 7.8 11.6

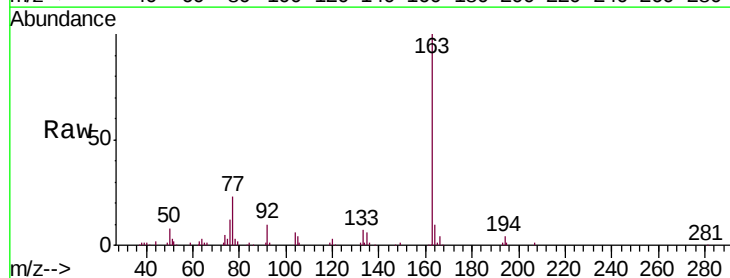

Abundance Ion 163.00 (162.70 to 163.70): BM024219.D (-1809) (-)

Ion 194.00 (193.70 to 194.70): BM024219.D (-1809) (-)

Ion 164.00 (163.70 to 164.70): BM024219.D (-1809) (-)

