

Data File : BM024275.D
Acq On : 25 Dec 2019 04:00
Operator : JU
Sample : K6240-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQS6

Quant Time: Dec 25 06:35:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	291020	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	1210817	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	693258	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1388630	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	1284756	20.00	ng/ul	0.00
86) Perylene-d12	23.20	264	1538458	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.99	96	31765	4.82	ng/uL	0.00
5) Phenol-d5	6.63	99	168568	6.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	419864	25.41	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	449498	22.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	320410	14.22	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	254305	29.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	287308	30.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	513345	27.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	83899	3.71	ng/ul	0.01
44) Dimethylphthalate-d6	13.52	166	1747755	34.09	ng/ul	0.00
47) Acenaphthylene-d8	13.78	160	2090462	34.03	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	40985	4.45	ng/ul	0.02
58) Fluorene-d10	15.10	176	1481861	32.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	136144	16.07	ng/ul	0.00
71) Anthracene-d10	16.95	188	2227868	35.26	ng/ul	0.00
79) Pyrene-d10	19.26	212	2360498	38.57	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2747753	35.96	ng/ul	0.00


Target Compounds					Qvalue	
45) Dimethylphthalate	13.57	163	66754	1.253	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM024275.D
Acq On : 25 Dec 2019 04:00
Operator : JU
Sample : K6240-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQS6

Quant Time: Dec 25 06:35:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

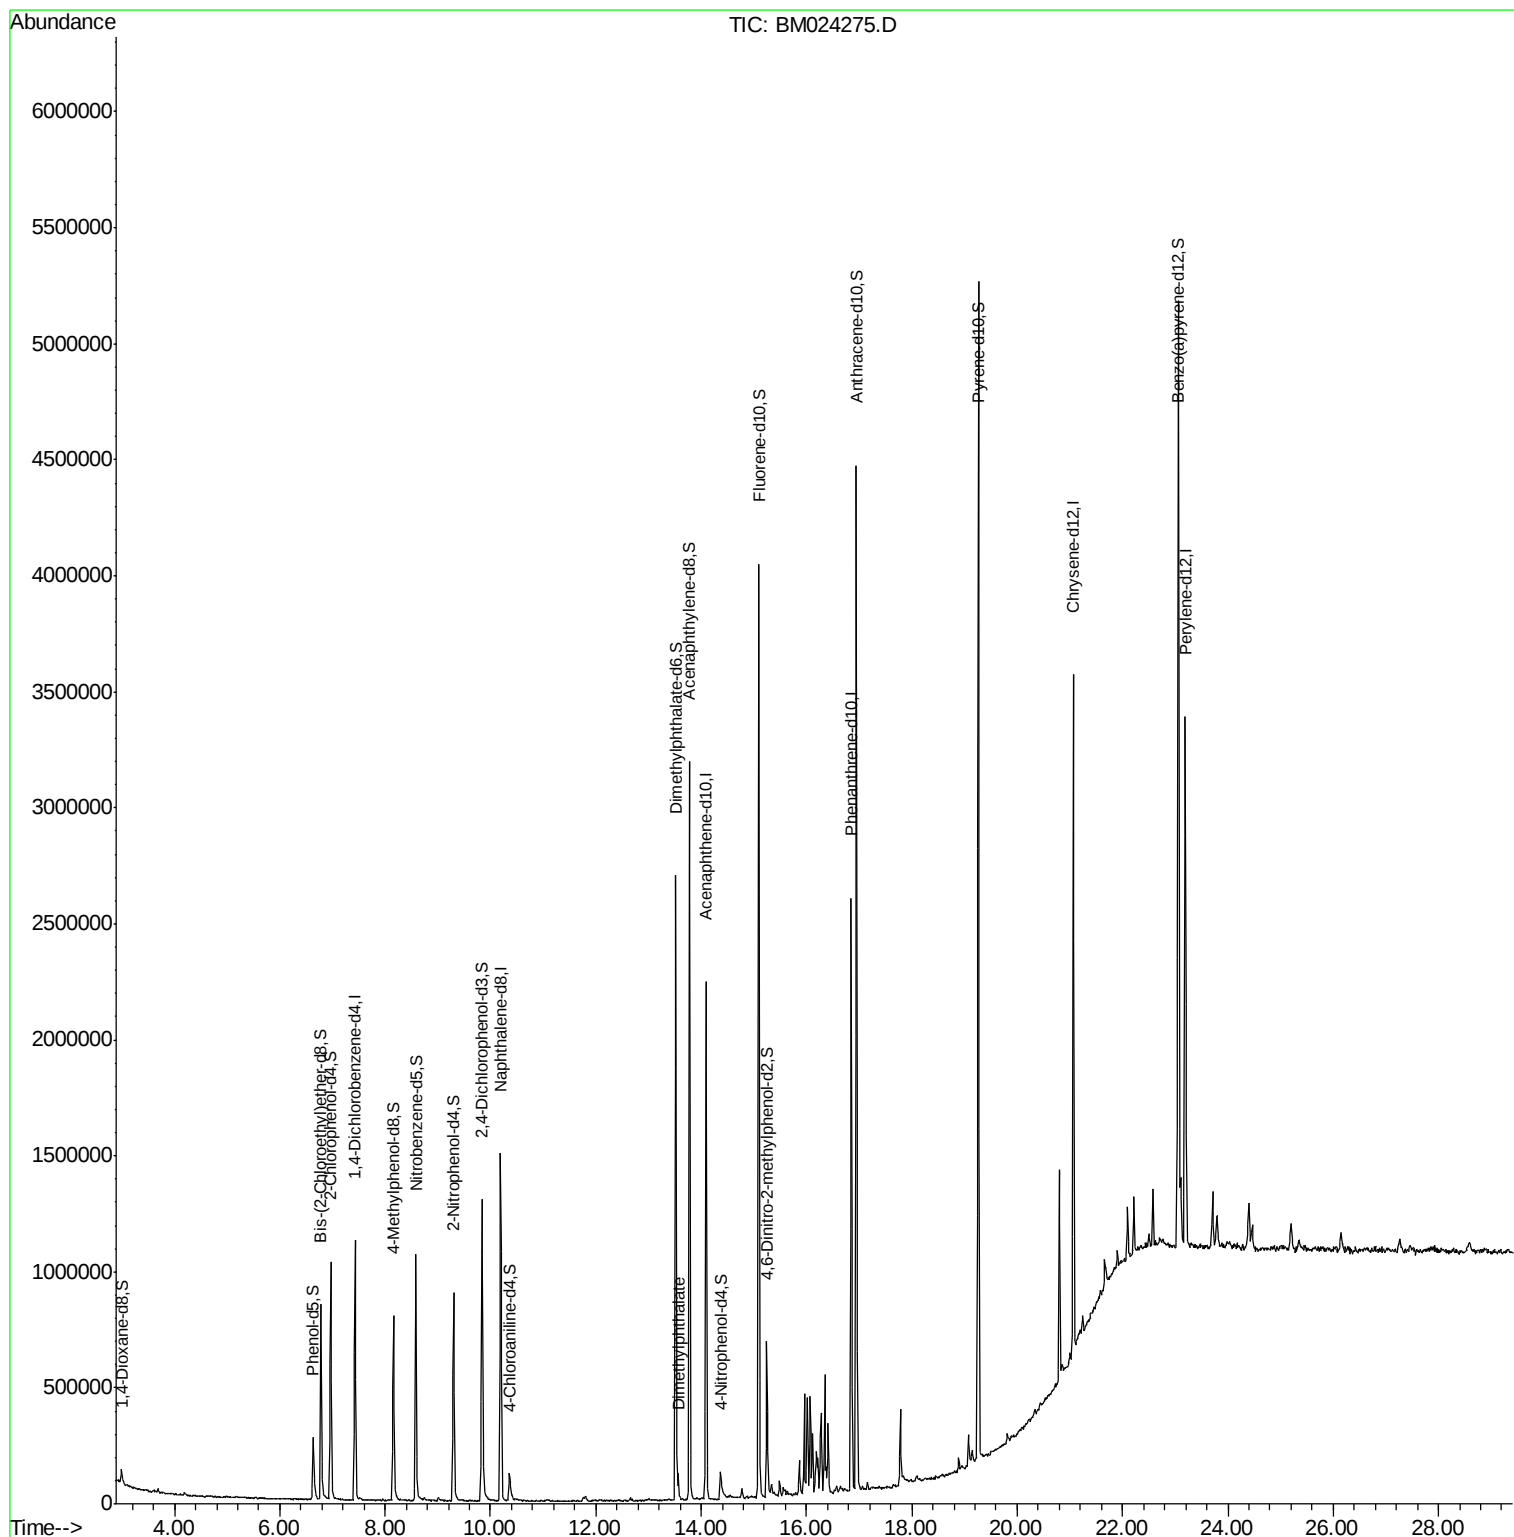

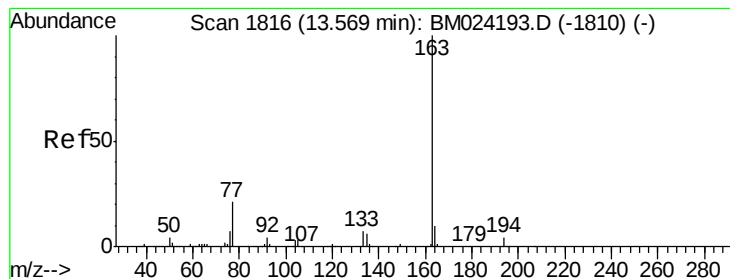

#45

Dimethylphthalate

Concen: 1.253 ng/ul

RT: 13.57 min Scan# 1816

Delta R.T. -0.00 min

Lab File: BM024275.D

Acq: 25 Dec 2019 04:00

Instrument :

BNA_M

ClientSampleId :

BFQS6


Tgt Ion:163 Resp: 66754

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 9.6 7.8 11.6

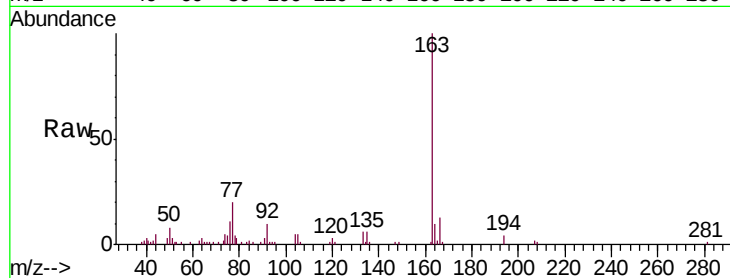

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

