

Data File : BM024276.D
Acq On : 25 Dec 2019 04:35
Operator : JU
Sample : K6240-22
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQS7

Quant Time: Dec 25 06:35:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	298556	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	1236297	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	706297	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1408682	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	1269671	20.00	ng/ul	0.00
86) Perylene-d12	23.20	264	1536484	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.99	96	37213	5.51	ng/uL	0.00
5) Phenol-d5	6.63	99	198584	7.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	457934	27.01	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	497935	24.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	356685	15.44	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	277741	31.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	316172	32.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	540578	28.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	42872	1.86	ng/ul	0.02
44) Dimethylphthalate-d6	13.52	166	1766223	33.82	ng/ul	0.00
47) Acenaphthylene-d8	13.78	160	2130851	34.05	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	49258	5.25	ng/ul	0.02
58) Fluorene-d10	15.10	176	1487933	32.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	129823	15.11	ng/ul	0.00
71) Anthracene-d10	16.95	188	2191953	34.20	ng/ul	0.00
79) Pyrene-d10	19.26	212	2290110	37.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2577158	33.77	ng/ul	0.00


Target Compounds					Qvalue	
45) Dimethylphthalate	13.56	163	70798	1.304	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM024276.D
Acq On : 25 Dec 2019 04:35
Operator : JU
Sample : K6240-22
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQS7

Quant Time: Dec 25 06:35:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

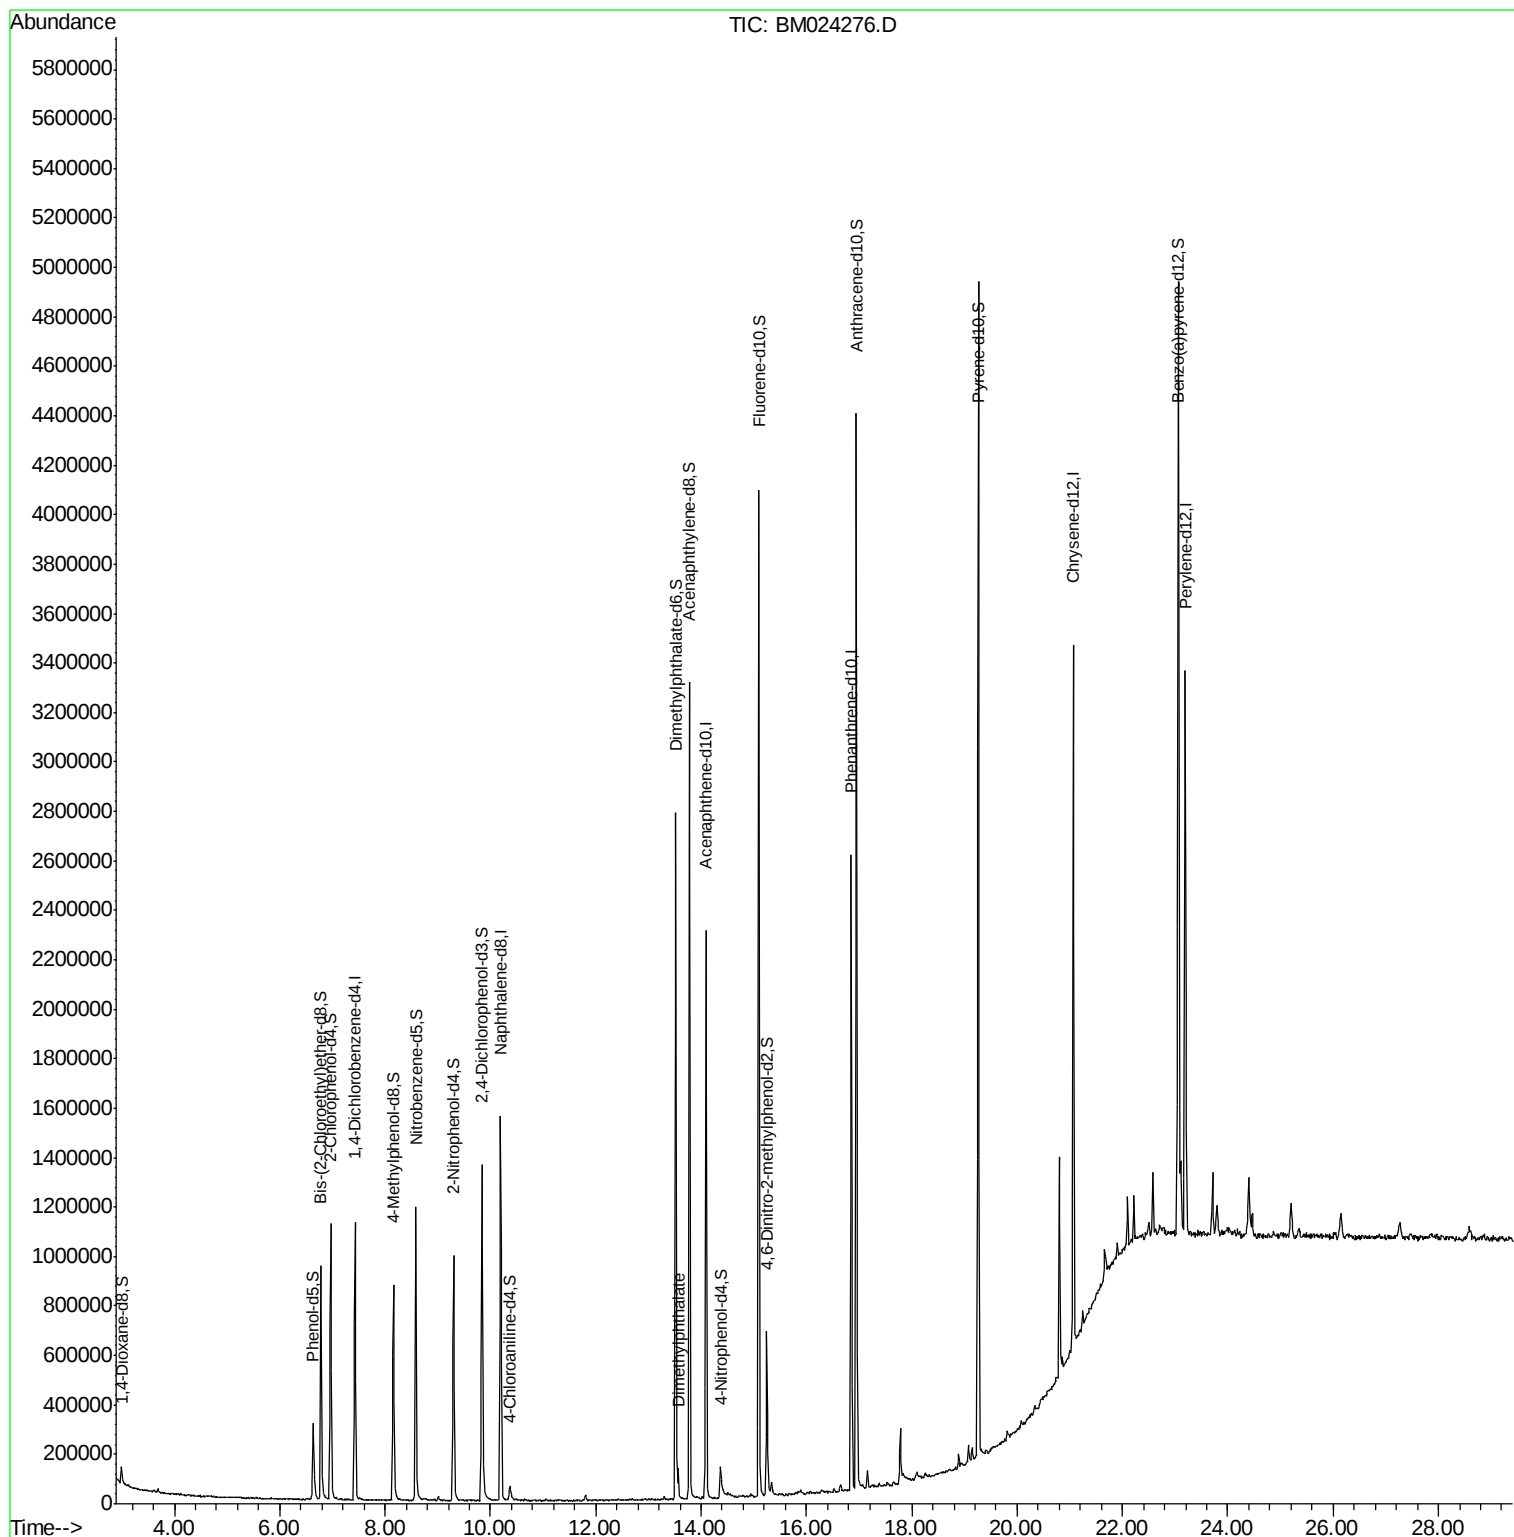

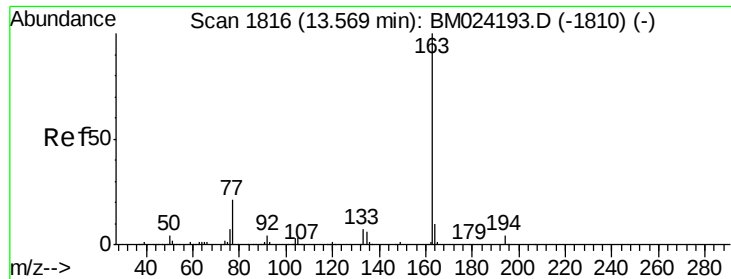

#45

Dimethylphthalate

Concen: 1.304 ng/ul

RT: 13.56 min Scan# 1815

Delta R.T. -0.01 min

Lab File: BM024276.D

Acq: 25 Dec 2019 04:35

Instrument :

BNA_M

ClientSampleId :

BFQS7


Tgt Ion:163 Resp: 70798

Ion Ratio Lower Upper

163 100

194 3.4 3.2 4.8

164 9.7 7.8 11.6

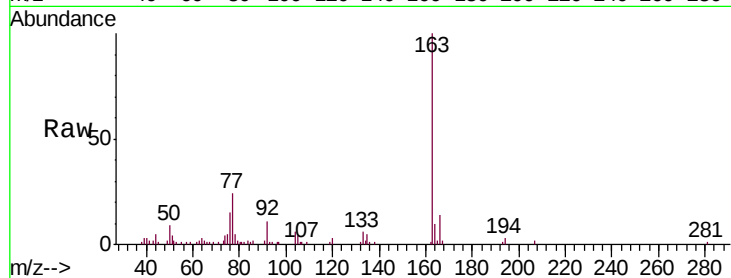

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

