

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122319\
 Data File : BM024286.D
 Acq On : 25 Dec 2019 13:17
 Operator : JU
 Sample : K6276-20
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 25 13:58:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 25 03:33:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	260282	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	1116416	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	647895	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.85	188	1298140	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1172259	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	1427809	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.99	96	28063	4.76	ng/uL	0.00
5) Phenol-d5	6.63	99	145436	5.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	406439	27.50	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	405595	23.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	276240	13.71	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	244395	30.46	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	271730	30.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.83	165	462248	26.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	23966	1.15	ng/ul	0.02
44) Dimethylphthalate-d6	13.52	166	1638781	34.21	ng/ul	0.00
47) Acenaphthylene-d8	13.77	160	1911107	33.29	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	34299	3.99	ng/ul	0.02
58) Fluorene-d10	15.09	176	1371246	32.65	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	143208	18.08	ng/ul	0.00
71) Anthracene-d10	16.94	188	2106095	35.66	ng/ul	0.00
79) Pyrene-d10	19.26	212	2259228	40.46	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2617105	36.90	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.56	163	57666	1.158	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122319\
Data File : BM024286.D
Acq On : 25 Dec 2019 13:17
Operator : JU
Sample : K6276-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 25 13:58:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

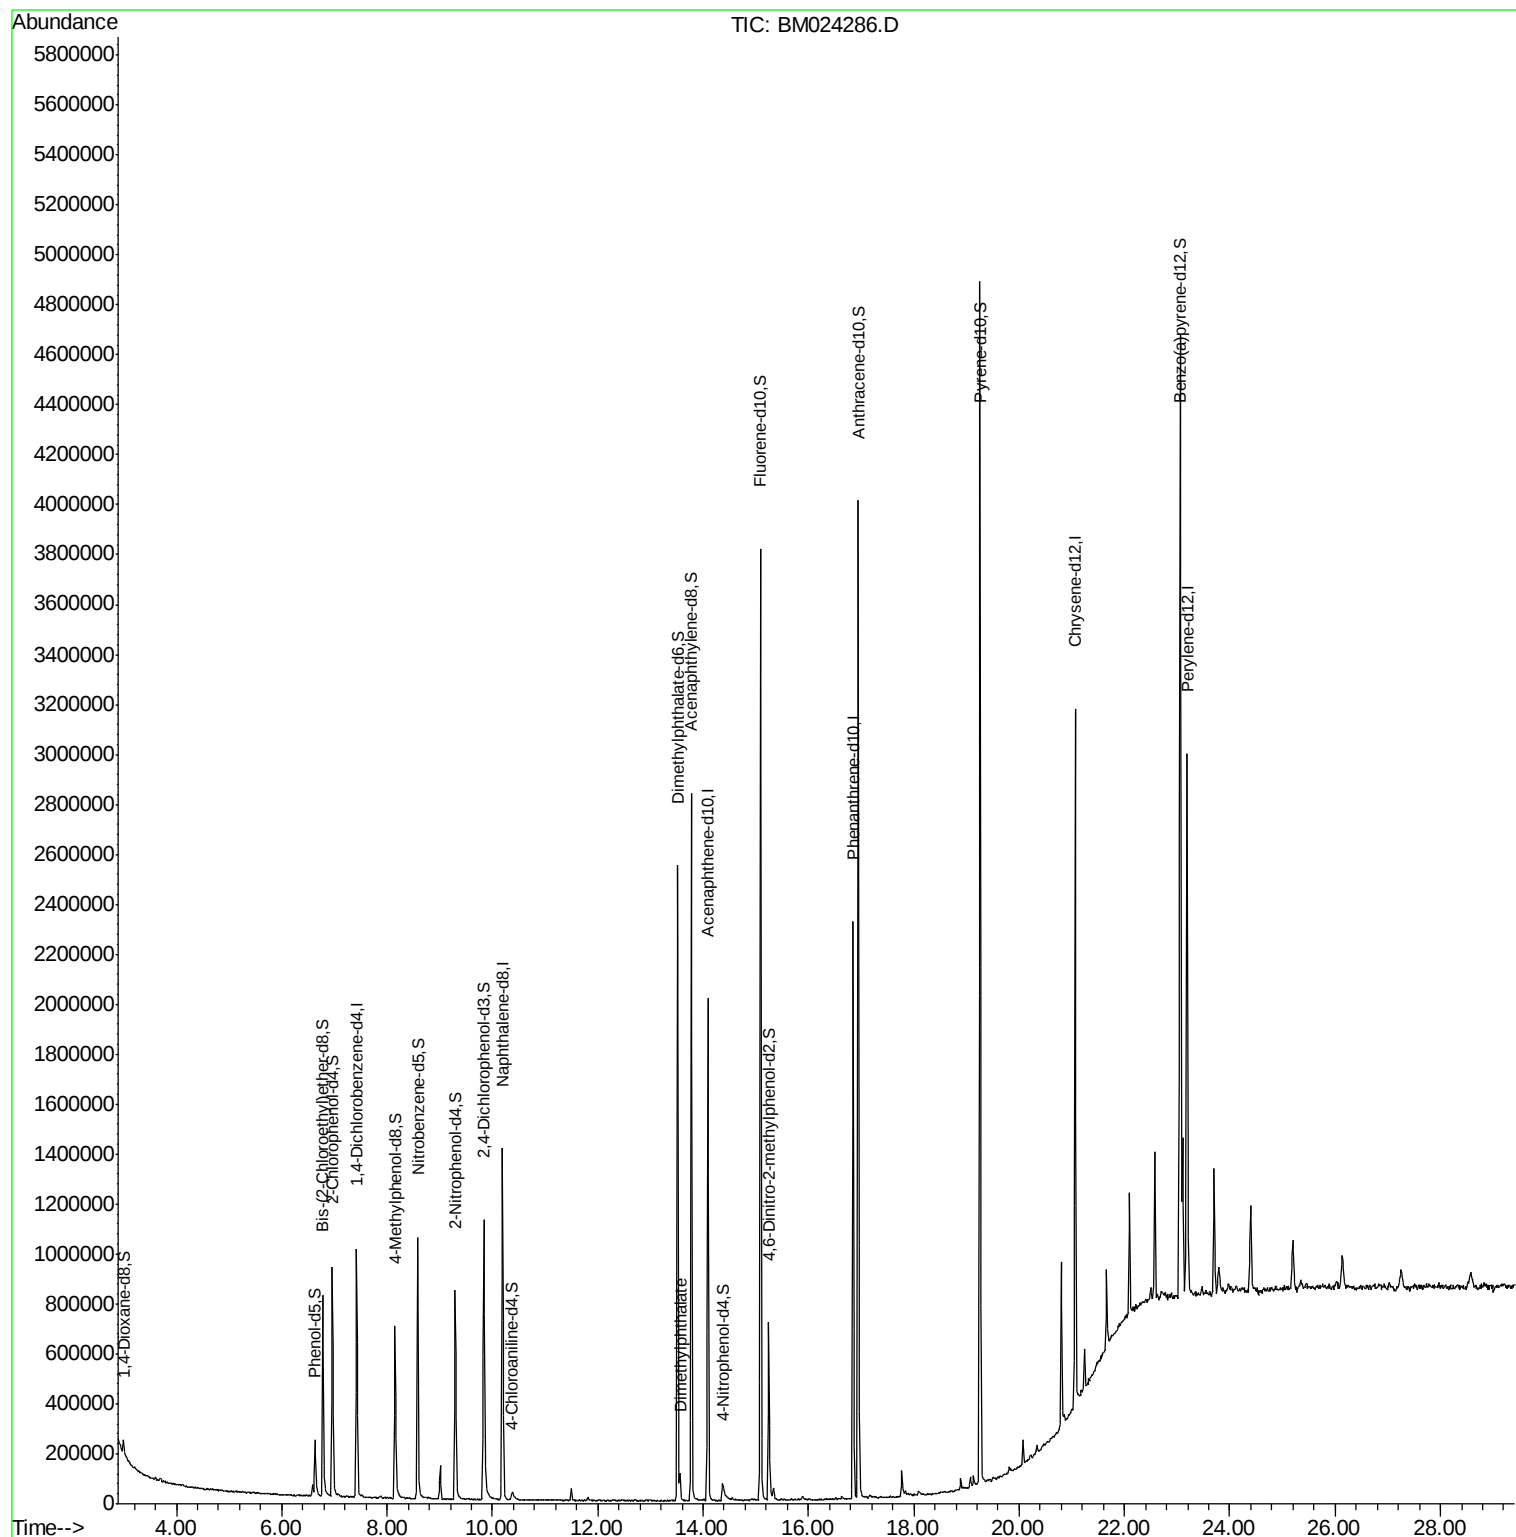

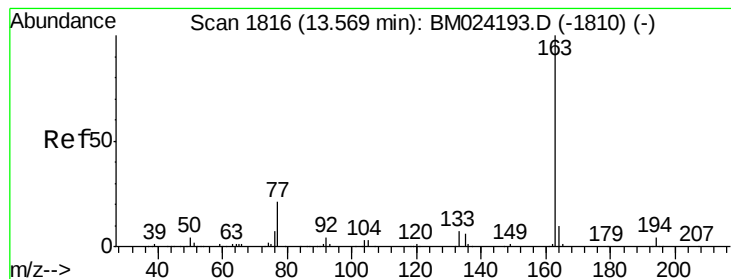

#45

Dimethylphthalate

Concen: 1.158 ng/ul

RT: 13.56 min Scan# 1815

Delta R.T. -0.01 min

Lab File: BM024286.D

Acq: 25 Dec 2019 13:17

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 57666

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 11.0 7.8 11.6

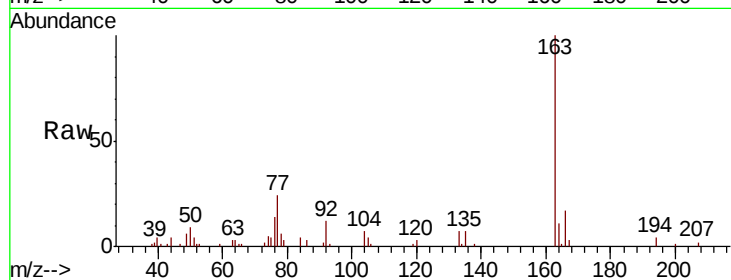

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

