

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM122319\
Quantitation Report (QT Reviewed)


Data File : BM024276.D
Acq On : 25 Dec 2019 04:35
Operator : JU
Sample : K6240-22
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 25 06:48:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

Instrument :
BNA_M
Client Sample ID :
BFQS7

Manual Integrations
APPROVED

mohammad
12/26/2019 4:00:35 PM

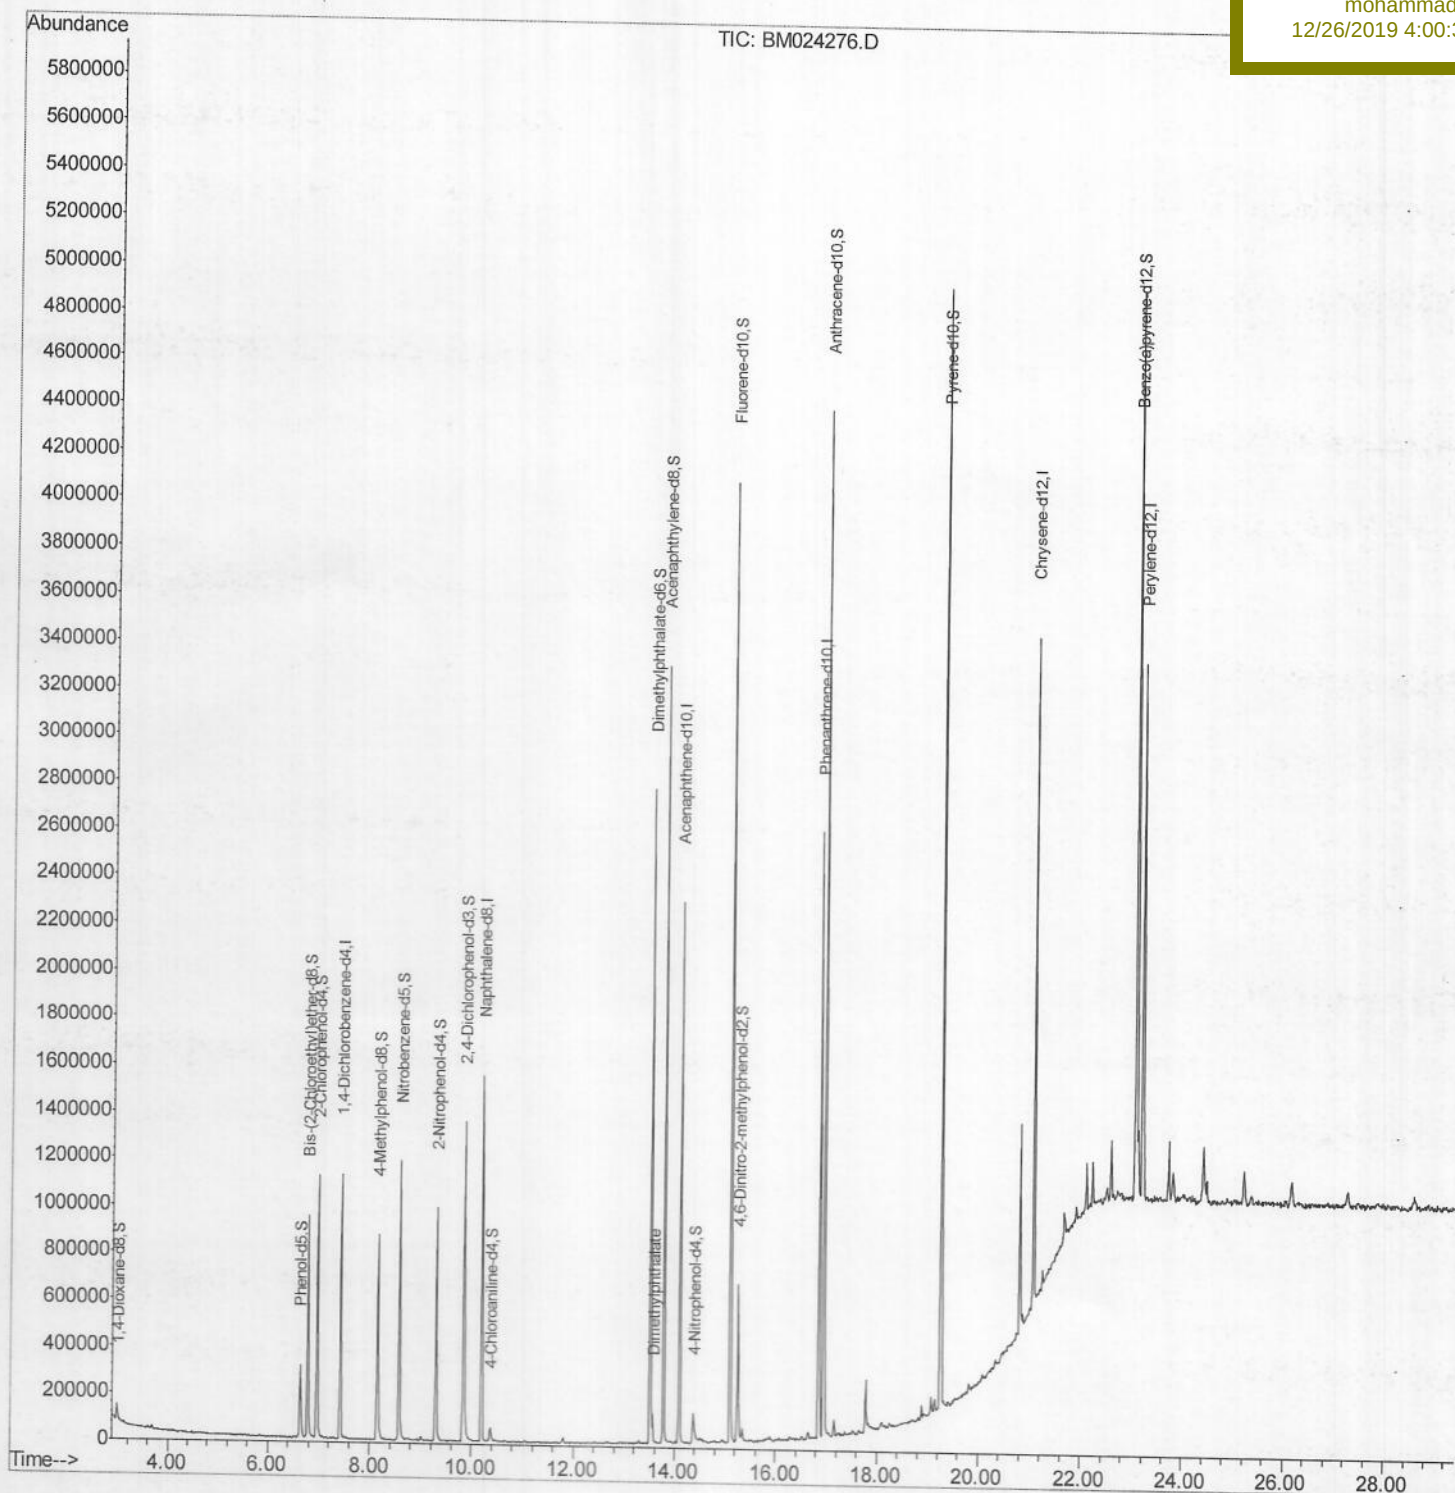

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM122319\
Quantitation Report (Qedit)




Data File : BM024276.D
Acq On : 25 Dec 2019 04:35
Operator : JU
Sample : K6240-22
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 25 06:35:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BFQS7

Manual Integrations
APPROVED

mohammad
12/26/2019 4:00:35 PM

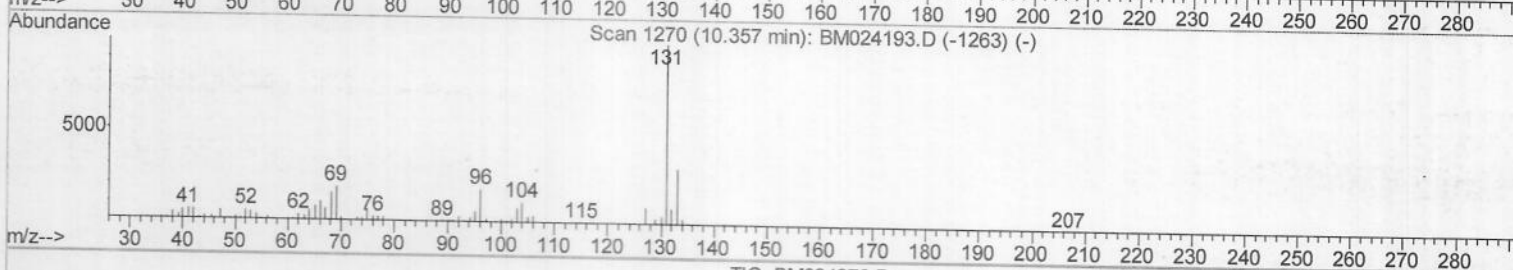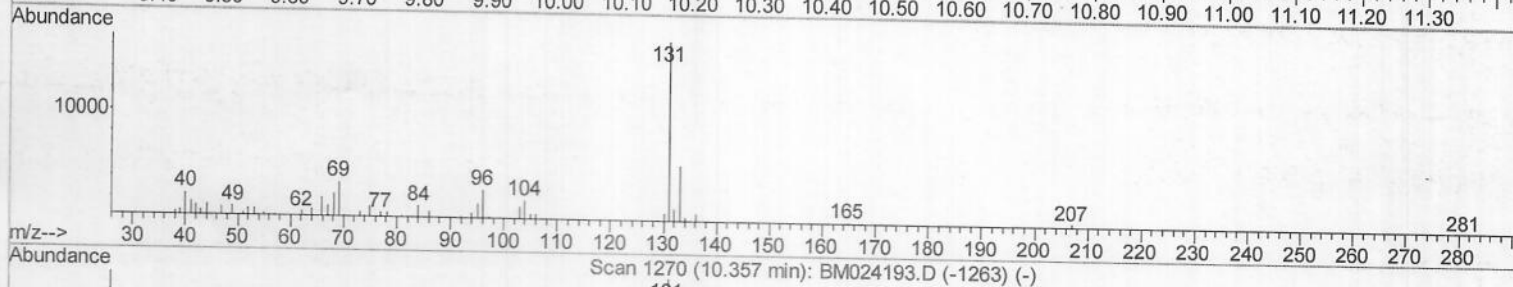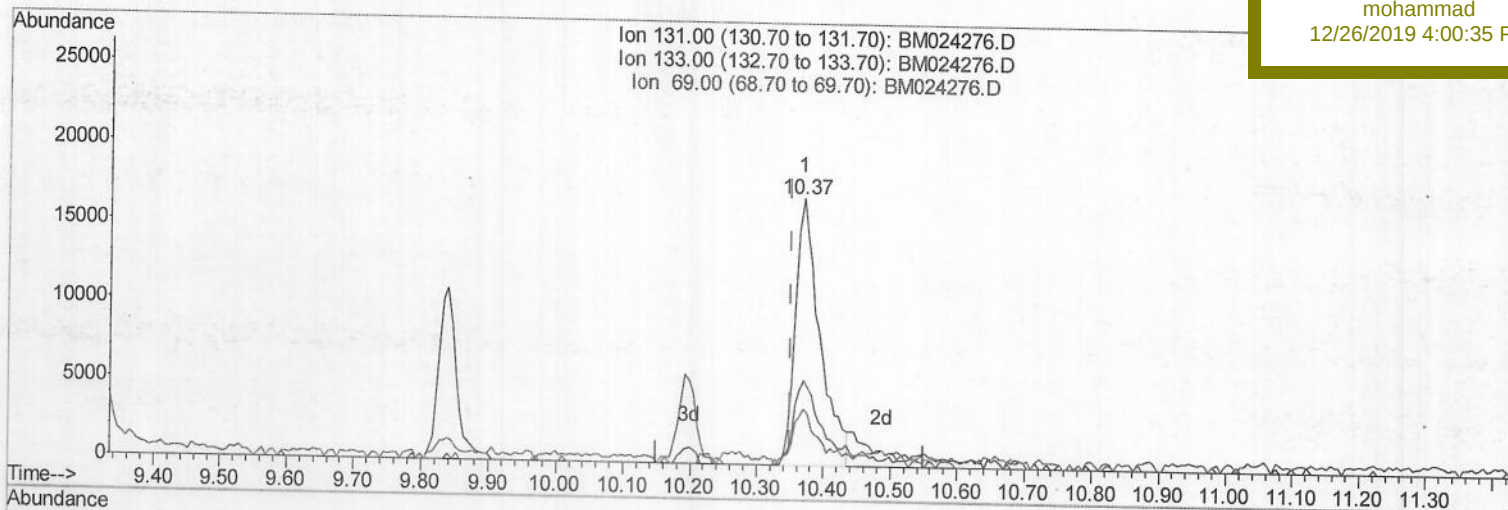

TIC: BM024276.D

(29) 4-Chloroaniline-d4 (S)
10.369min (+0.018) 1.86ng/ul
response 42872

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	31.90
69.00	19.00	20.90
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM122319\

Quantitation Report (Qedit)

Data File : BM024276.D

Acq On : 25 Dec 2019 04:35

Operator : JU

Sample : K6240-22

Misc :

ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 25 06:35:28 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Dec 25 03:33:48 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




BFQS7

Manual Integrations

APPROVED

mohammad

12/26/2019 4:00:35 PM

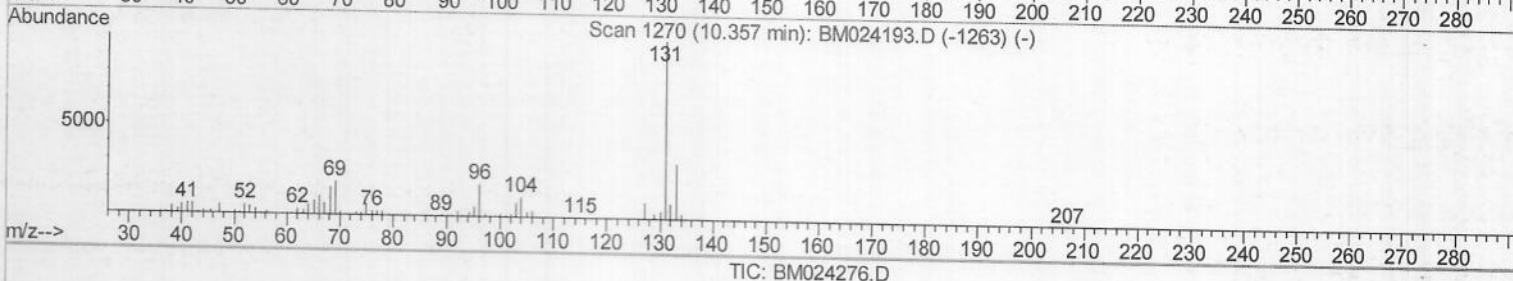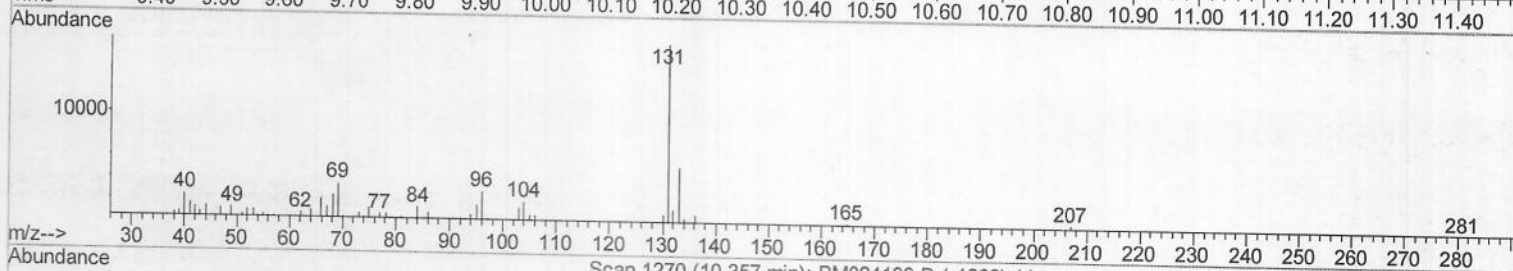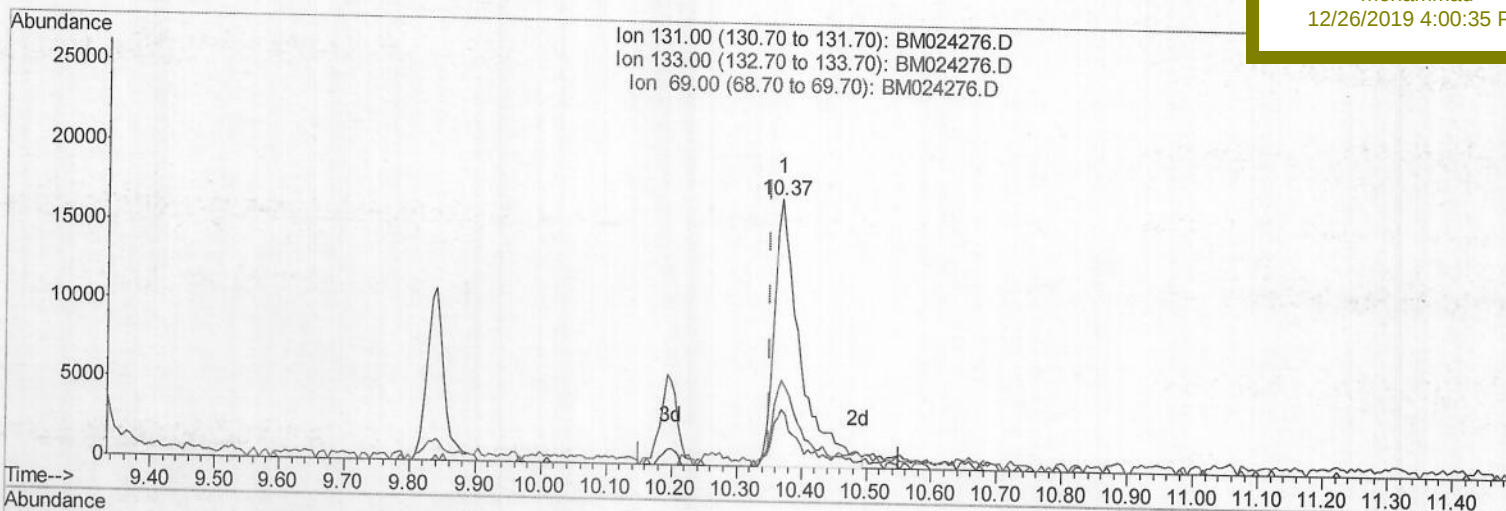

(29) 4-Chloroaniline-d4 (S)

10.369min (+0.018) 2.07ng/ul m

response 47650

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	31.90
69.00	19.00	20.90
0.00	0.00	0.00

JU 12/27/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM122319\

Quantitation Report (QT Reviewed)

Data File : BM024276.D

Acq On : 25 Dec 2019 04:35

Operator : JU

Sample : K6240-22

Misc :

ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 25 06:48:18 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Dec 25 03:33:48 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

BFQS7

Manual Integrations

APPROVED

mohammad

12/26/2019 4:00:35 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	298556	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	1236297	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	706297	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1408682	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	1269671	20.00	ng/ul	0.00
86) Perylene-d12	23.20	264	1536484	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.99	96	37213	5.51	ng/uL	0.00
5) Phenol-d5	6.63	99	198584	7.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	457934	27.01	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	497935	24.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	356685	15.44	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	277741	31.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	316172	32.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	540578	28.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	47650m	2.07	ng/ul	0.02
44) Dimethylphthalate-d6	13.52	166	1766223	33.82	ng/ul	0.00
47) Acenaphthylene-d8	13.78	160	2130851	34.05	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	49258	5.25	ng/ul	0.02
58) Fluorene-d10	15.10	176	1487933	32.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	129823	15.11	ng/ul	0.00
71) Anthracene-d10	16.95	188	2191953	34.20	ng/ul	0.00
79) Pyrene-d10	19.26	212	2290110	37.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2577158	33.77	ng/ul	0.00

JU 12/27/19

Target Compounds

45) Dimethylphthalate	13.56	163	70798	1.304	ng/ul	99
-----------------------	-------	-----	-------	-------	-------	----

(#) = qualifier out of range (m) = manual integration (+) = signals summed