

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122319\
 Data File : BM024247.D
 Acq On : 24 Dec 2019 10:31
 Operator : JU
 Sample : K6200-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFF08

Quant Time: Dec 24 11:37:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 24 05:54:49 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	226703	20.00	ng/ul	0.00
18) Naphthalene-d8	10.20	136	985641	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	616889	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1243367	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	1107165	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	1199317	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.00	96	8217	1.60	ng/uL	0.01
5) Phenol-d5	6.63	99	231704	10.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	558096	43.35	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	243272	15.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	240948	13.73	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	313794	44.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	207514	26.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	378021	24.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	128511	6.99	ng/ul	0.01
44) Dimethylphthalate-d6	13.52	166	2307691	50.59	ng/ul	0.00
47) Acenaphthylene-d8	13.78	160	892778	16.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	71681	8.75	ng/ul	0.02
58) Fluorene-d10	15.10	176	1156144	28.91	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.24	200	148746	19.61	ng/ul	0.00
71) Anthracene-d10	16.95	188	1095413	19.36	ng/ul	0.00
79) Pyrene-d10	19.26	212	1879600	35.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	842273	14.14	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.56	163	116643	2.460	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122319\
Data File : BM024247.D
Acq On : 24 Dec 2019 10:31
Operator : JU
Sample : K6200-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFF08

Quant Time: Dec 24 11:37:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 05:54:49 2019
Response via : Initial Calibration

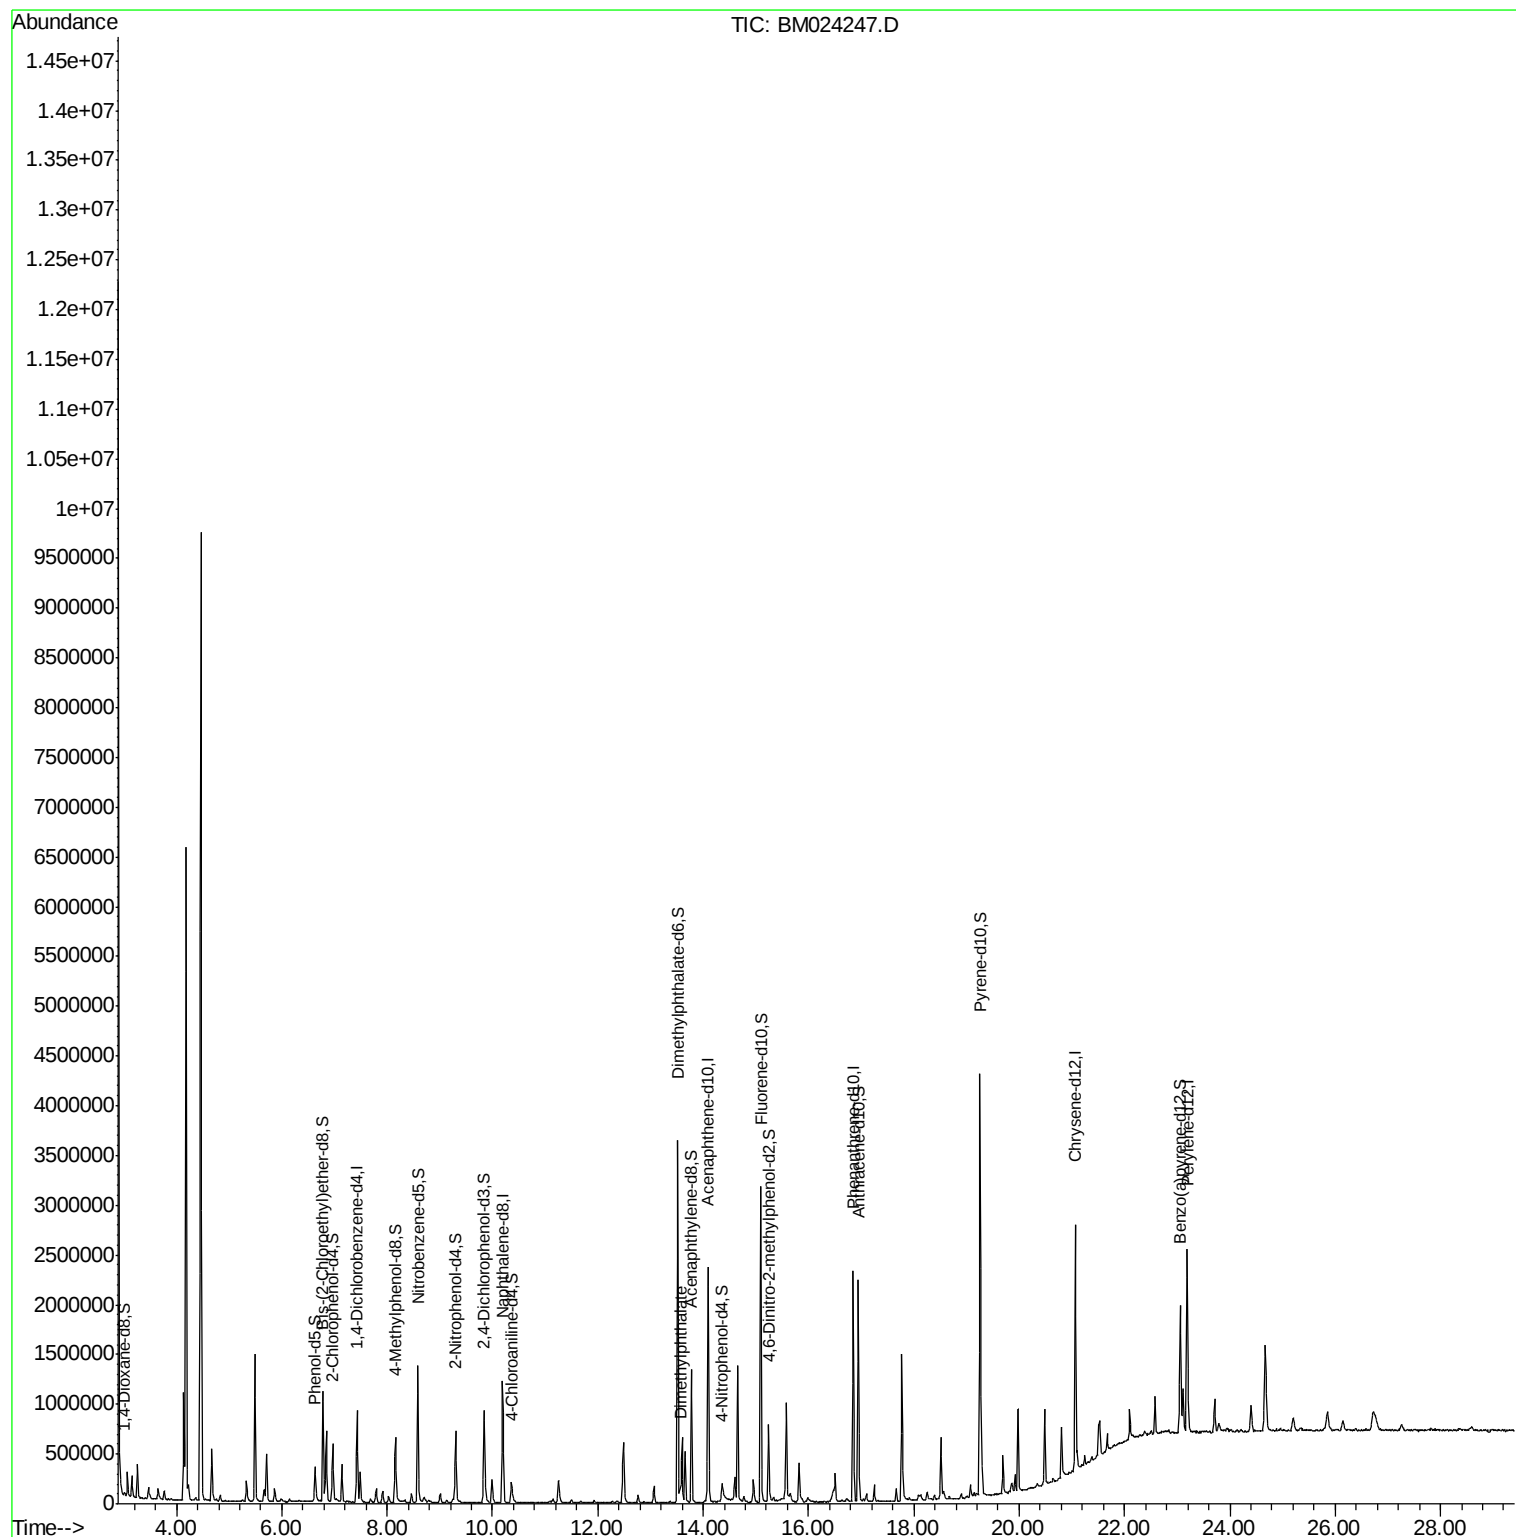

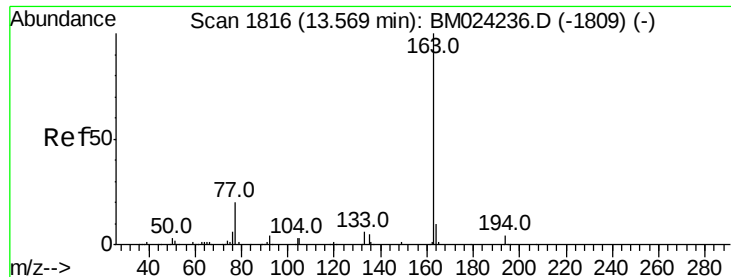

#45

Dimethylphthalate

Concen: 2.460 ng/ul

RT: 13.56 min Scan# 1815

Delta R.T. -0.01 min

Lab File: BM024247.D

Acq: 24 Dec 2019 10:31

Instrument :

BNA_M

ClientSampleId :

BFF08


Tot Ion:163 Resp: 116643

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 10.3 7.8 11.6

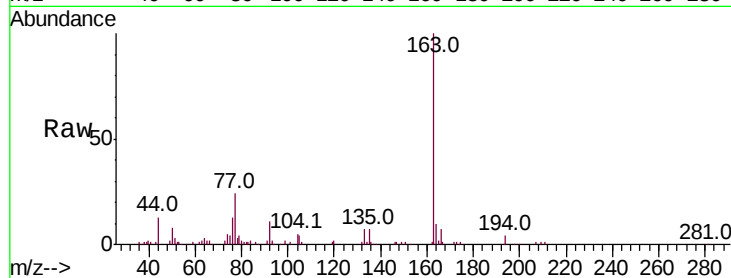

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

