

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122319\
 Data File : BM024250.D
 Acq On : 24 Dec 2019 12:19
 Operator : JU
 Sample : K6236-22
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFEY3

Manual Integrations
 APPROVED

mohammad
 12/24/2019 2:59:05 PM

Quant Time: Dec 24 12:57:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 24 05:54:49 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	284158	20.00	ng/ul	0.00
18) Naphthalene-d8	10.20	136	1214801	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	733978	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1485356	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1307039	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	1507583	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.00	96	18751	2.92	ng/uL	0.00
5) Phenol-d5	6.63	99	323844	12.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	242320	15.02	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	264175	13.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	155768	7.08	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	124924	14.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	132216	13.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	241466	12.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	267000	11.78	ng/ul	0.00
44) Dimethylphthalate-d6	13.52	166	893451	16.46	ng/ul	0.00
47) Acenaphthylene-d8	13.78	160	995012	15.30	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	71477m	7.33	ng/ul	0.02
58) Fluorene-d10	15.09	176	762884	16.03	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	68232	7.53	ng/ul	0.00
71) Anthracene-d10	16.95	188	1033738	15.30	ng/ul	0.00
79) Pyrene-d10	19.26	212	1255537	20.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	1339287	17.88	ng/ul	0.00

Target Compounds					Ovalue	
6) Phenol	6.66	94	50698	1.825	ng/ul#	90
45) Dimethylphthalate	13.57	163	145420	2.578	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122319\
Data File : BM024250.D
Acq On : 24 Dec 2019 12:19
Operator : JU
Sample : K6236-22
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BFEY3

Manual Integrations
APPROVED

mohammad
12/24/2019 2:59:05 PM

Quant Time: Dec 24 12:57:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 05:54:49 2019
Response via : Initial Calibration

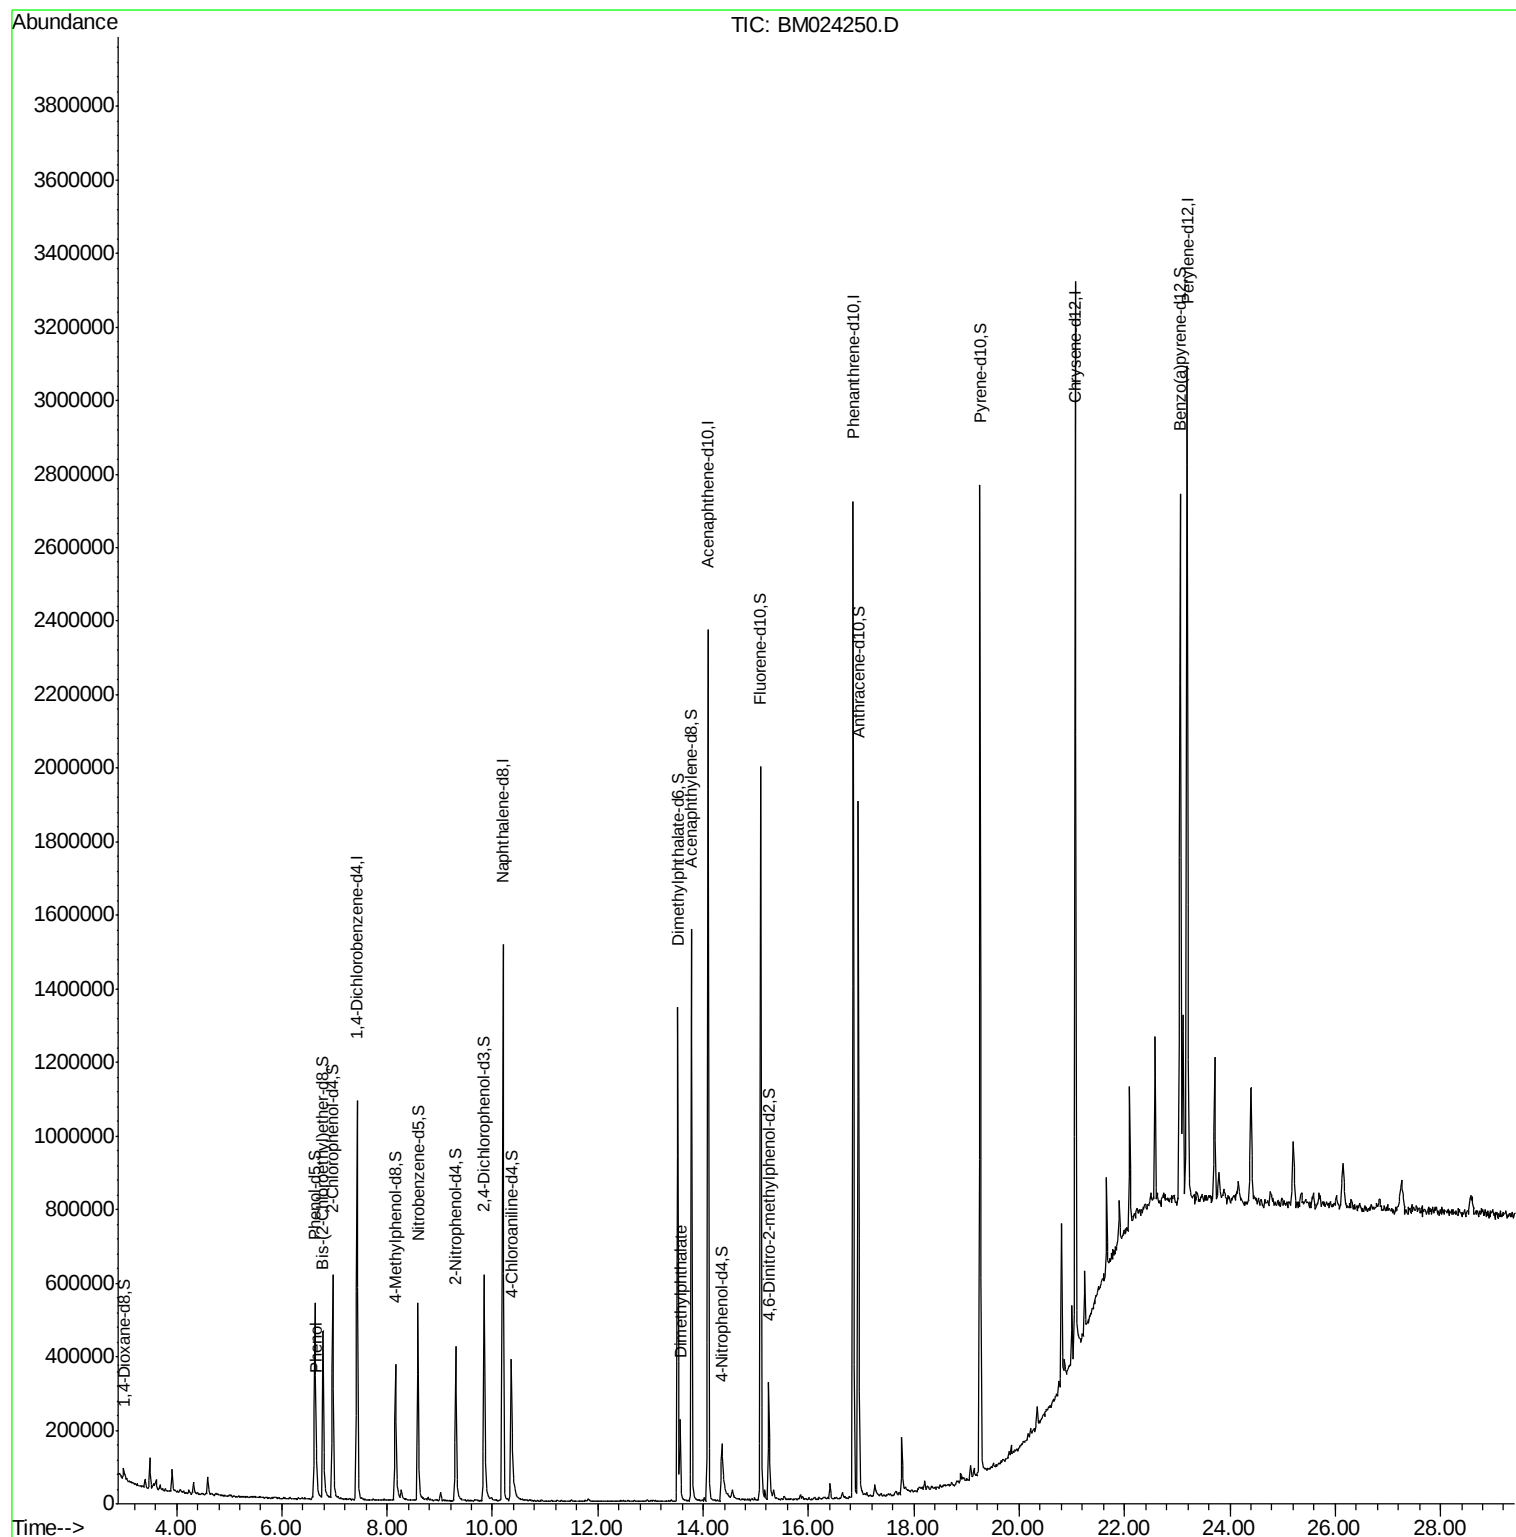

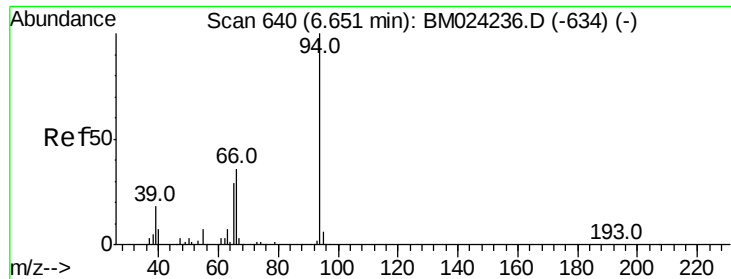

#6

Phenol

Concen: 1.825 ng/ul

RT: 6.66 min Scan# 641

Delta R.T. 0.01 min

Lab File: BM024250.D

Acq: 24 Dec 2019 12:19

Instrument :

BNA_M

ClientSampleId :

BFEY3

Tot Ion: 94 Resp: 50698

Ion Ratio Lower Upper

94 100

65 31.1 22.6 33.8





66 46.8 30.7 46.1#

Manual Integrations

APPROVED

mohammad

12/24/2019 2:59:05 PM

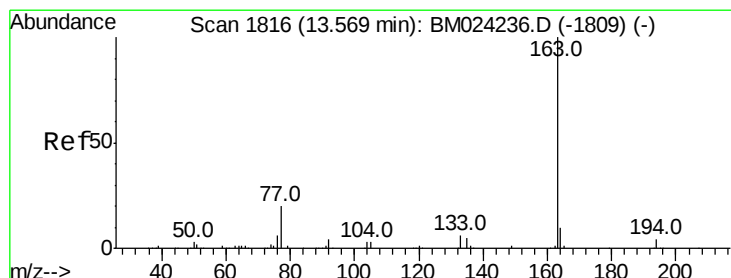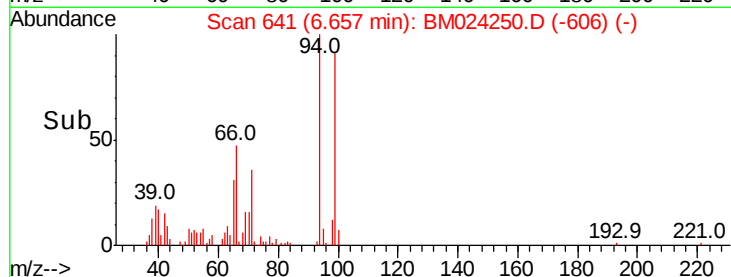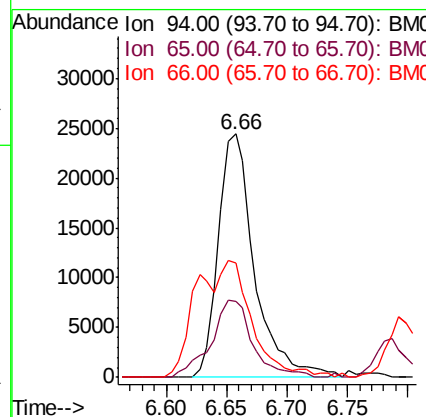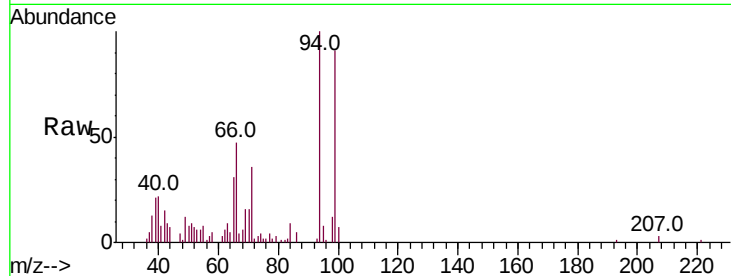

#45

Dimethylphthalate

Concen: 2.578 ng/ul

RT: 13.57 min Scan# 1816

Delta R.T. -0.00 min

Lab File: BM024250.D

Acq: 24 Dec 2019 12:19

Tgt Ion: 163 Resp: 145420

Ion Ratio Lower Upper

163 100

194 4.6 3.2 4.8

164 9.5 7.8 11.6

