

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122319\
 Data File : BM024273.D
 Acq On : 25 Dec 2019 02:48
 Operator : JU
 Sample : K6240-19
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFQS2

Quant Time: Dec 25 03:36:59 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 25 03:33:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	289247	20.00	ng/ul	0.00
18) Naphthalene-d8	10.20	136	1212095	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	696673	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1398716	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	1256192	20.00	ng/ul	0.00
86) Perylene-d12	23.20	264	1534349	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.99	96	39442	6.02	ng/uL	0.00
5) Phenol-d5	6.63	99	171535	6.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	461380	28.09	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	478608	24.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	327616	14.63	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	283716	32.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	316061	33.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	540733	29.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	81307	3.60	ng/ul	0.01
44) Dimethylphthalate-d6	13.52	166	1771590	34.39	ng/ul	0.00
47) Acenaphthylene-d8	13.78	160	2190579	35.49	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	40218	4.35	ng/ul	0.02
58) Fluorene-d10	15.10	176	1521205	33.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	138187	16.19	ng/ul	0.00
71) Anthracene-d10	16.95	188	2278072	35.80	ng/ul	0.00
79) Pyrene-d10	19.26	212	2395076	40.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2738930	35.94	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.57	163	105555	1.971	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122319\
Data File : BM024273.D
Acq On : 25 Dec 2019 02:48
Operator : JU
Sample : K6240-19
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQS2

Quant Time: Dec 25 03:36:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

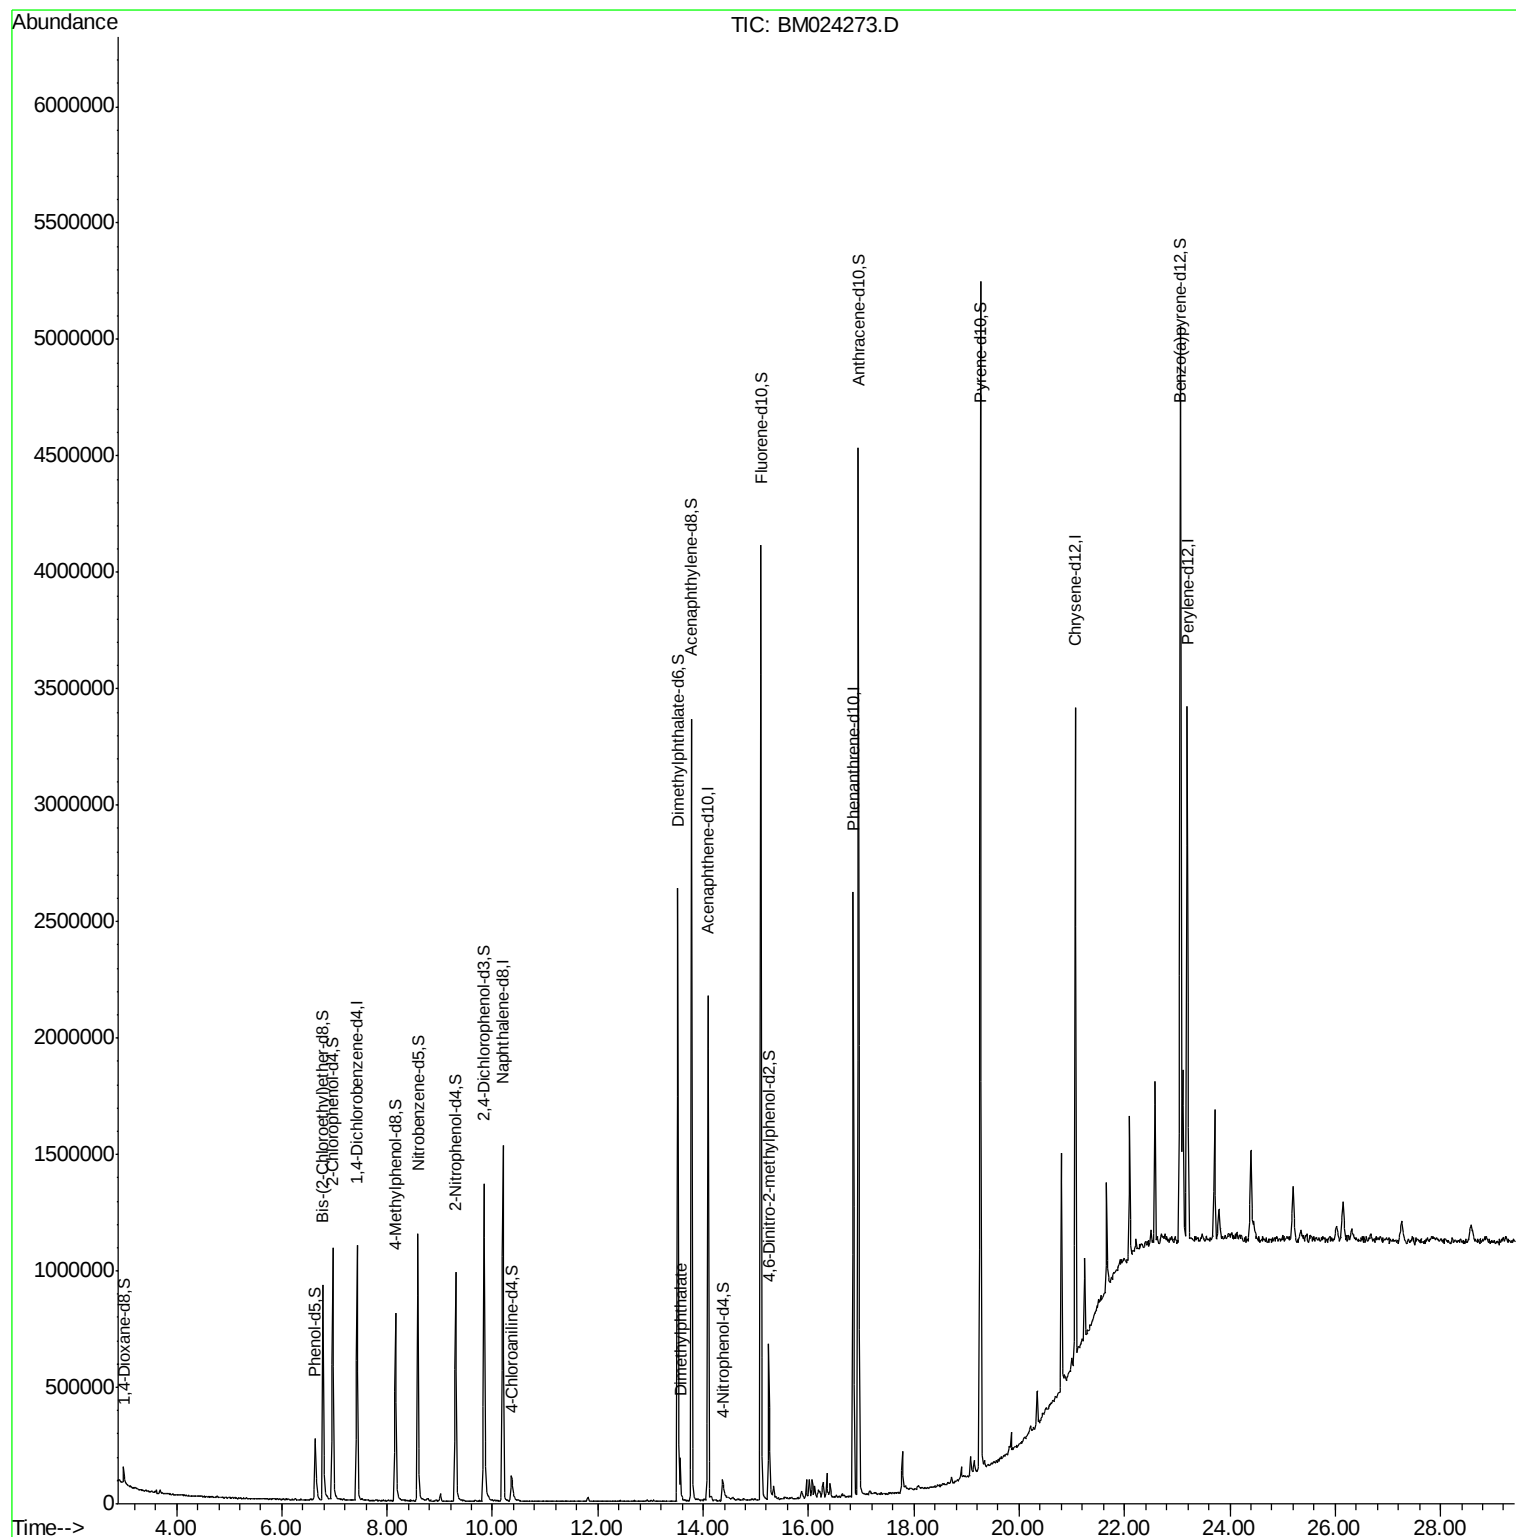

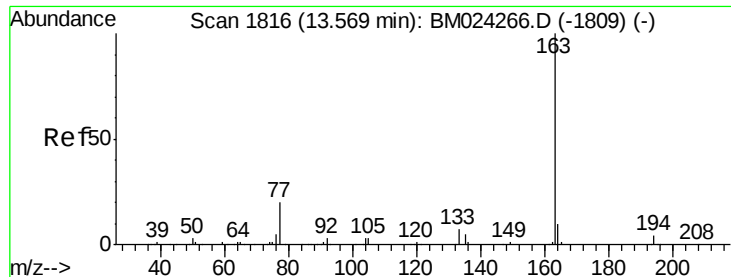

#45

Dimethylphthalate

Concen: 1.971 ng/ul

RT: 13.57 min Scan# 1816

Delta R.T. -0.00 min

Lab File: BM024273.D

Acq: 25 Dec 2019 02:48

Instrument :

BNA_M

ClientSampleId :

BFQS2


Tot Ion:163 Resp: 105555

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 10.8 7.8 11.6

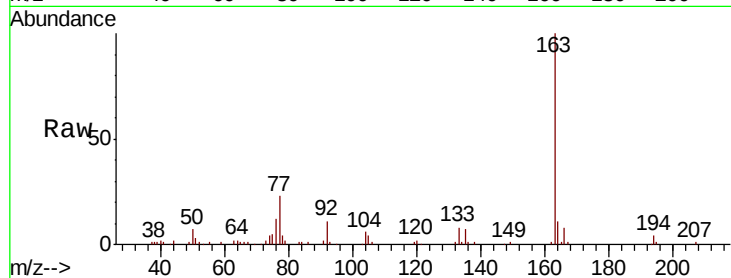

Abundance Ion 163.00 (162.70 to 163.70): E

100000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

