

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122319\
 Data File : BM024274.D
 Acq On : 25 Dec 2019 03:24
 Operator : JU
 Sample : K6240-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFQS3

Quant Time: Dec 25 06:35:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 25 03:33:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	326412	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	1332545	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	760069	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1512638	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	1360299	20.00	ng/ul	0.00
86) Perylene-d12	23.20	264	1657265	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.99	96	36757	4.97	ng/uL	0.00
5) Phenol-d5	6.63	99	197549	6.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	485675	26.20	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	498371	22.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	355824	14.08	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	290326	30.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	326382	31.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	565935	27.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	86226	3.47	ng/ul	0.01
44) Dimethylphthalate-d6	13.52	166	1847616	32.87	ng/ul	0.00
47) Acenaphthylene-d8	13.78	160	2274223	33.77	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	46655	4.62	ng/ul	0.02
58) Fluorene-d10	15.10	176	1556065	31.58	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	139136	15.08	ng/ul	0.00
71) Anthracene-d10	16.95	188	2332472	33.89	ng/ul	0.00
79) Pyrene-d10	19.26	212	2448484	37.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2822539	34.29	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.57	163	117768	2.016	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122319\
Data File : BM024274.D
Acq On : 25 Dec 2019 03:24
Operator : JU
Sample : K6240-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQS3

Quant Time: Dec 25 06:35:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

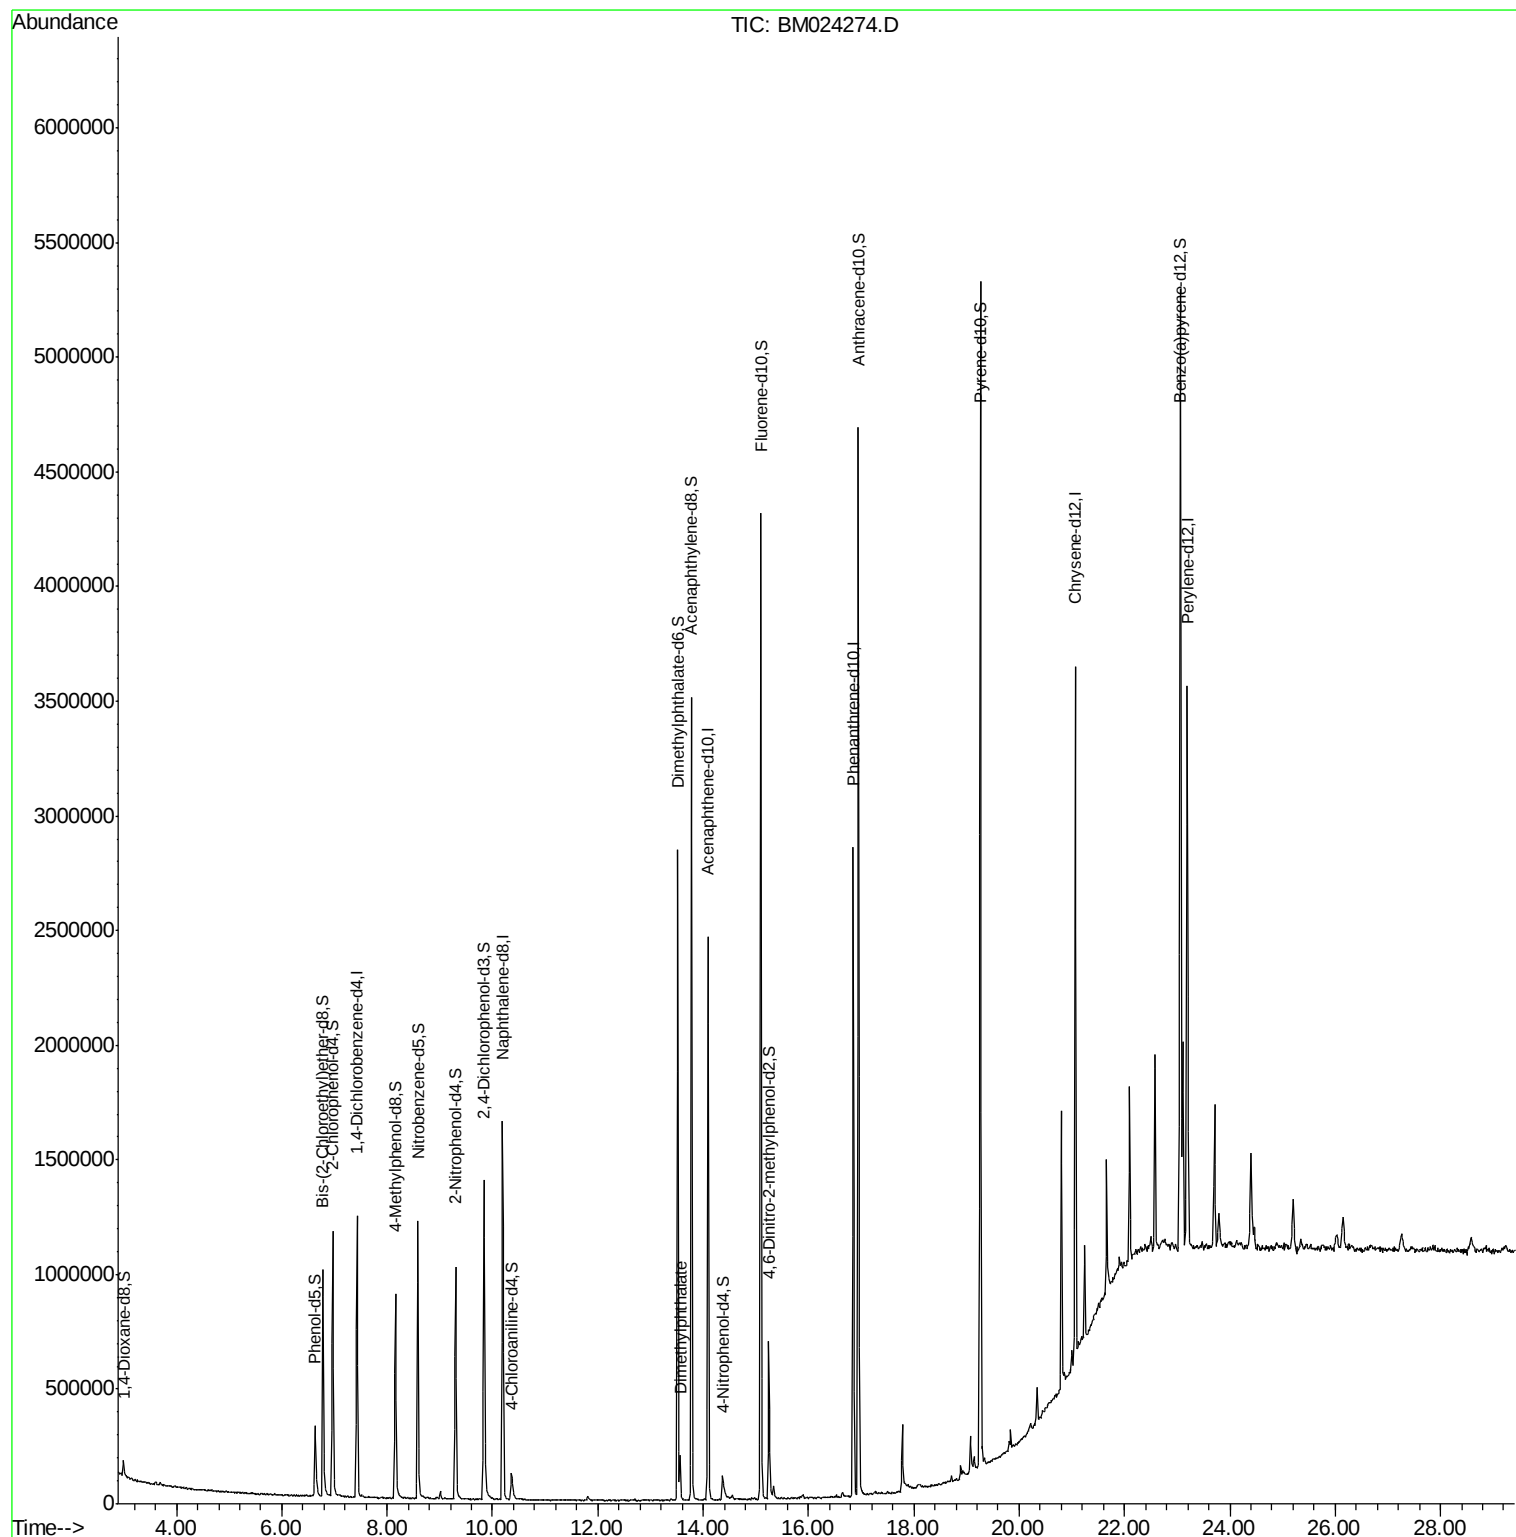

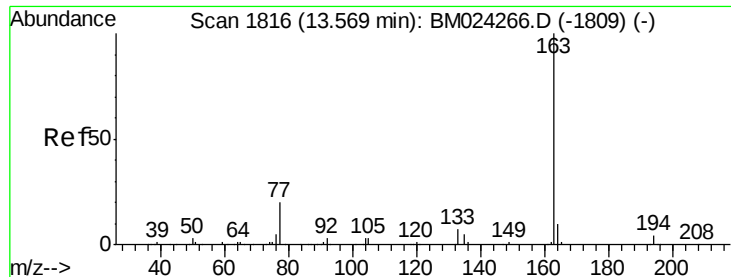

#45

Dimethylphthalate

Concen: 2.016 ng/ul

RT: 13.57 min Scan# 1816

Delta R.T. -0.00 min

Lab File: BM024274.D

Acq: 25 Dec 2019 03:24

Instrument :

BNA_M

ClientSampleId :

BFQS3


Tot Ion:163 Resp: 117768

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 9.4 7.8 11.6

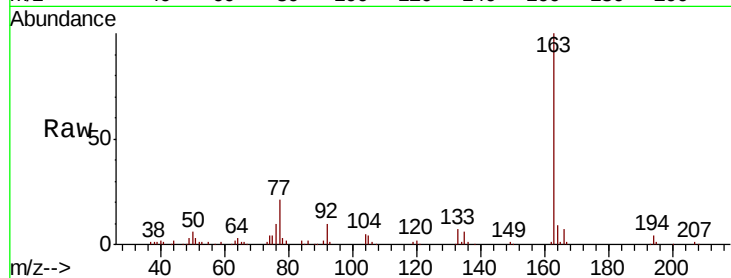

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

